

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121115\
 Data File : BG020101.D
 Acq On : 11 Dec 2015 8:39
 Operator : UM/SJ
 Sample : G4729-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 11 10:45:34 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	19400	20.00	ng	-0.02
21) Naphthalene-d8	10.93	136	82821	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	73741	20.00	ng	-0.02
63) Phenanthrene-d10	17.48	188	131057	20.00	ng	-0.03
75) Chrysene-d12	21.75	240	167642	20.00	ng	-0.04
86) Perylene-d12	25.03	264	157019	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	78532	73.16	ng	-0.01
7) Phenol-d6	7.26	99	74616	46.04	ng	-0.02
23) Nitrobenzene-d5	9.28	82	163237	100.59	ng	-0.02
41) 2,4,6-Tribromophenol	16.23	330	117098	103.78	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	383351	70.98	ng	-0.02
78) Terphenyl-d14	20.08	244	626822	91.20	ng	-0.03
Target Compounds						Qvalue
15) Benzyl Alcohol	8.44	79	3191	2.24	ng	# 54
18) Hexachloroethane	9.22	117	24699	43.05	ng	# 1
24) Nitrobenzene	9.31	77	5130	2.91	ng	# 1
32) Benzoic acid	10.13	122	134	6.13	ng	# 1
37) 2-Methylnaphthalene	12.80	142	187300	57.60	ng	# 94
53) 2,4-Dinitrophenol	14.91	184	54	9.34	ng	# 1
59) Diethylphthalate	15.41	149	77460	10.79	ng	# 50
64) 4,6-Dinitro-2-methylphenol	15.82	198	60	6.18	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121115\
Data File : BG020101.D
Acq On : 11 Dec 2015 8:39
Operator : UM/SJ
Sample : G4729-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 11 10:45:34 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

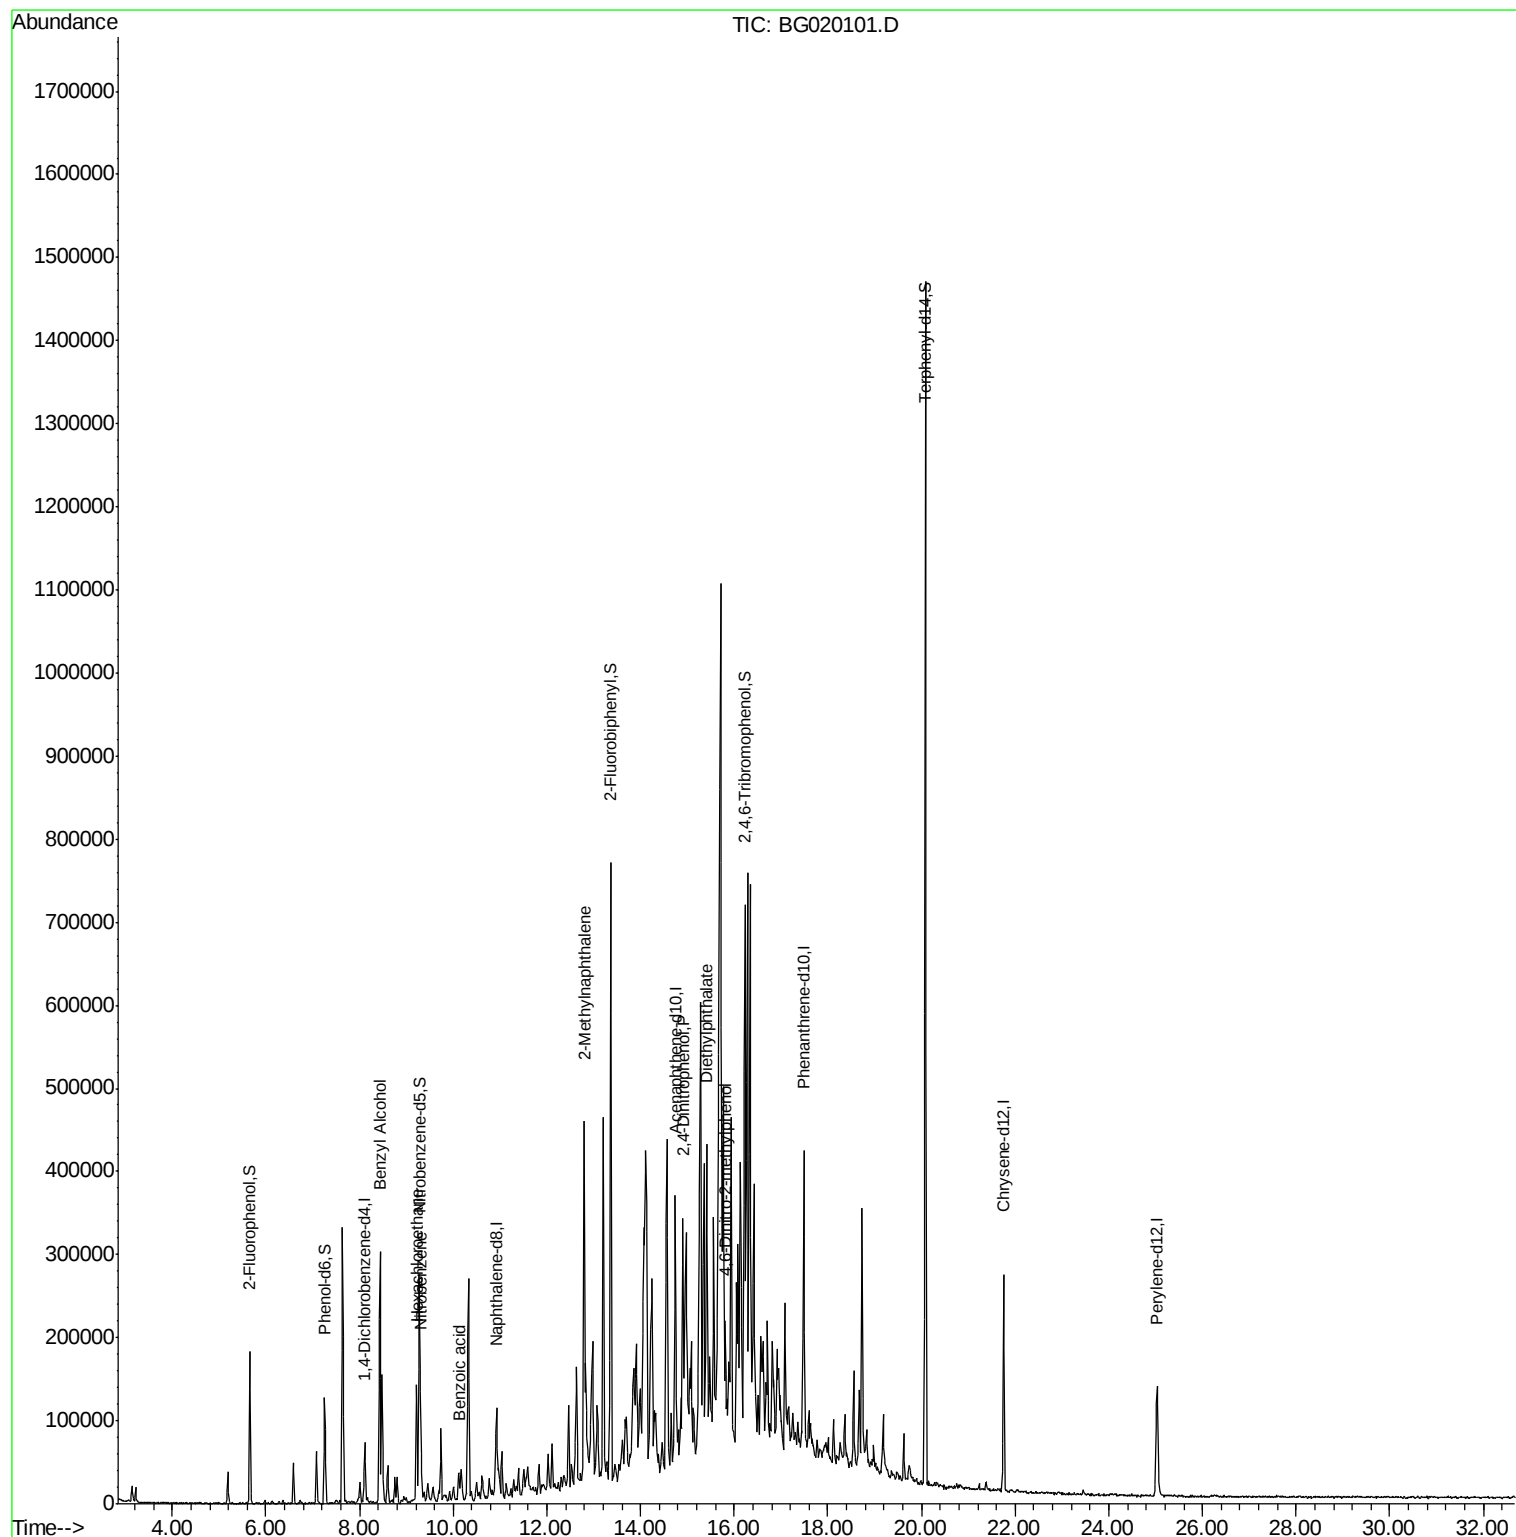







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 8.11 min Scan# 898
 Delta R.T. -0.02 min
 Lab File: BG020101.D
 Acq: 11 Dec 2015 8:39

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:152 Resp: 19400
 Ion Ratio Lower Upper
 152 100
 150 147.9 115.0 172.4
 115 58.7 43.9 65.9

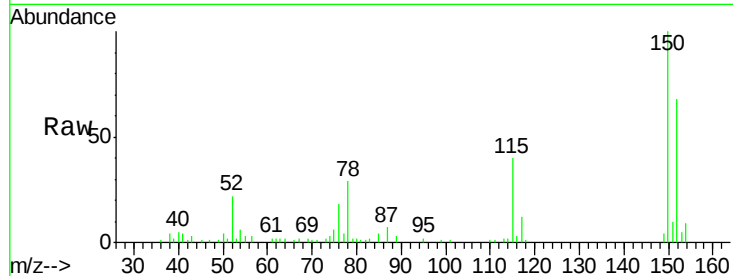


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

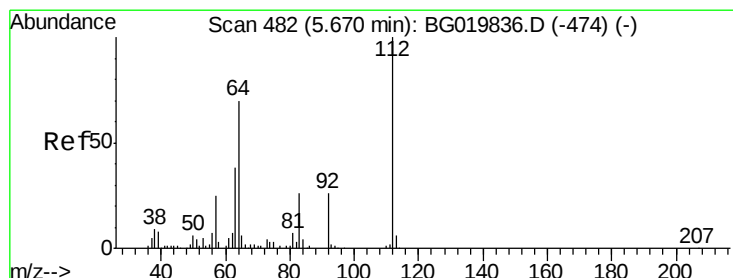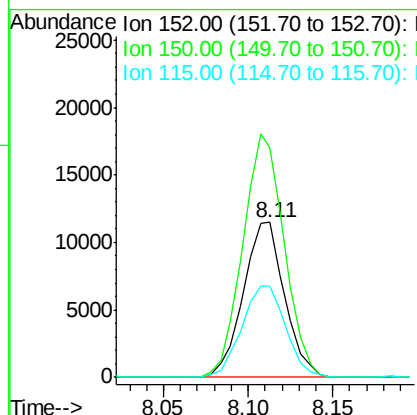
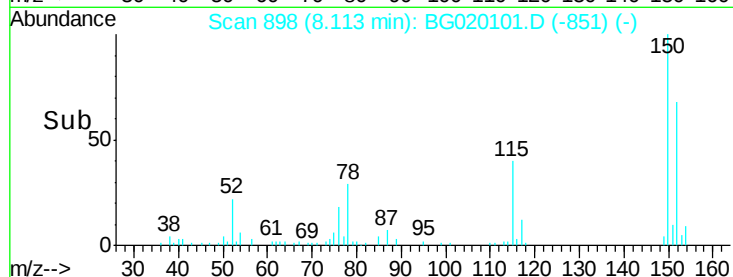



#5
 2-Fluorophenol
 Concen: 73.16 ng
 RT: 5.66 min Scan# 480
 Delta R.T. -0.01 min
 Lab File: BG020101.D
 Acq: 11 Dec 2015 8:39

Tgt Ion:112 Resp: 78532
 Ion Ratio Lower Upper
 112 100
 64 65.6 43.7 65.5#
 63 35.1 24.0 36.0

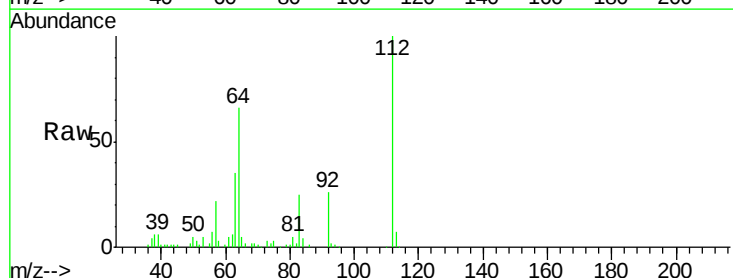

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

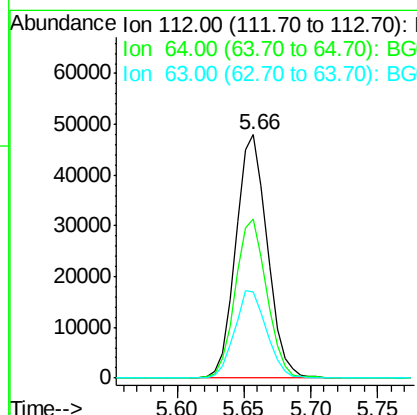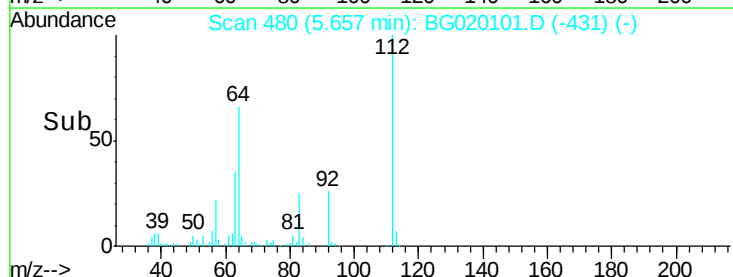

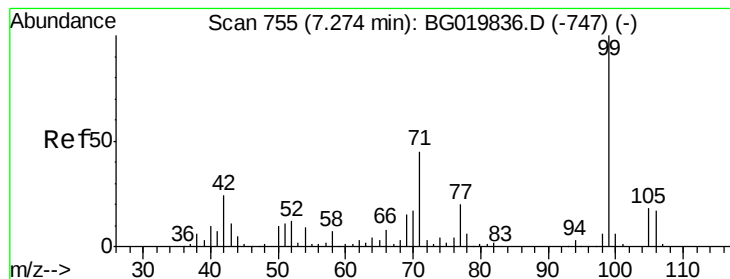

#7

Phenol-d6

Concen: 46.04 ng

RT: 7.26 min Scan# 752

Delta R.T. -0.02 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 74616

Ion Ratio Lower Upper




99 100

42 19.5 11.5 17.3#

71 39.6 22.6 34.0#

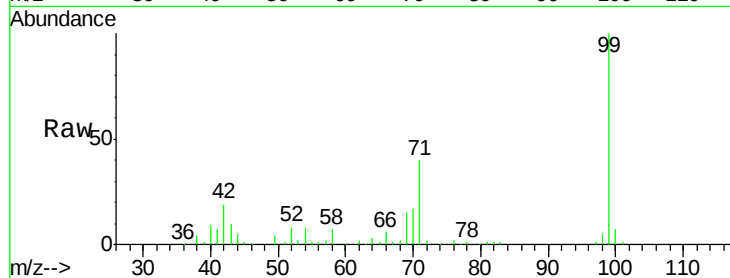

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

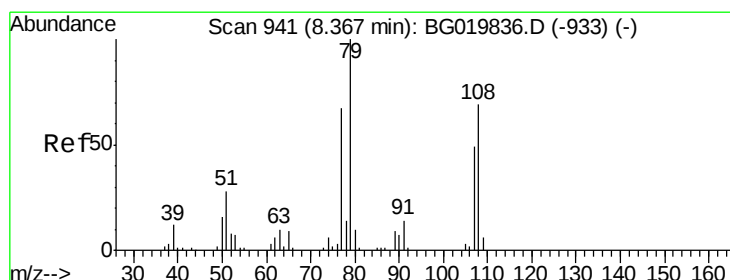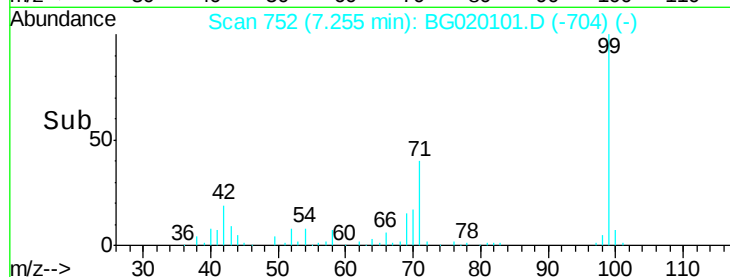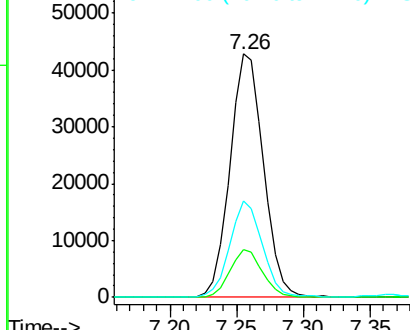

#15

Benzyl Alcohol

Concen: 2.24 ng

RT: 8.44 min Scan# 953

Delta R.T. 0.07 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39


Tgt Ion: 79 Resp: 3191

Ion Ratio Lower Upper



79 100


108 33.5 65.5 98.3#

77 91.8 51.3 76.9#

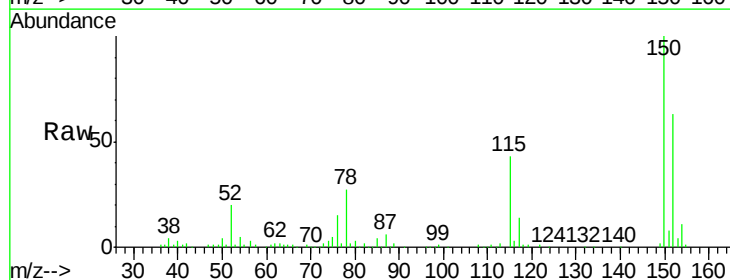

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

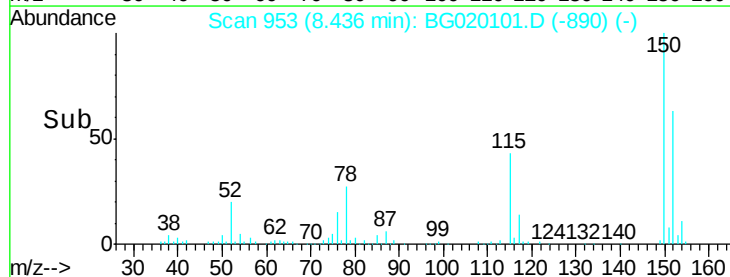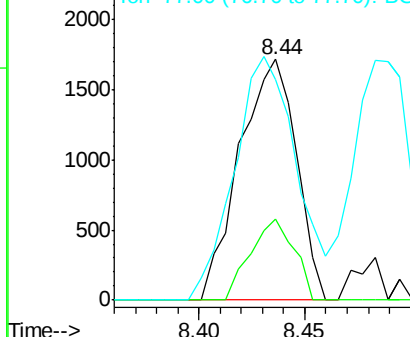







#18
Hexachloroethane
Concen: 43.05 ng
RT: 9.22 min Scan# 1087
Delta R.T. -0.00 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39

Instrument :
BNA_G
ClientSampled :

Tot Ion:117 Resp: 24699
Ion Ratio Lower Upper
117 100
119 235.4 71.7 107.5#
201 0.0 90.9 136.3#

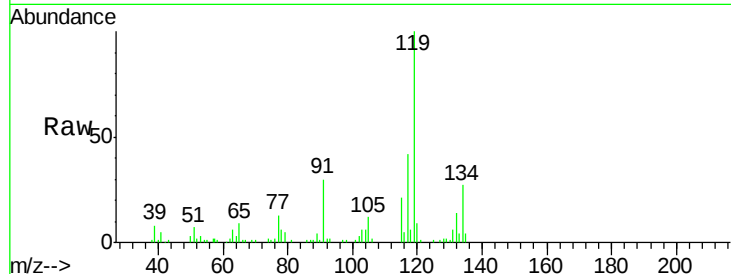


Abundance Ion 117.00 (116.70 to 117.70): E
Ion 119.00 (118.70 to 119.70): E
Ion 201.00 (200.70 to 201.70): E

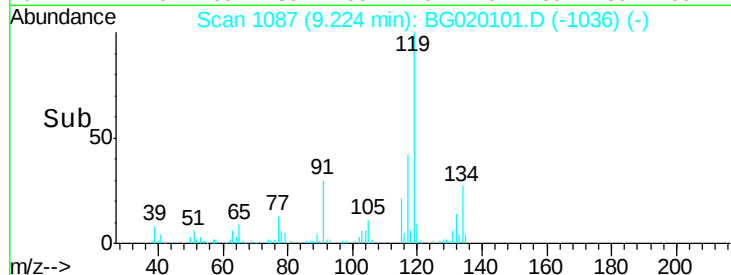
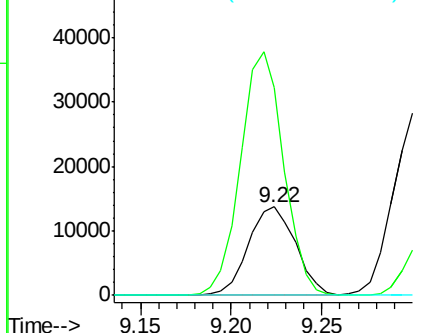



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.93 min Scan# 1377
Delta R.T. -0.02 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39

Tgt Ion:136 Resp: 82821
Ion Ratio Lower Upper
136 100
137 12.9 8.6 12.8#
54 10.3 5.4 8.2#
68 7.4 5.3 7.9



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



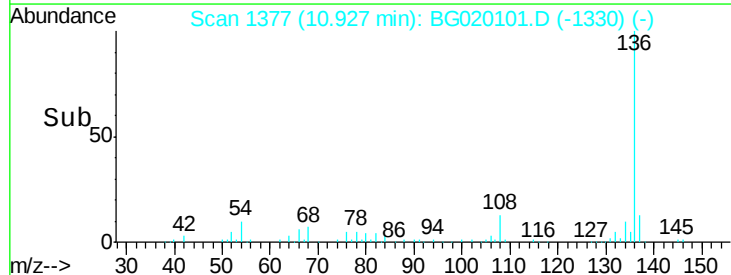
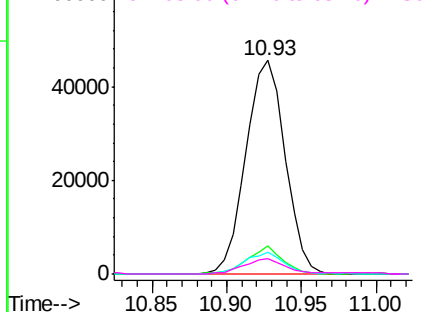




#23
Nitrobenzene-d5
Concen: 100.59 ng
RT: 9.28 min Scan# 1096
Delta R.T. -0.02 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39




Instrument :
BNA_G
ClientSampleId :


Tot Ion	82	Resp	163237
Ion Ratio	100	Lower	Upper
128	40.2	36.7	55.1
54	49.8	33.8	50.8

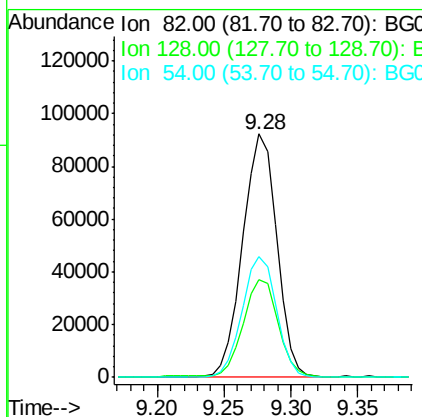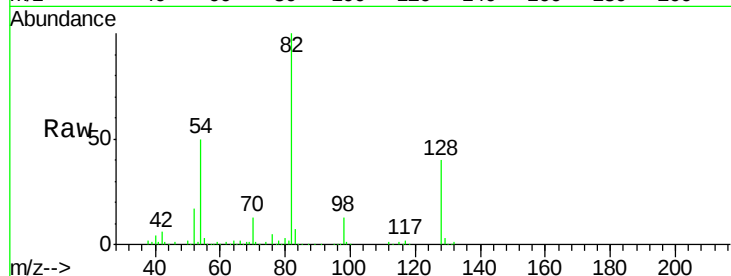

#24
Nitrobenzene
Concen: 2.91 ng
RT: 9.31 min Scan# 1101
Delta R.T. -0.04 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39

Tgt Ion	77	Resp	5130
Ion Ratio	100	Lower	Upper
123	0.0	38.2	57.2#
65	94.2	10.6	16.0#



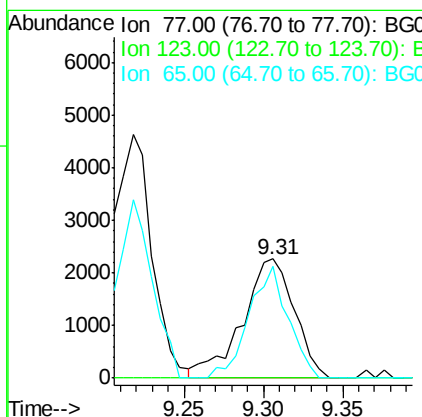



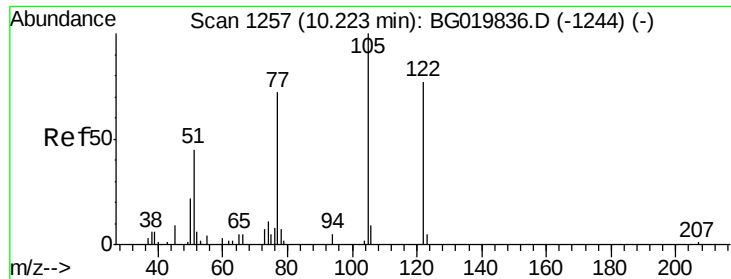

#32
Benzoic acid
Concen: 6.13 ng
RT: 10.13 min Scan# 1242
Delta R.T. -0.09 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
122	100		
105	449.8	103.8	143.8#
77	295.8	68.8	108.8#

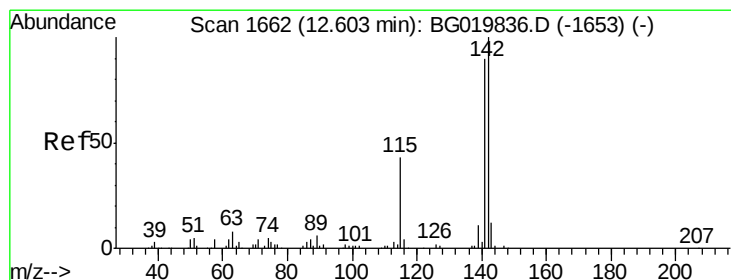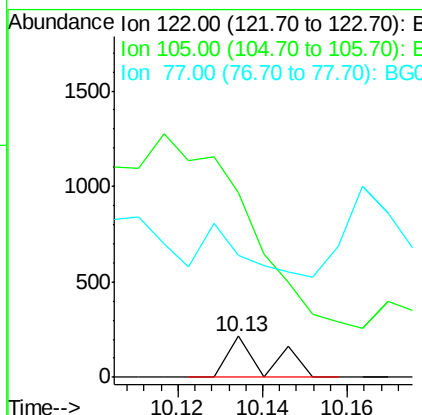

#37
2-Methylnaphthalene
Concen: 57.60 ng
RT: 12.80 min Scan# 1695
Delta R.T. 0.19 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39

Tgt Ion	Ratio	Lower	Upper
142	100		
141	95.0	74.6	112.0
115	44.3	27.4	41.0#

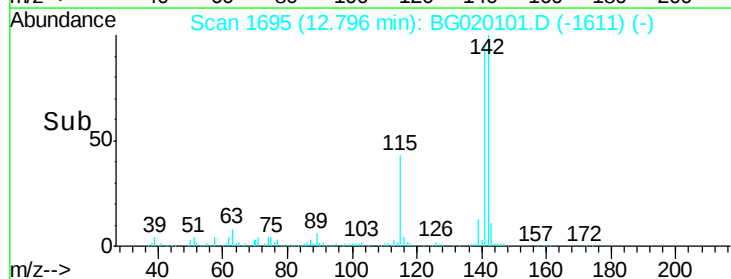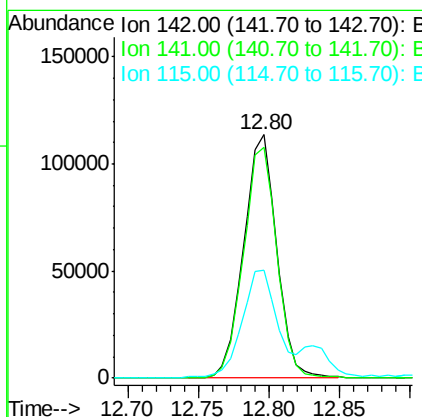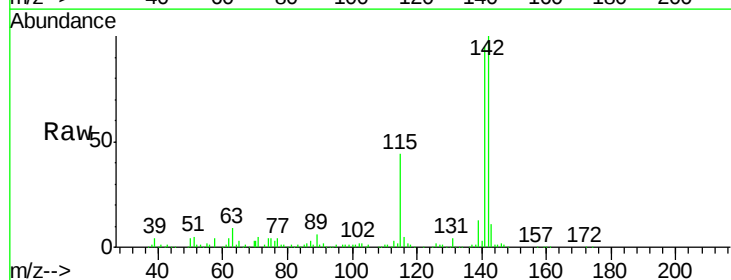

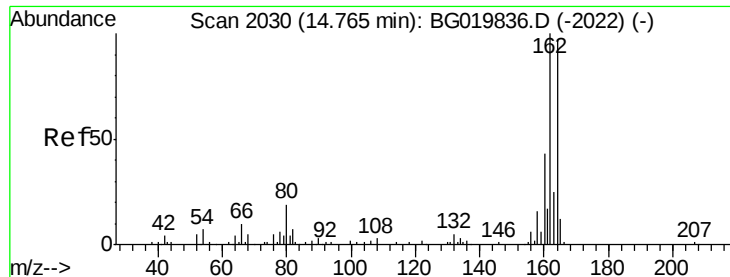

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.74 min Scan# 2026

Delta R.T. -0.02 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 73741

Ion Ratio Lower Upper

164 100

162 80.1 78.8 118.2




160 55.3 36.4 54.6#

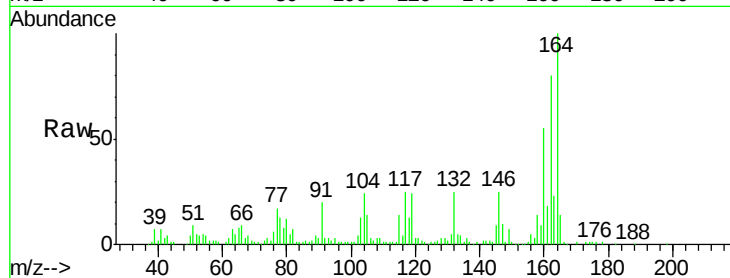

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

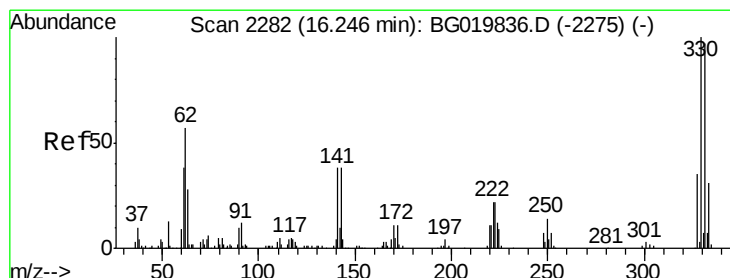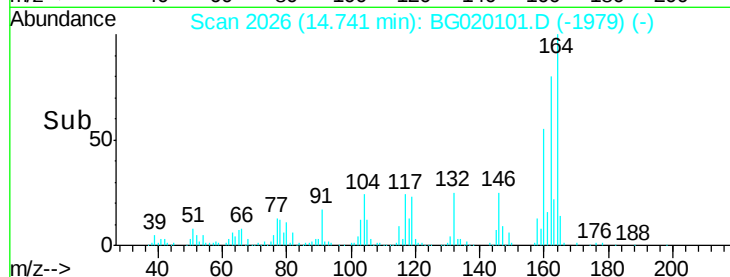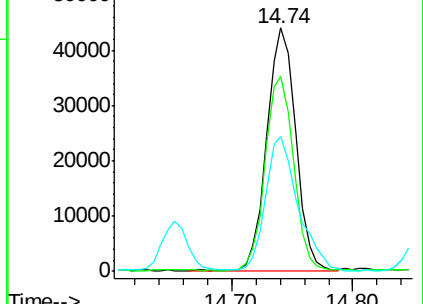

#41

2,4,6-Tribromophenol

Concen: 103.78 ng

RT: 16.23 min Scan# 2279

Delta R.T. -0.02 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39


Tgt Ion:330 Resp: 117098

Ion Ratio Lower Upper

330 100

332 95.8 78.1 117.1



141 36.1 28.2 42.2

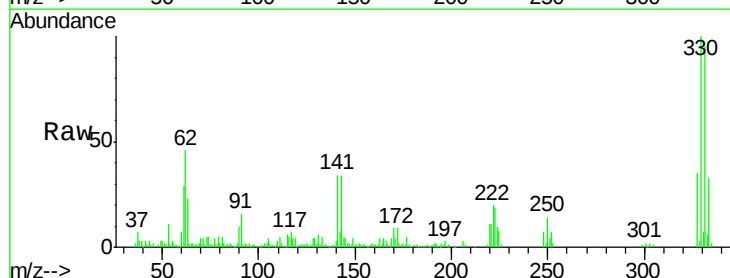


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



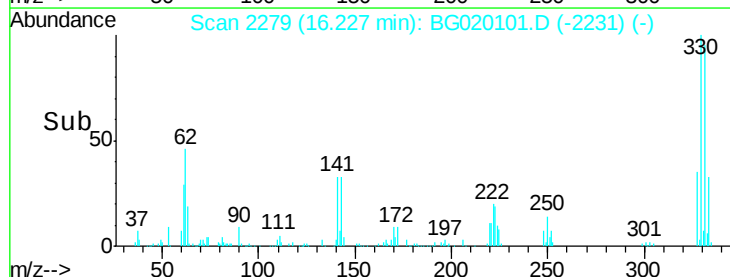
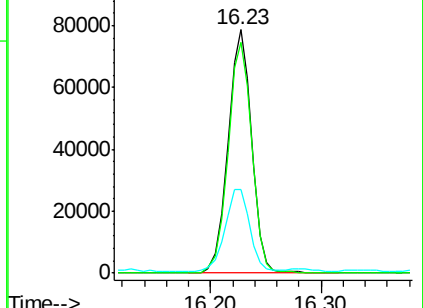




#44
 2-Fluorobiphenyl
 Concen: 70.98 ng
 RT: 13.37 min Scan# 1792
 Delta R.T. -0.02 min
 Lab File: BG020101.D
 Acq: 11 Dec 2015 8:39




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:172 Resp: 383351
 Ion Ratio Lower Upper
 172 100
 171 37.0 29.0 43.6
 170 24.5 19.9 29.9

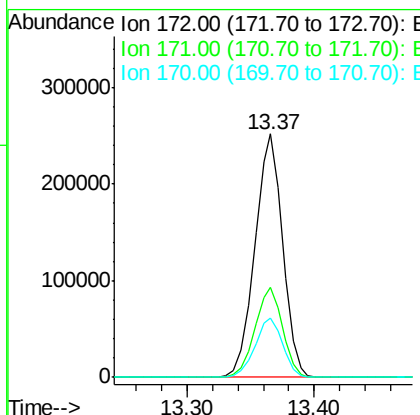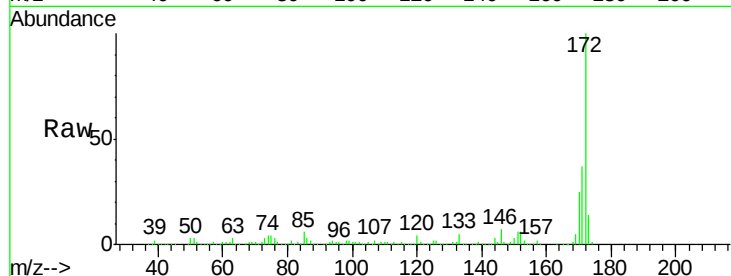

#53
 2,4-Dinitrophenol
 Concen: 9.34 ng
 RT: 14.91 min Scan# 2054
 Delta R.T. 0.05 min
 Lab File: BG020101.D
 Acq: 11 Dec 2015 8:39

Tgt Ion:184 Resp: 54
 Ion Ratio Lower Upper
 184 100
 63 3487.0 42.7 64.1#
 154 0.0 44.3 66.5#



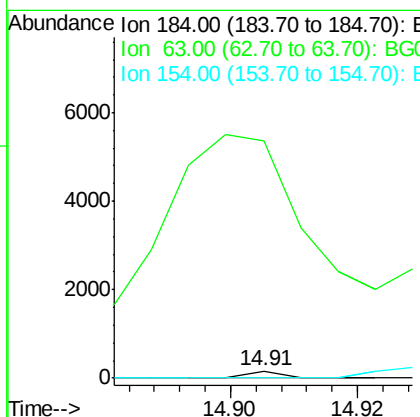





#59
Diethylphthalate
Concen: 10.79 ng
RT: 15.41 min Scan# 2140
Delta R.T. -0.17 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39




Instrument :
BNA_G
ClientSampleId :


Tot Ion:149 Resp: 77460
Ion Ratio Lower Upper
149 100
177 2.7 19.6 29.4#
150 37.0 10.2 15.2#

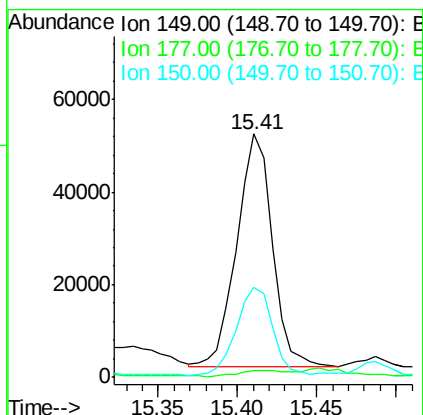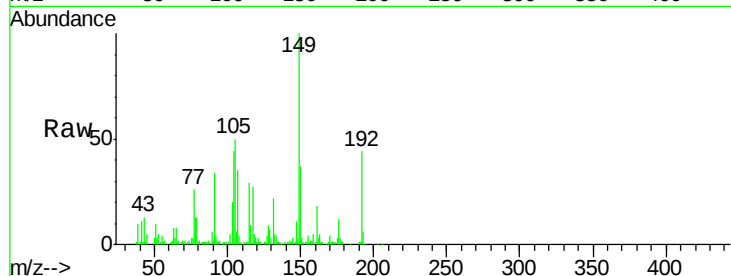

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.48 min Scan# 2492
Delta R.T. -0.03 min
Lab File: BG020101.D
Acq: 11 Dec 2015 8:39

Tgt Ion:188 Resp: 131057
Ion Ratio Lower Upper
188 100
94 6.9 7.7 11.5#
80 8.3 7.8 11.8

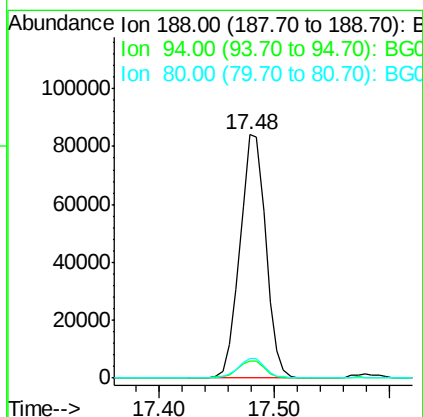

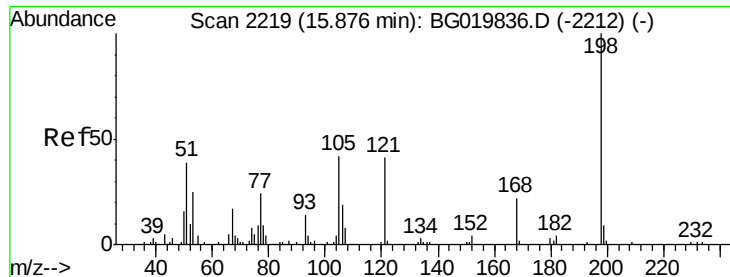

#64

4,6-Dinitro-2-methylphenol

Concen: 6.18 ng

RT: 15.82 min Scan# 2210

Delta R.T. -0.05 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39

Instrument :

BNA_G

ClientSampled :


Tot Ion:198 Resp: 60

Ion Ratio Lower Upper

198 100

51 1130.8 14.2 54.2#




105 2810.1 21.1 61.1#

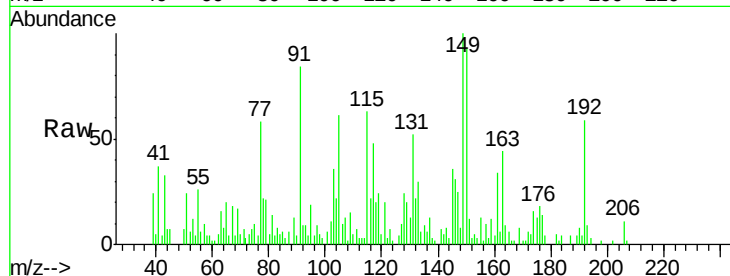

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG0

Ion 105.00 (104.70 to 105.70): E

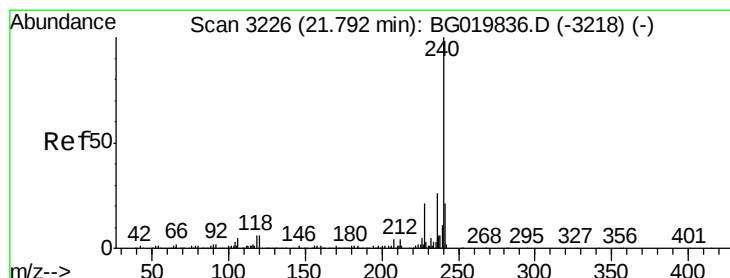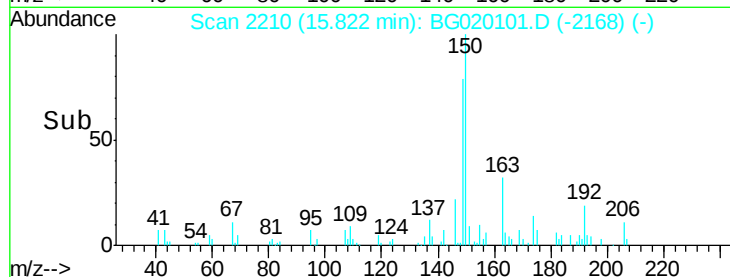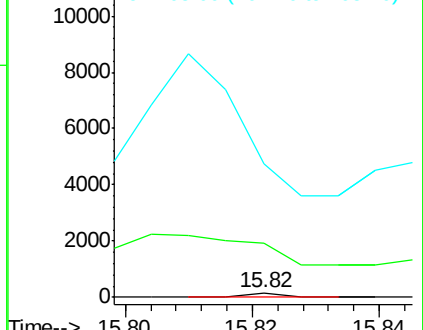

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.75 min Scan# 3219

Delta R.T. -0.04 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39


Tgt Ion:240 Resp: 167642

Ion Ratio Lower Upper

240 100

120 7.1 7.4 11.0#



236 26.1 20.7 31.1

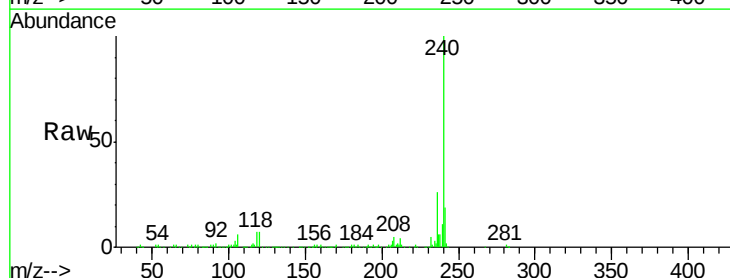


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

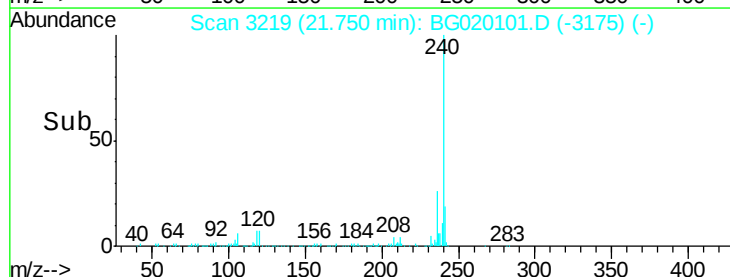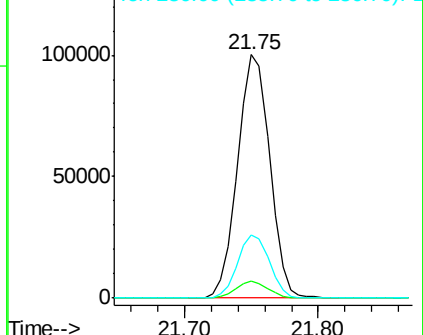



#78

Terphenyl-d14

Concen: 91.20 ng

RT: 20.08 min Scan# 2935

Delta R.T. -0.03 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 626822

Ion Ratio Lower Upper

244 100

212 8.2 6.9 10.3


122 7.9 10.2 15.2#

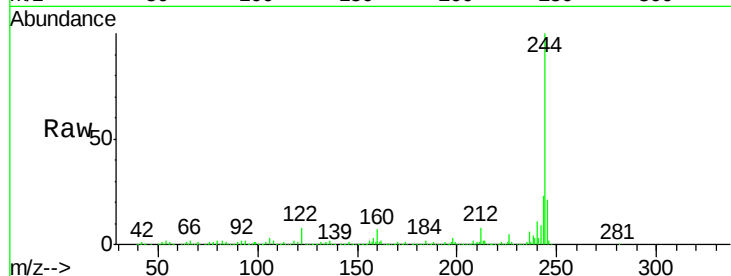



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

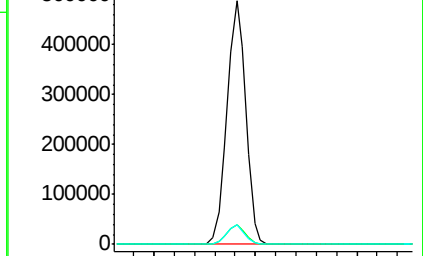

Time-->



#86

Perylene-d12

Concen: 20.00 ng

RT: 25.03 min Scan# 3777

Delta R.T. -0.07 min

Lab File: BG020101.D

Acq: 11 Dec 2015 8:39


Tgt Ion:264 Resp: 157019

Ion Ratio Lower Upper

264 100

260 25.1 18.5 27.7


265 19.8 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

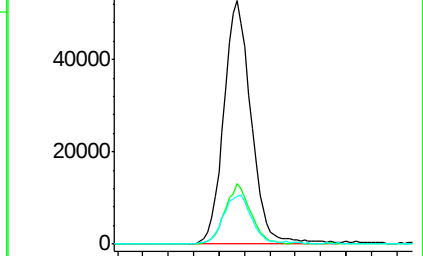

Time-->

