

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121115\
 Data File : BG020093.D
 Acq On : 11 Dec 2015 3:28
 Operator : UM/SJ
 Sample : PB87183BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB87183BL

Quant Time: Dec 11 04:51:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	16752	20.00	ng	-0.03
21) Naphthalene-d8	10.93	136	75853	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	52969	20.00	ng	-0.03
63) Phenanthrene-d10	17.48	188	129278	20.00	ng	-0.03
75) Chrysene-d12	21.75	240	159206	20.00	ng	-0.04
86) Perylene-d12	25.03	264	141869	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	117012	126.24	ng	-0.01
7) Phenol-d6	7.26	99	169263	120.95	ng	-0.02
23) Nitrobenzene-d5	9.28	82	110843	74.58	ng	-0.02
41) 2,4,6-Tribromophenol	16.22	330	84405	104.14	ng	-0.02
44) 2-Fluorobiphenyl	13.36	172	276364	71.24	ng	-0.03
78) Terphenyl-d14	20.08	244	492529	75.46	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121115\
Data File : BG020093.D
Acq On : 11 Dec 2015 3:28
Operator : UM/SJ
Sample : PB87183BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB87183BL

Quant Time: Dec 11 04:51:43 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

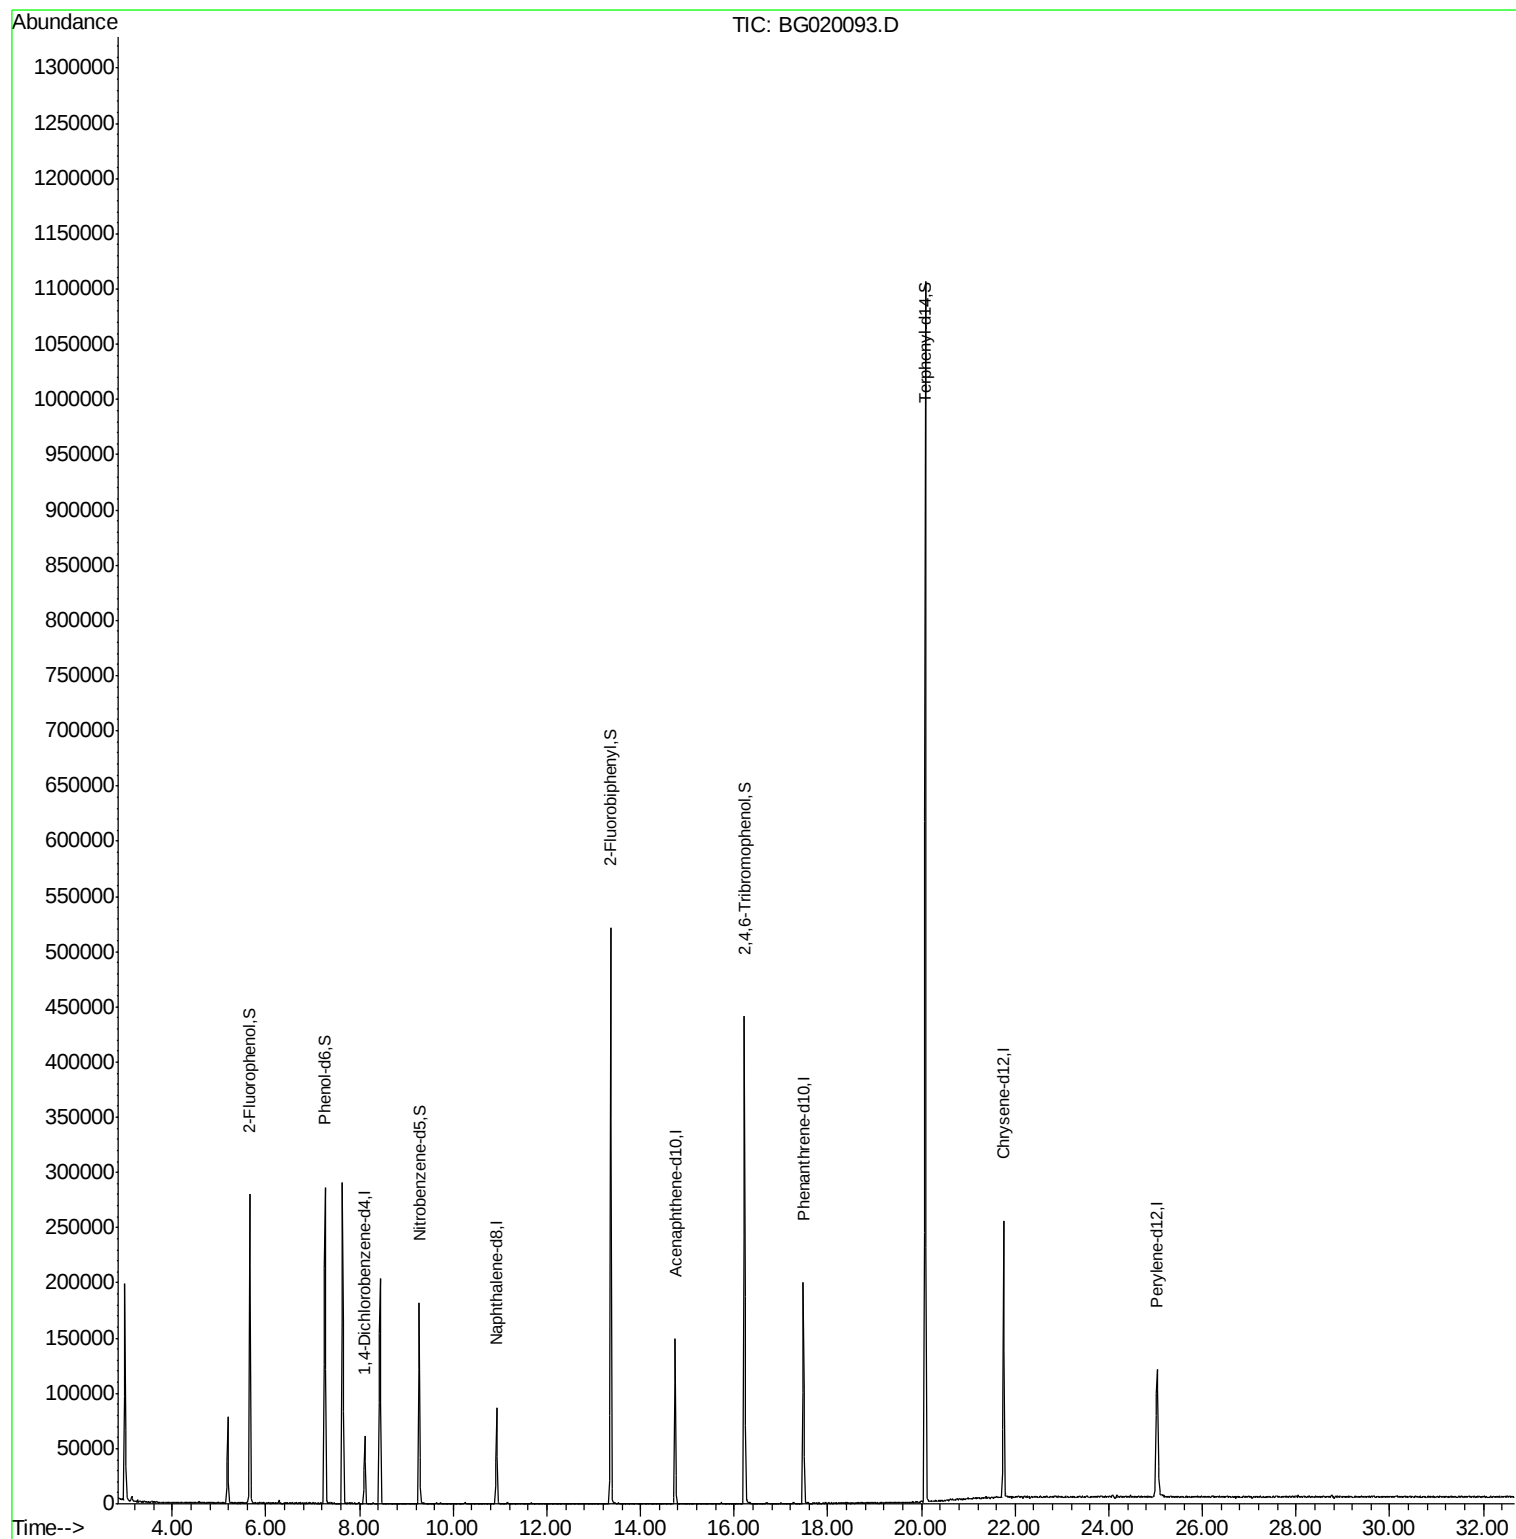

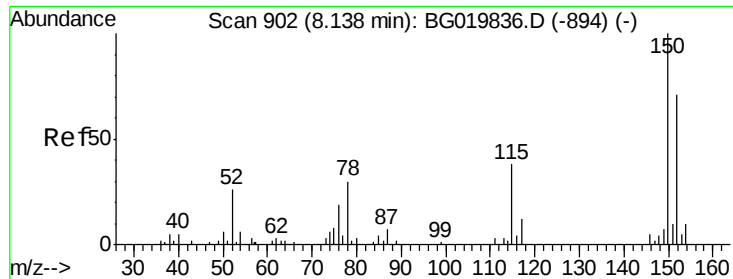


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.11 min Scan# 897
Delta R.T. -0.03 min
Lab File: BG020093.D
Acq: 11 Dec 2015 3:28

Instrument :
BNA_G
ClientSampleId :
PB87183BL

Tot Ion:152 Resp: 16752
Ion Ratio Lower Upper
152 100
150 154.8 115.0 172.4
115 58.7 43.9 65.9

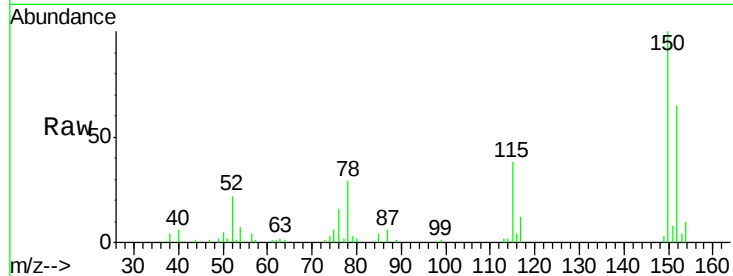


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

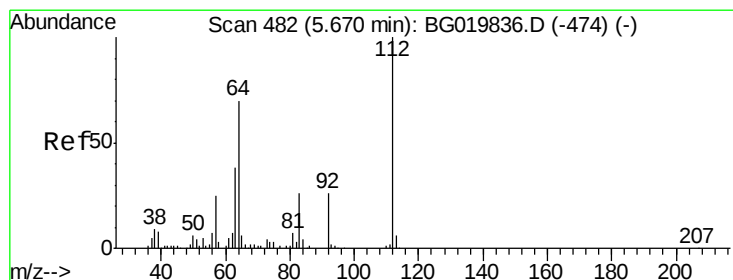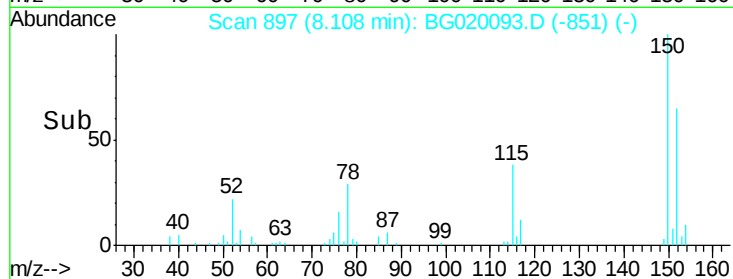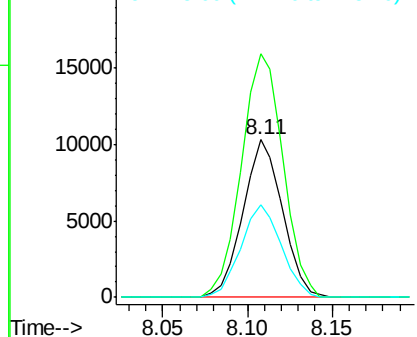



#5


2-Fluorophenol
Concen: 126.24 ng
RT: 5.66 min Scan# 480
Delta R.T. -0.01 min
Lab File: BG020093.D
Acq: 11 Dec 2015 3:28

Tgt Ion:112 Resp: 117012
Ion Ratio Lower Upper
112 100
64 64.2 43.7 65.5
63 35.9 24.0 36.0

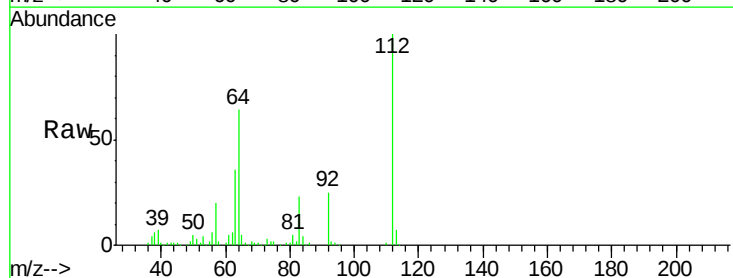

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

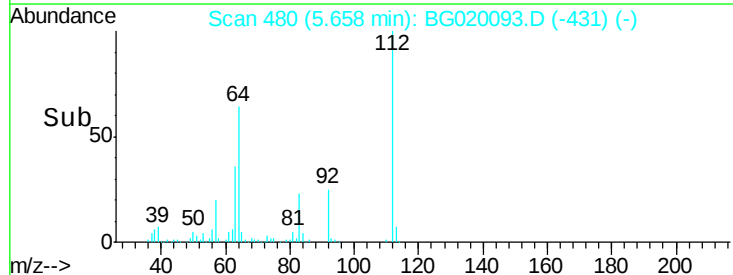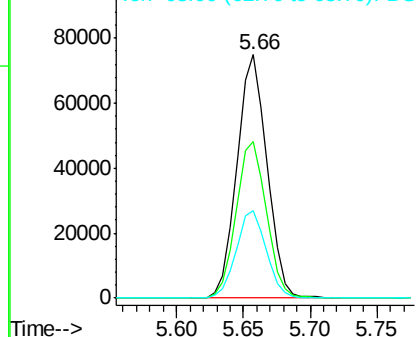

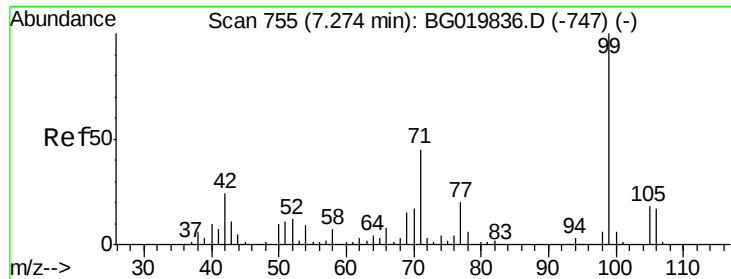

#7

Phenol-d6

Concen: 120.95 ng

RT: 7.26 min Scan# 752

Delta R.T. -0.02 min

Lab File: BG020093.D

Acq: 11 Dec 2015 3:28

Instrument :

BNA_G

ClientSampleId :

PB87183BL


Tot Ion: 99 Resp: 169263

Ion Ratio Lower Upper

99 100

42 19.0 11.5 17.3#




71 39.2 22.6 34.0#

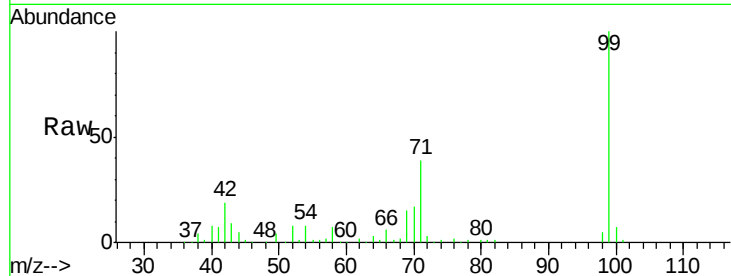

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

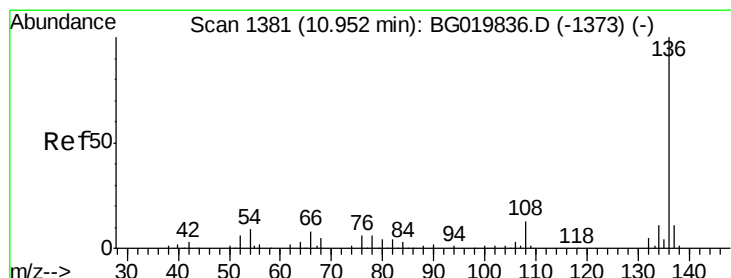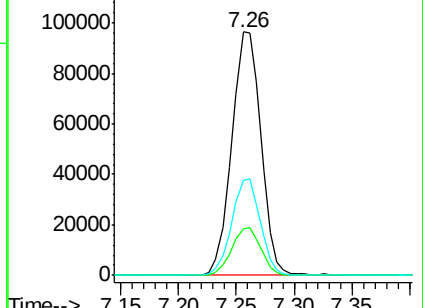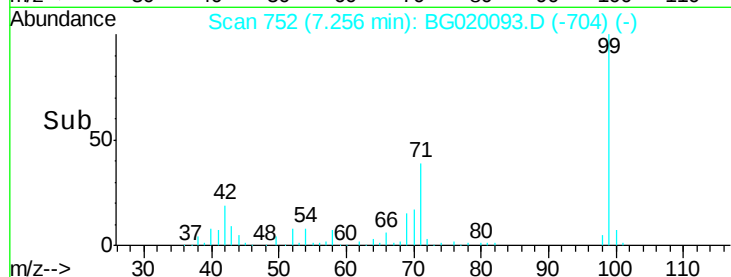

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.02 min

Lab File: BG020093.D

Acq: 11 Dec 2015 3:28

Tgt Ion: 136 Resp: 75853


Ion Ratio Lower Upper

136 100

137 11.6 8.6 12.8

54 8.5 5.4 8.2#

68 5.3 5.3 7.9


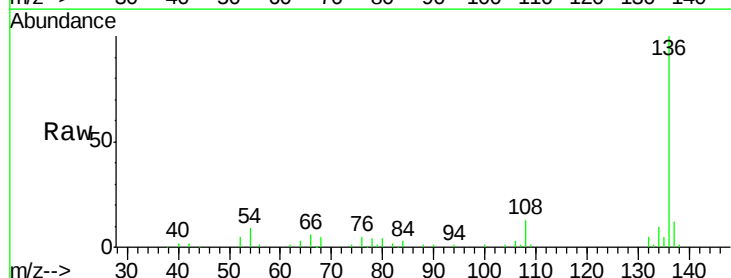



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



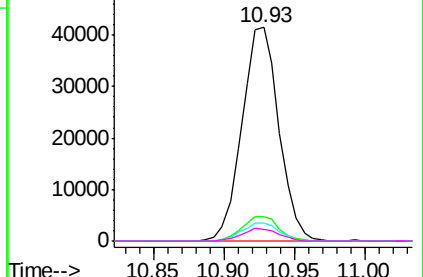
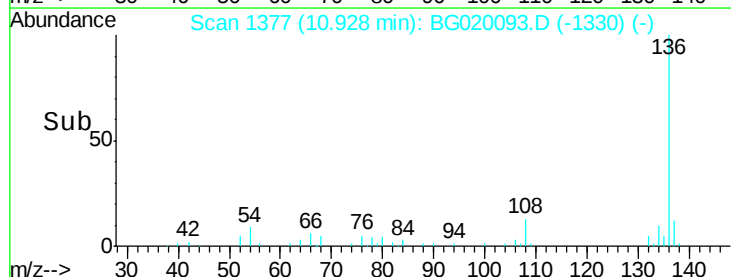


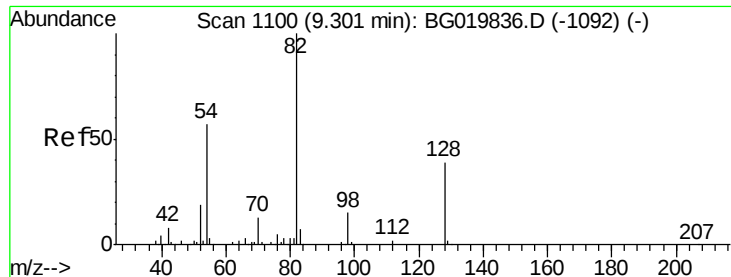

#23
 Nitrobenzene-d5
 Concen: 74.58 ng
 RT: 9.28 min Scan# 1096
 Delta R.T. -0.02 min
 Lab File: BG020093.D
 Acq: 11 Dec 2015 3:28




Instrument :
 BNA_G
 ClientSampleId :
 PB87183BL


Tot Ion	82	Resp	110843
Ion Ratio	Lower	Upper	
82	100		
128	39.7	36.7	55.1
54	48.4	33.8	50.8

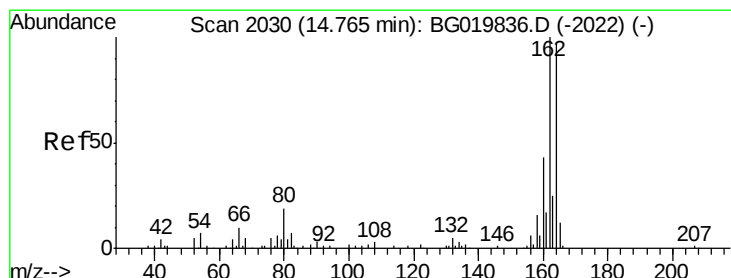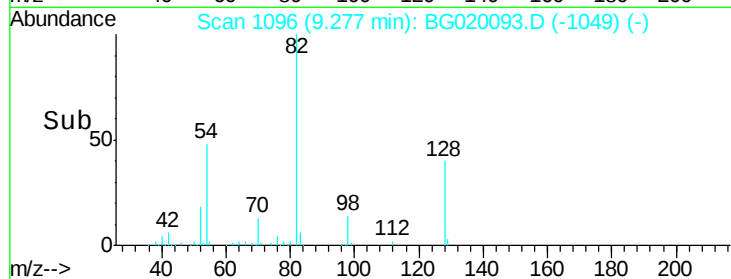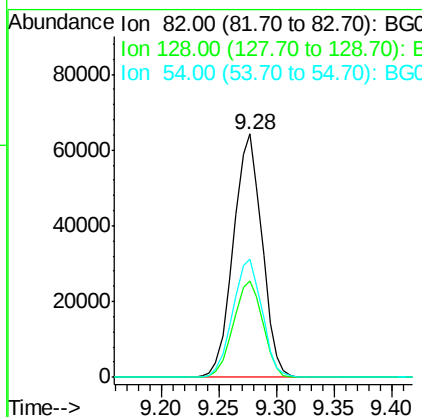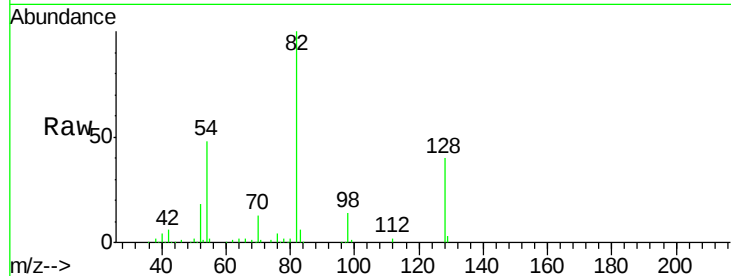

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.74 min Scan# 2025
 Delta R.T. -0.03 min
 Lab File: BG020093.D
 Acq: 11 Dec 2015 3:28

Tgt Ion	164	Resp	52969
Ion Ratio	Lower	Upper	
164	100		
162	105.8	78.8	118.2
160	47.0	36.4	54.6

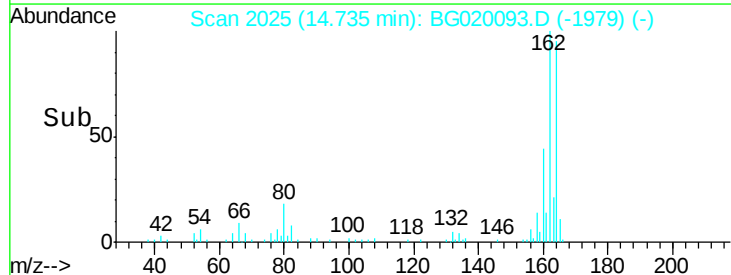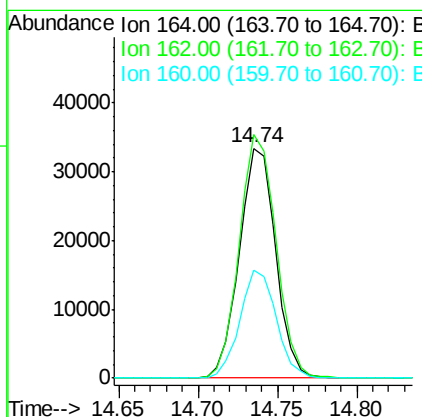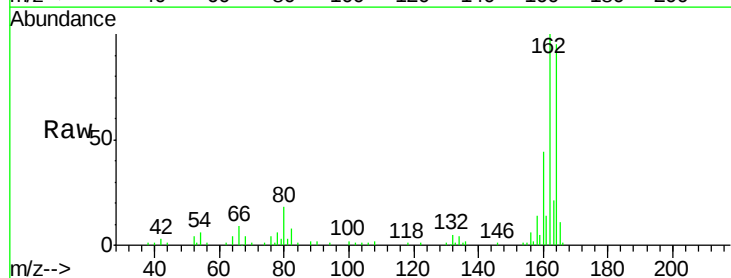


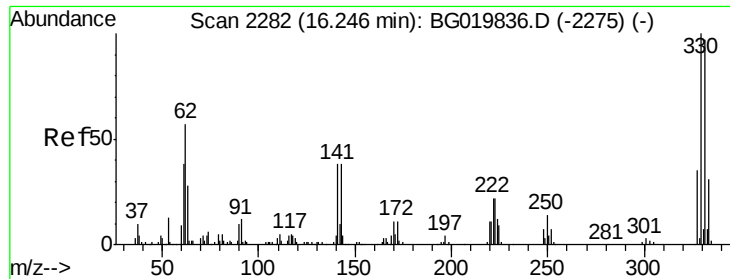




#41
 2,4,6-Tribromophenol
 Concen: 104.14 ng
 RT: 16.22 min Scan# 2278
 Delta R.T. -0.02 min
 Lab File: BG020093.D
 Acq: 11 Dec 2015 3:28

Instrument :
 BNA_G
 ClientSampleId :
 PB87183BL

Tot Ion:330 Resp: 84405
 Ion Ratio Lower Upper
 330 100
 332 96.5 78.1 117.1
 141 35.8 28.2 42.2

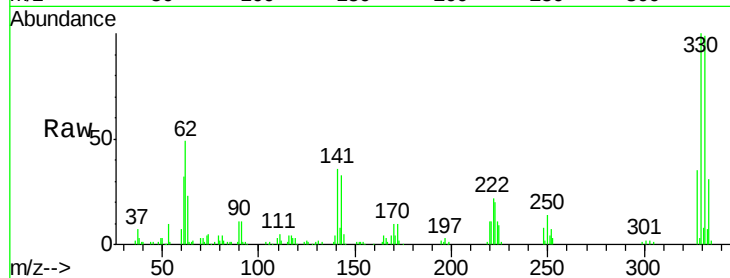


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

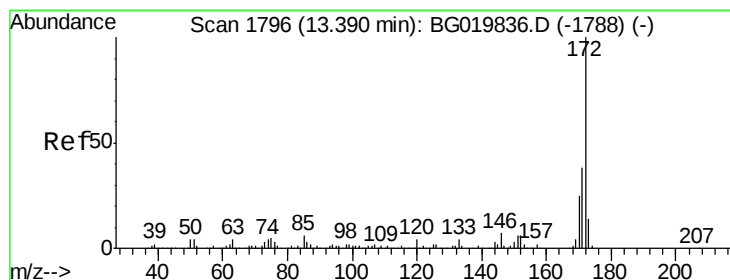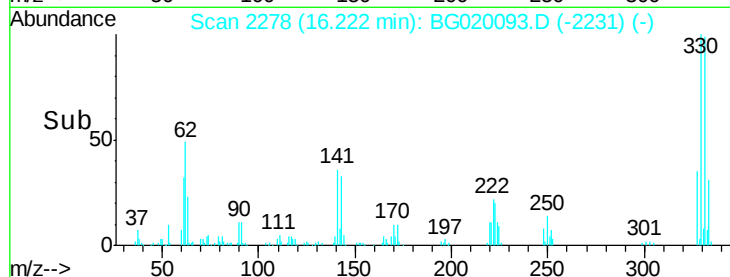
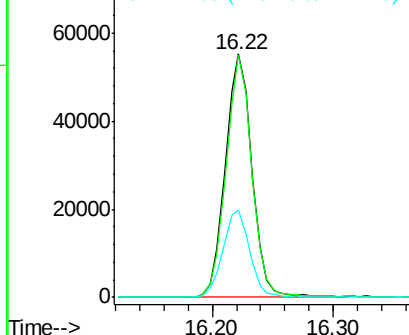



#44
 2-Fluorobiphenyl
 Concen: 71.24 ng
 RT: 13.36 min Scan# 1791
 Delta R.T. -0.03 min
 Lab File: BG020093.D
 Acq: 11 Dec 2015 3:28

Tgt Ion:172 Resp: 276364
 Ion Ratio Lower Upper
 172 100
 171 37.1 29.0 43.6
 170 24.5 19.9 29.9

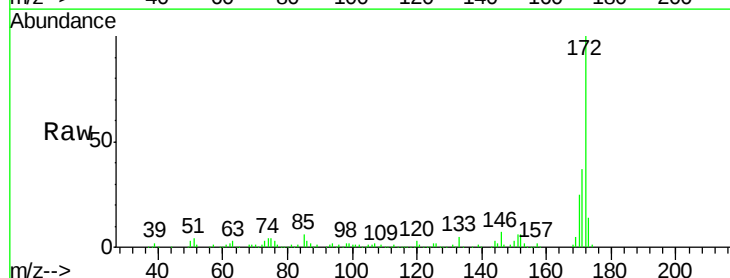

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

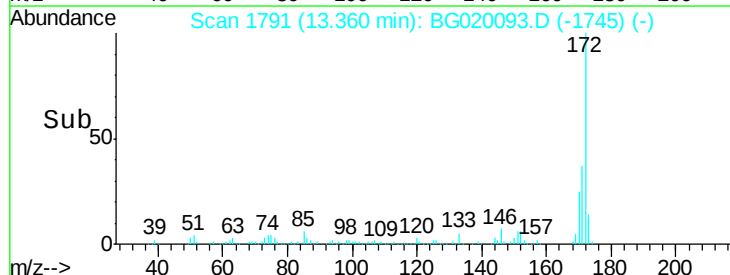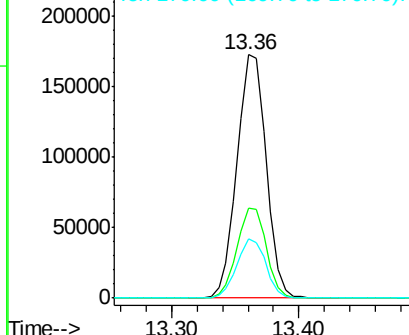

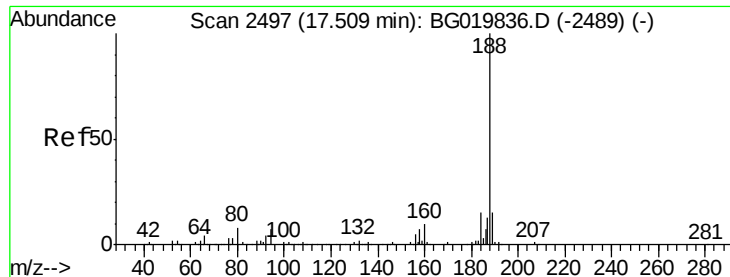

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.48 min Scan# 2492

Delta R.T. -0.03 min

Lab File: BG020093.D

Acq: 11 Dec 2015 3:28

Instrument :

BNA_G

ClientSampleId :

PB87183BL


Tot Ion:188 Resp: 129278

Ion Ratio Lower Upper

188 100

94 7.3 7.7 11.5#




80 8.5 7.8 11.8

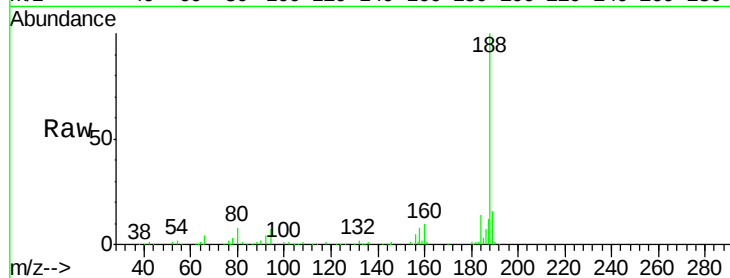

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

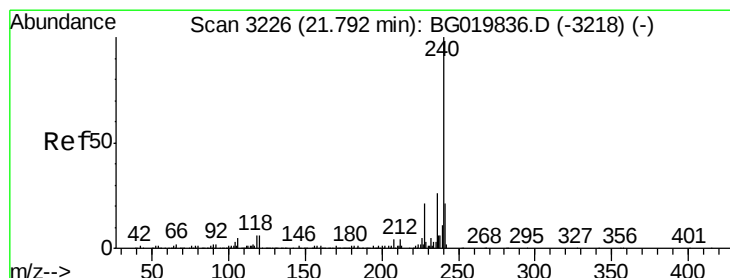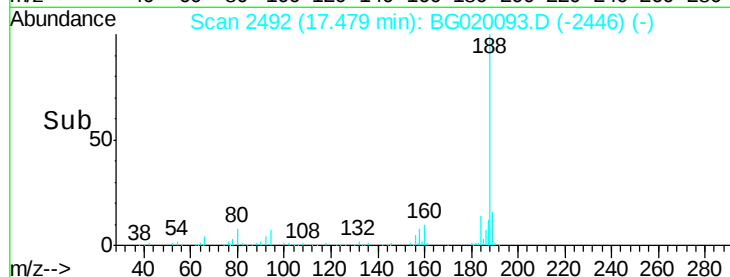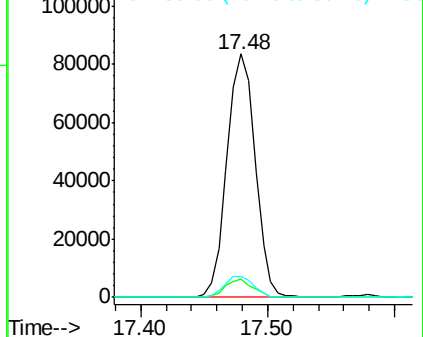

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.75 min Scan# 3219

Delta R.T. -0.04 min

Lab File: BG020093.D

Acq: 11 Dec 2015 3:28


Tgt Ion:240 Resp: 159206

Ion Ratio Lower Upper

240 100

120 6.9 7.4 11.0#



236 26.3 20.7 31.1

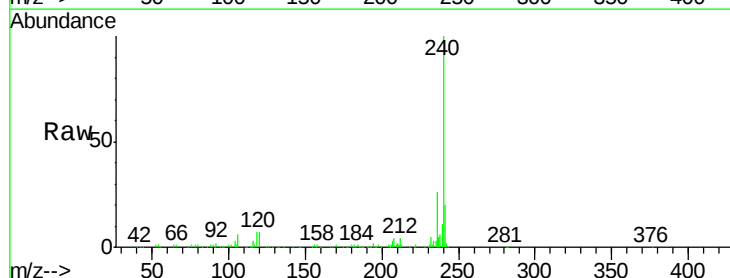


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

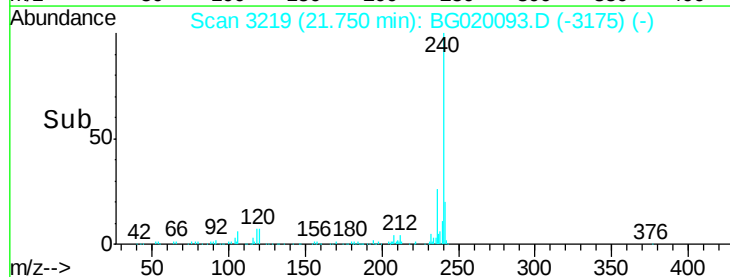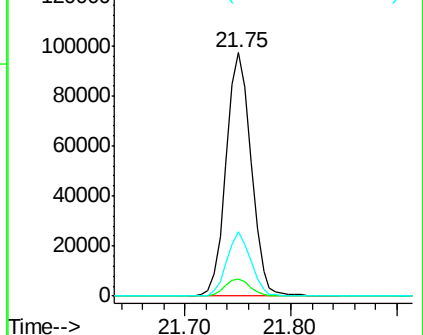

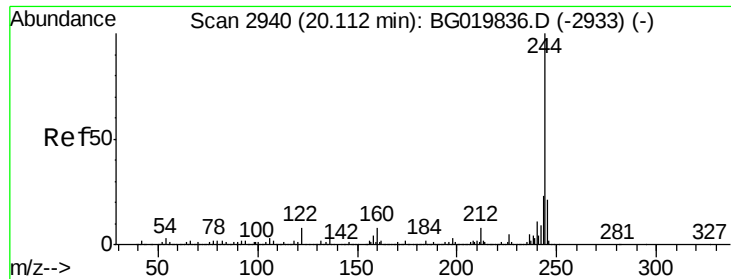

#78

Terphenyl-d14

Concen: 75.46 ng

RT: 20.08 min Scan# 2935

Delta R.T. -0.03 min

Lab File: BG020093.D

Acq: 11 Dec 2015 3:28

Instrument :

BNA_G

ClientSampleId :

PB87183BL


Tot Ion:244 Resp: 492529

Ion Ratio Lower Upper




244 100

212 7.6 6.9 10.3

122 7.0 10.2 15.2#

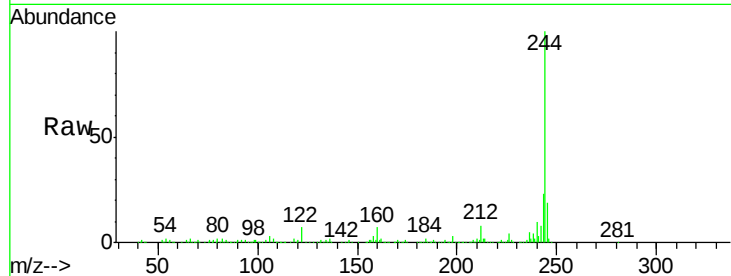

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

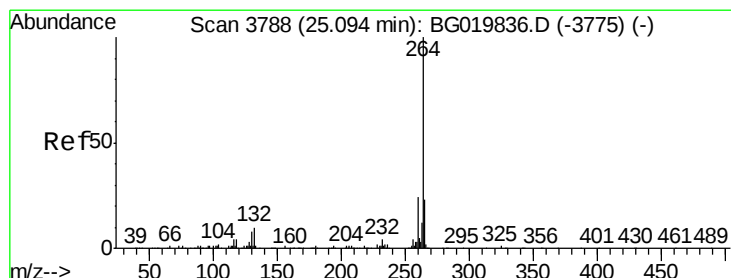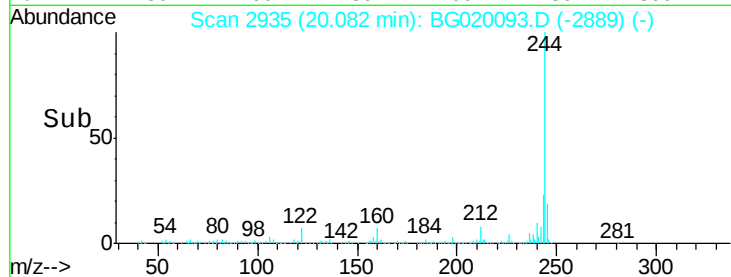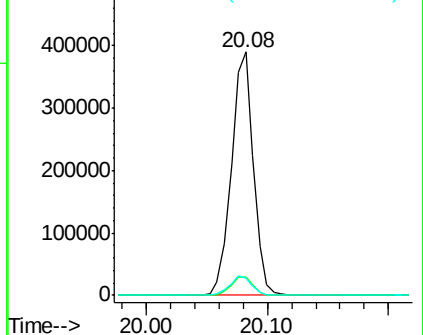

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.03 min Scan# 3777

Delta R.T. -0.07 min

Lab File: BG020093.D

Acq: 11 Dec 2015 3:28


Tgt Ion:264 Resp: 141869

Ion Ratio Lower Upper

264 100

260 23.1 18.5 27.7

265 21.0 17.2 25.8

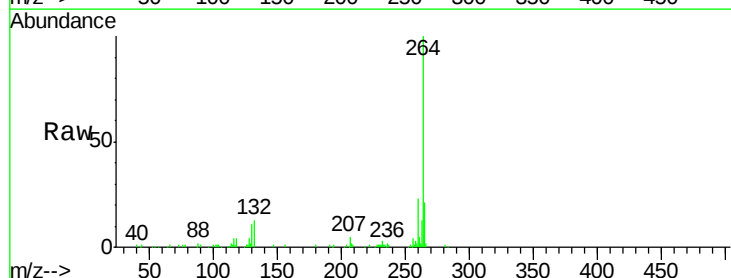

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

