


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG121117\
 Data File : BG031451.D
 Acq On : 11 Dec 2017 12:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 11 17:25:55 2017

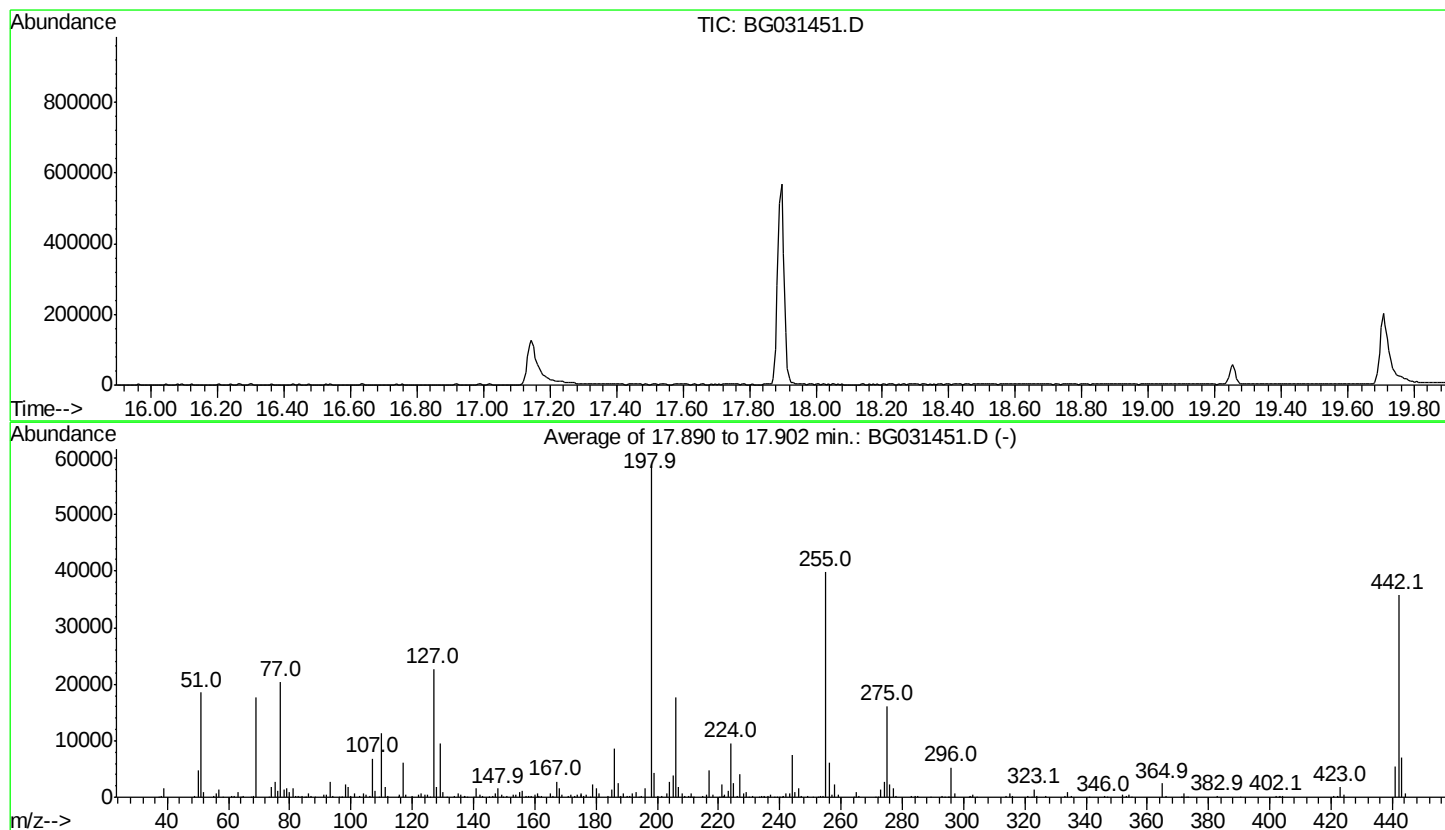

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	18552	PASS
68	69	0.00	2	1.8	323	PASS
69	198	0.00	100	30.2	17717	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.6	22656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58642	PASS
199	198	5	9	7.3	4284	PASS
275	198	10	60	27.6	16162	PASS
365	198	1	100	4.1	2407	PASS
441	442	0.01	24	15.1	5400	PASS
442	198	50	100	61.1	35842	PASS
443	442	15	24	19.4	6939	PASS