




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

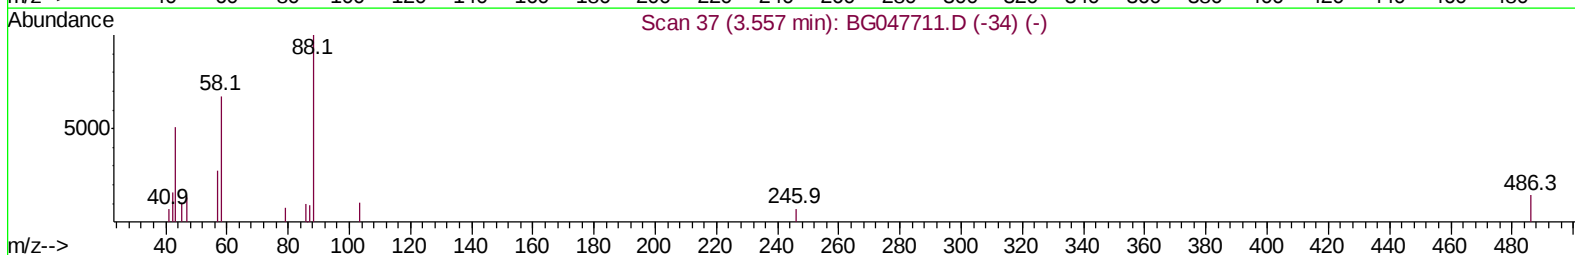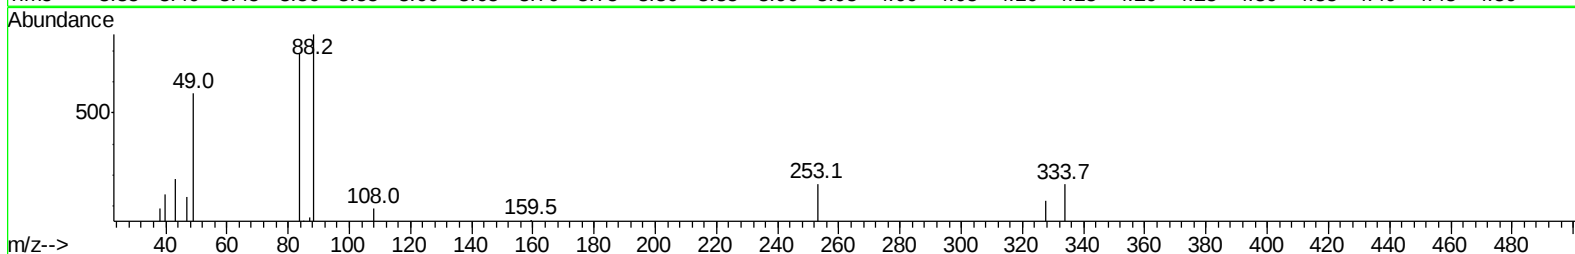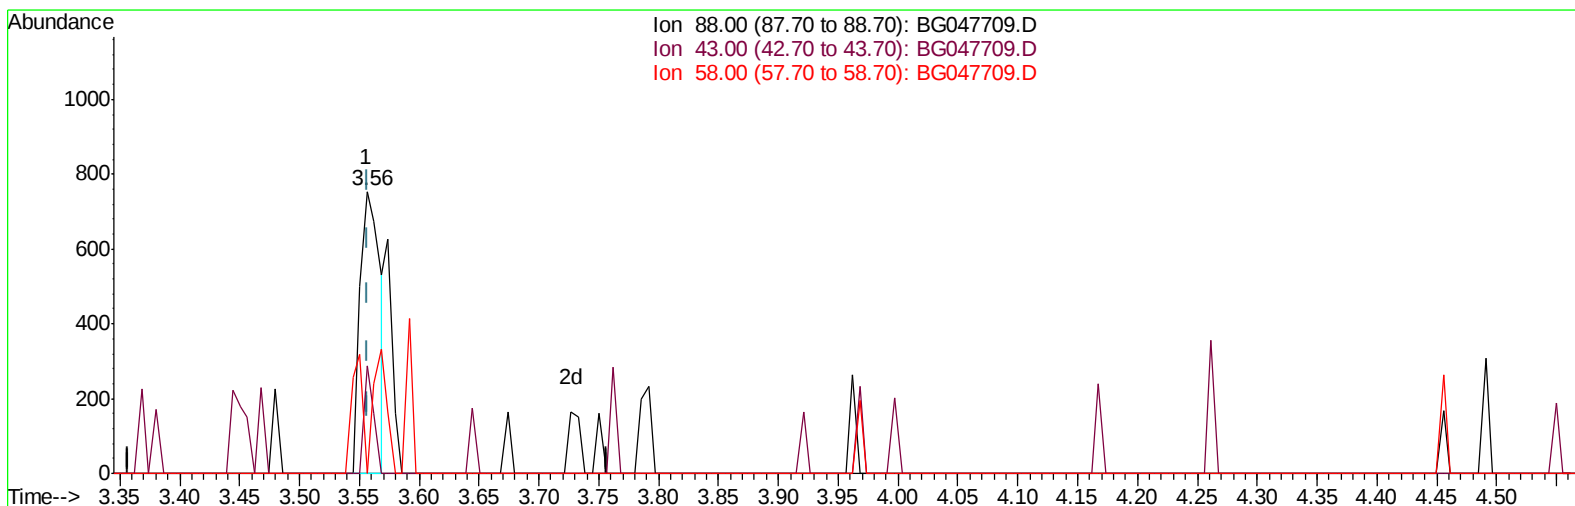

TIC: BG047709.D

(2) 1,4-Dioxane

3.556min (-0.001) 1.91ng/uL

response 868

Ion	Exp%	Act%
88.00	100	100
43.00	50.80	38.25#
58.00	67.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SST00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

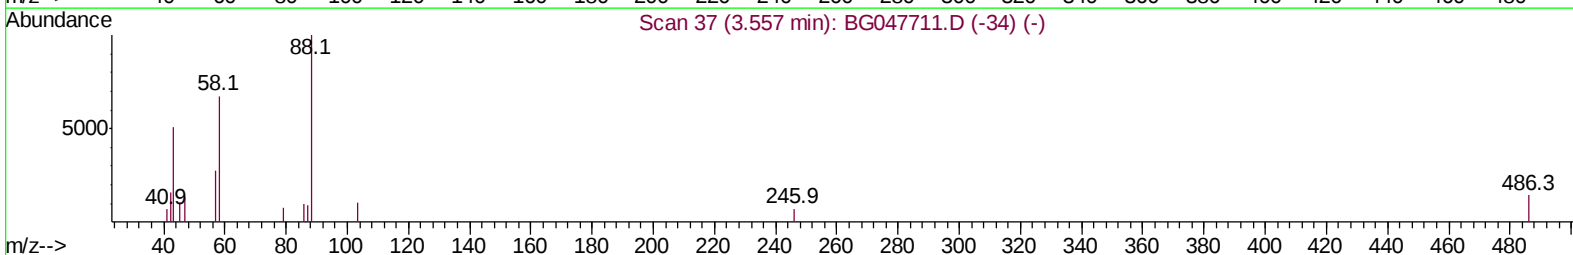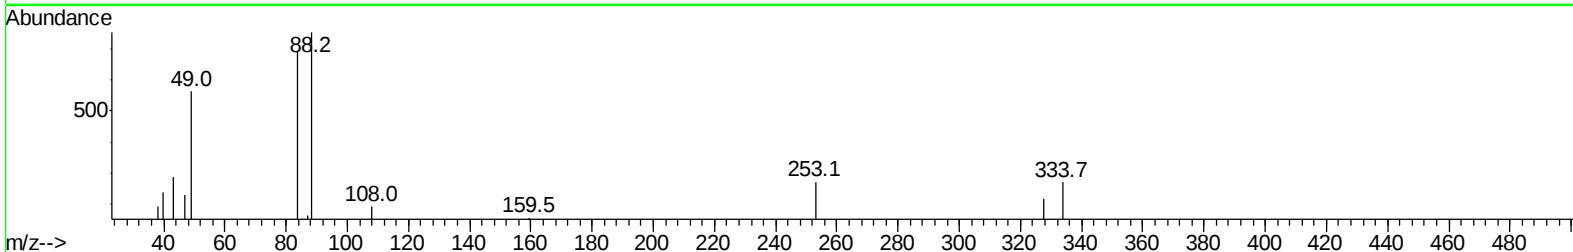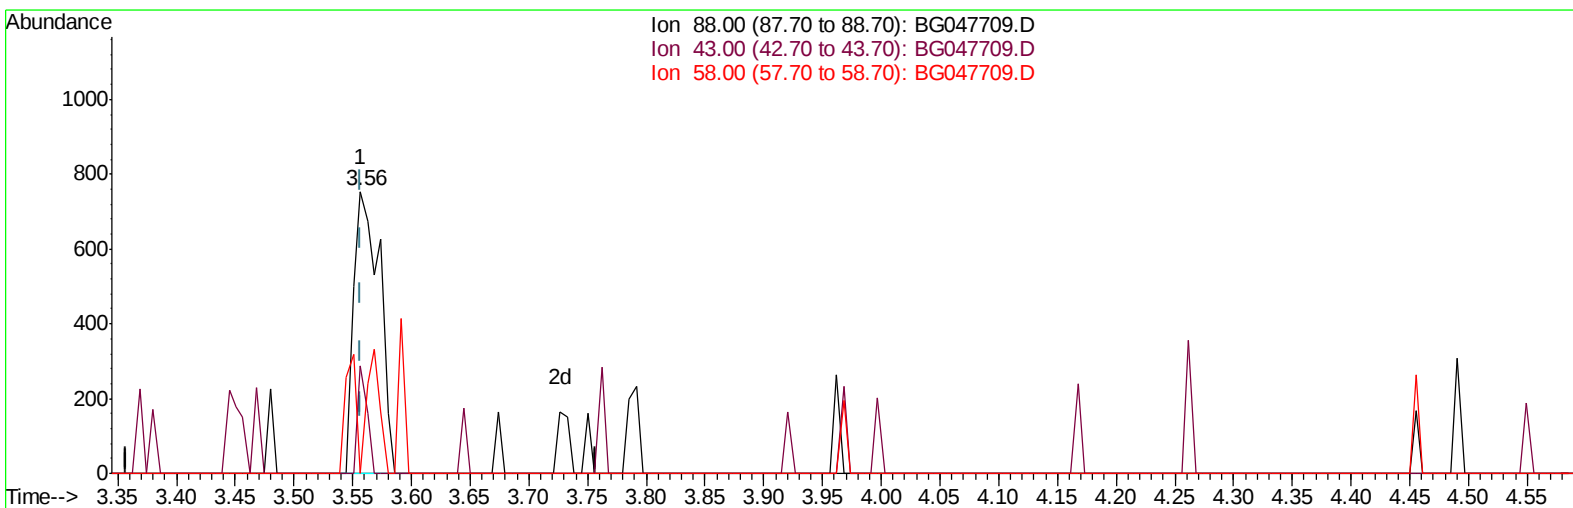

TIC: BG047709.D

(2) 1,4-Dioxane

3.556min (-0.001) 2.52ng/uL m

response 1145

Ion	Exp%	Act%
88.00	100	100
43.00	50.80	38.25#
58.00	67.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

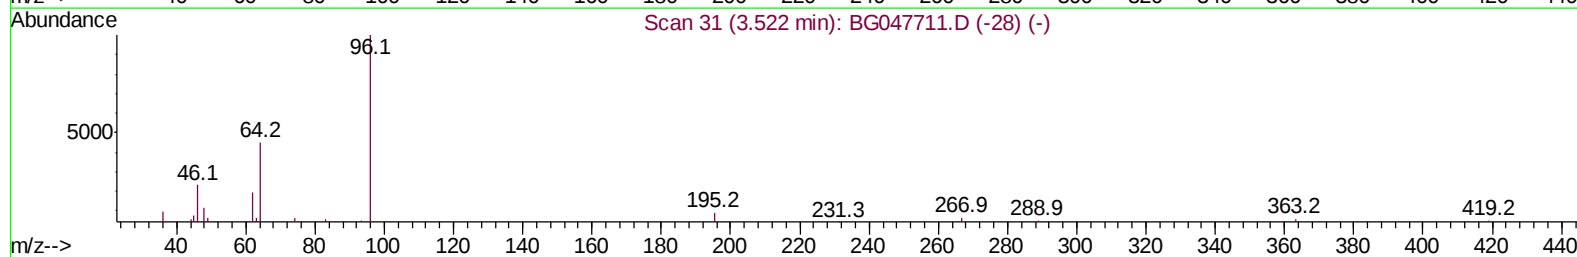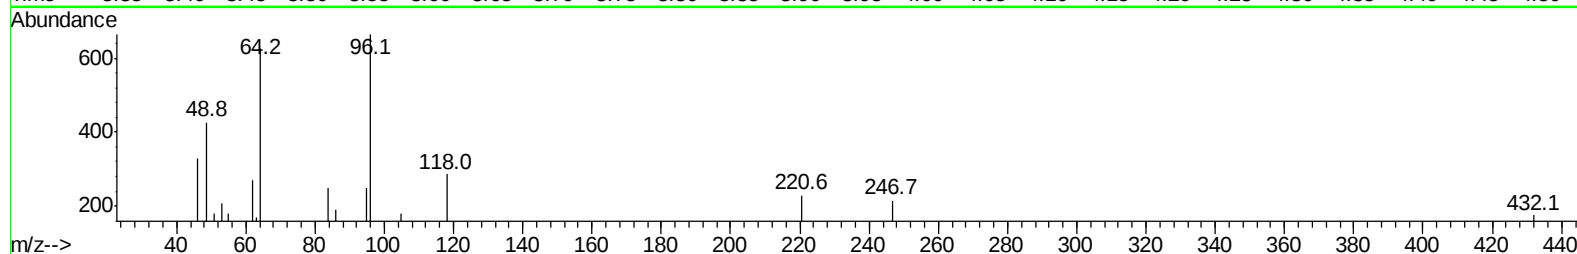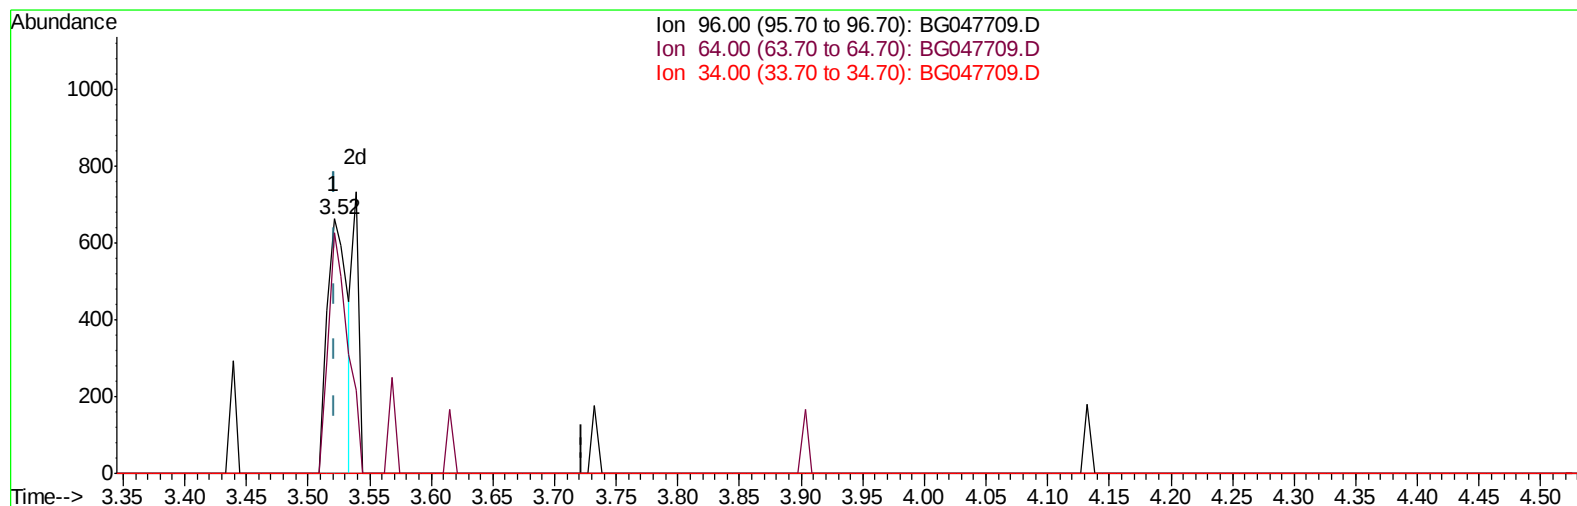

TIC: BG047709.D

(3) 1,4-Dioxane-d8 (S)

3.521min (-0.001) 1.71ng/uL

response 750

Ion	Exp%	Act%
96.00	100	100
64.00	56.60	94.43#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

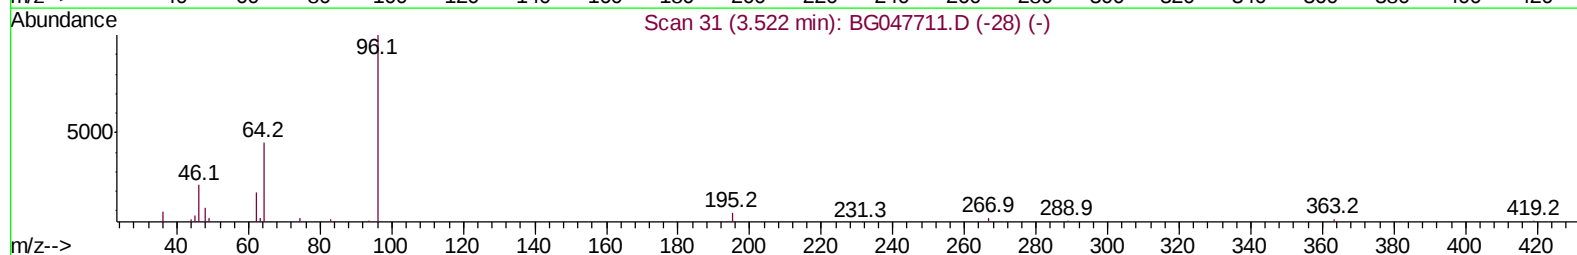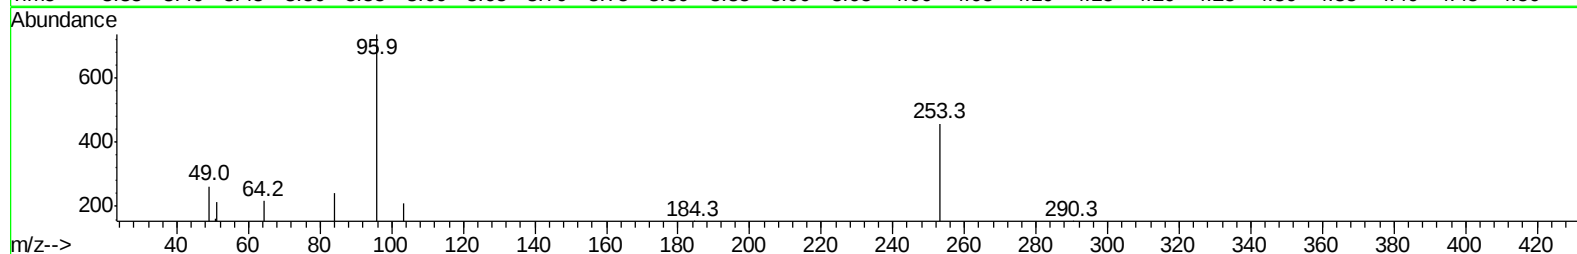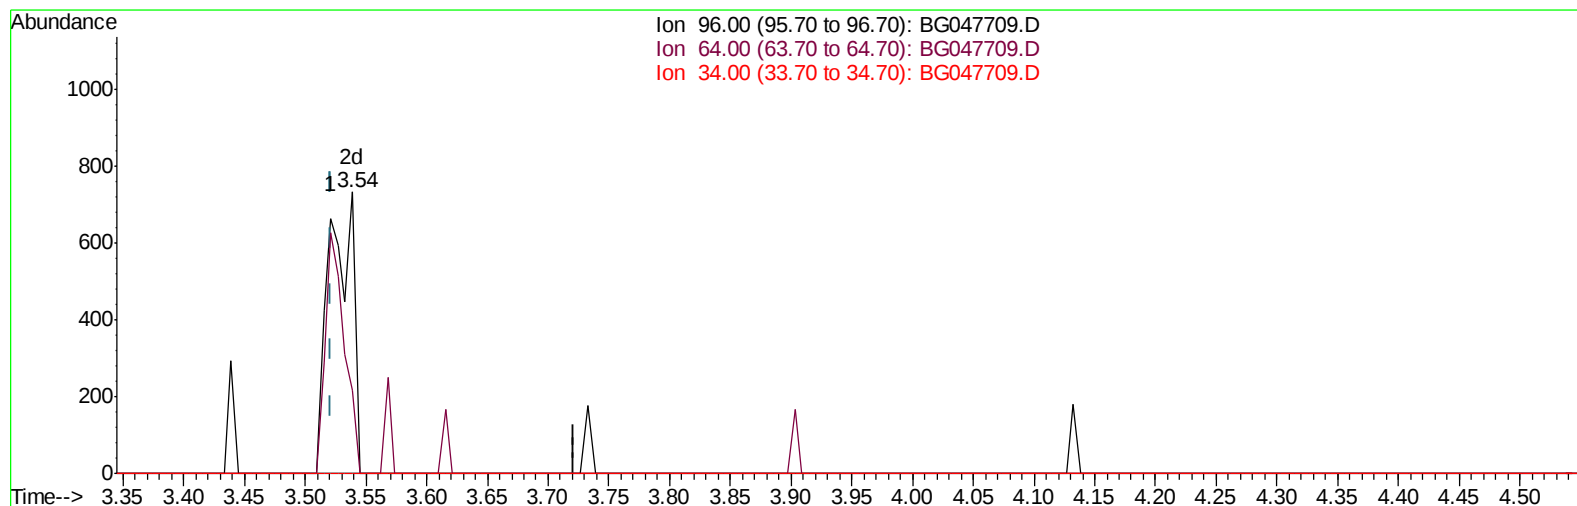

TIC: BG047709.D

(3) 1,4-Dioxane-d8 (S)

3.539min (+0.017) 2.30ng/uL m

response 1009

Ion	Exp%	Act%
96.00	100	100
64.00	56.60	29.43#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SSTD00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

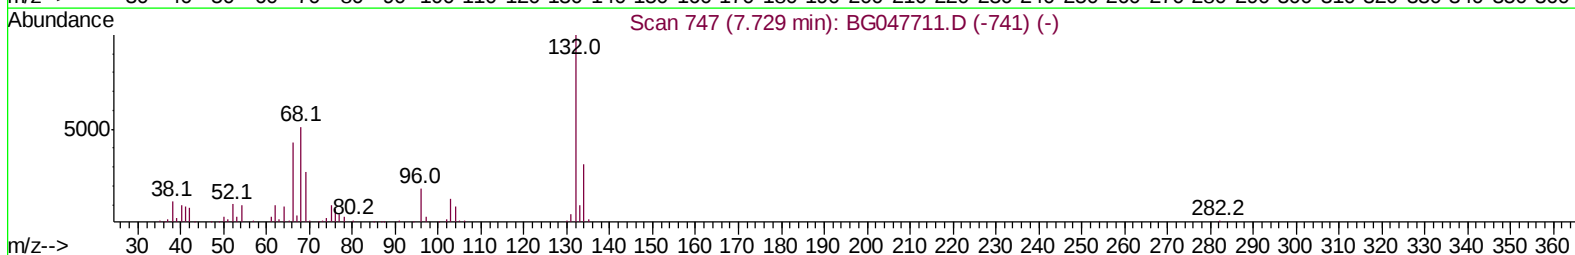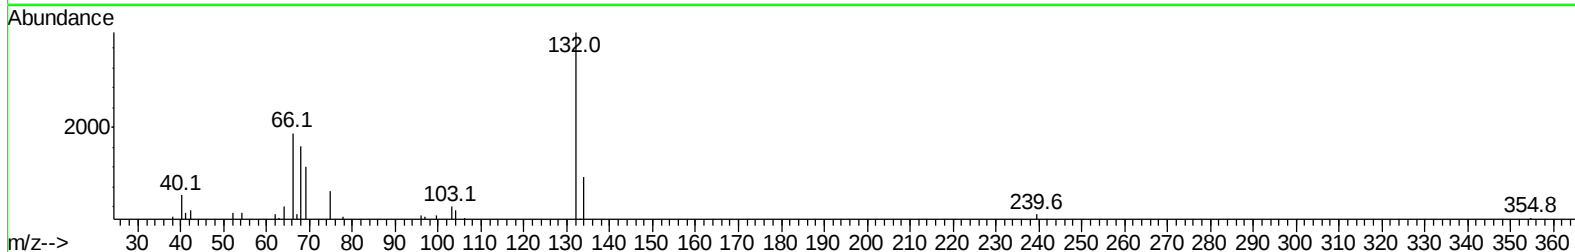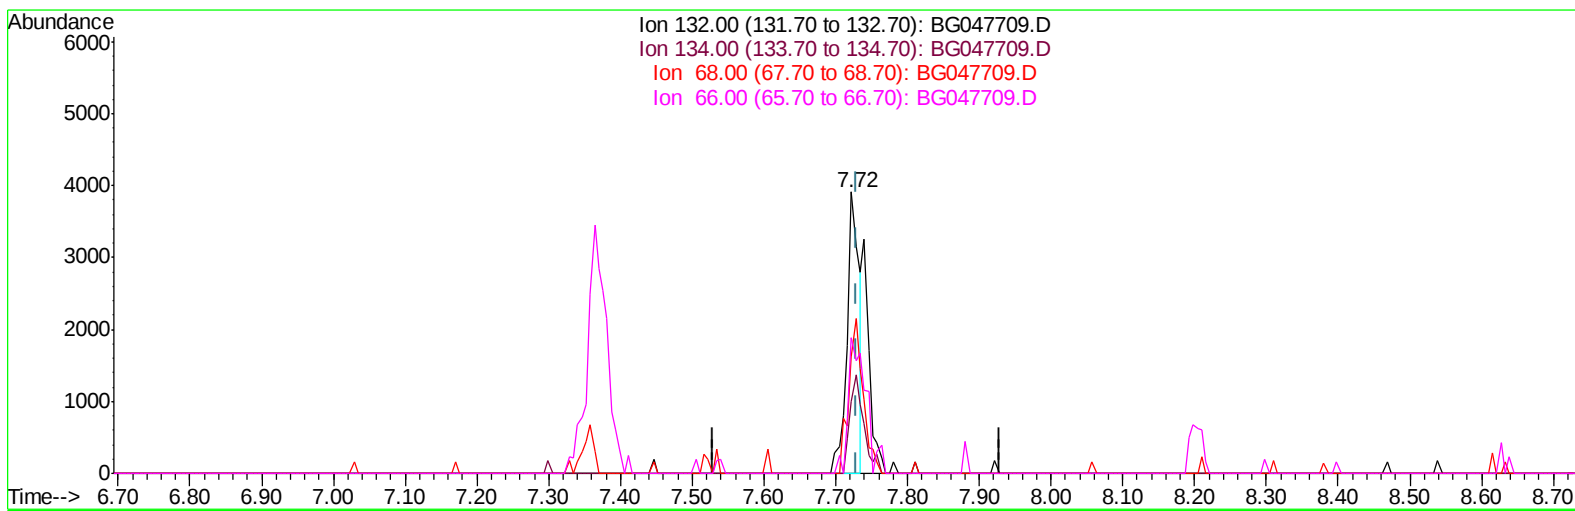

TIC: BG047709.D

(11) 2-Chlorophenol-d4 (S)

7.722min (-0.007) 3.44ng/ul

response 4613

Ion	Exp%	Act%
132.00	100	100
134.00	31.40	25.42
68.00	51.30	41.21
66.00	43.10	48.24




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

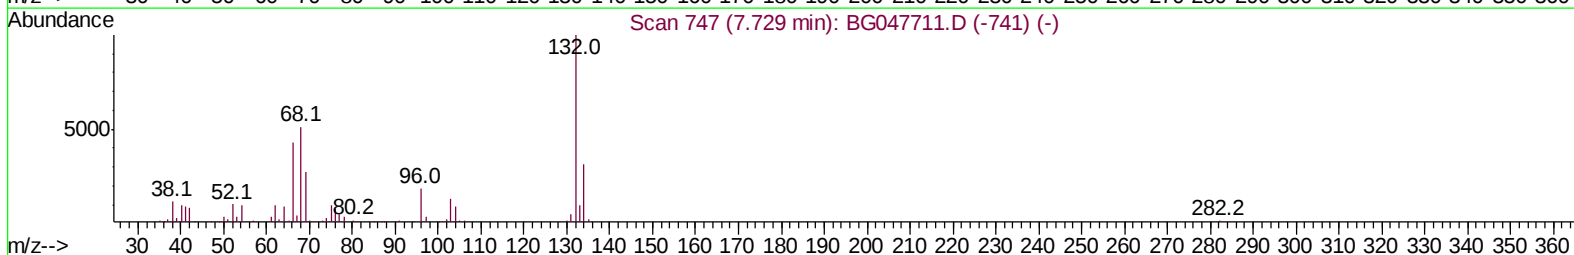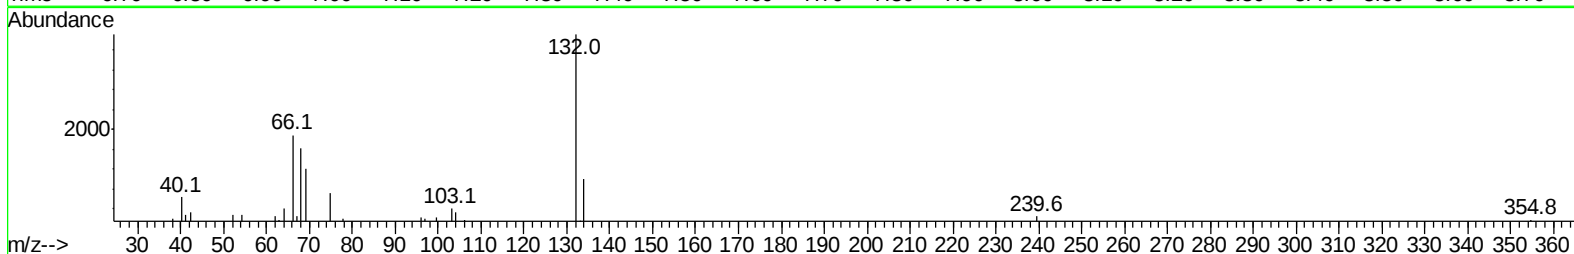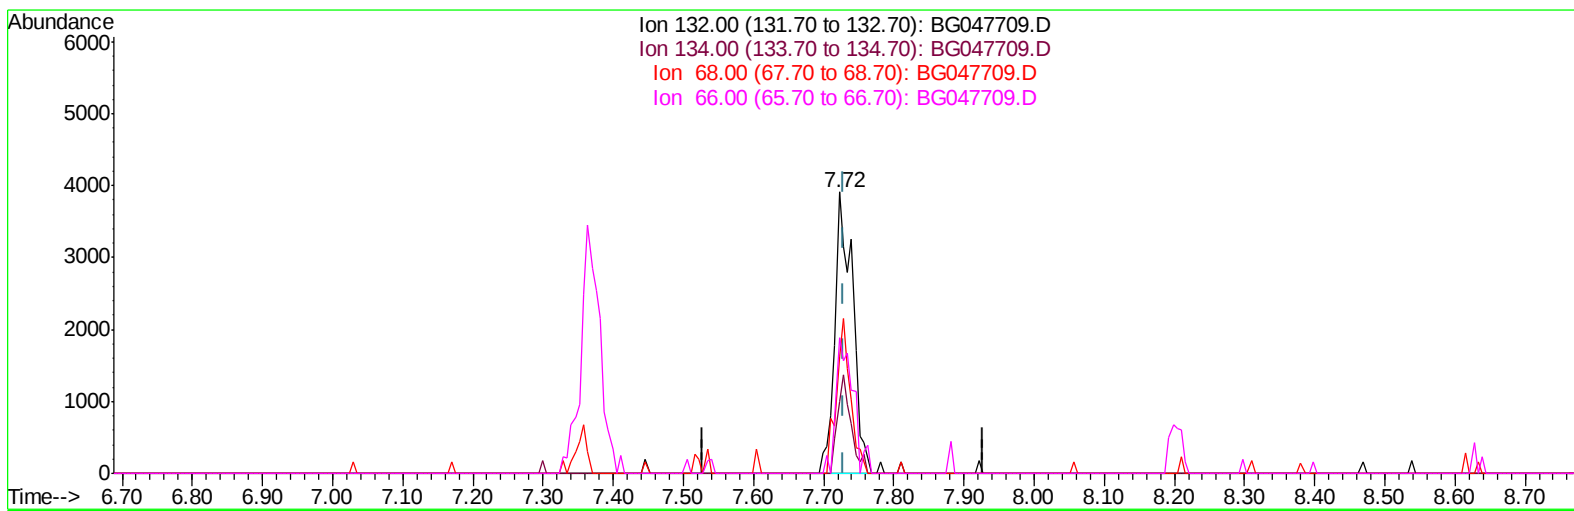

TIC: BG047709.D

(11) 2-Chlorophenol-d4 (S)

7.722min (-0.007) 5.06ng/ul m

response 6776

Ion	Exp%	Act%
132.00	100	100
134.00	31.40	25.42
68.00	51.30	41.21
66.00	43.10	48.24




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

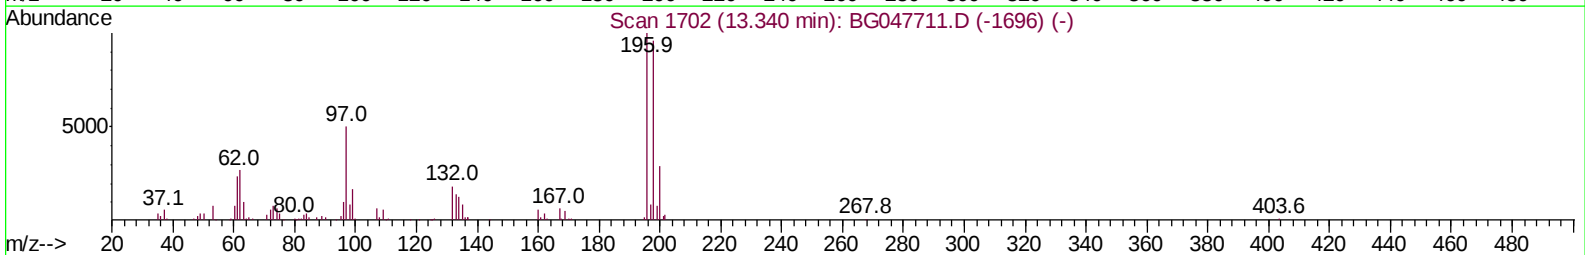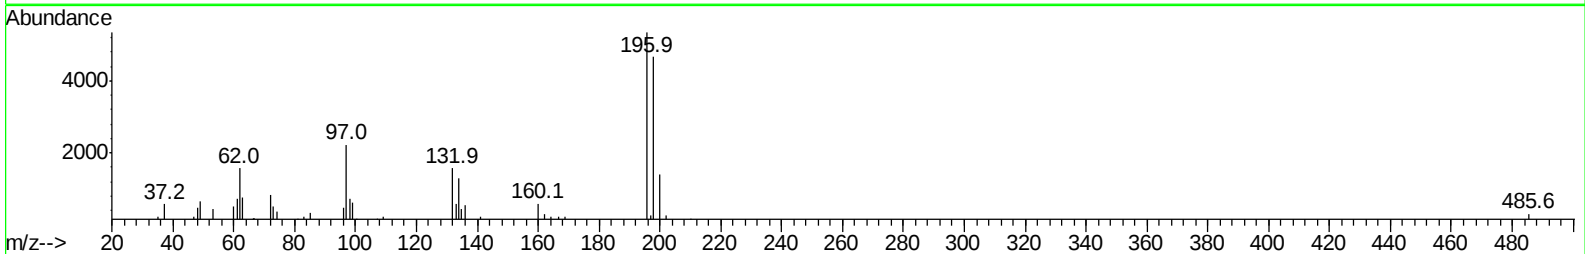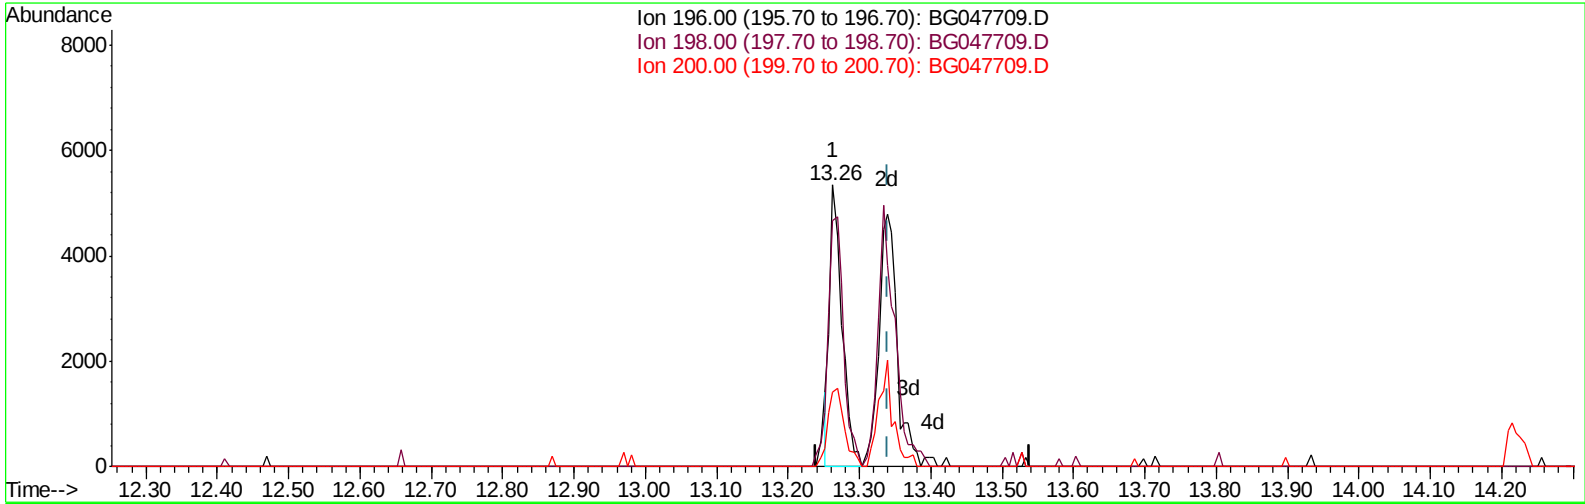

TIC: BG047709.D

(42) 2,4,5-Trichlorophenol
13.263min (-0.077) 3.73ng/ul
response 6510

Ion	Exp%	Act%
196.00	100	100
198.00	95.60	87.38
200.00	29.20	26.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST000503
Misc :
ALS Vial : 2 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

Ion 196.00 (195.70 to 196.70): BG047709.D
Ion 198.00 (197.70 to 198.70): BG047709.D
Ion 200.00 (199.70 to 200.70): BG047709.D

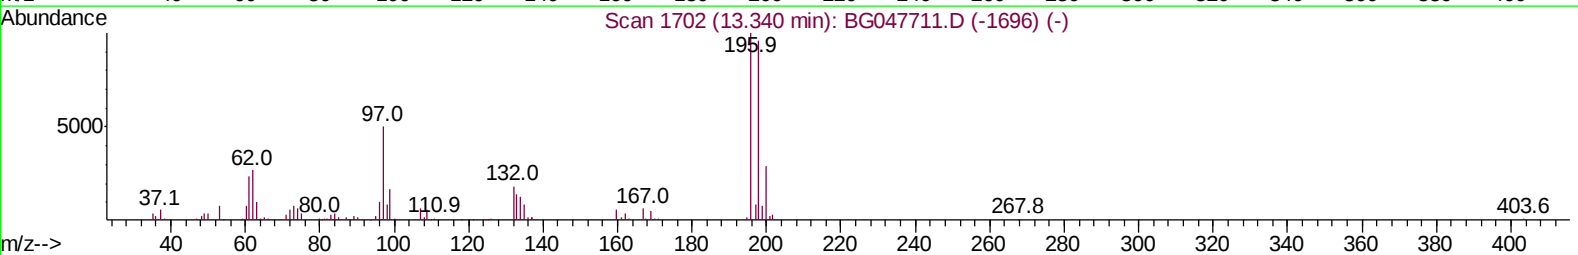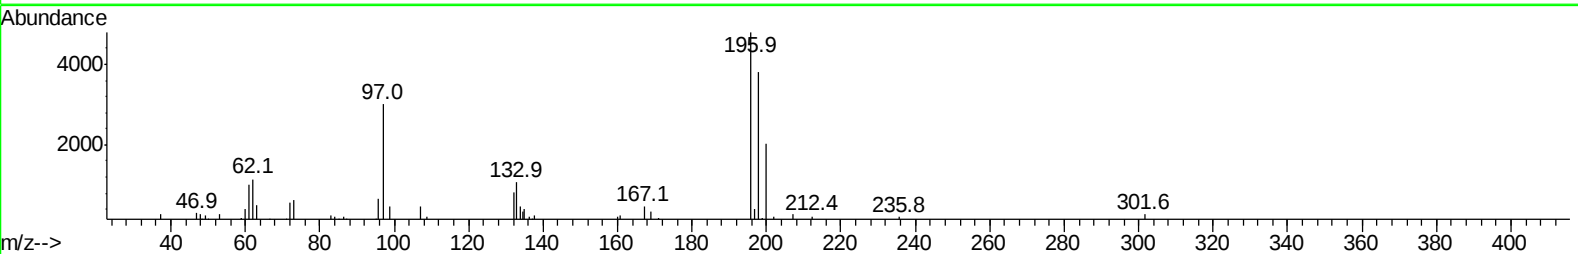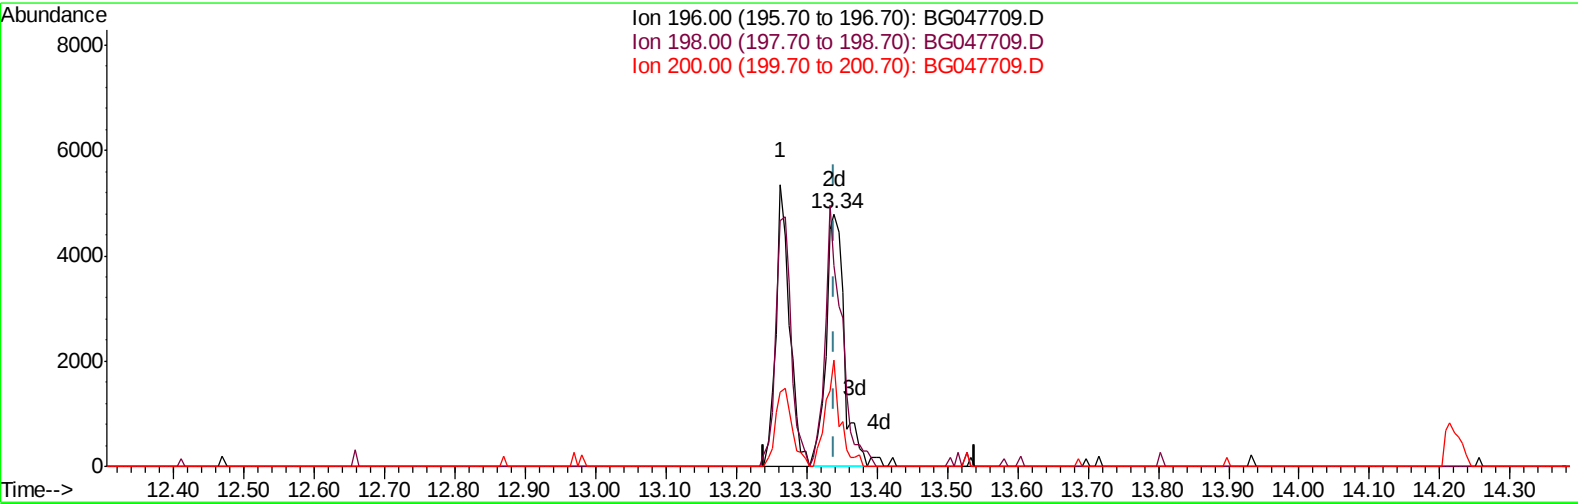

TIC: BG047709.D

(42) 2,4,5-Trichlorophenol

13.339min (-0.001) 4.86ng/ul m

response 8488

Ion	Exp%	Act%
196.00	100	100
198.00	95.60	79.61
200.00	29.20	42.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

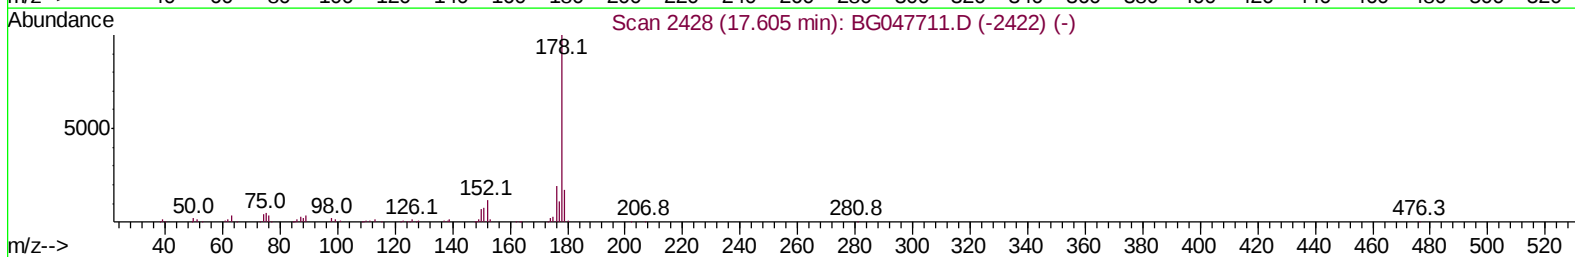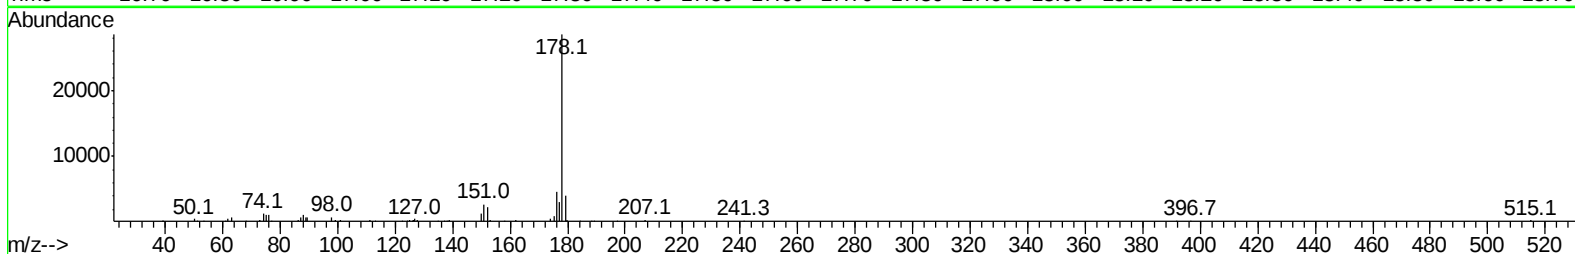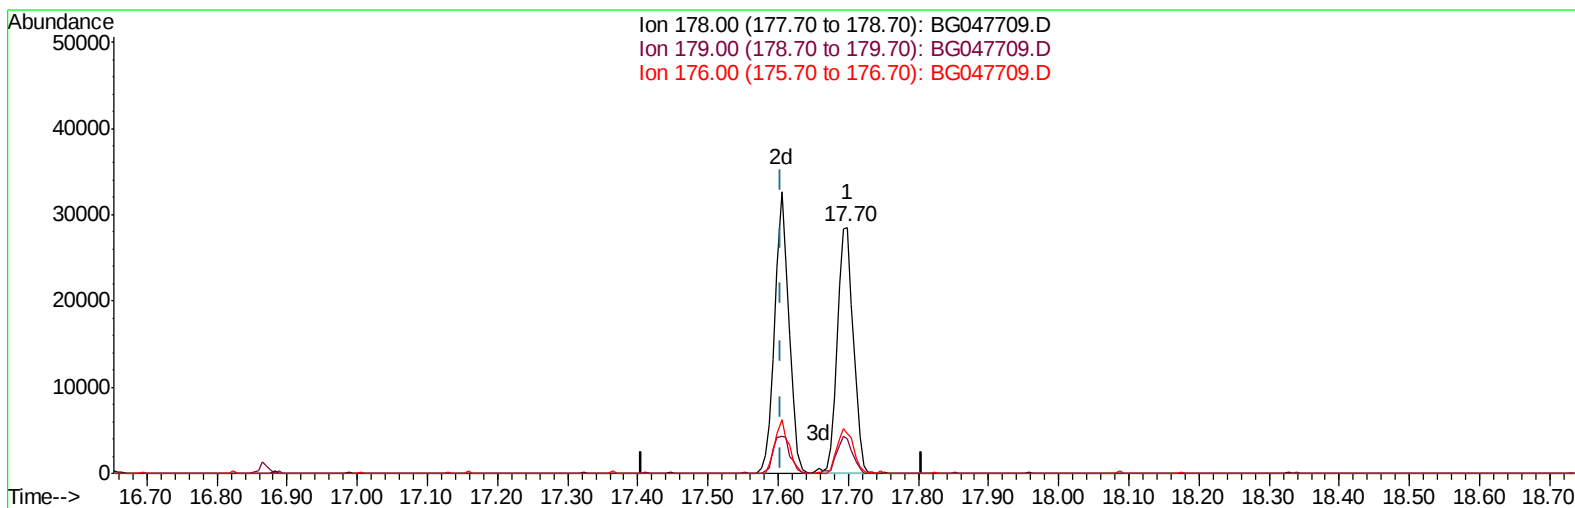

TIC: BG047709.D

(72) Phenanthrene

17.699min (+0.093) 5.05ng/ul

response 44746

Ion	Exp%	Act%
178.00	100	100
179.00	16.90	13.97
176.00	19.10	16.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SST00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1




Instrument :
 BNA_G
 ClientSampleId :
 SST005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

Ion 178.00 (177.70 to 178.70): BG047709.D
 Ion 179.00 (178.70 to 179.70): BG047709.D
 Ion 176.00 (175.70 to 176.70): BG047709.D

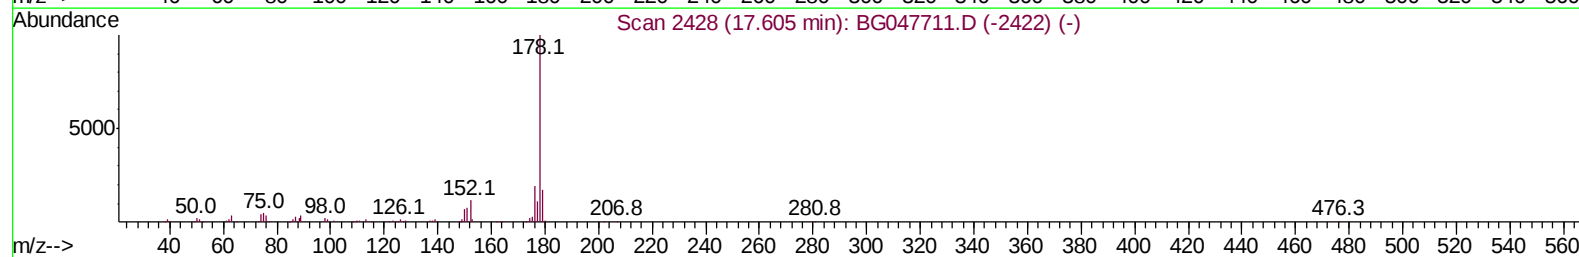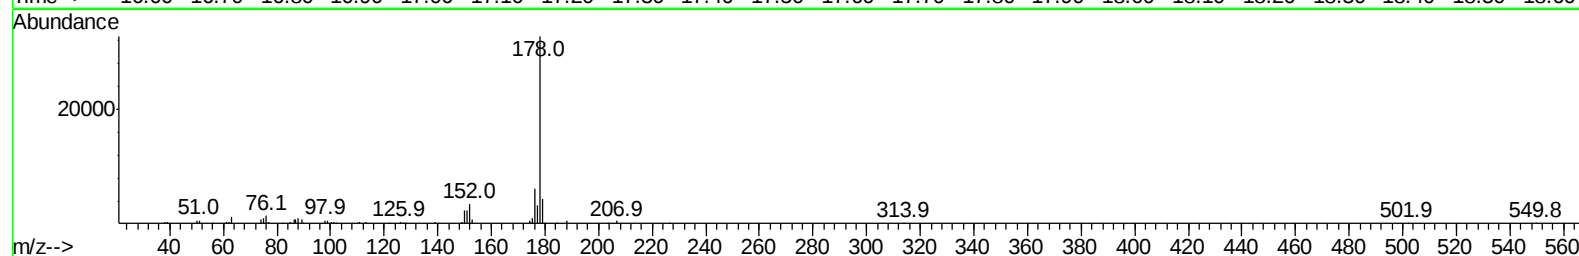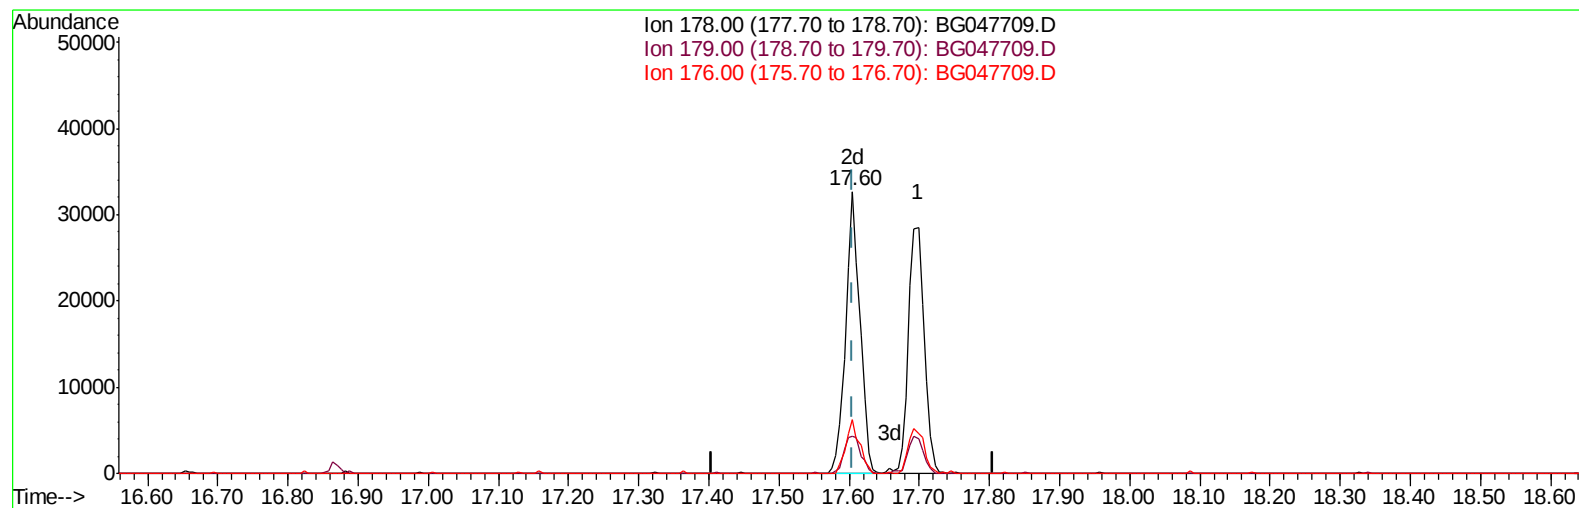

TIC: BG047709.D

(72) Phenanthrene

17.605min (-0.001) 5.19ng/ul m

response 45926

Ion	Exp%	Act%
178.00	100	100
179.00	16.90	13.30#
176.00	19.10	18.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SSTD00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

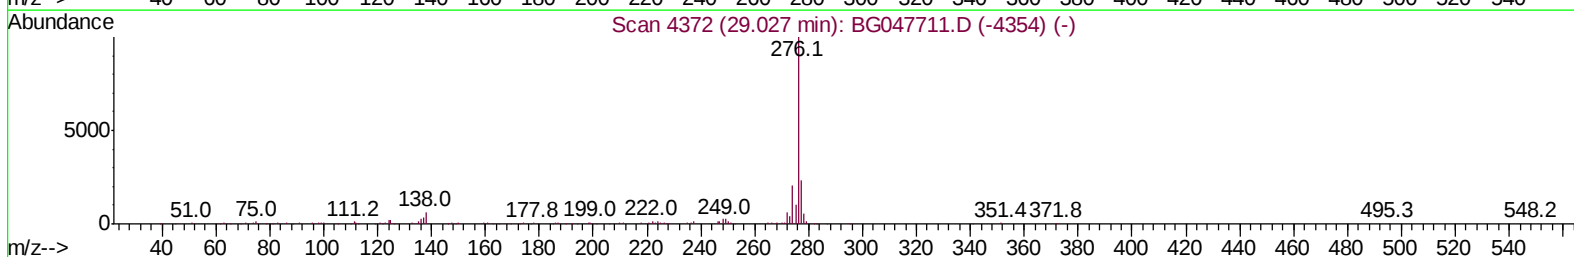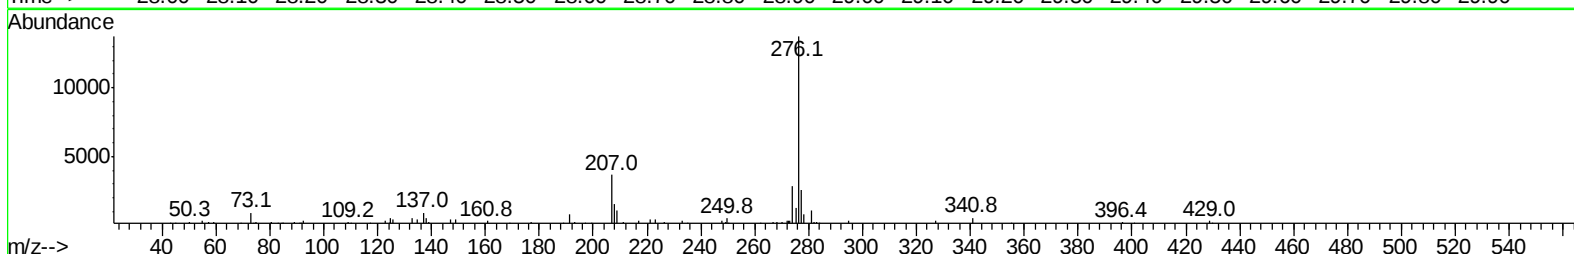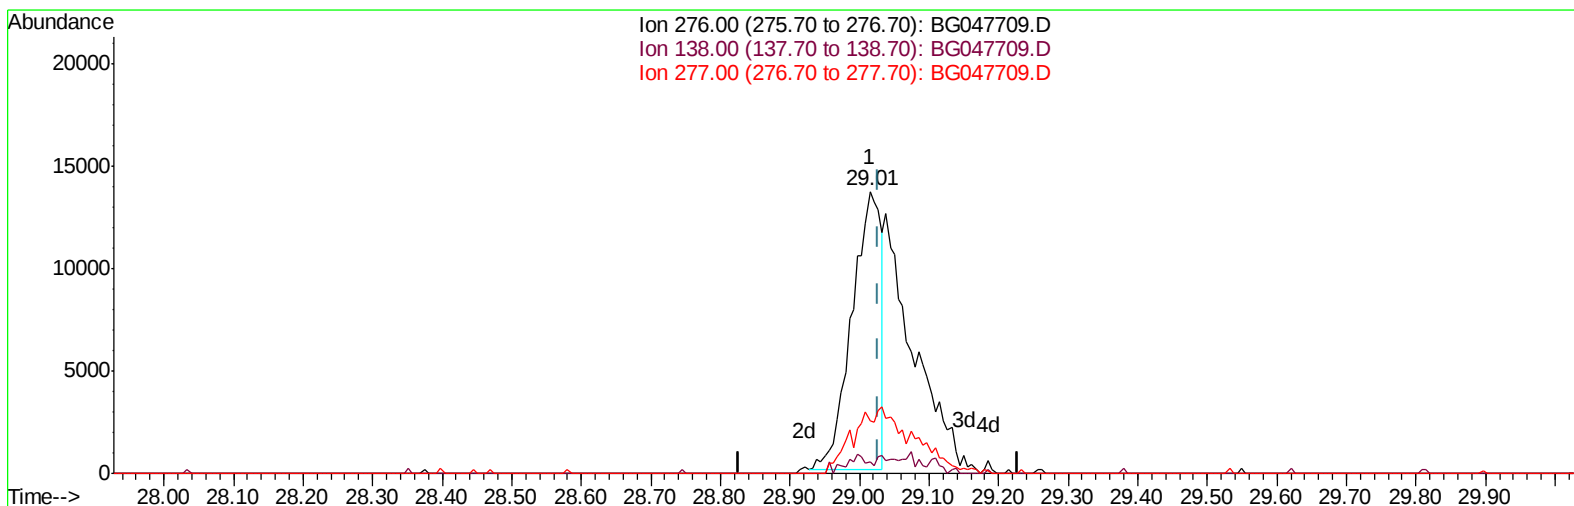

TIC: BG047709.D

(94) Indeno(1,2,3-cd)pyrene

29.015min (-0.012) 2.63ng/ul

response 40114

Ion	Exp%	Act%
276.00	100	100
138.00	6.40	4.08#
277.00	23.00	18.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

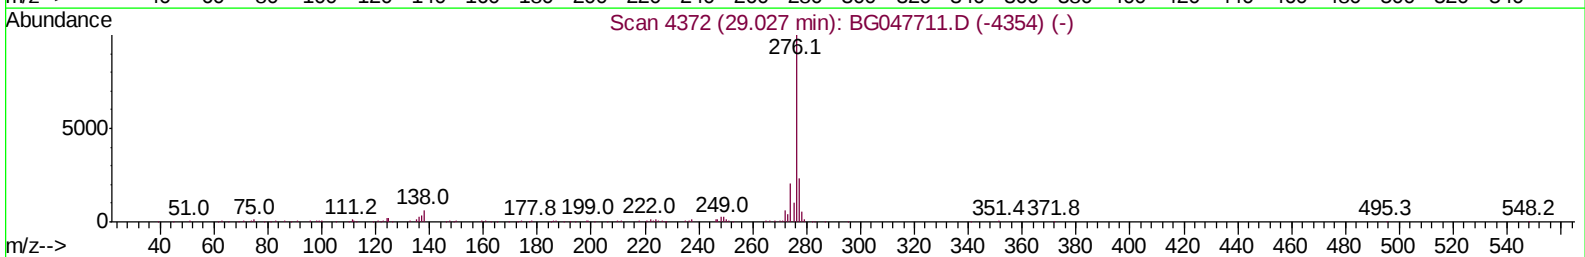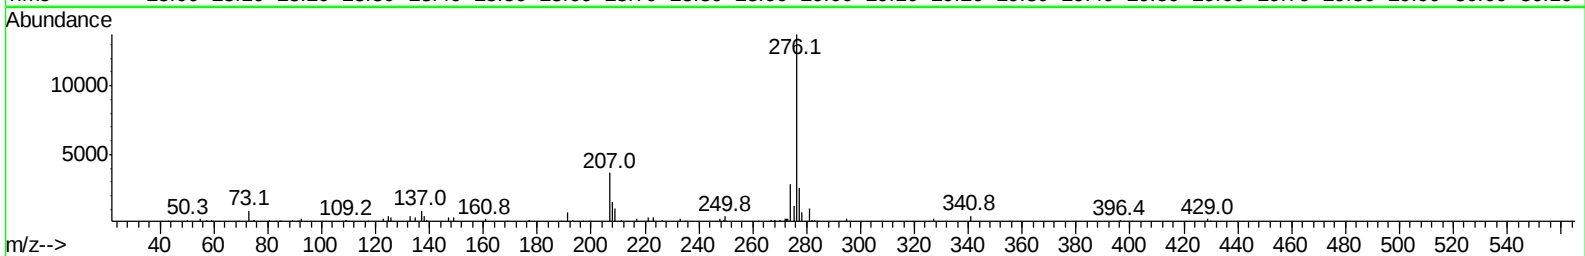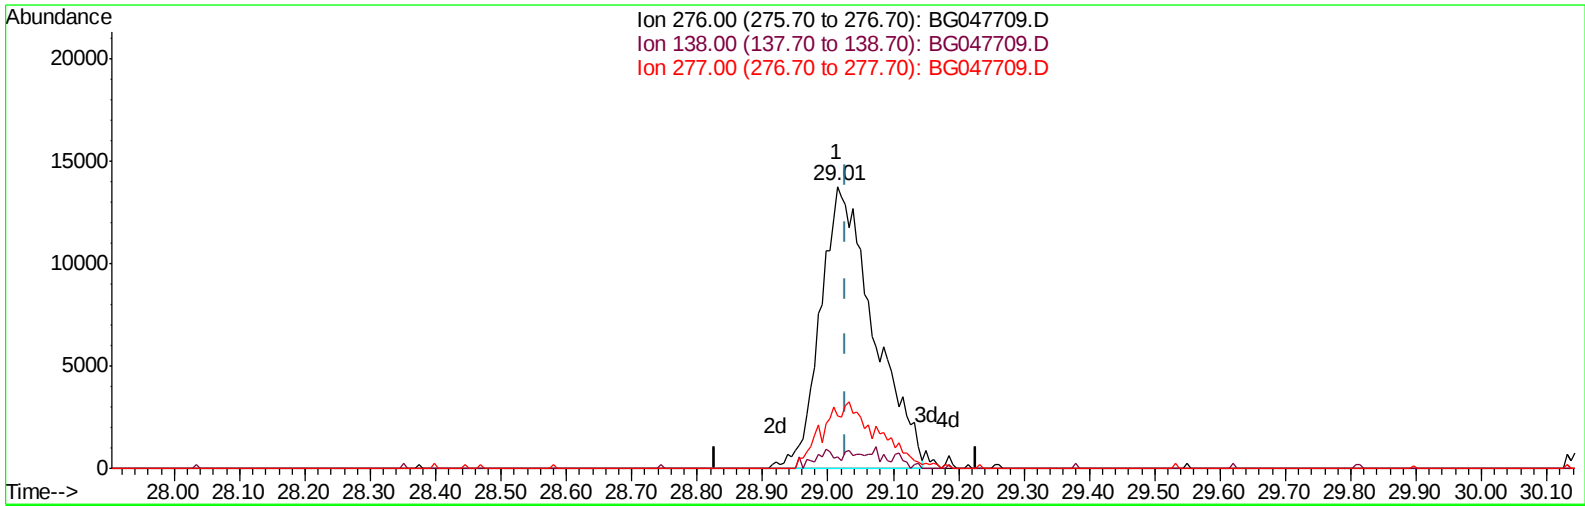

TIC: BG047709.D

(94) Indeno(1,2,3-cd)pyrene

29.015min (-0.012) 5.11ng/ul m

response 77875

Ion	Exp%	Act%
276.00	100	100
138.00	6.40	4.08#
277.00	23.00	18.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST00503
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
BNA_G
ClientSampleId :
SSTD005003

Manual Integrations
APPROVED


mohammad
12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

Ion 278.00 (277.70 to 278.70): BG047709.D
Ion 139.00 (138.70 to 139.70): BG047709.D
Ion 279.00 (278.70 to 279.70): BG047709.D

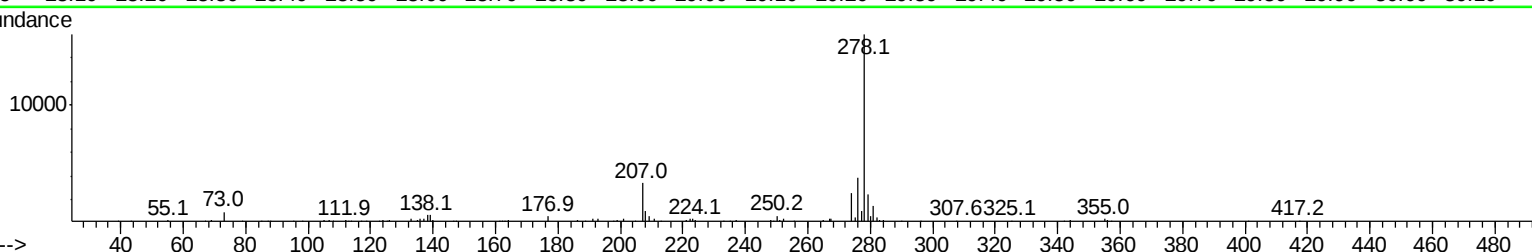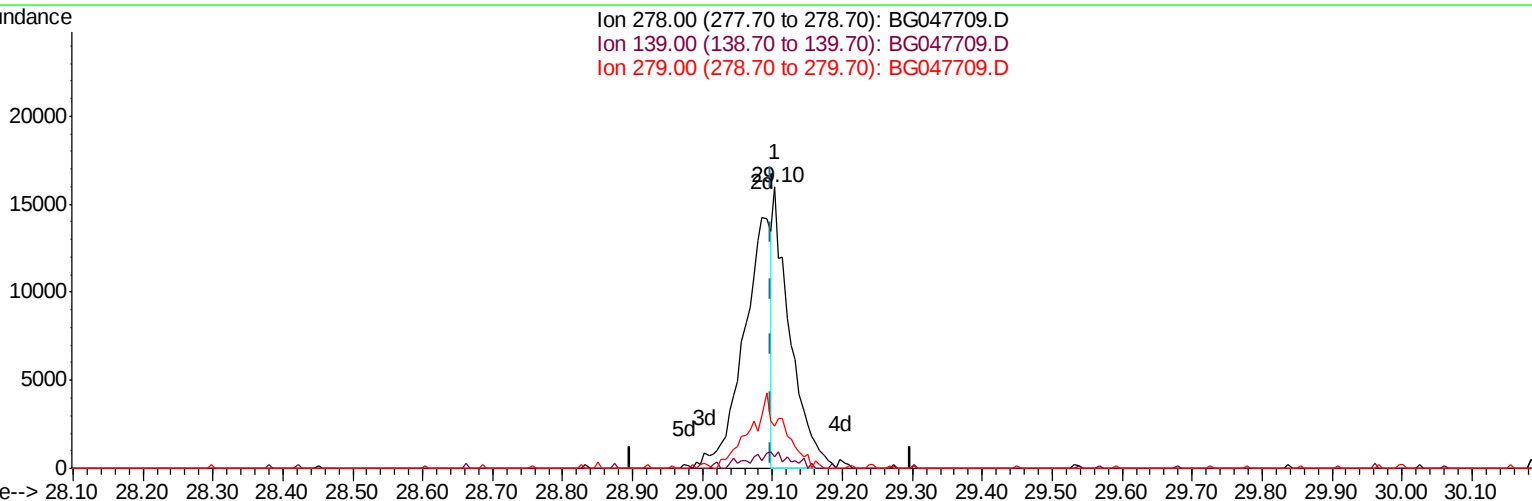

Scan 4384 (29.098 min): BG047711.D (-4371) (-)

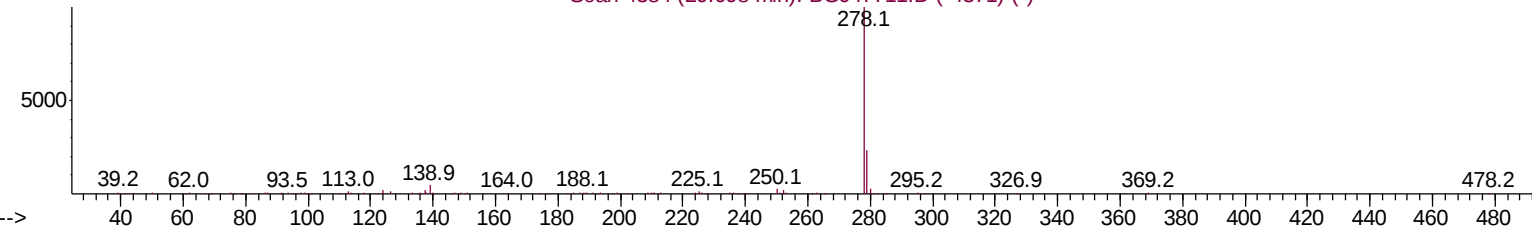

TIC: BG047709.D

(95) Dibenzo(a,h)anthracene

29.103min (+0.005) 2.14ng/ul

response 27282

Ion	Exp%	Act%
278.00	100	100
139.00	4.40	4.13
279.00	23.30	14.94#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SST00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

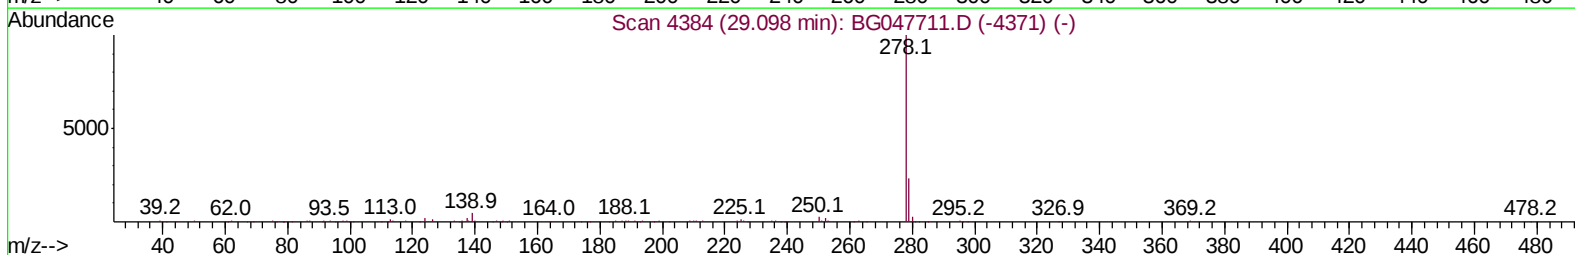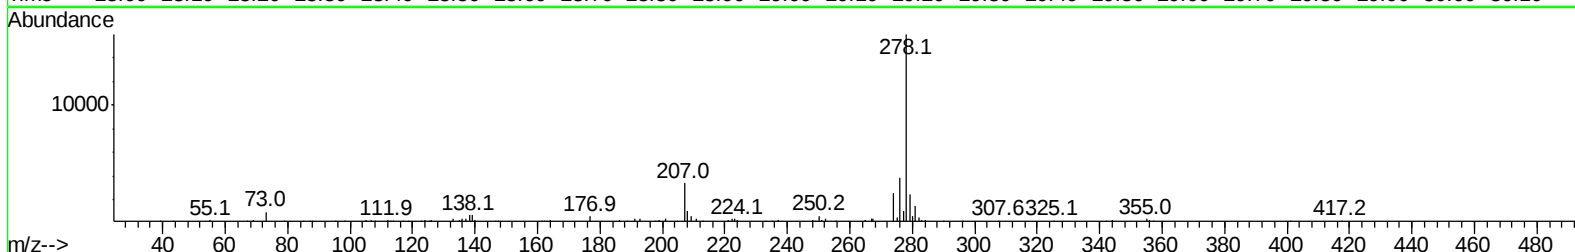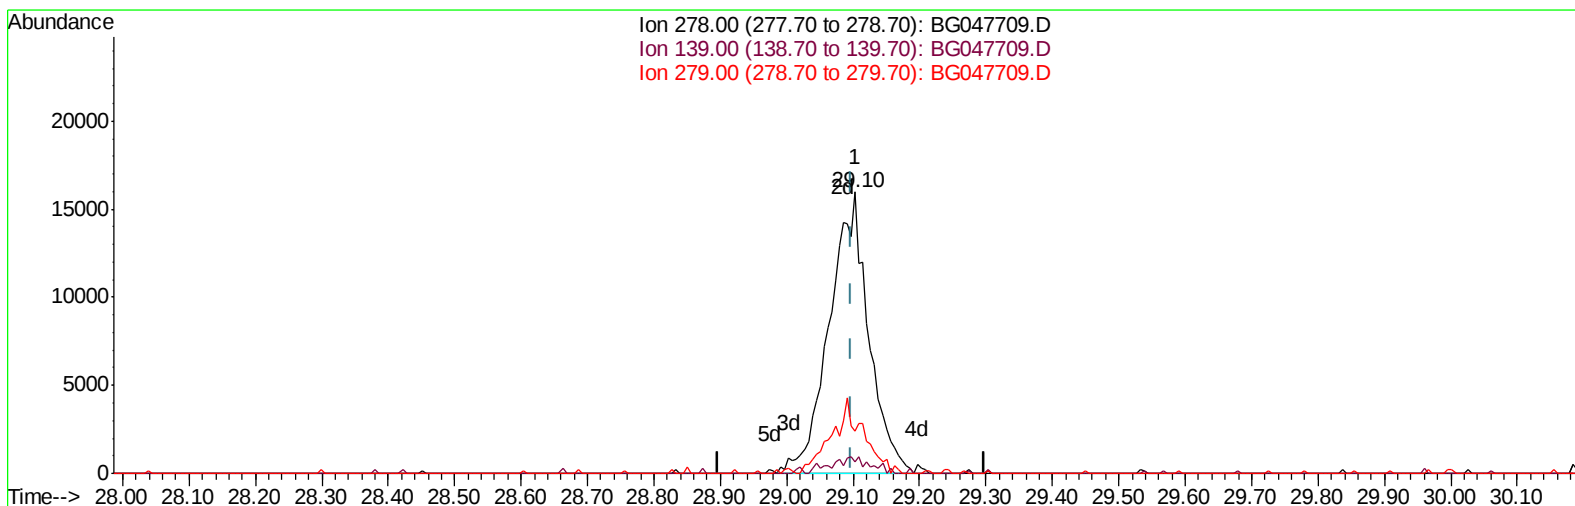

TIC: BG047709.D

(95) Dibenzo(a,h)anthracene

29.103min (+0.005) 5.18ng/ul m

response 66038

Ion	Exp%	Act%
278.00	100	100
139.00	4.40	4.13
279.00	23.30	14.94#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
Data File : BG047709.D
Acq On : 11 Dec 2020 10:11
Operator : CG/JU
Sample : SST000503
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005003

Quant Time: Dec 11 13:04:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 11 12:42:47 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
12/14/2020 2:43:50 PM

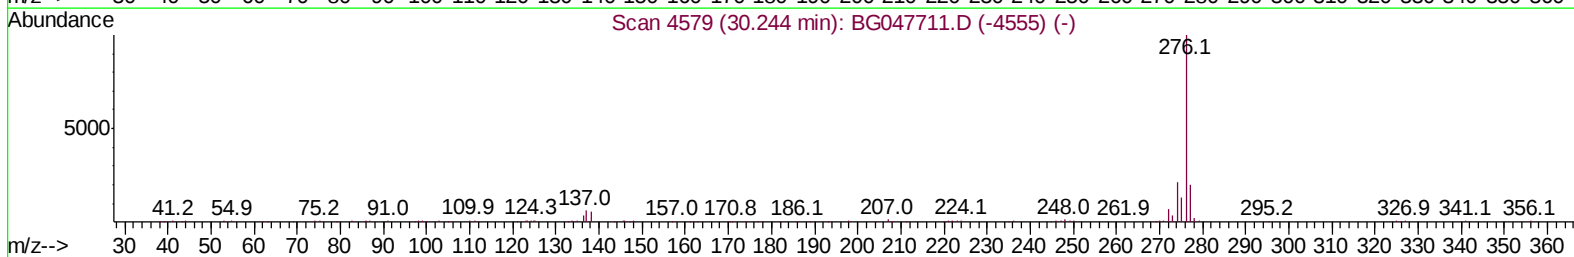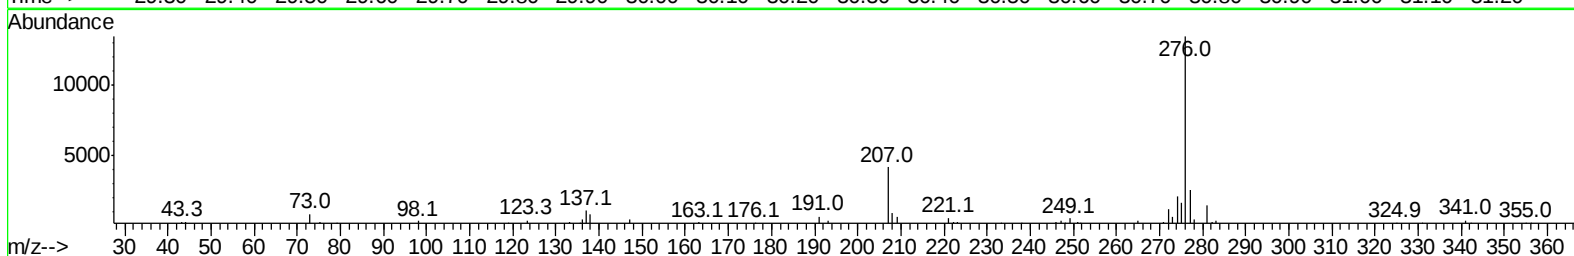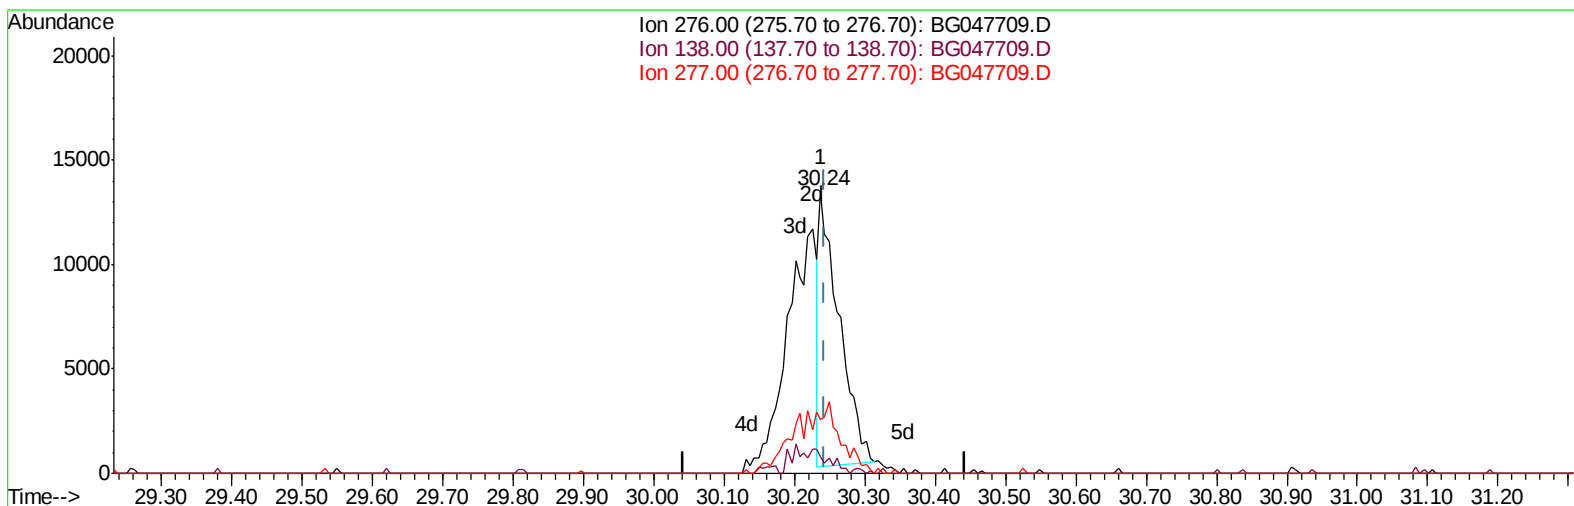

TIC: BG047709.D

(96) Benzo(g,h,i)perylene

30.237min (-0.007) 2.07ng/ul

response 25894

Ion	Exp%	Act%
276.00	100	100
138.00	5.30	6.12
277.00	20.00	18.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SST00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:04:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

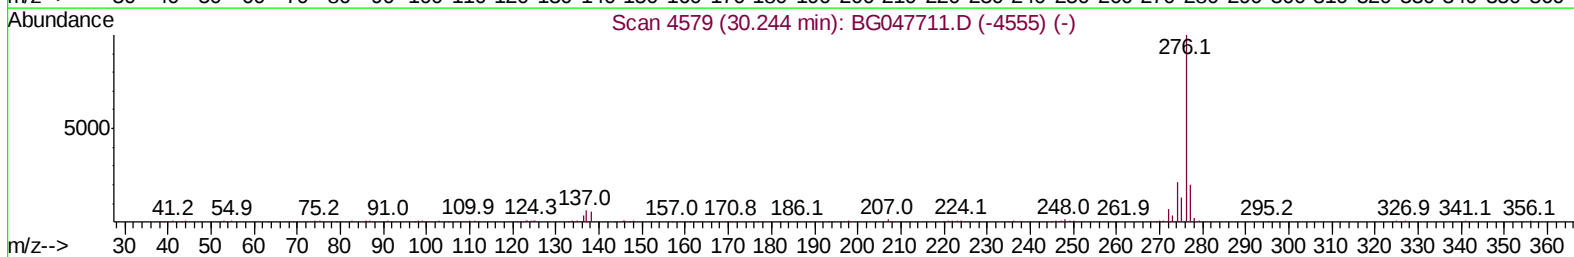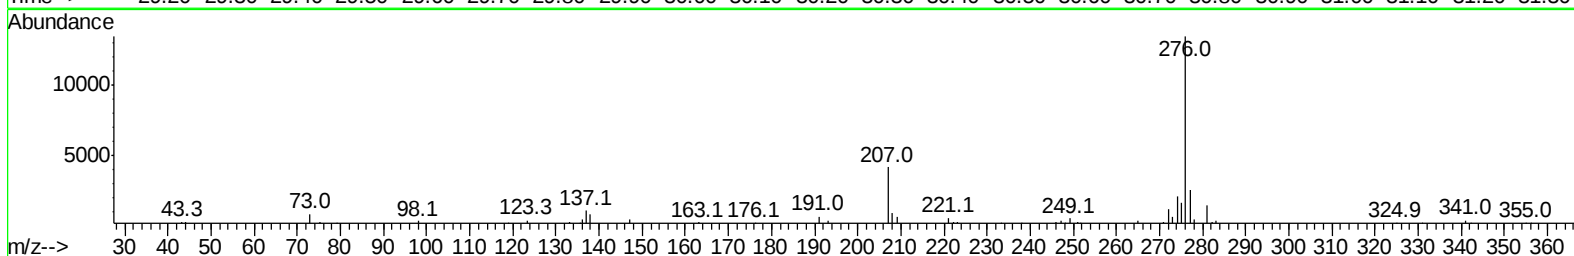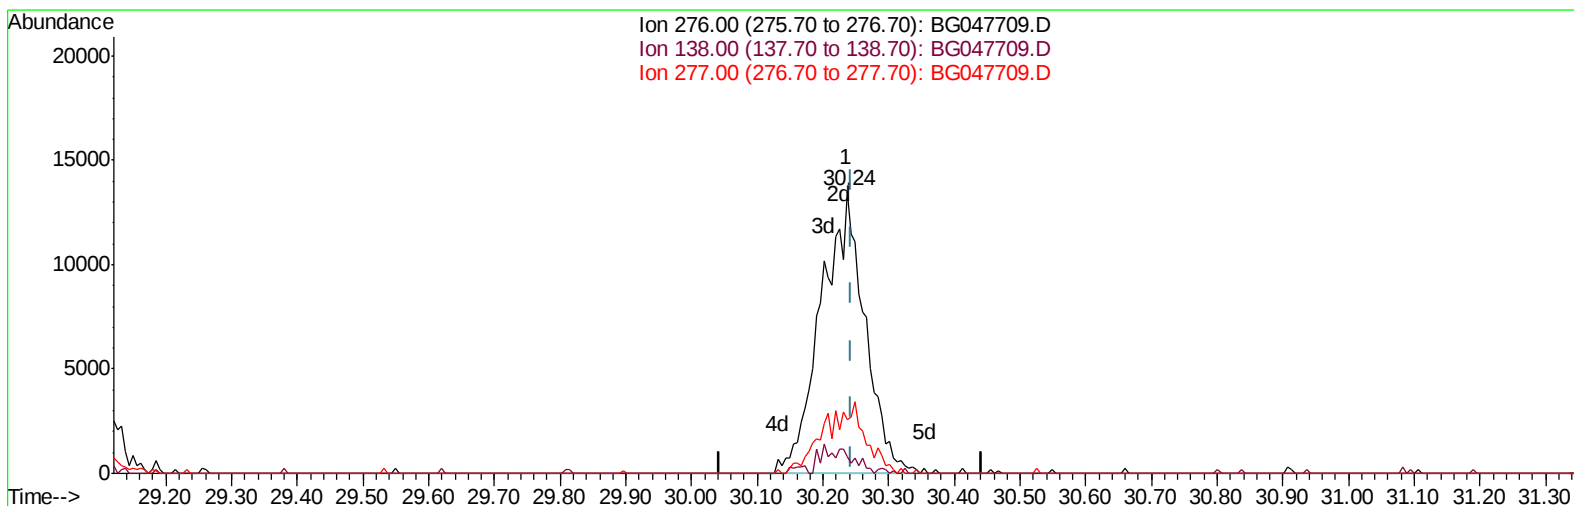

TIC: BG047709.D

(96) Benzo(g,h,i)perylene

30.237min (-0.007) 5.05ng/ul m

response 63034

Ion	Exp%	Act%
276.00	100	100
138.00	5.30	6.12
277.00	20.00	18.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SST00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:14:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	21006	20.00	ng/ul	0.00
20) Naphthalene-d8	11.03	136	82593	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.83	164	62899	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.56	188	165018	20.00	ng/ul	0.00
79) Chrysene-d12	21.84	240	191304	20.00	ng/ul	0.00
88) Perylene-d12	25.19	264	202965	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	1009m	2.30	ng/uL	0.02
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	0.00	99	0d	0.00	ng/ul	
9) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul	
11) 2-Chlorophenol-d4	7.72	132	6776m	5.06	ng/ul	0.00
15) 4-Methylphenol-d8	0.00	113	0d	0.00	ng/ul	
21) Nitrobenzene-d5	9.37	128	3454	5.02	ng/ul	0.00
24) 2-Nitrophenol-d4	10.10	143	3362	4.01	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.64	165	8139	4.90	ng/ul	0.00
31) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
46) Dimethylphthalate-d6	14.21	166	25605	4.79	ng/ul	0.00
49) Acenaphthylene-d8	14.53	160	29439	4.81	ng/ul	0.00
54) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
60) Fluorene-d10	15.81	176	25146	5.15	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
73) Anthracene-d10	17.66	188	40616	5.08	ng/ul	0.00
81) Pyrene-d10	19.93	212	49572	4.19	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.95	264	54178	4.74	ng/ul	-0.01

Target Compounds

				Ovalue	
2) 1,4-Dioxane	3.56	88	1145m	2.521	ng/uL
12) 2-Chlorophenol	7.76	128	7028	5.207	ng/ul
17) N-Nitroso-di-n-propylamine	9.00	70	6039	4.773	ng/ul#
19) Hexachloroethane	9.30	117	3080	4.806	ng/ul#
22) Nitrobenzene	9.41	77	10234	4.905	ng/ul#
23) Isophorone	9.94	82	18080	4.929	ng/ul#
25) 2-Nitrophenol	10.14	139	3929	4.668	ng/ul#
26) 2,4-Dimethylphenol	10.18	107	9134	4.650	ng/ul
27) Bis(2-Chloroethoxy)methane	10.42	93	9086	5.469	ng/ul#
29) 2,4-Dichlorophenol	10.67	162	7386	4.828	ng/ul
30) Naphthalene	11.08	128	22212	4.847	ng/ul#
33) Hexachlorobutadiene	11.36	225	8718	5.553	ng/ul
35) 4-Chloro-3-methylphenol	12.29	107	8299	4.764	ng/ul#
36) 2-Methylnaphthalene	12.68	142	16368	4.703	ng/ul
37) 1-Methylnaphthalene	12.89	142	15624	4.674	ng/ul#
39) 1,2,4,5-Tetrachlorobenzene	13.03	216	13838	5.405	ng/ul
41) 2,4,6-Trichlorophenol	13.26	196	7183	4.502	ng/ul#
42) 2,4,5-Trichlorophenol	13.34	196	8488m	4.864	ng/ul
43) 1,1'-Biphenyl	13.66	154	24906	5.100	ng/ul#
44) 2-Chloronaphthalene	13.71	162	18850	4.794	ng/ul#
45) 2-Nitroaniline	13.90	65	5773	4.276	ng/ul
47) Dimethylphthalate	14.27	163	25794	4.647	ng/ul#

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047709.D
 Acq On : 11 Dec 2020 10:11
 Operator : CG/JU
 Sample : SSTD00503
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD005003

Manual Integrations
 APPROVED

mohammad
 12/14/2020 2:43:50 PM

Quant Time: Dec 11 13:14:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 11 12:42:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
48) 2,6-Dinitrotoluene	14.38	165	5122	4.412	ng/ul#	87
50) Acenaphthylene	14.56	152	27164	4.717	ng/ul#	92
52) Acenaphthene	14.89	153	19757	4.728	ng/ul	94
56) Dibenzofuran	15.22	168	28615	4.720	ng/ul	96
57) 2,4-Dinitrotoluene	15.17	165	8600	5.185	ng/ul#	87
58) 2,3,4,6-Tetrachlorophenol	15.44	232	6966	4.344	ng/ul	99
59) Diethylphthalate	15.61	149	27121	5.015	ng/ul	93
61) Fluorene	15.87	166	25339	4.947	ng/ul	99
62) 4-Chlorophenyl-phenylether	15.85	204	15388	4.908	ng/ul#	84
67) N-Nitrosodiphenylamine	16.07	169	23132	5.095	ng/ul	99
68) 4-Bromophenyl-phenylether	16.75	248	10457	4.853	ng/ul	90
69) Hexachlorobenzene	16.87	284	11380	4.958	ng/ul#	86
72) Phenanthrene	17.60	178	45926m	5.186	ng/ul	
74) Anthracene	17.70	178	44746	5.046	ng/ul	95
75) 1,2,3,4-Tetrachlorobenzene	13.63	216	12831	4.790	ng/ul#	92
76) Pentachlorobenzene	15.14	250	12859	4.817	ng/ul	99
78) Di-n-butylphthalate	18.50	149	43604	5.071	ng/ul	97
80) Fluoranthene	19.60	202	62024	4.292	ng/ul	99
82) Pyrene	19.96	202	63686	4.504	ng/ul#	97
83) Butylbenzylphthalate	20.82	149	21241	4.502	ng/ul	90
85) Benzo(a)anthracene	21.82	228	66671	4.909	ng/ul	98
86) Bis(2-ethylhexyl)phthalate	21.70	149	29063	4.535	ng/ul	96
87) Chrysene	21.88	228	65721	5.106	ng/ul	96
90) Benzo(b)fluoranthene	24.12	252	71522	5.093	ng/ul#	96
91) Benzo(k)fluoranthene	24.19	252	69415	5.052	ng/ul#	93
93) Benzo(a)pyrene	25.03	252	61356	4.872	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	29.01	276	77875m	5.109	ng/ul	
95) Dibenzo(a,h)anthracene	29.10	278	66038m	5.183	ng/ul	
96) Benzo(a,h,i)perylene	30.24	276	63034m	5.047	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

