


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121120\
 Data File : BG047708.D
 Acq On : 11 Dec 2020 9:30
 Operator : CG/JU
 Sample : DFTPP69
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP691

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG121120.M
 Title : SVOA CALIBRATION
 Last Update : Fri Dec 11 14:20:11 2020

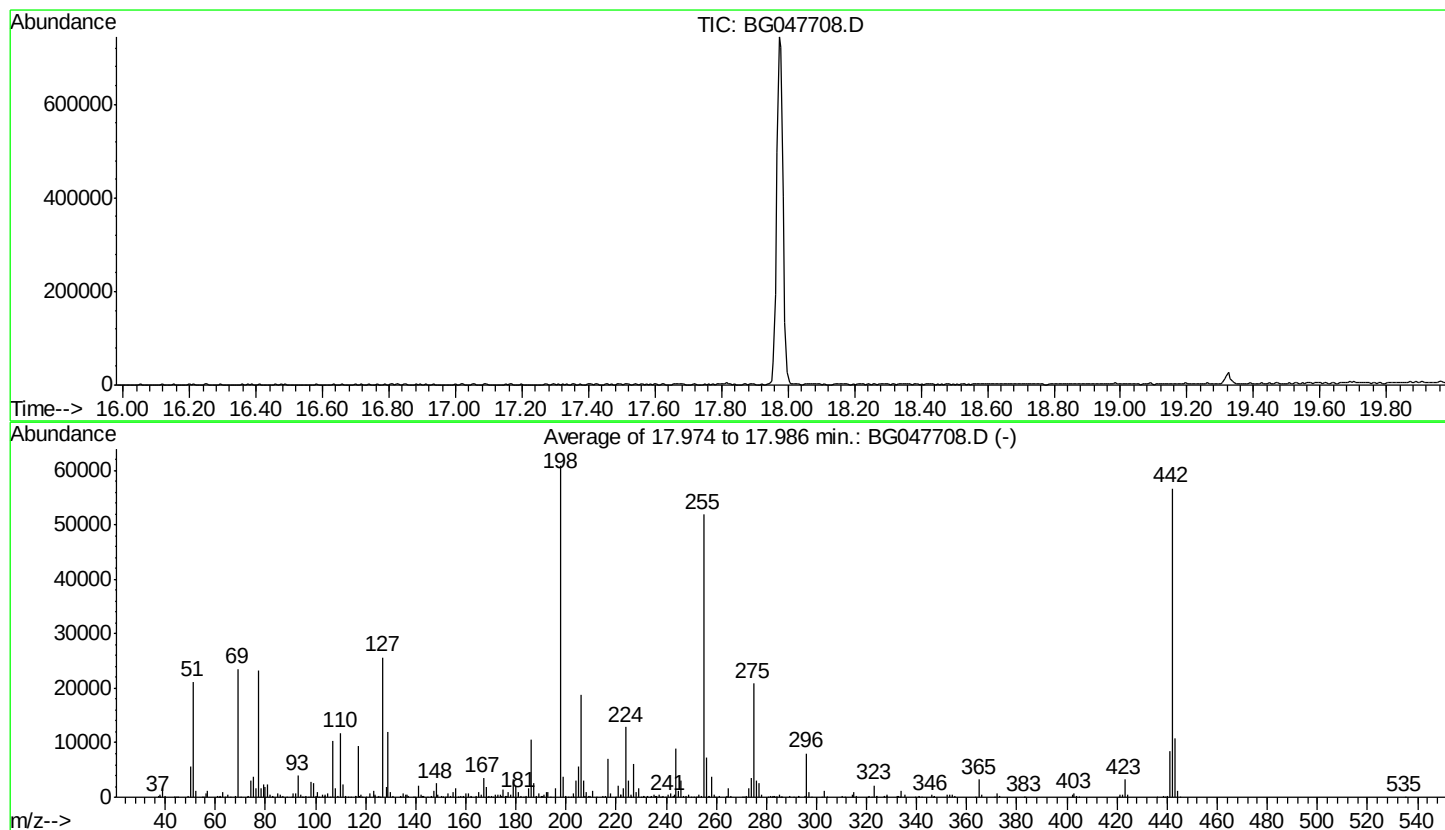

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	21232	PASS
68	69	0.00	2	0.7	156	PASS
69	198	0.00	100	38.6	23535	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	42.1	25640	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60901	PASS
199	198	5	9	6.4	3883	PASS
275	198	10	60	34.3	20863	PASS
365	198	1	100	5.3	3220	PASS
441	198	0.01	100	13.9	8489	PASS
442	198	50	100	93.2	56736	PASS
443	442	15	24	19.1	10815	PASS

Scan 2484 (17.933 min): BG047708.D
DFTPP69

m/z	Abundance
81.90	152.0
102.70	245.0
125.90	202.0
129.90	164.0
135.50	157.0
195.20	165.0
206.60	272.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

m/z	Abundance
37.10	287.0
38.10	506.0
39.00	2155.0
40.10	245.0
44.00	218.0
45.20	360.0
49.00	231.0
50.10	7780.0
51.10	28576.0
52.10	1589.0
54.80	173.0
56.10	938.0
57.00	1778.0
61.00	773.0
62.00	577.0
63.10	1434.0
65.00	633.0
66.00	170.0
69.00	31256.0
70.00	200.0
73.00	443.0
74.10	3810.0
75.00	5229.0
76.10	2785.0
77.10	29456.0
78.10	2274.0
79.10	2803.0
80.00	2044.0
81.00	2745.0
82.10	701.0
83.00	666.0
85.10	762.0
86.10	825.0
90.40	159.0
91.00	486.0
91.90	414.0
93.00	4918.0
94.10	586.0
94.80	158.0
96.00	216.0
98.00	4280.0
99.00	2706.0
100.00	371.0
101.00	1403.0
103.10	682.0
103.90	1071.0
105.10	827.0
105.80	158.0
107.00	12586.0
108.00	2278.0
109.10	440.0
110.00	15039.0
111.00	3389.0
112.10	328.0
112.80	231.0
114.20	173.0
115.90	697.0
117.00	12522.0
118.10	907.0
118.80	192.0
120.20	196.0
122.00	851.0
123.00	1399.0
124.00	781.0
125.10	668.0
126.00	440.0
127.00	31768.0
128.10	2197.0
129.00	15677.0
130.00	1634.0
131.10	229.0
134.00	554.0
135.10	725.0
136.00	588.0
137.10	675.0
139.80	232.0
141.00	3037.0
142.00	489.0
142.90	320.0
146.00	691.0
147.00	1406.0
148.00	3163.0
149.00	791.0
150.20	179.0
150.70	179.0
152.90	884.0
153.90	371.0
155.00	1093.0
156.00	2138.0
156.90	180.0
158.00	367.0
158.80	339.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

159.90	1035.0
161.10	1014.0
162.00	195.0
164.00	233.0
165.10	812.0
166.00	815.0
167.00	4098.0
168.00	2098.0
168.80	202.0
172.00	421.0
173.00	724.0
173.90	801.0
175.00	1881.0
176.20	393.0
177.00	903.0
177.90	522.0
179.00	4237.0
179.90	2391.0
181.00	1127.0
182.00	236.0
185.10	2207.0
186.00	11857.0
186.90	3742.0
187.90	474.0
189.00	940.0
189.90	204.0
190.90	414.0
192.10	1066.0
192.90	1119.0
194.00	243.0
195.10	167.0
196.00	2032.0
198.00	71224.0
199.00	4779.0
200.00	251.0
201.70	362.0
202.90	813.0
204.00	3704.0
205.00	6989.0
206.00	21344.0
207.00	3472.0
208.00	1245.0
209.10	487.0
209.80	368.0
210.80	1062.0
215.00	175.0
217.00	8331.0
218.00	1145.0
219.80	183.0
221.00	2146.0
221.90	746.0
223.00	1784.0
224.00	16239.0
225.00	4079.0
226.10	789.0
226.90	7573.0
228.00	1236.0
229.00	2019.0
231.10	396.0
232.20	198.0
232.70	238.0
234.00	240.0
235.10	445.0
235.80	700.0
237.10	575.0
237.90	187.0
238.20	156.0
238.90	388.0
239.90	206.0
240.90	428.0
241.90	828.0
242.90	614.0
244.00	10644.0
245.00	1544.0
246.00	3994.0
247.10	415.0
247.90	305.0
248.80	530.0
249.80	167.0
253.10	686.0
255.00	60320.0
256.00	7900.0
257.00	679.0
258.00	4342.0
259.00	524.0
261.10	232.0
264.10	516.0
265.00	1578.0
266.00	428.0
270.80	309.0
271.90	312.0
273.10	1783.0
274.00	4571.0
275.00	24616.0
276.00	3956.0
277.00	2947.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

278.00	459.0
281.70	151.0
282.80	246.0
283.50	194.0
285.10	613.0
285.80	170.0
289.10	262.0
292.70	397.0
296.00	9149.0
297.00	1441.0
303.00	1309.0
303.90	194.0
310.00	397.0
311.10	313.0
314.20	674.0
315.00	1302.0
316.00	453.0
321.00	529.0
322.20	298.0
323.10	2501.0
323.90	399.0
326.90	295.0
328.20	523.0
332.00	203.0
332.30	202.0
332.90	254.0
334.00	1354.0
335.10	491.0
340.80	196.0
346.00	212.0
346.90	175.0
352.10	656.0
353.10	465.0
354.10	713.0
355.00	226.0
363.60	224.0
365.00	3259.0
365.80	393.0
371.00	196.0
372.00	852.0
373.10	494.0
382.90	324.0
402.00	575.0
403.10	309.0
403.90	241.0
421.00	461.0
422.00	464.0
423.10	3301.0
424.10	566.0
436.10	256.0
438.80	229.0
441.00	8312.0
442.00	57936.0
443.00	10552.0
444.00	1589.0
445.00	155.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

m/z	Abundance
38.00	554.0
39.00	1677.0
40.10	153.0
43.70	176.0
44.30	362.0
48.90	270.0
50.10	6089.0
51.10	22936.0
52.00	1107.0
55.10	173.0
56.00	617.0
57.10	1190.0
61.20	266.0
61.80	446.0
63.10	1332.0
63.90	373.0
65.10	682.0
69.00	26776.0
72.90	179.0
74.00	3044.0
75.10	4405.0
76.20	1508.0
77.10	27648.0
78.00	1776.0
79.10	3182.0
80.00	2436.0
81.00	3390.0
82.00	775.0
83.00	338.0
85.10	729.0
85.90	371.0
87.10	212.0
88.60	164.0
91.00	1025.0
92.00	738.0
93.10	4183.0
94.10	196.0
95.10	176.0
96.00	200.0
97.10	167.0
98.00	2830.0
99.00	3306.0
101.00	1260.0
102.90	425.0
104.10	870.0
105.00	1128.0
107.00	12270.0
108.10	1636.0
110.00	13921.0
111.00	1979.0
116.20	662.0
117.00	10206.0
117.80	844.0
121.90	726.0
123.00	1275.0
123.60	445.0
124.80	280.0
127.00	30760.0
128.10	2579.0
129.00	13336.0
130.00	1199.0
134.20	236.0
135.00	1265.0
136.00	393.0
136.80	608.0
139.00	190.0
141.00	2566.0
142.10	350.0
143.20	470.0
144.80	175.0
146.30	310.0
147.00	1140.0
148.10	2443.0
149.00	471.0
150.10	220.0
151.00	237.0
151.80	181.0
152.20	258.0
152.90	741.0
153.90	414.0
155.00	1435.0
156.00	2069.0
157.10	281.0
158.00	389.0
158.80	275.0
160.00	927.0
161.00	766.0
162.20	242.0
165.00	1260.0
165.80	300.0
167.00	4921.0
168.00	2065.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

169.10	515.0
170.10	273.0
170.90	213.0
172.00	639.0
172.80	441.0
174.10	791.0
174.90	1507.0
176.20	351.0
176.90	951.0
178.00	266.0
179.00	3206.0
180.00	2615.0
180.90	887.0
182.80	163.0
184.10	399.0
185.00	1816.0
186.00	13513.0
186.90	2768.0
187.90	354.0
189.00	667.0
190.00	384.0
191.10	644.0
192.00	1373.0
193.00	1221.0
196.00	1821.0
197.90	74864.0
199.00	4102.0
199.90	572.0
201.10	355.0
202.90	994.0
204.10	3194.0
205.00	5789.0
206.00	23136.0
207.00	3672.0
208.10	1258.0
209.00	201.0
209.70	471.0
210.80	1307.0
215.00	455.0
215.80	345.0
216.90	8526.0
218.00	791.0
221.00	2794.0
222.10	1108.0
223.00	1876.0
224.00	13788.0
225.00	3404.0
226.00	726.0
227.00	6591.0
228.00	1067.0
229.00	1742.0
230.00	214.0
231.10	625.0
232.70	297.0
233.90	453.0
235.00	565.0
235.70	332.0
236.10	310.0
237.00	482.0
239.00	360.0
240.80	350.0
242.00	800.0
243.20	1053.0
244.10	9474.0
245.00	859.0
246.00	3553.0
247.00	471.0
248.00	326.0
248.90	612.0
249.80	153.0
251.20	166.0
252.10	168.0
253.00	232.0
255.00	60568.0
256.00	8767.0
257.30	703.0
258.00	4475.0
259.00	413.0
259.90	294.0
261.00	194.0
263.70	221.0
265.00	2107.0
266.00	458.0
270.30	169.0
271.90	359.0
272.90	2311.0
274.00	3935.0
275.00	23024.0
276.00	3588.0
277.00	2813.0
278.00	448.0
281.80	412.0
283.10	480.0
283.80	174.0
284.10	170.0
285.00	328.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

289.20	203.0
290.80	179.0
293.00	478.0
296.00	9893.0
297.00	744.0
302.00	288.0
303.00	1411.0
304.20	203.0
310.10	209.0
314.00	751.0
314.90	966.0
315.90	316.0
320.70	315.0
320.90	315.0
323.00	2621.0
324.10	517.0
326.90	692.0
327.90	744.0
332.00	234.0
332.90	266.0
334.00	1559.0
335.10	540.0
339.50	171.0
340.90	193.0
341.90	292.0
346.00	643.0
347.00	318.0
352.10	527.0
353.00	554.0
354.00	448.0
355.00	186.0
365.00	3592.0
365.90	263.0
372.00	1047.0
373.00	229.0
383.10	372.0
402.00	331.0
403.00	1035.0
403.90	245.0
404.80	238.0
420.90	556.0
422.00	521.0
423.00	4228.0
424.10	844.0
438.70	162.0
440.10	406.0
441.00	10548.0
442.00	65704.0
443.10	13609.0
444.00	1350.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

m/z	Abundance
37.20	204.0
37.70	184.0
38.20	253.0
39.10	807.0
40.00	274.0
49.10	297.0
50.10	2870.0
51.10	12185.0
52.00	644.0
55.00	191.0
56.00	420.0
56.90	777.0
61.00	242.0
62.10	227.0
63.20	399.0
64.90	157.0
68.10	468.0
69.00	12574.0
72.50	166.0
74.10	2384.0
75.10	1936.0
76.00	938.0
77.10	12713.0
78.00	737.0
79.00	1224.0
80.00	1006.0
81.00	931.0
81.90	278.0
82.70	204.0
85.10	334.0
85.80	374.0
87.20	244.0
90.90	407.0
91.90	641.0
93.00	2651.0
94.00	358.0
98.00	1713.0
98.90	1492.0
100.00	195.0
101.20	349.0
103.20	187.0
104.00	648.0
105.20	231.0
105.80	162.0
107.00	5963.0
108.00	878.0
110.00	6492.0
111.10	1384.0
112.10	297.0
116.00	228.0
117.00	5802.0
118.00	263.0
122.10	256.0
123.00	712.0
123.90	341.0
126.00	217.0
127.00	14394.0
128.00	1048.0
129.00	6792.0
129.90	825.0
131.00	245.0
135.00	473.0
135.90	336.0
136.70	476.0
141.10	626.0
142.00	408.0
142.80	286.0
143.20	326.0
146.00	224.0
147.00	712.0
148.00	1845.0
149.00	191.0
153.00	312.0
153.90	184.0
155.00	432.0
156.10	811.0
159.00	220.0
160.00	350.0
160.90	698.0
161.90	191.0
164.00	199.0
164.90	649.0
166.10	394.0
166.90	1813.0
168.00	1273.0
170.00	284.0
171.80	265.0
172.20	169.0
173.00	333.0
173.90	848.0
175.00	1096.0
175.80	464.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

177.00	766.0
177.80	346.0
178.90	2267.0
180.00	1372.0
181.10	716.0
181.90	177.0
184.20	325.0
185.00	867.0
186.00	6430.0
187.00	1523.0
187.90	246.0
189.00	657.0
190.40	216.0
191.00	472.0
192.00	419.0
193.00	696.0
196.10	1196.0
198.00	36616.0
198.90	2768.0
200.10	179.0
203.10	369.0
204.00	1951.0
205.10	4297.0
206.00	12085.0
207.10	2147.0
207.80	489.0
208.10	455.0
208.90	261.0
210.90	864.0
212.00	227.0
214.90	230.0
215.80	161.0
216.90	4542.0
218.00	493.0
221.00	1474.0
221.90	763.0
222.90	1003.0
224.00	8753.0
225.00	1680.0
225.80	244.0
226.90	4175.0
227.90	758.0
229.00	888.0
230.80	473.0
233.70	357.0
234.90	391.0
236.00	181.0
236.90	365.0
238.90	220.0
240.80	567.0
242.10	426.0
243.10	462.0
244.00	6764.0
245.00	1152.0
246.00	1588.0
247.20	189.0
252.70	308.0
253.20	178.0
253.80	384.0
255.00	34952.0
256.00	4993.0
257.00	373.0
258.00	2789.0
259.00	636.0
264.90	956.0
272.00	267.0
273.00	882.0
274.00	2171.0
275.00	14949.0
275.90	1644.0
277.00	2135.0
278.10	323.0
280.70	182.0
282.20	254.0
282.80	234.0
284.00	203.0
285.20	195.0
285.50	165.0
286.10	191.0
292.80	314.0
295.20	454.0
296.00	5317.0
296.90	589.0
298.10	225.0
303.10	821.0
315.10	469.0
315.90	275.0
323.00	1485.0
324.00	335.0
327.10	454.0
328.00	444.0
333.20	168.0
333.90	661.0
334.90	362.0
341.10	218.0
345.80	327.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691

346.60	186.0
352.00	413.0
352.90	403.0
353.90	386.0
364.90	2809.0
365.90	648.0
372.10	377.0
402.00	373.0
402.90	480.0
403.90	239.0
420.60	157.0
421.00	168.0
421.90	758.0
423.00	2251.0
439.20	180.0
441.00	6607.0
442.00	46568.0
443.10	8285.0
443.90	964.0
534.90	163.0

Instrument :
BNA_G
ClientSampleId :
DFTPP691