


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121121\
 Data File : BG051477.D
 Acq On : 11 Dec 2021 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 23:03:39 2021

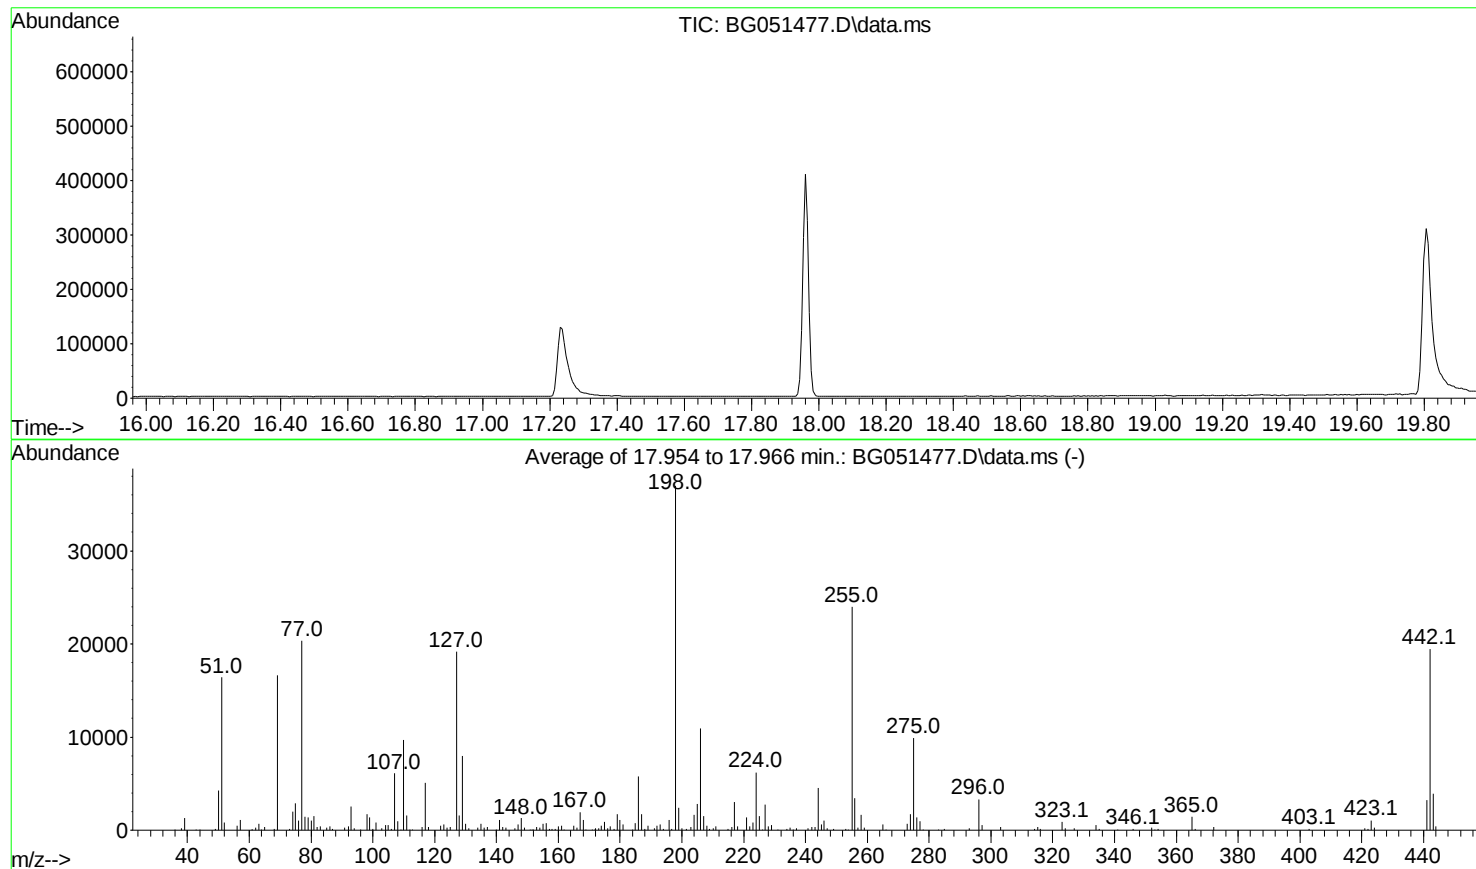

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	44.4	16427	PASS
68	69	0.00	2	1.0	173	PASS
69	198	0.00	100	44.9	16603	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	19197	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36984	PASS
199	198	5	9	6.5	2393	PASS
275	198	10	60	26.9	9931	PASS
365	198	1	100	3.9	1428	PASS
441	198	0.01	100	8.7	3233	PASS
442	442	50	100	100.0	19485	PASS
443	442	15	24	20.1	3919	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/11/2021	BNA_G	<u>BG051477.D</u>
Compound Name	Response	Retention Time
DDT	159702	21.009
DDD	714	20.616
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
714	160416	0.45

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121121\
Data File : BG051477.D
Acq On : 11 Dec 2021 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 11 23:37:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 23:03:39 2021
Response via : Initial Calibration

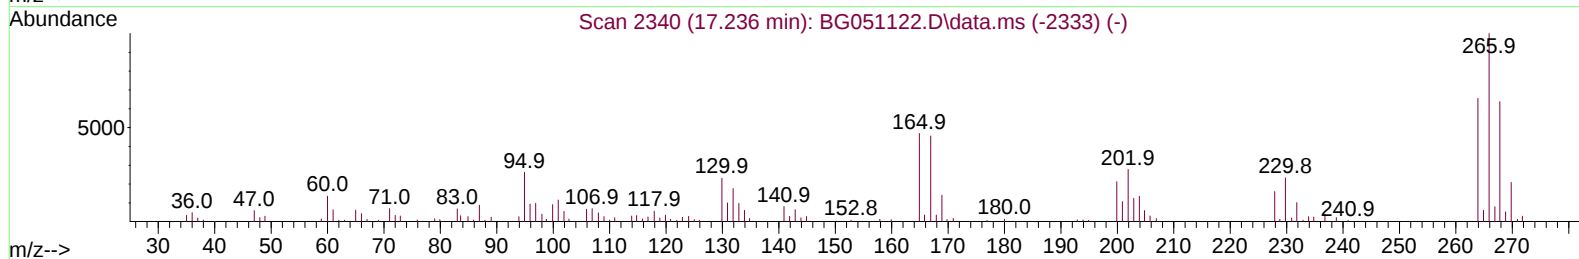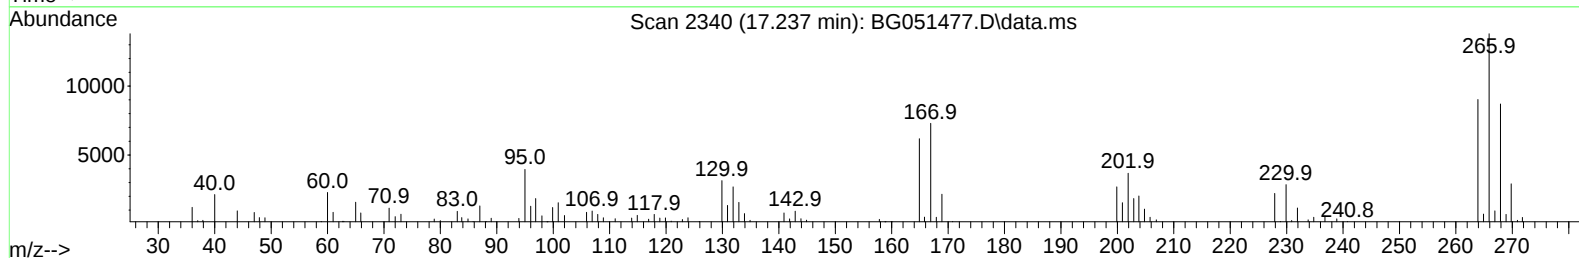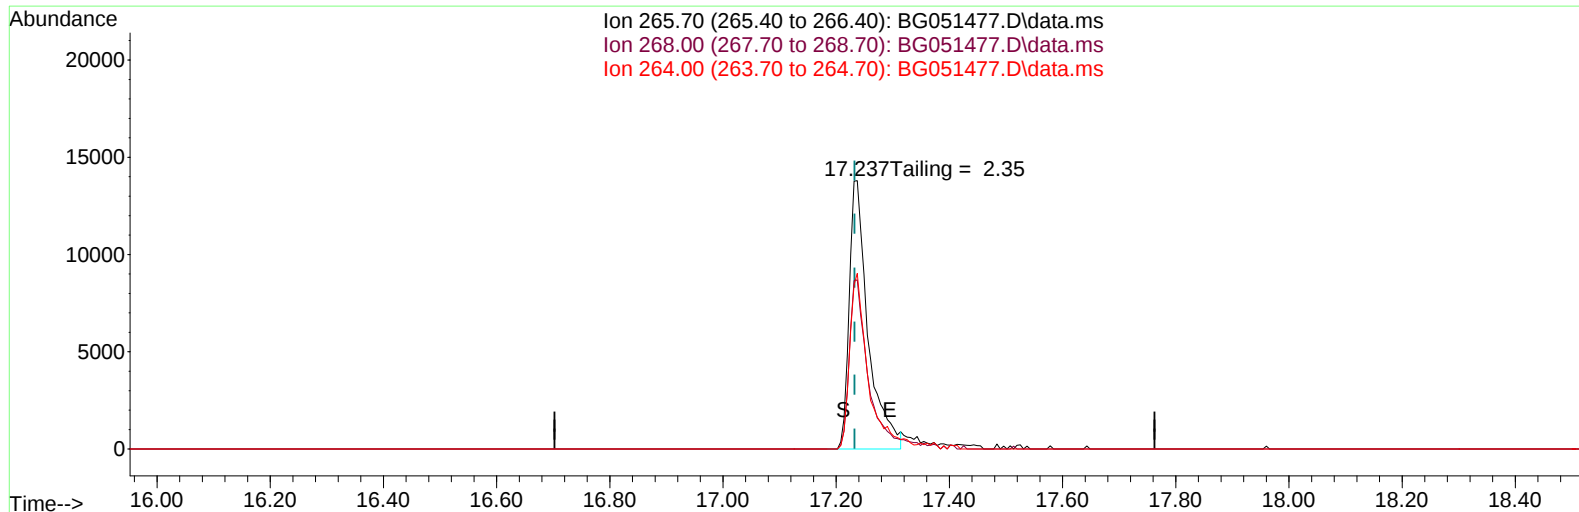

TIC: BG051477.D\data.ms

(70) Pentachlorophenol (C)

17.237min (+ 0.005) 43610.31 ng




response 33782

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.01
264.00	61.30	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121121\
Data File : BG051477.D
Acq On : 11 Dec 2021 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 11 23:37:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 23:03:39 2021
Response via : Initial Calibration

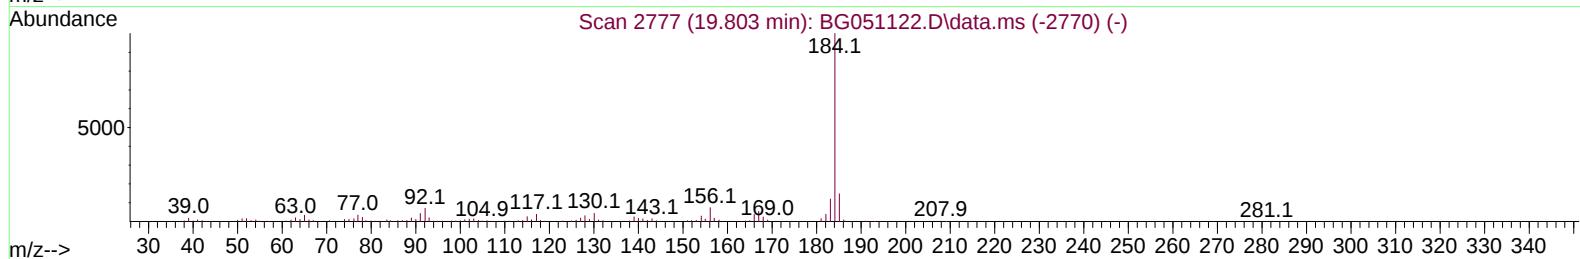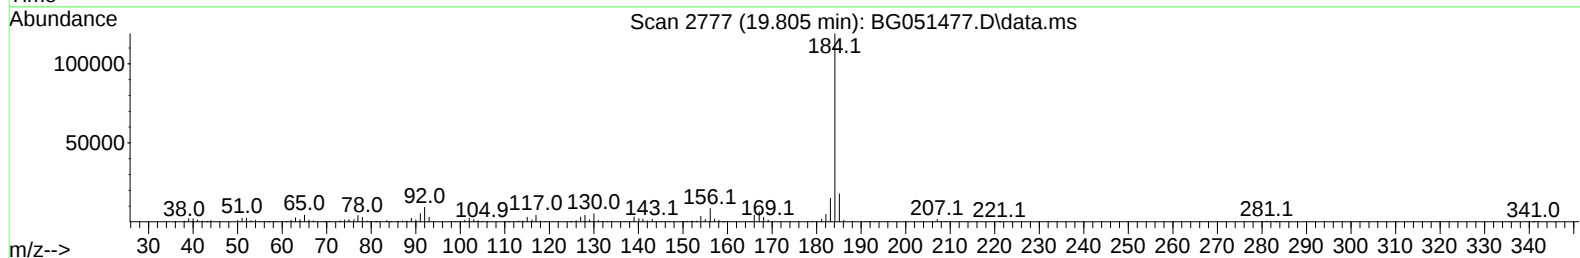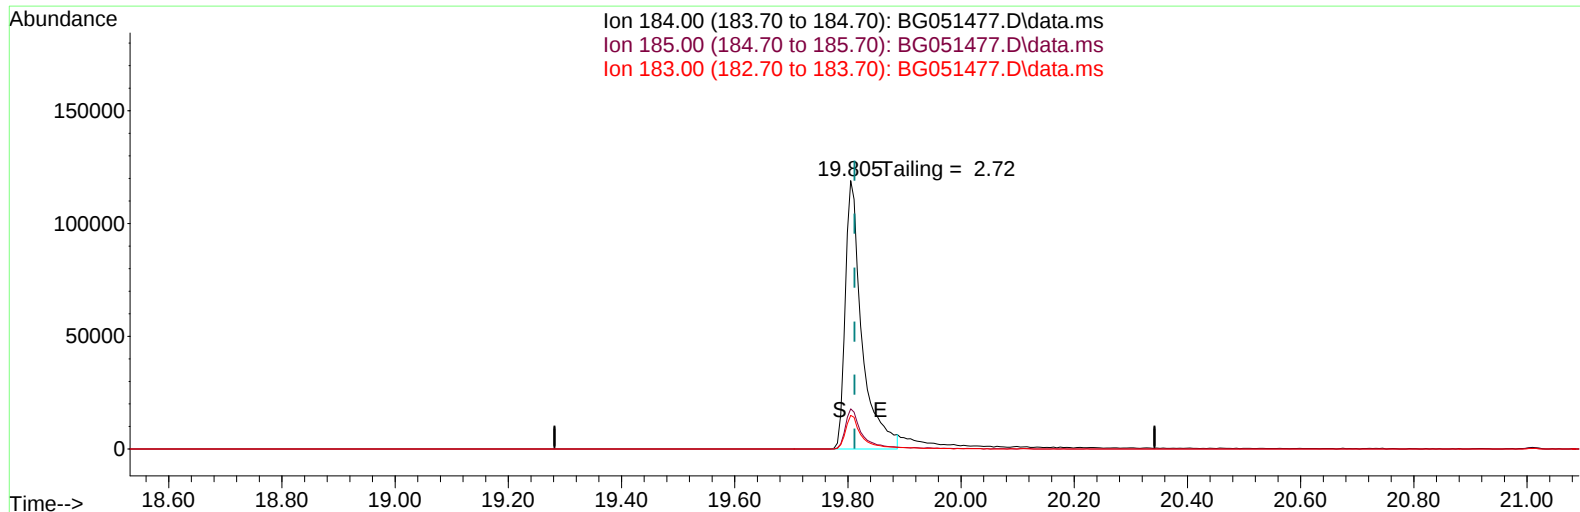

TIC: BG051477.D\data.ms

(77) Benzidine

19.805min (-0.007) 0.00 ng

response 268222

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.96
183.00	11.70	12.52
0.00	0.00	0.00