

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121215\
 Data File : BG020105.D
 Acq On : 11 Dec 2015 11:37
 Operator : UM/SJ
 Sample : G4683-09DL 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S21-15DL

Quant Time: Dec 11 14:39:11 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	21162	20.00	ng	-0.03
21) Naphthalene-d8	10.93	136	91560	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	61193	20.00	ng	-0.03
63) Phenanthrene-d10	17.48	188	145588	20.00	ng	-0.03
75) Chrysene-d12	21.76	240	179010	20.00	ng	-0.04
86) Perylene-d12	25.03	264	168109	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	87836	75.02	ng	-0.01
7) Phenol-d6	7.26	99	130577	73.86	ng	-0.02
23) Nitrobenzene-d5	9.28	82	86075	47.98	ng	-0.02
41) 2,4,6-Tribromophenol	16.22	330	62776	67.05	ng	-0.02
44) 2-Fluorobiphenyl	13.36	172	177558	39.62	ng	-0.03
78) Terphenyl-d14	20.08	244	297706	40.57	ng	-0.03
Target Compounds						Qvalue
31) Naphthalene	10.98	128	21652	4.41	ng	98
32) Benzoic acid	10.39	122	182	6.15	ng	# 1
37) 2-Methylnaphthalene	12.79	142	8443	2.35	ng	97
49) Dimethylphthalate	14.18	163	68578	12.46	ng	97
51) Acenaphthene	14.80	154	28376	7.09	ng	96
54) Dibenzofuran	15.13	168	32655	5.49	ng	94
55) 4-Nitrophenol	15.13	139	12568	13.42	ng	# 11
57) Fluorene	15.78	166	38885	7.30	ng	96
70) Phenanthrene	17.53	178	541428	65.73	ng	97
71) Anthracene	17.61	178	124822	14.88	ng	96
72) Carbazole	17.88	167	42610	5.76	ng	97
74) Fluoranthene	19.53	202	559603	53.11	ng	93
77) Pvrene	19.89	202	483092	45.87	ng	96
80) Benzo(a)anthracene	21.73	228	245726	22.42	ng	98
82) Chrysene	21.80	228	221241	21.26	ng	96
85) Indeno(1,2,3-cd)pyrene	28.78	276	84028	7.33	ng	# 100
87) Benzo(b)fluoranthene	24.25	252	23281	2.19	ng	93
88) Benzo(k)fluoranthene	24.25	252	30543	2.89	ng	93
89) Benzo(a)pvrene	24.72	252	96282	9.52	ng	97
90) Dibenzo(a,h)anthracene	28.84	278	24367	2.44	ng	# 91
91) Benzo(g,h,i)perylene	29.94	276	73964	7.54	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121215\
Data File : BG020105.D
Acq On : 11 Dec 2015 11:37
Operator : UM/SJ
Sample : G4683-09DL 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S21-15DL

Quant Time: Dec 11 14:39:11 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 8.11 min Scan# 897
 Delta R.T. -0.03 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37




Instrument :
 BNA_G
 ClientSampleId :
 S21-15DL


Tot Ion:152 Resp: 21162
 Ion Ratio Lower Upper
 152 100
 150 172.6 115.0 172.4#
 115 66.9 43.9 65.9#



#5
 2-Fluorophenol
 Concen: 75.02 ng
 RT: 5.66 min Scan# 480
 Delta R.T. -0.01 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37

Tgt Ion:112 Resp: 87836
 Ion Ratio Lower Upper
 112 100
 64 64.3 43.7 65.5
 63 35.1 24.0 36.0





#7

Phenol-d6

Concen: 73.86 ng

RT: 7.26 min Scan# 752

Delta R.T. -0.02 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampleId :

S21-15DL


Tot Ion: 99 Resp: 130577

Ion Ratio Lower Upper




99 100

42 18.2 11.5 17.3#

71 41.1 22.6 34.0#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.02 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Tgt Ion: 136 Resp: 91560


Ion Ratio Lower Upper

136 100



137 11.8 8.6 12.8


54 8.6 5.4 8.2#

68 6.6 5.3 7.9



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC







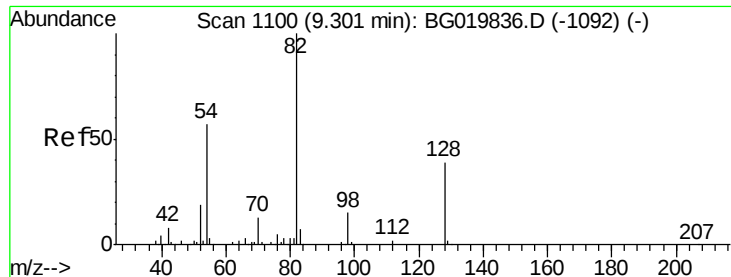

#23
 Nitrobenzene-d5
 Concen: 47.98 ng
 RT: 9.28 min Scan# 1096
 Delta R.T. -0.02 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37




Instrument :
 BNA_G
 ClientSampleId :
 S21-15DL


Tot Ion	82	Resp	86075
Ion Ratio	100	Lower	Upper
128	39.9	36.7	55.1
54	53.3	33.8	50.8#



#31
 Naphthalene
 Concen: 4.41 ng
 RT: 10.98 min Scan# 1385
 Delta R.T. -0.03 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37

Tgt Ion	128	Resp	21652
Ion Ratio	100	Lower	Upper
129	11.4	8.5	12.7
127	12.6	10.6	16.0





#32

Benzoic acid

Concen: 6.15 ng

RT: 10.39 min Scan# 1285

Delta R.T. 0.16 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampleId :

S21-15DL


Tot Ion:122 Resp: 182

Ion Ratio Lower Upper

122 100

105 0.0 103.8 143.8#




77 0.0 68.8 108.8#



Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): B



#37

2-Methylnaphthalene

Concen: 2.35 ng

RT: 12.79 min Scan# 1694

Delta R.T. 0.19 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37


Tgt Ion:142 Resp: 8443

Ion Ratio Lower Upper

142 100

141 94.3 74.6 112.0



115 39.0 27.4 41.0




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E





#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.74 min Scan# 2025

Delta R.T. -0.03 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampleId :

S21-15DL


Tot Ion:164 Resp: 61193

Ion Ratio Lower Upper

164 100

162 102.9 78.8 118.2




160 45.2 36.4 54.6



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



#41

2,4,6-Tribromophenol

Concen: 67.05 ng

RT: 16.22 min Scan# 2278

Delta R.T. -0.02 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37


Tgt Ion:330 Resp: 62776

Ion Ratio Lower Upper

330 100

332 95.5 78.1 117.1



141 36.0 28.2 42.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E









#44
2-Fluorobiphenyl
Concen: 39.62 ng
RT: 13.36 min Scan# 1791
Delta R.T. -0.03 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37




Instrument :
BNA_G
ClientSampleId :
S21-15DL


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.0	29.0	43.6
170	23.5	19.9	29.9



#49
Dimethylphthalate
Concen: 12.46 ng
RT: 14.18 min Scan# 1931
Delta R.T. -0.04 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.1	4.7
164	9.7	8.8	13.2





#51

Acenaphthene

Concen: 7.09 ng

RT: 14.80 min Scan# 2036

Delta R.T. -0.03 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampled :

S21-15DL


Tot Ion:154 Resp: 28376

Ion Ratio Lower Upper




154 100

153 114.1 92.9 139.3

152 51.2 45.8 68.8



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



#54

Dibenzofuran

Concen: 5.49 ng

RT: 15.13 min Scan# 2092

Delta R.T. -0.03 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37


Tgt Ion:168 Resp: 32655

Ion Ratio Lower Upper



168 100


139 38.8 27.4 41.0

169 13.8 11.0 16.4



Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 169.00 (168.70 to 169.70): E









#55
4-Nitrophenol
Concen: 13.42 ng
RT: 15.13 min Scan# 2092
Delta R.T. 0.18 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Instrument :
BNA_G
ClientSampled :
S21-15DL

Tot Ion:139 Resp: 12568
Ion Ratio Lower Upper
139 100
109 0.0 43.2 83.2#
65 0.0 67.8 107.8#




Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): B






#57
Fluorene
Concen: 7.30 ng
RT: 15.78 min Scan# 2203
Delta R.T. -0.03 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Tgt Ion:166 Resp: 38885
Ion Ratio Lower Upper
166 100
165 104.4 80.0 120.0
167 15.3 11.1 16.7



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E









#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.48 min Scan# 2492
Delta R.T. -0.03 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Instrument :
BNA_G
ClientSampleId :
S21-15DL

Tot Ion:188 Resp: 145588
Ion Ratio Lower Upper
188 100
94 6.7 7.7 11.5#
80 8.1 7.8 11.8




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGO
Ion 80.00 (79.70 to 80.70): BGO






#70
Phenanthrene
Concen: 65.73 ng
RT: 17.53 min Scan# 2500
Delta R.T. -0.02 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Tgt Ion:178 Resp: 541428
Ion Ratio Lower Upper
178 100
176 19.3 16.7 25.1
179 16.3 13.9 20.9



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E









#71
 Anthracene
 Concen: 14.88 ng
 RT: 17.61 min Scan# 2515
 Delta R.T. -0.02 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37




Instrument :
 BNA_G
 ClientSampleId :
 S21-15DL


Tot Ion	Ratio	Lower	Upper
178	100		
176	18.9	16.8	25.2
179	15.7	13.9	20.9



#72
 Carbazole
 Concen: 5.76 ng
 RT: 17.88 min Scan# 2560
 Delta R.T. -0.02 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37

Tgt Ion	Ratio	Lower	Upper
167	100		
166	22.0	19.0	28.6
139	13.2	10.2	15.4





#74

Fluoranthene

Concen: 53.11 ng

RT: 19.53 min Scan# 2841

Delta R.T. -0.02 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampleId :

S21-15DL


Tot Ion:202 Resp: 559603

Ion Ratio Lower Upper

202 100

101 7.4 0.0 32.4




203 17.9 0.0 39.5



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.76 min Scan# 3220

Delta R.T. -0.04 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37


Tgt Ion:240 Resp: 179010

Ion Ratio Lower Upper

240 100

120 6.7 7.4 11.0#



236 25.5 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E









#77
Pvrene
Concen: 45.87 ng
RT: 19.89 min Scan# 2902
Delta R.T. -0.02 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37




Instrument :
BNA_G
ClientSampleId :
S21-15DL


Tot Ion	Ratio	Lower	Upper
202	100		
200	21.5	19.4	29.0
203	18.8	15.5	23.3



#78
Terphenyl-d14
Concen: 40.57 ng
RT: 20.08 min Scan# 2935
Delta R.T. -0.03 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.7	6.9	10.3
122	7.3	10.2	15.2#









#80
Benzo(a)anthracene
Concen: 22.42 ng
RT: 21.73 min Scan# 3216
Delta R.T. -0.04 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37




Instrument :
BNA_G
ClientSampleId :
S21-15DL


Tot Ion:228 Resp: 245726
Ion Ratio Lower Upper
228 100
226 28.0 23.4 35.0
229 21.4 16.6 25.0



#82
Chrysene
Concen: 21.26 ng
RT: 21.80 min Scan# 3228
Delta R.T. -0.04 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Tgt Ion:228 Resp: 221241
Ion Ratio Lower Upper
228 100
226 30.2 26.7 40.1
229 22.3 17.0 25.6









#85
 Indeno(1,2,3-cd)pyrene
 Concen: 7.33 ng
 RT: 28.78 min Scan# 4415
 Delta R.T. -0.11 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37




Instrument :
 BNA_G
 ClientSampleId :
 S21-15DL


Tot Ion:276 Resp: 84028
 Ion Ratio Lower Upper
 276 100
 138 14.1 0.0 0.0#
 277 23.7 0.0 0.0#



#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.03 min Scan# 3777
 Delta R.T. -0.06 min
 Lab File: BG020105.D
 Acq: 11 Dec 2015 11:37

Tgt Ion:264 Resp: 168109
 Ion Ratio Lower Upper
 264 100
 260 22.6 18.5 27.7
 265 21.8 17.2 25.8









#87
Benzo(b)fluoranthene
Concen: 2.19 ng
RT: 24.25 min Scan# 3644
Delta R.T. 0.20 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37




Instrument :
BNA_G
ClientSampleId :
S21-15DL


Tot Ion:252 Resp: 23281
Ion Ratio Lower Upper
252 100
253 28.4 19.1 28.7
125 10.2 8.9 13.3



#88
Benzo(k)fluoranthene
Concen: 2.89 ng
RT: 24.25 min Scan# 3644
Delta R.T. 0.13 min
Lab File: BG020105.D
Acq: 11 Dec 2015 11:37

Tgt Ion:252 Resp: 30543
Ion Ratio Lower Upper
252 100
253 28.4 19.0 28.4
125 10.2 8.9 13.3





#89

Benzo(a)pyrene

Concen: 9.52 ng

RT: 24.72 min Scan# 3725

Delta R.T. -0.22 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampleId :

S21-15DL


Tot Ion:252 Resp: 96282

Ion Ratio Lower Upper

252 100

253 22.5 18.7 28.1




125 9.7 9.1 13.7



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#90

Dibenzo(a,h)anthracene

Concen: 2.44 ng

RT: 28.84 min Scan# 4425

Delta R.T. -0.12 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37


Tgt Ion:278 Resp: 24367

Ion Ratio Lower Upper

278 100

139 10.1 13.8 20.6#



279 22.2 19.4 29.0




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E





#91

Benzo(a,h,i)perylene

Concen: 7.54 ng

RT: 29.94 min Scan# 4613

Delta R.T. -0.13 min

Lab File: BG020105.D

Acq: 11 Dec 2015 11:37

Instrument :

BNA_G

ClientSampleId :

S21-15DL


Tot Ion: 276 Resp: 73964

Ion Ratio Lower Upper

276 100

277 26.3 18.4 27.6

138 14.4 17.4 26.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

