
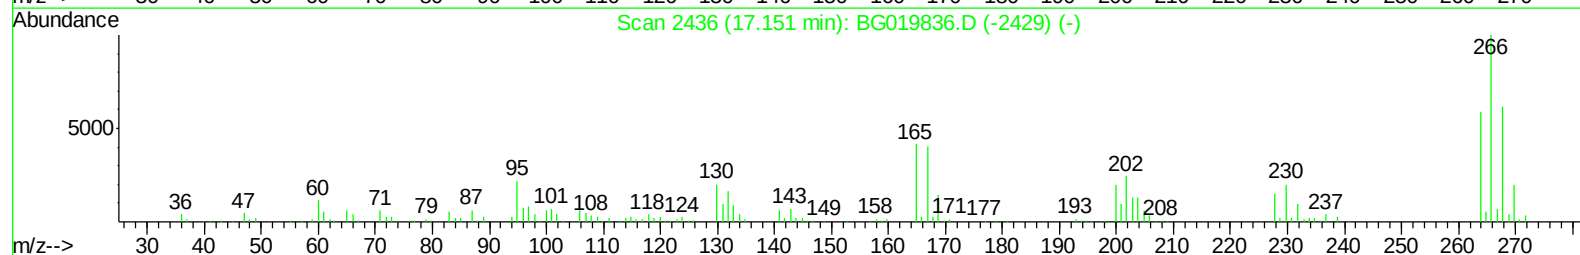
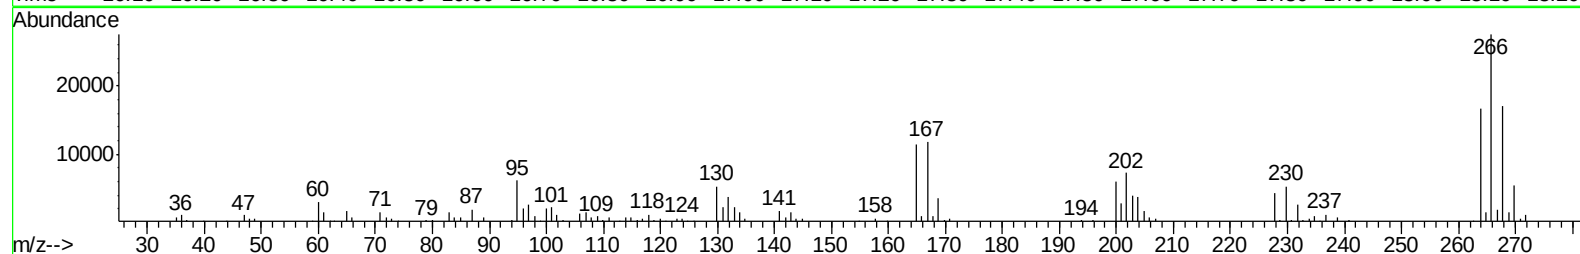


Data Path : Z:\HPCHEM1\BNA\_G\Data\BG121215\  
Data File : BG020102.D  
Acq On : 11 Dec 2015 9:18  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 04:44:55 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG120215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 02 18:50:01 2015  
Response via : Initial Calibration

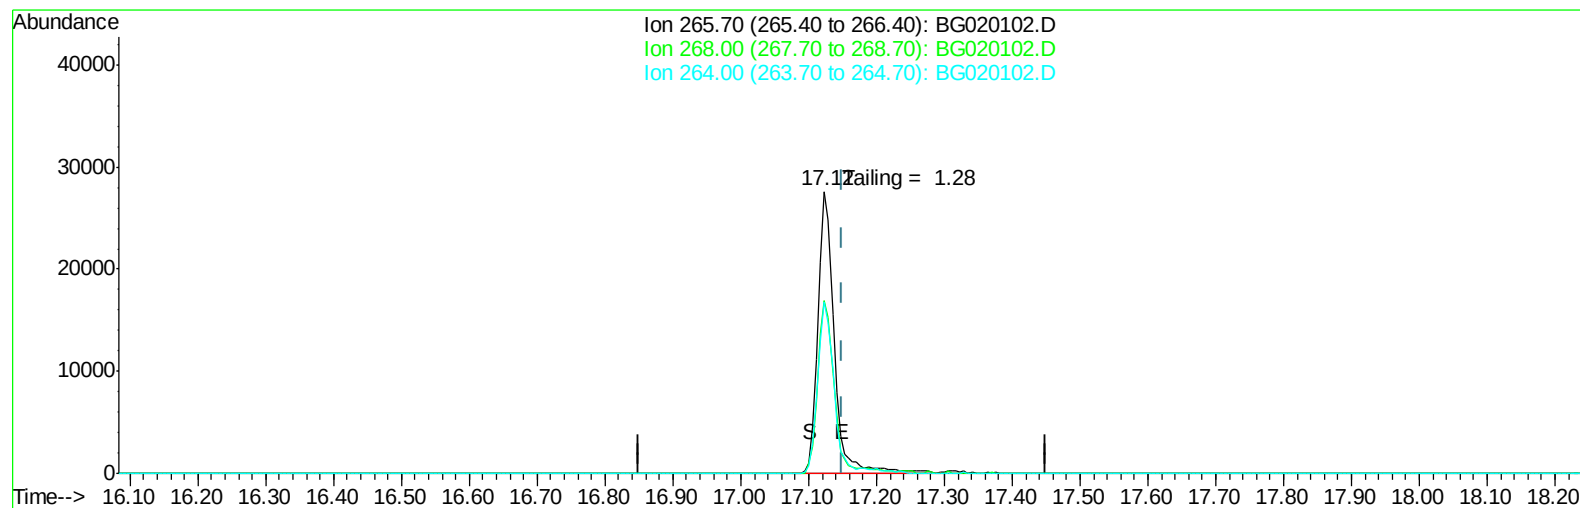

TIC: BG020102.D

(69) Pentachlorophenol (C)




17.123min (-0.027) 0.00ng

response 45300

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 59.50 | 61.59 |
| 264.00 | 60.10 | 60.78 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\Data\BG121215\  
 Data File : BG020102.D  
 Acq On : 11 Dec 2015 9:18  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 04:44:55 2015  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG120215.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 02 18:50:01 2015  
 Response via : Initial Calibration

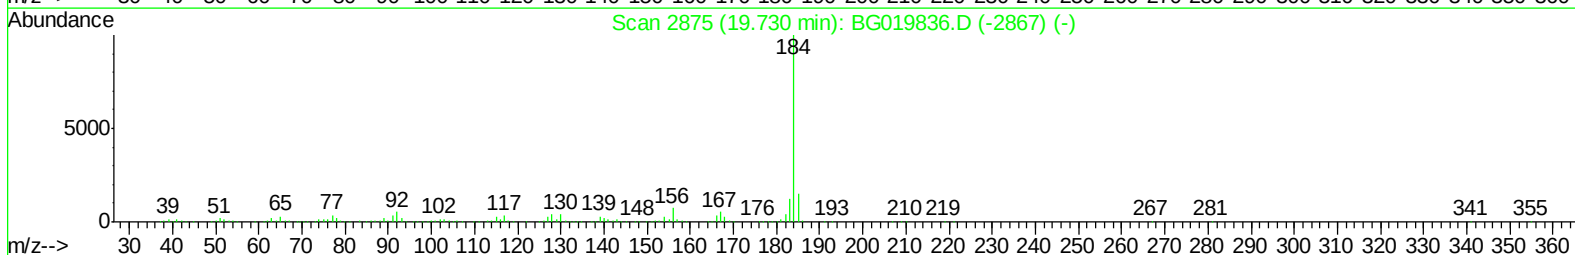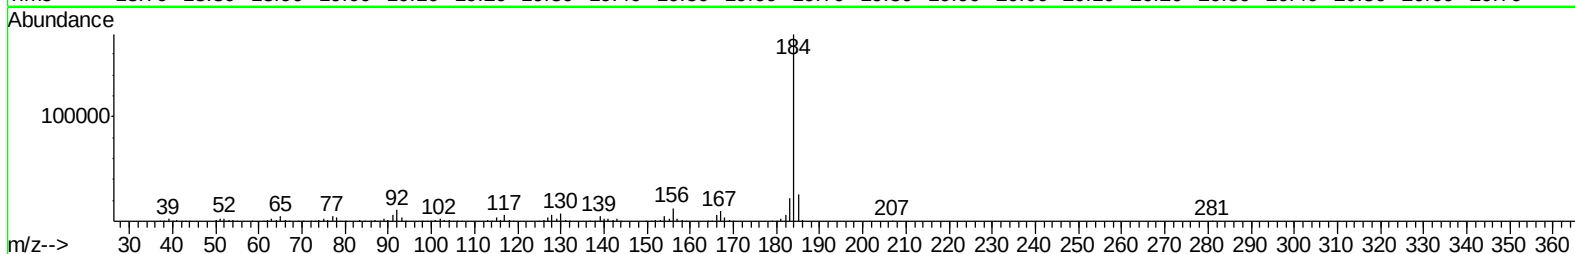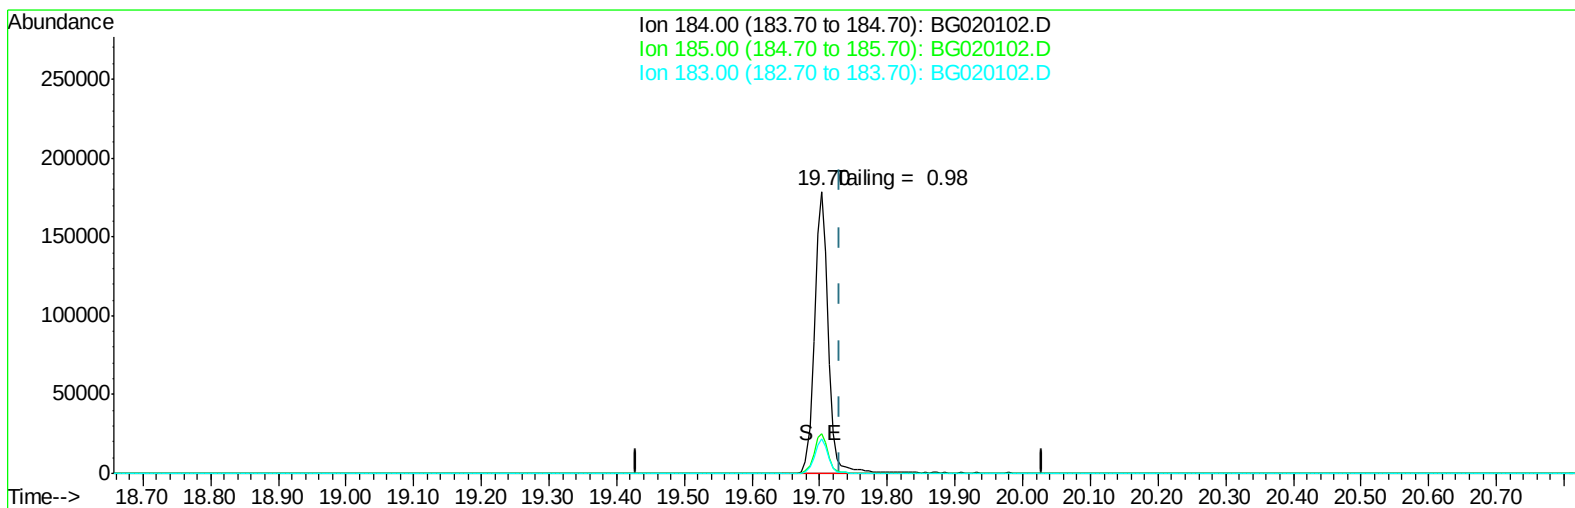

TIC: BG020102.D

(76) Benzidine

19.703min (-0.027) 0.00ng

response 256192

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.80 | 14.25 |
| 183.00 | 12.60 | 12.28 |
| 0.00   | 0.00  | 0.00  |