
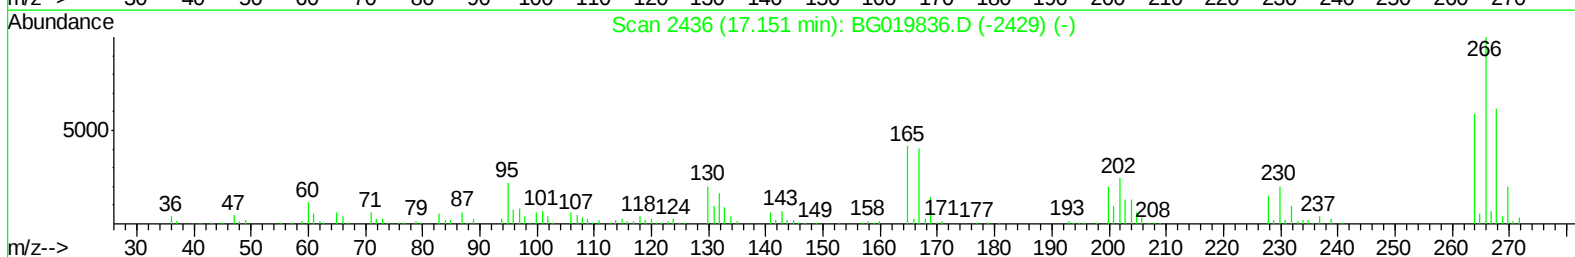
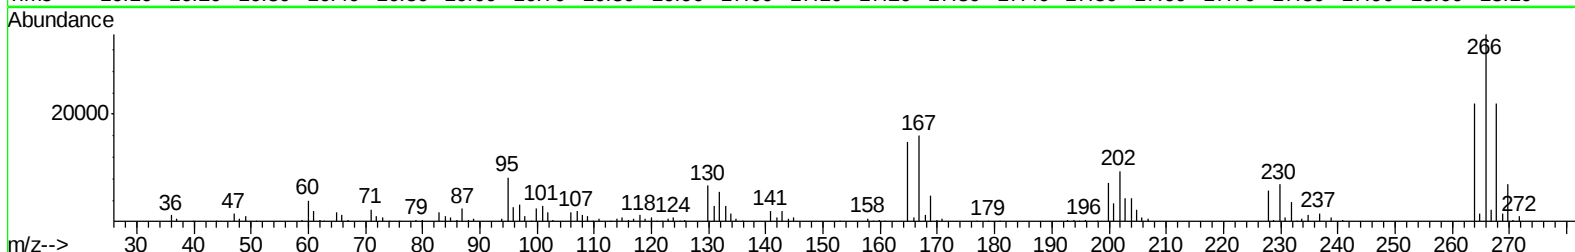


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121215\
Data File : BG020108.D
Acq On : 11 Dec 2015 16:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 04:45:46 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

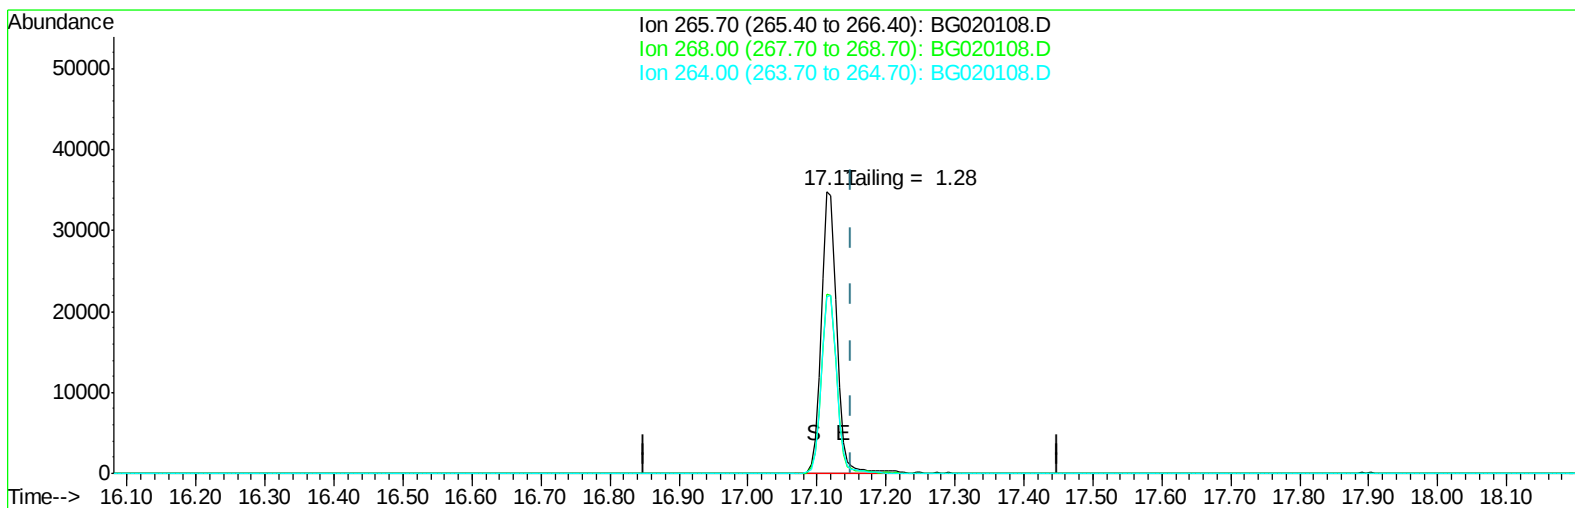

TIC: BG020108.D

(69) Pentachlorophenol (C)




17.115min (-0.035) 0.00ng

response 53195

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	63.53
264.00	60.10	62.93
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_G\Data\BG121215\  
Data File : BG020108.D  
Acq On    : 11 Dec 2015   16:02  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Dec 12 04:45:46 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

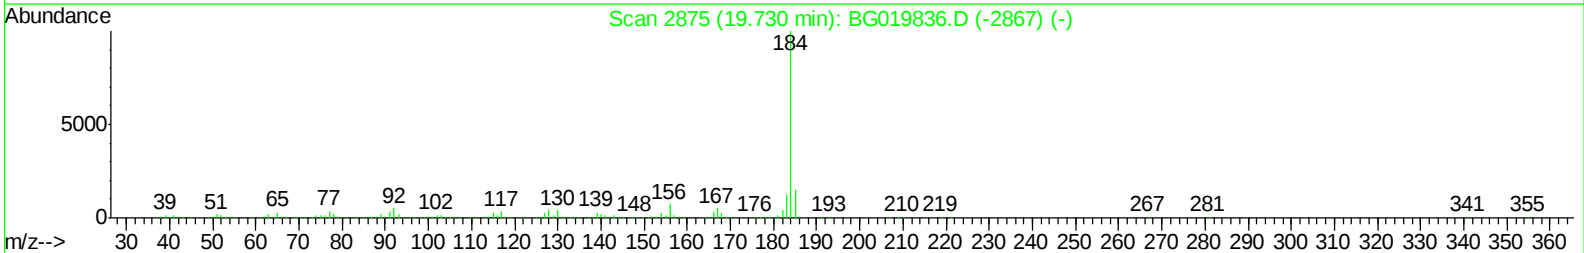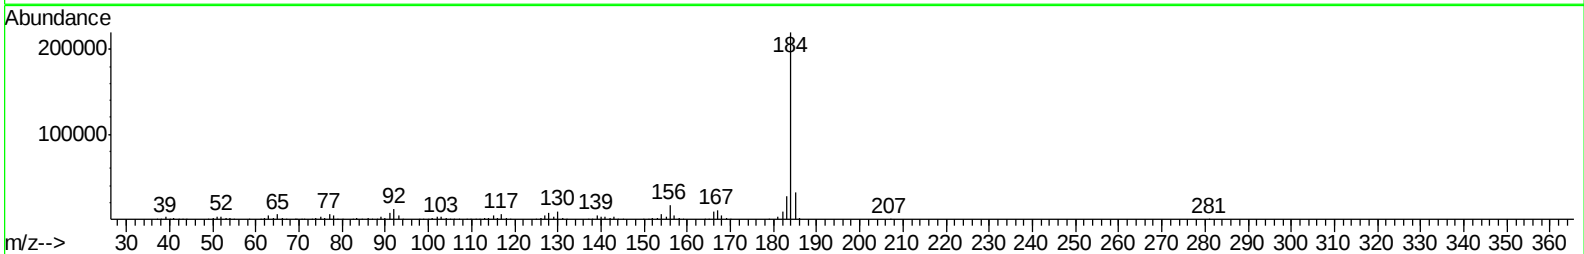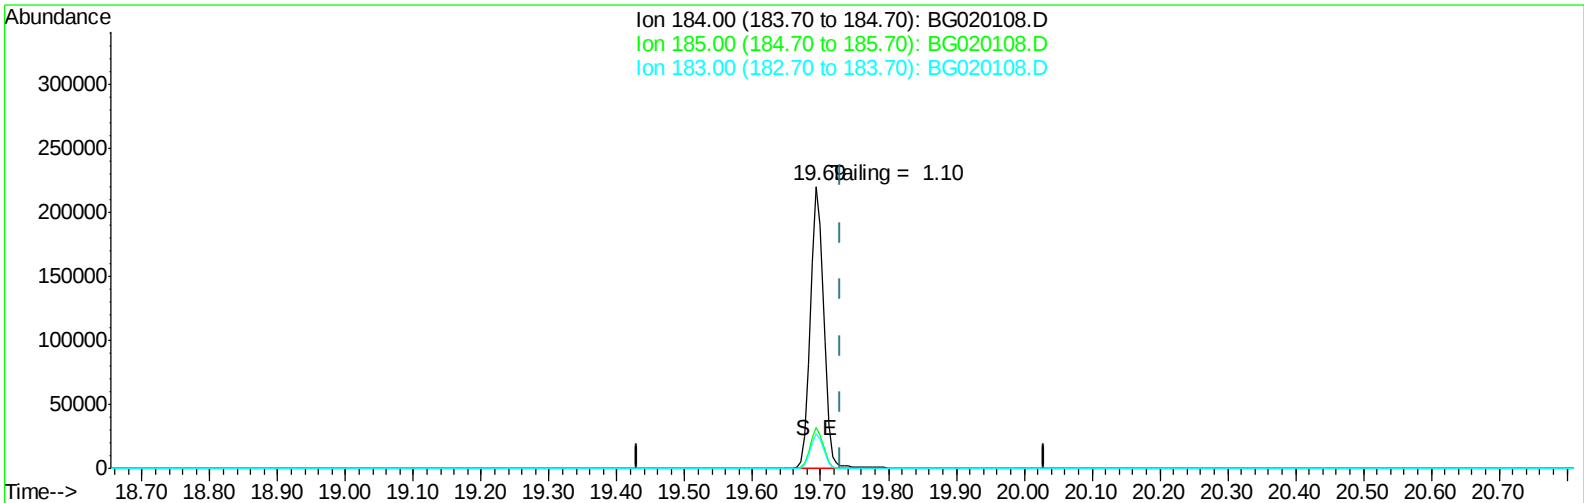

TIC: BG020108.D

(76) Benzidine

19.694min (-0.036) 0.00ng

response 296886

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.48
183.00	12.60	12.47
0.00	0.00	0.00