

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121215\  
 Data File : BG020119.D  
 Acq On : 11 Dec 2015 23:22  
 Operator : UM/SJ  
 Sample : PB87210BL  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB87210BL

Quant Time: Dec 12 00:21:40 2015  
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 02 18:50:01 2015  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|-----------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.10  | 152  | 22531    | 20.00 | ng    | -0.03    |
| 21) Naphthalene-d8          | 10.92 | 136  | 90437    | 20.00 | ng    | -0.03    |
| 38) Acenaphthene-d10        | 14.73 | 164  | 67599    | 20.00 | ng    | -0.04    |
| 63) Phenanthrene-d10        | 17.47 | 188  | 188104   | 20.00 | ng    | -0.04    |
| 75) Chrysene-d12            | 21.74 | 240  | 224468   | 20.00 | ng    | -0.05    |
| 86) Perylene-d12            | 25.01 | 264  | 207651   | 20.00 | ng    | -0.09    |
| System Monitoring Compounds |       |      |          |       |       |          |
| 5) 2-Fluorophenol           | 5.65  | 112  | 93890    | 75.32 | ng    | -0.02    |
| 7) Phenol-d6                | 7.25  | 99   | 136423   | 72.48 | ng    | -0.02    |
| 23) Nitrobenzene-d5         | 9.27  | 82   | 125455   | 70.80 | ng    | -0.03    |
| 41) 2,4,6-Tribromophenol    | 16.21 | 330  | 76306    | 73.77 | ng    | -0.03    |
| 44) 2-Fluorobiphenyl        | 13.35 | 172  | 323213   | 65.28 | ng    | -0.04    |
| 78) Terphenyl-d14           | 20.07 | 244  | 664975   | 72.26 | ng    | -0.04    |


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121215\  
Data File : BG020119.D  
Acq On : 11 Dec 2015 23:22  
Operator : UM/SJ  
Sample : PB87210BL  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB87210BL

Quant Time: Dec 12 00:21:40 2015  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 02 18:50:01 2015  
Response via : Initial Calibration

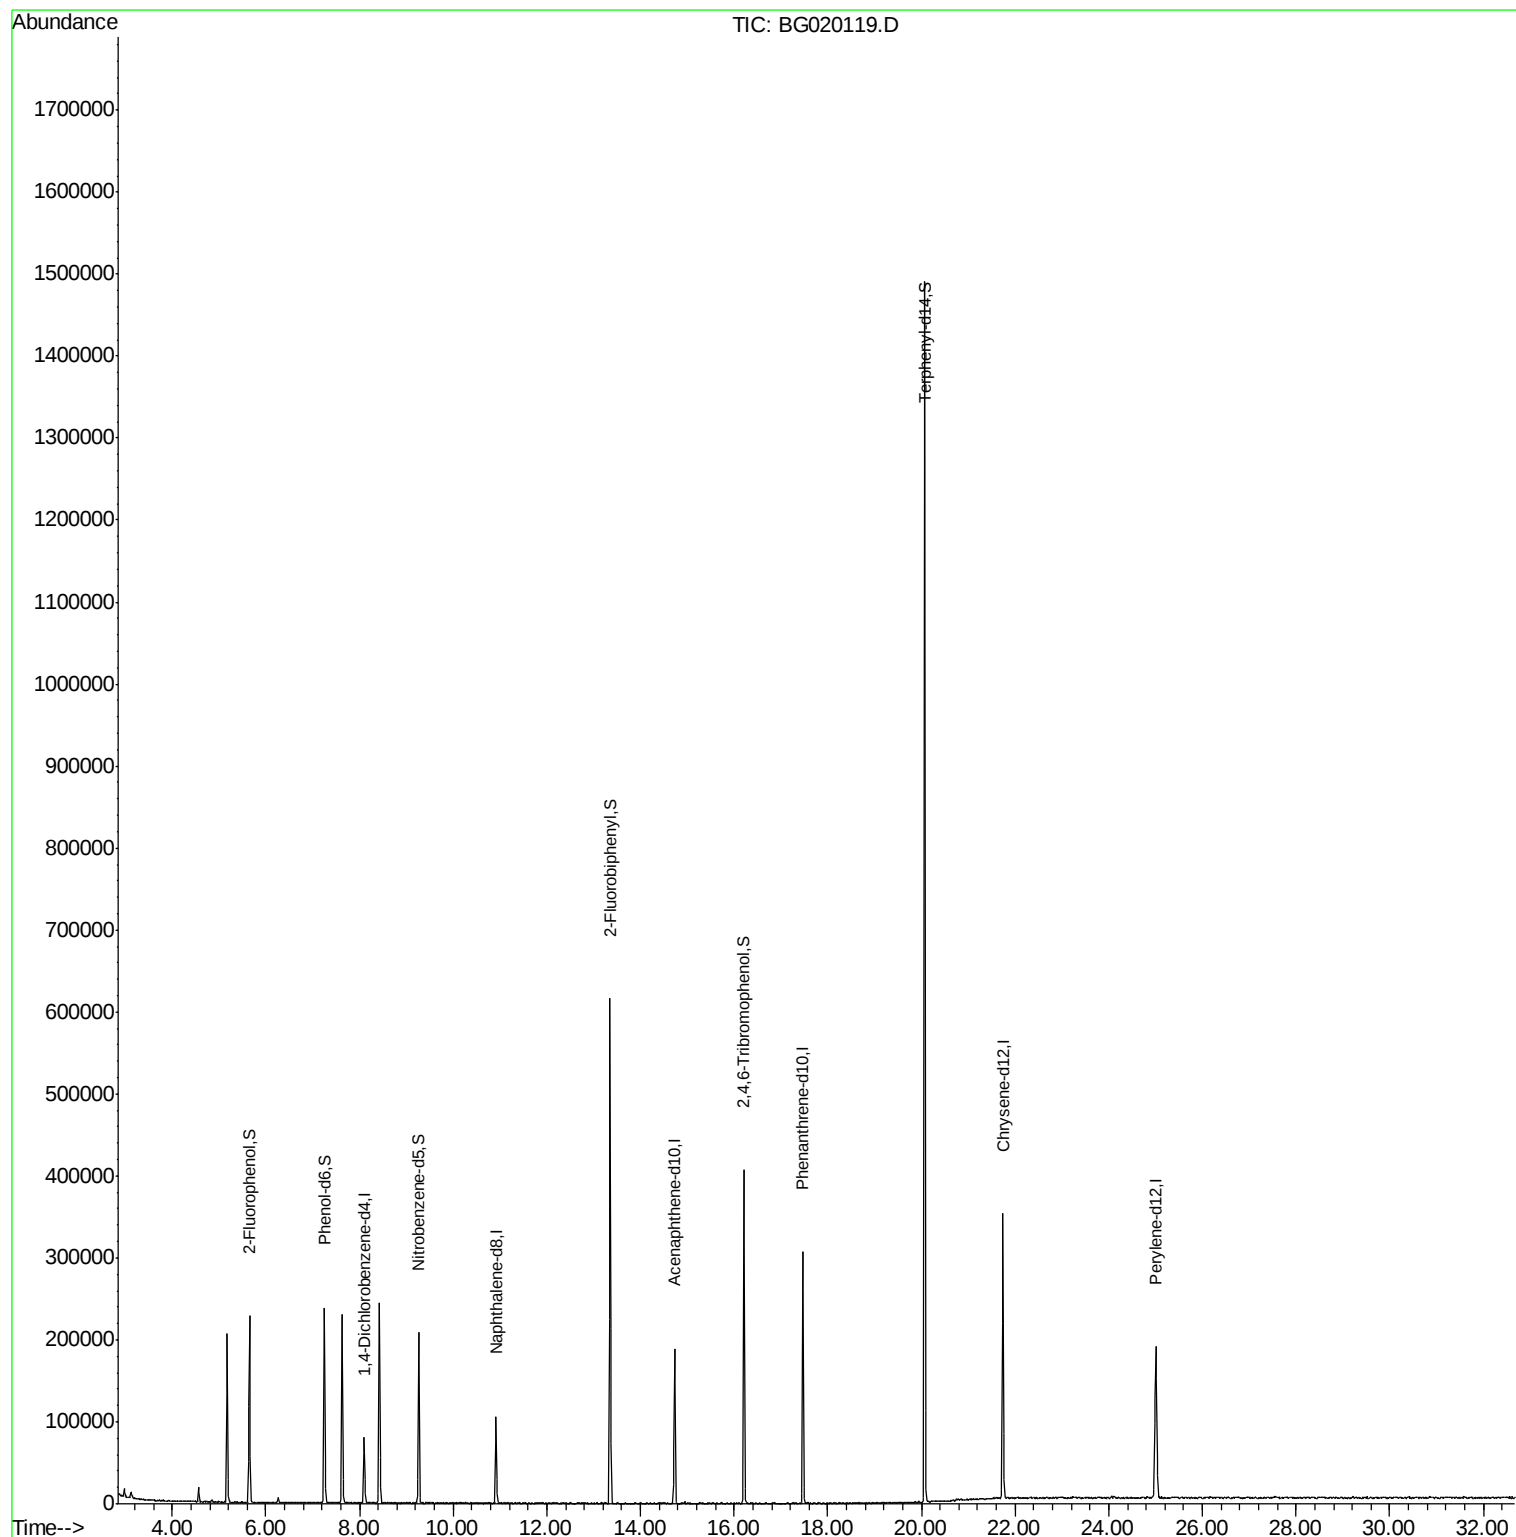

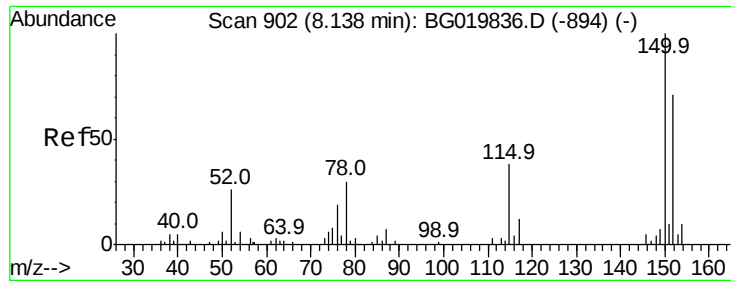

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.10 min Scan# 896

Delta R.T. -0.03 min

Lab File: BG020119.D

Acq: 11 Dec 2015 23:22

Instrument :

BNA\_G

ClientSampled :

PB87210BL


Tot Ion:152 Resp: 22531

Ion Ratio Lower Upper

152 100

150 140.9 115.0 172.4




115 55.3 43.9 65.9

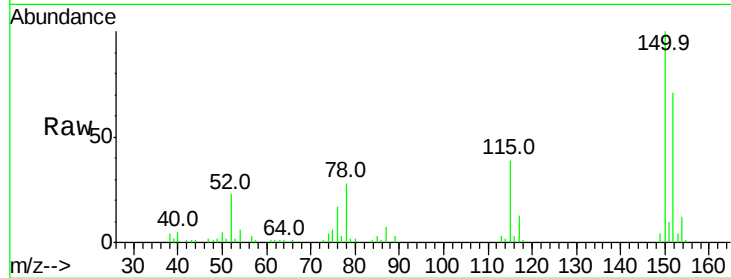

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

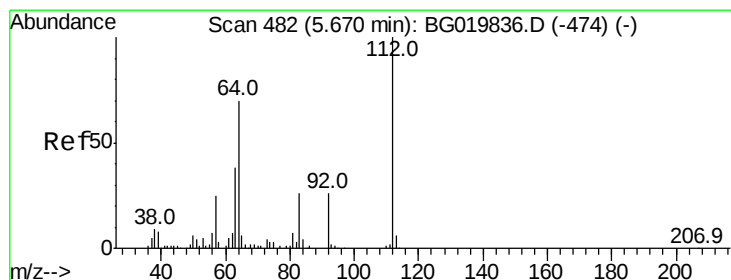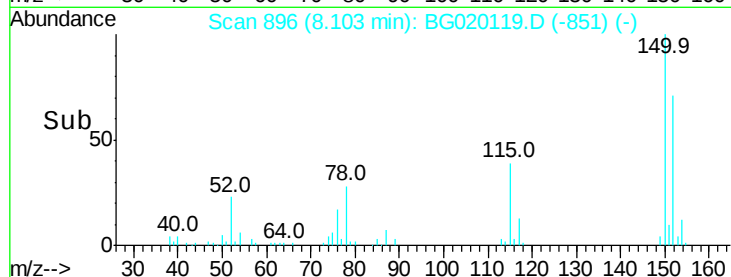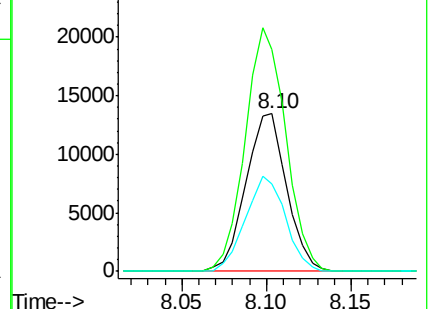

#5

2-Fluorophenol

Concen: 75.32 ng

RT: 5.65 min Scan# 478

Delta R.T. -0.02 min

Lab File: BG020119.D

Acq: 11 Dec 2015 23:22


Tgt Ion:112 Resp: 93890

Ion Ratio Lower Upper

112 100

64 63.7 43.7 65.5



63 35.6 24.0 36.0

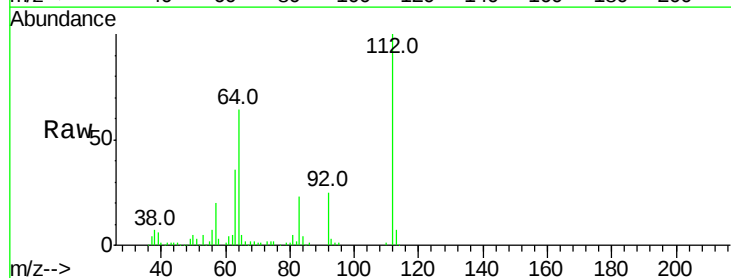


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

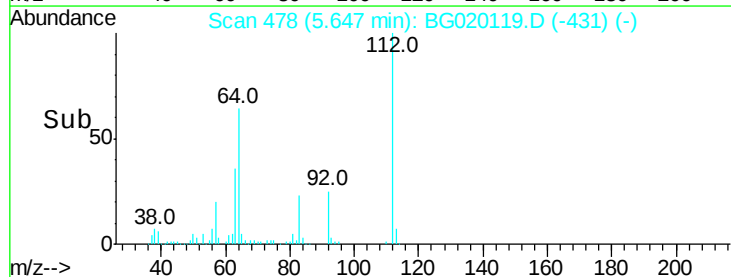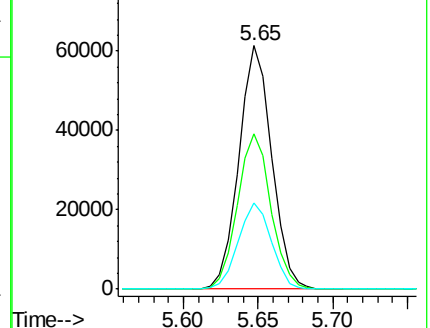

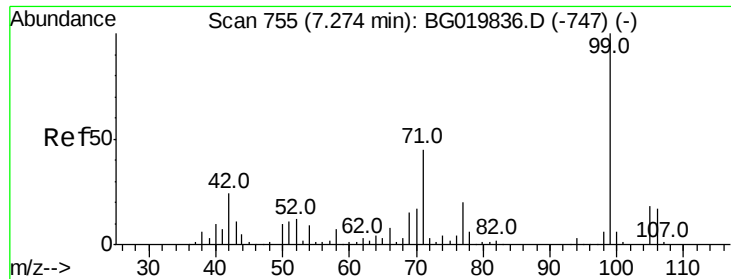

#7

Phenol-d6

Concen: 72.48 ng

RT: 7.25 min Scan# 751

Delta R.T. -0.02 min

Lab File: BG020119.D

Acq: 11 Dec 2015 23:22

Instrument :

BNA\_G

ClientSampled :

PB87210BL


Tot Ion: 99 Resp: 136423

Ion Ratio Lower Upper




99 100

42 18.0 11.5 17.3#

71 39.6 22.6 34.0#

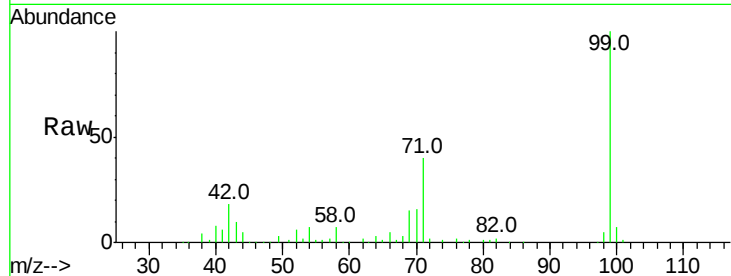

Abundance Ion 99.00 (98.70 to 99.70): BGC  
Ion 42.00 (41.70 to 42.70): BGC  
Ion 71.00 (70.70 to 71.70): BGC

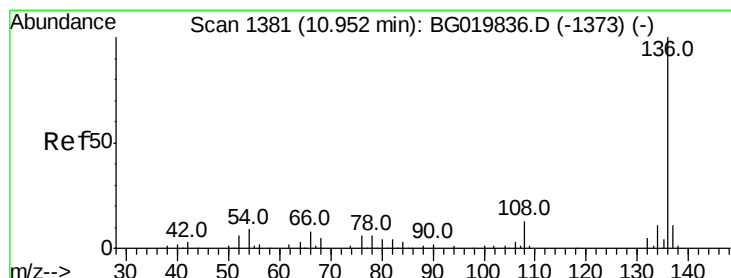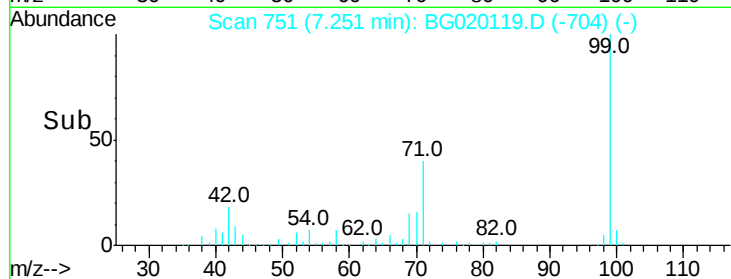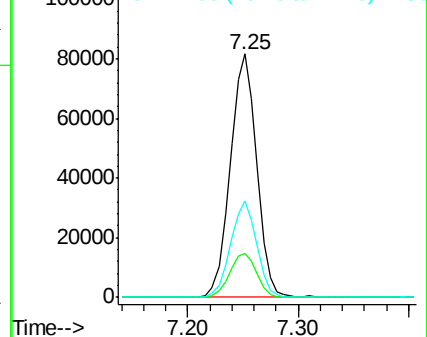

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.92 min Scan# 1375

Delta R.T. -0.03 min

Lab File: BG020119.D

Acq: 11 Dec 2015 23:22

Tgt Ion: 136 Resp: 90437


Ion Ratio Lower Upper

136 100



137 11.2 8.6 12.8


54 8.5 5.4 8.2#

68 6.9 5.3 7.9

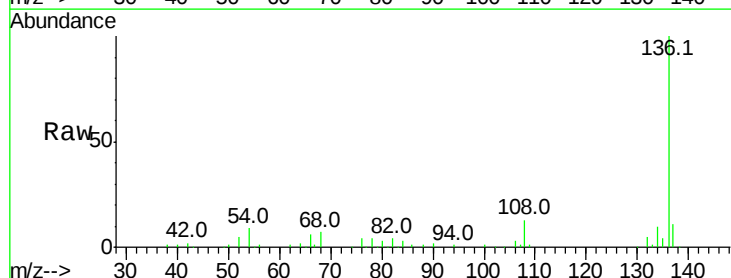

Abundance Ion 136.00 (135.70 to 136.70): BGC  
Ion 137.00 (136.70 to 137.70): BGC  
Ion 54.00 (53.70 to 54.70): BGC  
Ion 68.00 (67.70 to 68.70): BGC


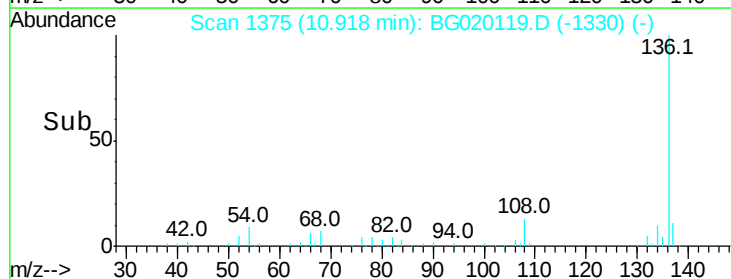
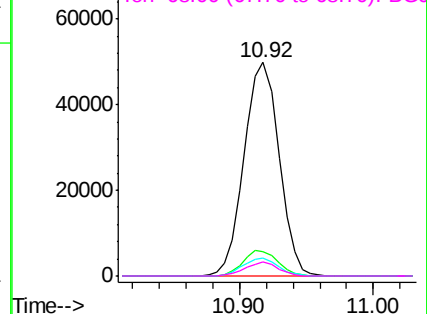


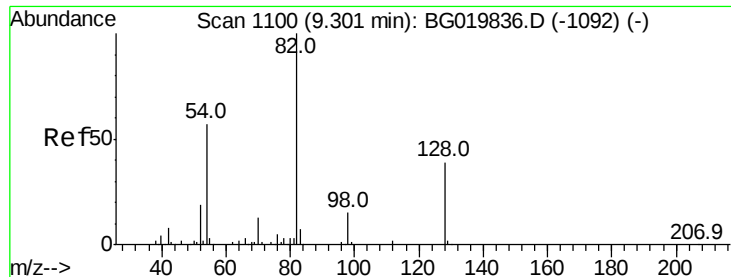

#23  
Nitrobenzene-d5  
Concen: 70.80 ng  
RT: 9.27 min Scan# 1094  
Delta R.T. -0.03 min  
Lab File: BG020119.D  
Acq: 11 Dec 2015 23:22




Instrument :  
BNA\_G  
ClientSampleId :  
PB87210BL

| Tot Ion   | 82   | Resp  | 125455 |
|-----------|------|-------|--------|
| Ion Ratio | 100  | Lower | Upper  |
| 128       | 39.6 | 36.7  | 55.1   |
| 54        | 49.9 | 33.8  | 50.8   |

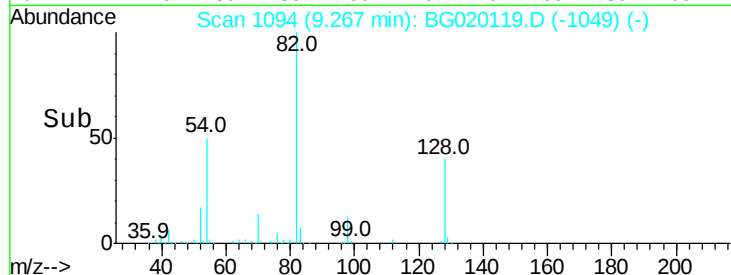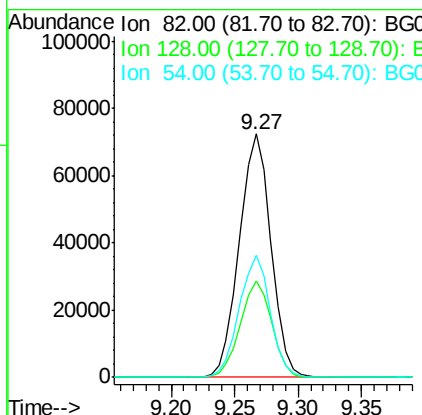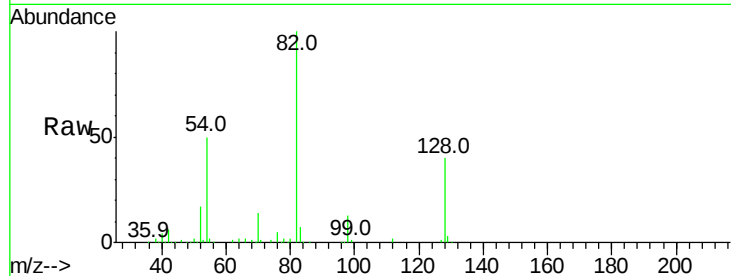

#38  
Acenaphthene-d10  
Concen: 20.00 ng  
RT: 14.73 min Scan# 2023  
Delta R.T. -0.04 min  
Lab File: BG020119.D  
Acq: 11 Dec 2015 23:22

| Tgt Ion   | 164   | Resp  | 67599 |
|-----------|-------|-------|-------|
| Ion Ratio | 100   | Lower | Upper |
| 162       | 103.1 | 78.8  | 118.2 |
| 160       | 44.8  | 36.4  | 54.6  |

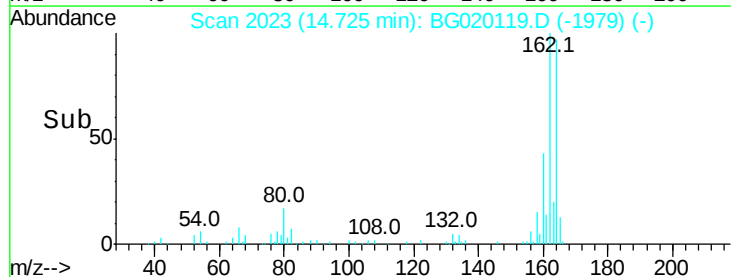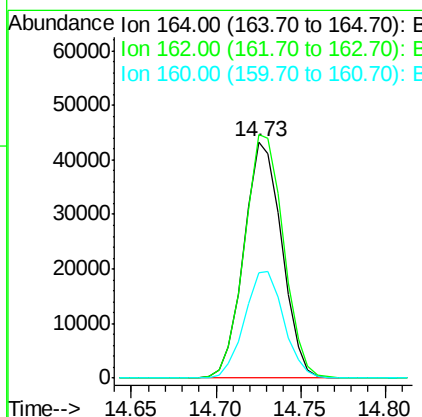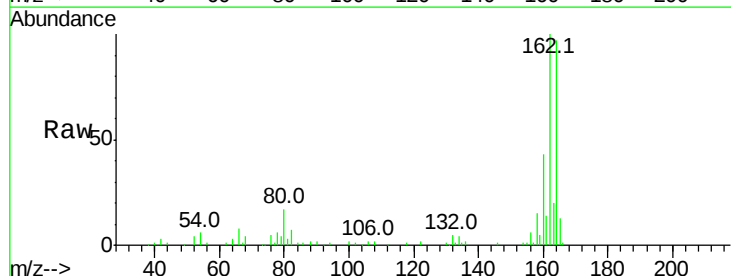






#41  
 2,4,6-Tribromophenol  
 Concen: 73.77 ng  
 RT: 16.21 min Scan# 2276  
 Delta R.T. -0.03 min  
 Lab File: BG020119.D  
 Acq: 11 Dec 2015 23:22

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB87210BL

Tot Ion:330 Resp: 76306  
 Ion Ratio Lower Upper  
 330 100  
 332 94.7 78.1 117.1  
 141 35.6 28.2 42.2

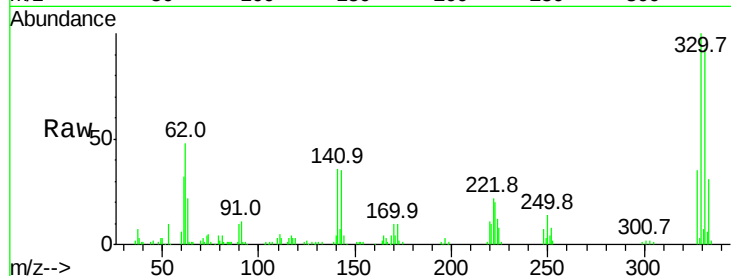


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

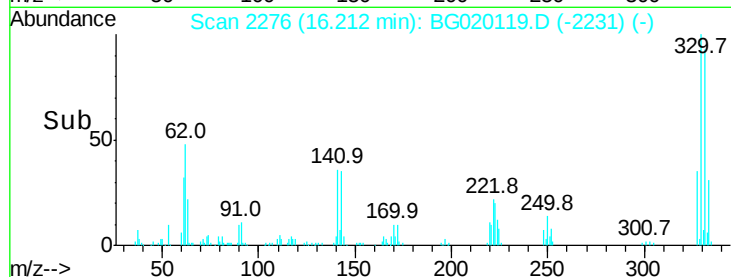
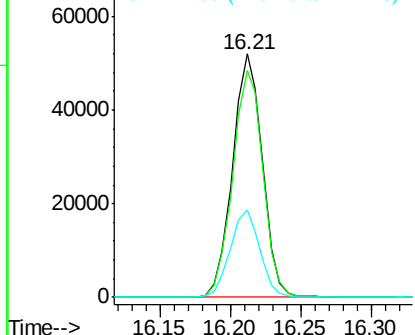



#44  
 2-Fluorobiphenyl  
 Concen: 65.28 ng  
 RT: 13.35 min Scan# 1789  
 Delta R.T. -0.04 min  
 Lab File: BG020119.D  
 Acq: 11 Dec 2015 23:22

Tgt Ion:172 Resp: 323213  
 Ion Ratio Lower Upper  
 172 100  
 171 37.7 29.0 43.6  
 170 24.2 19.9 29.9

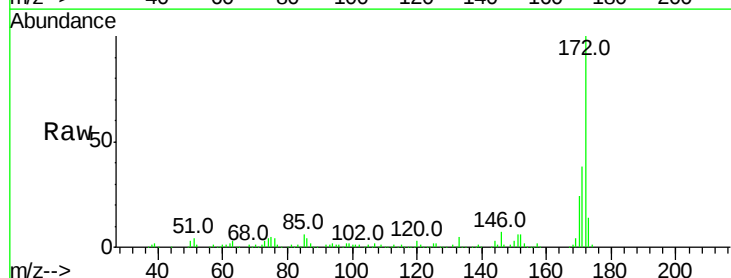

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E



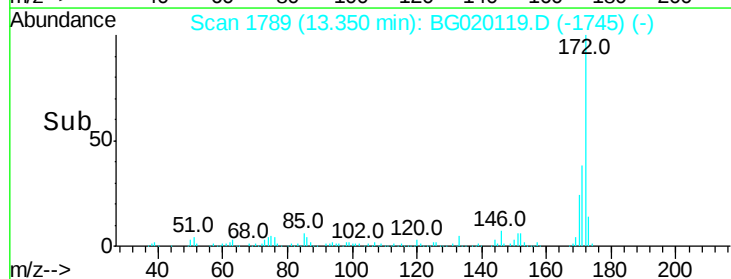
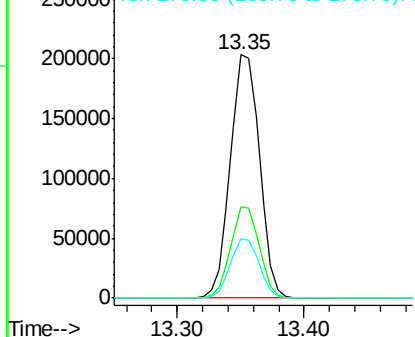


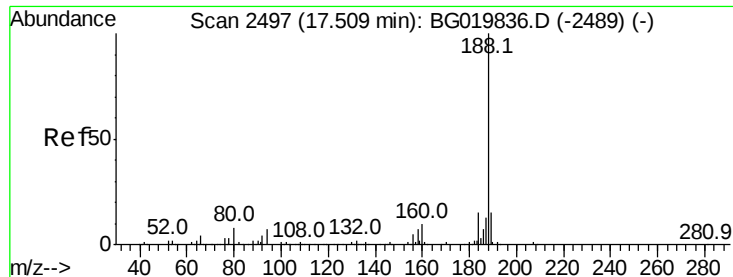

#63  
Phenanthrene-d10  
Concen: 20.00 ng  
RT: 17.47 min Scan# 2490  
Delta R.T. -0.04 min  
Lab File: BG020119.D  
Acq: 11 Dec 2015 23:22




Instrument :  
BNA\_G  
ClientSampleId :  
PB87210BL


Tot Ion:188 Resp: 188104  
Ion Ratio Lower Upper  
188 100  
94 7.4 7.7 11.5#  
80 7.7 7.8 11.8#

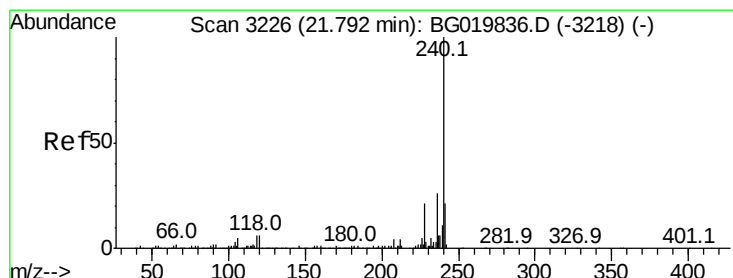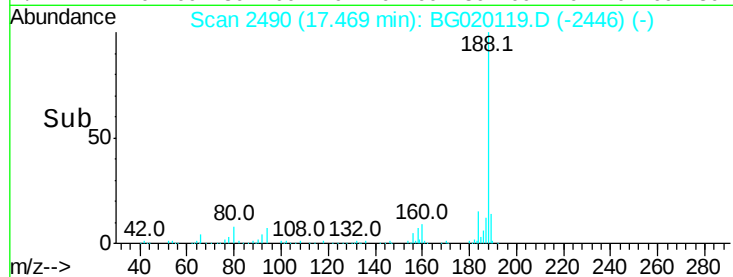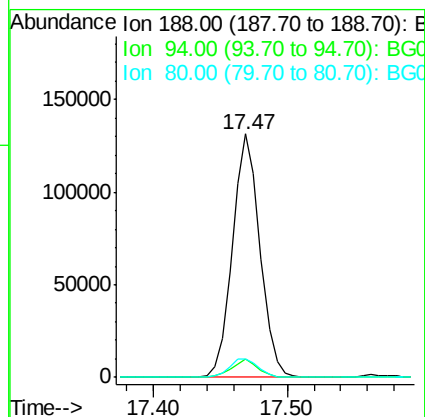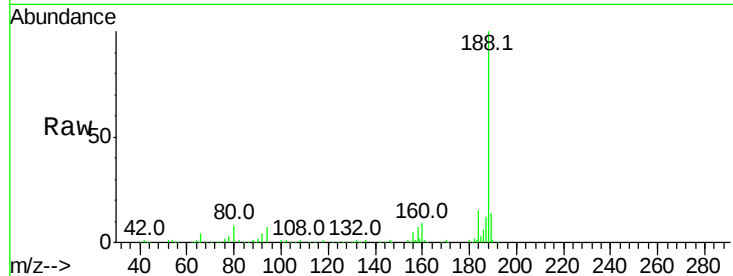

#75  
Chrysene-d12  
Concen: 20.00 ng  
RT: 21.74 min Scan# 3217  
Delta R.T. -0.05 min  
Lab File: BG020119.D  
Acq: 11 Dec 2015 23:22

Tgt Ion:240 Resp: 224468  
Ion Ratio Lower Upper  
240 100  
120 6.6 7.4 11.0#  
236 25.7 20.7 31.1

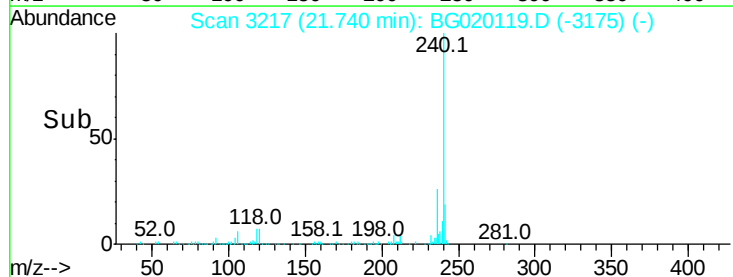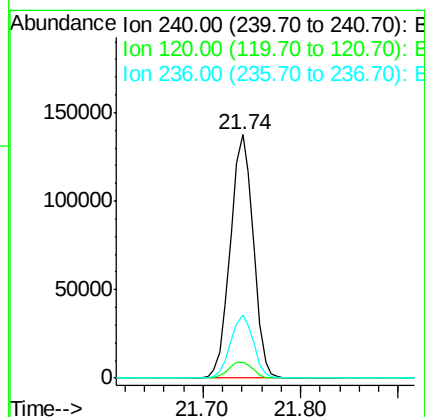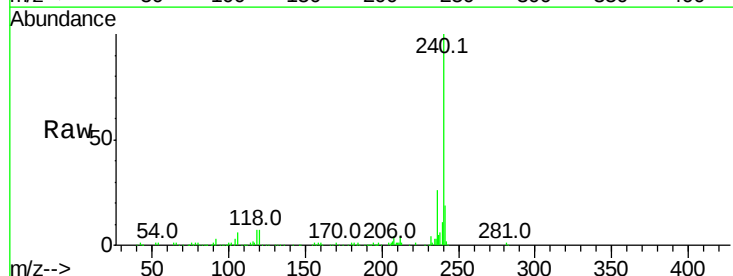

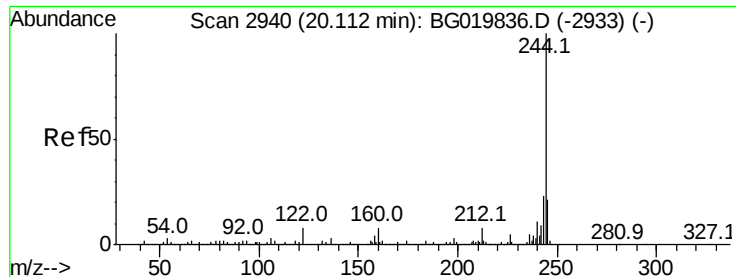

#78

Terphenyl-d14

Concen: 72.26 ng

RT: 20.07 min Scan# 2933

Delta R.T. -0.04 min

Lab File: BG020119.D

Acq: 11 Dec 2015 23:22

Instrument :

BNA\_G

ClientSampleId :

PB87210BL





Tot Ion:244 Resp: 664975

Ion Ratio Lower Upper

244 100

212 8.0 6.9 10.3

122 7.9 10.2 15.2#

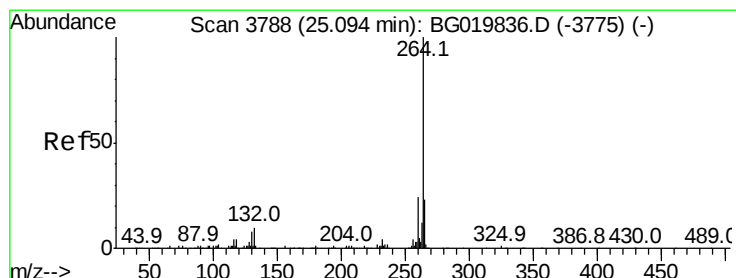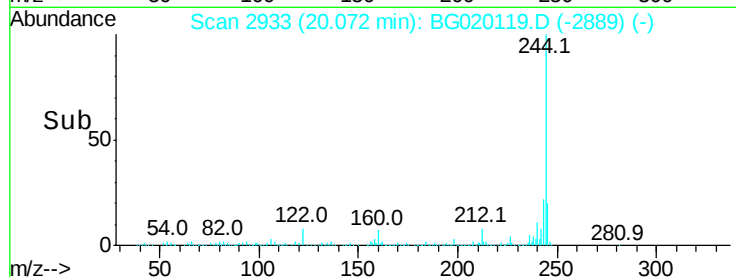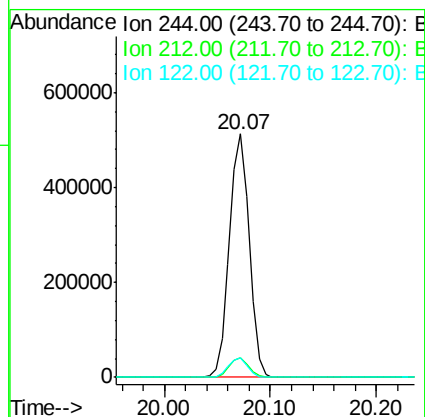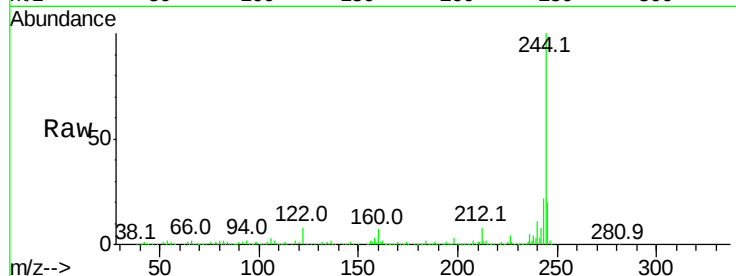

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.01 min Scan# 3773

Delta R.T. -0.09 min

Lab File: BG020119.D

Acq: 11 Dec 2015 23:22

Tgt Ion:264 Resp: 207651

Ion Ratio Lower Upper

264 100

260 22.9 18.5 27.7

265 20.8 17.2 25.8

