

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121215\
 Data File : BG020131.D
 Acq On : 12 Dec 2015 7:11
 Operator : UM/SJ
 Sample : G4755-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 121015-D534-E-U-S

Quant Time: Dec 14 00:59:03 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	21399	20.00	ng	-0.04
21) Naphthalene-d8	10.92	136	91305	20.00	ng	-0.04
38) Acenaphthene-d10	14.73	164	69190	20.00	ng	-0.04
63) Phenanthrene-d10	17.47	188	181361	20.00	ng	-0.04
75) Chrysene-d12	21.74	240	212274	20.00	ng	-0.05
86) Perylene-d12	25.01	264	199111	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	51114	43.17	ng	-0.02
7) Phenol-d6	7.25	99	50026	27.98	ng	-0.02
23) Nitrobenzene-d5	9.27	82	149704	83.68	ng	-0.04
41) 2,4,6-Tribromophenol	16.21	330	86700	81.90	ng	-0.03
44) 2-Fluorobiphenyl	13.35	172	395637	78.08	ng	-0.04
78) Terphenyl-d14	20.07	244	709968	81.58	ng	-0.04


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121215\
Data File : BG020131.D
Acq On : 12 Dec 2015 7:11
Operator : UM/SJ
Sample : G4755-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
121015-D534-E-U-S

Quant Time: Dec 14 00:59:03 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

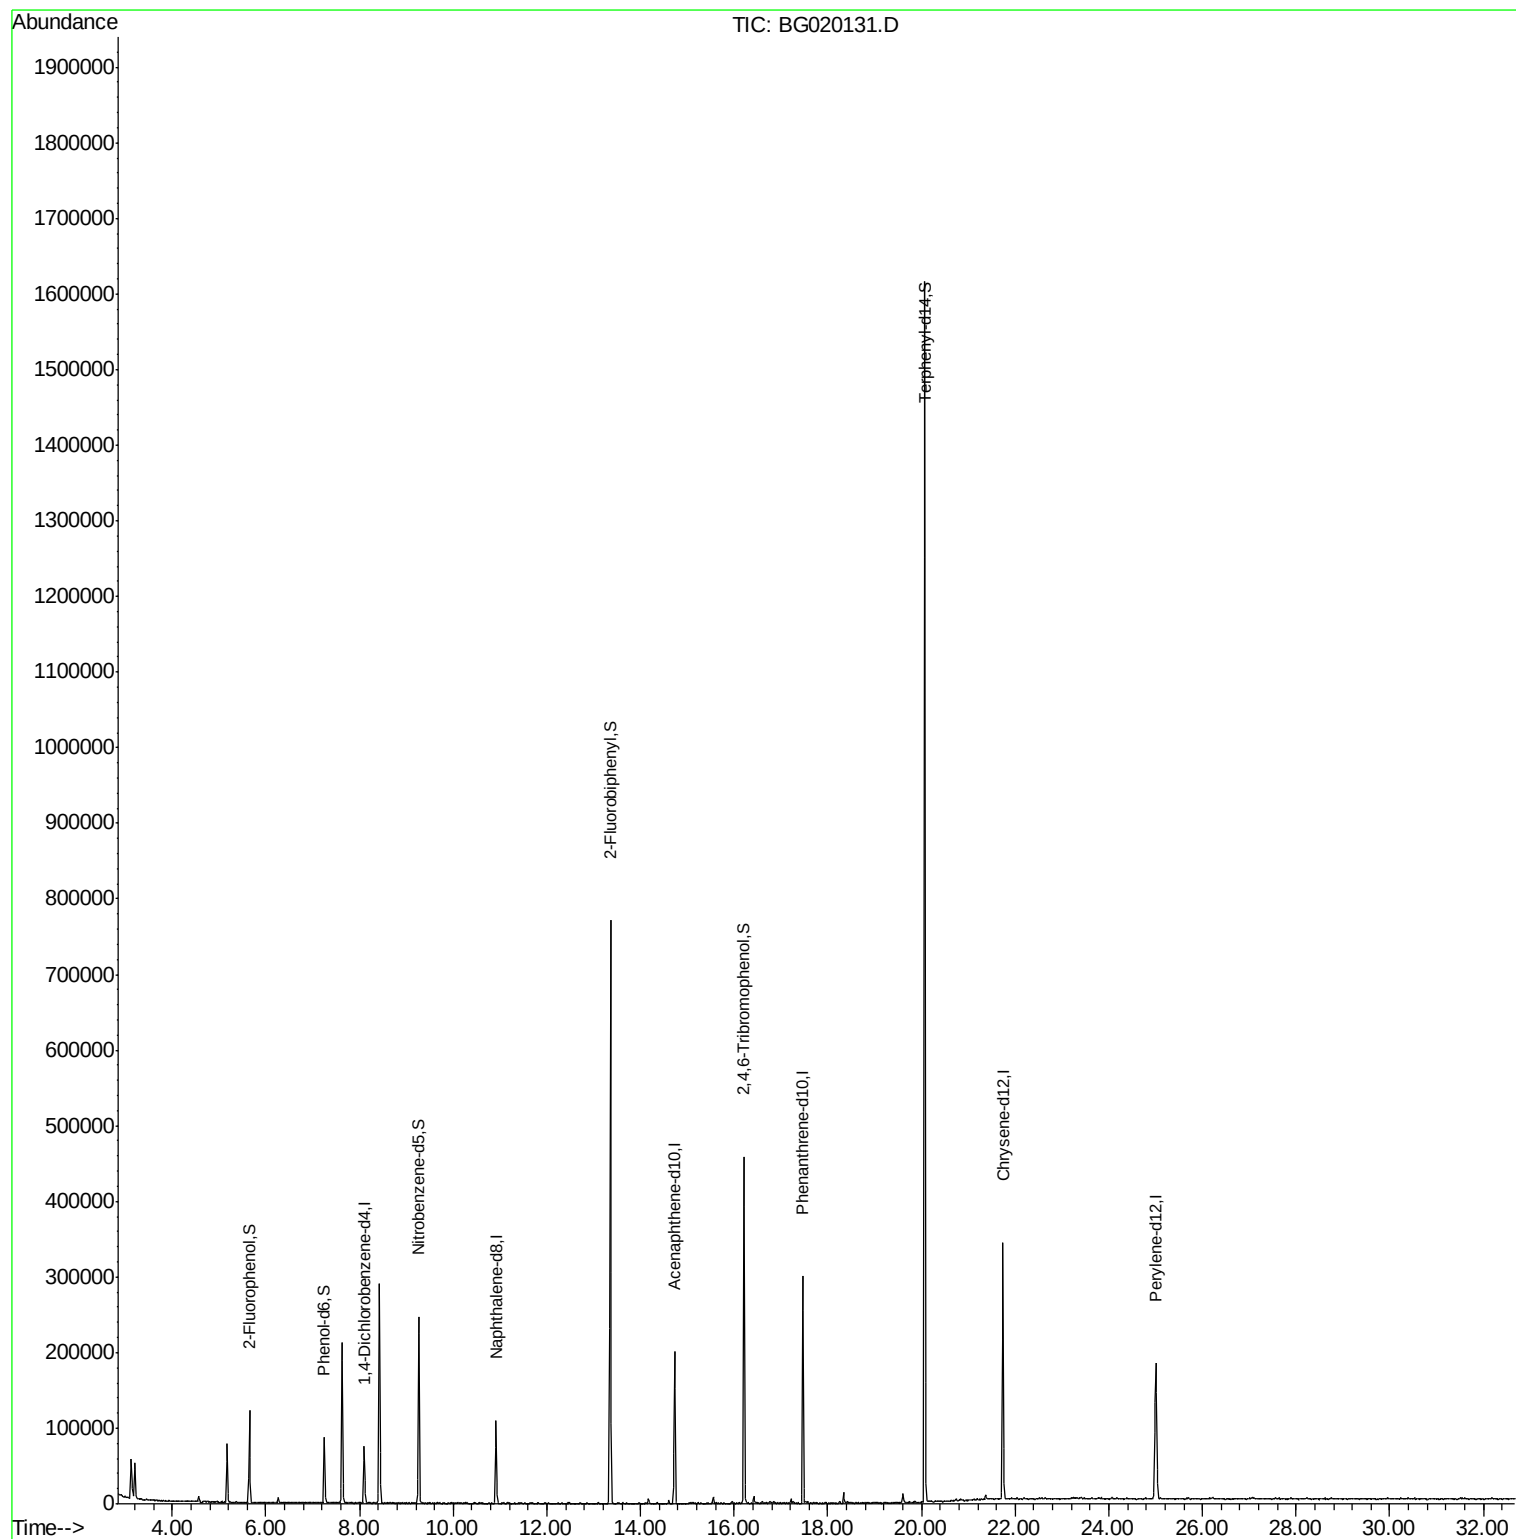

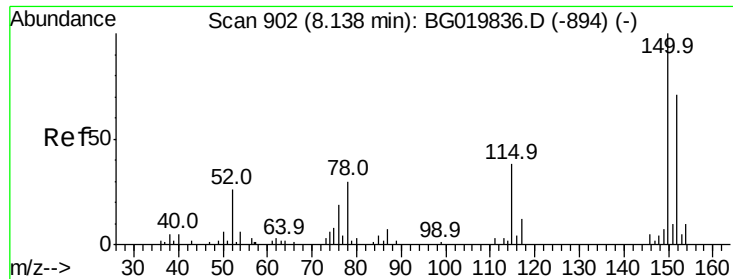

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.10 min Scan# 895

Delta R.T. -0.04 min

Lab File: BG020131.D

Acq: 12 Dec 2015 7:11

Instrument :

BNA_G

ClientSampleId :

121015-D534-E-U-S


Tot Ion:152 Resp: 21399

Ion Ratio Lower Upper

152 100

150 154.7 115.0 172.4




115 59.2 43.9 65.9

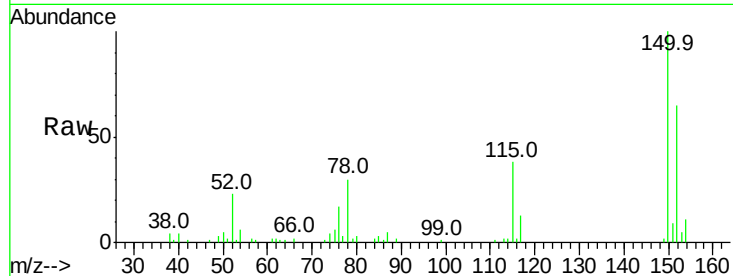

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

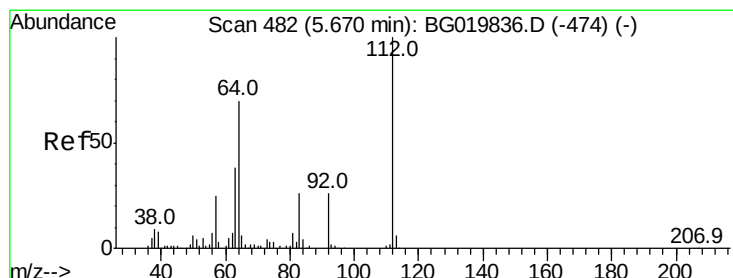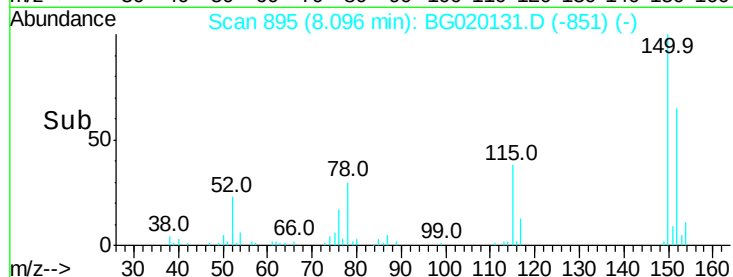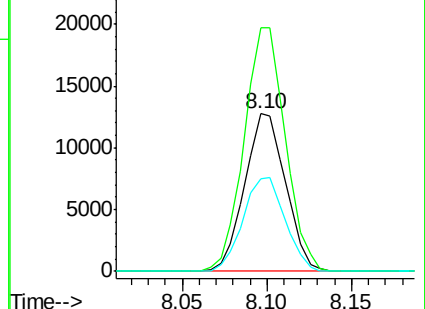

#5

2-Fluorophenol

Concen: 43.17 ng

RT: 5.65 min Scan# 478

Delta R.T. -0.02 min

Lab File: BG020131.D

Acq: 12 Dec 2015 7:11


Tgt Ion:112 Resp: 51114

Ion Ratio Lower Upper

112 100

64 64.9 43.7 65.5



63 36.4 24.0 36.0#

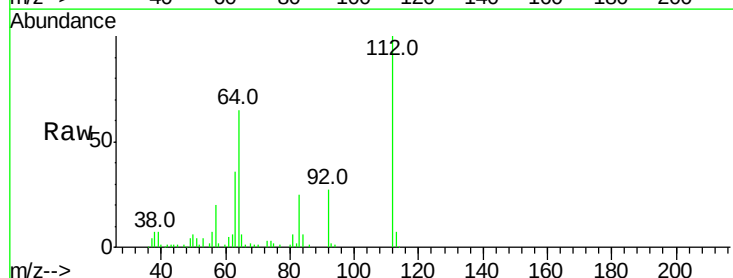


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

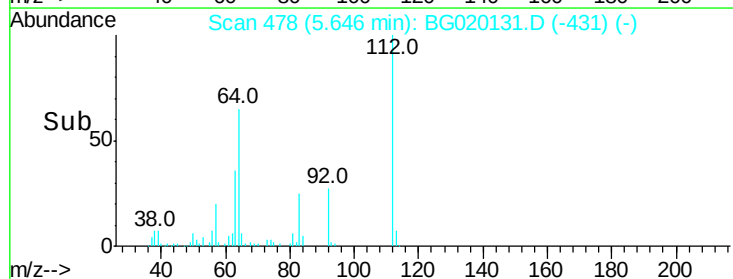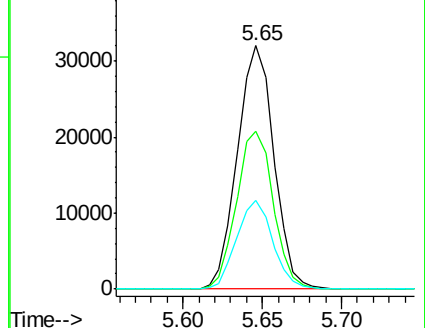

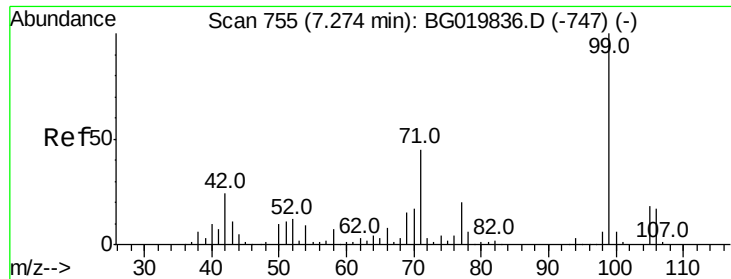

#7

Phenol-d6

Concen: 27.98 ng

RT: 7.25 min Scan# 751

Delta R.T. -0.02 min

Lab File: BG020131.D

Acq: 12 Dec 2015 7:11

Instrument :

BNA_G

ClientSampleId :

121015-D534-E-U-S


Tot Ion: 99 Resp: 50026

Ion Ratio Lower Upper




99 100

42 17.4 11.5 17.3#

71 36.9 22.6 34.0#

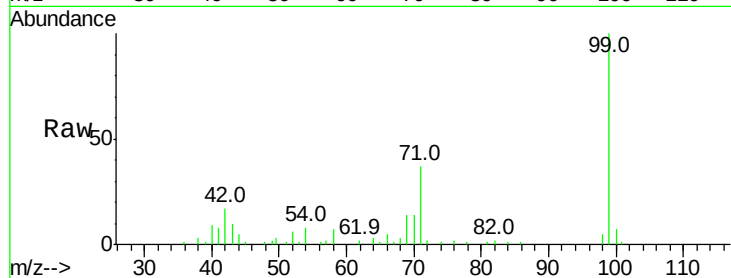

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

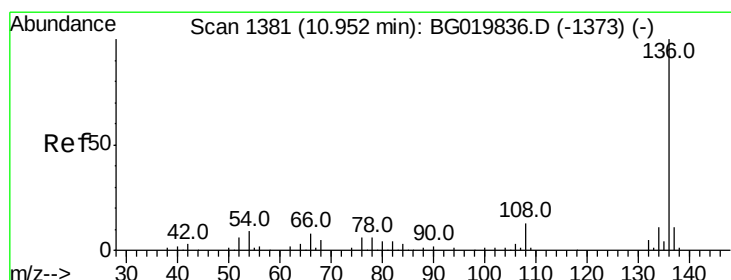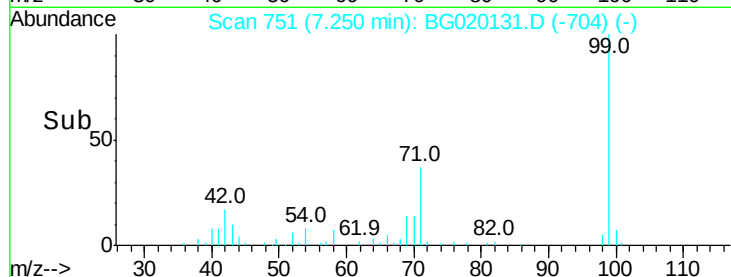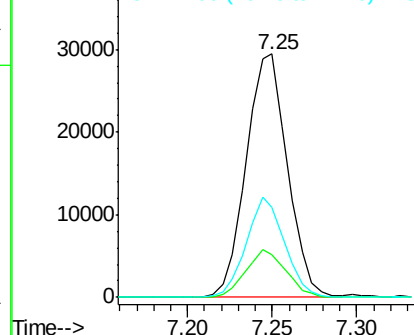

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.92 min Scan# 1375

Delta R.T. -0.04 min

Lab File: BG020131.D

Acq: 12 Dec 2015 7:11

Tgt Ion: 136 Resp: 91305


Ion Ratio Lower Upper

136 100



137 11.9 8.6 12.8


54 7.9 5.4 8.2

68 5.4 5.3 7.9

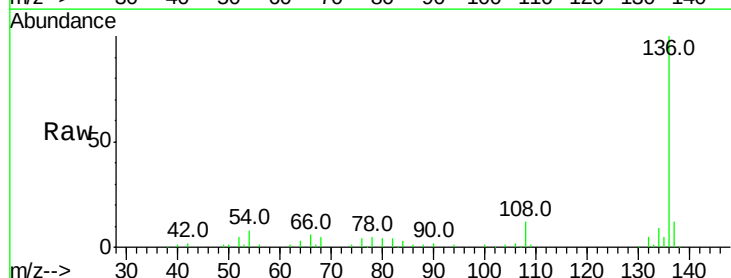

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



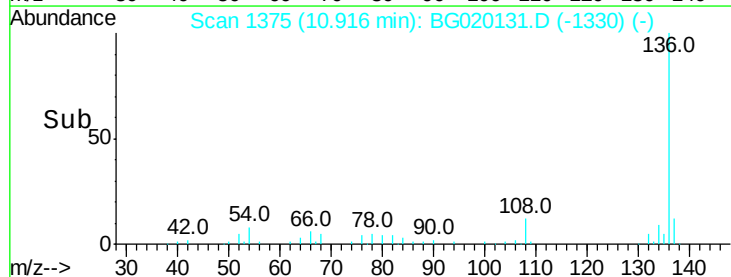
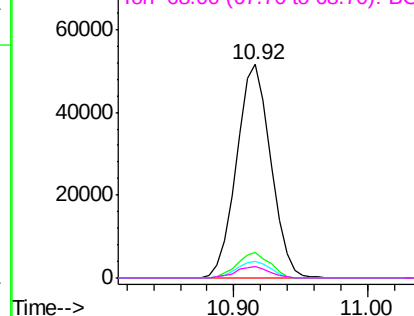


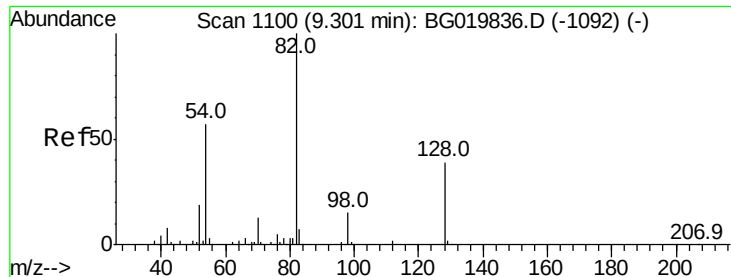

#23
 Nitrobenzene-d5
 Concen: 83.68 ng
 RT: 9.27 min Scan# 1094
 Delta R.T. -0.04 min
 Lab File: BG020131.D
 Acq: 12 Dec 2015 7:11




Instrument :
 BNA_G
 ClientSampleId :
 121015-D534-E-U-S


Tot Ion	Ratio	Lower	Upper
82	100		
128	40.2	36.7	55.1
54	48.3	33.8	50.8

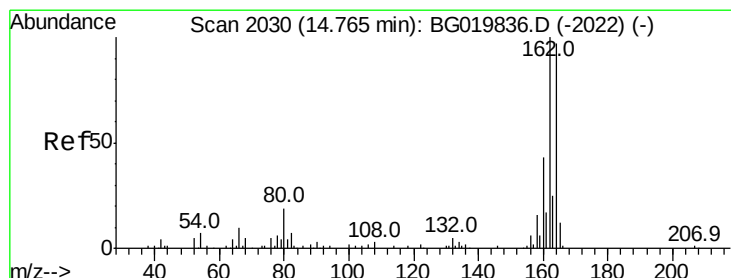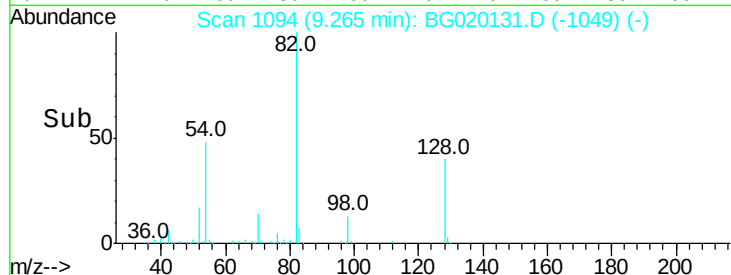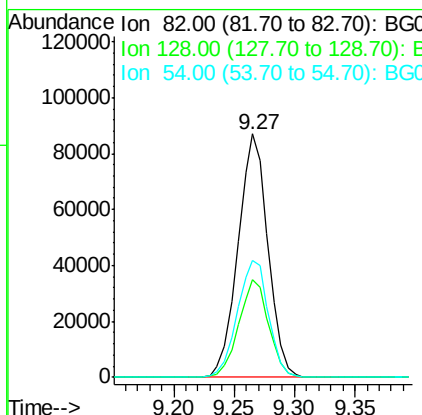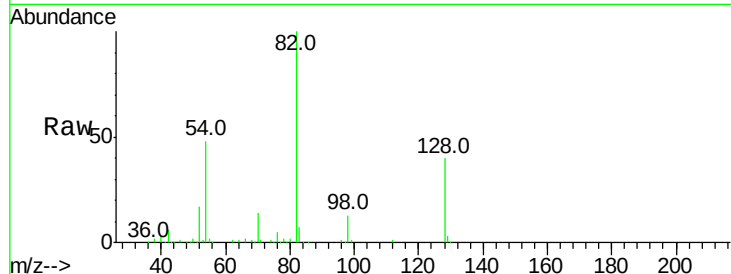

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.73 min Scan# 2024
 Delta R.T. -0.04 min
 Lab File: BG020131.D
 Acq: 12 Dec 2015 7:11

Tgt Ion	Ratio	Lower	Upper
164	100		
162	107.0	78.8	118.2
160	47.4	36.4	54.6

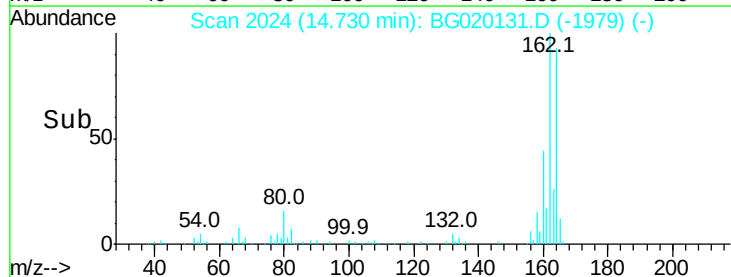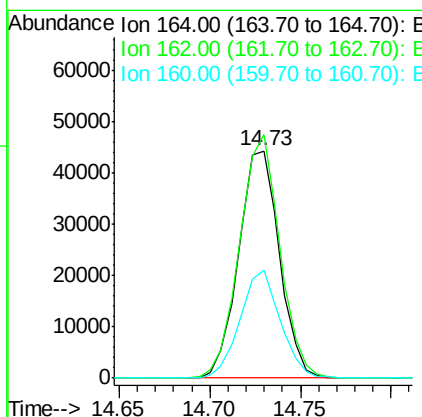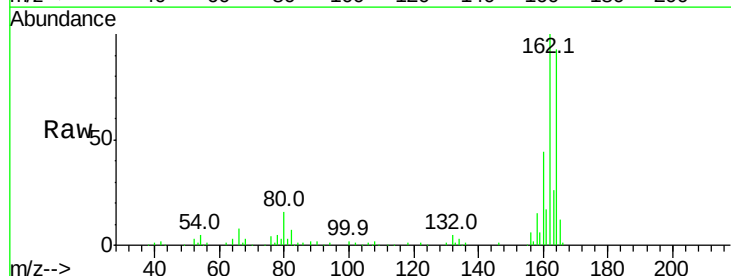


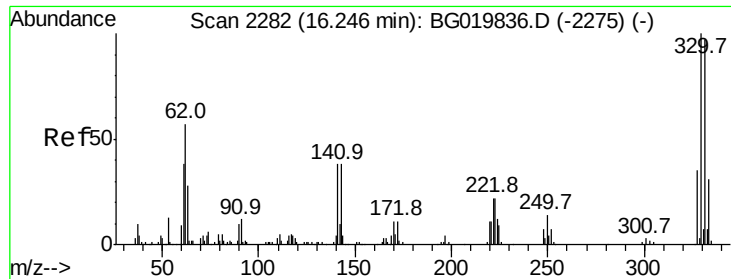




#41
 2,4,6-Tribromophenol
 Concen: 81.90 ng
 RT: 16.21 min Scan# 2276
 Delta R.T. -0.03 min
 Lab File: BG020131.D
 Acq: 12 Dec 2015 7:11

Instrument :
 BNA_G
 ClientSampleId :
 121015-D534-E-U-S

Tot Ion:330 Resp: 86700
 Ion Ratio Lower Upper
 330 100
 332 98.5 78.1 117.1
 141 35.7 28.2 42.2

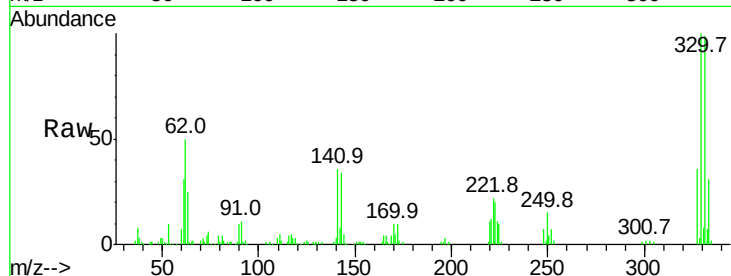


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

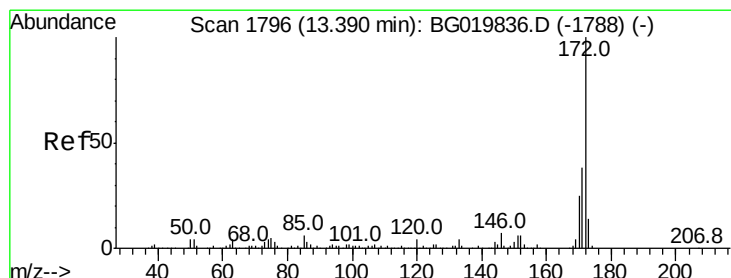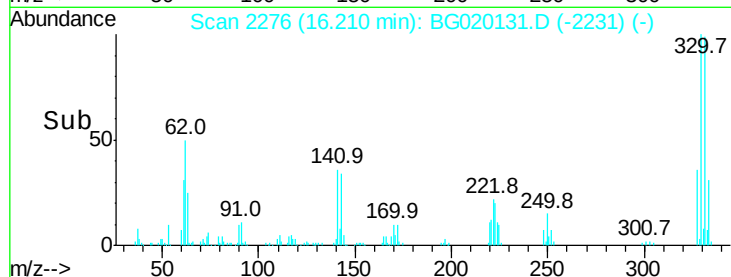
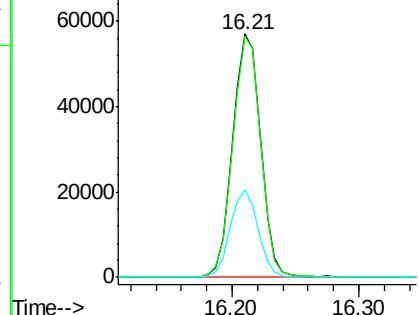



#44
 2-Fluorobiphenyl
 Concen: 78.08 ng
 RT: 13.35 min Scan# 1790
 Delta R.T. -0.04 min
 Lab File: BG020131.D
 Acq: 12 Dec 2015 7:11

Tgt Ion:172 Resp: 395637
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.0 43.6
 170 24.6 19.9 29.9

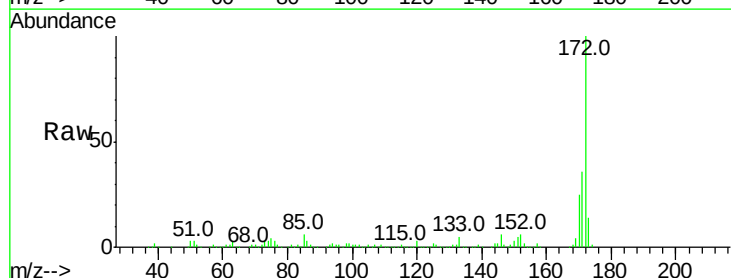

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



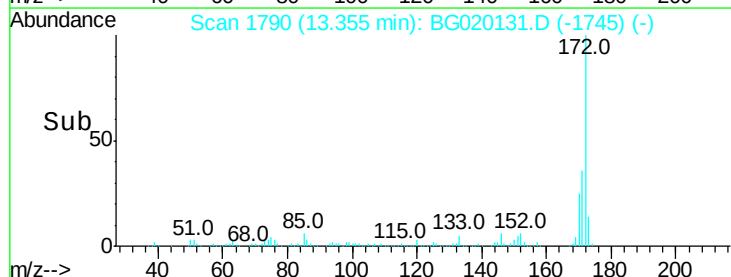
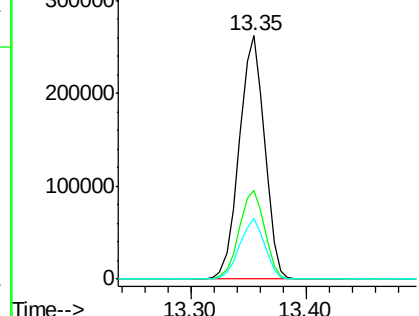


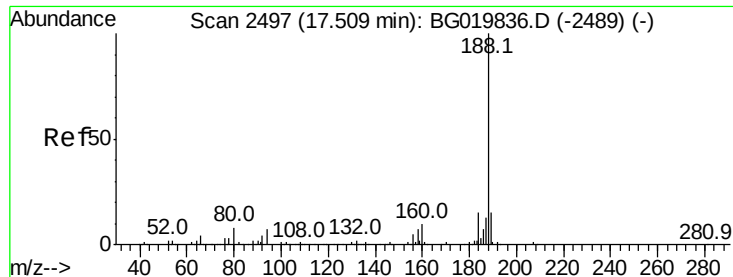

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.47 min Scan# 2490
Delta R.T. -0.04 min
Lab File: BG020131.D
Acq: 12 Dec 2015 7:11




Instrument :
BNA_G
ClientSampleId :
121015-D534-E-U-S


Tot Ion	Ratio	Lower	Upper
188	100		
94	6.7	7.7	11.5#
80	8.4	7.8	11.8

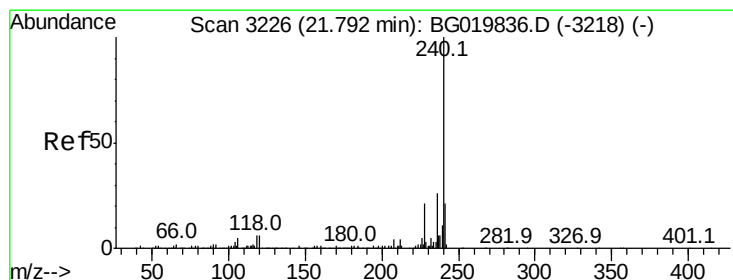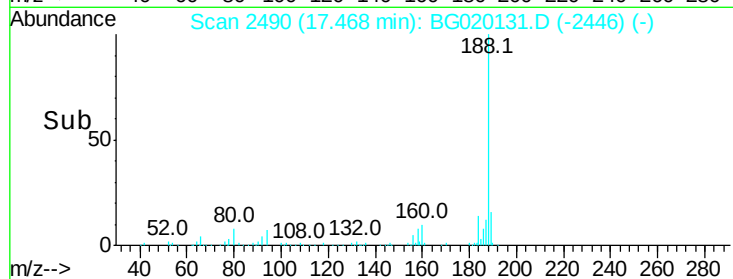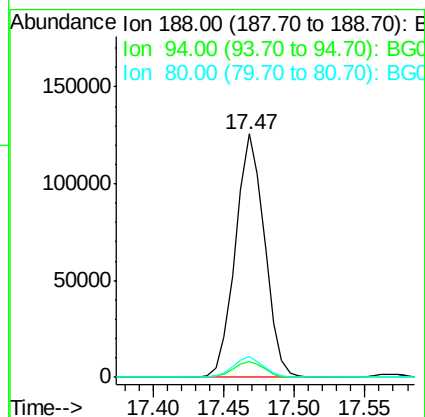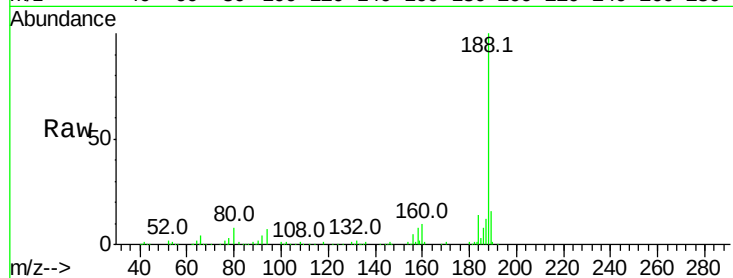

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.74 min Scan# 3217
Delta R.T. -0.05 min
Lab File: BG020131.D
Acq: 12 Dec 2015 7:11

Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.8	7.4	11.0#
236	24.6	20.7	31.1


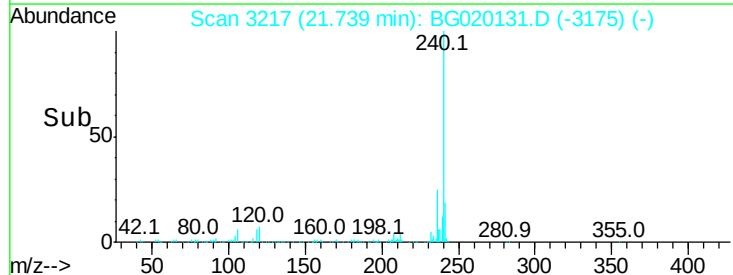
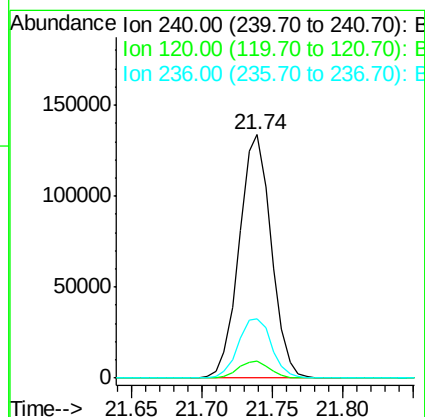
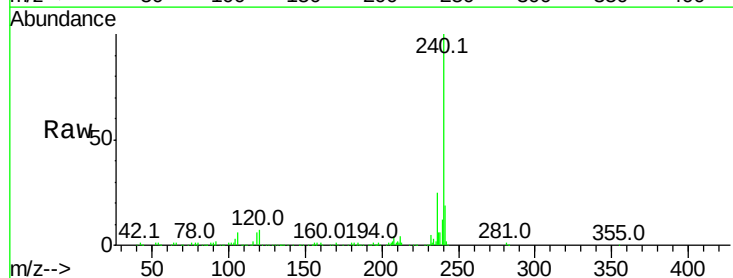


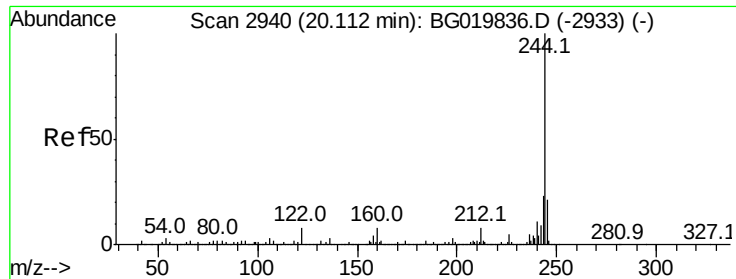

#78
 Terphenyl-d14
 Concen: 81.58 ng
 RT: 20.07 min Scan# 2933
 Delta R.T. -0.04 min
 Lab File: BG020131.D
 Acq: 12 Dec 2015 7:11

Instrument :
 BNA_G
 ClientSampleId :
 121015-D534-E-U-S

Tot Ion	Ratio	Lower	Upper
244	100		
212	8.1	6.9	10.3
122	8.0	10.2	15.2#

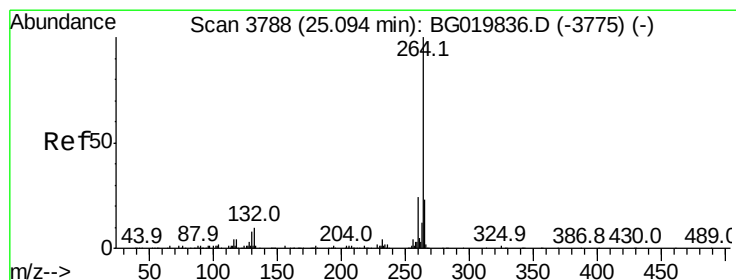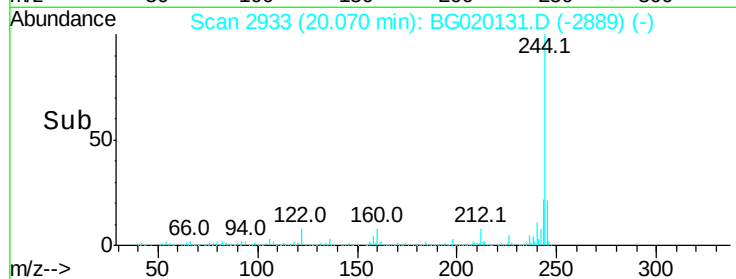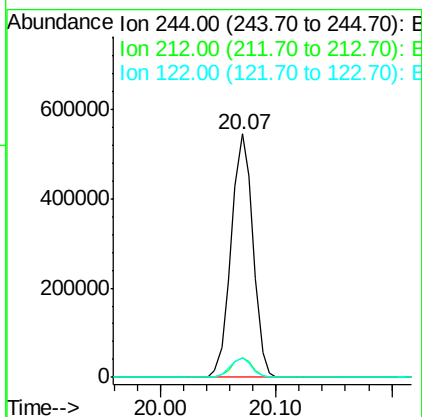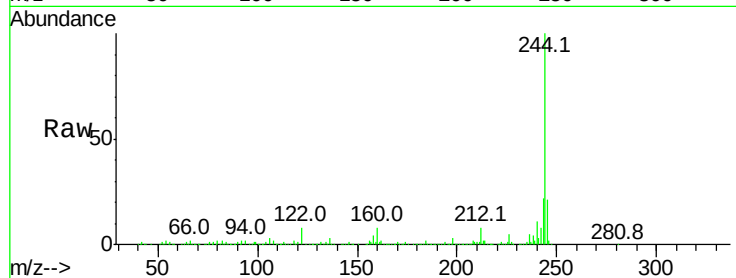

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.01 min Scan# 3773
 Delta R.T. -0.09 min
 Lab File: BG020131.D
 Acq: 12 Dec 2015 7:11

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.8	18.5	27.7
265	22.6	17.2	25.8

