

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121216\
 Data File : BG025117.D
 Acq On : 12 Dec 2016 16:46
 Operator : UM/SJ
 Sample : H5860-20 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DA8E6

Manual Integrations
 APPROVED

sohil
 12/13/2016 6:06:38 PM

Quant Time: Dec 13 00:58:13 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 13 00:29:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	90352	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	375985	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.86	164	311564	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.60	188	638232	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	735855	20.00	ng/ul	0.00
83) Perylene-d12	25.32	264	762403	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.60	96	1255	0.72	ng/uL	0.00
5) Phenol-d5	7.38	99	23807	3.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	16299	3.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	19263	3.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.94	113	22742	3.49	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	8578	3.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	10349	3.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.69	165	21506	3.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	11159	1.78	ng/ul	0.01
43) Dimethylphthalate-d6	14.26	166	76649	3.58	ng/ul	0.00
46) Acenaphthylene-d8	14.56	160	87162	3.71	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	3379	0.92	ng/ul	0.01
57) Fluorene-d10	15.85	176	76406	3.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.97	200	7895	2.00	ng/ul	0.00
70) Anthracene-d10	17.70	188	117157	4.35	ng/ul	0.00
76) Pyrene-d10	19.97	212	137526	4.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.08	264	132178	4.28	ng/ul	0.00

Target Compounds

						Ovalue
69) Phenanthrene	17.65	178	110030	3.61	ng/ul	94
74) Fluoranthene	19.64	202	275825	7.62	ng/ul	97
77) Pyrene	20.00	202	210849	5.96	ng/ul#	96
80) Benzo(a)anthracene	21.88	228	105830m	2.77	ng/ul	
82) Chrysene	21.95	228	113126	3.16	ng/ul	99
85) Benzo(b)fluoranthene	24.22	252	158413m	4.19	ng/ul	
86) Benzo(k)fluoranthene	24.27	252	51783m	1.44	ng/ul	
88) Benzo(a)pyrene	25.16	252	83549	2.30	ng/ul#	96
89) Indeno(1,2,3-cd)pyrene	29.24	276	76990m	1.70	ng/ul	
91) Benzo(g,h,i)perylene	30.50	276	56468m	1.50	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121216\
Data File : BG025117.D
Acq On : 12 Dec 2016 16:46
Operator : UM/SJ
Sample : H5860-20 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampled :
DA8E6

Manual Integrations
APPROVED

sohil
12/13/2016 6:06:38 PM

Quant Time: Dec 13 00:58:13 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 13 00:29:17 2016
Response via : Initial Calibration

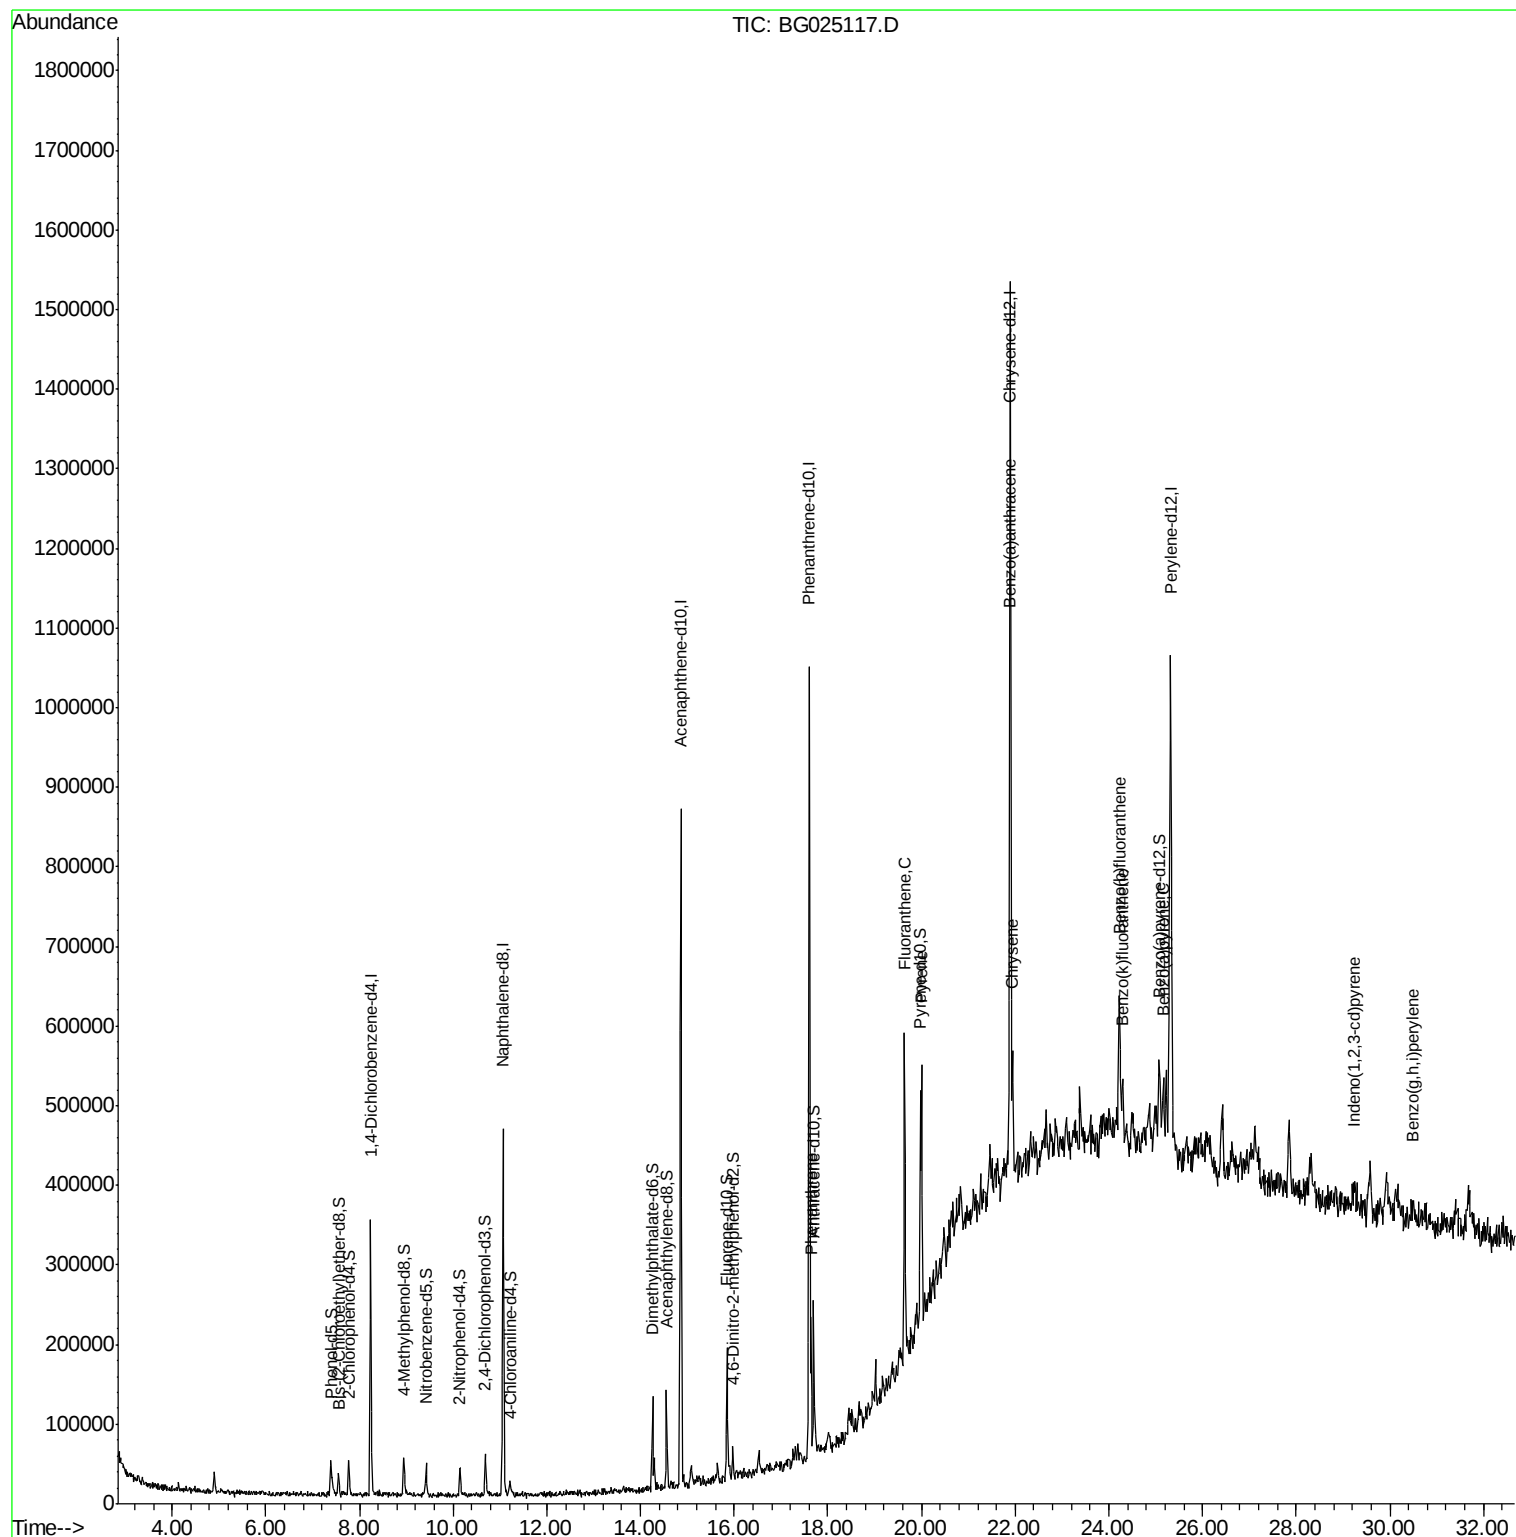

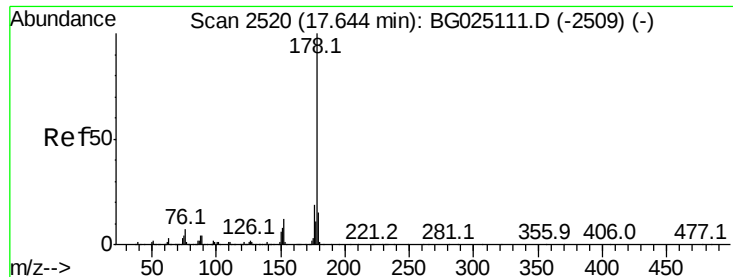

#69

Phenanthrene

Concen: 3.61 ng/ul

RT: 17.65 min Scan# 2520

Delta R.T. 0.00 min

Lab File: BG025117.D

Acq: 12 Dec 2016 16:46

Instrument :

BNA_G





ClientSampleId :

DA8E6

Tot Ion:	178	Resp:	110030
Ion Ratio	Lower	Upper	
178	100		
179	18.3	12.4	18.6
176	17.9	16.5	24.7

Manual Integrations
APPROVED

sohil
12/13/2016 6:06:38 PM

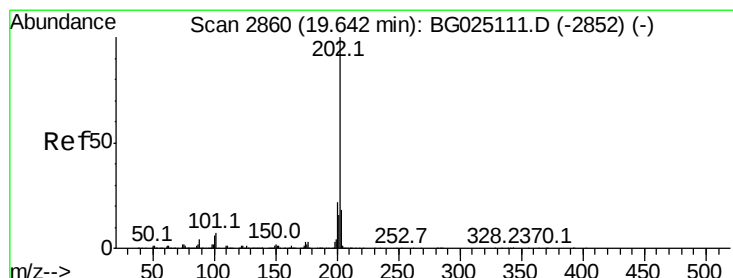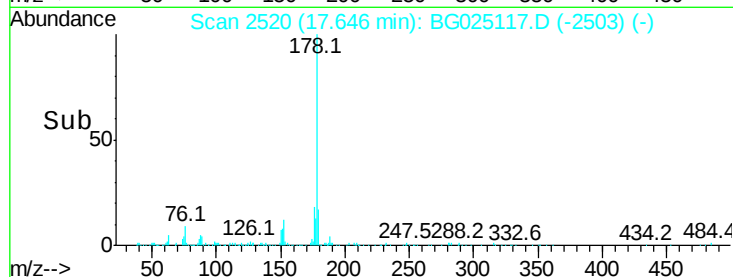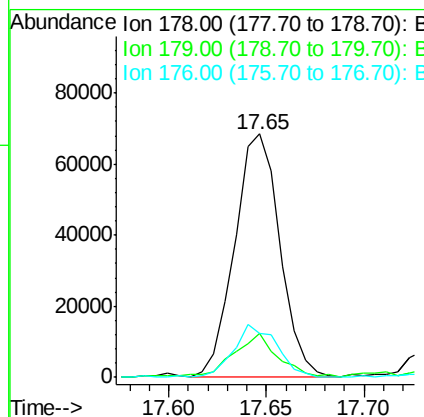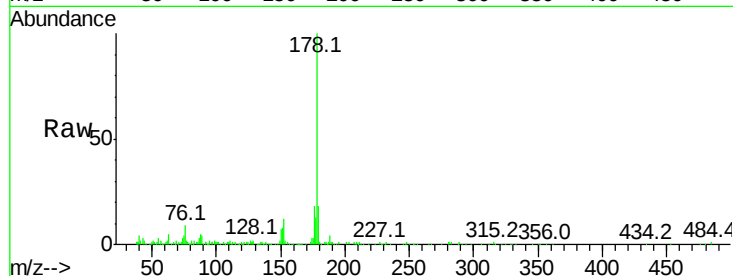

#74

Fluoranthene

Concen: 7.62 ng/ul




RT: 19.64 min Scan# 2859


Delta R.T. -0.00 min

Lab File: BG025117.D

Acq: 12 Dec 2016 16:46

Tgt Ion:	202	Resp:	275825
Ion Ratio	Lower	Upper	
202	100		
101	6.4	6.2	9.2
100	5.8	5.2	7.8

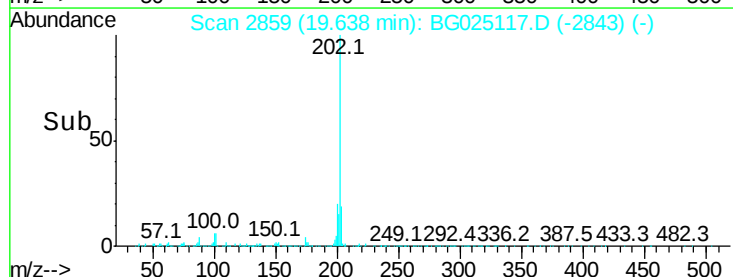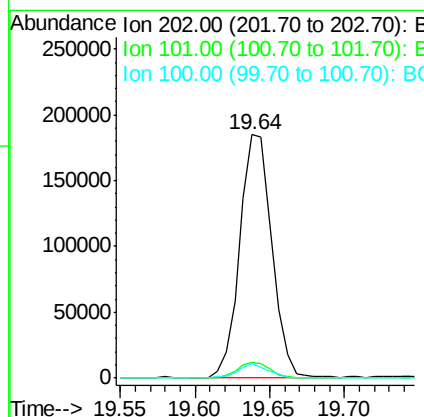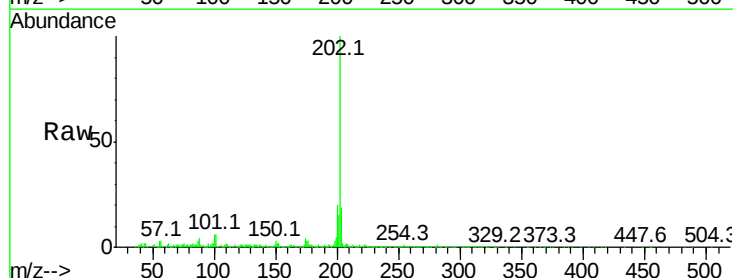

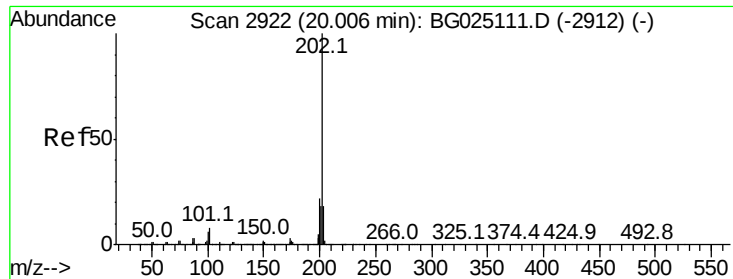

#77

Pvrene

Concen: 5.96 ng/ul

RT: 20.00 min Scan# 2921

Delta R.T. -0.00 min

Lab File: BG025117.D

Acq: 12 Dec 2016 16:46

Instrument :

BNA_G





ClientSampleId :

DA8E6

Tot Ion:	202	Resp:	210849
Ion Ratio	Lower	Upper	
202	100		
101	7.6	6.9	10.3
100	6.6	6.6	10.0#

Manual Integrations
APPROVED

sohil
12/13/2016 6:06:38 PM

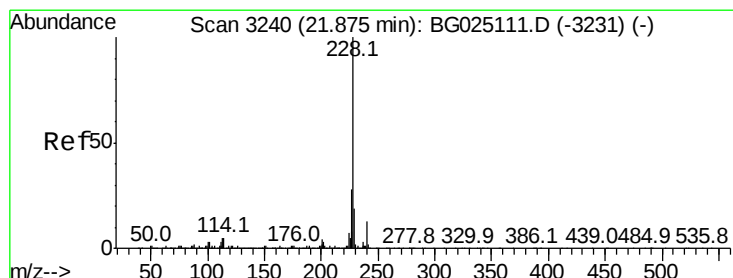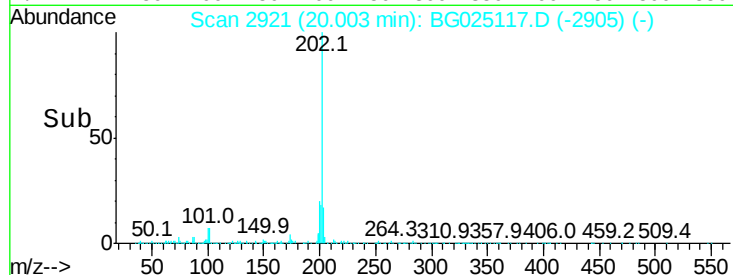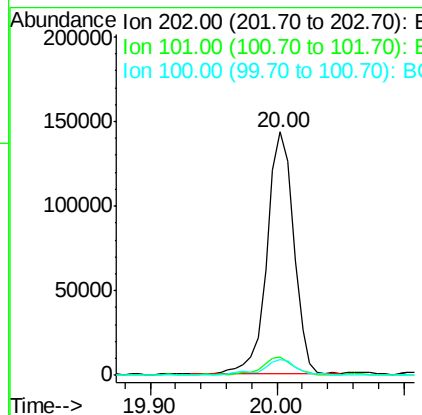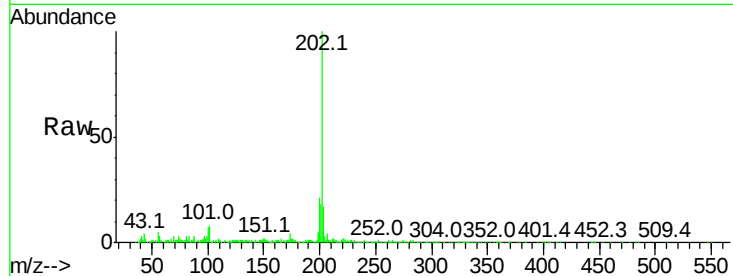

#80

Benzo(a)anthracene

Concen: 2.77 ng/ul m




RT: 21.88 min Scan# 3240


Delta R.T. 0.00 min

Lab File: BG025117.D

Acq: 12 Dec 2016 16:46

Tgt Ion:	228	Resp:	105830
Ion Ratio	Lower	Upper	
228	100		
229	19.0	16.3	24.5
226	26.4	21.9	32.9

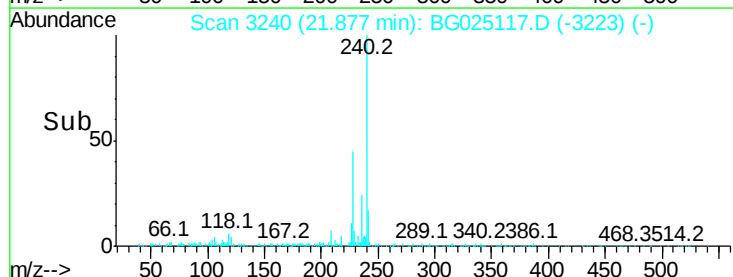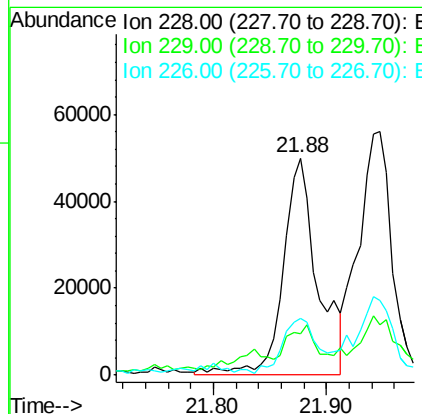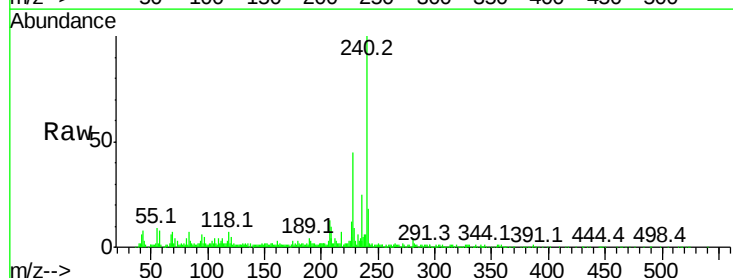

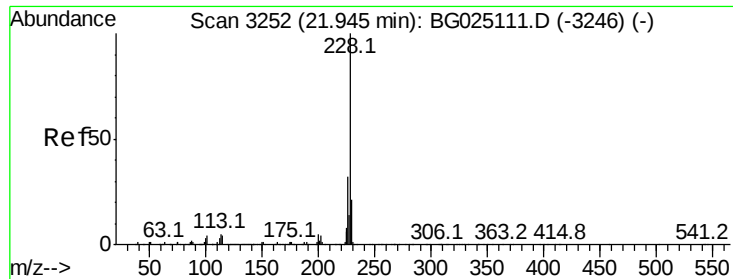





#82
Chrysene
Concen: 3.16 ng/ul
RT: 21.95 min Scan# 3252
Delta R.T. 0.00 min
Lab File: BG025117.D
Acq: 12 Dec 2016 16:46

Instrument :
BNA_G
ClientSampled :
DA8E6

Tot Ion:	228	Resp:	113126
Ion Ratio		Lower	Upper
228	100		
226	30.6	24.0	36.0
229	20.6	16.9	25.3




Manual Integrations
APPROVED


sohil
12/13/2016 6:06:38 PM

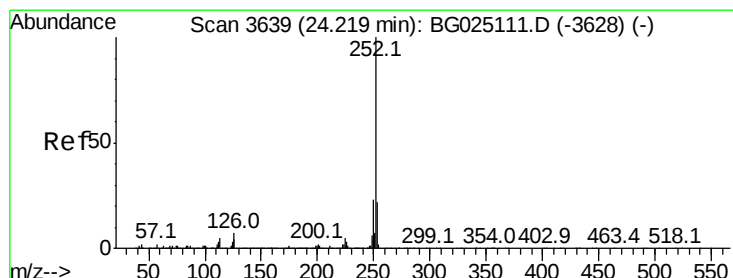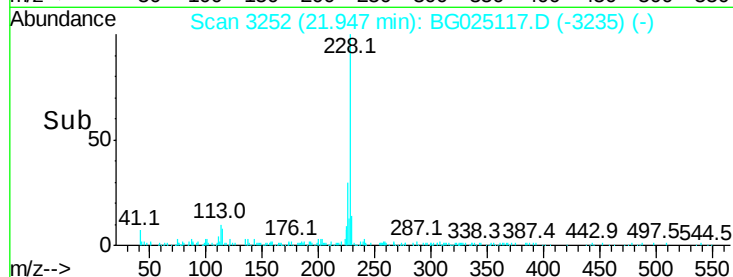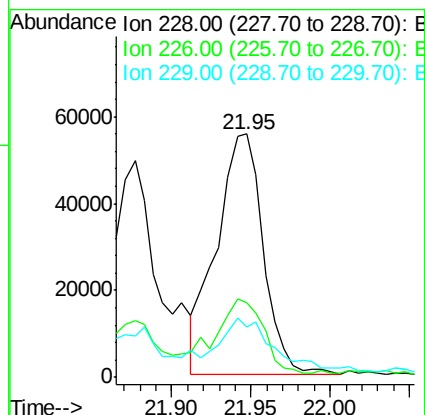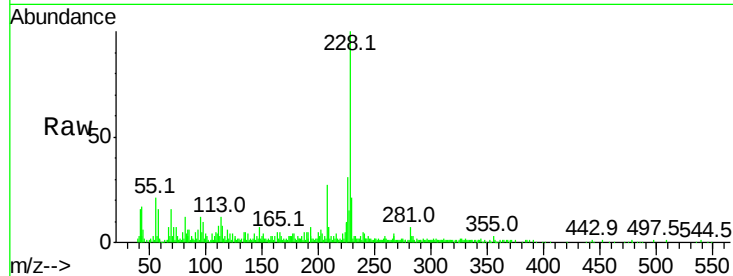

#85
Benzo(b)fluoranthene
Concen: 4.19 ng/ul m
RT: 24.22 min Scan# 3639
Delta R.T. 0.00 min
Lab File: BG025117.D
Acq: 12 Dec 2016 16:46

Tgt Ion:	252	Resp:	158413
Ion Ratio		Lower	Upper
252	100		
253	27.5	17.7	26.5#
125	6.3	4.0	6.0#

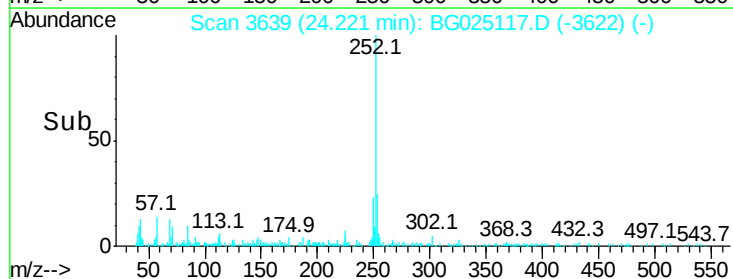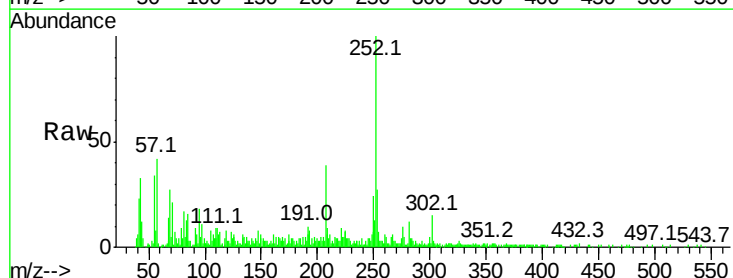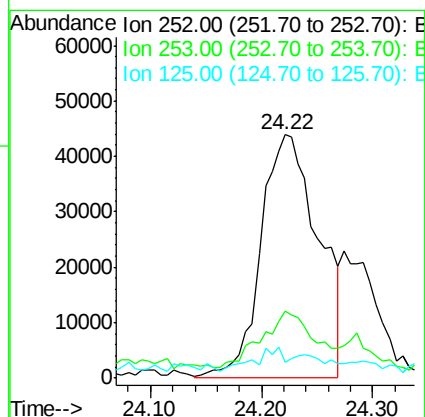

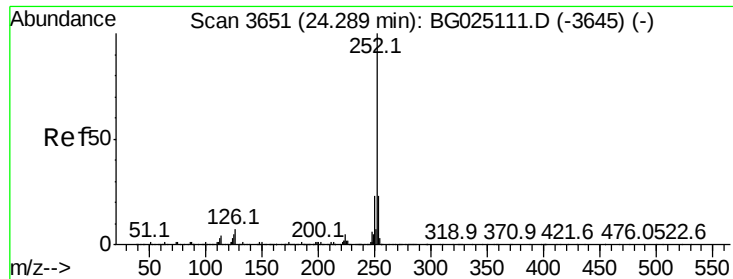

#86

Benzo(k)fluoranthene

Concen: 1.44 ng/ul m

RT: 24.27 min Scan# 3648

Delta R.T. -0.02 min

Lab File: BG025117.D

Acq: 12 Dec 2016 16:46

Instrument :

BNA_G





ClientSampleId :

DA8E6

Tot Ion:	252	Resp:	51783
Ion Ratio	Lower	Upper	
252	100		
253	25.4	18.5	27.7
125	10.9	4.1	6.1#

Manual Integrations
APPROVED

sohil
12/13/2016 6:06:38 PM

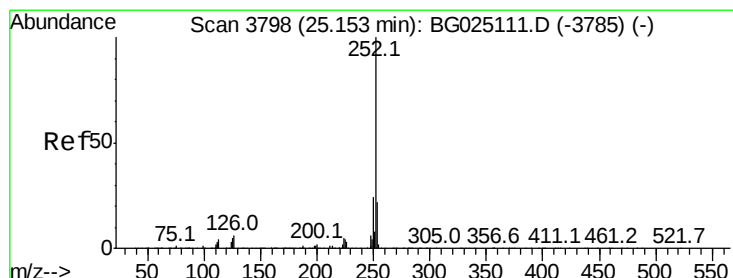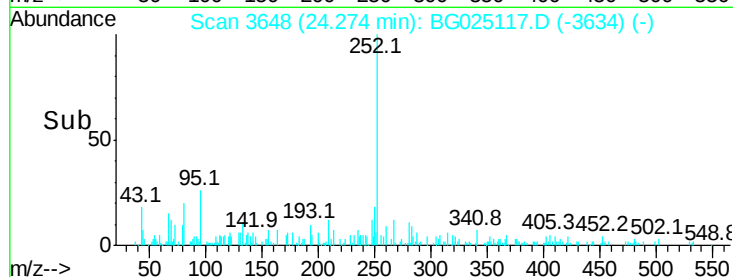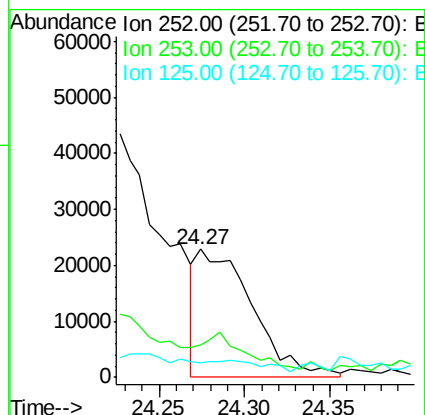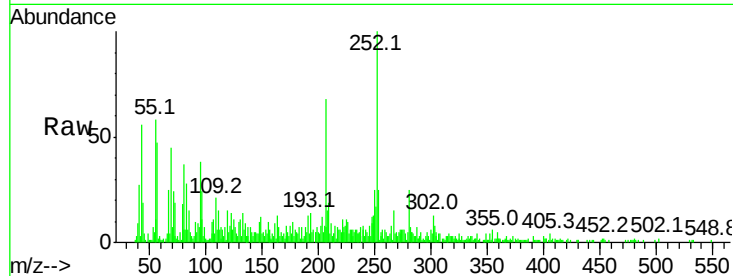

#88

Benzo(a)pyrene

Concen: 2.30 ng/ul




RT: 25.16 min Scan# 3798


Delta R.T. 0.00 min

Lab File: BG025117.D

Acq: 12 Dec 2016 16:46

Tgt Ion:	252	Resp:	83549
Ion Ratio	Lower	Upper	
252	100		
253	23.8	17.8	26.6
125	8.8	5.4	8.0#

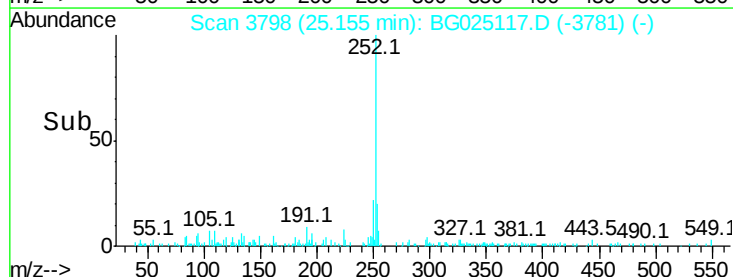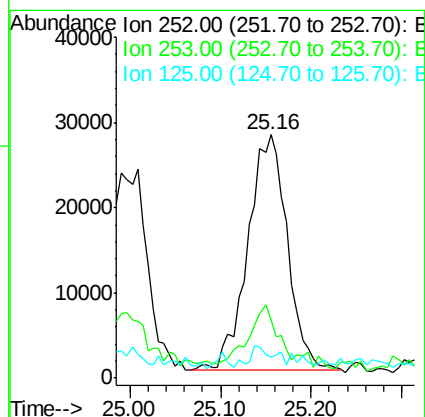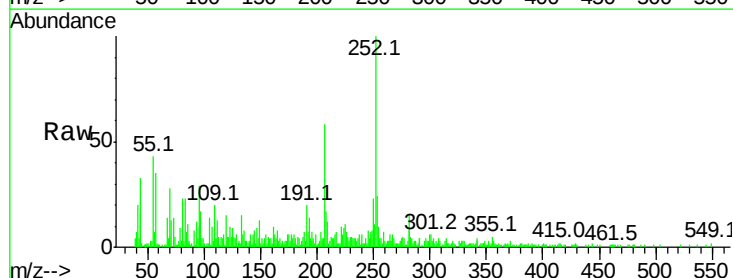

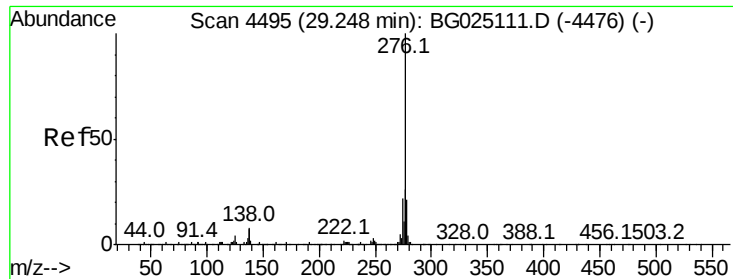

#89





Indeno(1,2,3-cd)pyrene
Concen: 1.70 ng/ul m
RT: 29.24 min Scan# 4494
Delta R.T. -0.00 min
Lab File: BG025117.D
Acq: 12 Dec 2016 16:46

Instrument :
BNA_G
ClientSampleId :
DA8E6

Tot Ion	Ratio	Resp Lower	Upper
276	100		
138	14.2	8.2	12.4#
277	16.4	18.6	28.0#

Manual Integrations
APPROVED

sohil
12/13/2016 6:06:38 PM

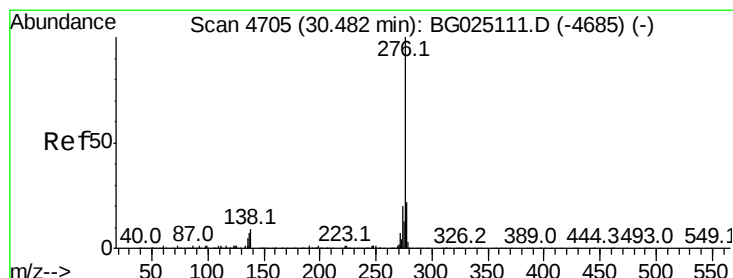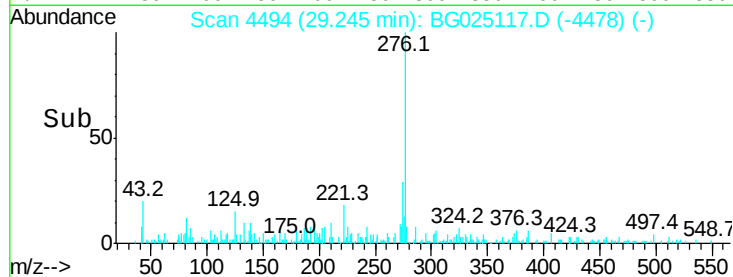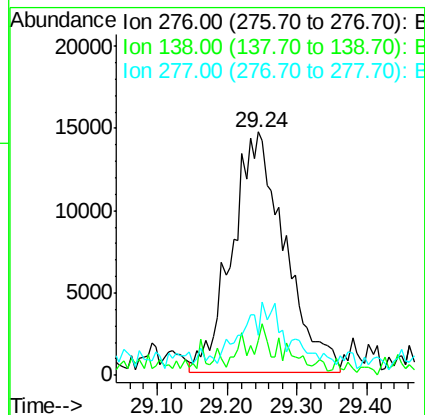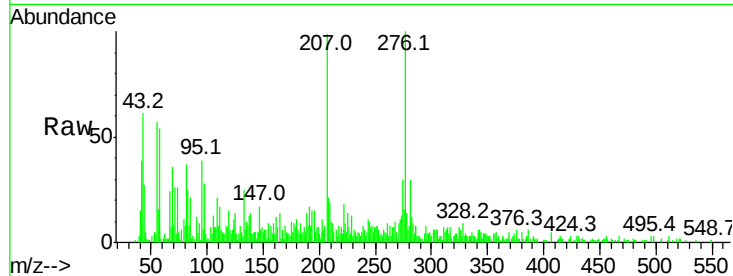

#91

Benzo(g,h,i)perylene
Concen: 1.50 ng/ul m
RT: 30.50 min Scan# 4707
Delta R.T. 0.01 min
Lab File: BG025117.D
Acq: 12 Dec 2016 16:46

Tgt Ion	Ratio	Resp Lower	Upper
276	100		
138	7.5	8.6	12.8#
277	17.1	17.6	26.4#

