

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121216\
 Data File : BG025138.D
 Acq On : 13 Dec 2016 6:36
 Operator : UM/SJ
 Sample : H5990-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P006-SS017-0612-03

Manual Integrations
 APPROVED

sohil
 12/13/2016 6:07:56 PM

Quant Time: Dec 13 07:15:52 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 13 06:23:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	136518	20.00	ng/ul	0.00
18) Naphthalene-d8	11.08	136	589901	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.87	164	423586	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.61	188	747409	20.00	ng/ul	0.00
75) Chrysene-d12	21.92	240	949679	20.00	ng/ul	0.02
83) Perylene-d12	25.35	264	926585	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.60	96	11363	4.30	ng/uL	0.00
5) Phenol-d5	7.40	99	280167	23.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.56	67	191301	26.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.78	132	199027	24.17	ng/ul	0.02
13) 4-Methylphenol-d8	8.95	113	233867	23.76	ng/ul	0.02
19) Nitrobenzene-d5	9.42	128	109210	26.14	ng/ul	0.00
22) 2-Nitrophenol-d4	10.15	143	134673	25.86	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	10.69	165	244491	24.41	ng/ul	0.00
29) 4-Chloroaniline-d4	11.21	131	162555	16.52	ng/ul	0.00
43) Dimethylphthalate-d6	14.26	166	784202	26.91	ng/ul	0.00
46) Acenaphthylene-d8	14.57	160	851217	26.67	ng/ul	0.02
51) 4-Nitrophenol-d4	15.08	143	110477	22.06	ng/ul	0.03
57) Fluorene-d10	15.86	176	658890	24.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	118198	25.58	ng/ul	0.02
70) Anthracene-d10	17.71	188	871290	27.62	ng/ul	0.02
76) Pyrene-d10	19.99	212	1018470	26.04	ng/ul	0.02
87) Benzo(a)pyrene-d12	25.12	264	1008912	26.87	ng/ul	0.04

Target Compounds

						Ovalue
6) Phenol	7.43	94	46279	3.83	ng/ul	98
44) Dimethylphthalate	14.31	163	105420	3.68	ng/ul#	95
49) Acenaphthene	14.93	153	62541	2.94	ng/ul	94
53) Dibenzofuran	15.26	168	38050	1.13	ng/ul	89
58) Fluorene	15.91	166	63118	2.31	ng/ul	98
69) Phenanthrene	17.66	178	1144624	32.09	ng/ul	98
71) Anthracene	17.75	178	309844	8.45	ng/ul	97
72) Carbazole	18.01	167	33413	1.09	ng/ul#	89
74) Fluoranthene	19.65	202	1977883	46.66	ng/ul	99
77) Pyrene	20.02	202	1590782	34.85	ng/ul	98
80) Benzo(a)anthracene	21.89	228	1124953	22.80	ng/ul	97
81) Bis(2-ethylhexyl)phthalate	21.74	149	29644	1.20	ng/ul#	64
82) Chrysene	21.96	228	948621	20.55	ng/ul	95
85) Benzo(b)fluoranthene	24.25	252	1138065	24.77	ng/ul#	91
86) Benzo(k)fluoranthene	24.31	252	398044m	9.11	ng/ul	
88) Benzo(a)pyrene	25.19	252	681394	15.42	ng/ul	98
89) Indeno(1,2,3-cd)pyrene	29.30	276	419924m	7.65	ng/ul	
90) Dibenzo(a,h)anthracene	29.35	278	57548	1.24	ng/ul#	85
91) Benzo(g,h,i)perylene	30.55	276	291005m	6.35	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121216\
Data File : BG025138.D
Acq On : 13 Dec 2016 6:36
Operator : UM/SJ
Sample : H5990-19
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
P006-SS017-0612-03

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

Quant Time: Dec 13 07:15:52 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 13 06:23:40 2016
Response via : Initial Calibration

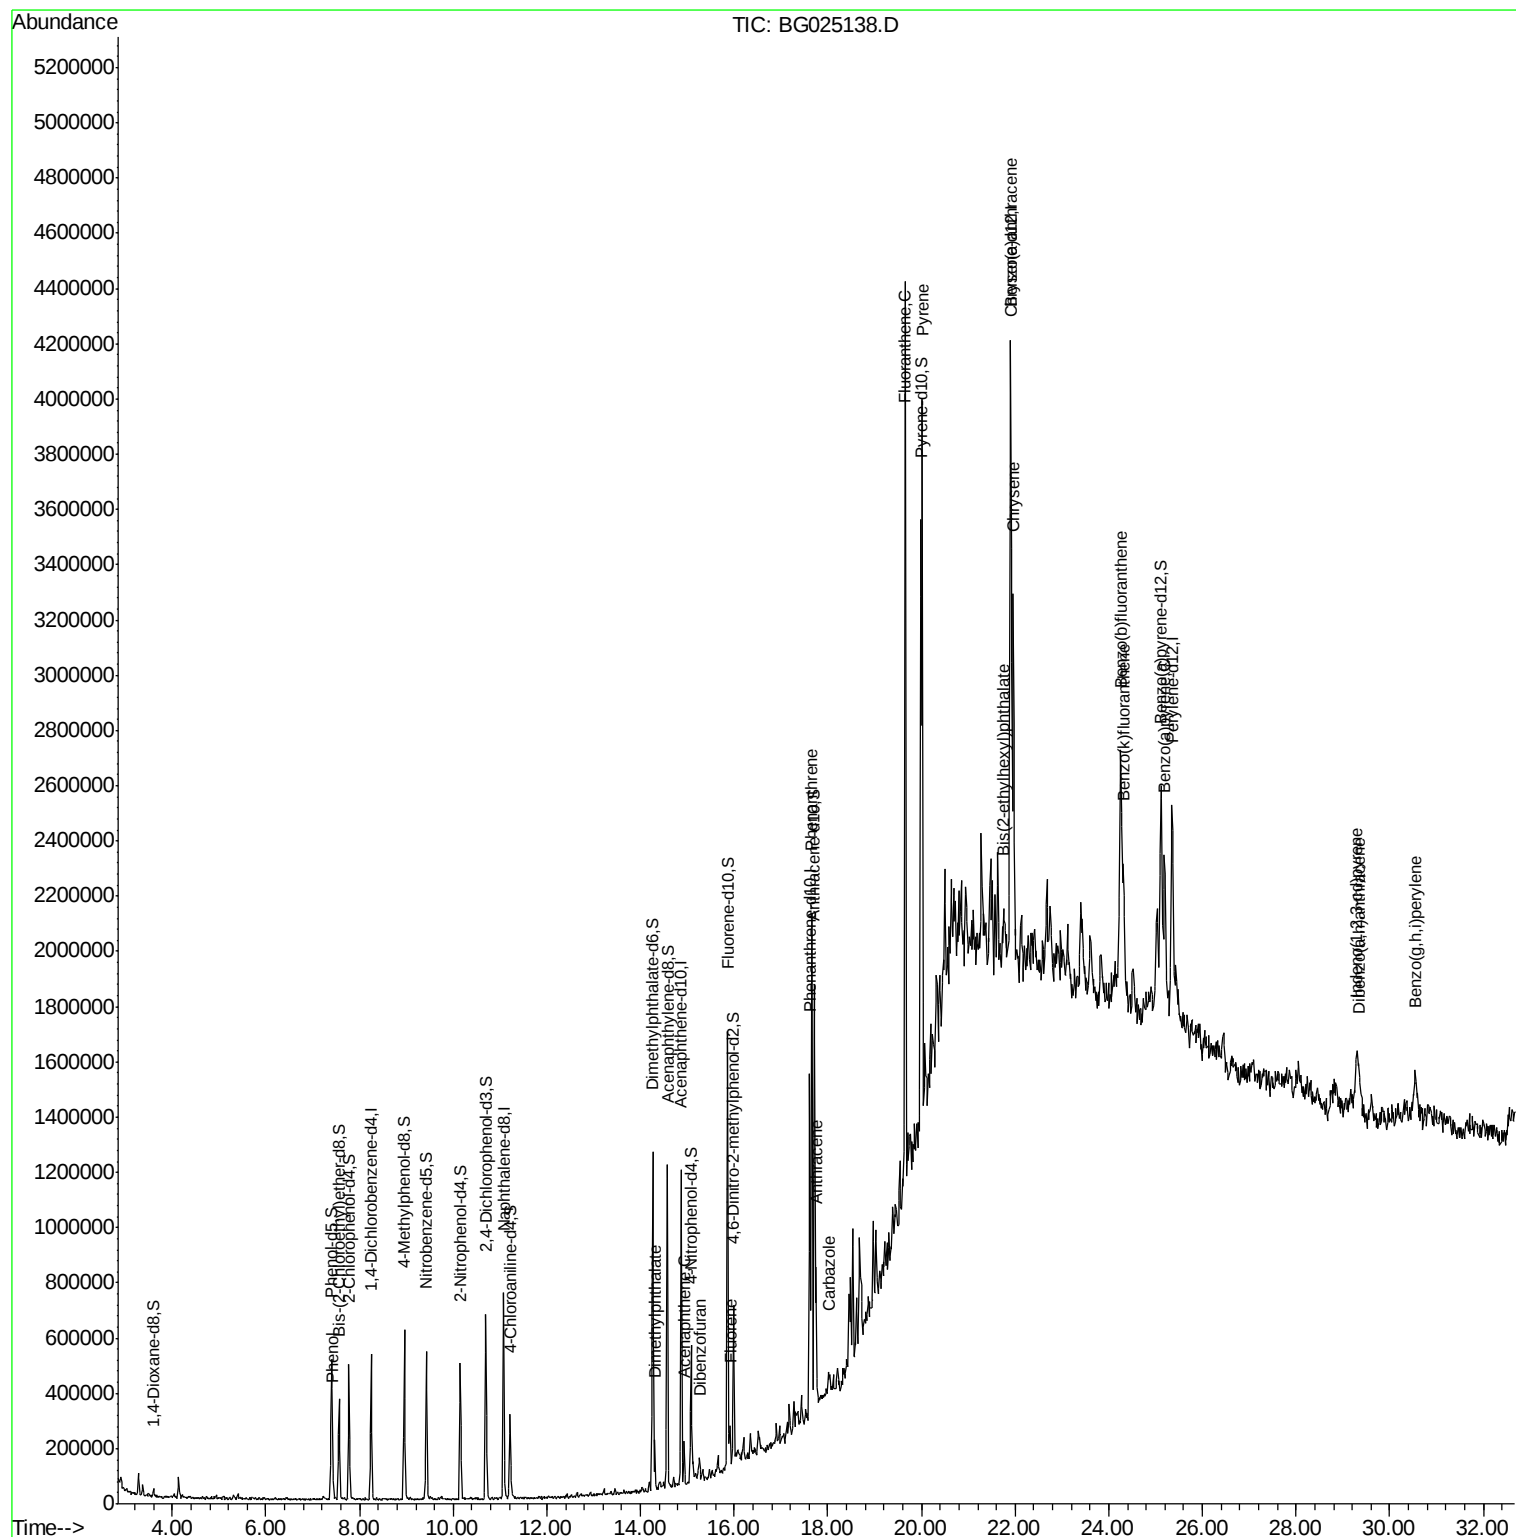

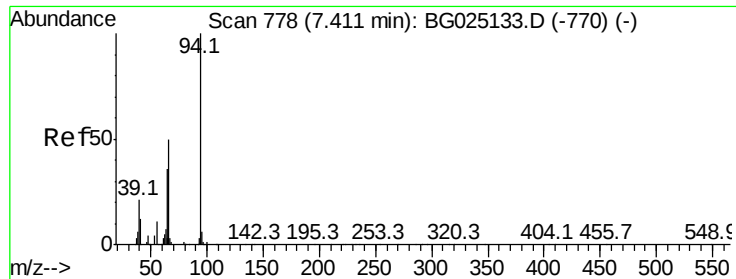

#6

Phenol

Concen: 3.83 ng/ul

RT: 7.43 min Scan# 781

Delta R.T. 0.02 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Instrument :

BNA_G





ClientSampleId :

P006-SS017-0612-03

Tot Ion:	94	Resp:	46279
Ion Ratio	Lower	Upper	
94	100		
65	36.7	26.8	40.2
66	55.2	44.4	66.6

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

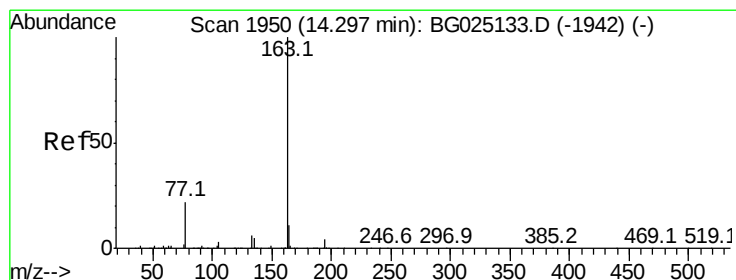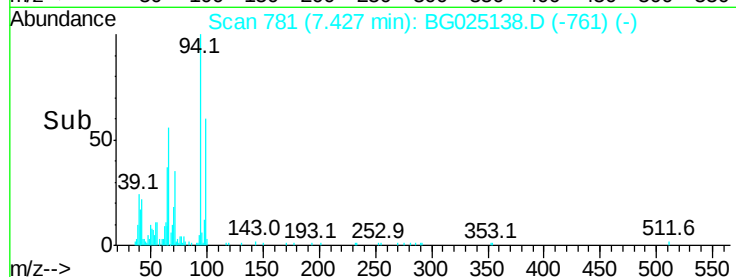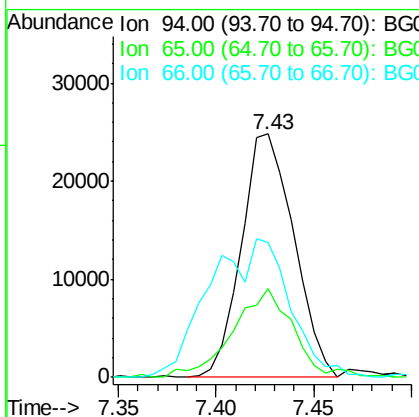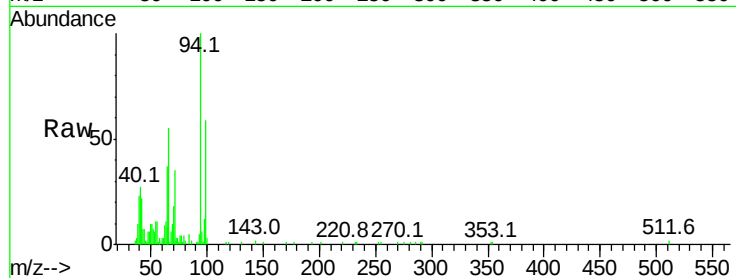

#44

Dimethylphthalate

Concen: 3.68 ng/ul




RT: 14.31 min Scan# 1952


Delta R.T. 0.01 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Tgt Ion:	163	Resp:	105420
Ion Ratio	Lower	Upper	
163	100		
194	5.3	3.4	5.0#
164	13.4	9.0	13.4

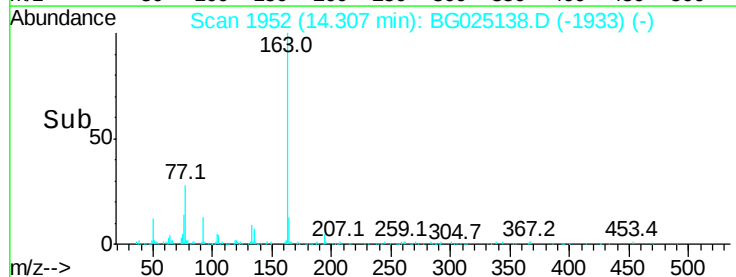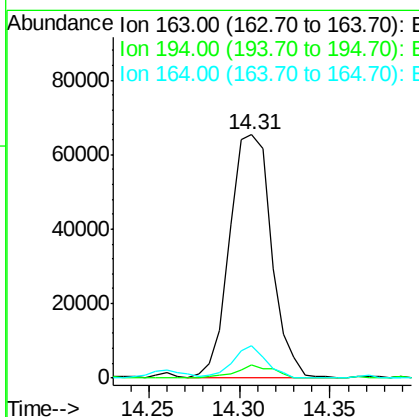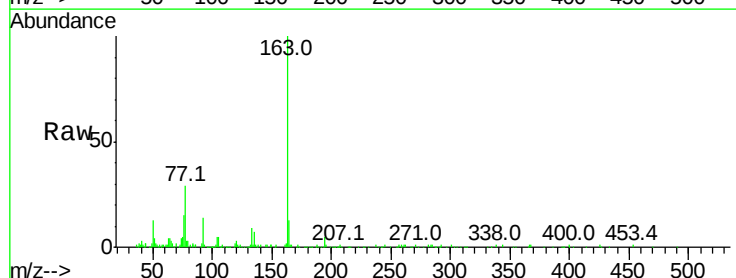

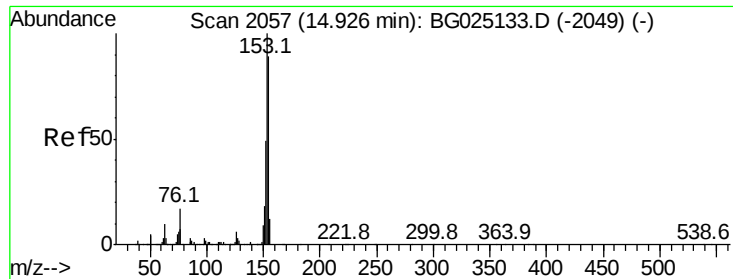

#49

Acenaphthene

Concen: 2.94 ng/ul

RT: 14.93 min Scan# 2058

Delta R.T. 0.00 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Instrument :

BNA_G





ClientSampleId :

P006-SS017-0612-03

Tot Ion:	153	Resp:	62541
Ion Ratio	Lower	Upper	
153	100		
152	41.1	36.5	54.7
154	95.7	72.3	108.5

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

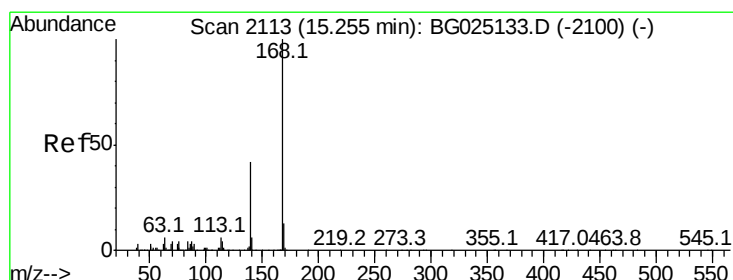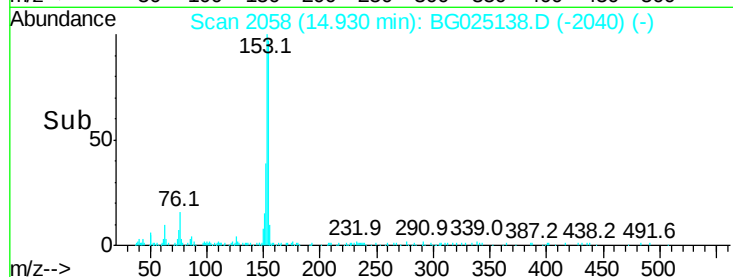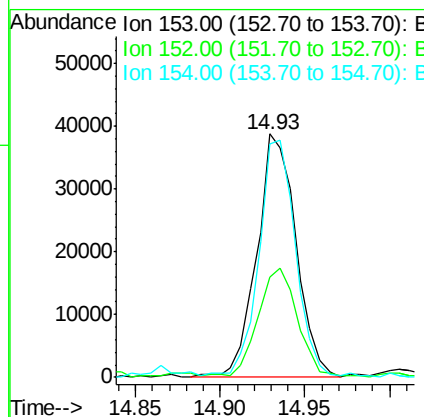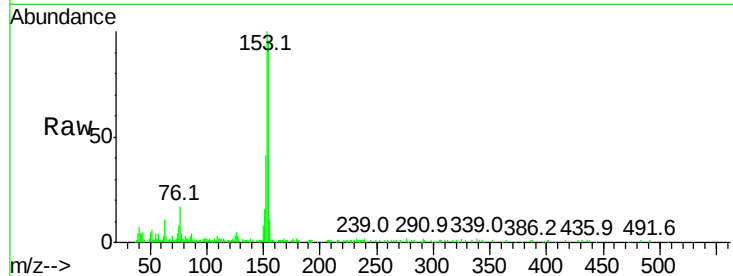

#53

Dibenzofuran

Concen: 1.13 ng/ul




RT: 15.26 min Scan# 2115


Delta R.T. 0.01 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Tgt Ion:	168	Resp:	38050
Ion Ratio	Lower	Upper	
168	100		
139	35.3	33.8	50.8

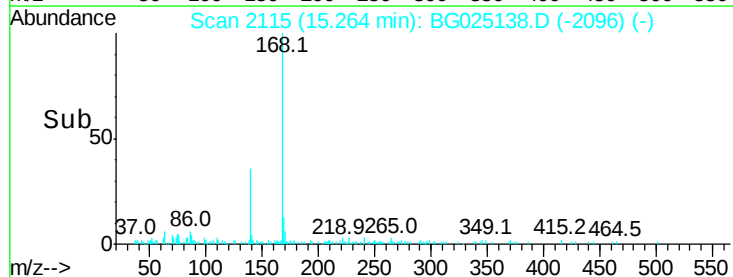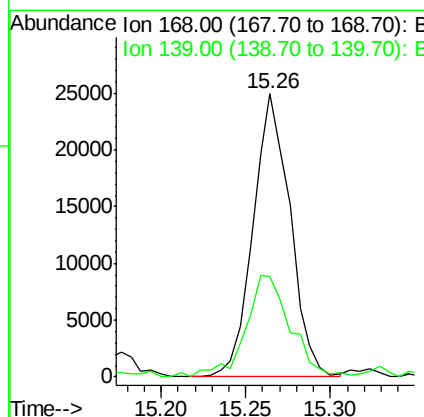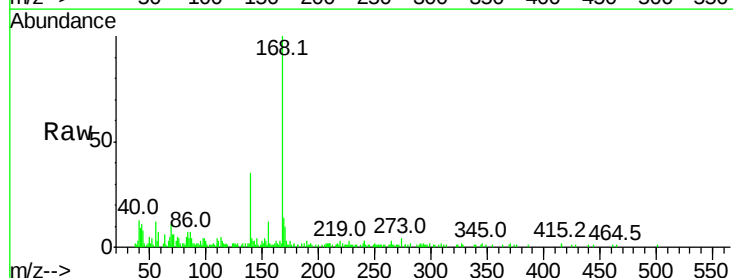

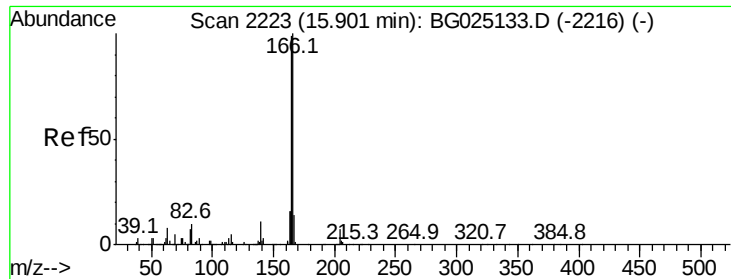

#58

Fluorene

Concen: 2.31 ng/ul

RT: 15.91 min Scan# 2225

Delta R.T. 0.01 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Instrument :

BNA_G





ClientSampleId :

P006-SS017-0612-03

Tot Ion:	166	Resp:	63118
Ion Ratio	Lower	Upper	
166	100		
165	97.7	79.7	119.5
167	13.8	11.4	17.2

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

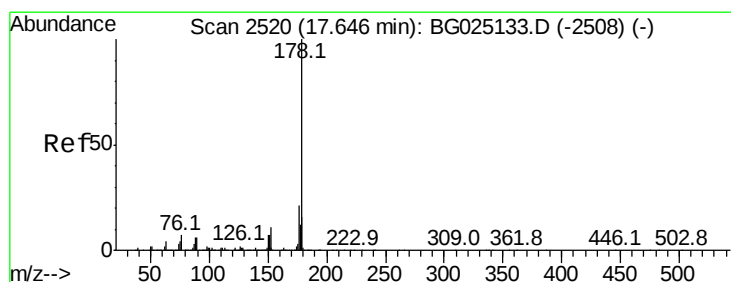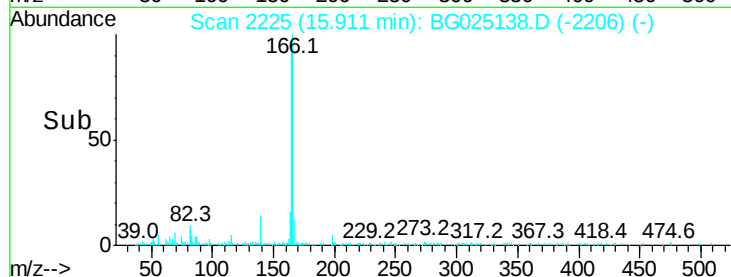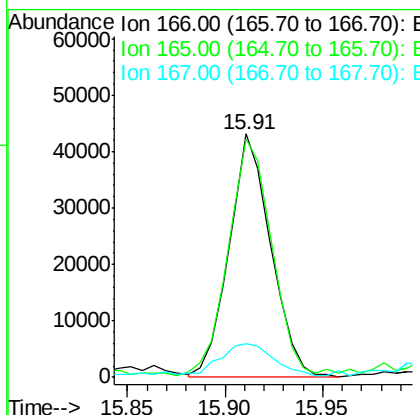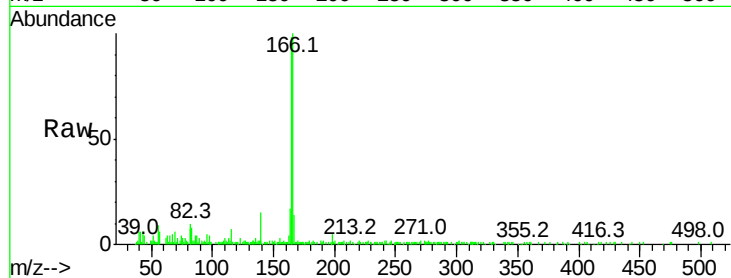

#69

Phenanthrene

Concen: 32.09 ng/ul




RT: 17.66 min Scan# 2522


Delta R.T. 0.01 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Tgt Ion:	178	Resp:	1144624
Ion Ratio	Lower	Upper	
178	100		
179	16.8	12.4	18.6
176	20.4	16.5	24.7

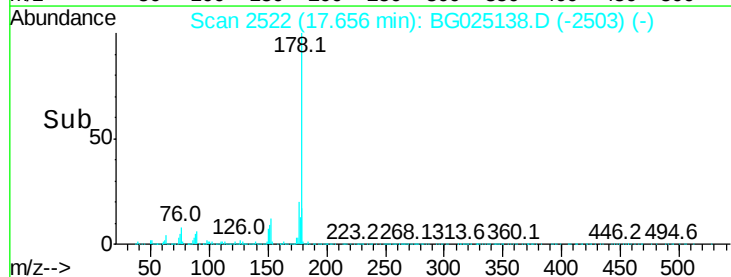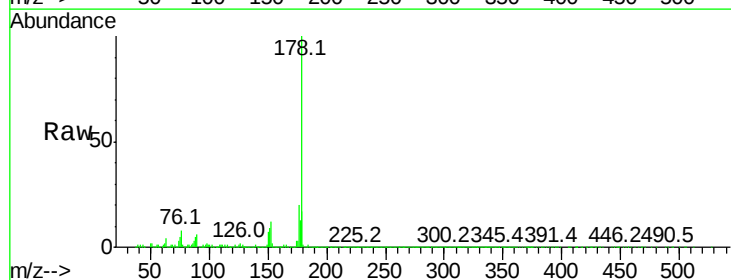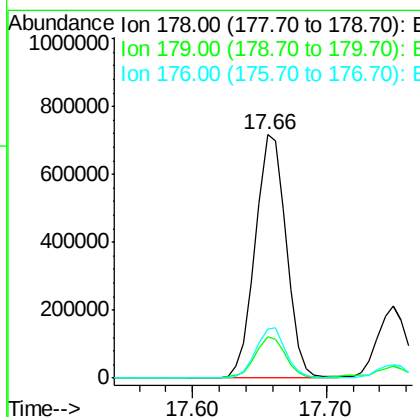

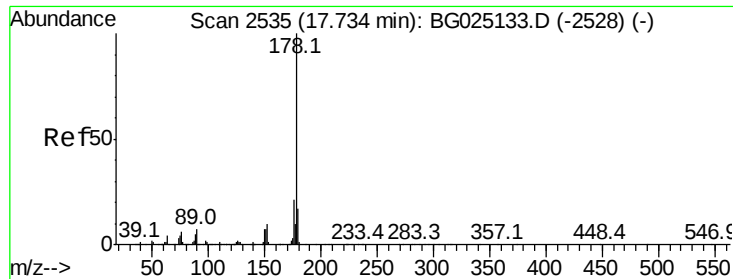





#71
 Anthracene
 Concen: 8.45 ng/ul
 RT: 17.75 min Scan# 2538
 Delta R.T. 0.02 min
 Lab File: BG025138.D
 Acq: 13 Dec 2016 6:36

Instrument :
 BNA_G
 ClientSampleId :
 P006-SS017-0612-03

Tot Ion	Ratio	Lower	Upper
178	100		
179	17.5	12.6	19.0
176	18.5	15.9	23.9




Manual Integrations
 APPROVED


sohil
 12/13/2016 6:07:56 PM

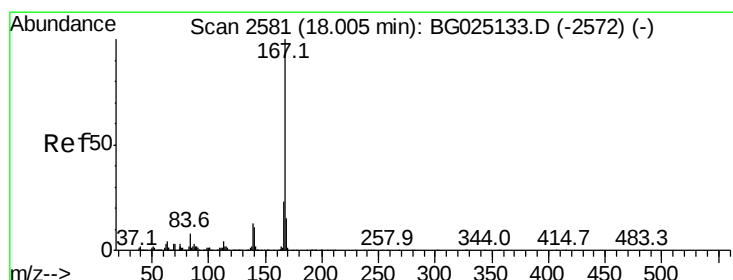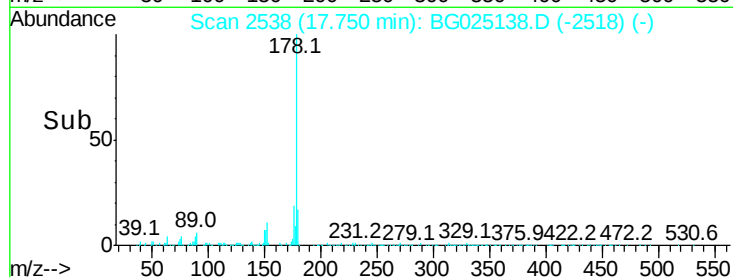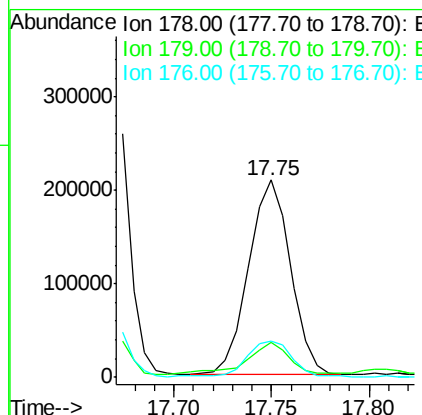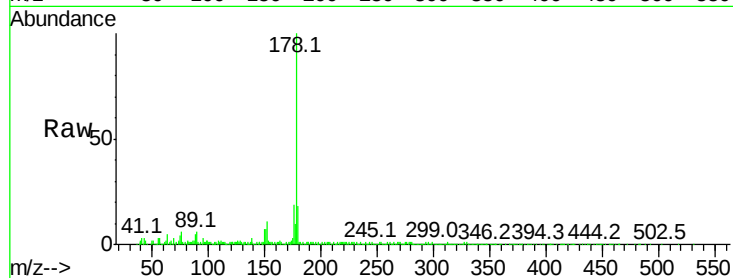

#72
 Carbazole
 Concen: 1.09 ng/ul
 RT: 18.01 min Scan# 2583
 Delta R.T. 0.01 min
 Lab File: BG025138.D
 Acq: 13 Dec 2016 6:36

Tgt Ion	Ratio	Lower	Upper
167	100		
166	27.0	17.9	26.9#
139	18.0	10.5	15.7#

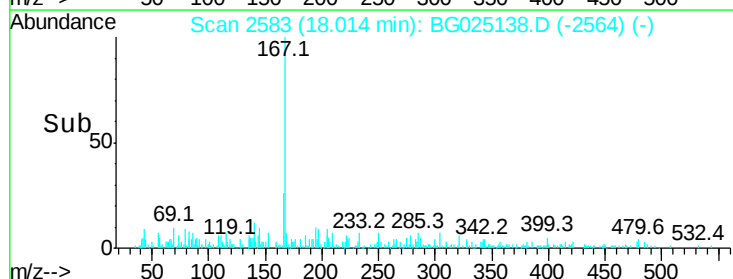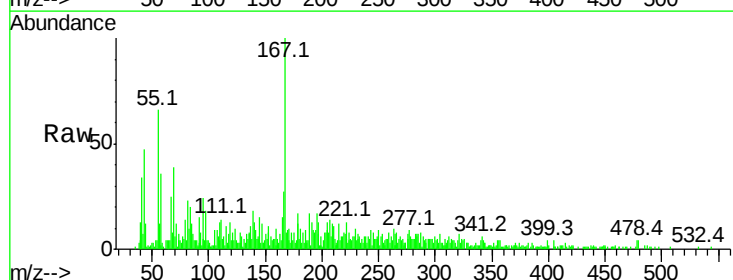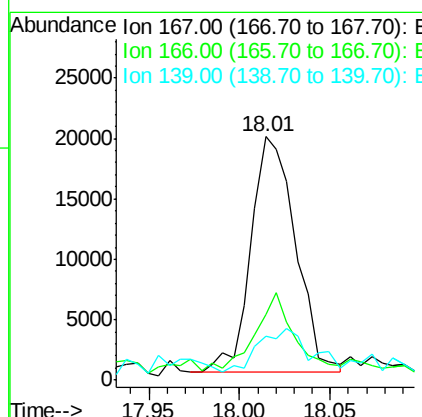

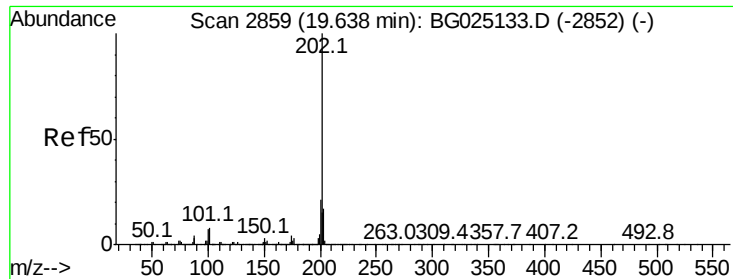

#74

Fluoranthene

Concen: 46.66 ng/ul

RT: 19.65 min Scan# 2862

Delta R.T. 0.02 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Instrument :

BNA_G





ClientSampleId :

P006-SS017-0612-03

Tot Ion:	202	Resp:	1977883
Ion Ratio	Lower	Upper	
202	100		
101	7.6	6.2	9.2
100	6.9	5.2	7.8

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

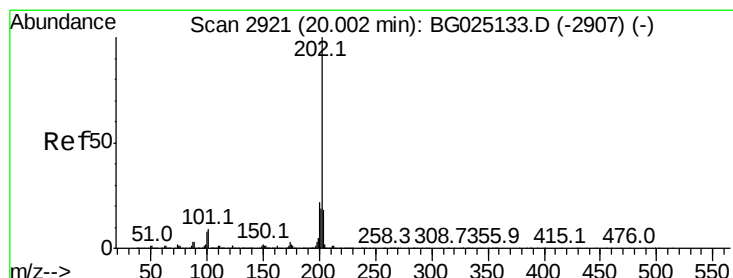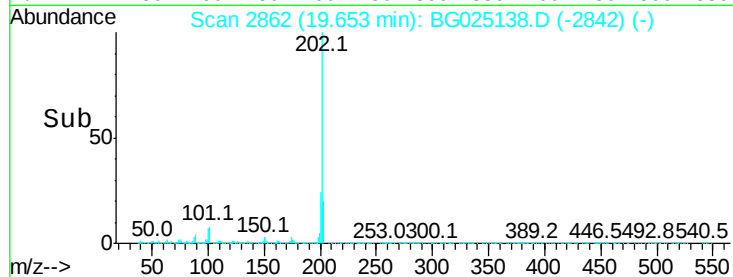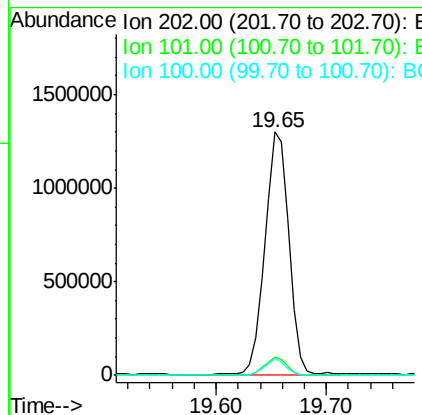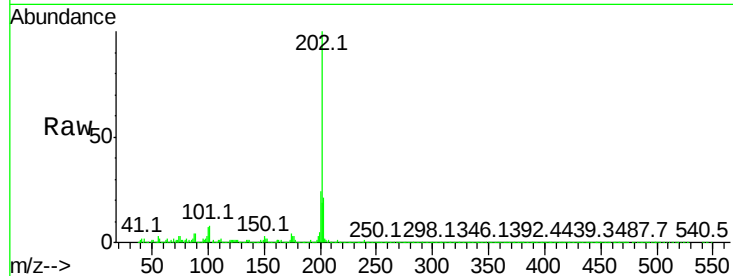

#77

Pyrene

Concen: 34.85 ng/ul




RT: 20.02 min Scan# 2924


Delta R.T. 0.02 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Tgt Ion:	202	Resp:	1590782
Ion Ratio	Lower	Upper	
202	100		
101	8.7	6.9	10.3
100	7.2	6.6	10.0

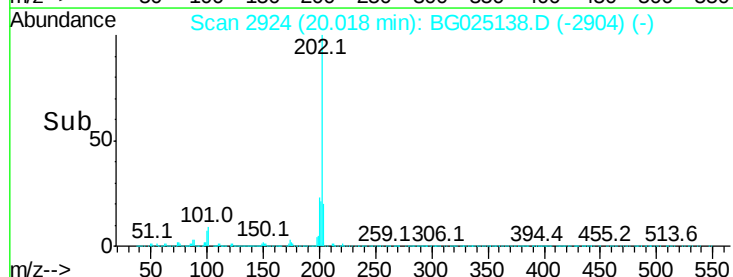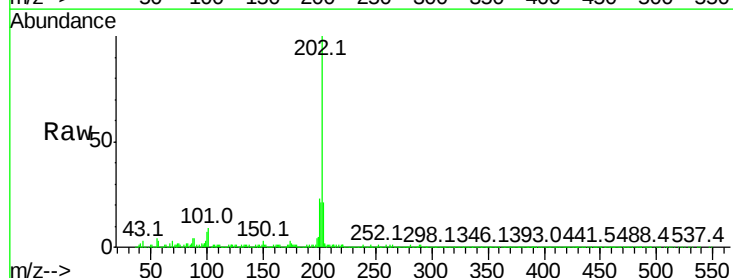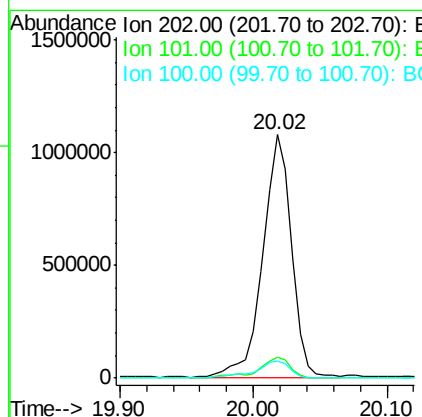

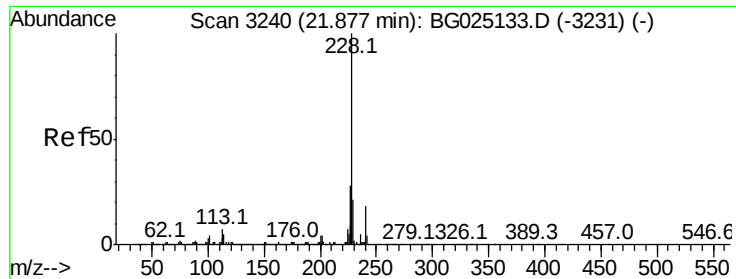

#80

Benzo(a)anthracene

Concen: 22.80 ng/ul

RT: 21.89 min Scan# 3243

Delta R.T. 0.02 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Instrument :

BNA_G





ClientSampleId :

P006-SS017-0612-03

Tot Ion:	228	Resp:	1124953
Ion	Ratio	Lower	Upper
228	100		
229	22.4	16.3	24.5
226	28.8	21.9	32.9

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

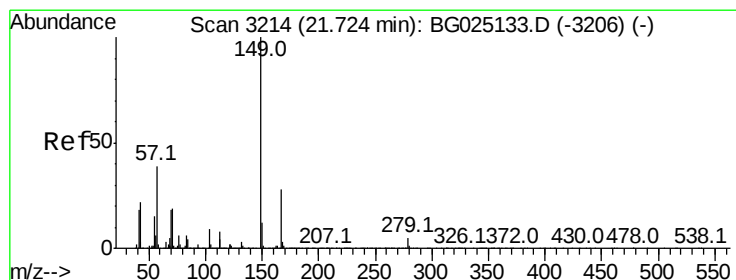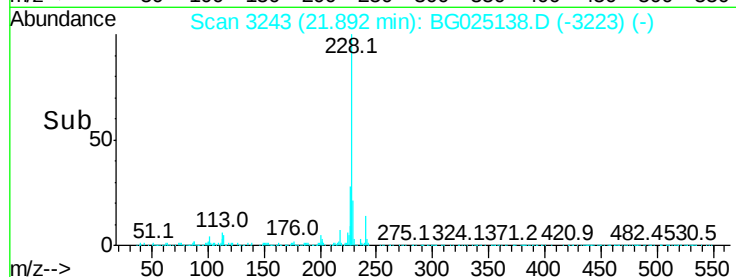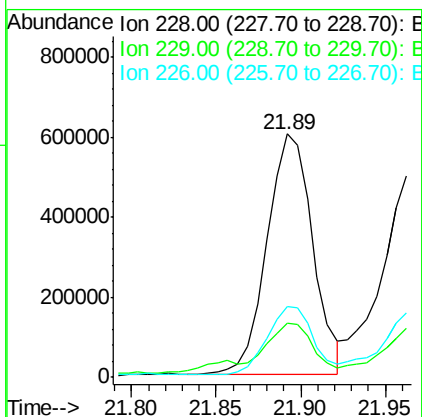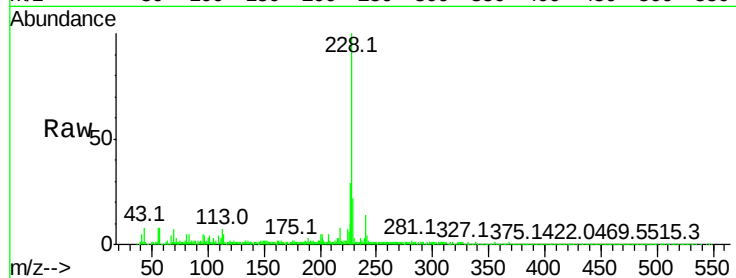

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.20 ng/ul




RT: 21.74 min Scan# 3217


Delta R.T. 0.02 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Tgt Ion:	149	Resp:	29644
Ion	Ratio	Lower	Upper
149	100		
167	45.0	21.8	32.8#
279	20.9	4.5	6.7#

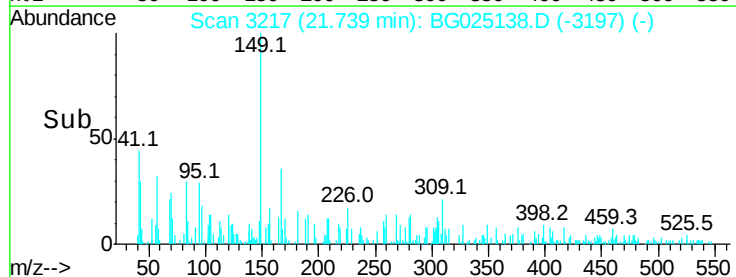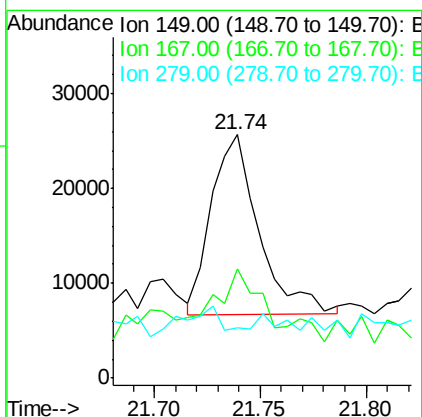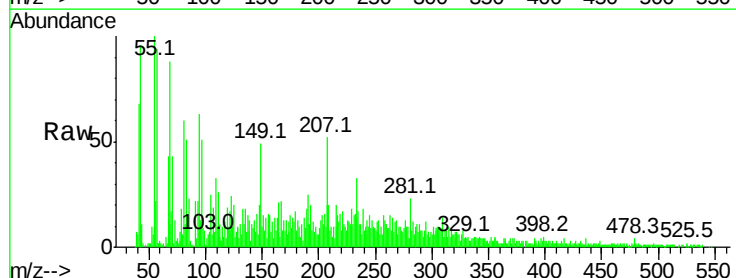

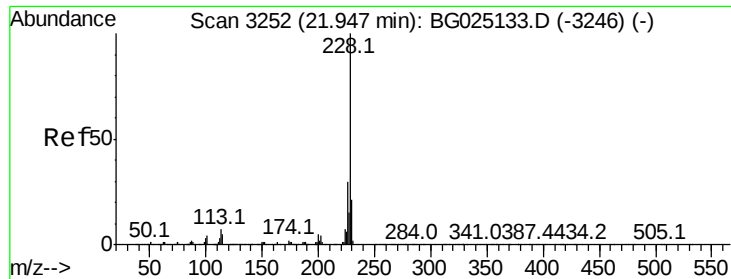

#82

Chrysene

Concen: 20.55 ng/ul

RT: 21.96 min Scan# 3255

Delta R.T. 0.02 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Instrument :

BNA_G





ClientSampleId :

P006-SS017-0612-03

Tot Ion:	228	Resp:	948621
Ion Ratio	Lower	Upper	
228	100		
226	32.3	24.0	36.0
229	24.2	16.9	25.3

Manual Integrations
APPROVED

sohil
12/13/2016 6:07:56 PM

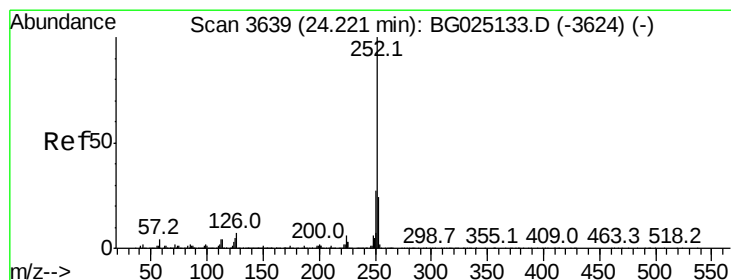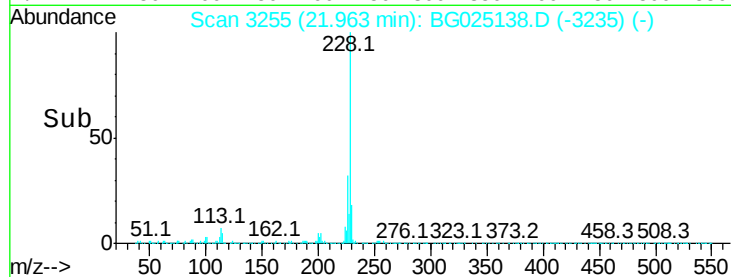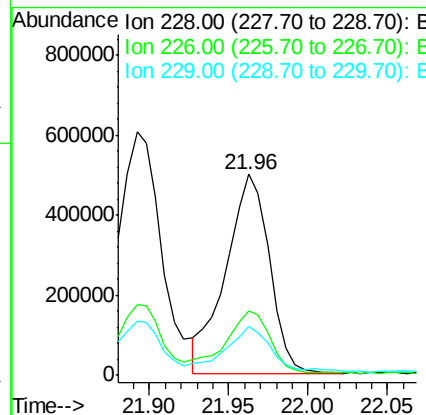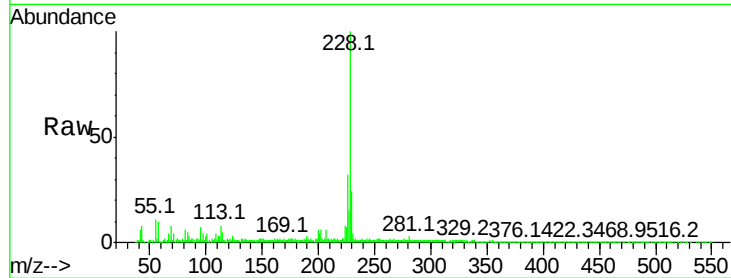

#85

Benzo(b)fluoranthene

Concen: 24.77 ng/ul




RT: 24.25 min Scan# 3645


Delta R.T. 0.03 min

Lab File: BG025138.D

Acq: 13 Dec 2016 6:36

Tgt Ion:	252	Resp:	1138065
Ion Ratio	Lower	Upper	
252	100		
253	26.4	17.7	26.5
125	7.1	4.0	6.0#

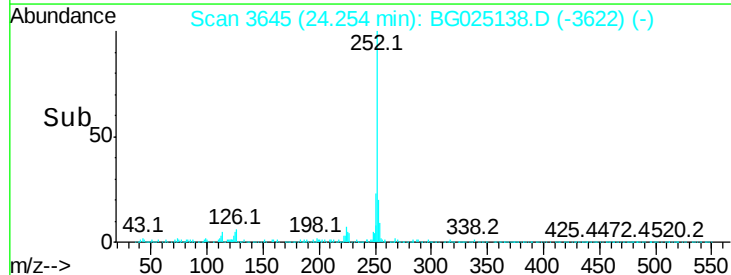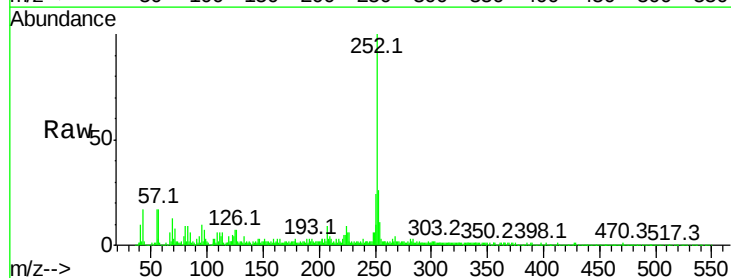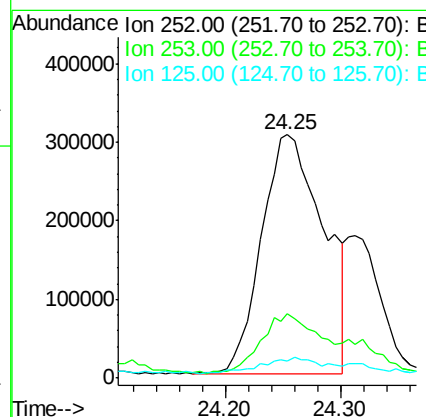

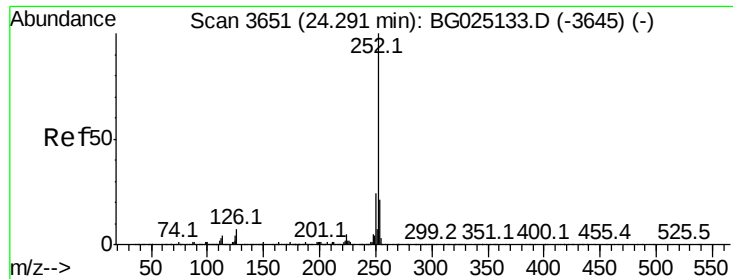





#86
Benzo(k)fluoranthene
Concen: 9.11 ng/ul m
RT: 24.31 min Scan# 3655
Delta R.T. 0.02 min
Lab File: BG025138.D
Acq: 13 Dec 2016 6:36

Instrument :
BNA_G
ClientSampleId :
P006-SS017-0612-03

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.9	18.5	27.7
125	10.2	4.1	6.1#




Manual Integrations
APPROVED


sohil
12/13/2016 6:07:56 PM

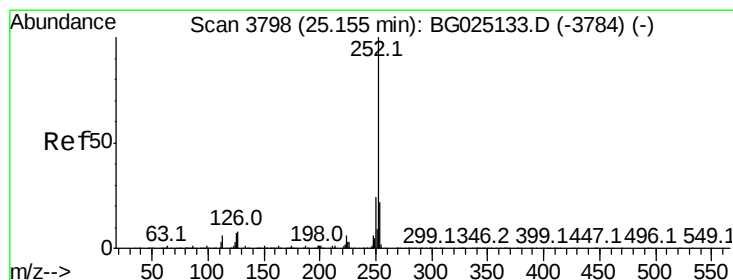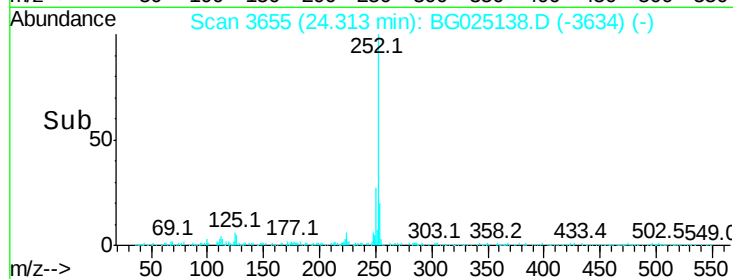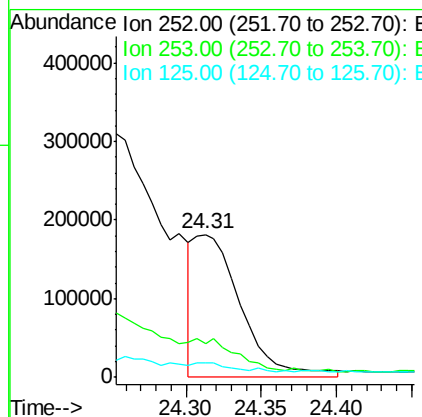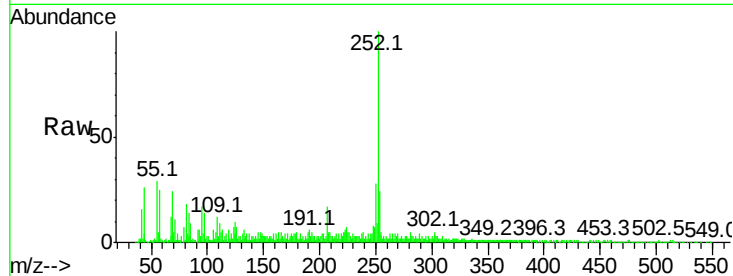

#88
Benzo(a)pyrene
Concen: 15.42 ng/ul
RT: 25.19 min Scan# 3805
Delta R.T. 0.04 min
Lab File: BG025138.D
Acq: 13 Dec 2016 6:36

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.8	26.6
125	8.0	5.4	8.0

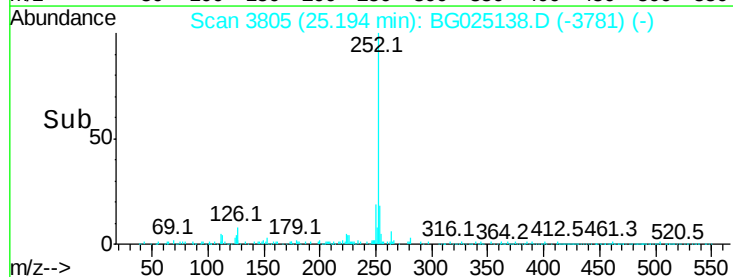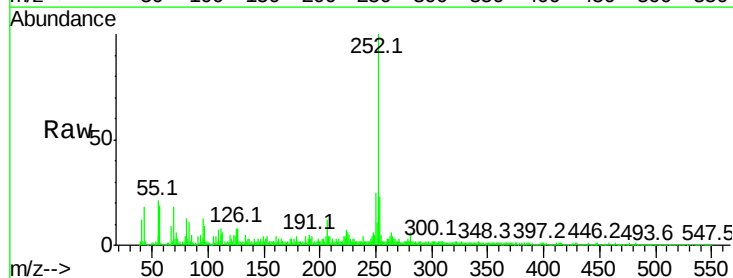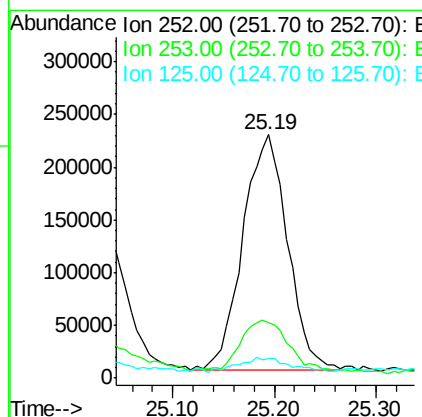

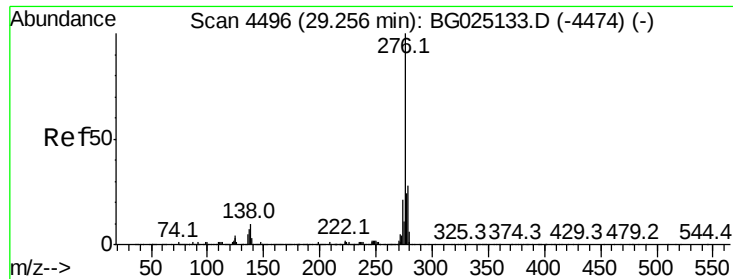

#89





Indeno(1,2,3-cd)pyrene
Concen: 7.65 ng/ul m
RT: 29.30 min Scan# 4503
Delta R.T. 0.04 min
Lab File: BG025138.D
Acq: 13 Dec 2016 6:36

Instrument :
BNA_G
ClientSampleId :
P006-SS017-0612-03

Tot Ion	Ratio	Lower	Upper
276	100		
138	12.2	8.2	12.4
277	28.1	18.6	28.0

Manual Integrations
APPROVED




sohil
12/13/2016 6:07:56 PM

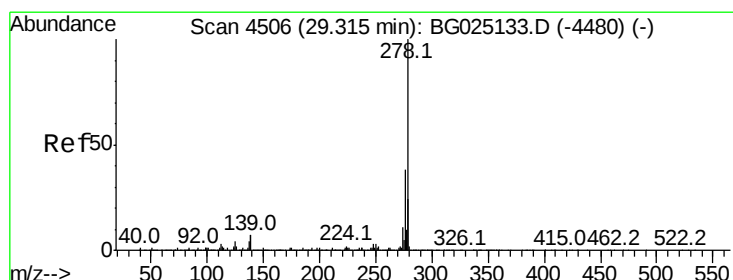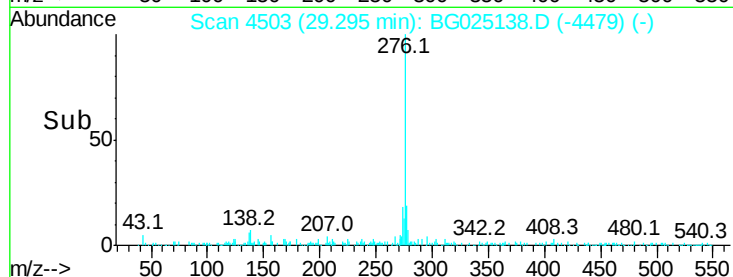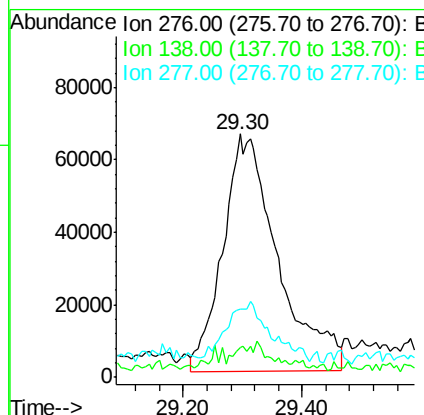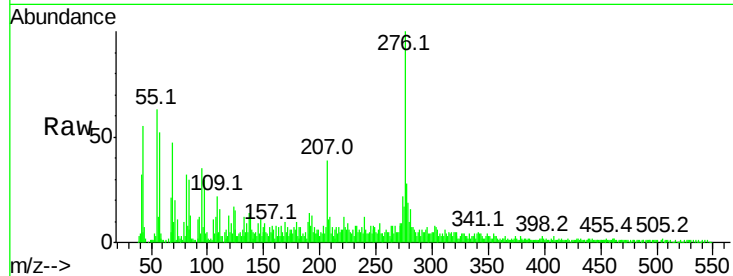


#90

Dibenzo(a,h)anthracene
Concen: 1.24 ng/ul
RT: 29.35 min Scan# 4513
Delta R.T. 0.04 min
Lab File: BG025138.D
Acq: 13 Dec 2016 6:36

Tgt Ion	Ratio	Lower	Upper
278	100		
139	19.4	6.7	10.1
279	31.4	20.9	31.3

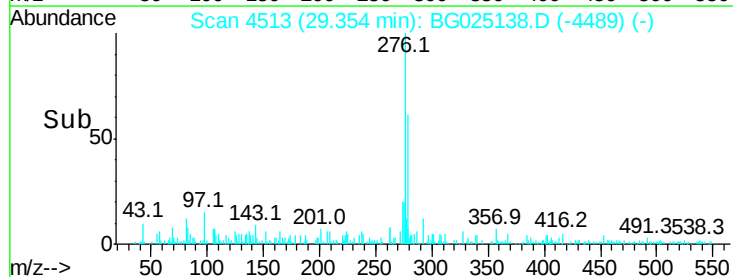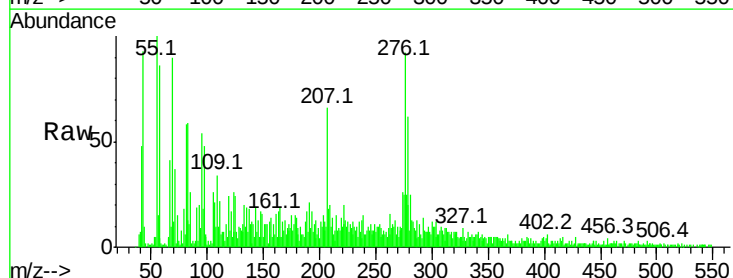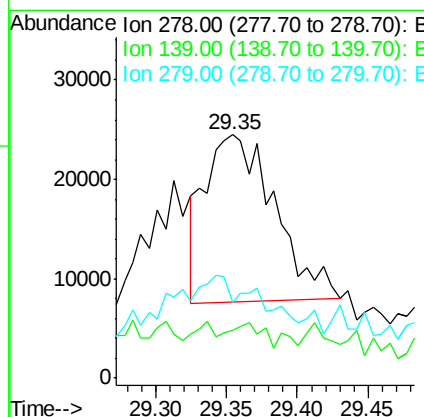

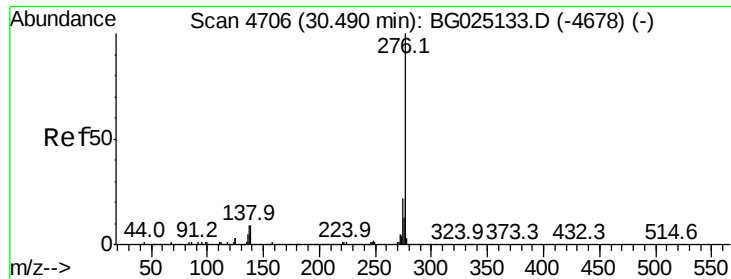

#91
 Benzo(a,h,i)perylene
 Concen: 6.35 ng/ul m
 RT: 30.55 min Scan# 4716
 Delta R.T. 0.06 min
 Lab File: BG025138.D
 Acq: 13 Dec 2016 6:36

Instrument :
 BNA_G
 ClientSampleId :
 P006-SS017-0612-03

Tot Ion	Ratio	Lower	Upper
276	100		
138	9.9	8.6	12.8
277	30.0	17.6	26.4

Manual Integrations
 APPROVED

sohil
 12/13/2016 6:07:56 PM

