

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121217\
 Data File : BG031493.D
 Acq On : 12 Dec 2017 15:46
 Operator : SJ/JU
 Sample : I6763-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 120517-JETT-F-U-B

Quant Time: Dec 13 05:51:56 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 17:25:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	50833	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	219329	20.00	ng	0.00
38) Acenaphthene-d10	14.73	164	149771	20.00	ng	0.00
63) Phenanthrene-d10	17.47	188	418830	20.00	ng	0.00
75) Chrysene-d12	21.75	240	494591	20.00	ng	0.00
86) Perylene-d12	25.03	264	470285	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	136519	47.60	ng	0.00
7) Phenol-d6	7.28	99	121797	30.59	ng	0.00
23) Nitrobenzene-d5	9.28	82	325412	91.45	ng	0.00
41) 2,4,6-Tribromophenol	16.22	330	191561	109.17	ng	0.00
44) 2-Fluorobiphenyl	13.35	172	975258	95.58	ng	0.00
78) Terphenyl-d14	20.06	244	1835005	84.41	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121217\
Data File : BG031493.D
Acq On : 12 Dec 2017 15:46
Operator : SJ/JU
Sample : I6763-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120517-JETT-F-U-B

Quant Time: Dec 13 05:51:56 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration




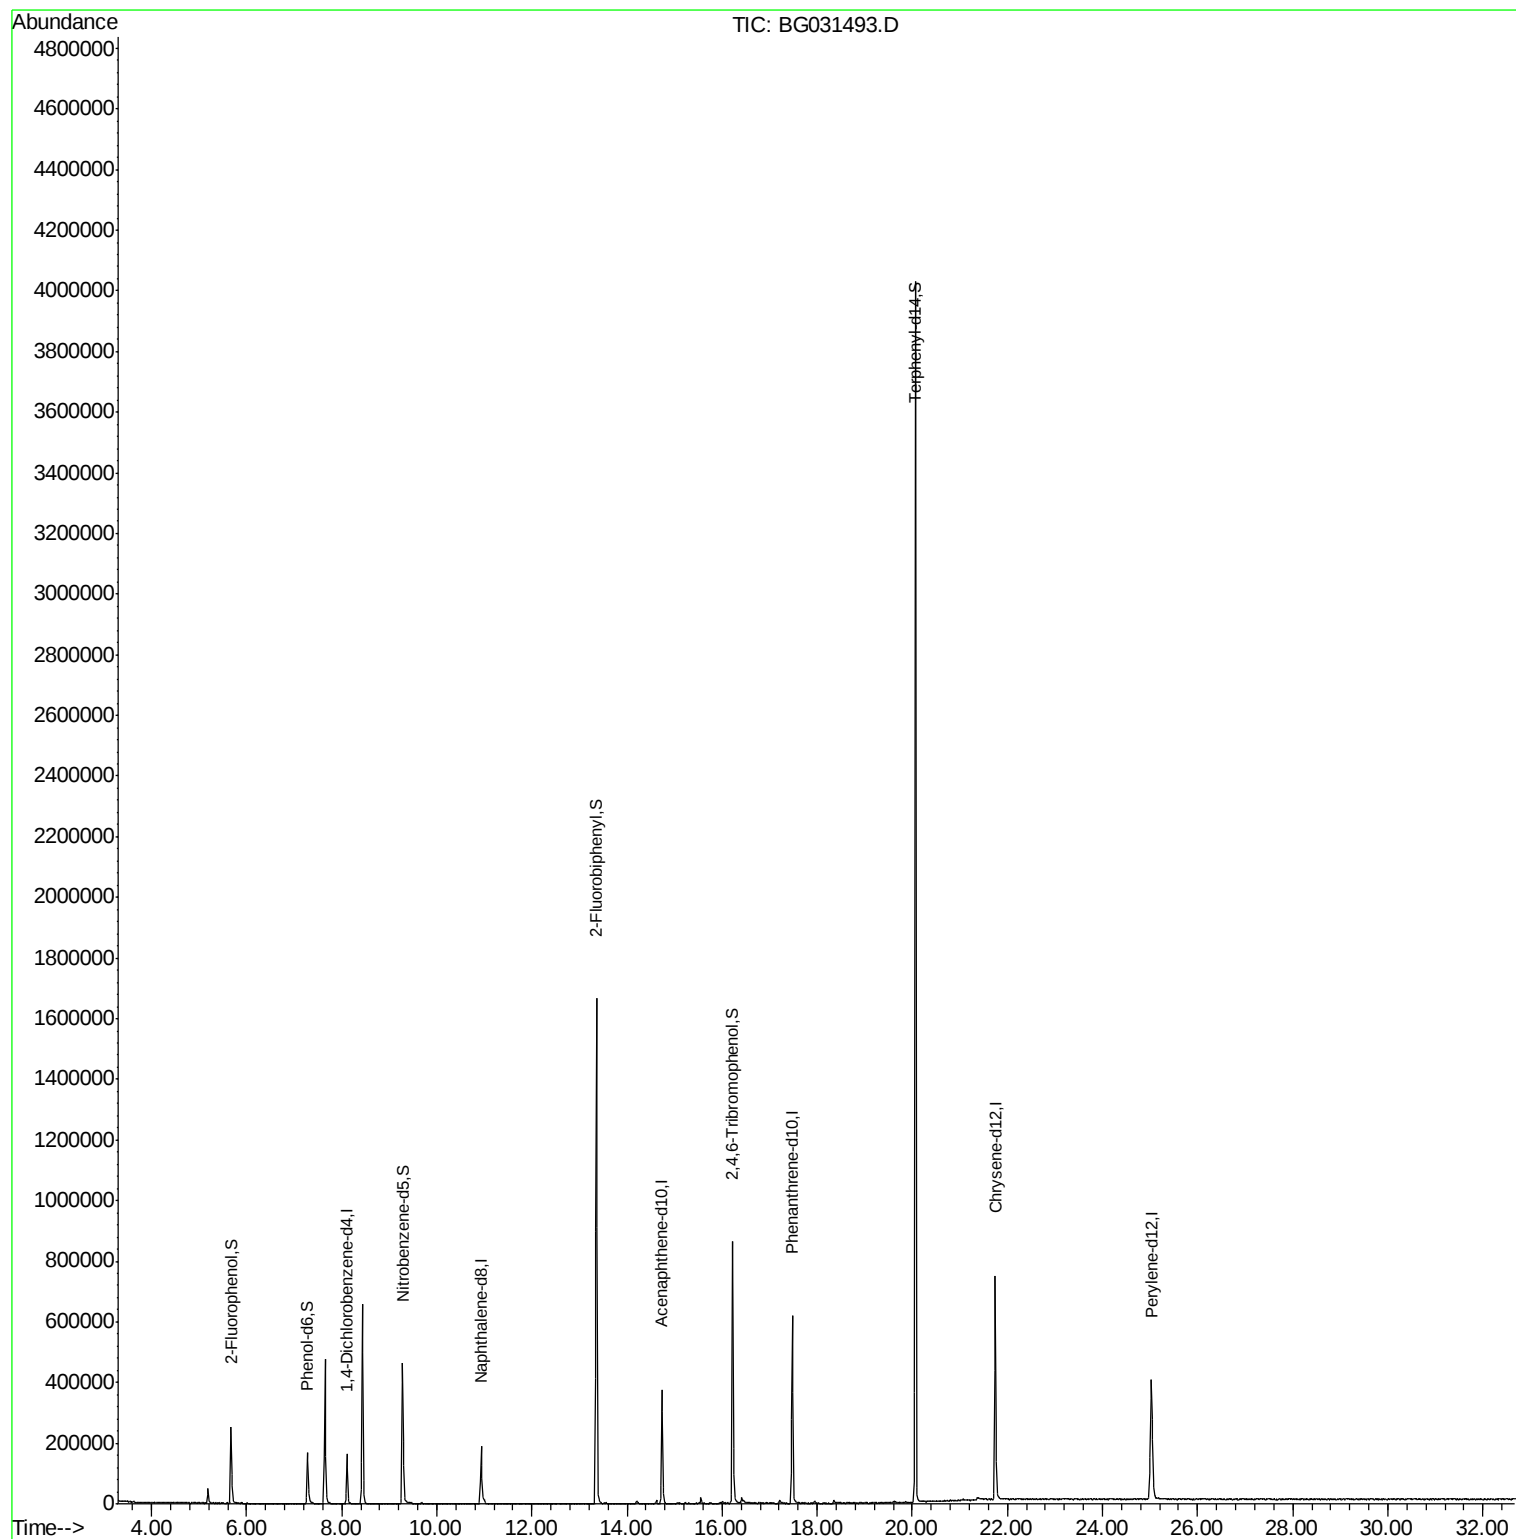


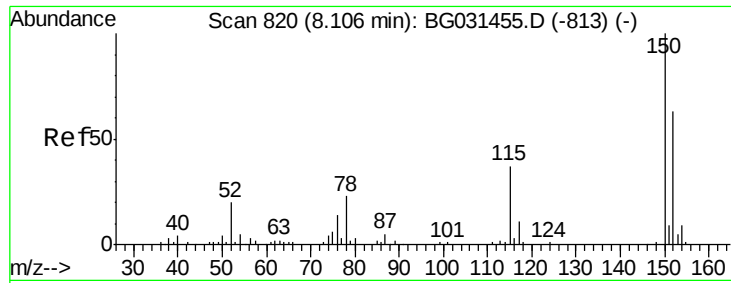

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.11 min Scan# 820
 Delta R.T. 0.00 min
 Lab File: BG031493.D
 Acq: 12 Dec 2017 15:46




Instrument :
 BNA_G
 ClientSampleId :
 120517-JETT-F-U-B


Tot Ion	Ratio	Lower	Upper
152	100		
150	154.3	126.6	189.8
115	60.8	53.0	79.4

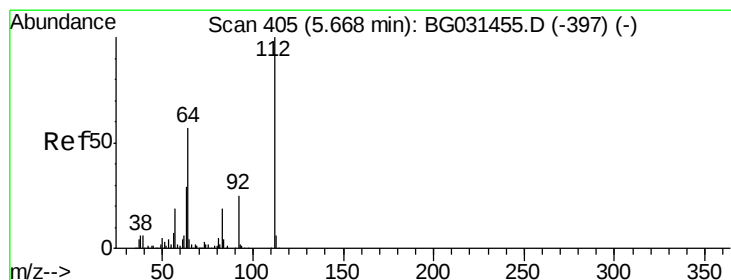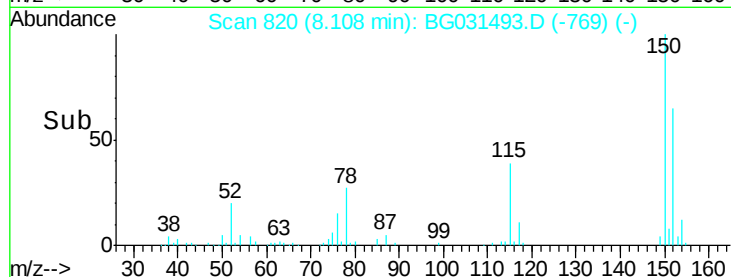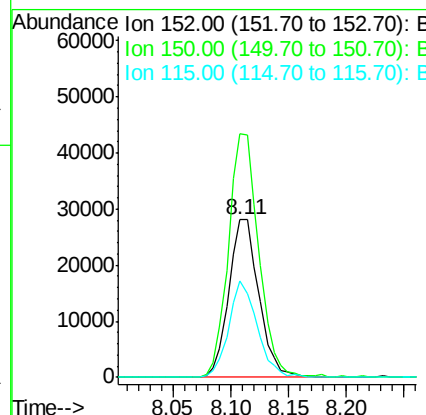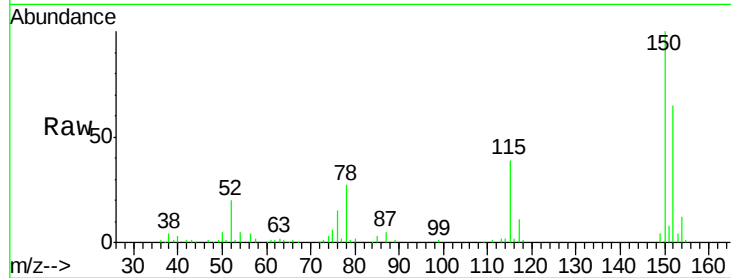

#5
 2-Fluorophenol
 Concen: 47.603 ng
 RT: 5.67 min Scan# 405
 Delta R.T. 0.00 min
 Lab File: BG031493.D
 Acq: 12 Dec 2017 15:46

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.3	56.3	84.5
63	30.1	30.1	45.1

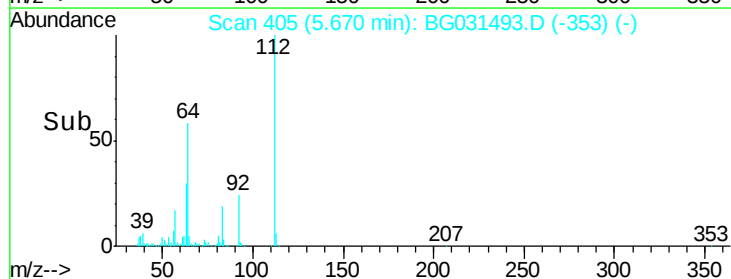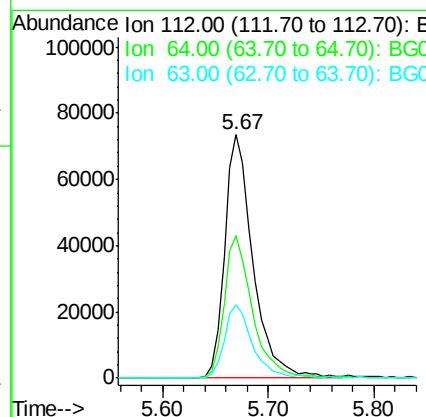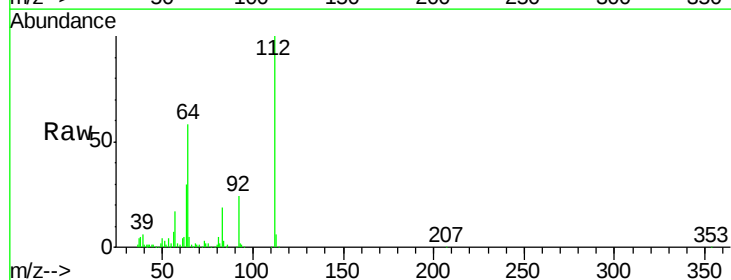

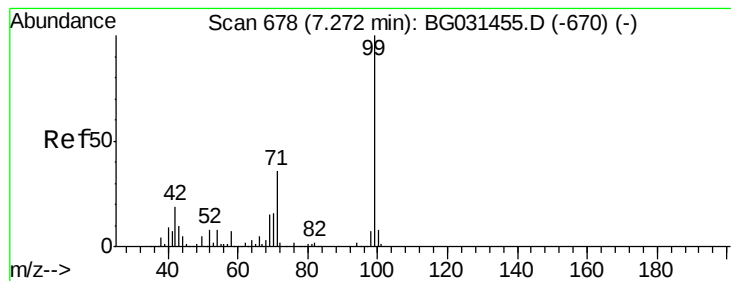

#7

Phenol-d6

Concen: 30.593 ng

RT: 7.28 min Scan# 679

Delta R.T. 0.01 min

Lab File: BG031493.D

Acq: 12 Dec 2017 15:46

Instrument :


BNA_G

ClientSampleId :

120517-JETT-F-U-B

Tot Ion: 99 Resp: 121797

Ion	Ratio	Lower	Upper
99	100		
42	16.5	14.1	21.1
71	33.6	26.1	39.1



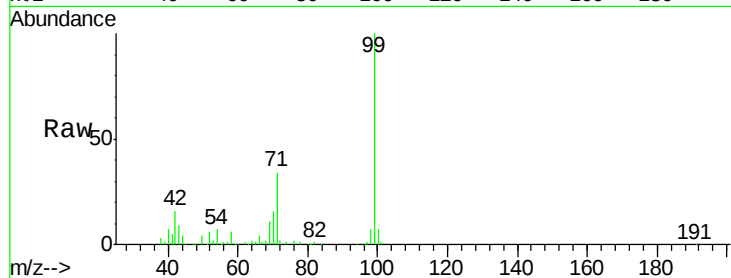


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

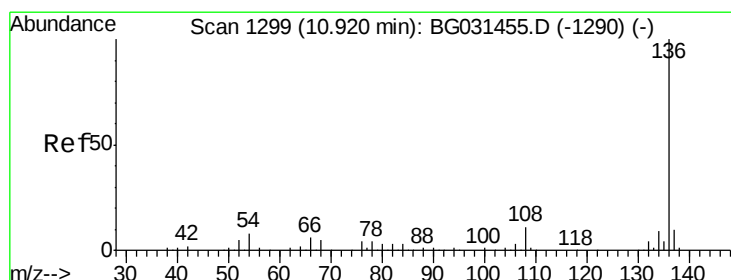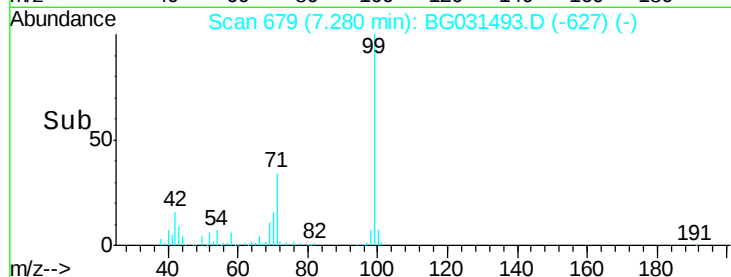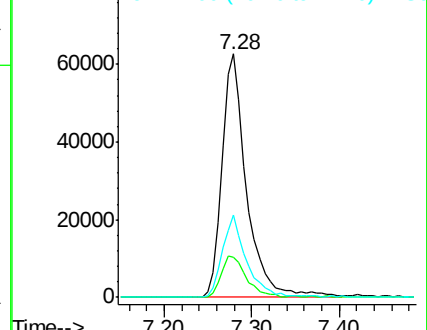

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.93 min Scan# 1300


Delta R.T. 0.01 min

Lab File: BG031493.D

Acq: 12 Dec 2017 15:46

Tgt Ion: 136 Resp: 219329

Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.2	13.8
54	7.5	10.3	15.5#
68	5.6	4.5	6.7

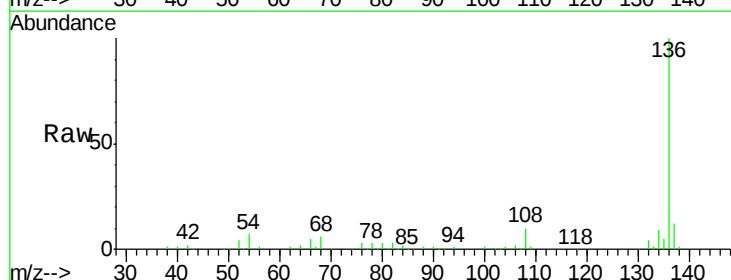



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



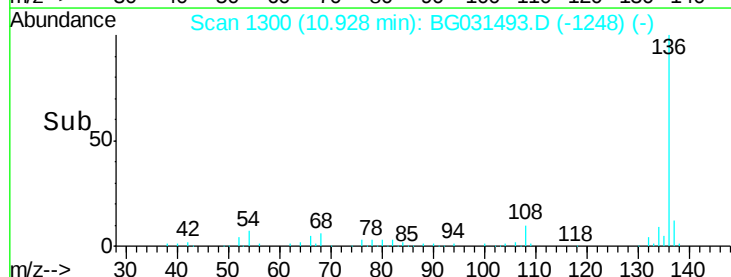
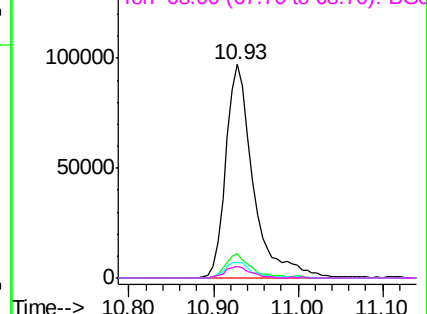


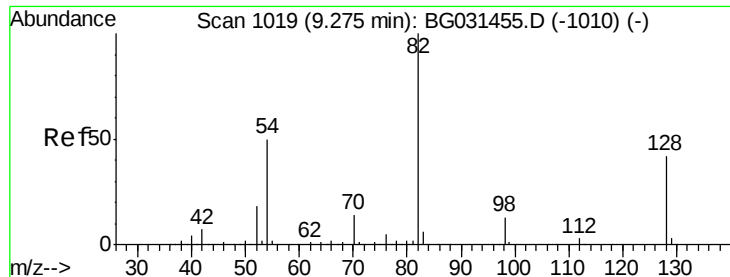

#23
Nitrobenzene-d5
Concen: 91.449 ng
RT: 9.28 min Scan# 1019
Delta R.T. 0.00 min
Lab File: BG031493.D
Acq: 12 Dec 2017 15:46




Instrument :
BNA_G
ClientSampleId :
120517-JETT-F-U-B


Tot Ion	82	Resp	325412
Ion Ratio	Lower	Upper	
82	100		
128	44.0	29.7	44.5
54	50.9	43.1	64.7

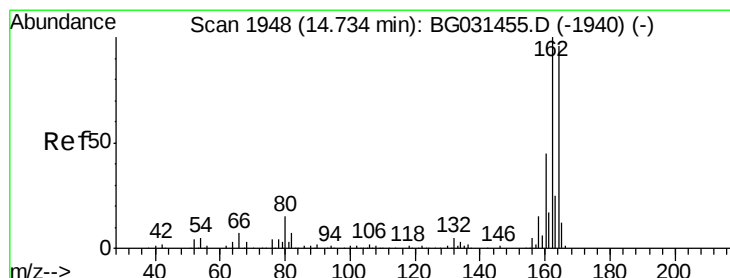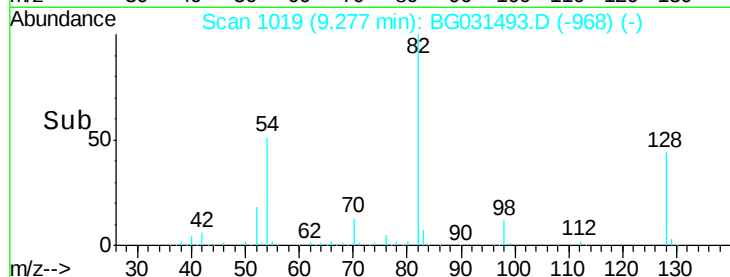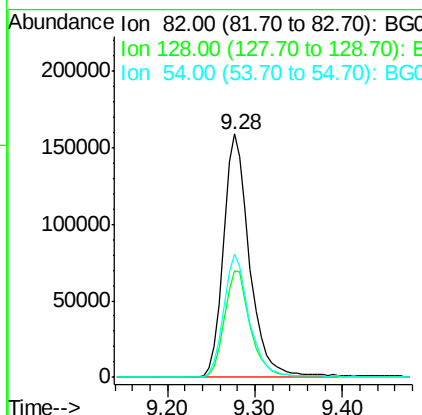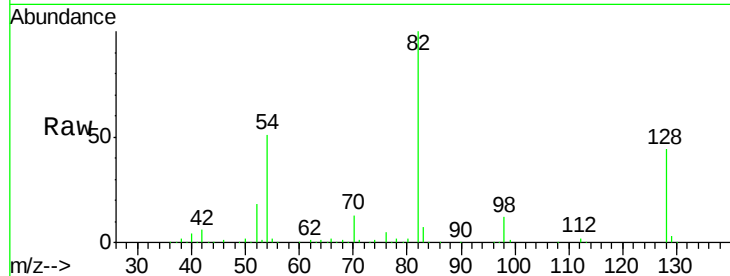

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1947
Delta R.T. -0.00 min
Lab File: BG031493.D
Acq: 12 Dec 2017 15:46

Tgt Ion	164	Resp	149771
Ion Ratio	Lower	Upper	
164	100		
162	103.5	78.8	118.2
160	44.4	35.4	53.0

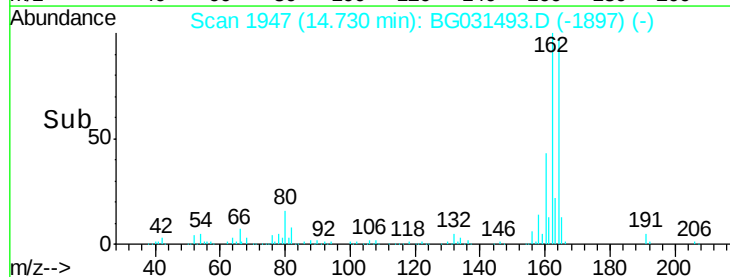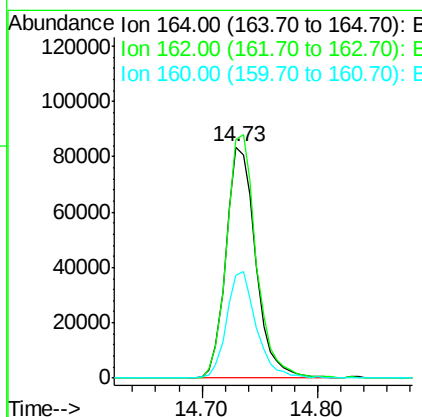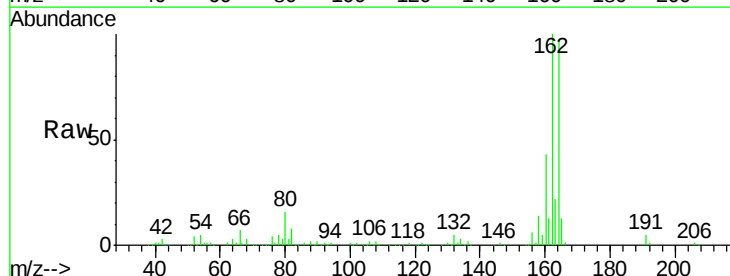


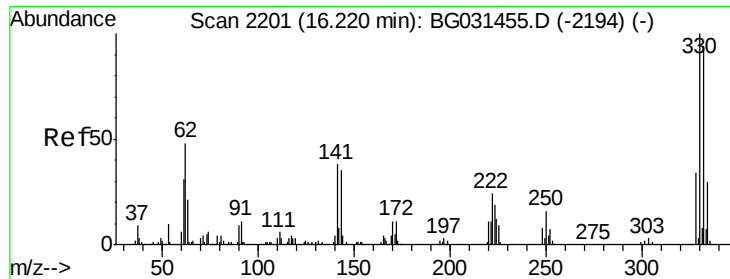

#41
 2,4,6-Tribromophenol
 Concen: 109.175 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. 0.00 min
 Lab File: BG031493.D
 Acq: 12 Dec 2017 15:46

Instrument :
 BNA_G
 ClientSampleId :
 120517-JETT-F-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.0	77.0	115.6
141	36.0	25.2	37.8



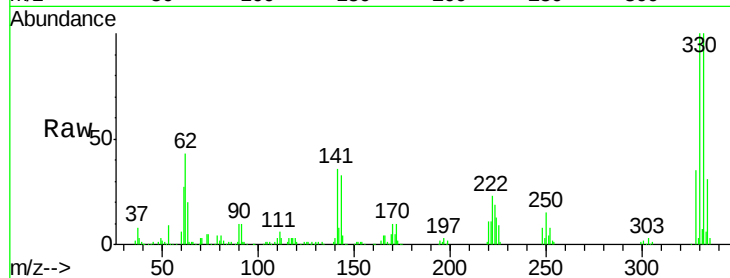


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

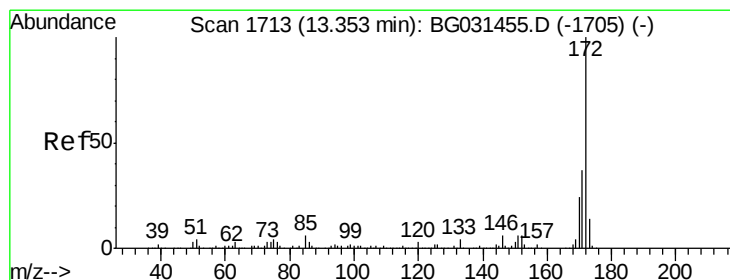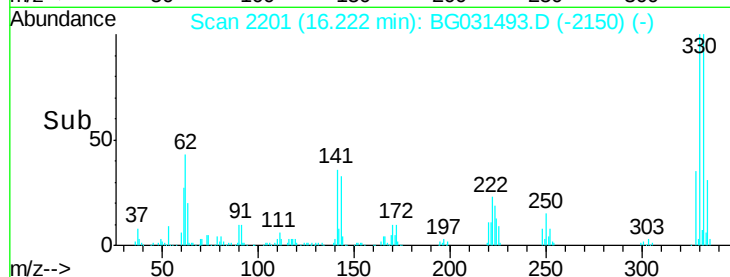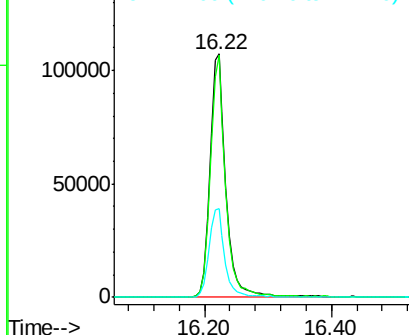

#44
 2-Fluorobiphenyl
 Concen: 95.583 ng
 RT: 13.35 min Scan# 1713
 Delta R.T. 0.00 min
 Lab File: BG031493.D
 Acq: 12 Dec 2017 15:46

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.4	30.0	45.0
170	24.8	19.5	29.3


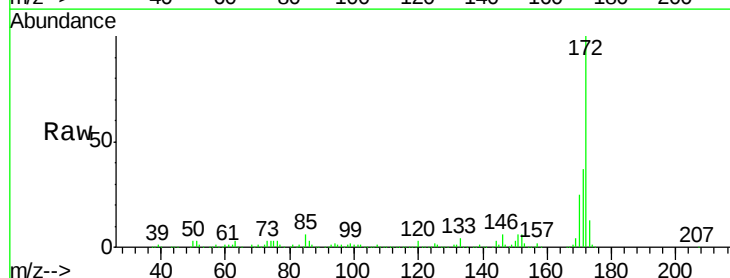



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

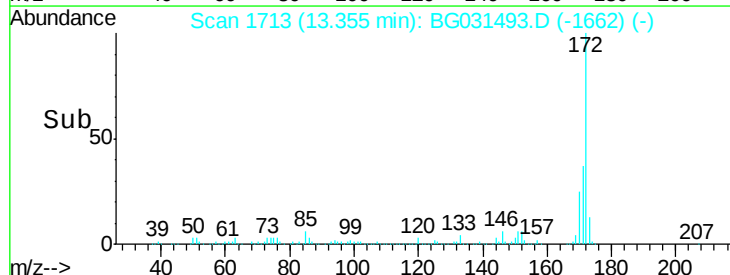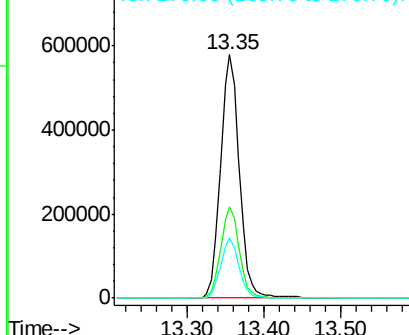

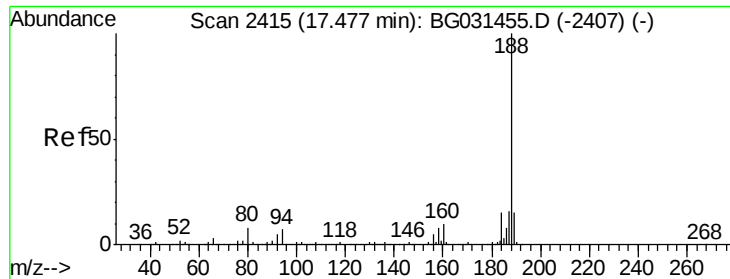

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.47 min Scan# 2414

Delta R.T. -0.00 min

Lab File: BG031493.D

Acq: 12 Dec 2017 15:46

Instrument :

BNA_G

ClientSampleId :

120517-JETT-F-U-B


Tot Ion:188 Resp: 418830

Ion Ratio Lower Upper

188 100

94 6.9 6.9 10.3




80 7.8 7.7 11.5

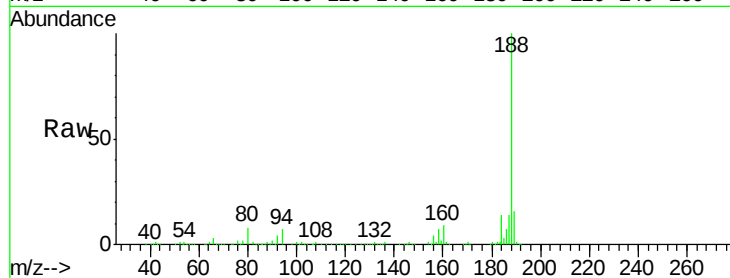

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

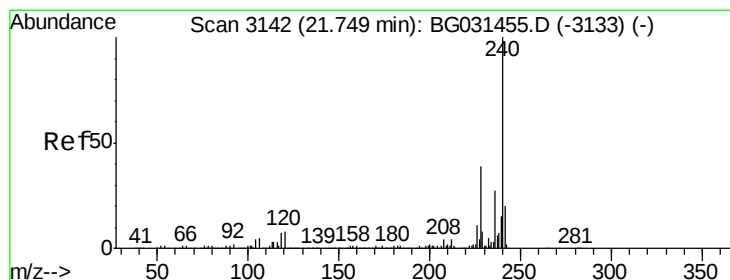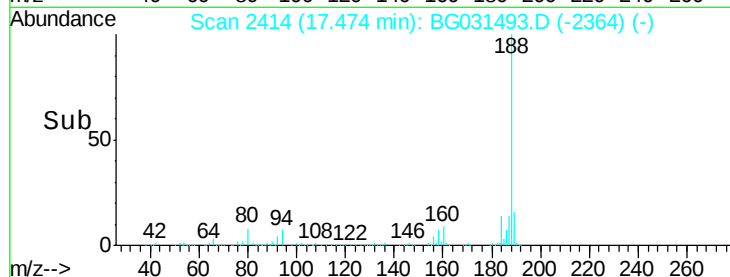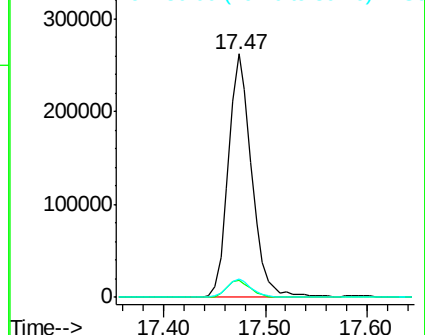

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.75 min Scan# 3141

Delta R.T. -0.00 min

Lab File: BG031493.D

Acq: 12 Dec 2017 15:46


Tgt Ion:240 Resp: 494591

Ion Ratio Lower Upper

240 100

120 7.9 6.8 10.2



236 27.0 20.9 31.3

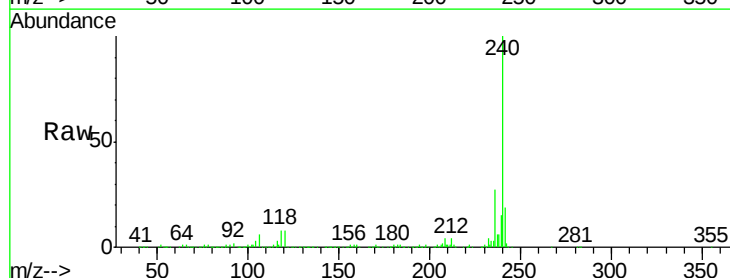


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

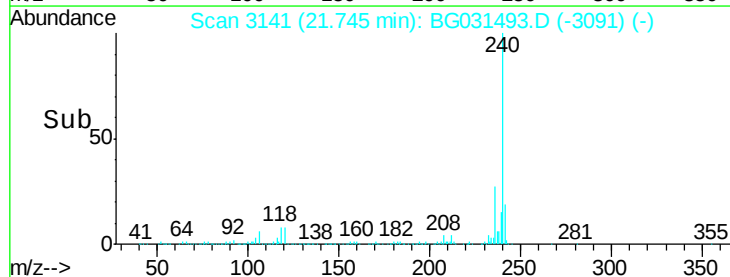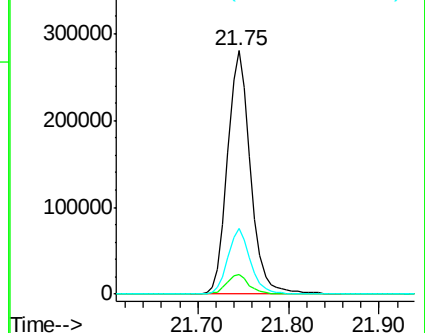

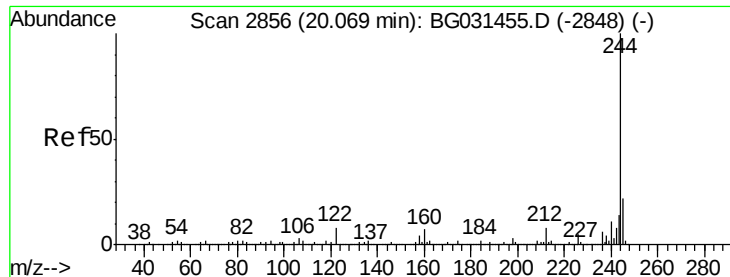

#78

Terphenyl-d14

Concen: 84.412 ng

RT: 20.06 min Scan# 2855

Delta R.T. -0.00 min

Lab File: BG031493.D

Acq: 12 Dec 2017 15:46

Instrument :

BNA_G

ClientSampleId :

120517-JETT-F-U-B


Tot Ion:244 Resp: 1835005

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8




122 9.1 7.0 10.4

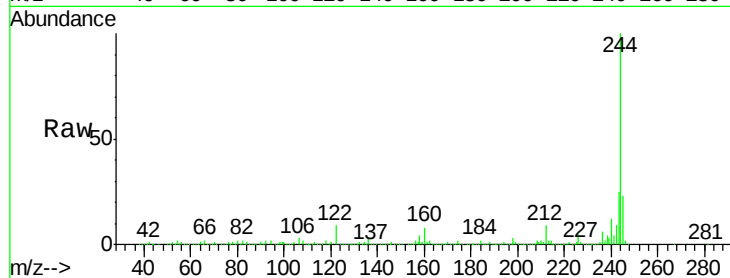

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

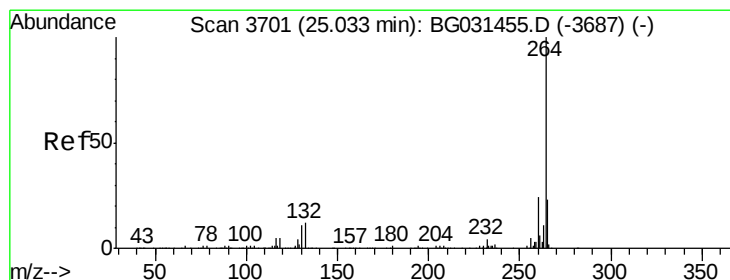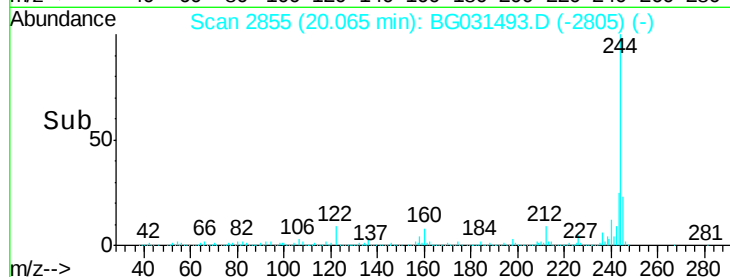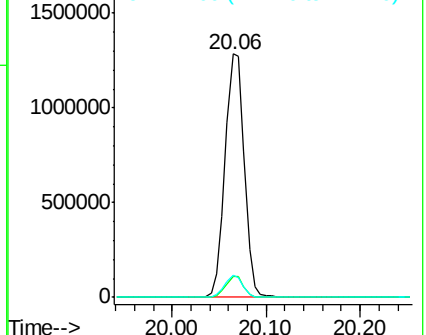

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.03 min Scan# 3700

Delta R.T. -0.00 min

Lab File: BG031493.D

Acq: 12 Dec 2017 15:46


Tgt Ion:264 Resp: 470285

Ion Ratio Lower Upper

264 100

260 24.6 17.4 26.0

265 20.7 17.7 26.5

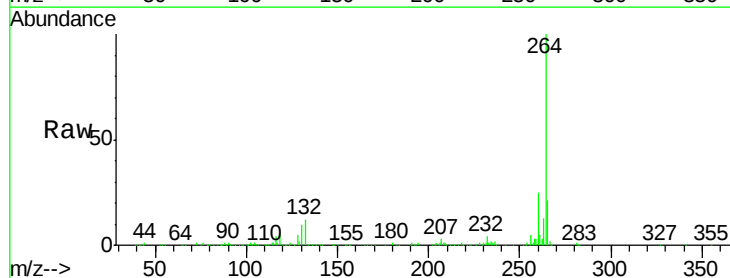

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

