
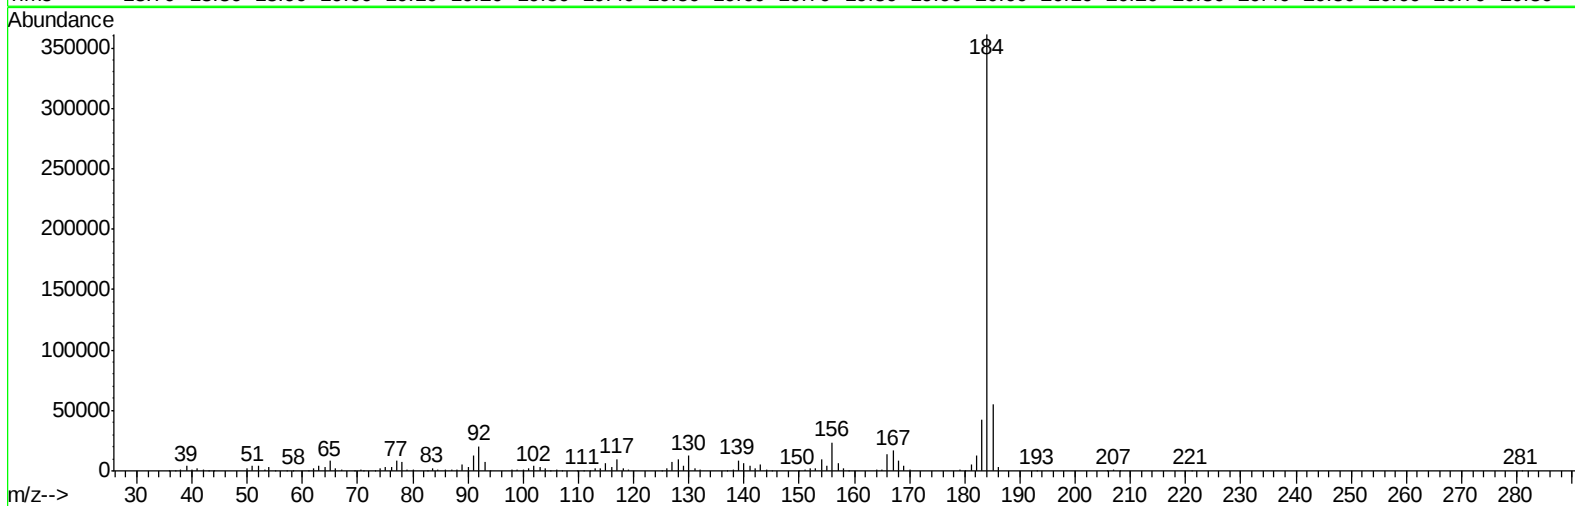


Data Path : Z:\HPCHEM1\BNA G\Data\BG121217\
Data File : BG031485.D
Acq On : 12 Dec 2017 10:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:12:38 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

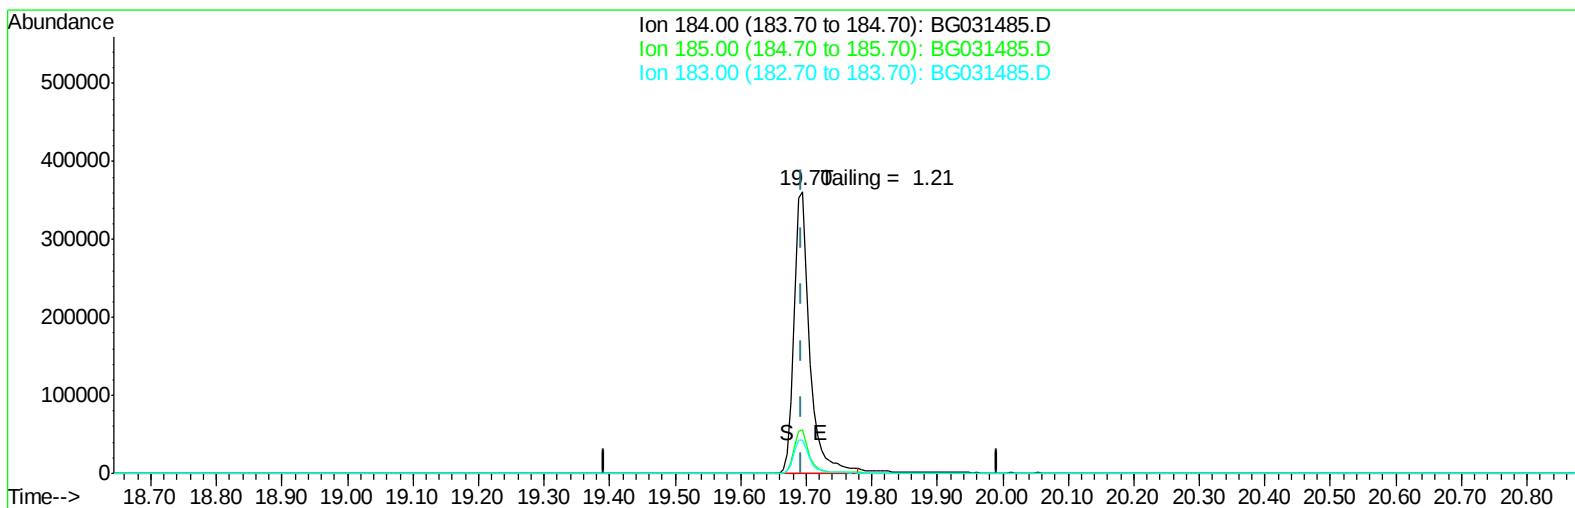

TIC: BG031485.D

(76) Benzidine



19.695min (+0.003) 0.00ng

response 617335

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.31
183.00	13.30	11.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG121217\
Data File : BG031485.D
Acq On : 12 Dec 2017 10:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:12:38 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

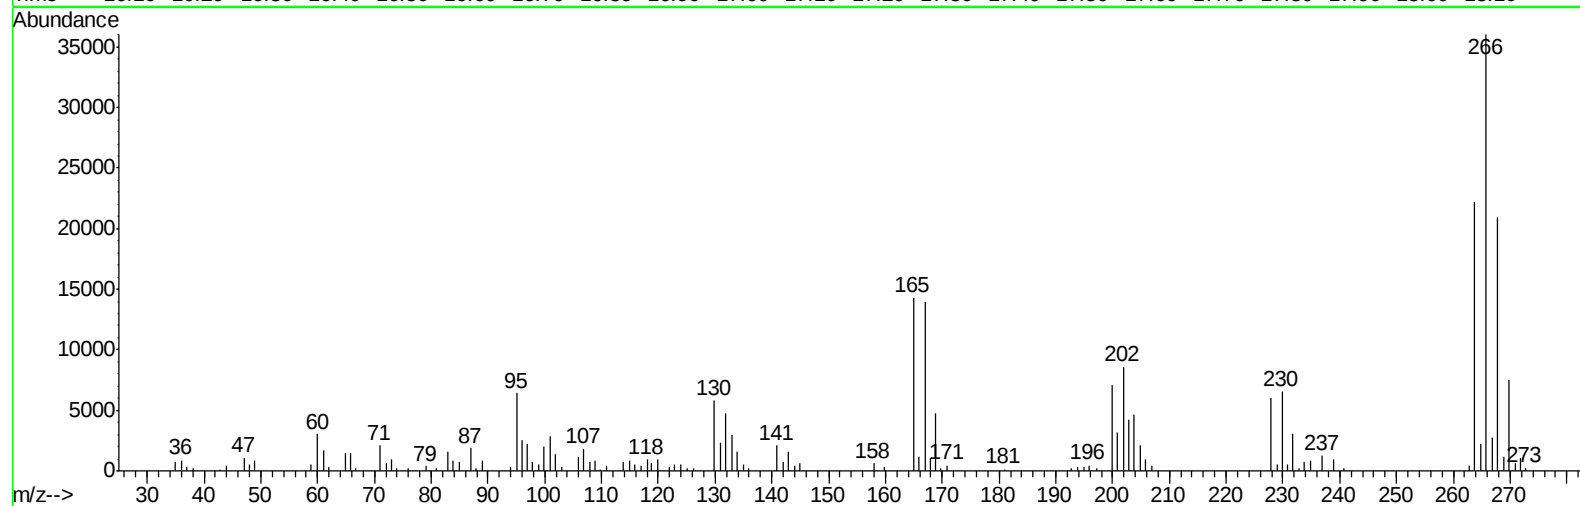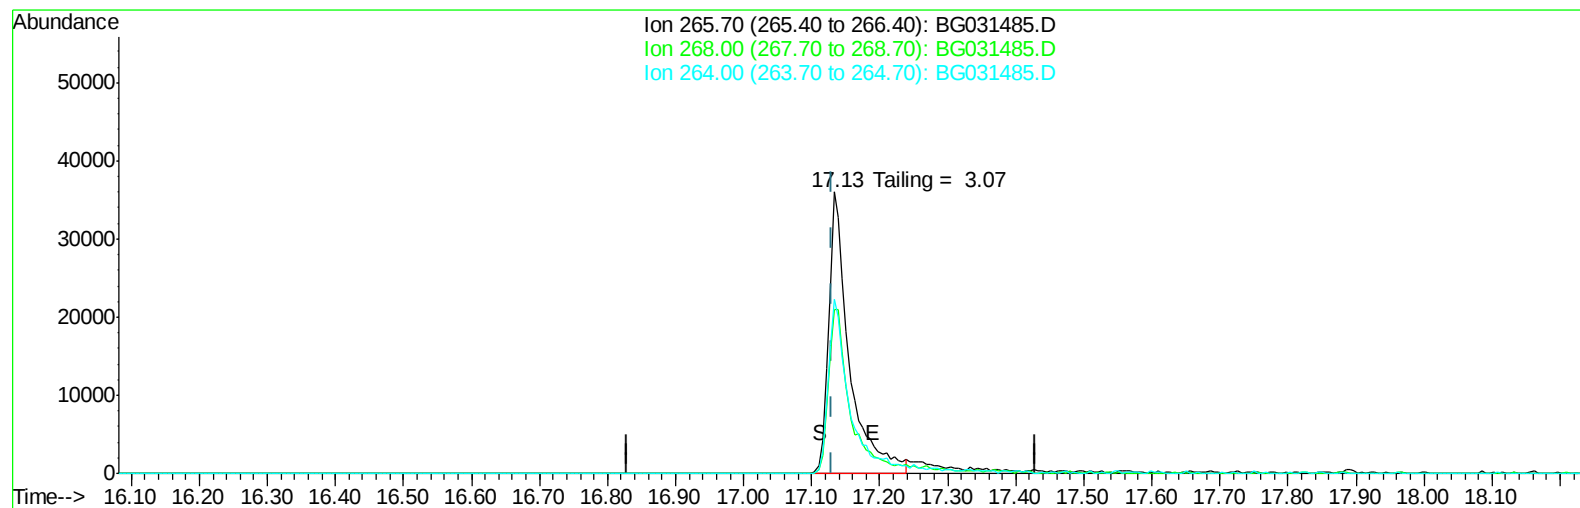

TIC: BG031485.D

(69) Pentachlorophenol (C)

17.133min (+0.003) 0.00ng

response 76153

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.16
264.00	62.00	61.62
0.00	0.00	0.00