
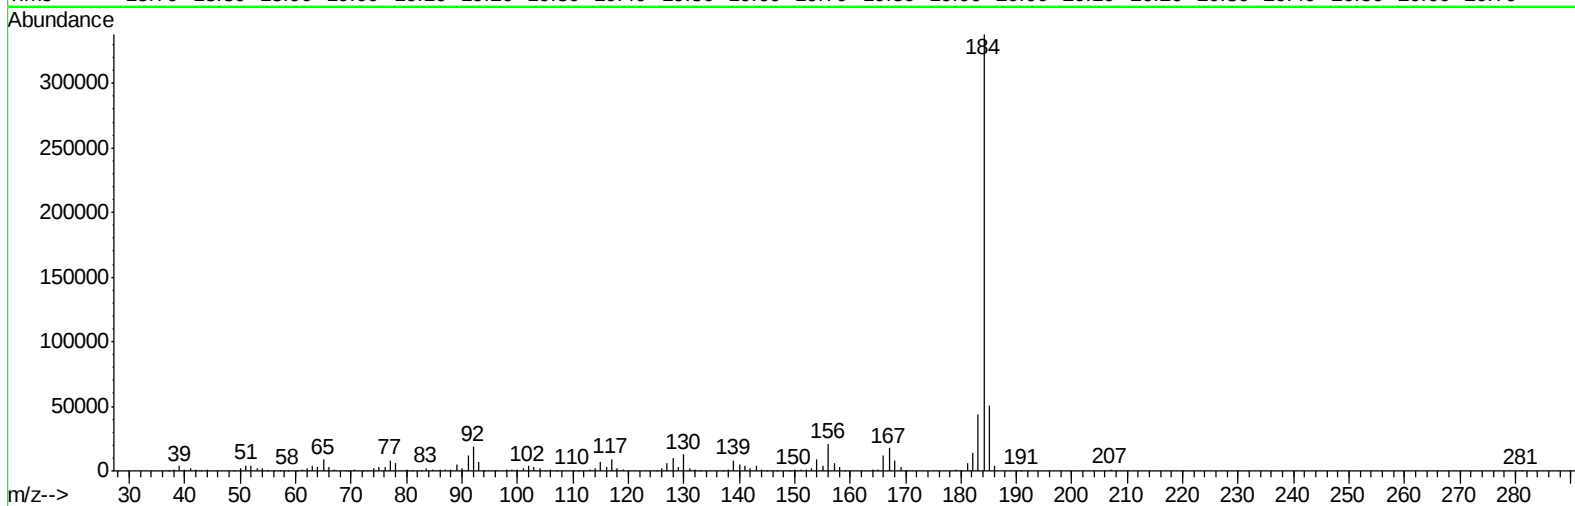


Data Path : Z:\HPCHEM1\BNA G\Data\BG121217\
Data File : BG031502.D
Acq On : 12 Dec 2017 22:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:14:08 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

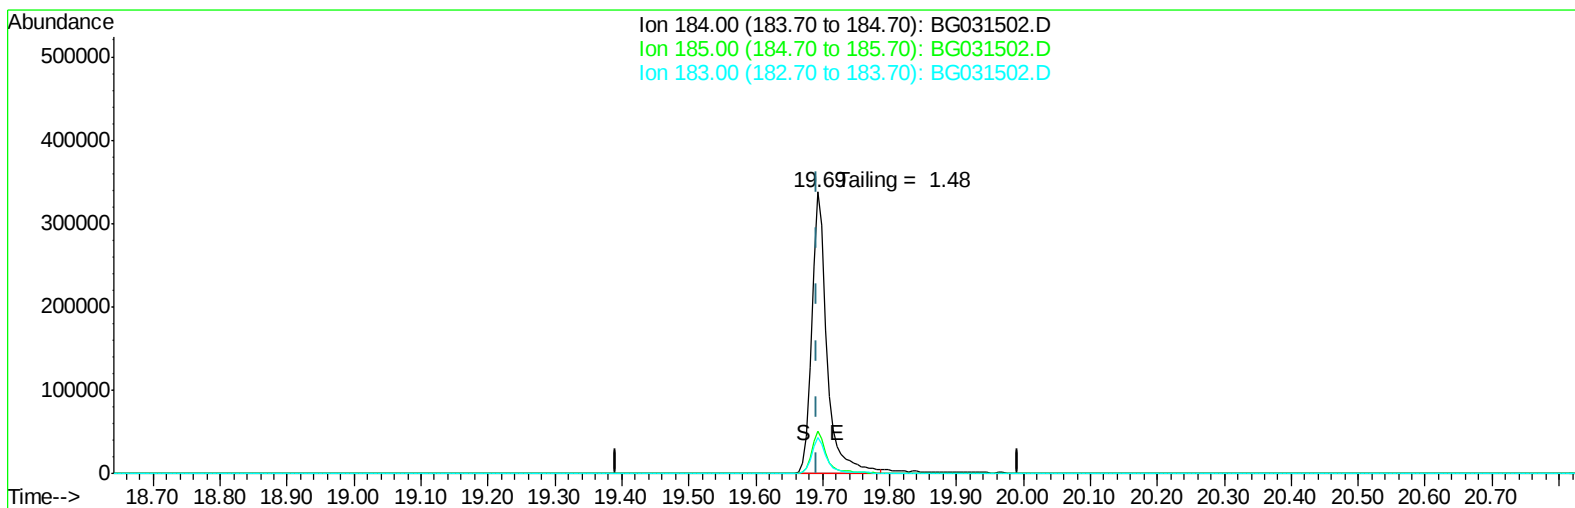

TIC: BG031502.D

(76) Benzidine



19.693min (+0.000) 406821.00ng

response 549116

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.98
183.00	13.30	12.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG121217\
Data File : BG031502.D
Acq On : 12 Dec 2017 22:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:14:08 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

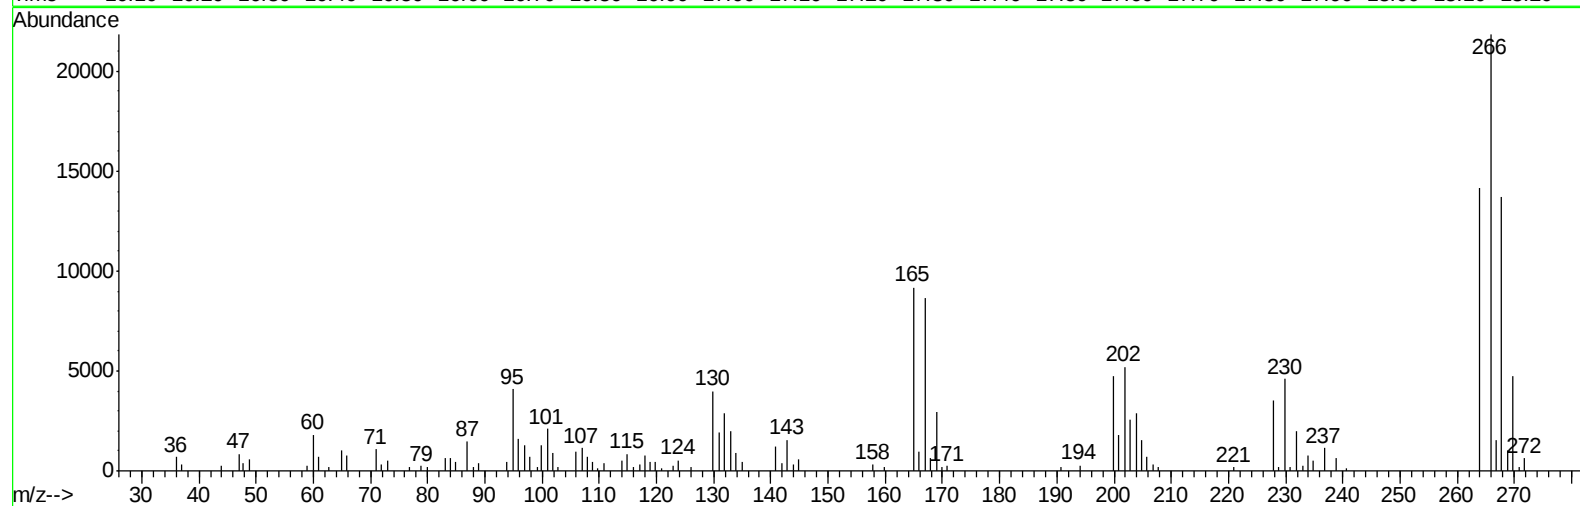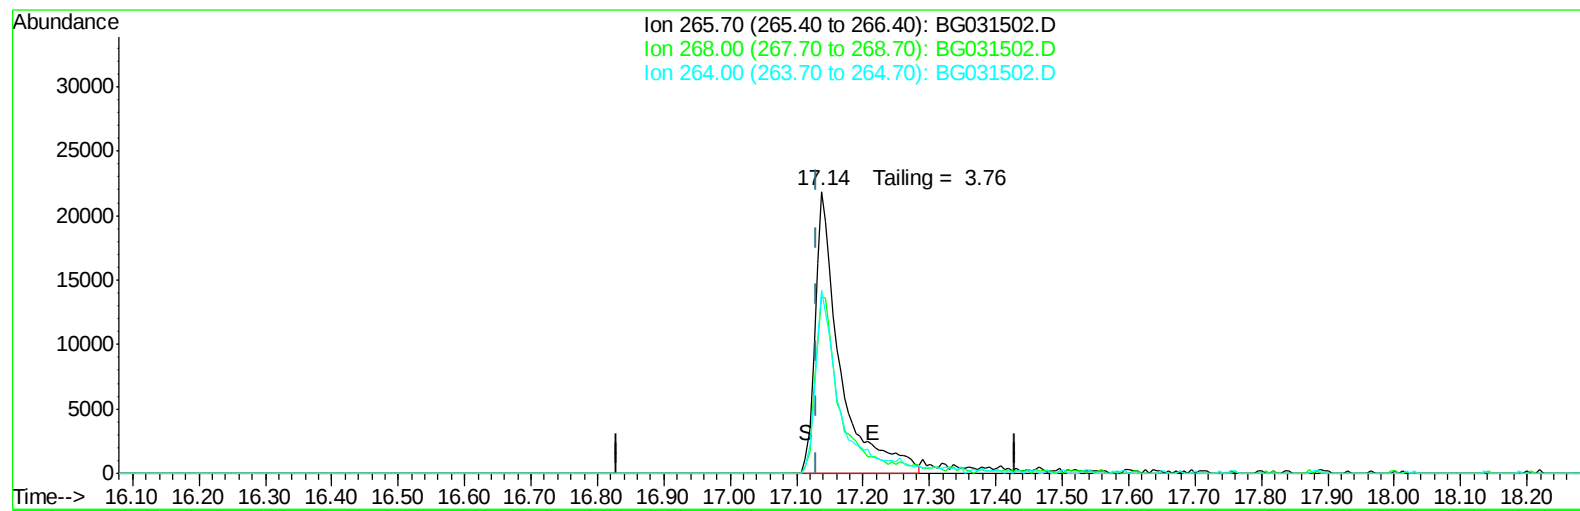

TIC: BG031502.D

(69) Pentachlorophenol (C)

17.137min (+0.007) 0.00ng

response 56993

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.78
264.00	62.00	64.85
0.00	0.00	0.00