

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121217\
 Data File : BG031491.D
 Acq On : 12 Dec 2017 14:30
 Operator : SJ/JU
 Sample : I6763-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 120517-JETT-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.182	317	322	332	rBV	52129	85058	1.61%	0.462%
2	5.670	399	405	417	rBV	265124	483261	9.14%	2.625%
3	7.280	672	679	690	rBV	177355	361534	6.84%	1.964%
4	7.644	734	741	753	rBV	482792	886595	16.77%	4.815%
5	8.108	813	820	829	rBV	173321	311578	5.90%	1.692%
6	8.431	866	875	890	rBV	655620	1218944	23.06%	6.621%
7	9.277	1010	1019	1032	rBV	447244	914294	17.30%	4.966%
8	10.928	1292	1300	1317	rBV	193218	438659	8.30%	2.383%
9	13.355	1706	1713	1725	rBV	1586990	2655242	50.24%	14.422%
10	14.736	1940	1948	1961	rVB2	398407	711090	13.45%	3.862%
11	16.216	2194	2200	2217	rBV	832198	1420198	26.87%	7.714%
12	17.474	2406	2414	2432	rBV	611949	1028688	19.46%	5.587%
13	20.065	2849	2855	2870	rBV	3896211	5285424	100.00%	28.707%
14	21.351	3066	3074	3080	rBV8	33282	78155	1.48%	0.424%
15	21.745	3134	3141	3156	rBV	744603	1299453	24.59%	7.058%
16	25.029	3686	3700	3716	rBV2	390512	1233317	23.33%	6.699%


Sum of corrected areas: 18411490

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121217\
Data File : BG031491.D
Acq On : 12 Dec 2017 14:30
Operator : SJ/JU
Sample : I6763-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120517-JETT-F-D-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

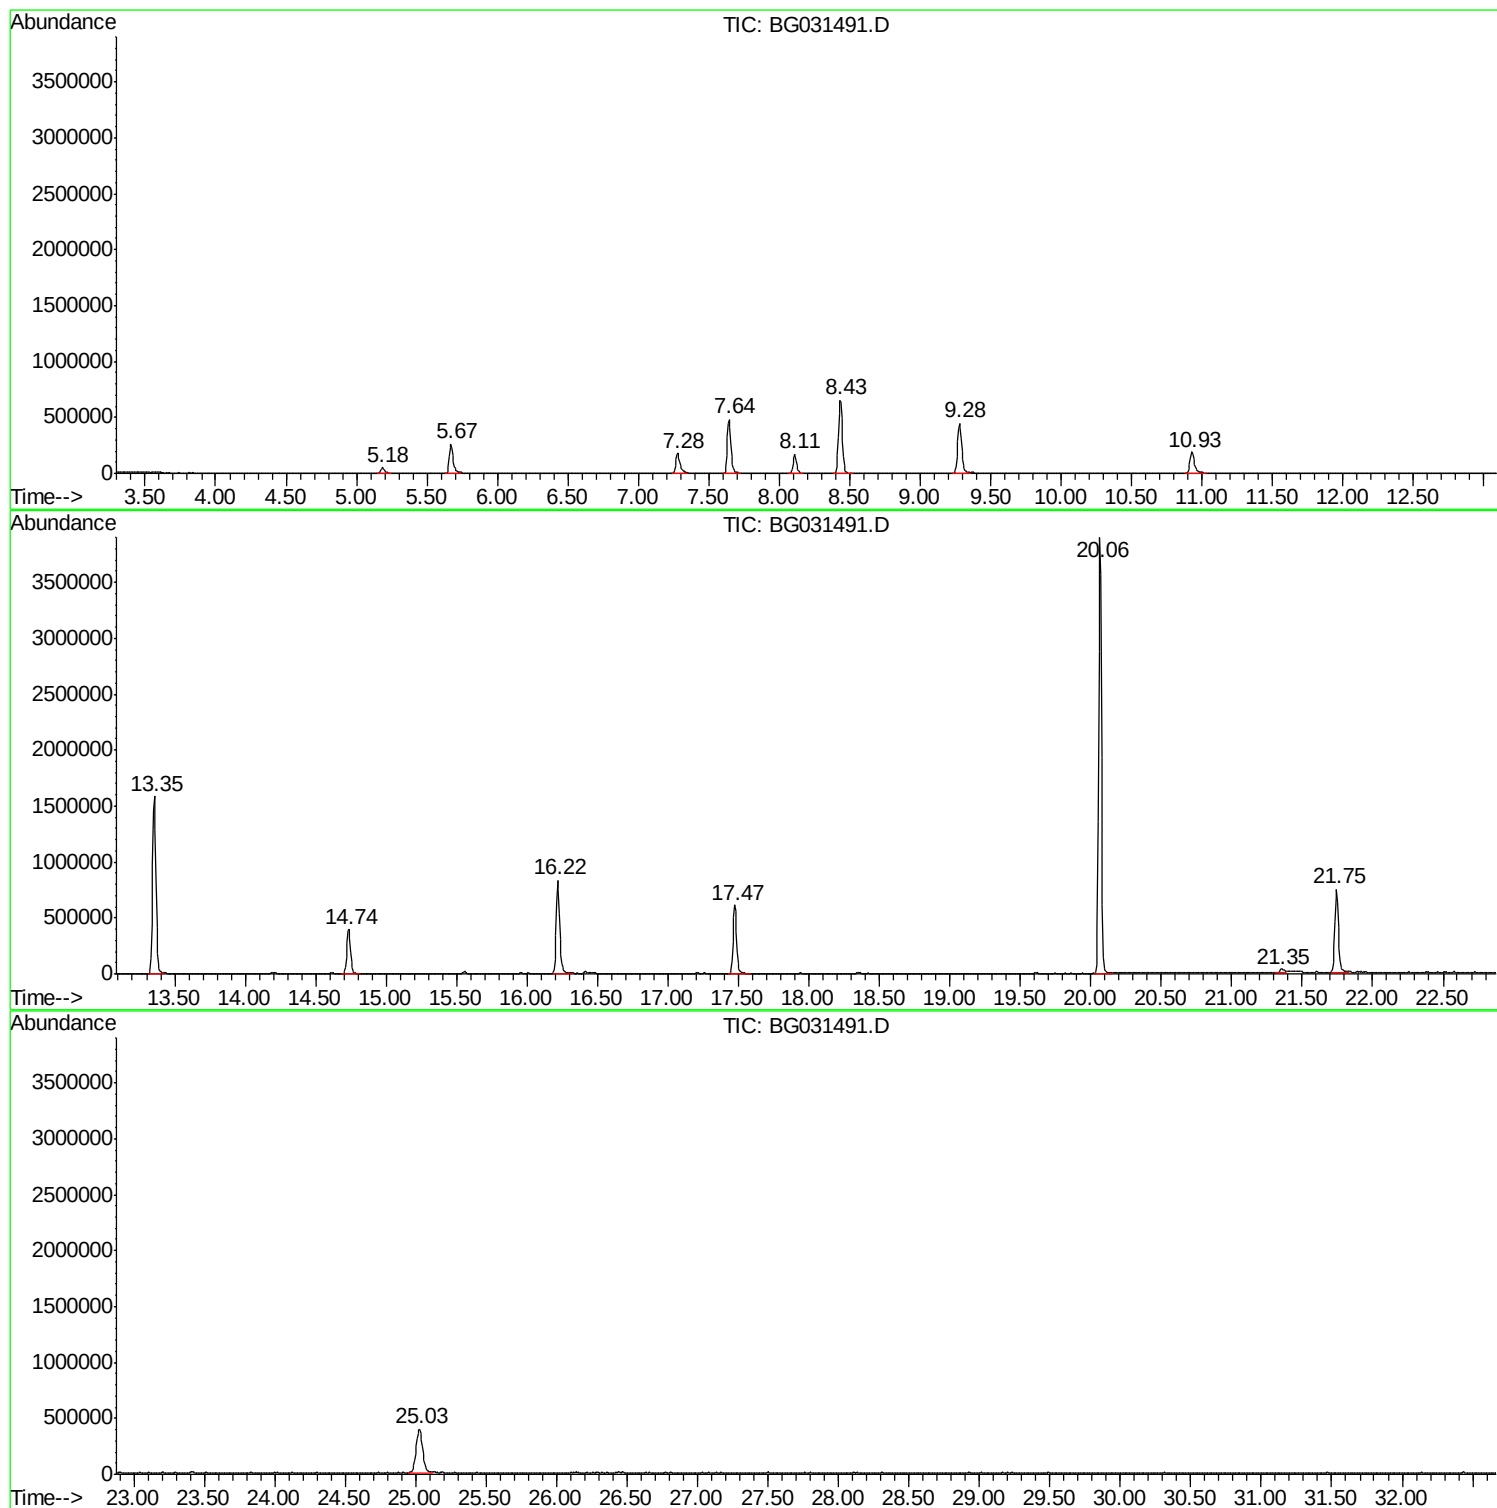

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121217\
Data File : BG031491.D
Acq On : 12 Dec 2017 14:30
Operator : SJ/JU
Sample : I6763-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120517-JETT-F-D-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.18	5.46 ng	85058	1,4-Dichlorobenzene-d4	8.11

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	50
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28
4			3-Hexanol, 4-ethyl-	130	C8H18O	019780-44-0	25
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23

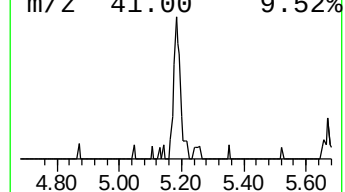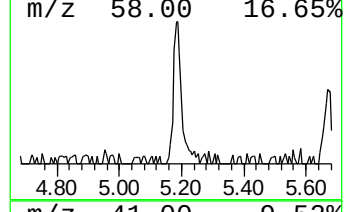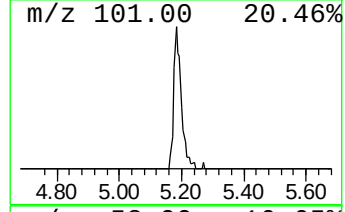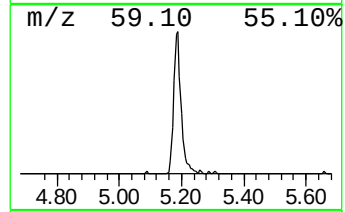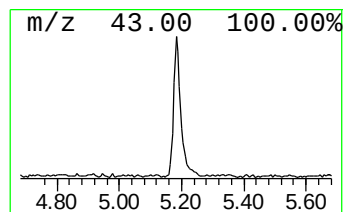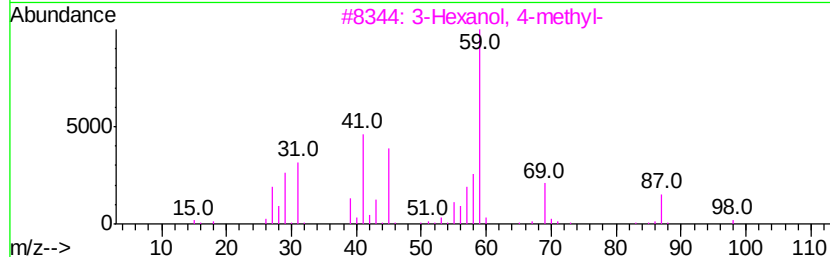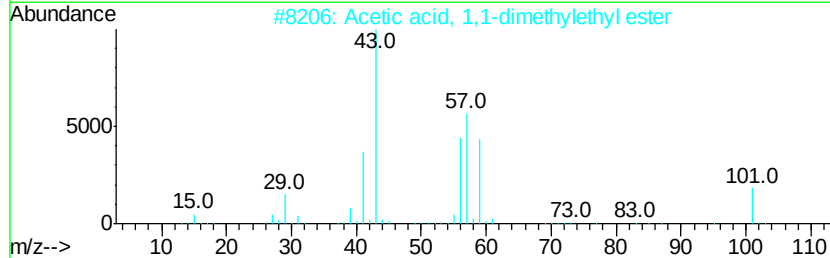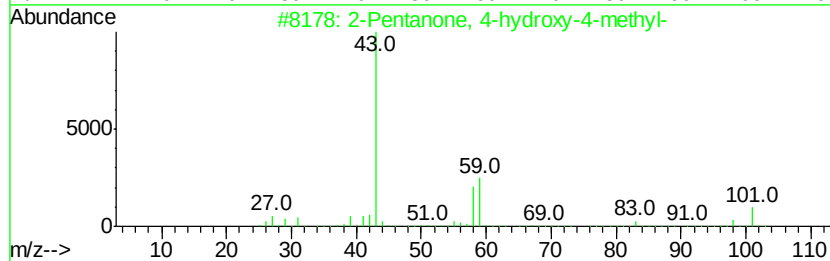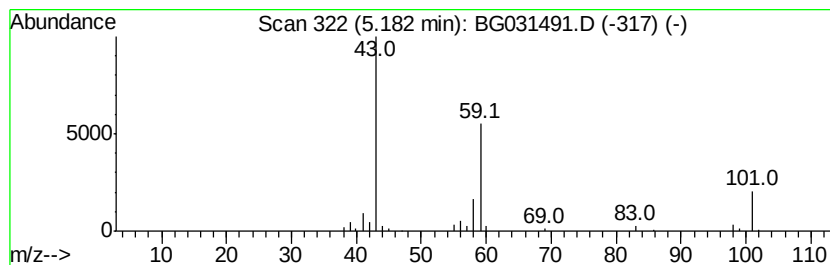

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121217\
Data File : BG031491.D
Acq On : 12 Dec 2017 14:30
Operator : SJ/JU
Sample : I6763-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120517-JETT-F-D-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.64 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.64	56.91 ng	886595	1,4-Dichlorobenzene-d4	8.11

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	23
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

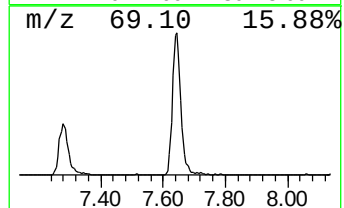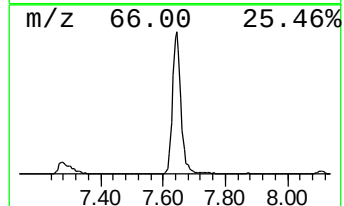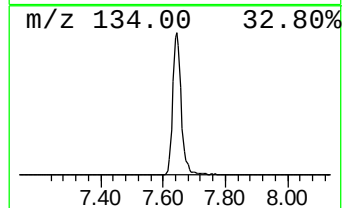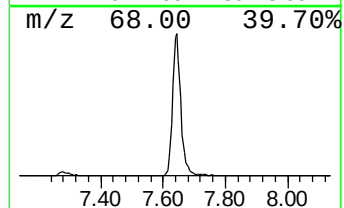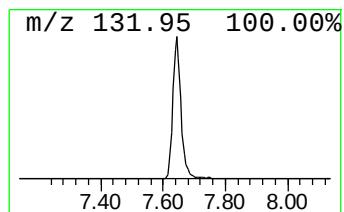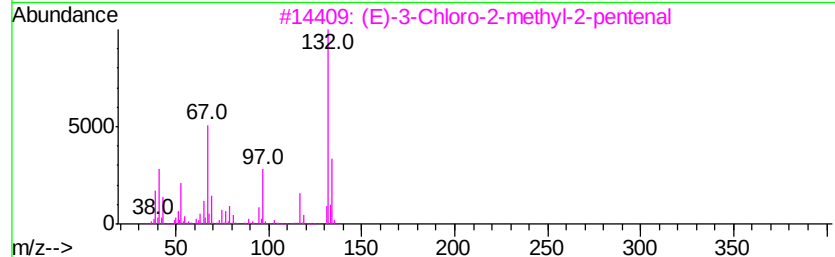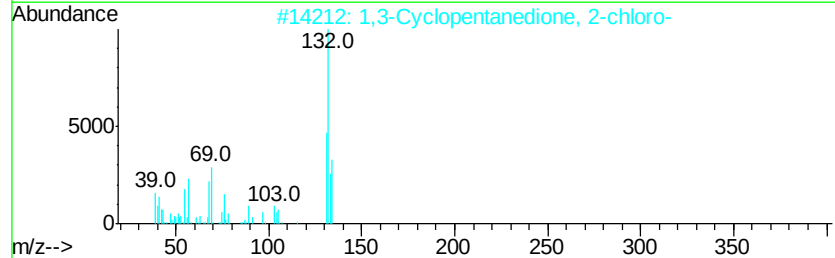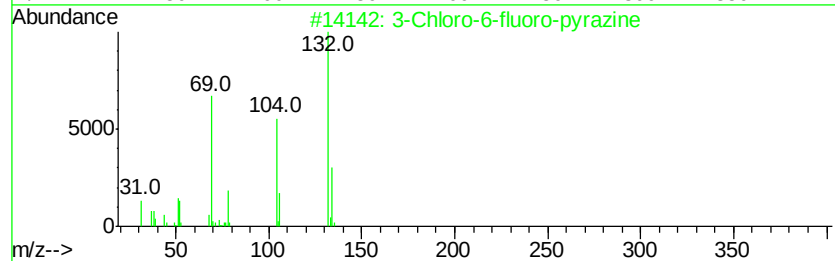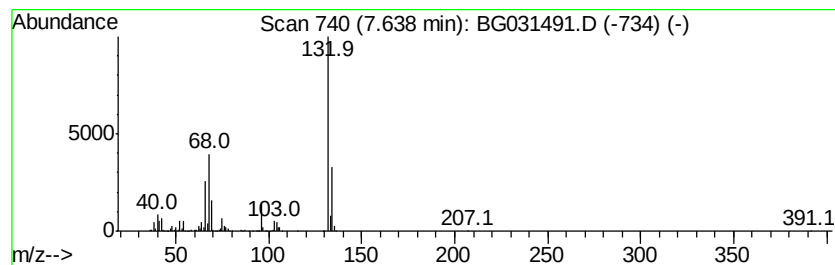

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG121217\
Data File : BG031491.D
Acq On : 12 Dec 2017 14:30
Operator : SJ/JU
Sample : I6763-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120517-JETT-F-D-M

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.18	5.5	ng	85058	1	8.11	311578	20.0
unknown7.64	7.64	56.9	ng	886595	1	8.11	311578	20.0