


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG121217\
 Data File : BG031485.D
 Acq On : 12 Dec 2017 10:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 11 17:25:55 2017

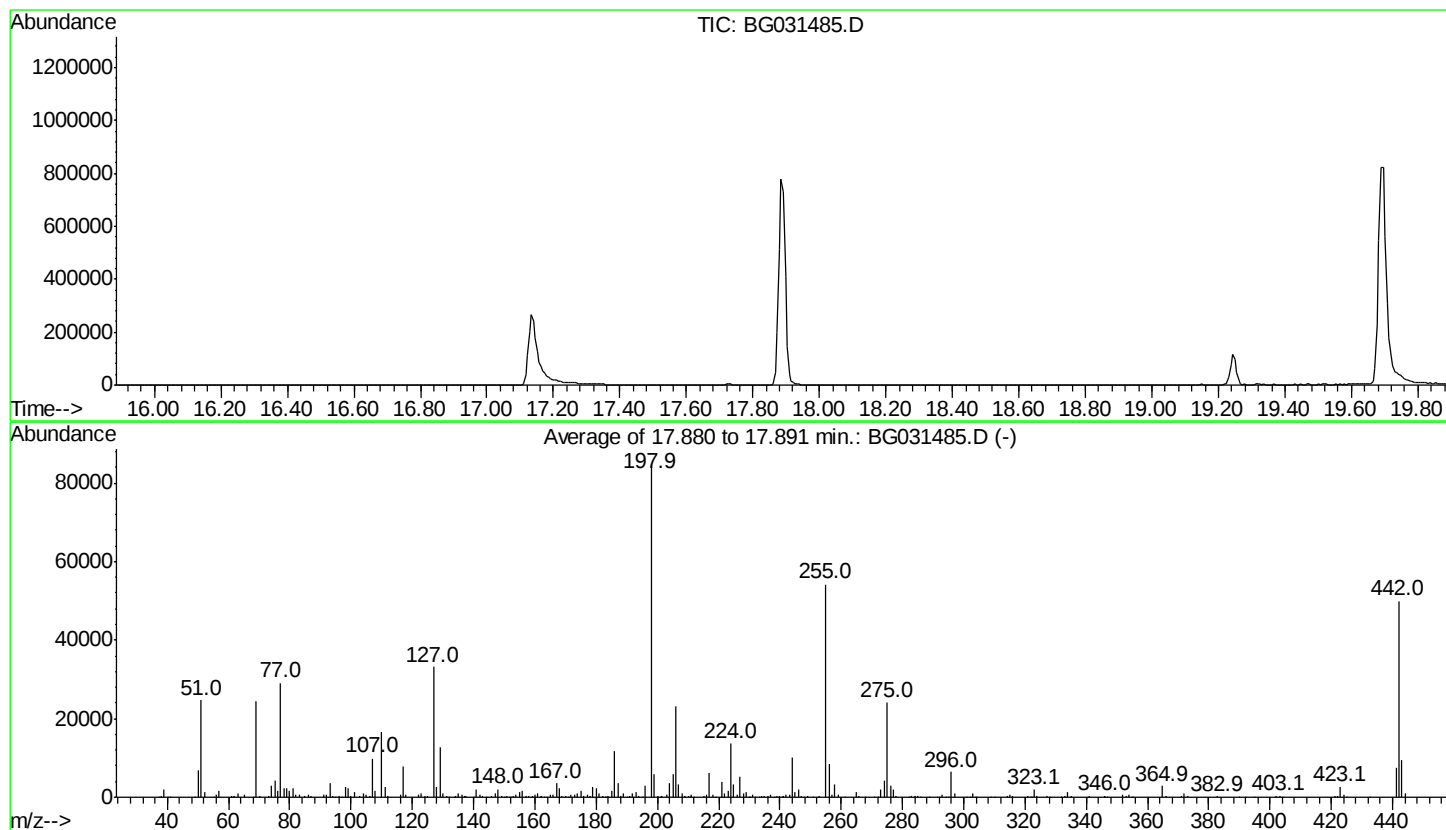

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	24618	PASS
68	69	0.00	2	0.6	137	PASS
69	198	0.00	100	29.0	24482	PASS
70	69	0.00	2	0.7	177	PASS
127	198	10	80	39.3	33157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84413	PASS
199	198	5	9	6.9	5846	PASS
275	198	10	60	28.5	24095	PASS
365	198	1	100	3.3	2825	PASS
441	442	0.01	24	14.8	7416	PASS
442	198	50	100	59.2	49946	PASS
443	442	15	24	19.1	9544	PASS