
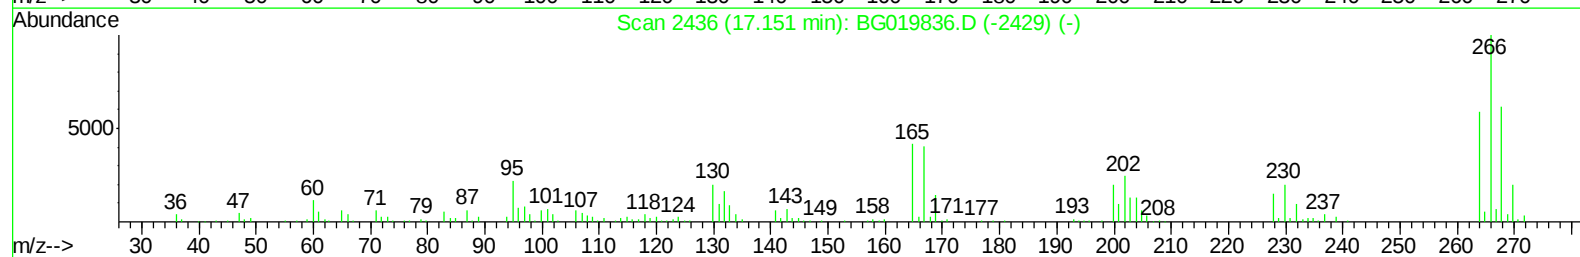
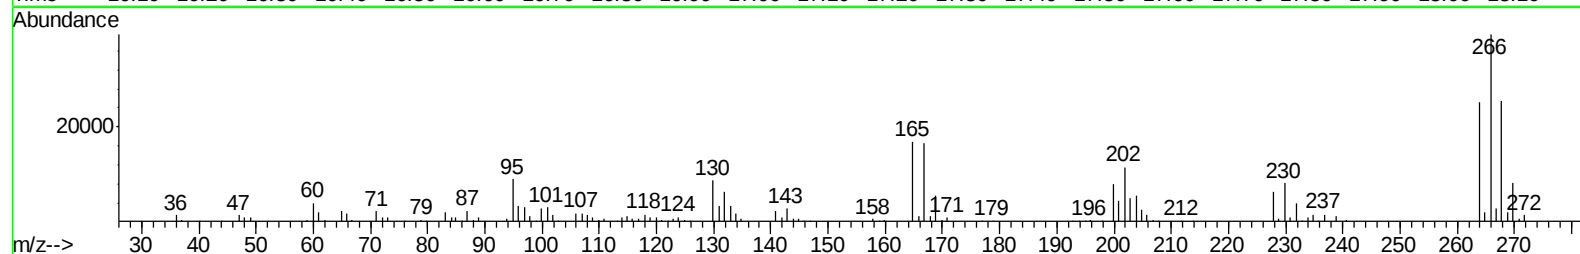


Data Path : Z:\HPCHEM1\BNA_G\Data\BG121315\
Data File : BG020136.D
Acq On : 13 Dec 2015 8:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:17:11 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

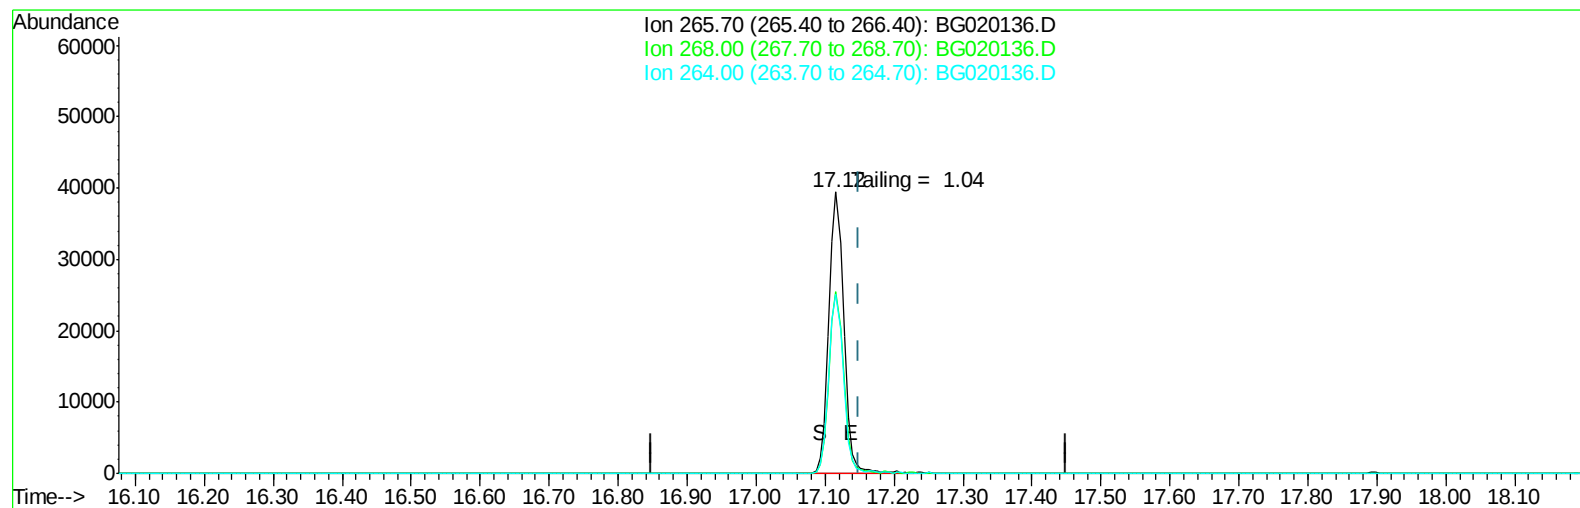

TIC: BG020136.D

(69) Pentachlorophenol (C)




17.116min (-0.034) 0.00ng

response 58885

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	64.74
264.00	60.10	63.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG121315\
 Data File : BG020136.D
 Acq On : 13 Dec 2015 8:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 08:17:11 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

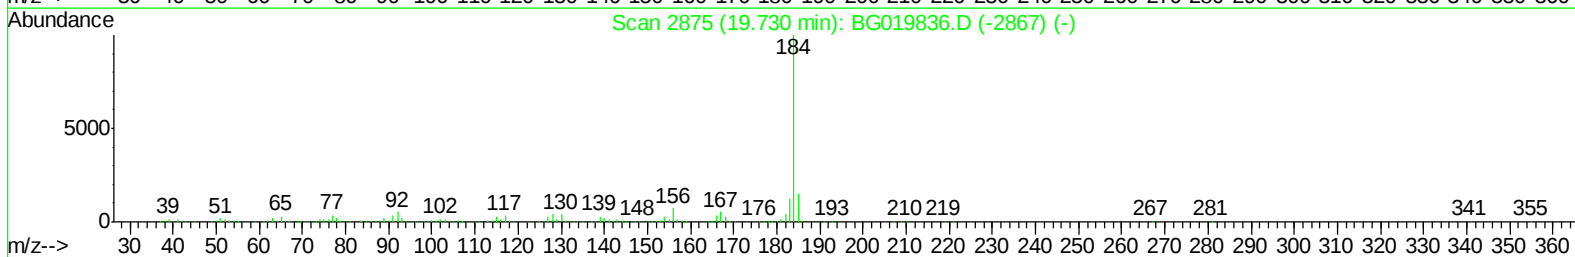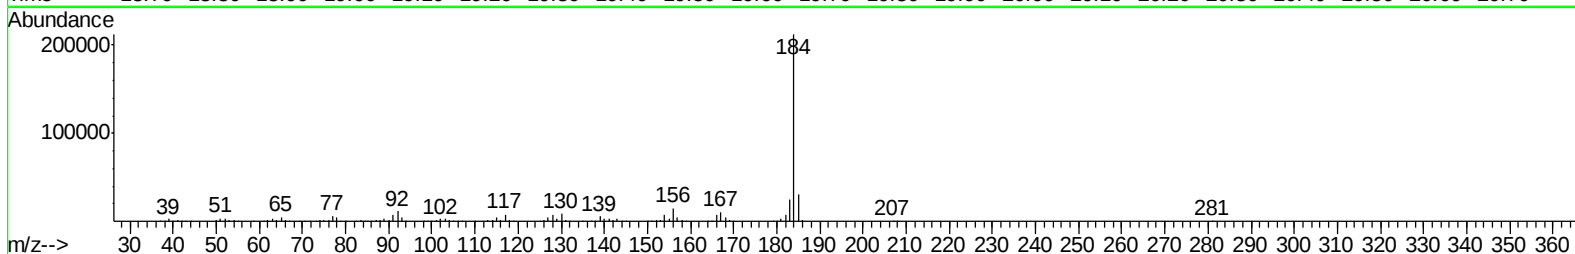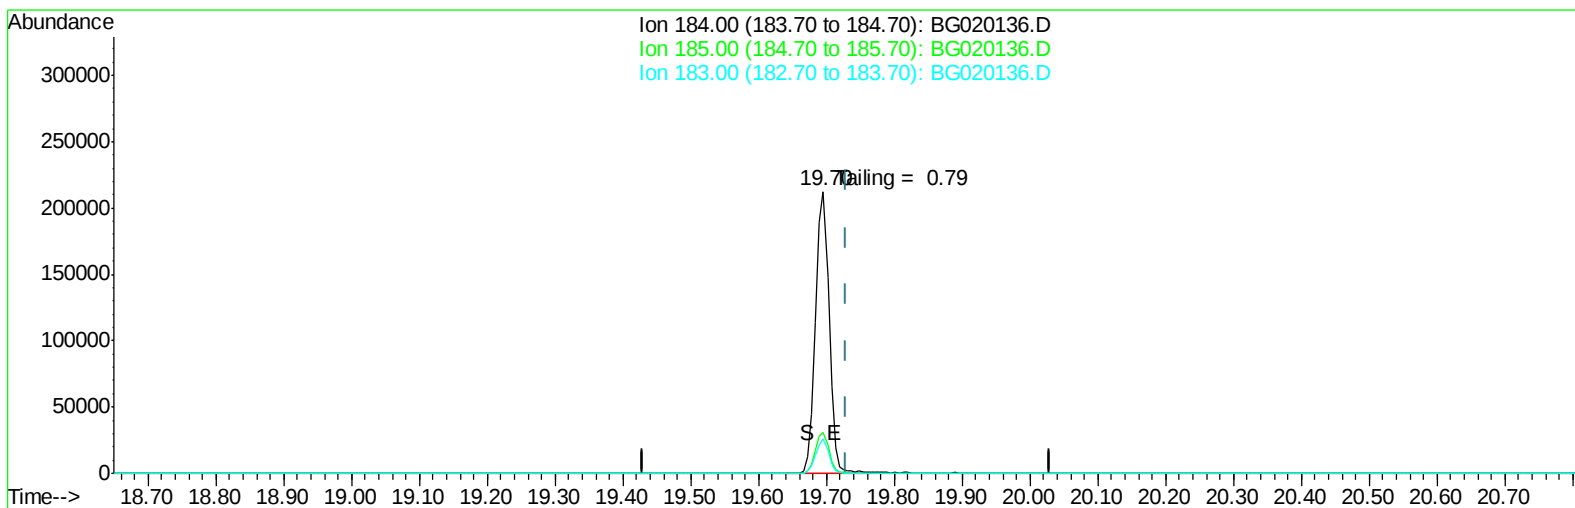

TIC: BG020136.D

(76) Benzidine

19.695min (-0.035) 1096.20ng

response 292202

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.61
183.00	12.60	12.07
0.00	0.00	0.00