
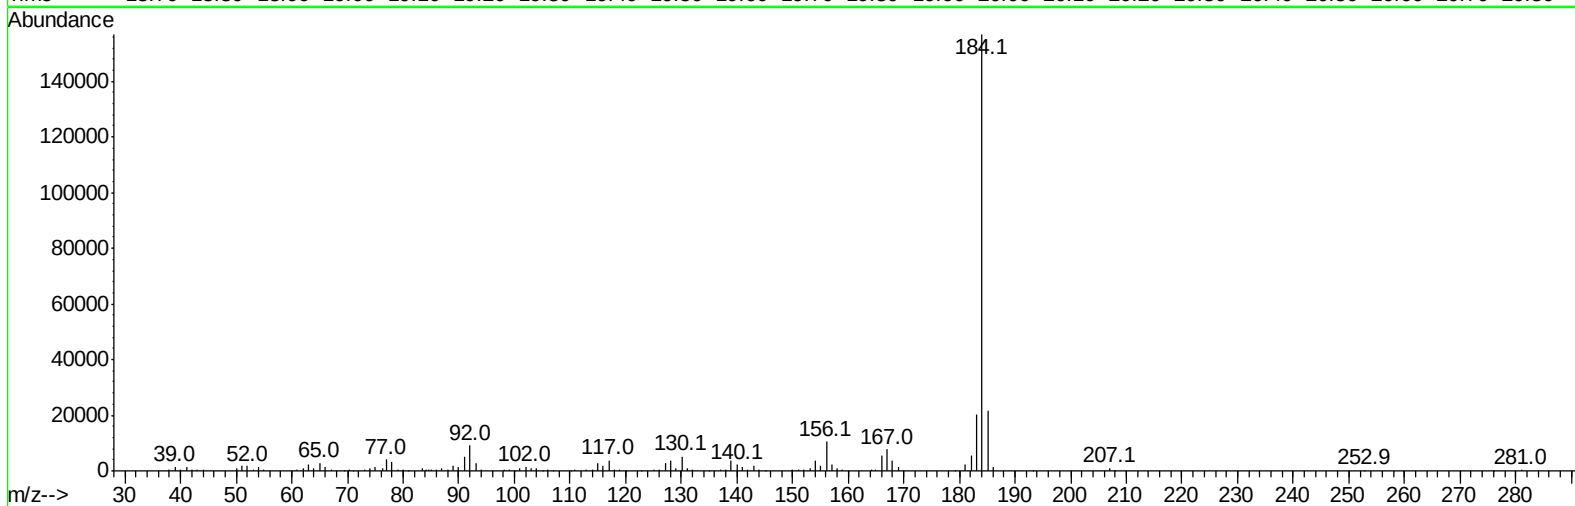


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121317\
Data File : BG031540.D
Acq On : 13 Dec 2017 22:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 04:21:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

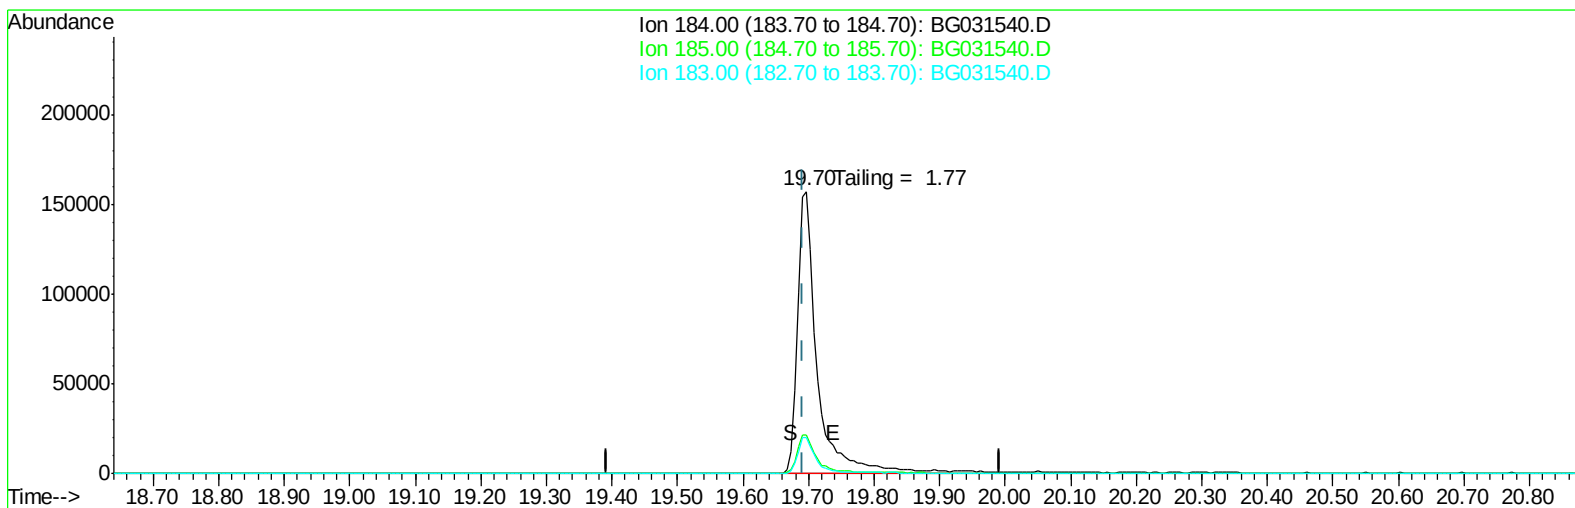

TIC: BG031540.D

(76) Benzidine



19.697min (+0.005) 190578.01ng m

response 328199

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.74
183.00	13.30	12.83
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121317\
Data File : BG031540.D
Acq On : 13 Dec 2017 22:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 04:21:33 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

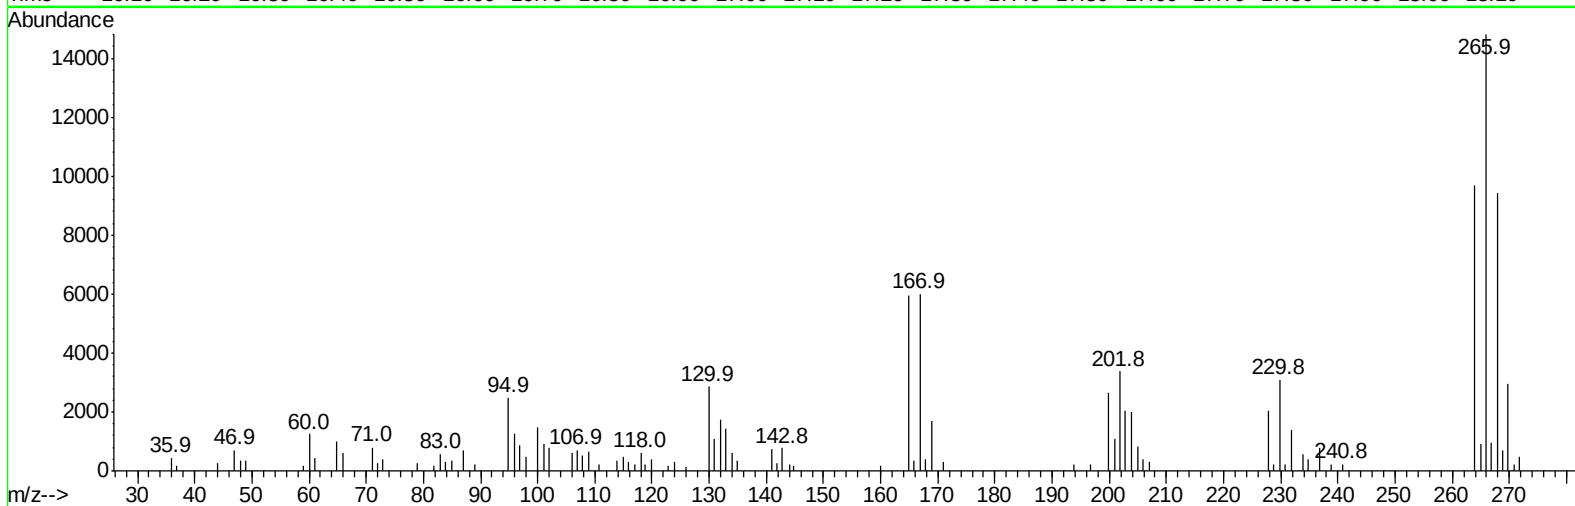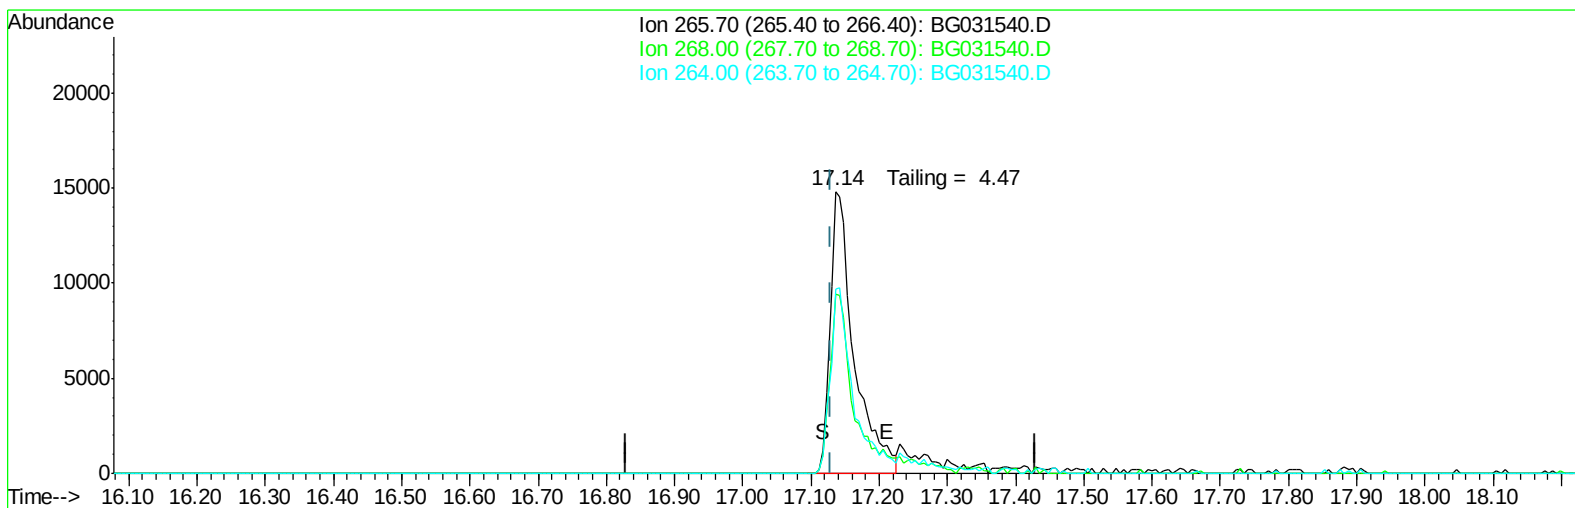

TIC: BG031540.D

(69) Pentachlorophenol (C)

17.136min (+0.006) 0.00ng

response 35977

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.62
264.00	62.00	65.36
0.00	0.00	0.00