

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121317\
 Data File : BG031555.D
 Acq On : 14 Dec 2017 8:15
 Operator : SJ/JU
 Sample : I6817-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 120617-FOPI-F-D-B

Quant Time: Dec 14 09:55:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 17:25:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	48051	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	200826	20.00	ng	0.00
38) Acenaphthene-d10	14.73	164	153079	20.00	ng	0.00
63) Phenanthrene-d10	17.47	188	472435	20.00	ng	0.00
75) Chrysene-d12	21.74	240	566174	20.00	ng	0.00
86) Perylene-d12	25.03	264	544167	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	113515	41.87	ng	0.00
7) Phenol-d6	7.28	99	92431	24.56	ng	0.01
23) Nitrobenzene-d5	9.28	82	287179	88.14	ng	0.00
41) 2,4,6-Tribromophenol	16.22	330	193913	108.13	ng	0.00
44) 2-Fluorobiphenyl	13.35	172	949854	91.08	ng	0.00
78) Terphenyl-d14	20.07	244	1910703	76.78	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121317\
Data File : BG031555.D
Acq On : 14 Dec 2017 8:15
Operator : SJ/JU
Sample : I6817-11
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
120617-FOPI-F-D-B

Quant Time: Dec 14 09:55:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

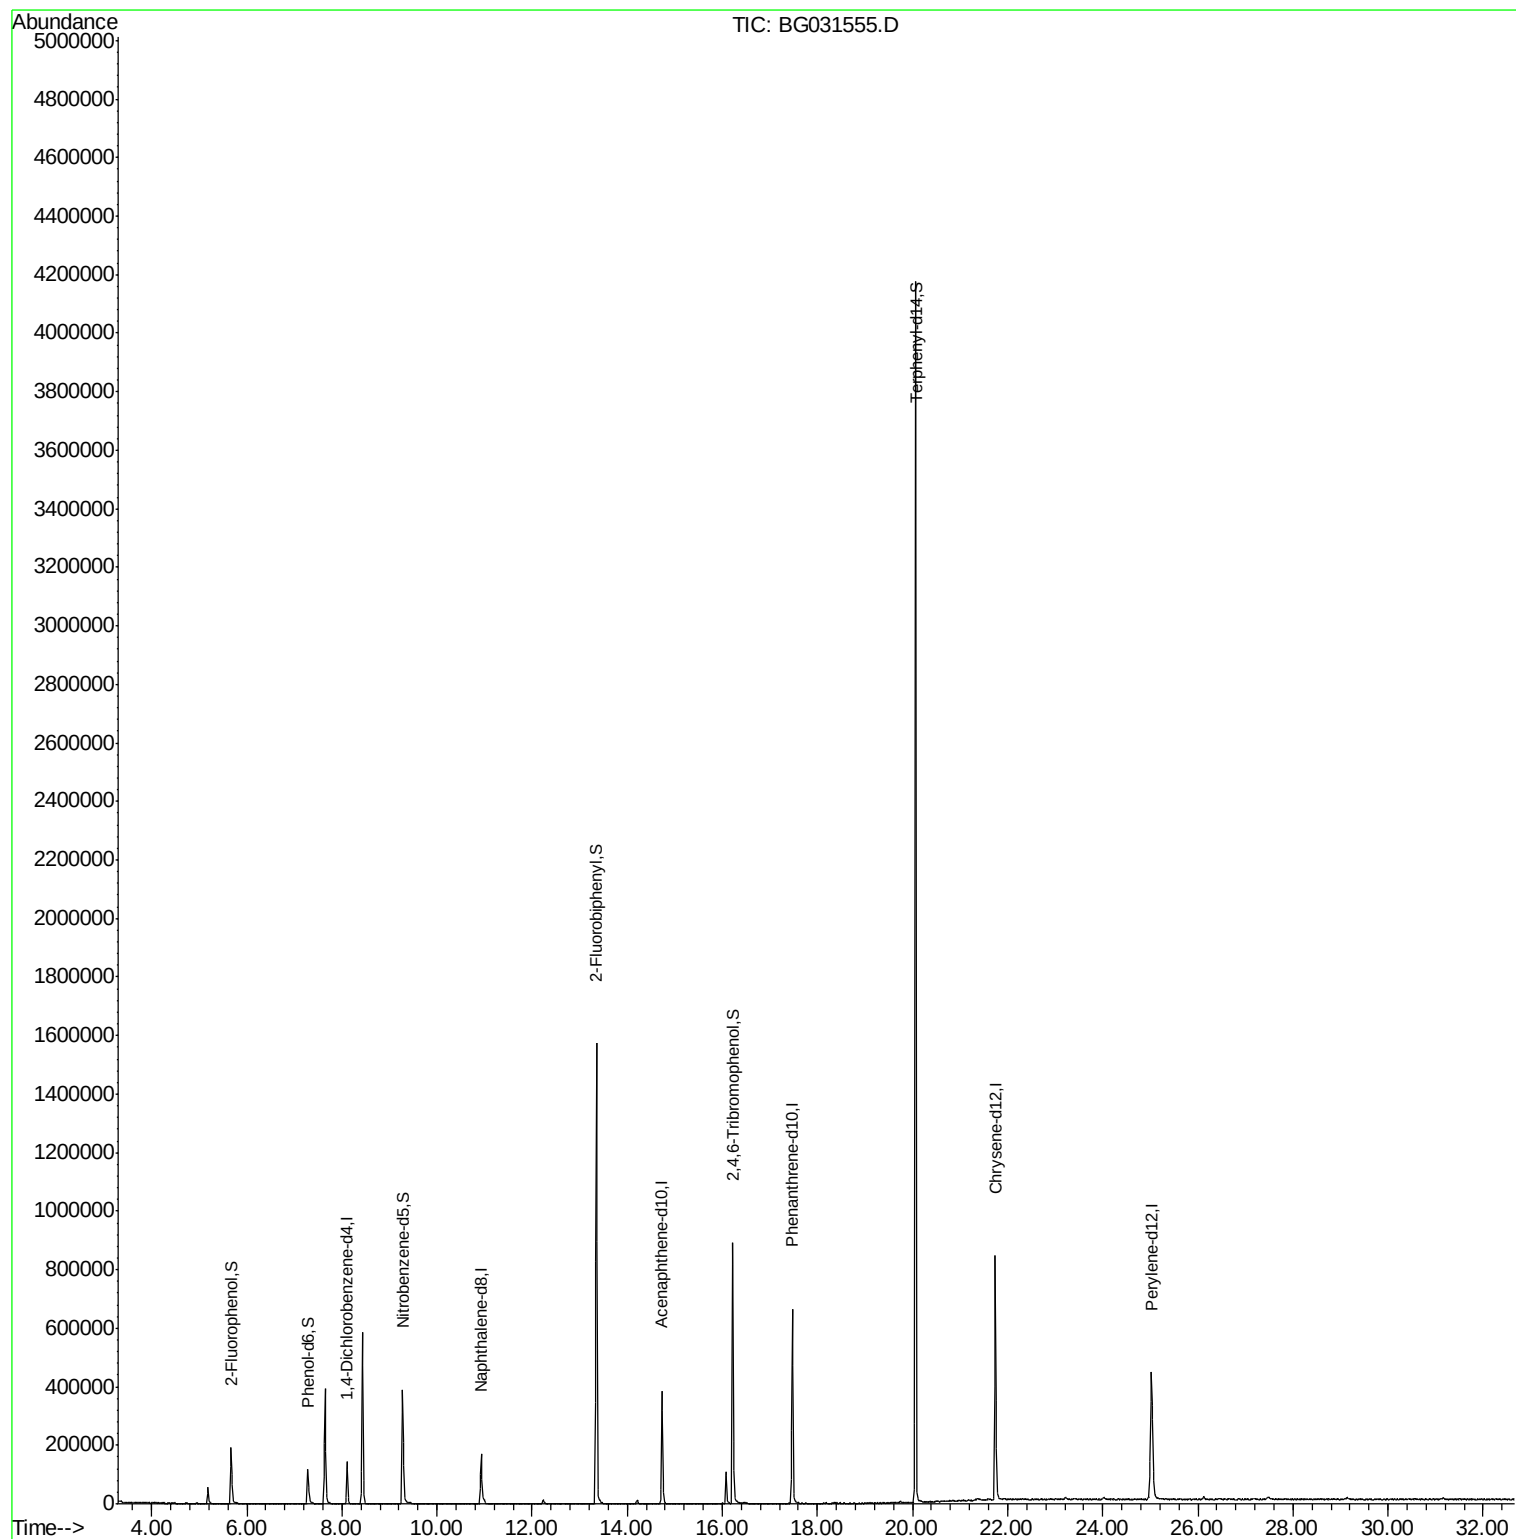




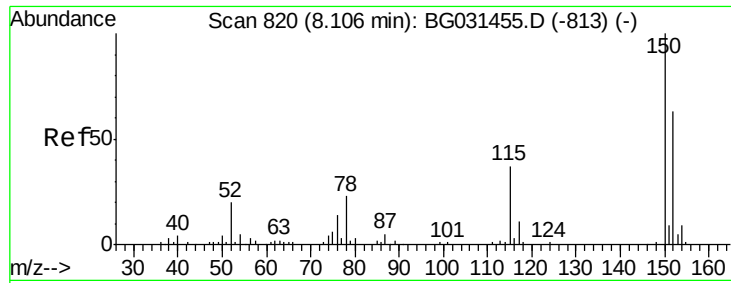


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.11 min Scan# 821
 Delta R.T. 0.00 min
 Lab File: BG031555.D
 Acq: 14 Dec 2017 8:15

Instrument :
 BNA_G
 ClientSampleId :
 120617-FOPI-F-D-B




Tot Ion:152 Resp: 48051
 Ion Ratio Lower Upper
 152 100
 150 158.1 126.6 189.8
 115 52.9 53.0 79.4#

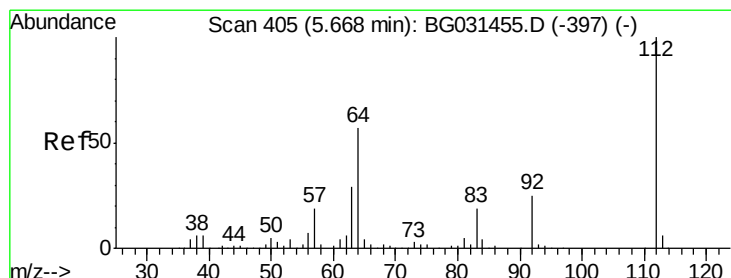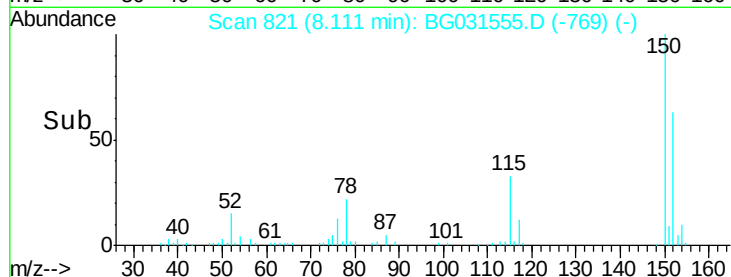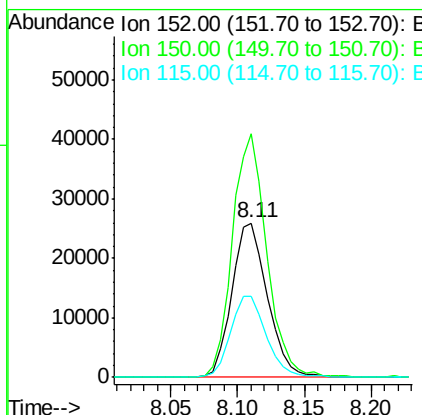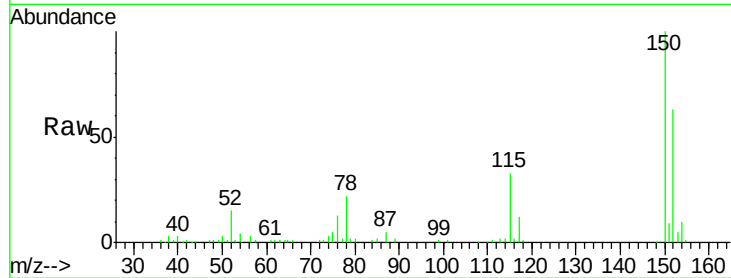


#5

2-Fluorophenol
 Concen: 41.874 ng
 RT: 5.67 min Scan# 406
 Delta R.T. 0.01 min
 Lab File: BG031555.D
 Acq: 14 Dec 2017 8:15

Tgt Ion:112 Resp: 113515
 Ion Ratio Lower Upper
 112 100
 64 54.2 56.3 84.5#
 63 27.8 30.1 45.1#

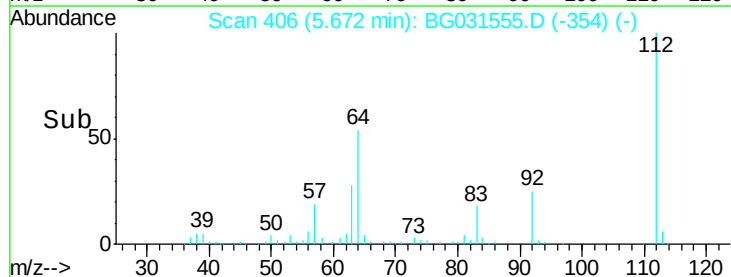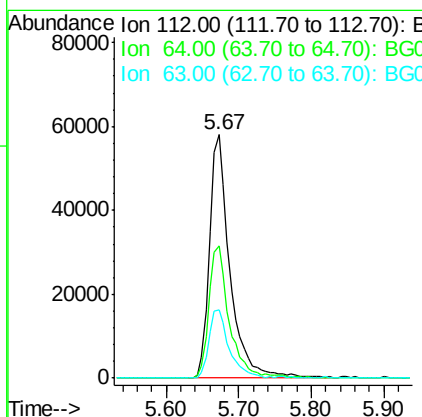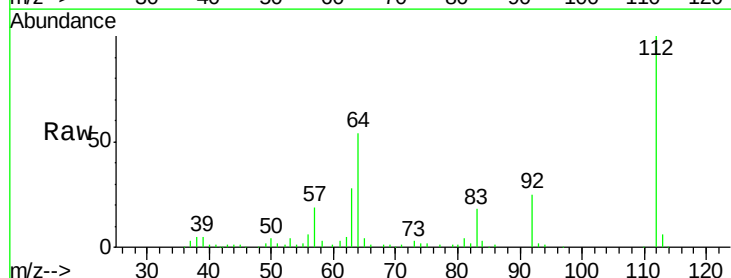

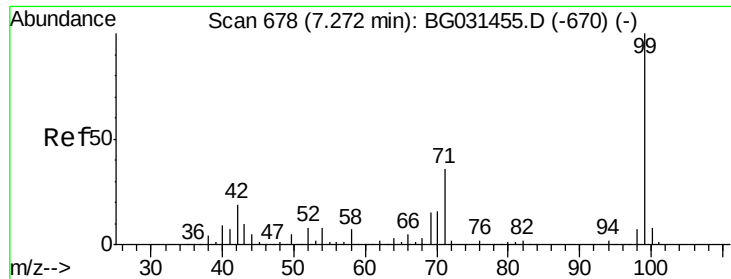

#7

Phenol-d6

Concen: 24.561 ng

RT: 7.28 min Scan# 680

Delta R.T. 0.01 min

Lab File: BG031555.D

Acq: 14 Dec 2017 8:15

Instrument :

BNA_G

ClientSampleId :

120617-FOPI-F-D-B


Tot Ion: 99 Resp: 92431

Ion Ratio Lower Upper




99 100

42 16.3 14.1 21.1

71 31.3 26.1 39.1

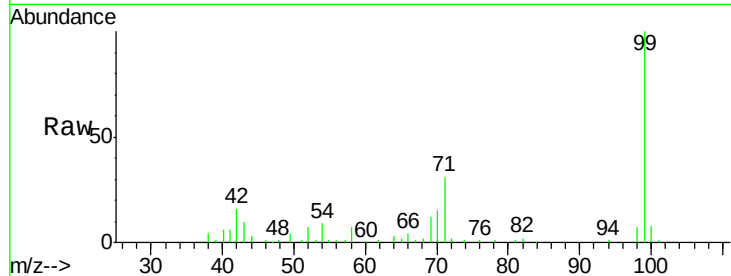

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

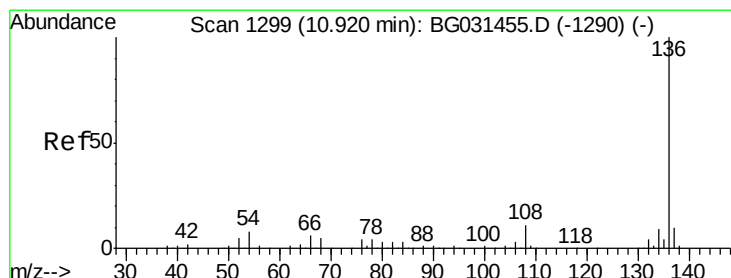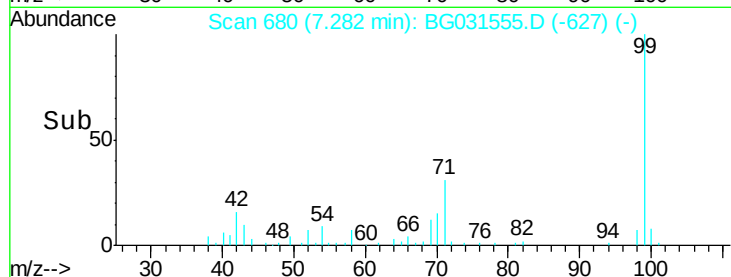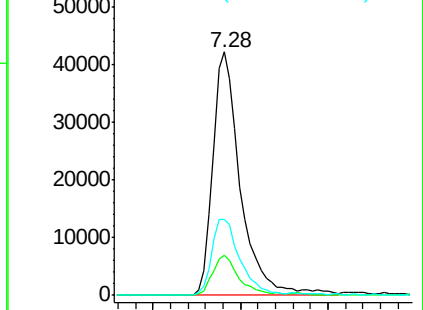

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1300

Delta R.T. 0.00 min

Lab File: BG031555.D

Acq: 14 Dec 2017 8:15

Tgt Ion: 136 Resp: 200826


Ion Ratio Lower Upper

136 100



137 11.2 9.2 13.8


54 6.9 10.3 15.5#

68 5.0 4.5 6.7

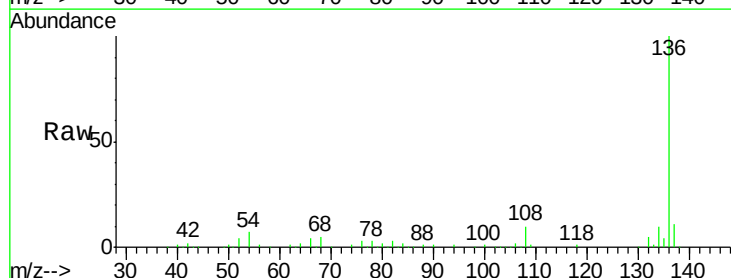

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



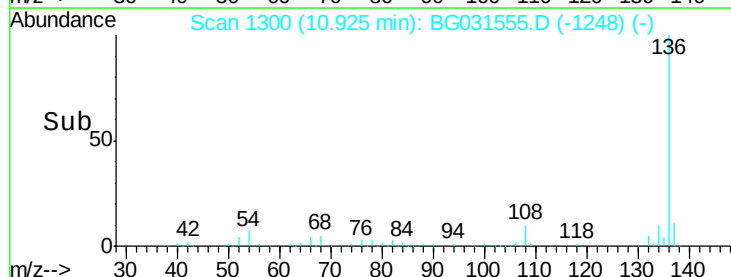
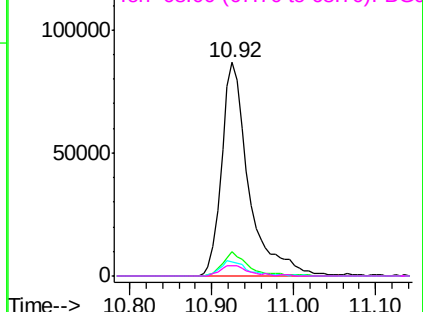


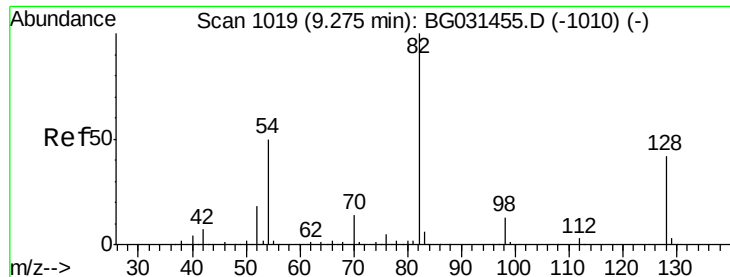

#23
 Nitrobenzene-d5
 Concen: 88.140 ng
 RT: 9.28 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: BG031555.D
 Acq: 14 Dec 2017 8:15




Instrument :
 BNA_G
 ClientSampleId :
 120617-FOPI-F-D-B


Tot Ion: 82 Resp: 287179
 Ion Ratio Lower Upper
 82 100
 128 45.6 29.7 44.5#
 54 48.5 43.1 64.7

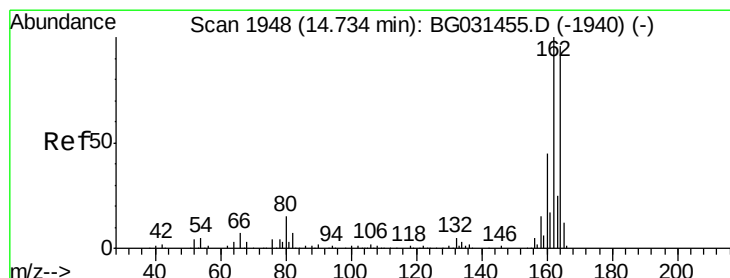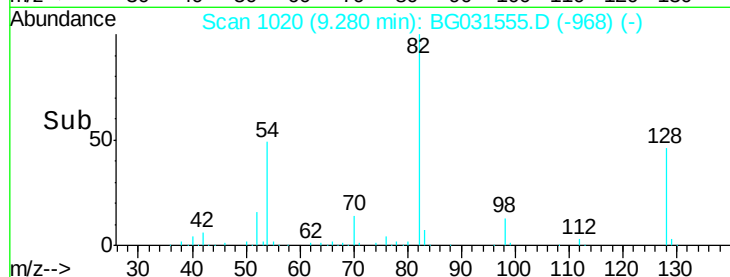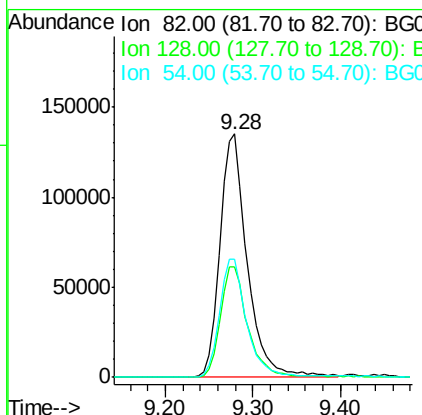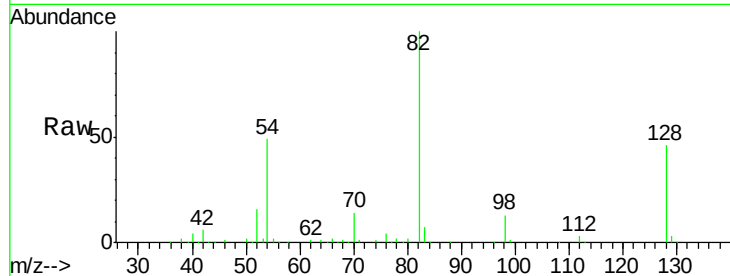

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. -0.00 min
 Lab File: BG031555.D
 Acq: 14 Dec 2017 8:15

Tgt Ion: 164 Resp: 153079
 Ion Ratio Lower Upper
 164 100
 162 98.0 78.8 118.2
 160 43.5 35.4 53.0


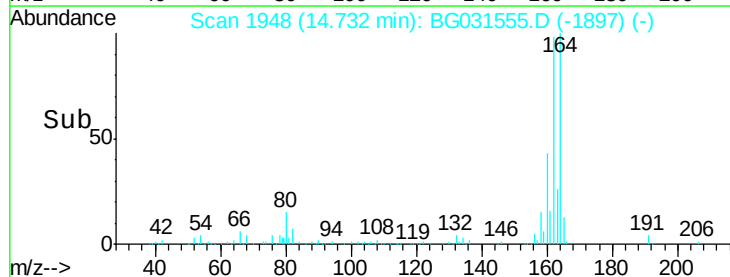
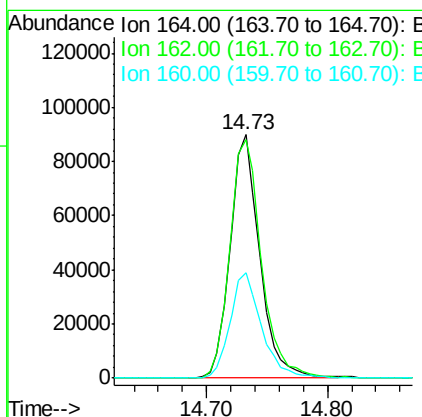
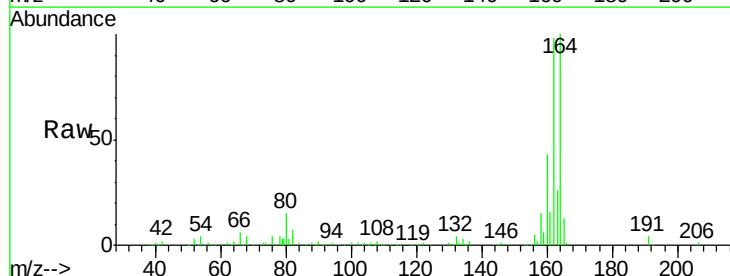


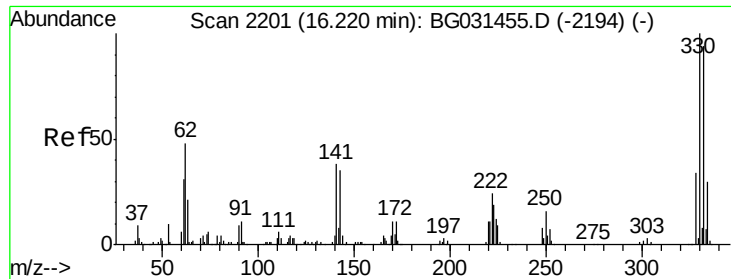

#41
 2,4,6-Tribromophenol
 Concen: 108.127 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. -0.00 min
 Lab File: BG031555.D
 Acq: 14 Dec 2017 8:15




Instrument :
 BNA_G
 ClientSampleId :
 120617-FOPI-F-D-B


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	77.0	115.6
141	35.1	25.2	37.8

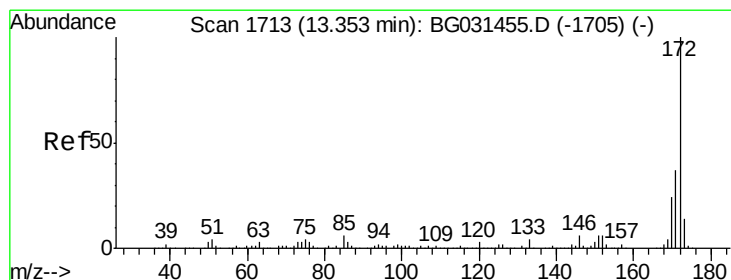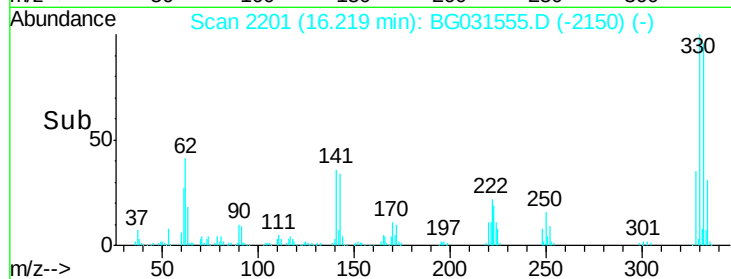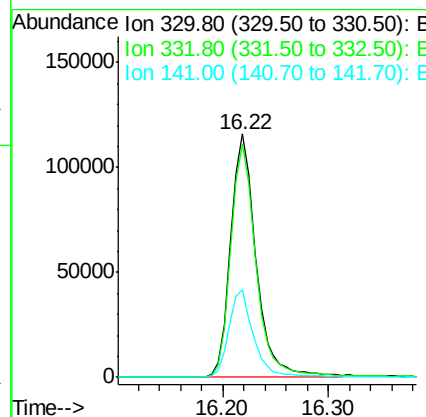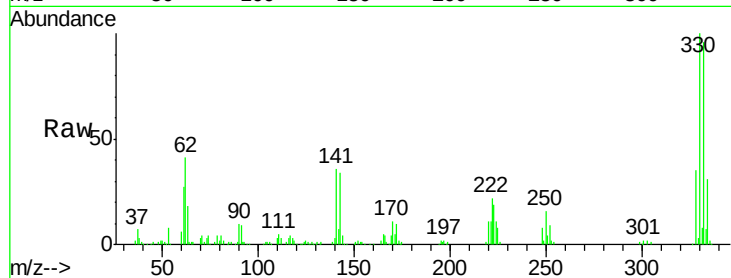

#44
 2-Fluorobiphenyl
 Concen: 91.081 ng
 RT: 13.35 min Scan# 1713
 Delta R.T. -0.00 min
 Lab File: BG031555.D
 Acq: 14 Dec 2017 8:15

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	30.0	45.0
170	24.0	19.5	29.3

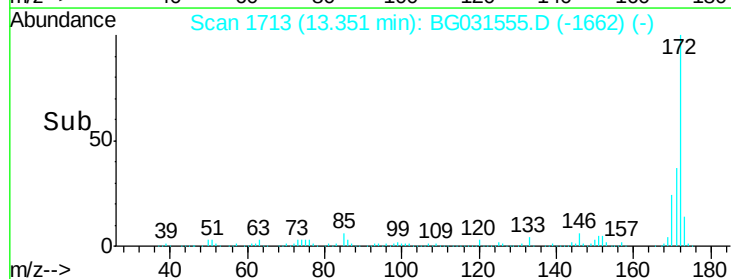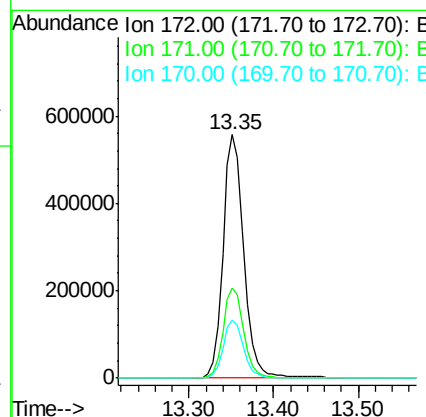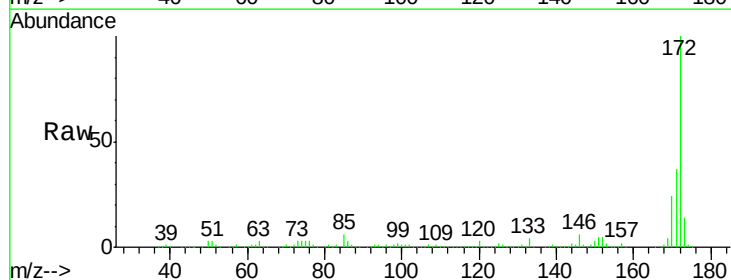


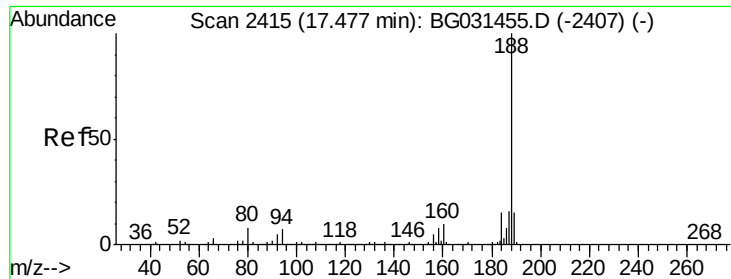




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2414
Delta R.T. -0.01 min
Lab File: BG031555.D
Acq: 14 Dec 2017 8:15

Instrument :
BNA_G
ClientSampleId :
120617-FOPI-F-D-B

Tot Ion:188 Resp: 472435
Ion Ratio Lower Upper
188 100
94 7.2 6.9 10.3
80 7.8 7.7 11.5

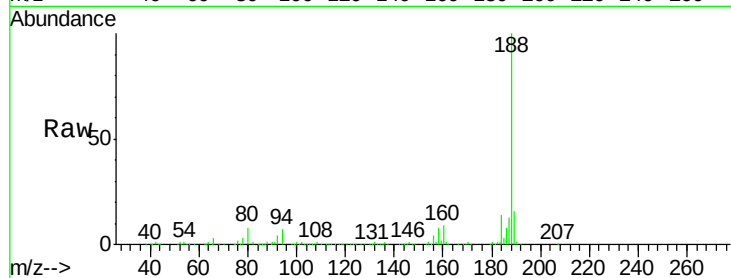


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

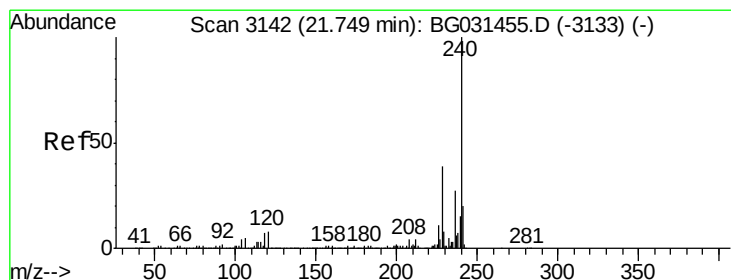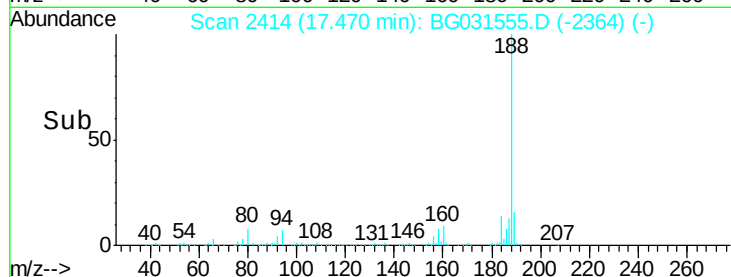
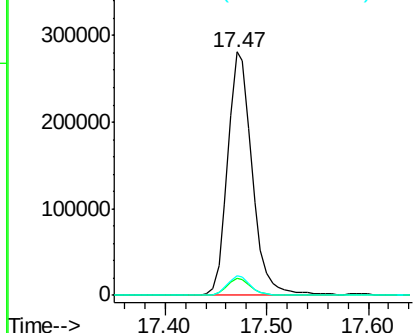



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.74 min Scan# 3141
Delta R.T. -0.01 min
Lab File: BG031555.D
Acq: 14 Dec 2017 8:15

Tgt Ion:240 Resp: 566174
Ion Ratio Lower Upper
240 100
120 8.0 6.8 10.2
236 26.5 20.9 31.3

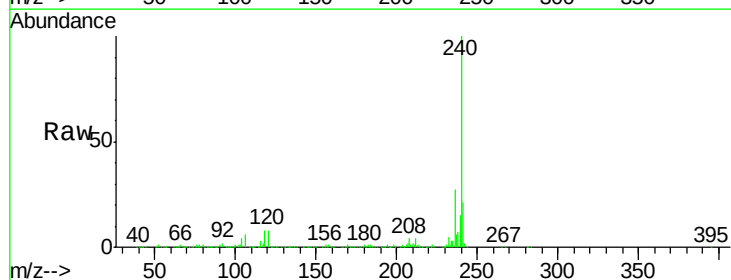

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

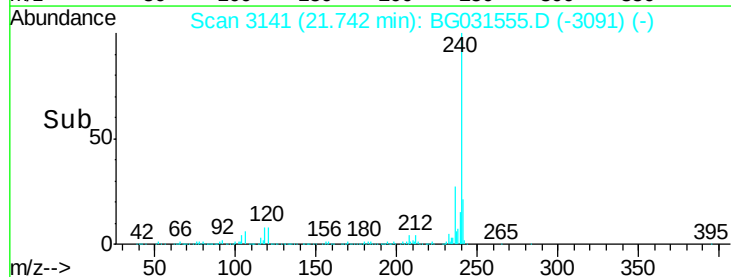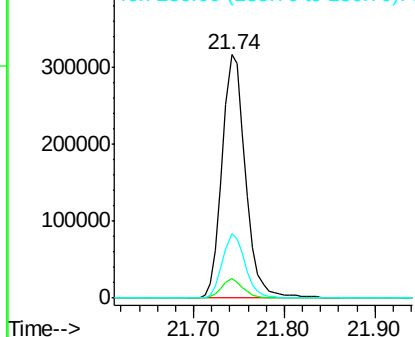

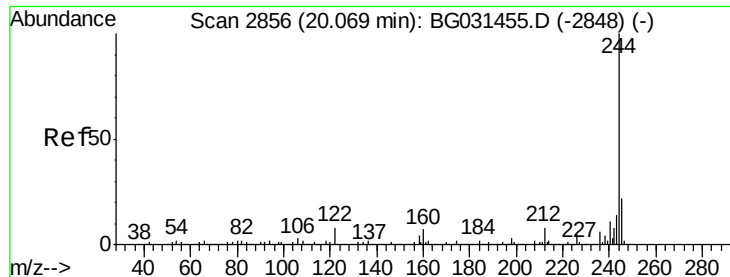

#78

Terphenyl-d14

Concen: 76.781 ng

RT: 20.07 min Scan# 2856

Delta R.T. -0.00 min

Lab File: BG031555.D

Acq: 14 Dec 2017 8:15

Instrument :

BNA_G

ClientSampleId :

120617-FOPI-F-D-B


Tot Ion:244 Resp: 1910703

Ion Ratio Lower Upper

244 100

212 8.7 5.8 8.8




122 8.8 7.0 10.4

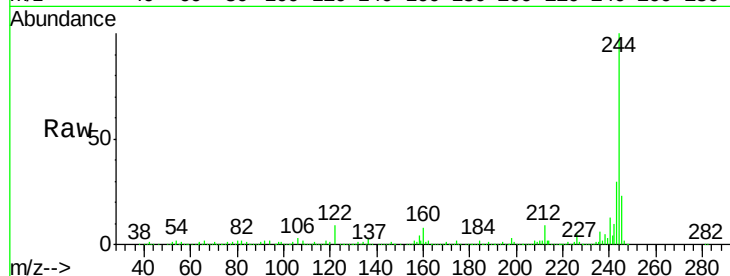

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

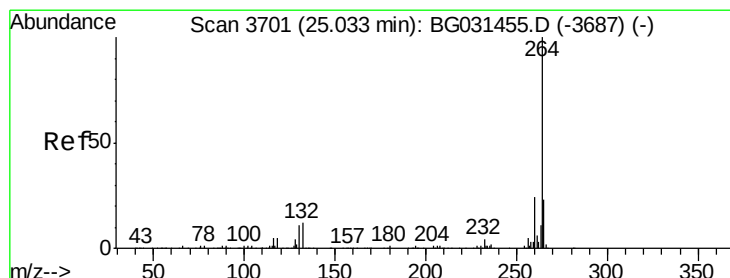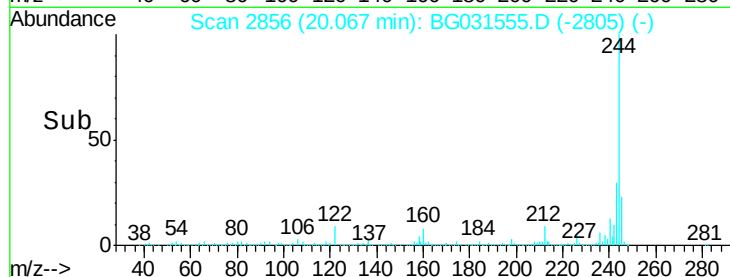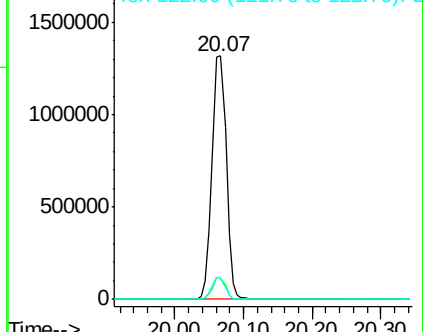

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.03 min Scan# 3700

Delta R.T. -0.01 min

Lab File: BG031555.D

Acq: 14 Dec 2017 8:15


Tgt Ion:264 Resp: 544167

Ion Ratio Lower Upper

264 100

260 24.1 17.4 26.0

265 21.3 17.7 26.5

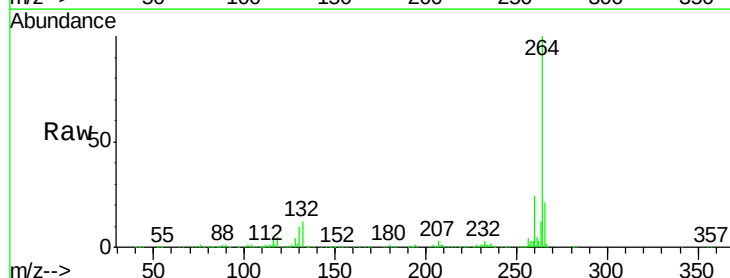

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

