


Data Path : Z:\HPCHEM1\BNA G\Data\BG121317\
 Data File : BG031521.D
 Acq On : 13 Dec 2017 10:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 11 17:25:55 2017

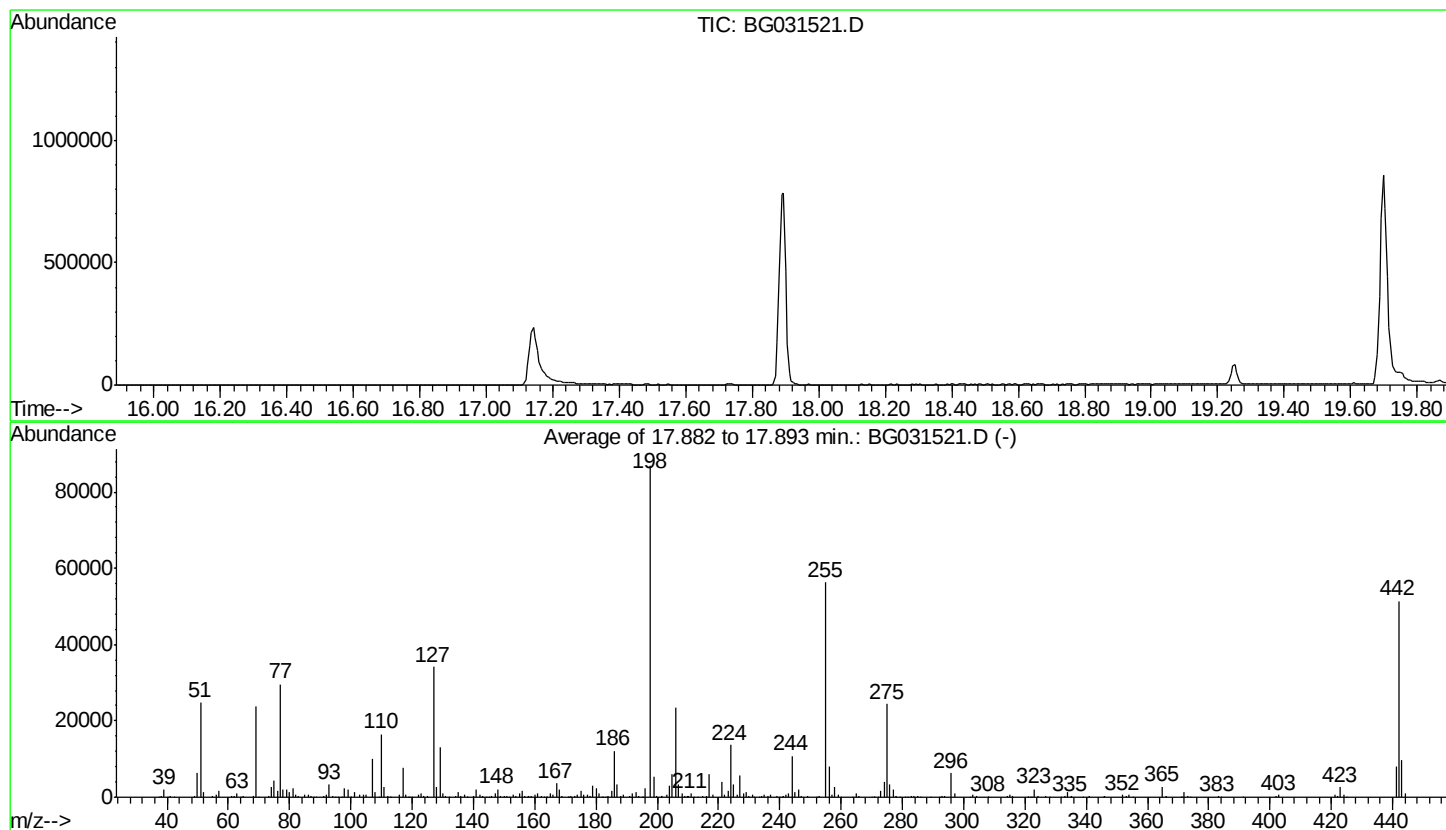

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	24696	PASS
68	69	0.00	2	0.9	224	PASS
69	198	0.00	100	27.6	23944	PASS
70	69	0.00	2	0.6	140	PASS
127	198	10	80	39.3	34176	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86893	PASS
199	198	5	9	6.4	5525	PASS
275	198	10	60	28.1	24399	PASS
365	198	1	100	3.3	2825	PASS
441	442	0.01	24	15.6	8022	PASS
442	198	50	100	59.2	51450	PASS
443	442	15	24	19.0	9794	PASS