
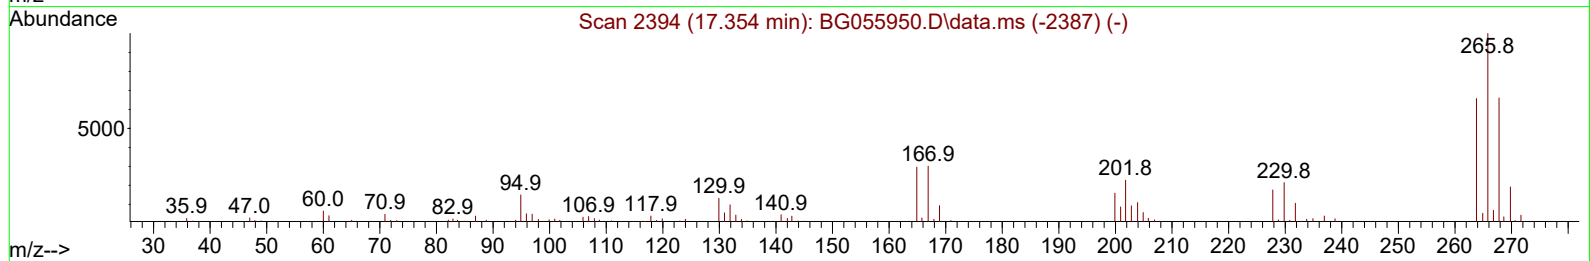
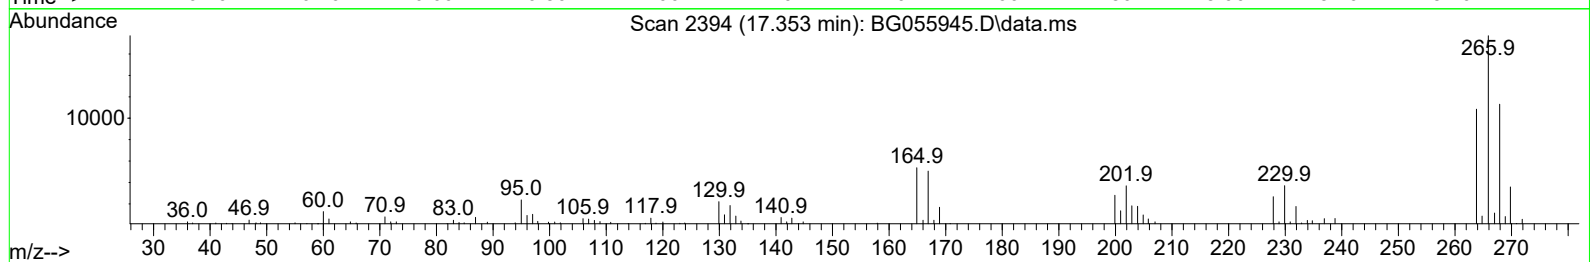


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121322\
Data File : BG055945.D
Acq On : 13 Dec 2022 16:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 06:48:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

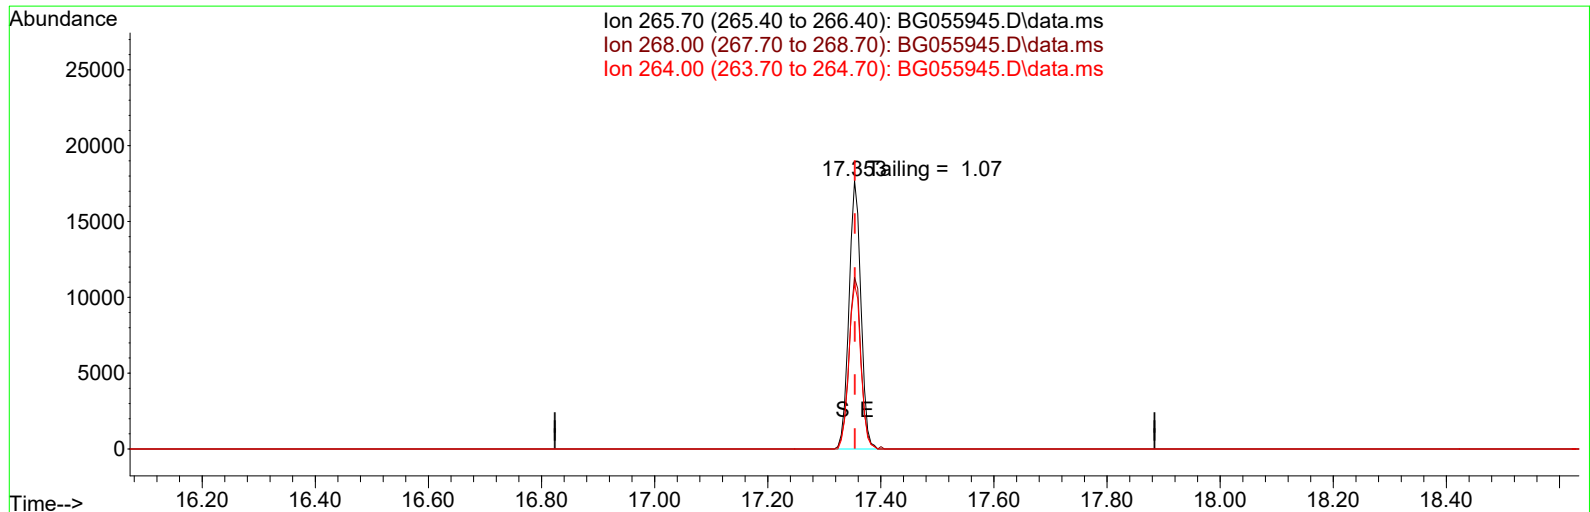

TIC: BG055945.D\data.ms

(70) Pentachlorophenol (C)




17.353min (-0.001) 0.00 ng

response 25948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	63.87
264.00	65.70	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121322\
 Data File : BG055945.D
 Acq On : 13 Dec 2022 16:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 06:48:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 02:24:06 2022
 Response via : Initial Calibration

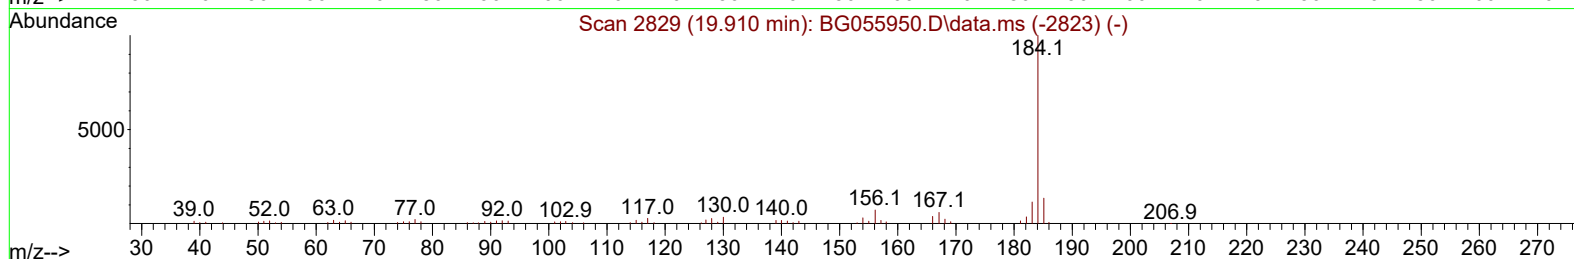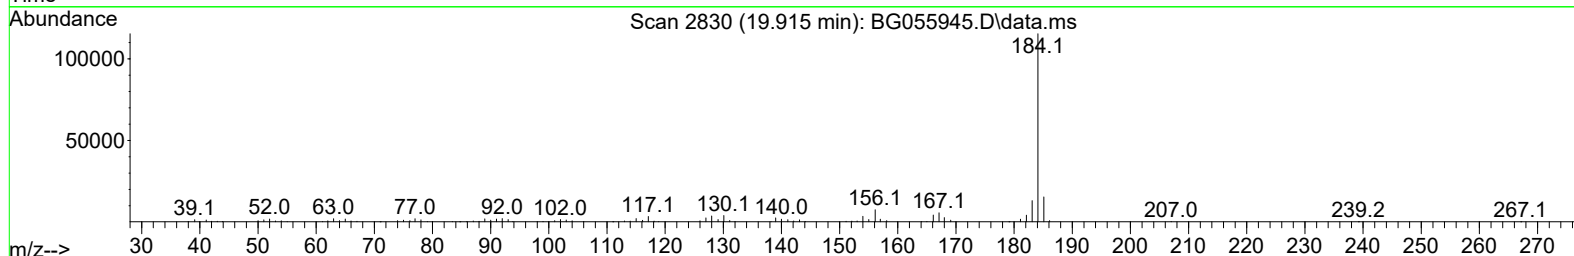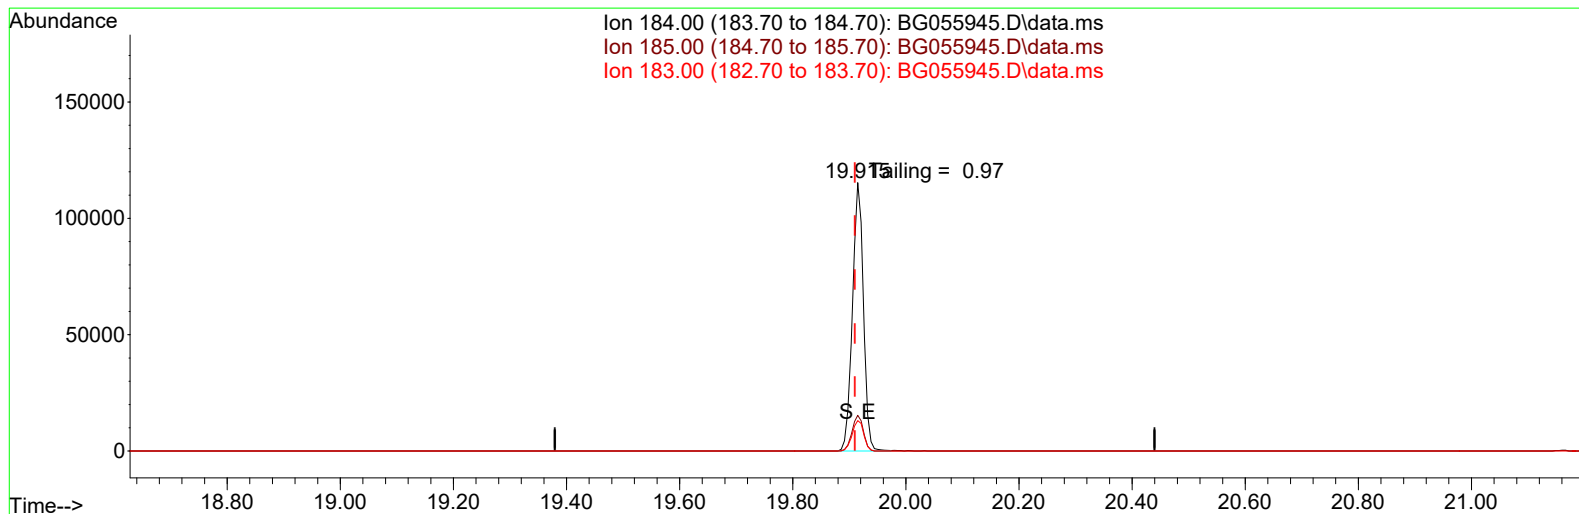

TIC: BG055945.D\data.ms

(77) Benzidine

19.915min (+ 0.005) 0.00 ng

response 155922

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.29
183.00	11.50	11.34
0.00	0.00	0.00