
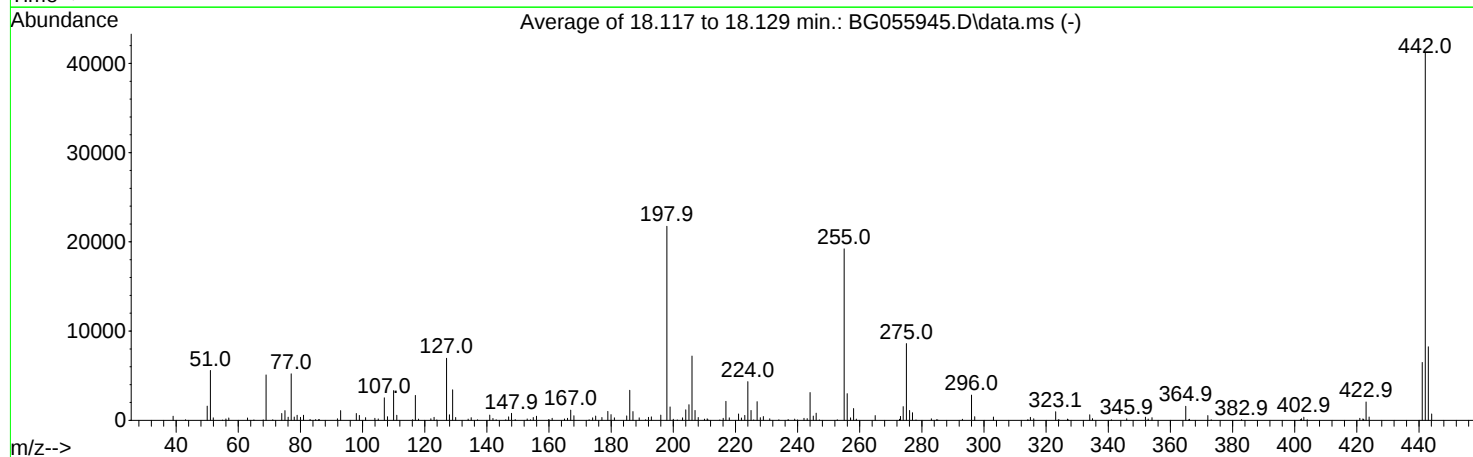


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121322\
 Data File : BG055945.D
 Acq On : 13 Dec 2022 16:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 14 02:24:06 2022

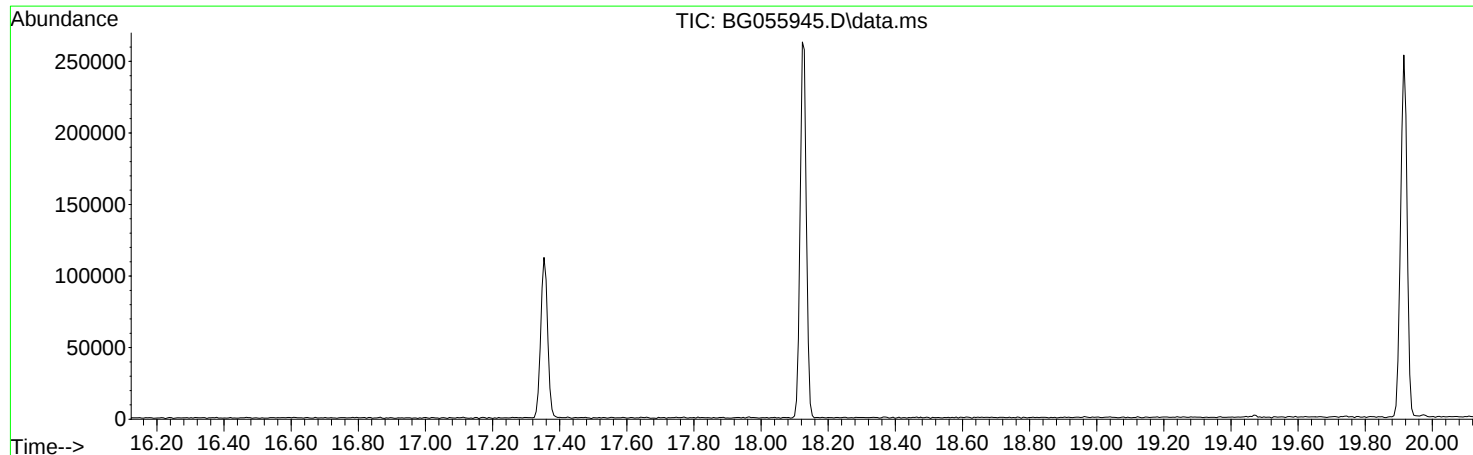




AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	5586	PASS
68	69	0.00	2	1.1	54	PASS
69	198	0.00	100	23.4	5094	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.0	6951	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21755	PASS
199	198	5	9	6.9	1493	PASS
275	198	10	60	39.5	8596	PASS
365	198	1	100	7.2	1573	PASS
441	198	0.01	100	29.8	6486	PASS
442	442	50	100	100.0	41237	PASS
443	442	15	24	20.0	8248	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121322\
 Data File : BG055945.D
 Acq On : 13 Dec 2022 16:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 14 06:48:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 02:24:06 2022
 Response via : Initial Calibration

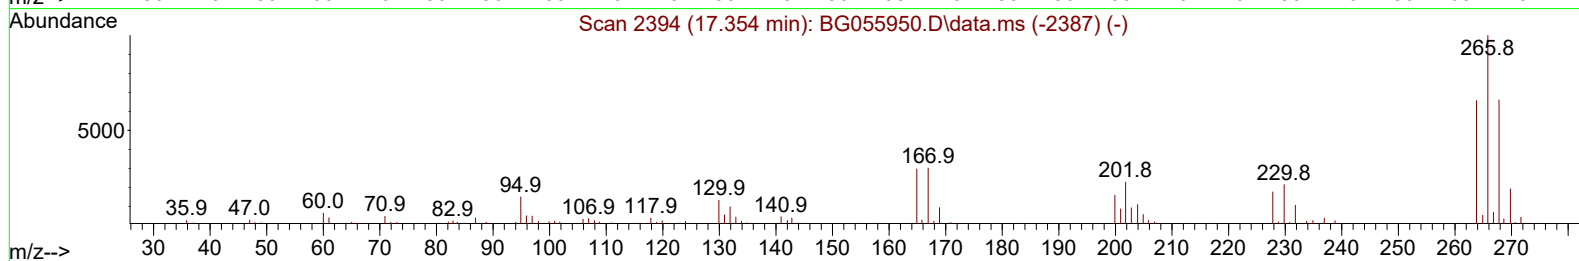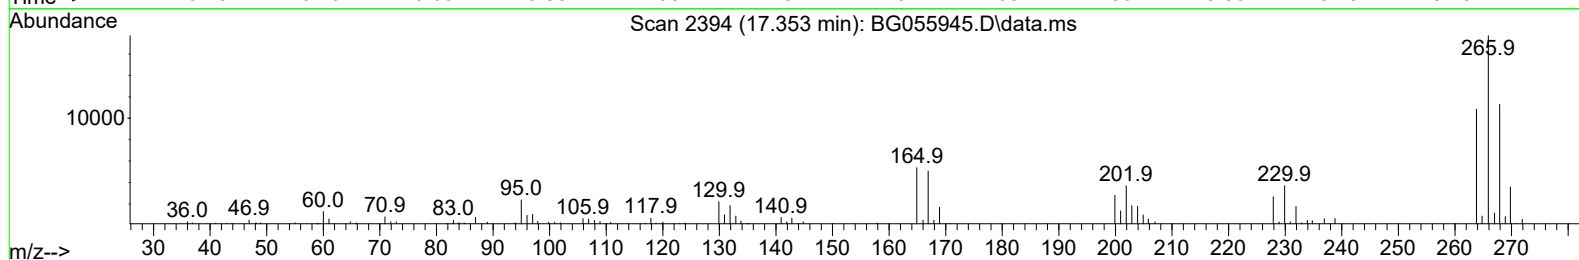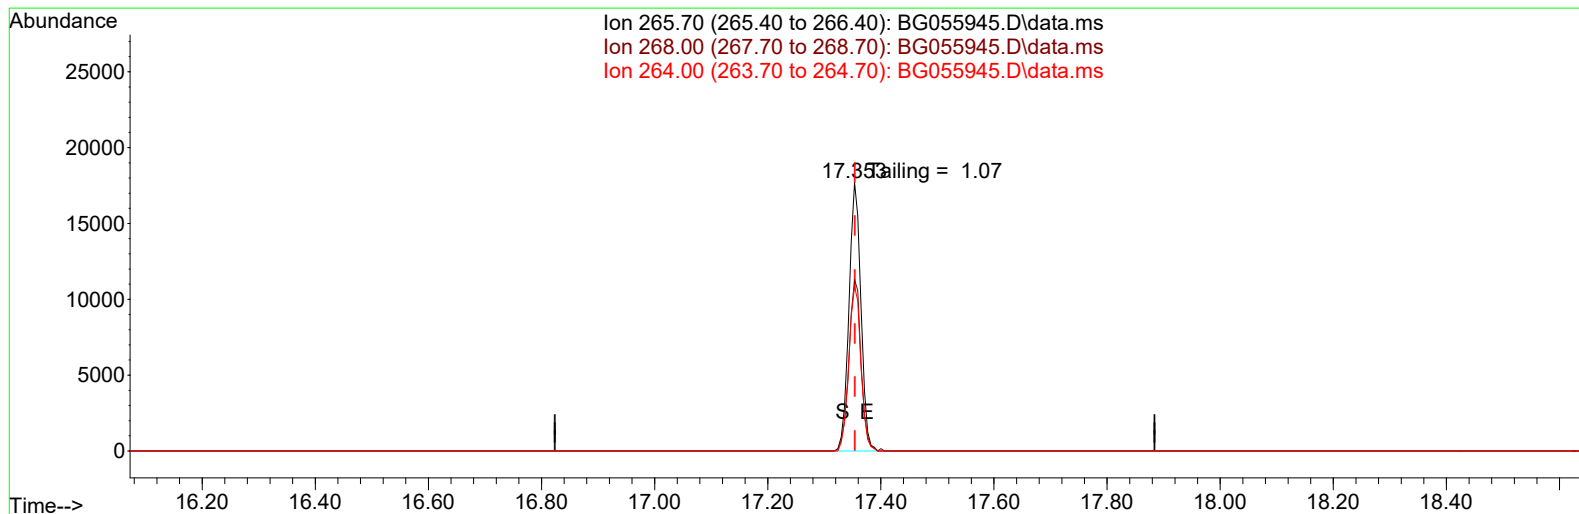

TIC: BG055945.D\data.ms

(70) Pentachlorophenol (C)

17.353min (-0.001) 0.00 ng




response 25948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	63.87
264.00	65.70	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121322\
Data File : BG055945.D
Acq On : 13 Dec 2022 16:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 14 06:48:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 02:24:06 2022
Response via : Initial Calibration

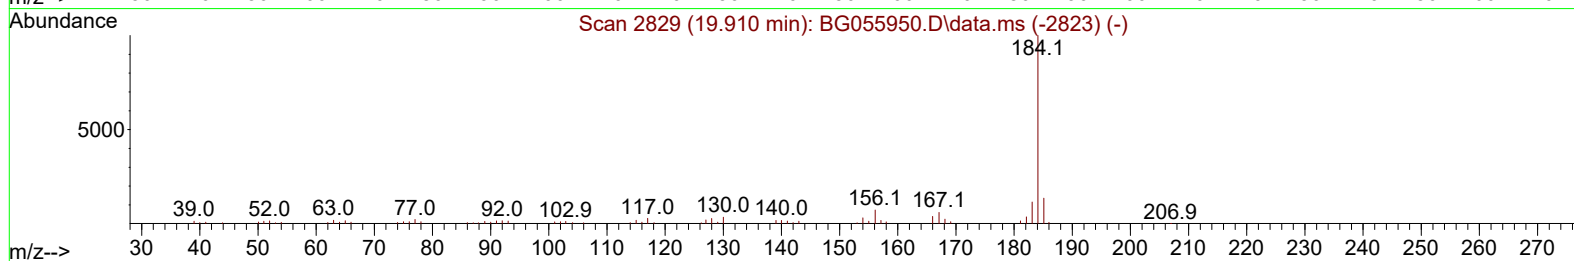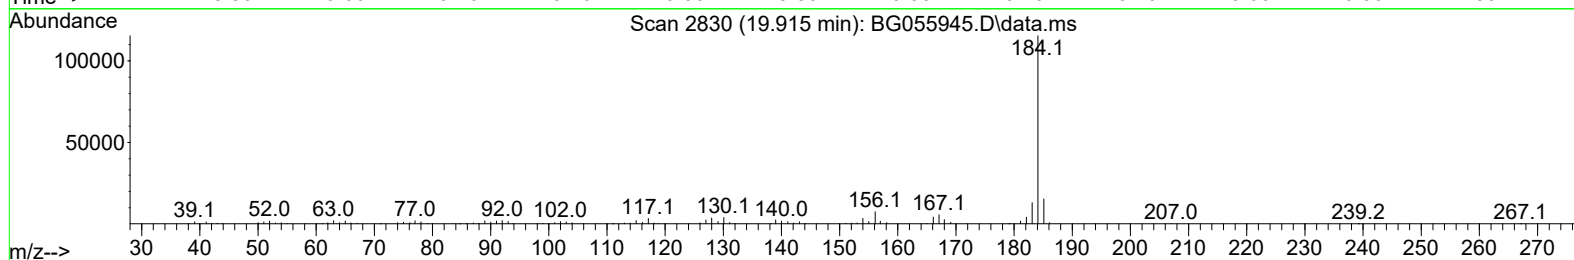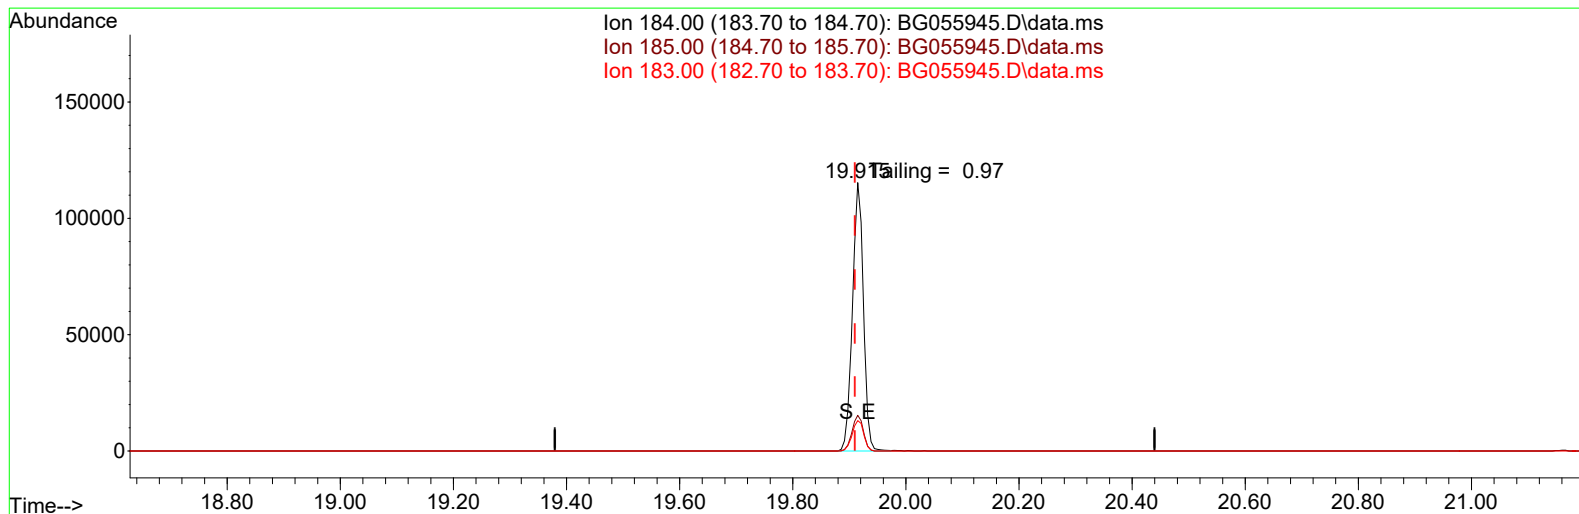

TIC: BG055945.D\data.ms

(77) Benzidine

19.915min (+ 0.005) 0.00 ng

response 155922

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.29
183.00	11.50	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/13/2022	BNA_G	BG055945.D
Compound Name	Response	Retention Time
DDT	68082	21.161
DDD	466	20.761
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
466	68548	0.68

Instrument :
BNA_G
ClientSampleId :
DFTPP