

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121324\
 Data File : BG063672.D
 Acq On : 13 Dec 2024 10:57
 Operator : RC/JU
 Sample : PB165551BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK551

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.273	29	31	36	rVB4	47686	56975	0.97%	0.102%
2	3.684	96	101	115	rBV	575353	994407	16.87%	1.788%
3	3.966	147	149	153	rBV4	13592	12827	0.22%	0.023%
4	5.047	330	333	335	rBV4	8293	10439	0.18%	0.019%
5	5.770	454	456	459	rVB2	8422	8864	0.15%	0.016%
6	5.870	470	473	474	rBV	12144	9666	0.16%	0.017%
7	5.958	485	488	490	rBV2	9243	12158	0.21%	0.022%
8	6.334	548	552	553	rBV4	7326	8170	0.14%	0.015%
9	6.440	568	570	573	rVB4	10519	10686	0.18%	0.019%
10	6.992	655	664	675	rBV	803536	1353607	22.96%	2.434%
11	7.139	682	689	698	rBV	673811	1099323	18.65%	1.977%
12	7.345	718	724	731	rBV	723451	1200169	20.36%	2.158%
13	7.544	756	758	760	rBV2	7272	7656	0.13%	0.014%
14	7.809	796	803	810	rBV	572792	984030	16.69%	1.770%
15	8.267	880	881	884	rBV3	10810	10809	0.18%	0.019%
16	8.296	884	886	888	rVB2	12492	10156	0.17%	0.018%
17	8.526	917	925	933	rBV	905636	1579281	26.79%	2.840%
18	8.825	973	976	980	rBV4	7636	9755	0.17%	0.018%
19	8.960	992	999	1008	rBV	736991	1298491	22.03%	2.335%
20	9.301	1055	1057	1062	rVB3	7132	8488	0.14%	0.015%
21	9.378	1067	1070	1071	rBV2	16105	12964	0.22%	0.023%
22	9.548	1095	1099	1101	rBV3	5633	9192	0.16%	0.017%
23	9.683	1113	1122	1134	rBV	616543	1102421	18.70%	1.983%
24	9.842	1146	1149	1153	rBV2	9513	16867	0.29%	0.030%
25	10.053	1184	1185	1188	rVB2	8847	8239	0.14%	0.015%
26	10.230	1208	1215	1225	rBV	863300	1589513	26.97%	2.859%
27	10.594	1270	1277	1286	rVB	779023	1400579	23.76%	2.519%
28	10.735	1293	1301	1313	rBV	821056	1545527	26.22%	2.780%
29	10.893	1326	1328	1331	rVB3	7645	7874	0.13%	0.014%
30	11.070	1357	1358	1361	rBV3	7193	8511	0.14%	0.015%
31	11.375	1409	1410	1416	rVB3	6949	9491	0.16%	0.017%
32	11.663	1456	1459	1461	rVB2	6590	7589	0.13%	0.014%
33	11.710	1464	1467	1469	rVB3	10165	9333	0.16%	0.017%
34	11.787	1479	1480	1487	rBV3	7252	10564	0.18%	0.019%
35	11.928	1501	1504	1509	rBV3	8878	15893	0.27%	0.029%
36	12.192	1545	1549	1556	rBV5	17054	35061	0.59%	0.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121324\
 Data File : BG063672.D
 Acq On : 13 Dec 2024 10:57
 Operator : RC/JU
 Sample : PB165551BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK551

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

37	12.480	1595	1598	1599	rBV	7175	8828	0.15%	0.016%
38	13.784	1818	1820	1823	rVB2	8394	8384	0.14%	0.015%
39	13.855	1826	1832	1839	rBV	1936262	2751364	46.68%	4.948%
40	13.943	1845	1847	1849	rVB	8999	7735	0.13%	0.014%
41	14.049	1860	1865	1868	rBV4	6730	12314	0.21%	0.022%
42	14.143	1873	1881	1892	rVV	2012711	3236962	54.91%	5.821%
43	14.307	1907	1909	1912	rBV	10737	9180	0.16%	0.017%
44	14.448	1925	1933	1941	rBV	1427137	2196173	37.26%	3.950%
45	14.677	1965	1972	1982	rBV	609097	1171416	19.87%	2.107%
46	14.848	2000	2001	2005	rVB4	9997	11150	0.19%	0.020%
47	15.441	2095	2102	2113	rBV	2649786	4209419	71.41%	7.570%
48	15.576	2119	2125	2132	rBV	773908	1148207	19.48%	2.065%
49	15.741	2150	2153	2156	rBV5	8594	10730	0.18%	0.019%
50	15.799	2160	2163	2165	rBV3	8079	10995	0.19%	0.020%
51	16.076	2209	2210	2214	rVB4	8885	9414	0.16%	0.017%
52	16.117	2214	2217	2220	rBV3	6717	7742	0.13%	0.014%
53	16.422	2267	2269	2271	rBV2	7580	7775	0.13%	0.014%
54	16.440	2271	2272	2276	rVB2	8714	10989	0.19%	0.020%
55	16.581	2294	2296	2299	rBV2	10819	10572	0.18%	0.019%
56	16.651	2307	2308	2311	rBV	7994	7777	0.13%	0.014%
57	16.681	2311	2313	2317	rVB	9241	8990	0.15%	0.016%
58	16.722	2317	2320	2323	rBV2	7619	11724	0.20%	0.021%
59	16.822	2333	2337	2338	rBV2	12456	12049	0.20%	0.022%
60	16.857	2340	2343	2344	rBV2	10249	12074	0.20%	0.022%
61	16.886	2346	2348	2352	rVB5	10599	13293	0.23%	0.024%
62	16.986	2363	2365	2372	rBV3	12090	15582	0.26%	0.028%
63	17.092	2380	2383	2385	rVB3	7619	8285	0.14%	0.015%
64	17.198	2395	2401	2410	rBV	1908178	2863928	48.59%	5.151%
65	17.298	2412	2418	2429	rVV	3280824	4925034	83.55%	8.857%
66	17.556	2458	2462	2466	rVB2	7748	10800	0.18%	0.019%
67	17.591	2466	2468	2470	rBV	10281	10275	0.17%	0.018%
68	17.750	2493	2495	2498	rVB3	14188	12173	0.21%	0.022%
69	17.815	2503	2506	2508	rBV3	9435	8190	0.14%	0.015%
70	17.885	2516	2518	2520	rVB3	9562	7655	0.13%	0.014%
71	17.938	2524	2527	2530	rBV3	11048	13174	0.22%	0.024%
72	18.020	2539	2541	2542	rBV	8720	7826	0.13%	0.014%
73	18.038	2542	2544	2546	rVB2	11831	9501	0.16%	0.017%
74	18.108	2553	2556	2558	rBV3	7275	8576	0.15%	0.015%
75	18.232	2574	2577	2578	rBV3	10483	9182	0.16%	0.017%
76	18.267	2582	2583	2590	rVB4	9361	11257	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121324\
Data File : BG063672.D
Acq On : 13 Dec 2024 10:57
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK551

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Title : SVOA CALIBRATION

77	19.160	2731	2735	2739	rBV4	48147	66494	1.13%	0.120%
78	19.231	2744	2747	2751	rBV3	38312	54050	0.92%	0.097%
79	19.601	2803	2810	2822	rBV	3944803	5894590	100.00%	10.601%
80	21.452	3119	3125	3134	rBV	1944976	3204491	54.36%	5.763%
81	24.260	3595	3603	3617	rVB2	2164690	5565435	94.42%	10.009%
82	24.466	3630	3638	3649	rVB	1377340	3516743	59.66%	6.325%




Sum of corrected areas: 55604072

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121324\
Data File : BG063672.D
Acq On : 13 Dec 2024 10:57
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

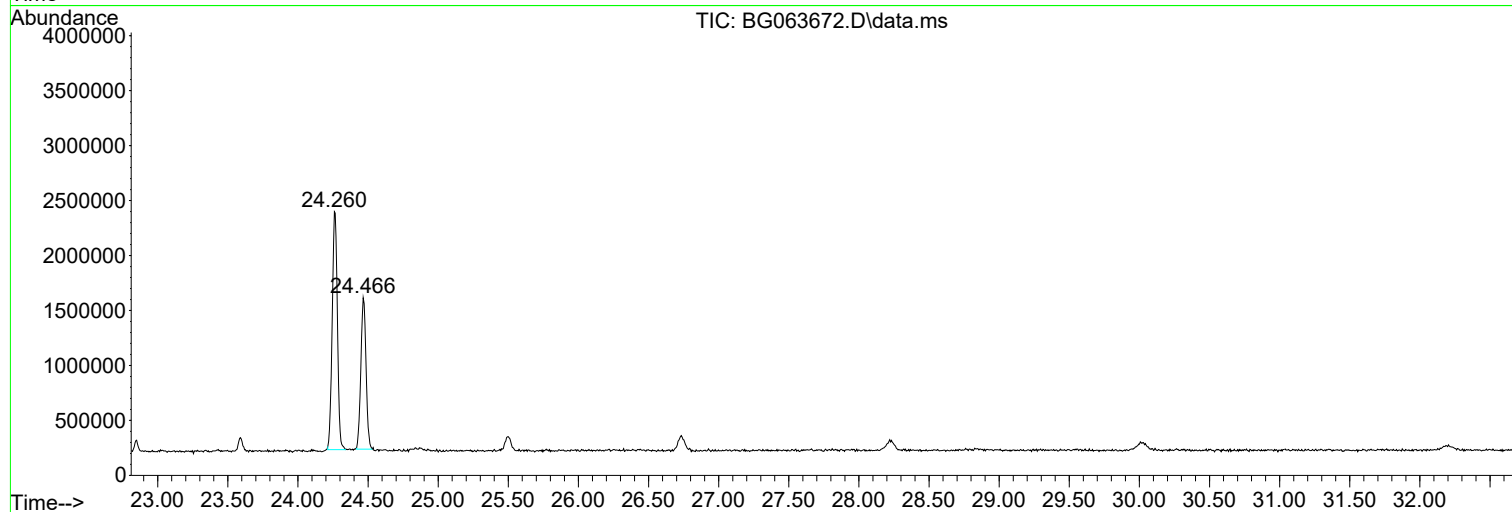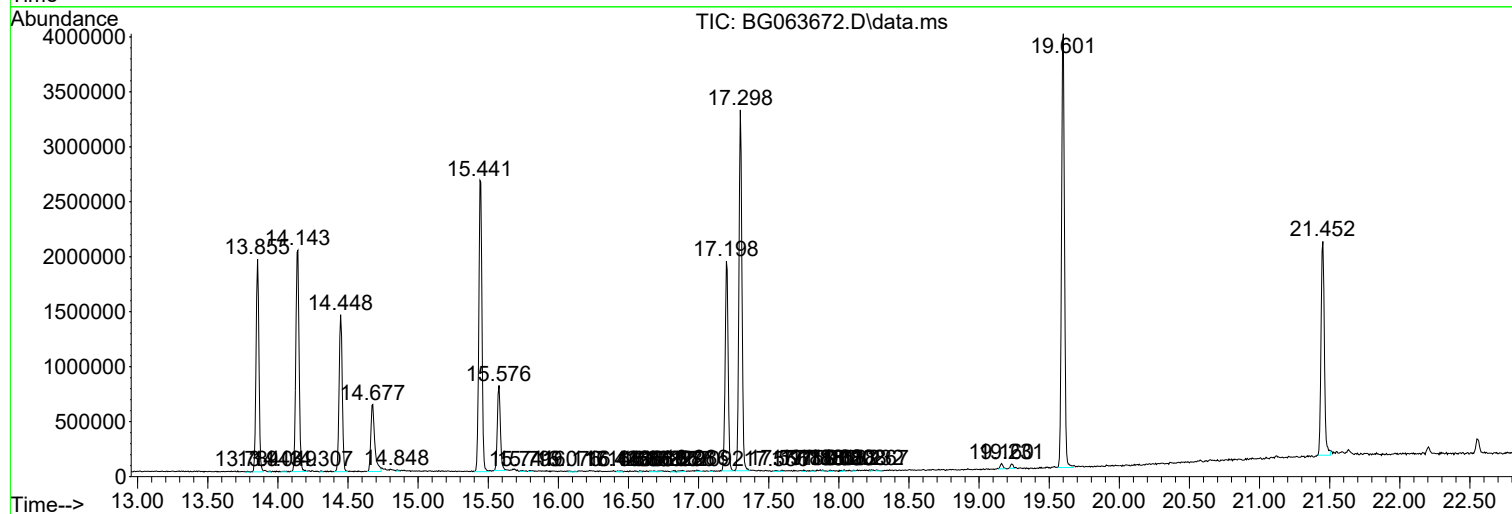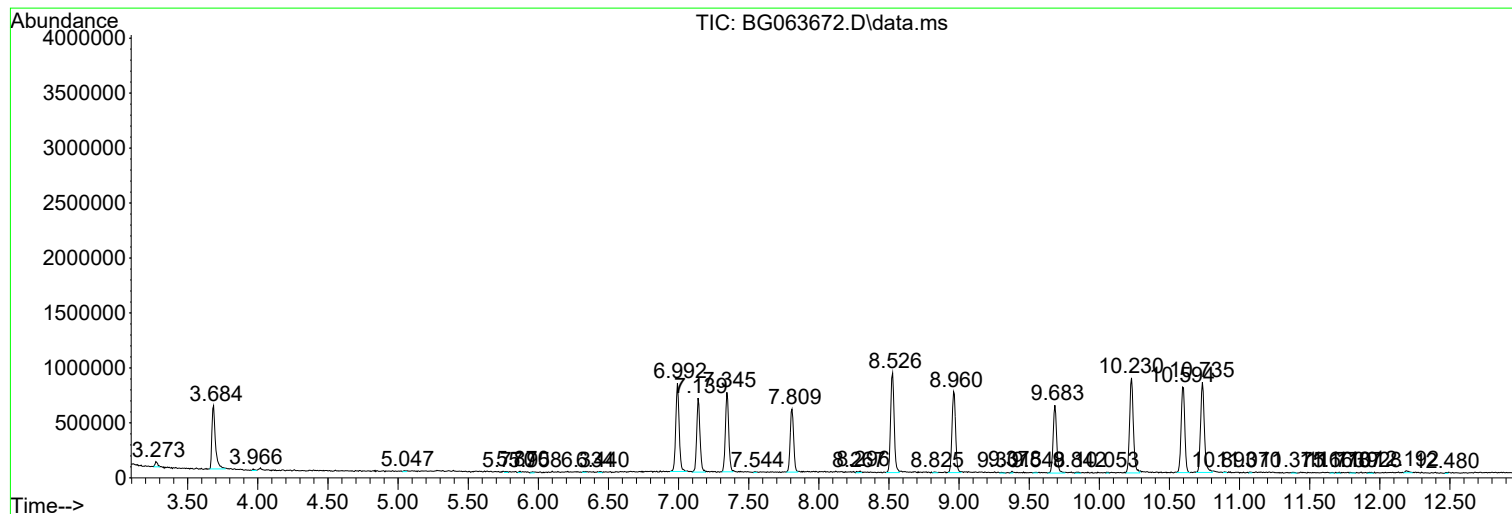

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121324\
Data File : BG063672.D
Acq On : 13 Dec 2024 10:57
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121324\
Data File : BG063672.D
Acq On : 13 Dec 2024 10:57
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc