

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121416\
 Data File : BG025184.D
 Acq On : 14 Dec 2016 20:19
 Operator : UM/SJ
 Sample : H5970-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DA854

Quant Time: Dec 15 04:02:06 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 03:57:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	78531	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	356823	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.86	164	309268	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.60	188	630573	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	754352	20.00	ng/ul	0.00
83) Perylene-d12	25.31	264	761712	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.58	96	4640	3.05	ng/uL	0.00
5) Phenol-d5	7.38	99	110834	16.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	75823	18.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	77046	16.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.94	113	95183	16.81	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	45135	17.86	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	34807	11.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	95378	15.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.20	131	97429	16.36	ng/ul	0.00
43) Dimethylphthalate-d6	14.25	166	411939	19.36	ng/ul	0.00
46) Acenaphthylene-d8	14.56	160	442749	19.00	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	34674	9.48	ng/ul	0.00
57) Fluorene-d10	15.84	176	379697	18.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.98	200	3986	1.02	ng/ul	0.00
70) Anthracene-d10	17.70	188	538294	20.23	ng/ul	0.00
76) Pyrene-d10	19.97	212	658860	21.20	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.07	264	651539	21.11	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.30	163	234035	11.19	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121416\
Data File : BG025184.D
Acq On : 14 Dec 2016 20:19
Operator : UM/SJ
Sample : H5970-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DA854

Quant Time: Dec 15 04:02:06 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 03:57:23 2016
Response via : Initial Calibration

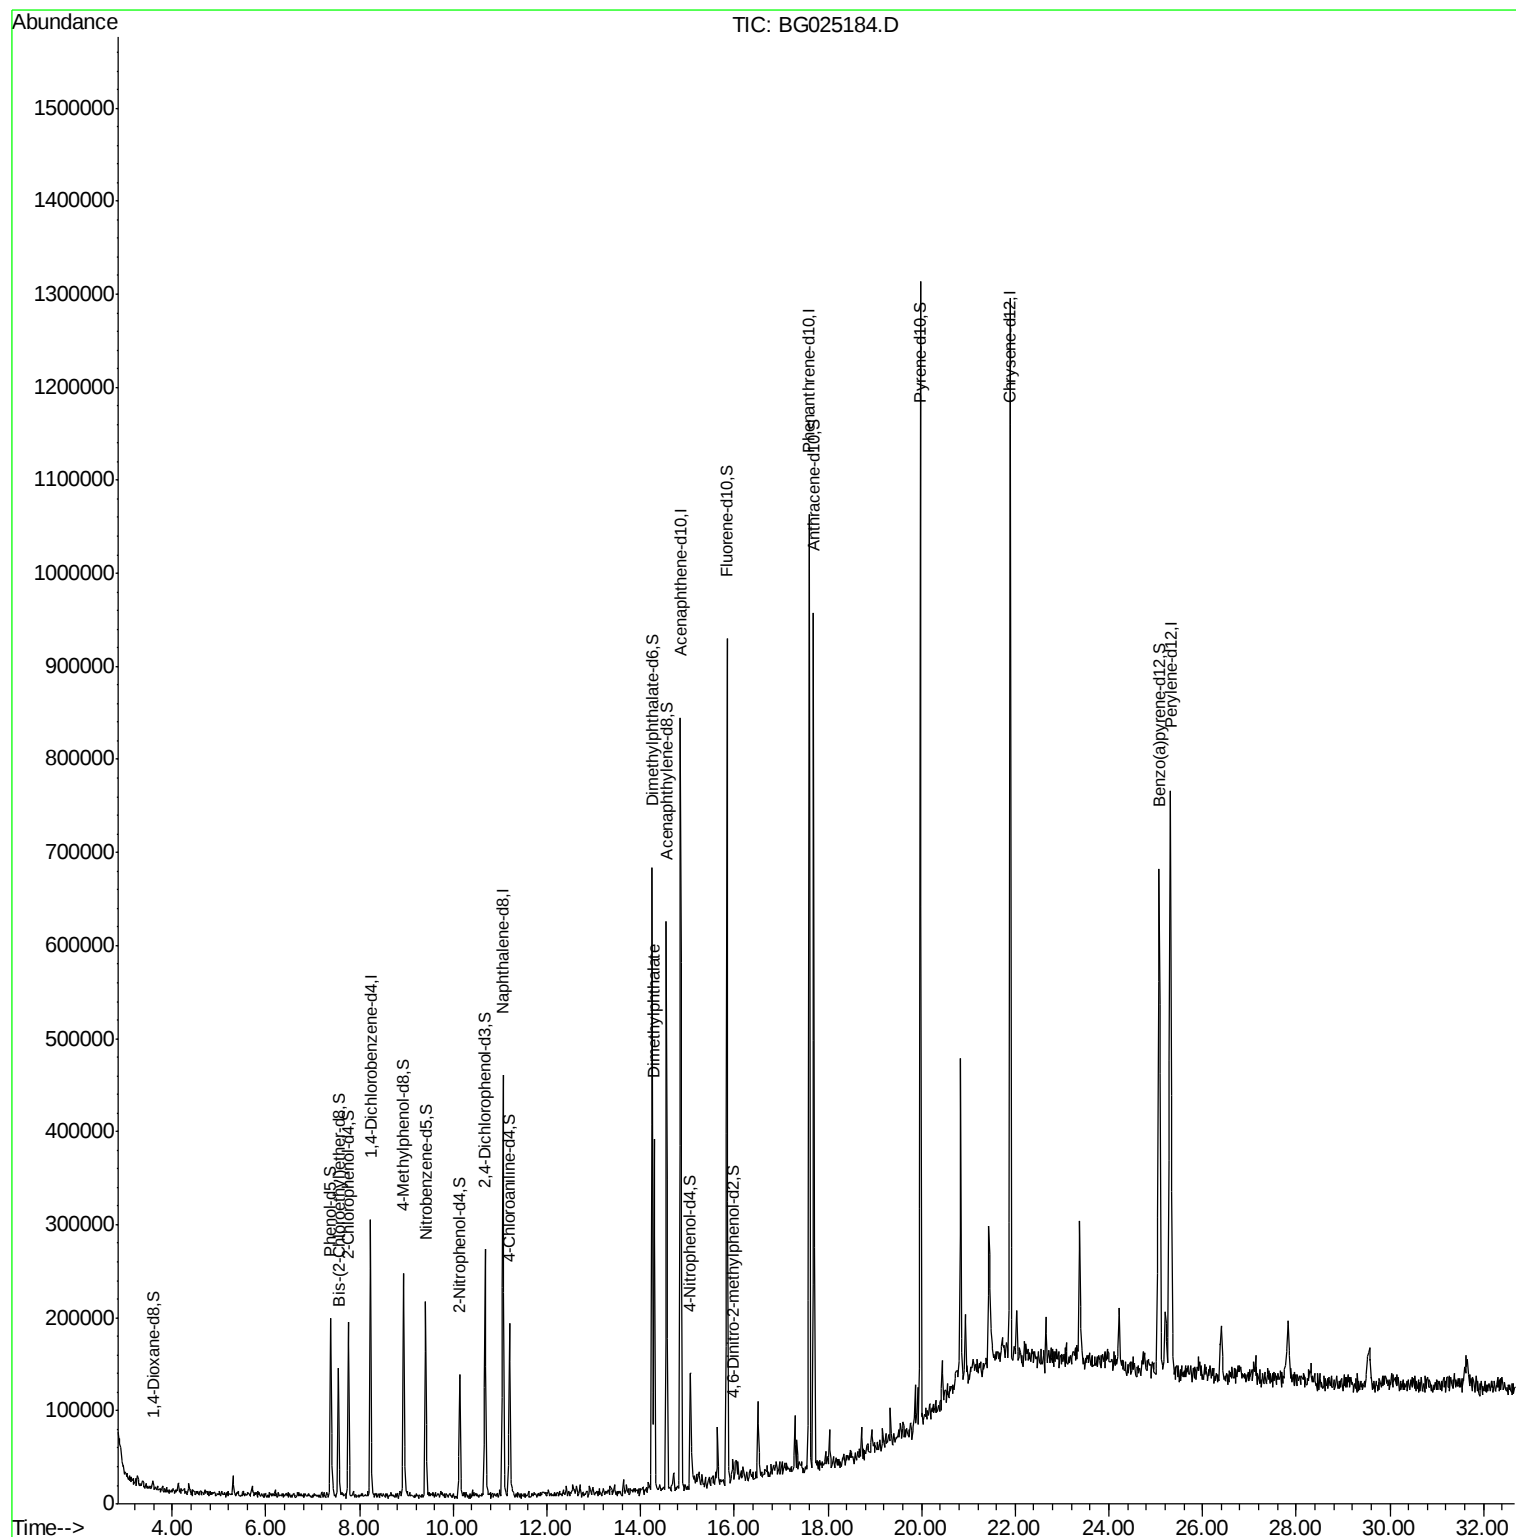

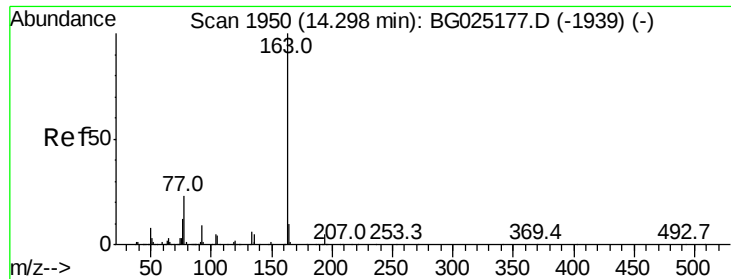

#44

Dimethylphthalate

Concen: 11.19 ng/ul

RT: 14.30 min Scan# 1950

Delta R.T. -0.00 min

Lab File: BG025184.D

Acq: 14 Dec 2016 20:19

Instrument :

BNA_G

ClientSampleId :

DA854


Tot Ion:163 Resp: 234035

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 9.2 9.0 13.4

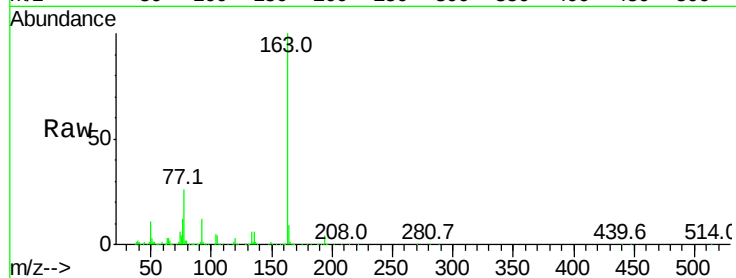

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

