

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121417\
 Data File : BG031566.D
 Acq On : 14 Dec 2017 19:48
 Operator : SJ/JU
 Sample : I6883-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 15 03:15:53 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 17:25:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	72758	20.00	ng	-0.01
21) Naphthalene-d8	10.92	136	302512	20.00	ng	0.00
38) Acenaphthene-d10	14.72	164	200090	20.00	ng	-0.01
63) Phenanthrene-d10	17.47	188	534523	20.00	ng	-0.01
75) Chrysene-d12	21.74	240	647336	20.00	ng	-0.01
86) Perylene-d12	25.02	264	561655	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	245313	59.76	ng	-0.01
7) Phenol-d6	7.27	99	185793	32.60	ng	0.00
23) Nitrobenzene-d5	9.27	82	444758	90.62	ng	0.00
41) 2,4,6-Tribromophenol	16.21	330	365638	155.98	ng	0.00
44) 2-Fluorobiphenyl	13.35	172	1281023	93.98	ng	0.00
78) Terphenyl-d14	20.06	244	2448355	86.05	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121417\
Data File : BG031566.D
Acq On : 14 Dec 2017 19:48
Operator : SJ/JU
Sample : I6883-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 15 03:15:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

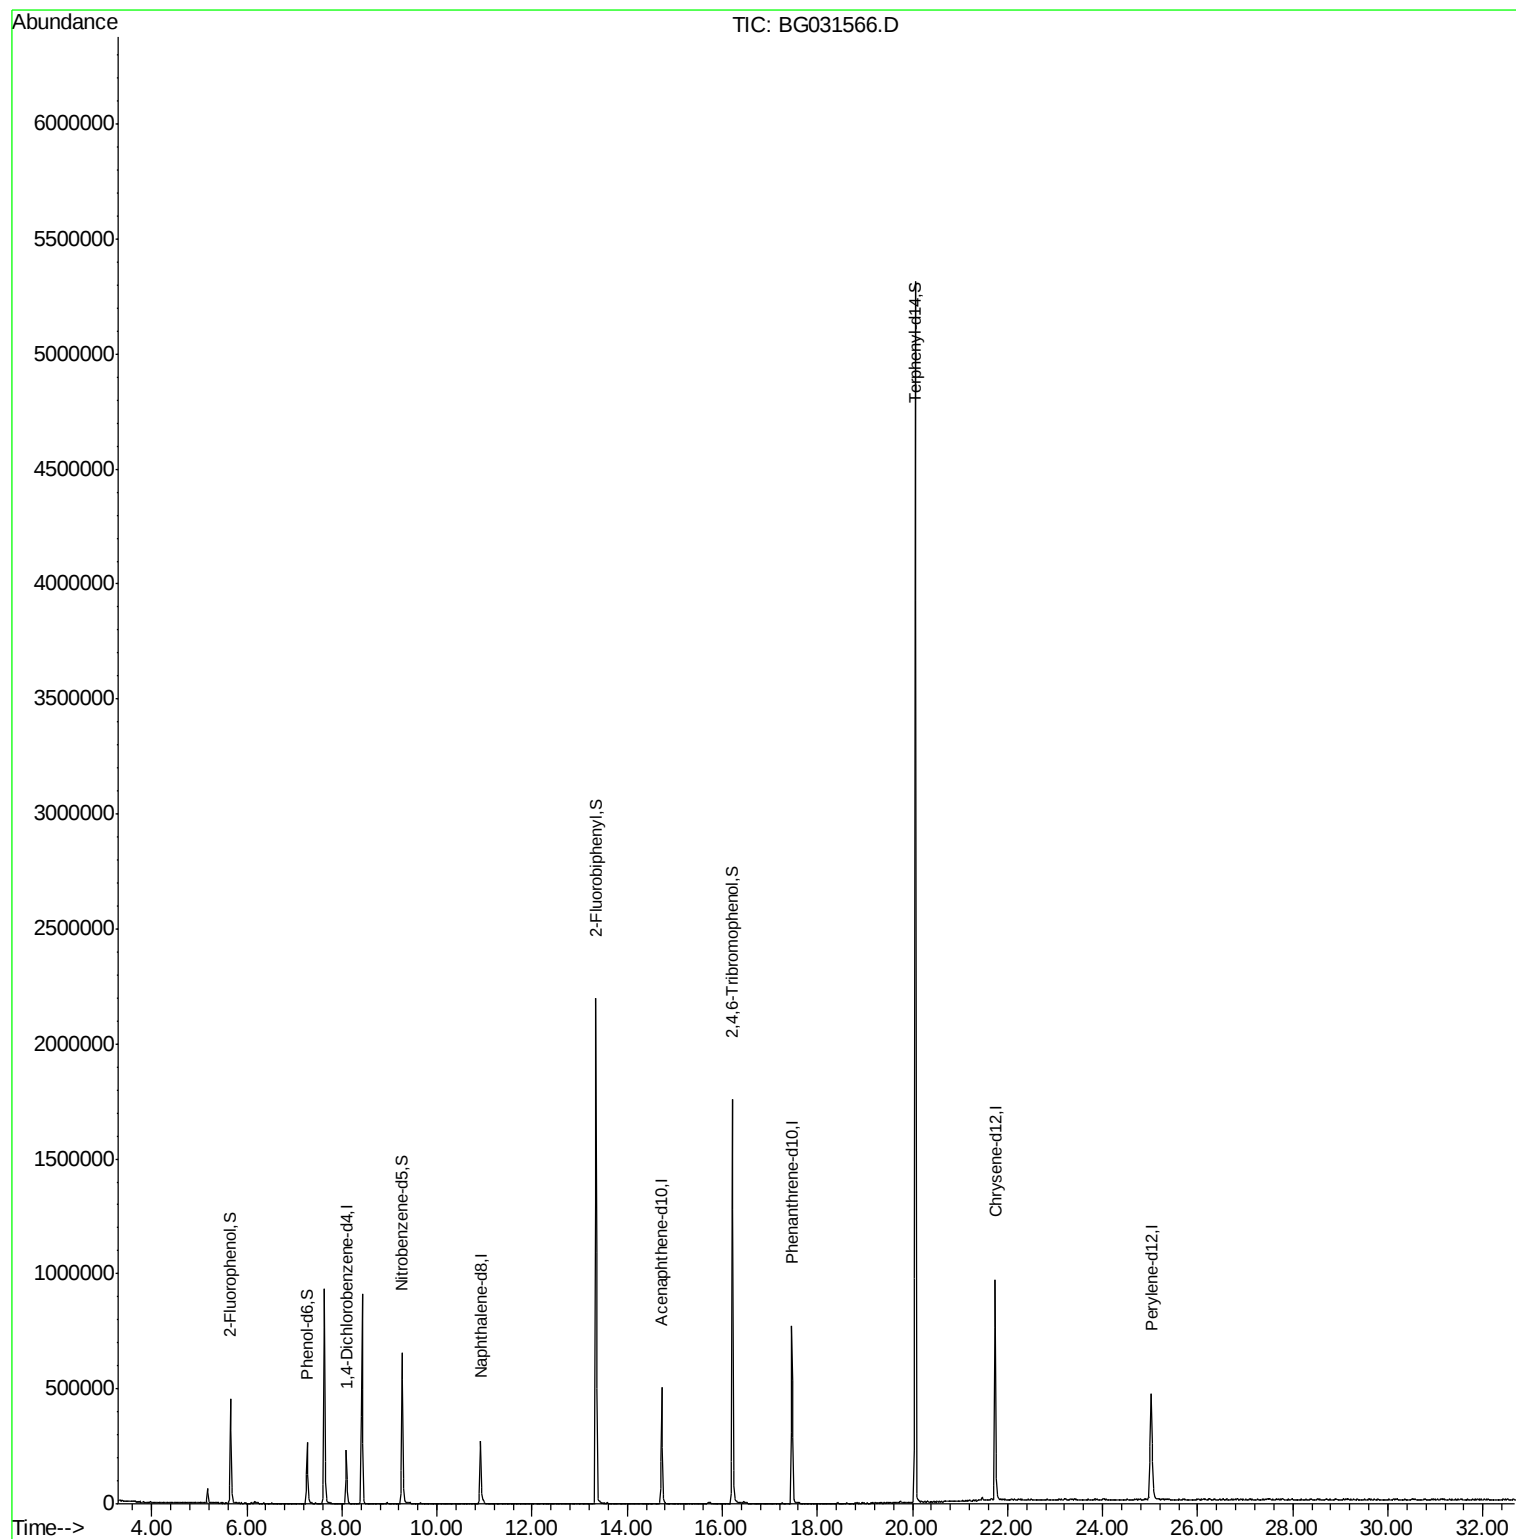

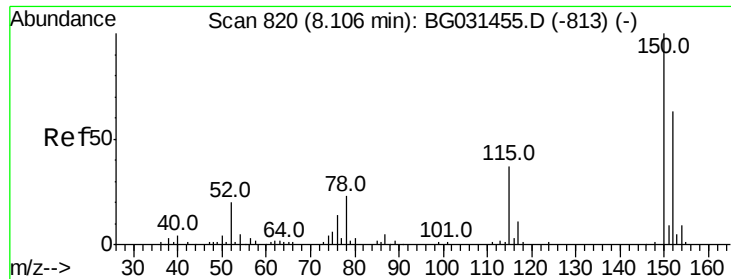


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.09 min Scan# 818
Delta R.T. -0.01 min
Lab File: BG031566.D
Acq: 14 Dec 2017 19:48

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 72758
Ion Ratio Lower Upper
152 100
150 154.3 126.6 189.8
115 58.6 53.0 79.4

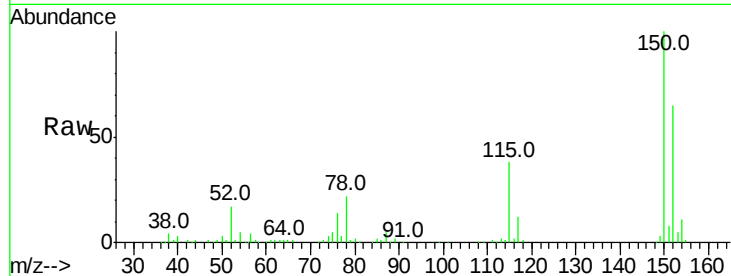


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

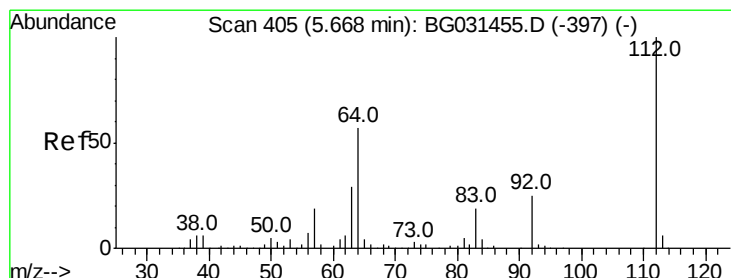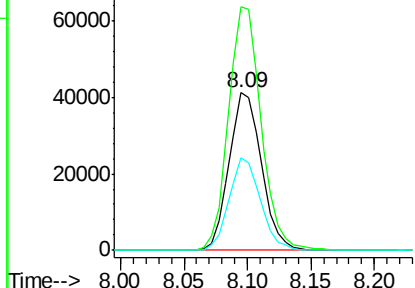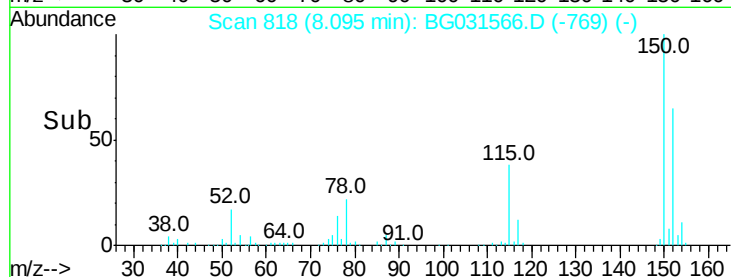



#5


2-Fluorophenol
Concen: 59.763 ng
RT: 5.66 min Scan# 403
Delta R.T. -0.01 min
Lab File: BG031566.D
Acq: 14 Dec 2017 19:48

Tgt Ion:112 Resp: 245313
Ion Ratio Lower Upper
112 100
64 58.3 56.3 84.5
63 29.8 30.1 45.1#

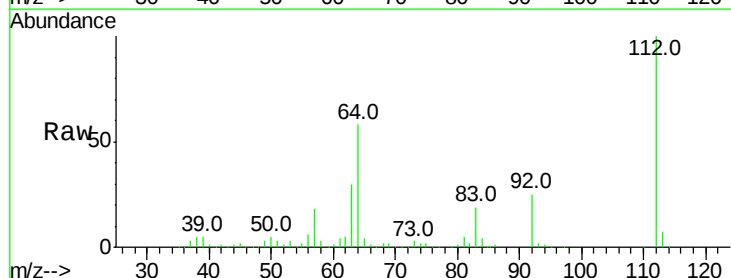

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

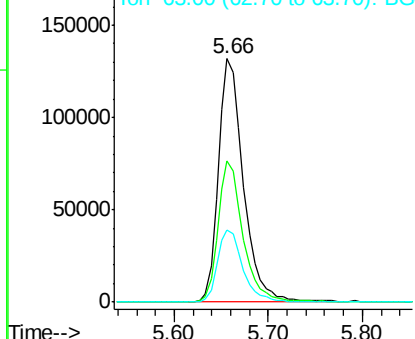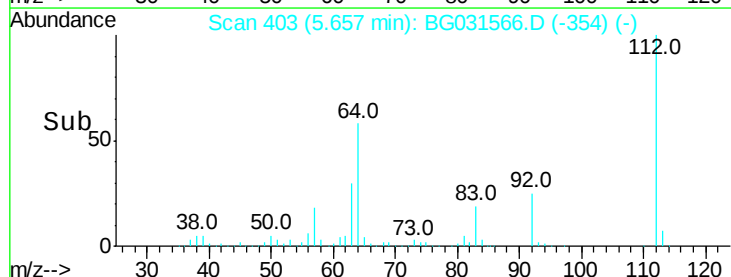

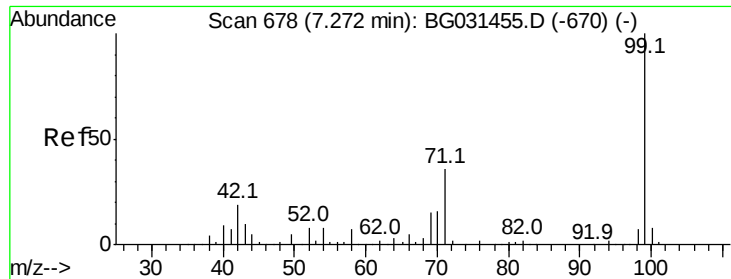

#7

Phenol-d6

Concen: 32.604 ng

RT: 7.27 min Scan# 677

Delta R.T. -0.01 min

Lab File: BG031566.D

Acq: 14 Dec 2017 19:48

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 185793

Ion Ratio Lower Upper




99 100

42 18.3 14.1 21.1

71 36.2 26.1 39.1

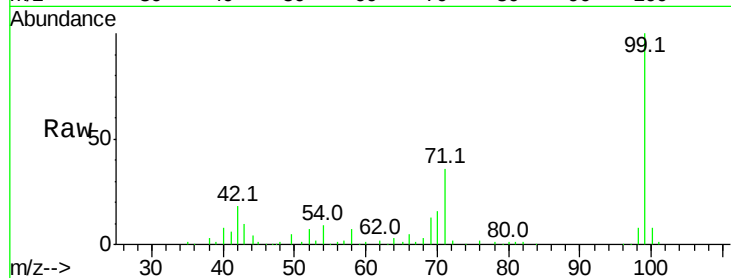

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

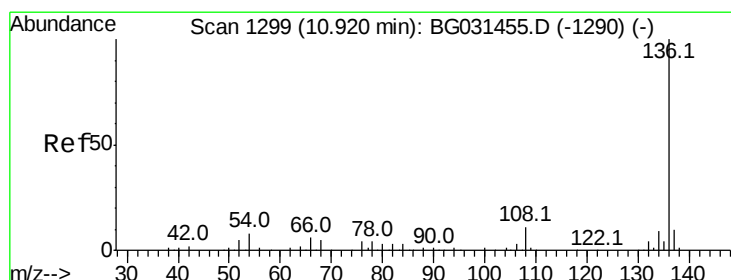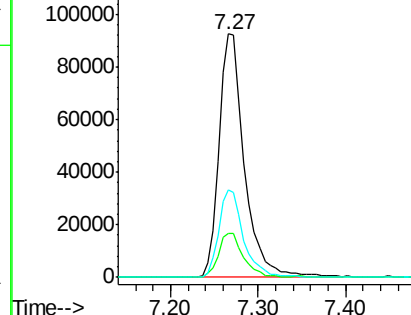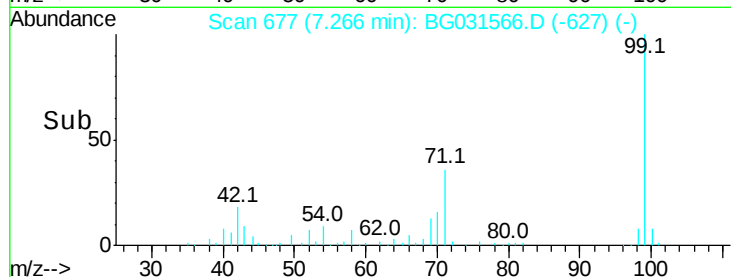

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BG031566.D

Acq: 14 Dec 2017 19:48

Tgt Ion: 136 Resp: 302512


Ion Ratio Lower Upper

136 100



137 11.1 9.2 13.8


54 7.9 10.3 15.5#

68 4.5 4.5 6.7#

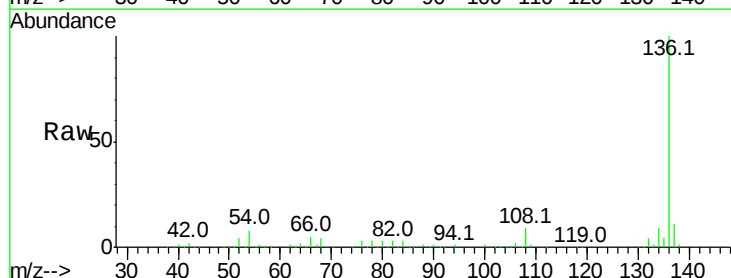

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

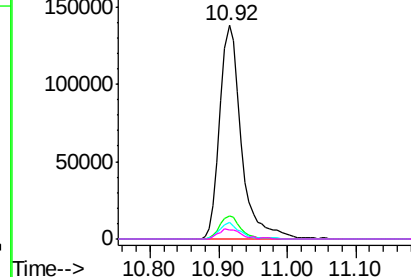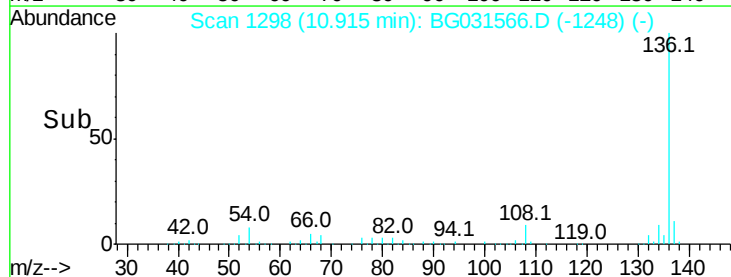


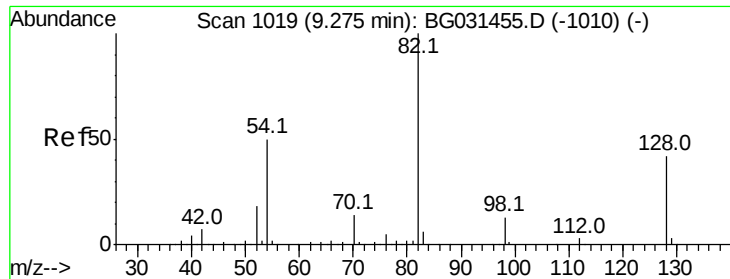




#23
Nitrobenzene-d5
Concen: 90.619 ng
RT: 9.27 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BG031566.D
Acq: 14 Dec 2017 19:48

Instrument :
BNA_G
ClientSampleId :

Tot Ion: 82 Resp: 444758
Ion Ratio Lower Upper
82 100
128 45.7 29.7 44.5#
54 48.2 43.1 64.7

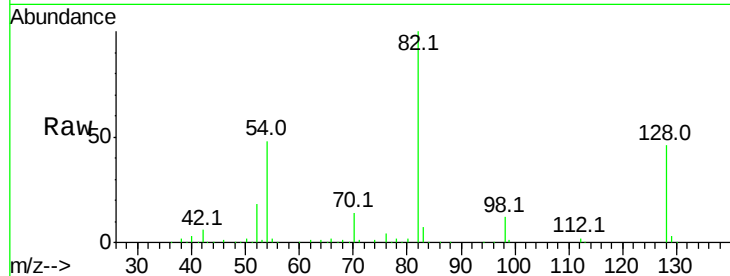


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

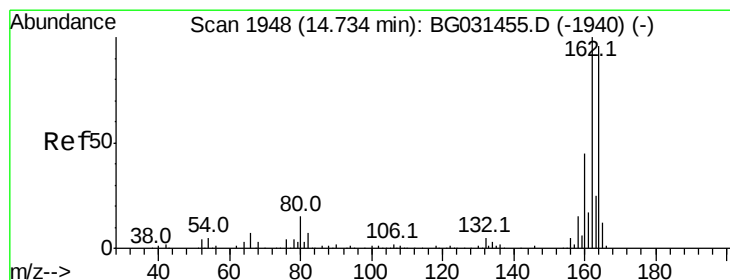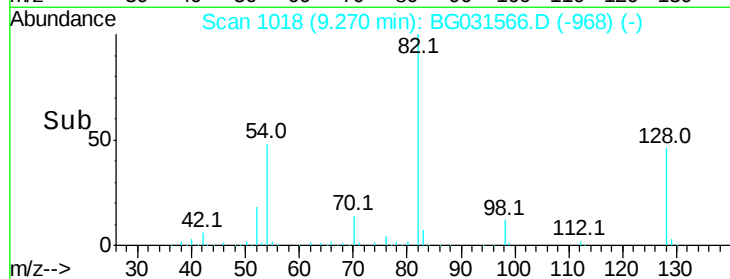
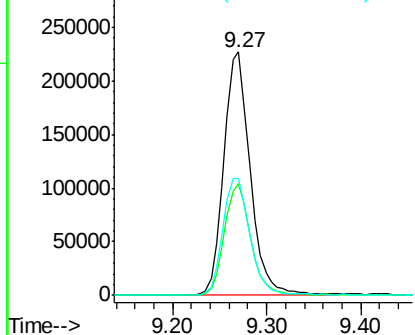



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.72 min Scan# 1946
Delta R.T. -0.01 min
Lab File: BG031566.D
Acq: 14 Dec 2017 19:48

Tgt Ion:164 Resp: 200090
Ion Ratio Lower Upper
164 100
162 103.8 78.8 118.2
160 46.2 35.4 53.0

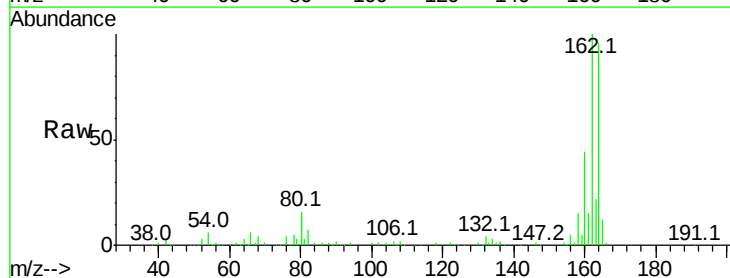

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

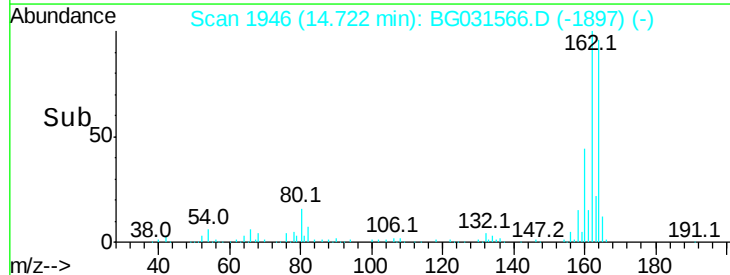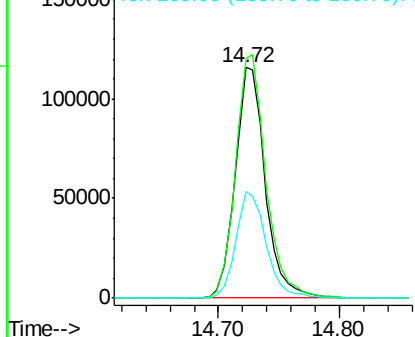


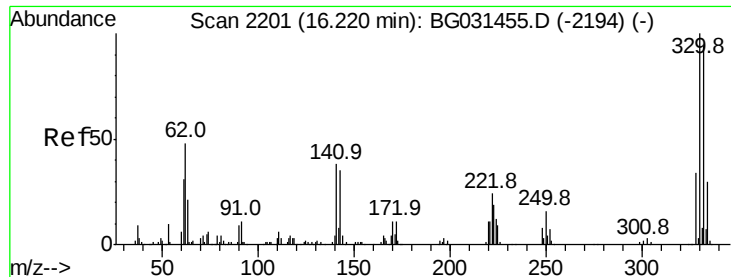




#41
 2,4,6-Tribromophenol
 Concen: 155.980 ng
 RT: 16.21 min Scan# 2200
 Delta R.T. -0.01 min
 Lab File: BG031566.D
 Acq: 14 Dec 2017 19:48

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.0	115.6
141	35.9	25.2	37.8

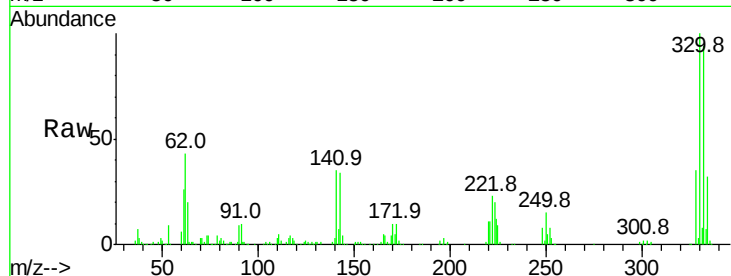


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

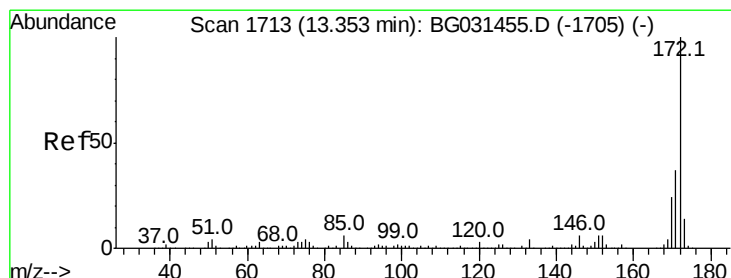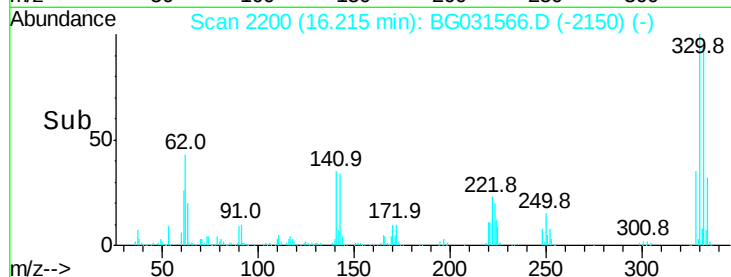
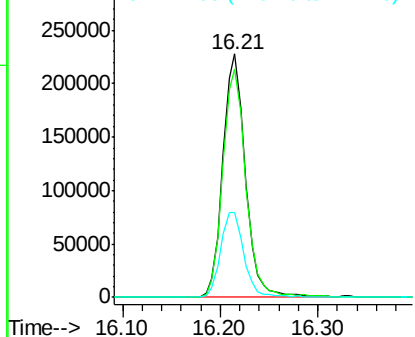


#44
 2-Fluorobiphenyl
 Concen: 93.976 ng
 RT: 13.35 min Scan# 1712
 Delta R.T. -0.01 min
 Lab File: BG031566.D
 Acq: 14 Dec 2017 19:48

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.4	30.0	45.0
170	24.8	19.5	29.3

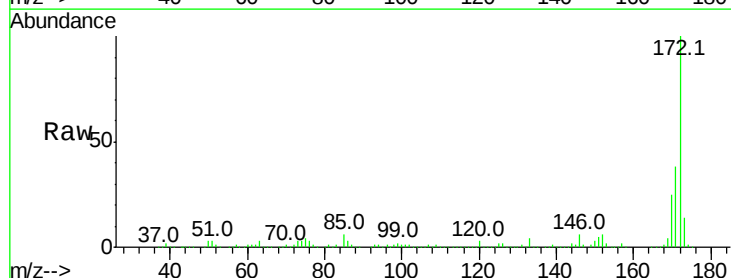

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



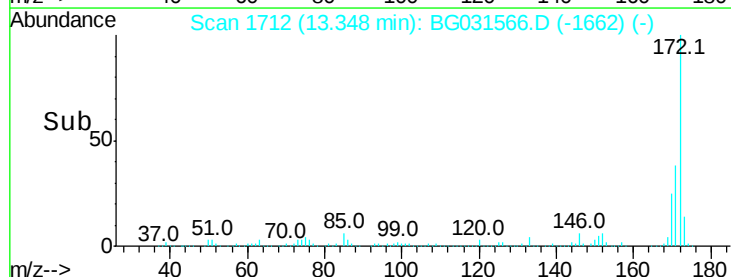
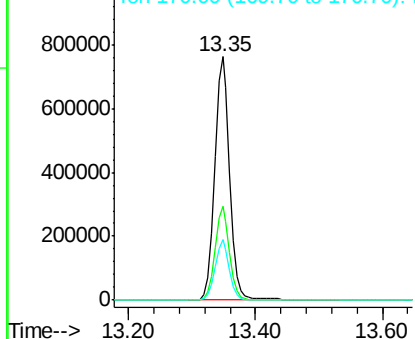




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2413
Delta R.T. -0.01 min
Lab File: BG031566.D
Acq: 14 Dec 2017 19:48




Instrument :
BNA_G
ClientSampleId :


Tot Ion:188 Resp: 534523
Ion Ratio Lower Upper
188 100
94 7.2 6.9 10.3
80 8.2 7.7 11.5

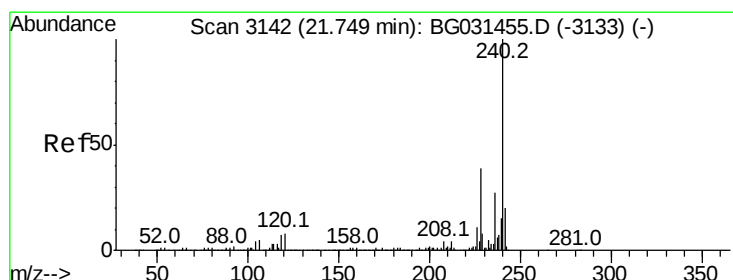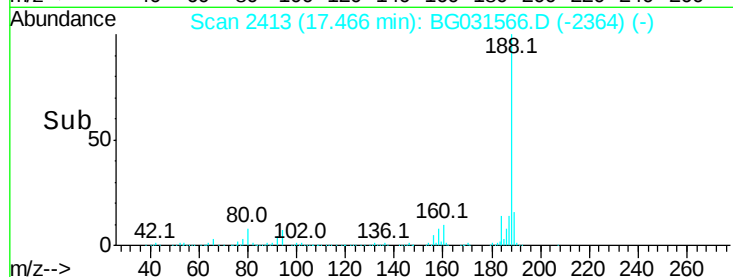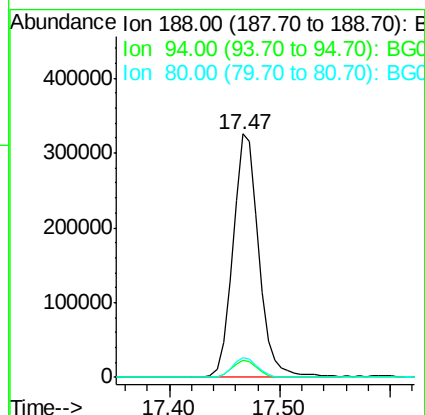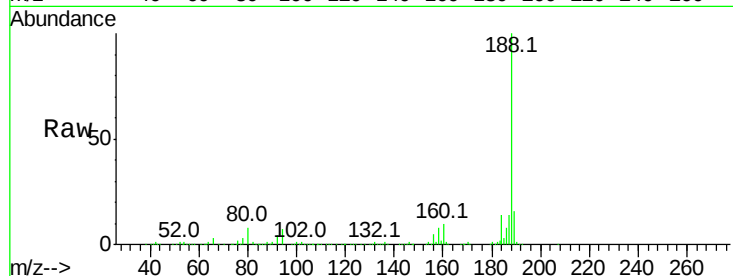

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.74 min Scan# 3140
Delta R.T. -0.01 min
Lab File: BG031566.D
Acq: 14 Dec 2017 19:48

Tgt Ion:240 Resp: 647336
Ion Ratio Lower Upper
240 100
120 7.7 6.8 10.2
236 26.7 20.9 31.3

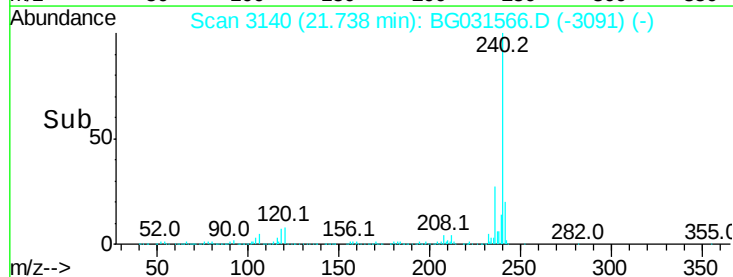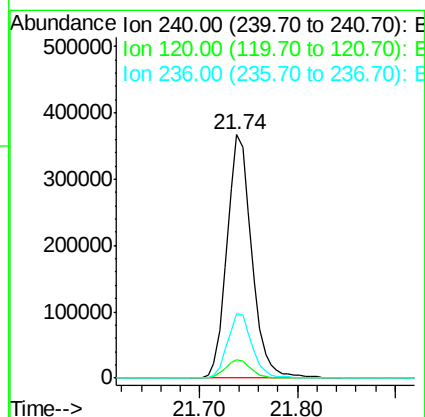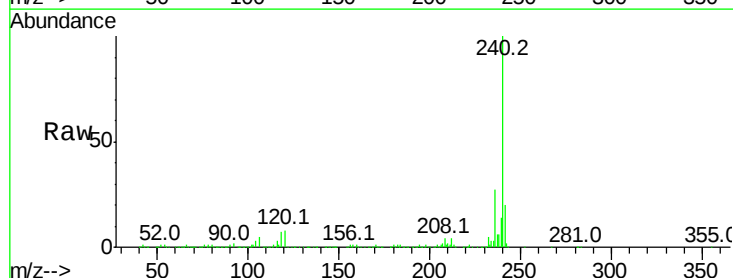

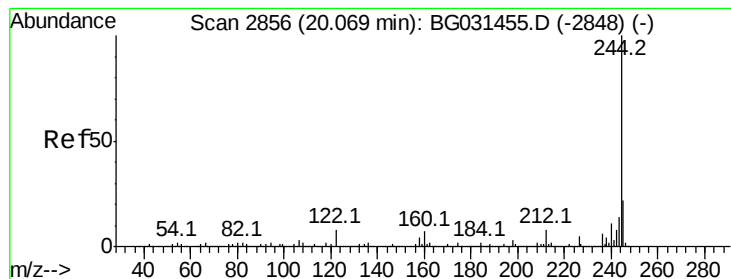

#78

Terphenyl-d14

Concen: 86.051 ng

RT: 20.06 min Scan# 2855

Delta R.T. -0.01 min

Lab File: BG031566.D

Acq: 14 Dec 2017 19:48

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 2448355

Ion Ratio Lower Upper

244 100

212 9.7 5.8 8.8#




122 9.4 7.0 10.4

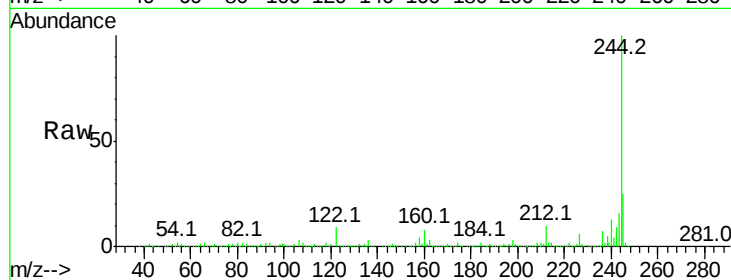

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

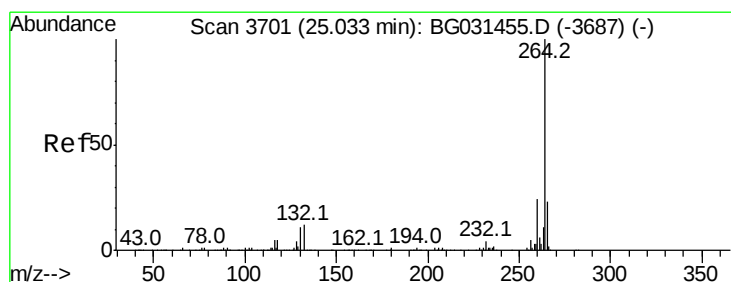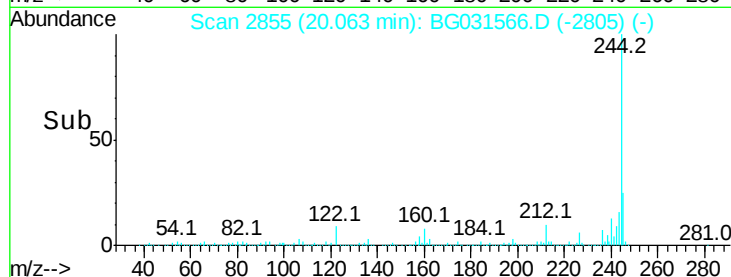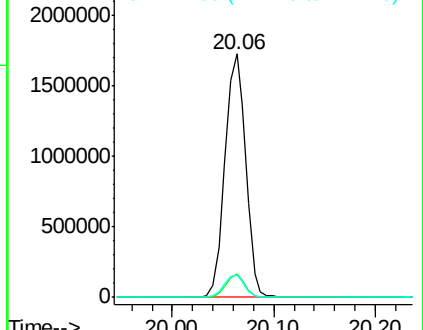

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.02 min Scan# 3698

Delta R.T. -0.02 min

Lab File: BG031566.D

Acq: 14 Dec 2017 19:48


Tgt Ion:264 Resp: 561655

Ion Ratio Lower Upper

264 100

260 24.1 17.4 26.0

265 21.4 17.7 26.5

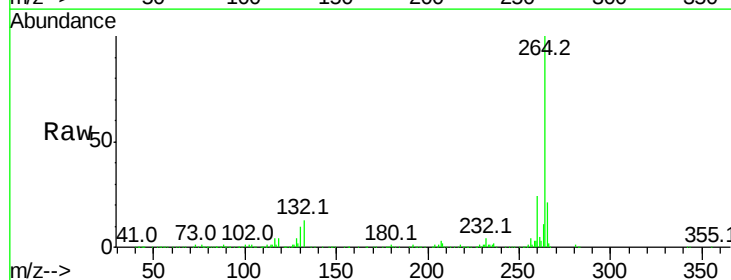

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

