

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121417\
 Data File : BG031569.D
 Acq On : 14 Dec 2017 21:41
 Operator : SJ/JU
 Sample : I6884-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 15 03:16:39 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 17:25:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	68200	20.00	ng	0.00
21) Naphthalene-d8	10.91	136	284221	20.00	ng	0.00
38) Acenaphthene-d10	14.73	164	188071	20.00	ng	0.00
63) Phenanthrene-d10	17.46	188	496838	20.00	ng	-0.01
75) Chrysene-d12	21.74	240	599603	20.00	ng	-0.01
86) Perylene-d12	25.01	264	530821	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	221325	57.52	ng	0.00
7) Phenol-d6	7.27	99	165763	31.03	ng	0.00
23) Nitrobenzene-d5	9.27	82	417442	90.53	ng	0.00
41) 2,4,6-Tribromophenol	16.21	330	343305	155.81	ng	0.00
44) 2-Fluorobiphenyl	13.35	172	1195612	93.32	ng	0.00
78) Terphenyl-d14	20.06	244	2199989	83.48	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121417\
Data File : BG031569.D
Acq On : 14 Dec 2017 21:41
Operator : SJ/JU
Sample : I6884-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 15 03:16:39 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

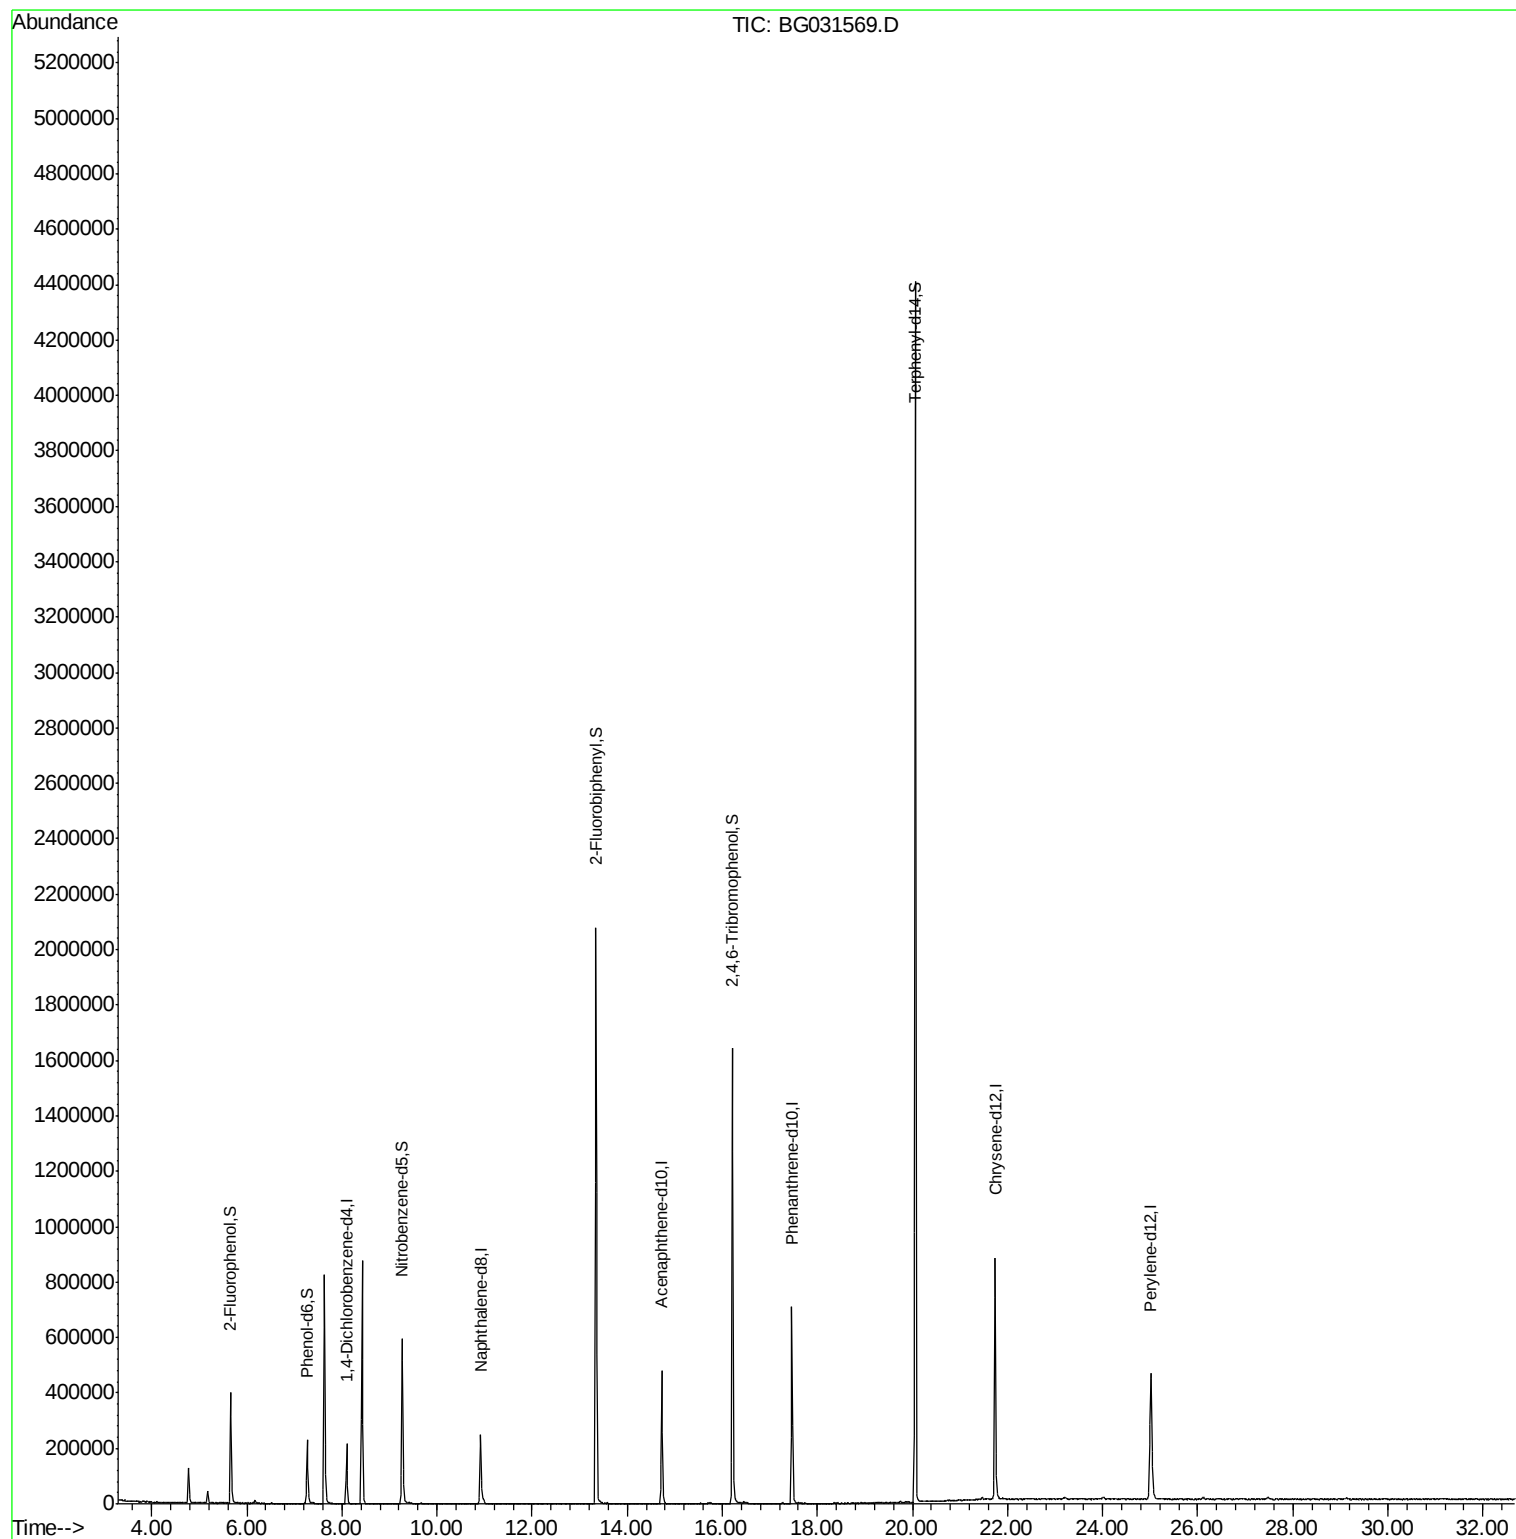

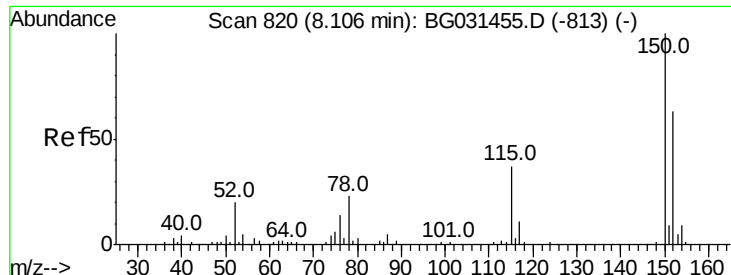


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG031569.D
Acq: 14 Dec 2017 21:41

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 68200
Ion Ratio Lower Upper
152 100
150 157.3 126.6 189.8
115 58.5 53.0 79.4

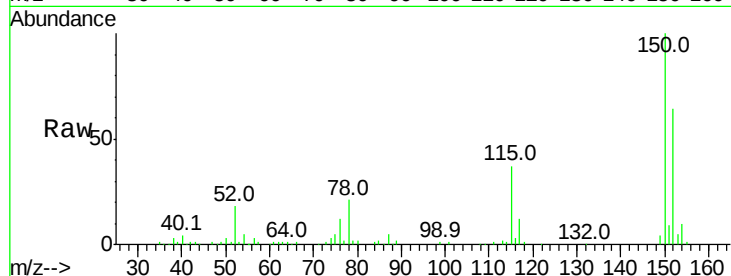


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

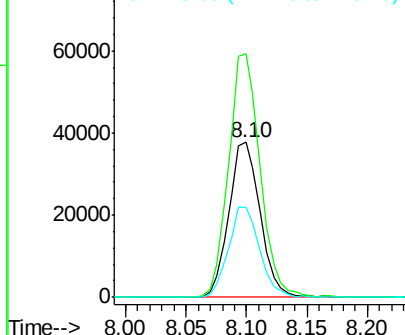



#5

2-Fluorophenol
Concen: 57.522 ng
RT: 5.66 min Scan# 404
Delta R.T. -0.01 min
Lab File: BG031569.D
Acq: 14 Dec 2017 21:41

Tgt Ion:112 Resp: 221325
Ion Ratio Lower Upper
112 100
64 52.9 56.3 84.5#
63 29.6 30.1 45.1#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

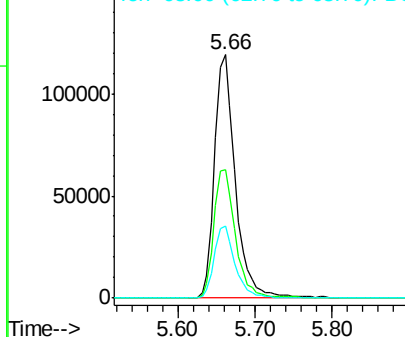



#7

Phenol-d6

Concen: 31.034 ng

RT: 7.27 min Scan# 678

Delta R.T. -0.00 min

Lab File: BG031569.D

Acq: 14 Dec 2017 21:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 165763

Ion Ratio Lower Upper




99 100

42 17.2 14.1 21.1

71 33.1 26.1 39.1



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

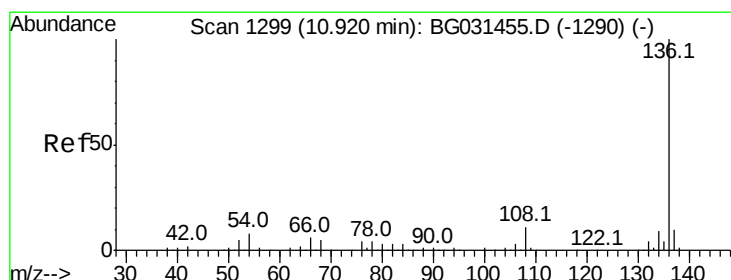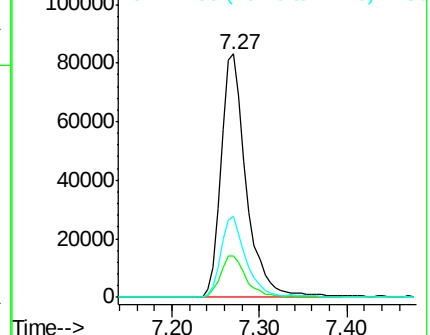

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.91 min Scan# 1298

Delta R.T. -0.01 min

Lab File: BG031569.D

Acq: 14 Dec 2017 21:41

Tgt Ion: 136 Resp: 284221


Ion Ratio Lower Upper

136 100



137 10.4 9.2 13.8


54 7.1 10.3 15.5#

68 5.8 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




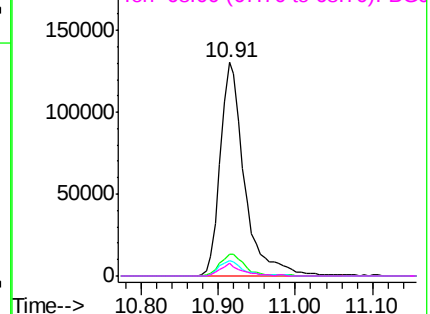


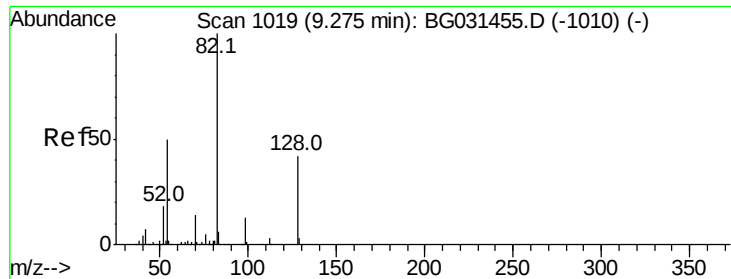

#23
Nitrobenzene-d5
Concen: 90.527 ng
RT: 9.27 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BG031569.D
Acq: 14 Dec 2017 21:41




Instrument :
BNA_G
ClientSampled :


Tot Ion: 82 Resp: 417442
Ion Ratio Lower Upper
82 100
128 46.0 29.7 44.5#
54 49.4 43.1 64.7

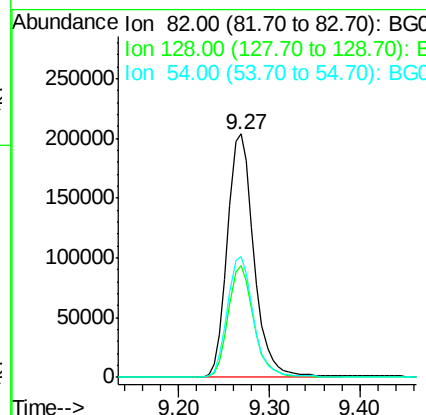

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.73 min Scan# 1947
Delta R.T. -0.01 min
Lab File: BG031569.D
Acq: 14 Dec 2017 21:41

Tgt Ion:164 Resp: 188071
Ion Ratio Lower Upper
164 100
162 102.8 78.8 118.2
160 46.6 35.4 53.0

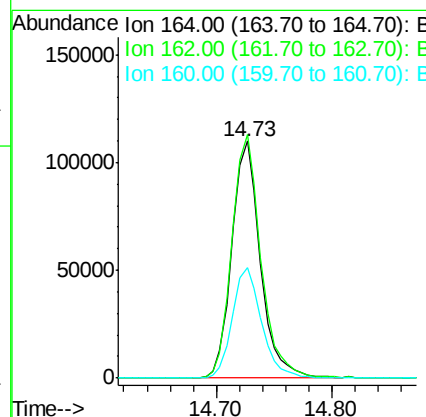


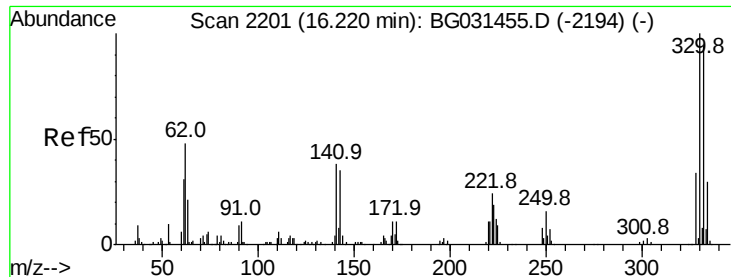




#41
 2,4,6-Tribromophenol
 Concen: 155.812 ng
 RT: 16.21 min Scan# 2200
 Delta R.T. -0.01 min
 Lab File: BG031569.D
 Acq: 14 Dec 2017 21:41

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.5	77.0	115.6
141	34.8	25.2	37.8

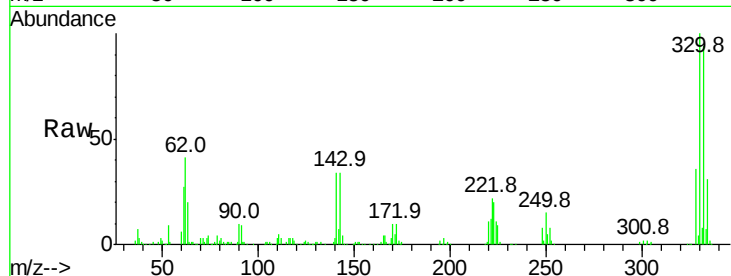


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

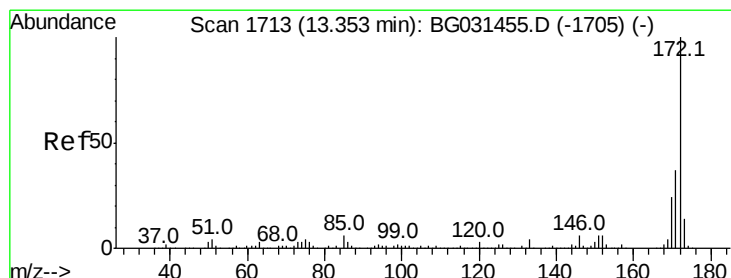
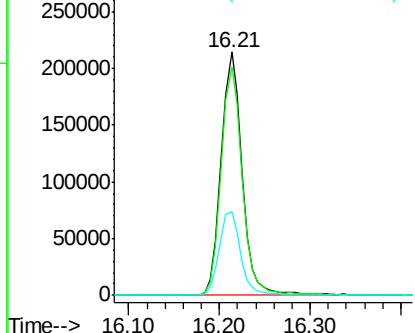


#44
 2-Fluorobiphenyl
 Concen: 93.316 ng
 RT: 13.35 min Scan# 1712
 Delta R.T. -0.01 min
 Lab File: BG031569.D
 Acq: 14 Dec 2017 21:41

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	30.0	45.0
170	23.2	19.5	29.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




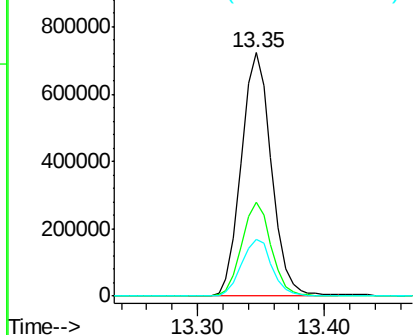




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.46 min Scan# 2413
Delta R.T. -0.01 min
Lab File: BG031569.D
Acq: 14 Dec 2017 21:41




Instrument :
BNA_G
ClientSampleId :


Tot Ion:188 Resp: 496838
Ion Ratio Lower Upper
188 100
94 7.1 6.9 10.3
80 8.4 7.7 11.5

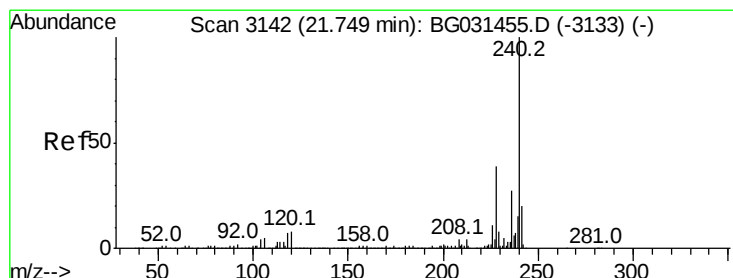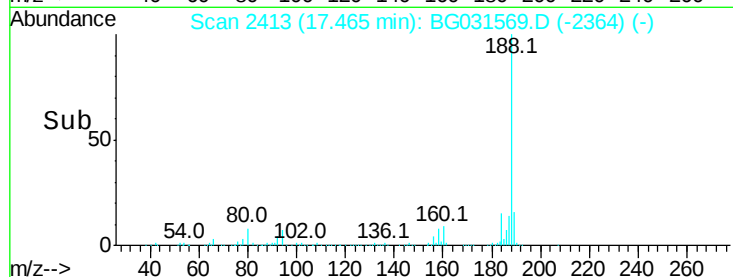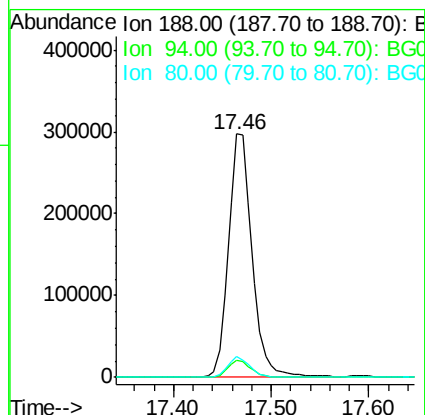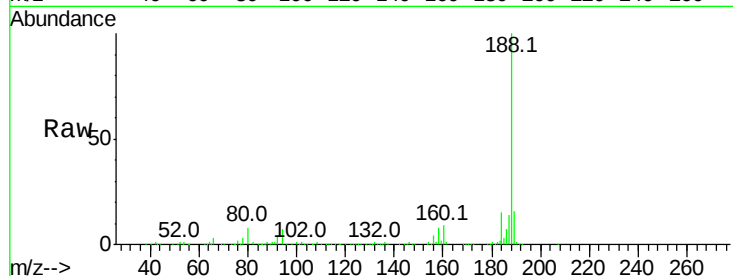

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.74 min Scan# 3140
Delta R.T. -0.01 min
Lab File: BG031569.D
Acq: 14 Dec 2017 21:41

Tgt Ion:240 Resp: 599603
Ion Ratio Lower Upper
240 100
120 8.4 6.8 10.2
236 26.4 20.9 31.3

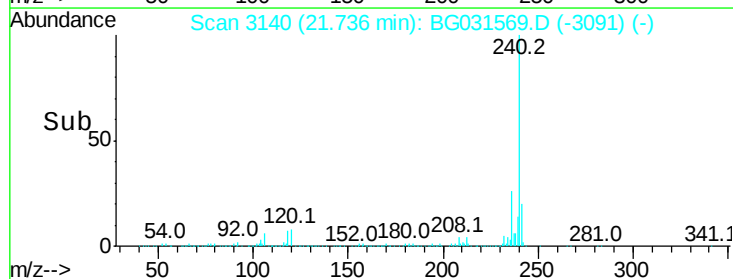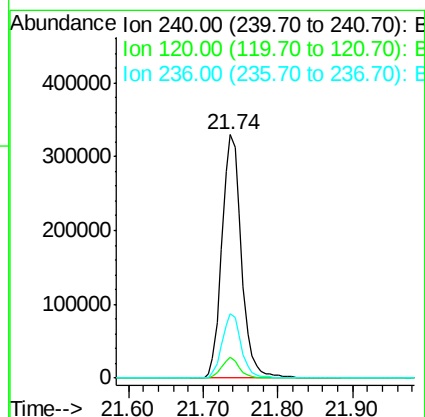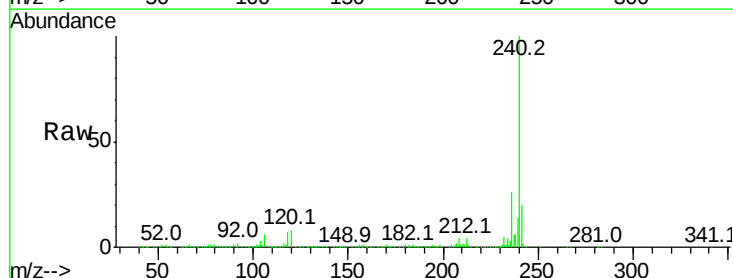



#78

Terphenyl-d14

Concen: 83.477 ng

RT: 20.06 min Scan# 2855

Delta R.T. -0.01 min

Lab File: BG031569.D

Acq: 14 Dec 2017 21:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 2199989

Ion Ratio Lower Upper

244 100

212 8.7 5.8 8.8




122 8.7 7.0 10.4

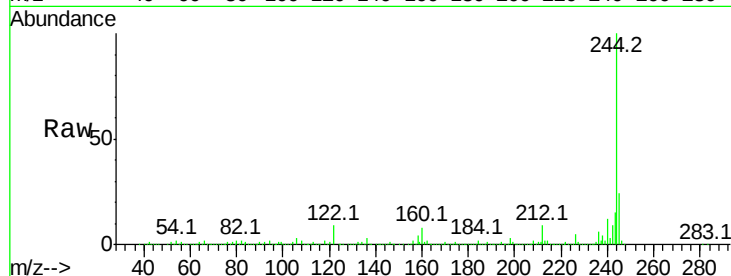

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

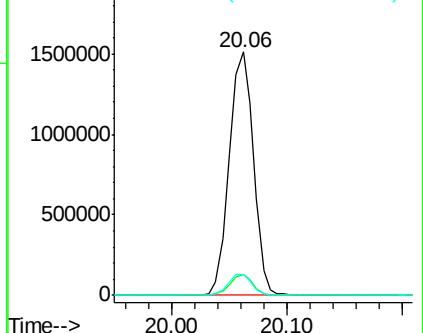

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.01 min Scan# 3698

Delta R.T. -0.02 min

Lab File: BG031569.D

Acq: 14 Dec 2017 21:41


Tgt Ion:264 Resp: 530821

Ion Ratio Lower Upper

264 100

260 24.7 17.4 26.0

265 22.2 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

