

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121417\
 Data File : BG031586.D
 Acq On : 15 Dec 2017 8:59
 Operator : SJ/JU
 Sample : I6679-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 15 09:56:49 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 17:25:55 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	80157	20.00	ng	0.00
21) Naphthalene-d8	10.92	136	337413	20.00	ng	0.00
38) Acenaphthene-d10	14.72	164	212874	20.00	ng	0.00
63) Phenanthrene-d10	17.47	188	550050	20.00	ng	0.00
75) Chrysene-d12	21.73	240	642231	20.00	ng	-0.02
86) Perylene-d12	25.02	264	548022	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	541254	119.69	ng	0.00
7) Phenol-d6	7.27	99	624169	99.42	ng	0.00
23) Nitrobenzene-d5	9.27	82	445935	81.46	ng	0.00
41) 2,4,6-Tribromophenol	16.21	330	347713	139.42	ng	0.00
44) 2-Fluorobiphenyl	13.34	172	1243650	85.76	ng	0.00
78) Terphenyl-d14	20.06	244	2229778	78.99	ng	0.00
Target Compounds						
31) Naphthalene	10.96	128	49986	3.016	ng	99
40) Hexachlorocyclopentadiene	13.01	237	60	8.693	ng	# 22
55) 4-Nitrophenol	15.15	139	1495	4.093	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121417\
Data File : BG031586.D
Acq On : 15 Dec 2017 8:59
Operator : SJ/JU
Sample : I6679-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 15 09:56:49 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

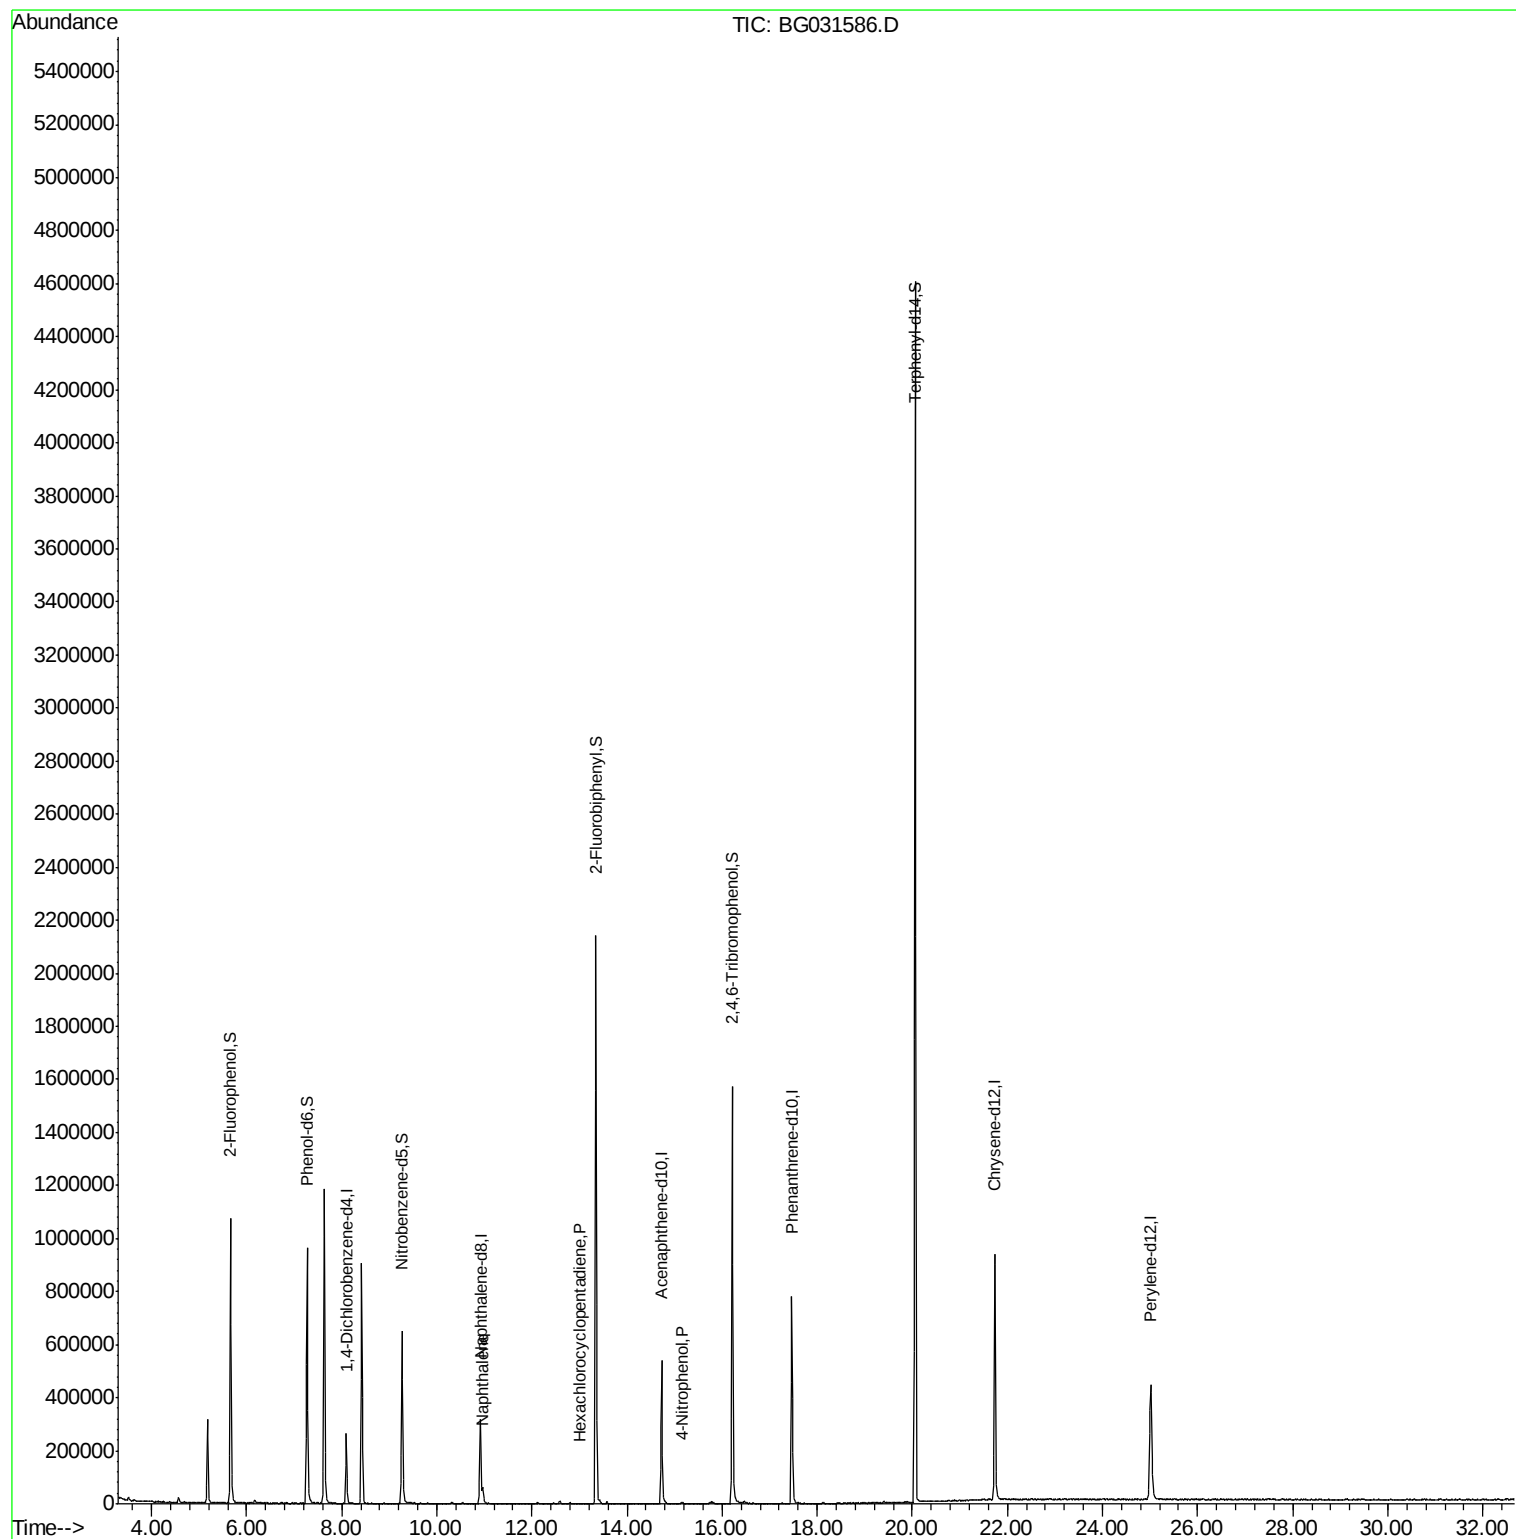

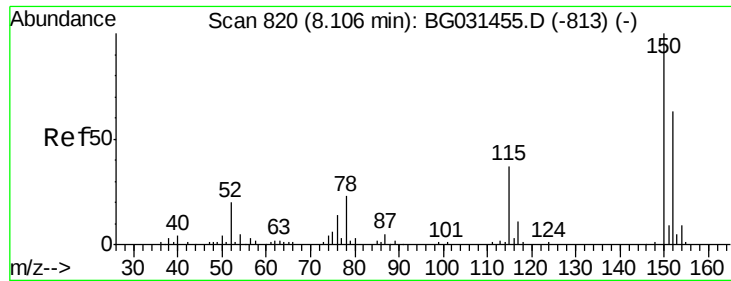


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 818
Delta R.T. -0.01 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59

Instrument :
BNA_G
ClientSampled :

Tot Ion:152 Resp: 80157
Ion Ratio Lower Upper
152 100
150 158.0 126.6 189.8
115 56.0 53.0 79.4

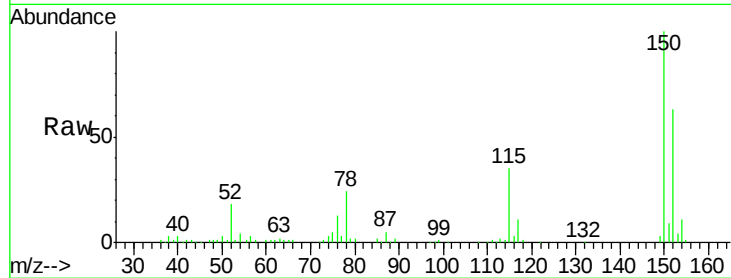


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

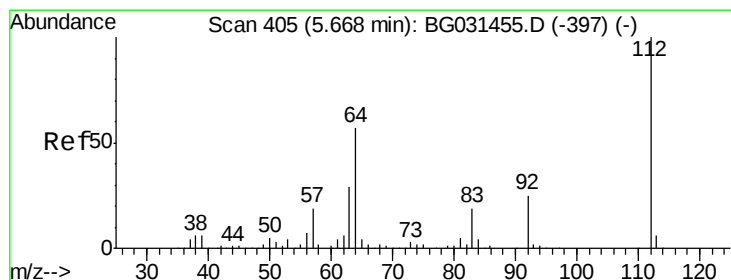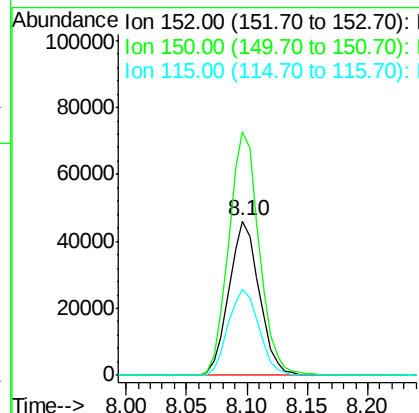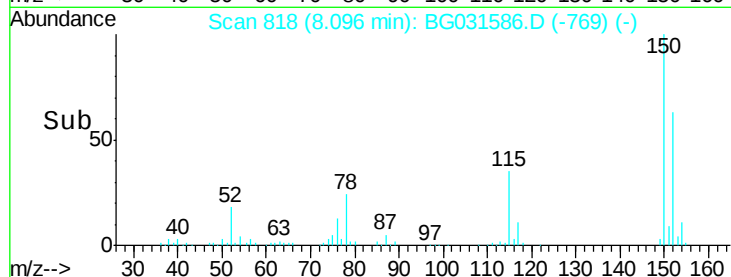



#5


2-Fluorophenol
Concen: 119.688 ng
RT: 5.66 min Scan# 403
Delta R.T. -0.01 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59

Tgt Ion:112 Resp: 541254
Ion Ratio Lower Upper
112 100
64 57.3 56.3 84.5
63 29.3 30.1 45.1#

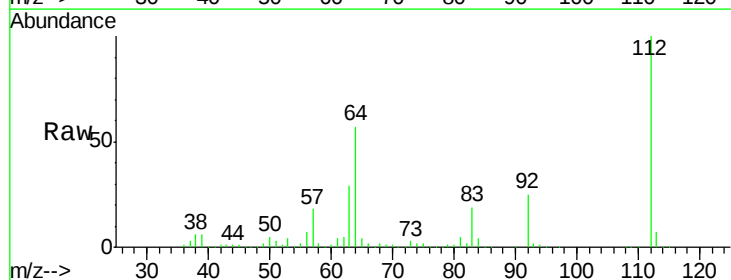

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

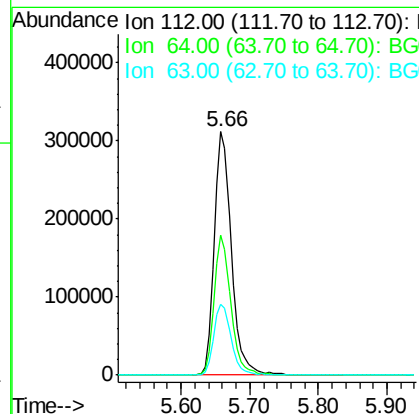

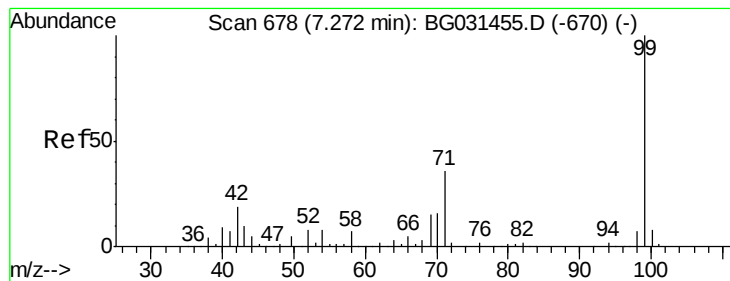

#7

Phenol-d6

Concen: 99.423 ng

RT: 7.27 min Scan# 677

Delta R.T. -0.00 min

Lab File: BG031586.D

Acq: 15 Dec 2017 8:59

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 624169

Ion Ratio Lower Upper




99 100

42 17.8 14.1 21.1

71 34.8 26.1 39.1

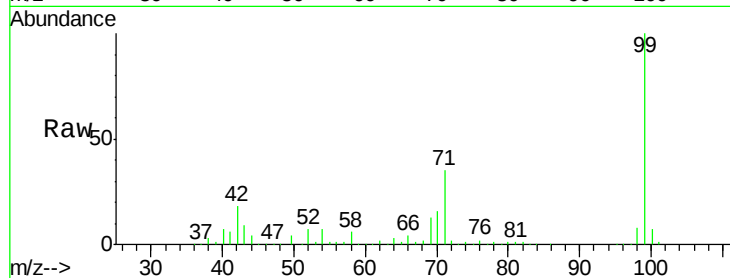

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

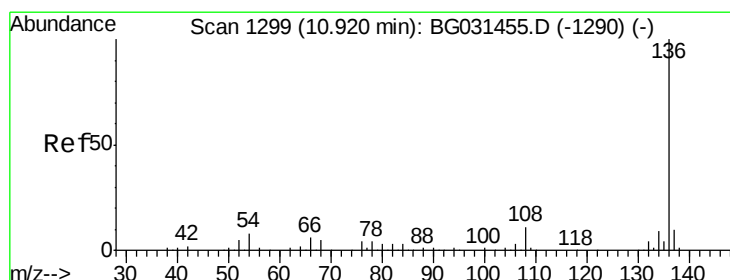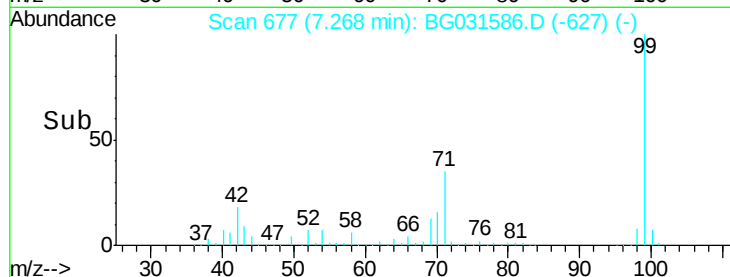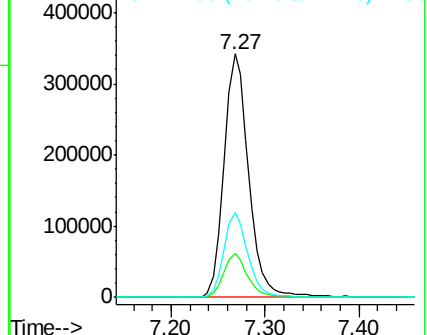

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.92 min Scan# 1298

Delta R.T. -0.00 min

Lab File: BG031586.D

Acq: 15 Dec 2017 8:59

Tgt Ion: 136 Resp: 337413


Ion Ratio Lower Upper

136 100



137 11.0 9.2 13.8


54 7.1 10.3 15.5#

68 4.5 4.5 6.7#

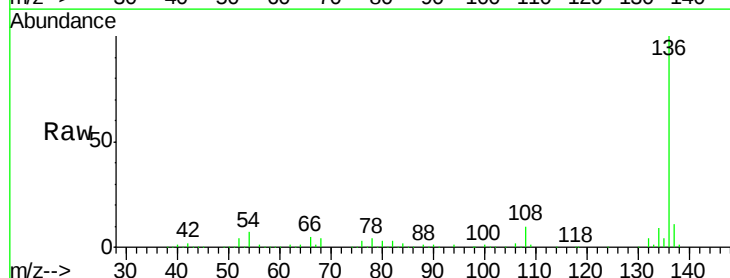

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



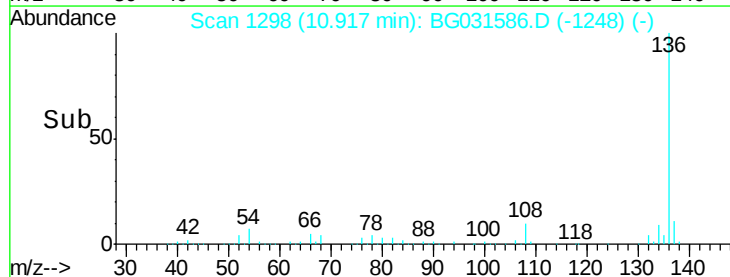
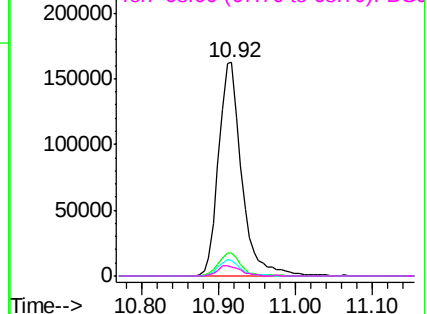




#23
 Nitrobenzene-d5
 Concen: 81.461 ng
 RT: 9.27 min Scan# 1017
 Delta R.T. -0.01 min
 Lab File: BG031586.D
 Acq: 15 Dec 2017 8:59




Instrument :
 BNA_G
 ClientSampled :


Tot Ion	82	Resp	445935
Ion Ratio	Lower	Upper	
82	100		
128	47.1	29.7	44.5#
54	48.3	43.1	64.7

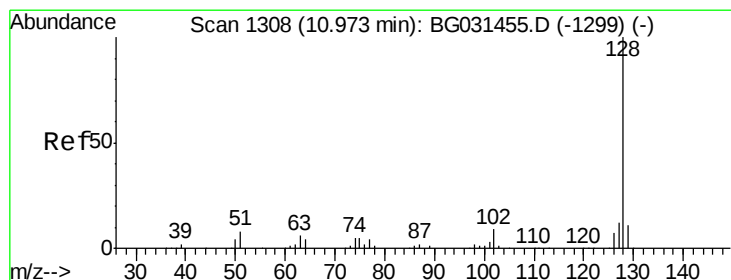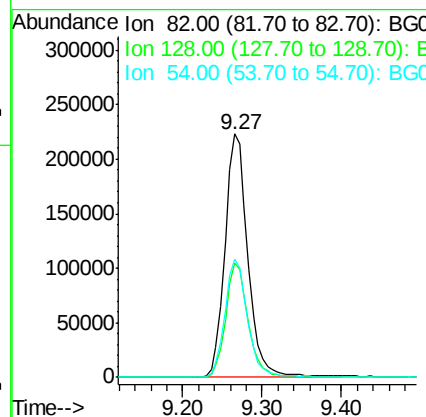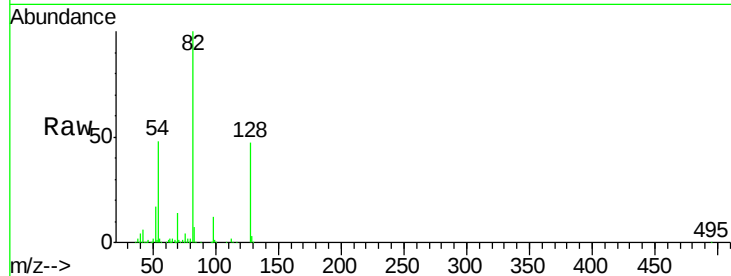

#31
 Naphthalene
 Concen: 3.016 ng
 RT: 10.96 min Scan# 1306
 Delta R.T. -0.01 min
 Lab File: BG031586.D
 Acq: 15 Dec 2017 8:59

Tgt Ion	128	Resp	49986
Ion Ratio	Lower	Upper	
128	100		
129	11.4	8.6	12.8
127	14.8	11.6	17.4


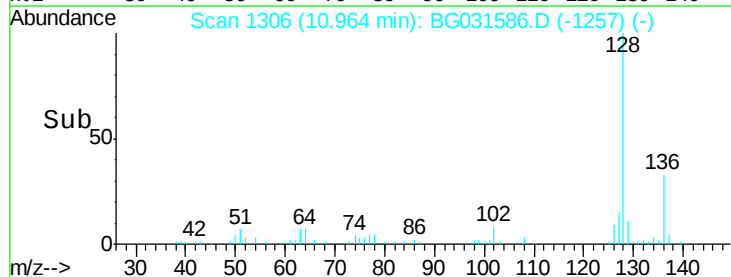
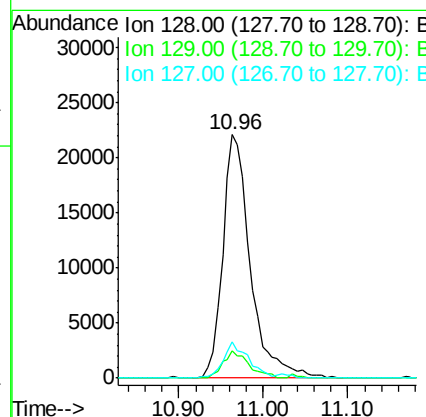
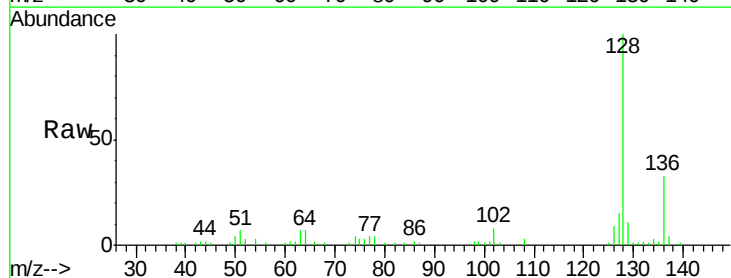




#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.72 min Scan# 1946
Delta R.T. -0.01 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	104.6	78.8	118.2
160	45.0	35.4	53.0

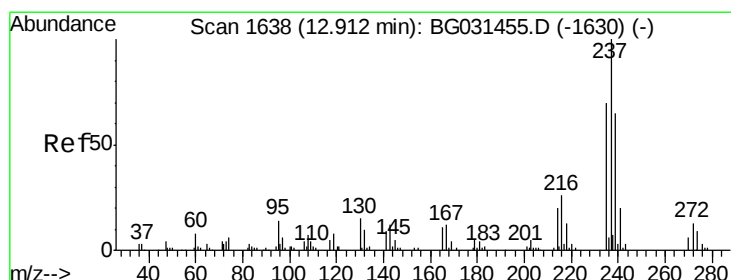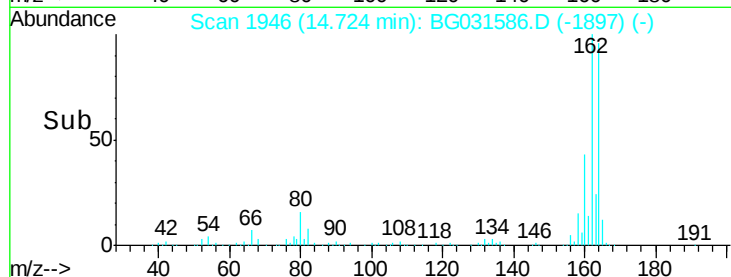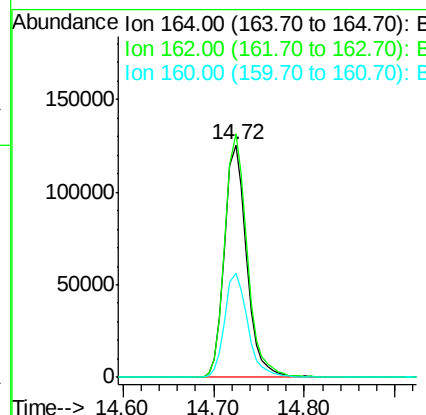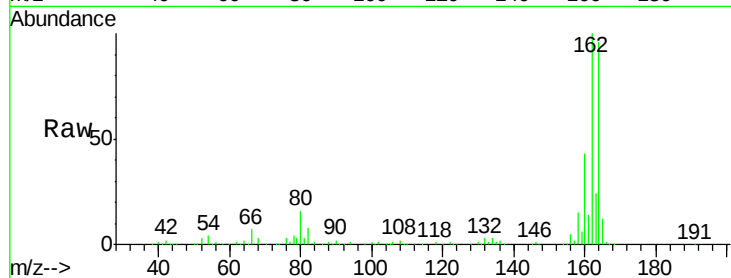

#40
Hexachlorocyclopentadiene
Concen: 8.693 ng
RT: 13.01 min Scan# 1654
Delta R.T. 0.10 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59

Tgt Ion	Ratio	Lower	Upper
237	100		
235	0.0	50.4	90.4#
272	0.0	0.0	31.8

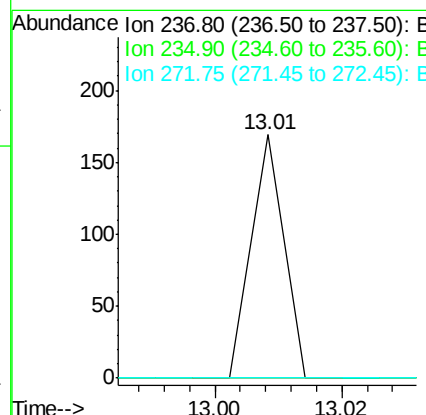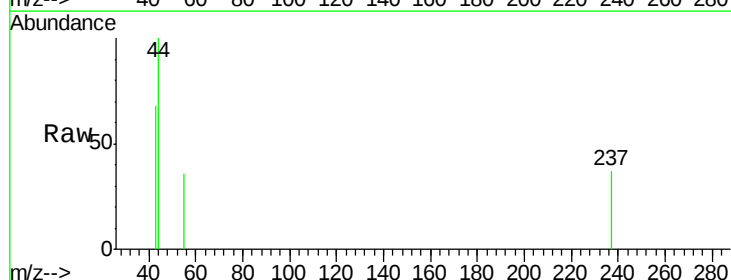







#41
 2,4,6-Tribromophenol
 Concen: 139.425 ng
 RT: 16.21 min Scan# 2199
 Delta R.T. -0.01 min
 Lab File: BG031586.D
 Acq: 15 Dec 2017 8:59

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:330 Resp: 347713
 Ion Ratio Lower Upper
 330 100
 332 95.3 77.0 115.6
 141 34.7 25.2 37.8

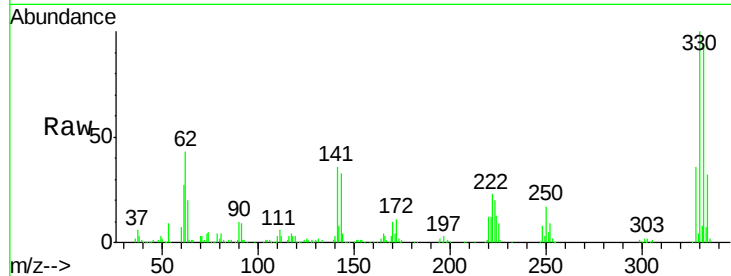


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

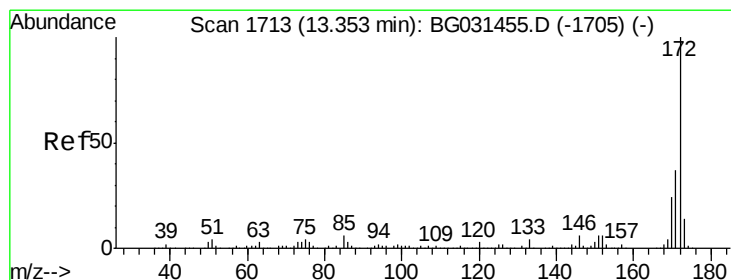
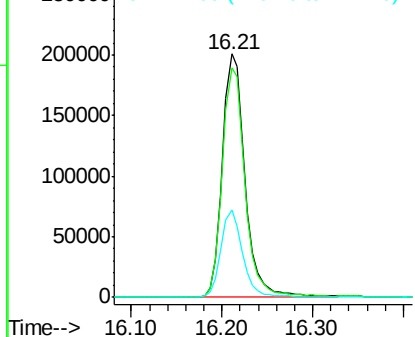



#44
 2-Fluorobiphenyl
 Concen: 85.756 ng
 RT: 13.34 min Scan# 1711
 Delta R.T. -0.01 min
 Lab File: BG031586.D
 Acq: 15 Dec 2017 8:59

Tgt Ion:172 Resp: 1243650
 Ion Ratio Lower Upper
 172 100
 171 37.7 30.0 45.0
 170 24.1 19.5 29.3

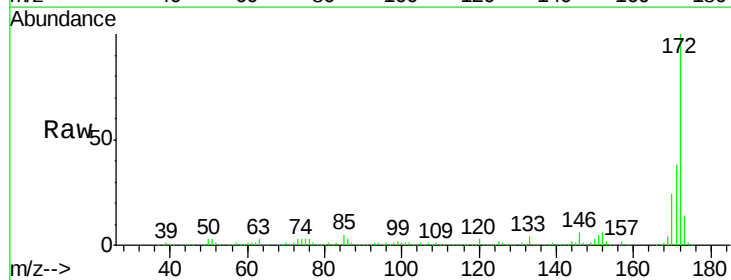

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

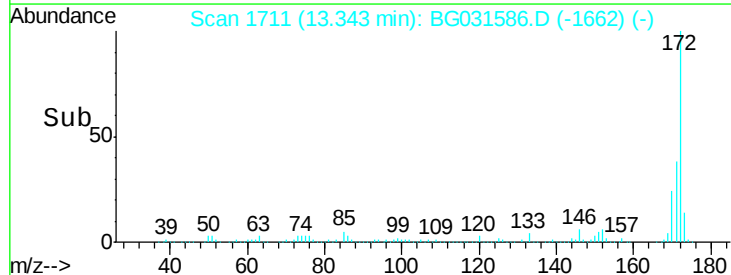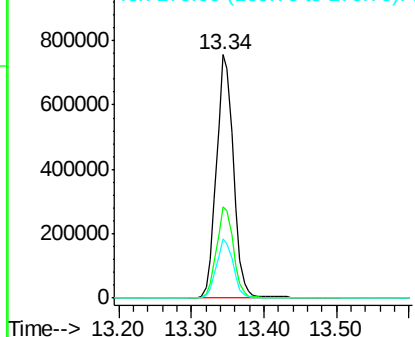







#55
4-Nitrophenol
Concen: 4.093 ng
RT: 15.15 min Scan# 2018
Delta R.T. 0.18 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59

Instrument :
BNA_G
ClientSampled :

Tot Ion:139 Resp: 1495
Ion Ratio Lower Upper
139 100
109 0.0 62.2 102.2#
65 0.0 97.2 137.2#

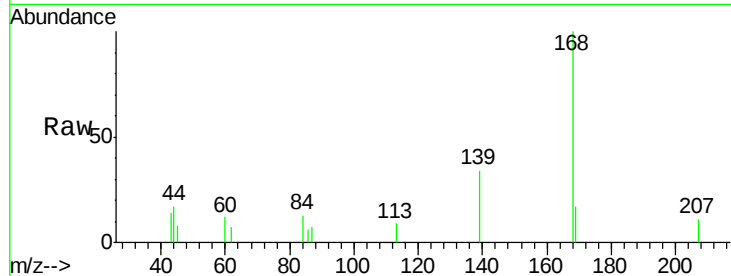


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BGC

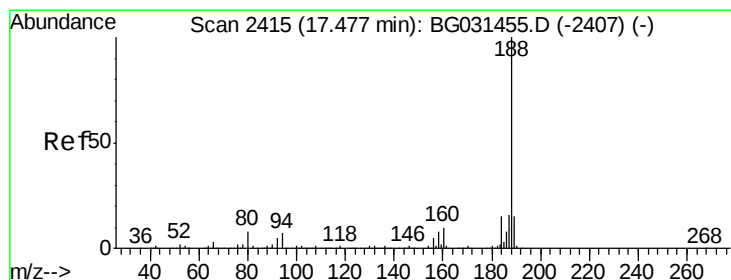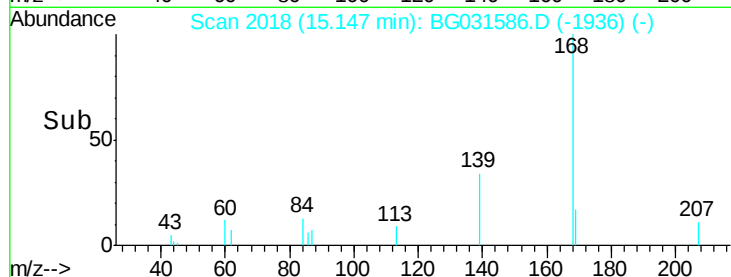
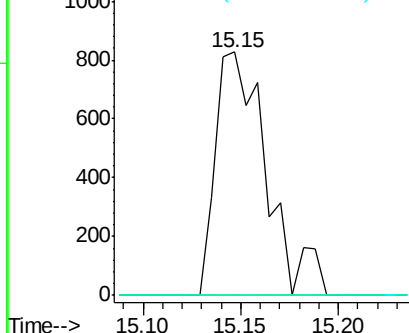



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.47 min Scan# 2413
Delta R.T. -0.01 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59

Tgt Ion:188 Resp: 550050
Ion Ratio Lower Upper
188 100
94 7.5 6.9 10.3
80 7.4 7.7 11.5#

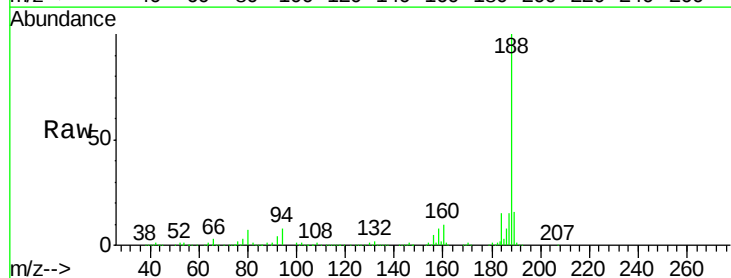

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

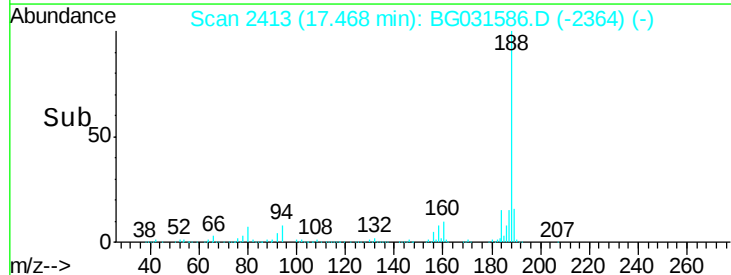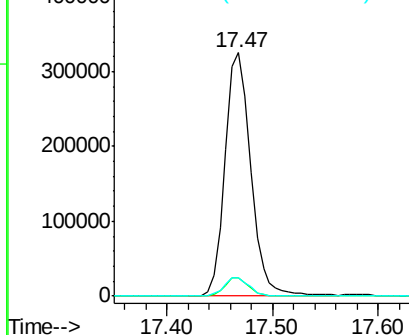



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.73 min Scan# 3139

Delta R.T. -0.02 min

Lab File: BG031586.D

Acq: 15 Dec 2017 8:59

Instrument :

BNA_G

ClientSampled :


Tot Ion:240 Resp: 642231

Ion Ratio Lower Upper

240 100

120 7.3 6.8 10.2




236 26.5 20.9 31.3

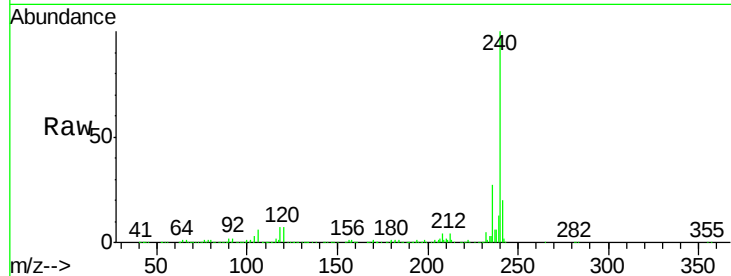

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

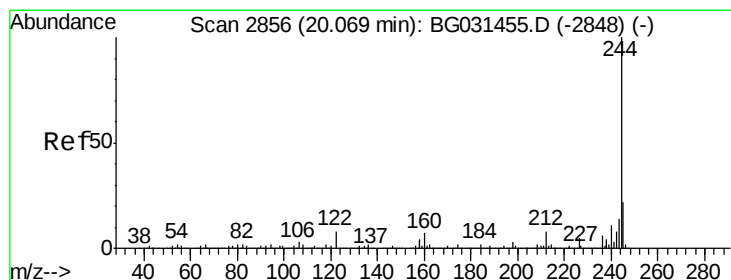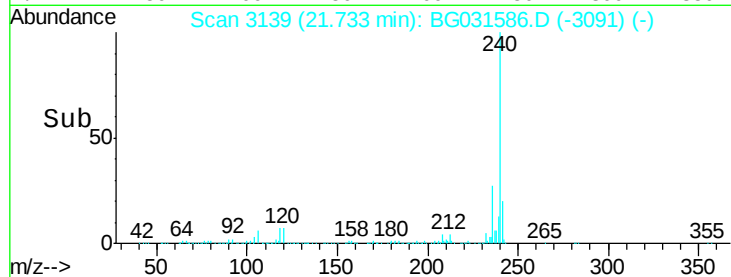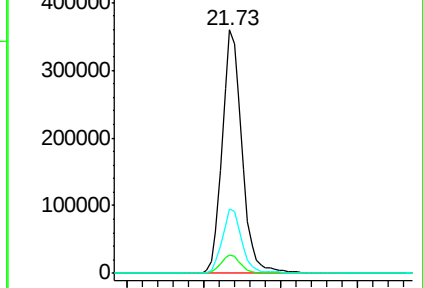

#78

Terphenyl-d14

Concen: 78.992 ng

RT: 20.06 min Scan# 2854

Delta R.T. -0.01 min

Lab File: BG031586.D

Acq: 15 Dec 2017 8:59


Tgt Ion:244 Resp: 2229778

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#



122 9.1 7.0 10.4

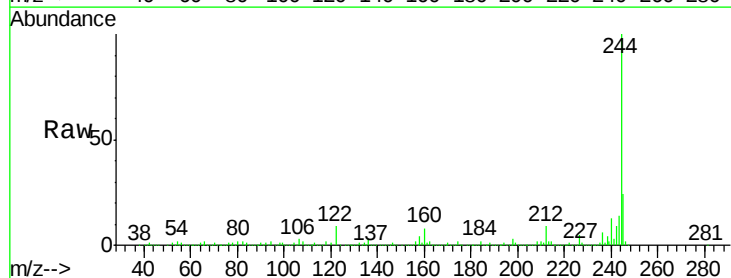


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

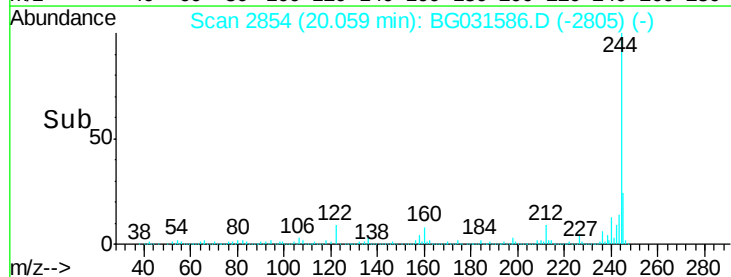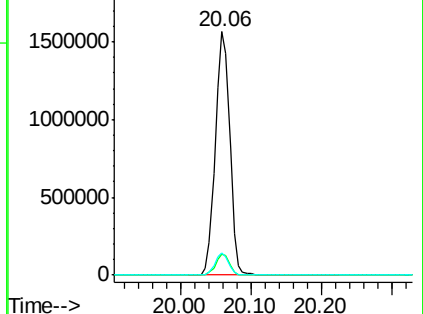



#86
Pervlene-d12
Concen: 20.000 ng
RT: 25.02 min Scan# 3698
Delta R.T. -0.02 min
Lab File: BG031586.D
Acq: 15 Dec 2017 8:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.7	17.4	26.0
265	21.4	17.7	26.5

