
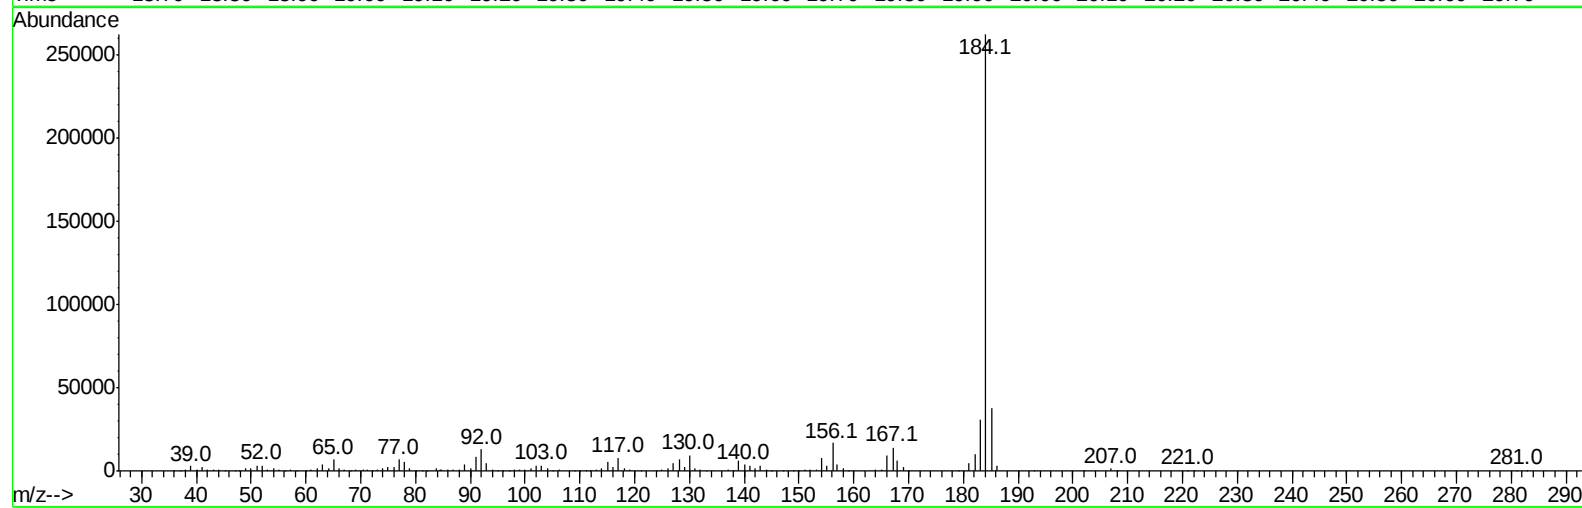


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121417\
Data File : BG031560.D
Acq On : 14 Dec 2017 15:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 06:32:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

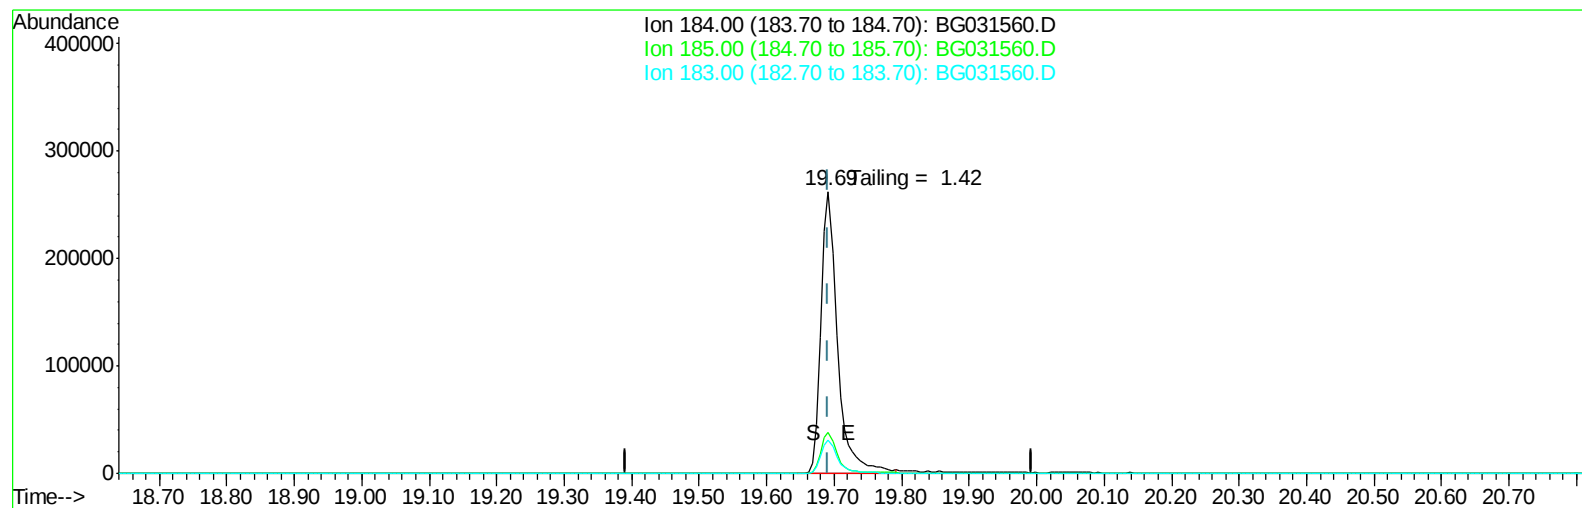

TIC: BG031560.D

(76) Benzidine



19.692min (-0.001) 3535.81ng

response 439814

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.38
183.00	13.30	11.76
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG121417\
Data File : BG031560.D
Acq On : 14 Dec 2017 15:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 06:32:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG121117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 17:25:55 2017
Response via : Initial Calibration

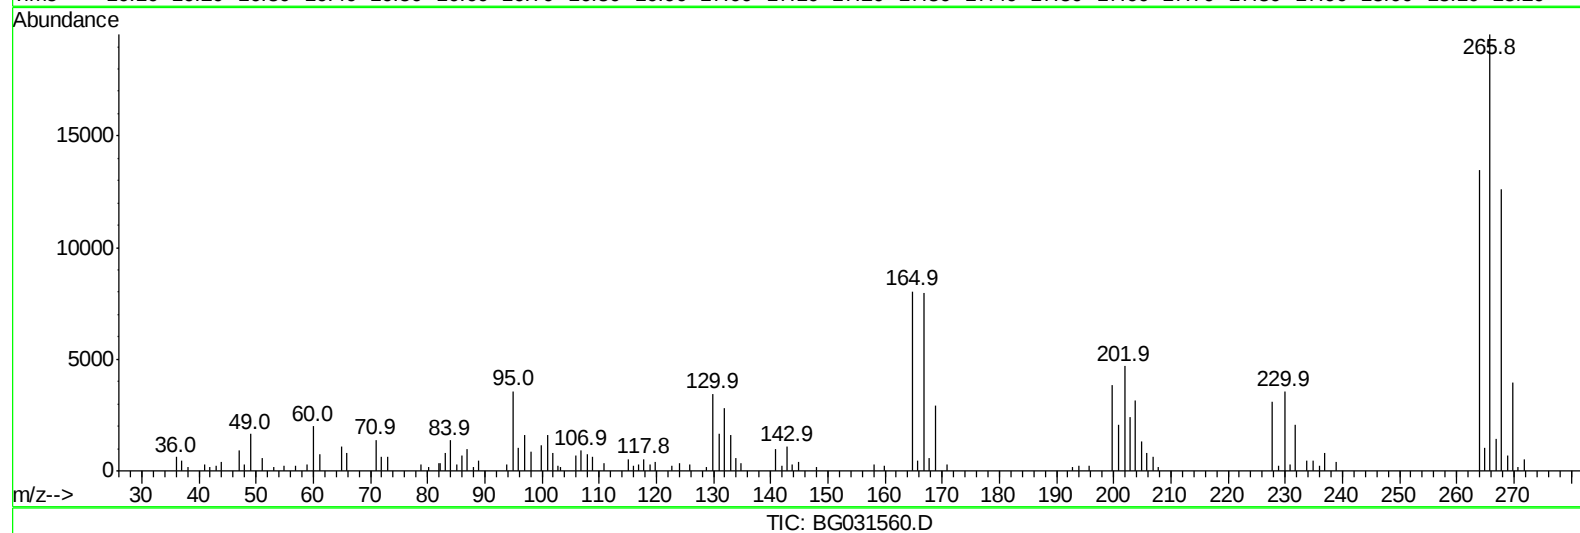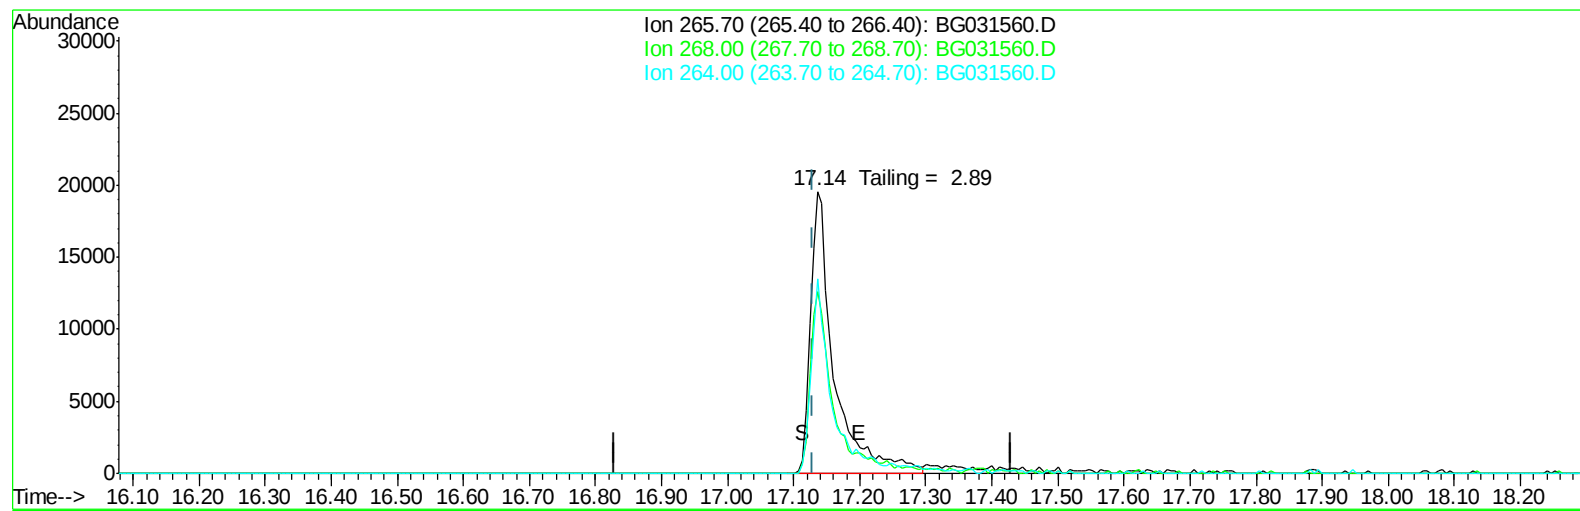

(69) Pentachlorophenol (C)

17.136min (+0.006) 12772.20ng

response 48531

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.56
264.00	62.00	68.97
0.00	0.00	0.00