


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG121417\
 Data File : BG031560.D
 Acq On : 14 Dec 2017 15:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG121117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 11 17:25:55 2017

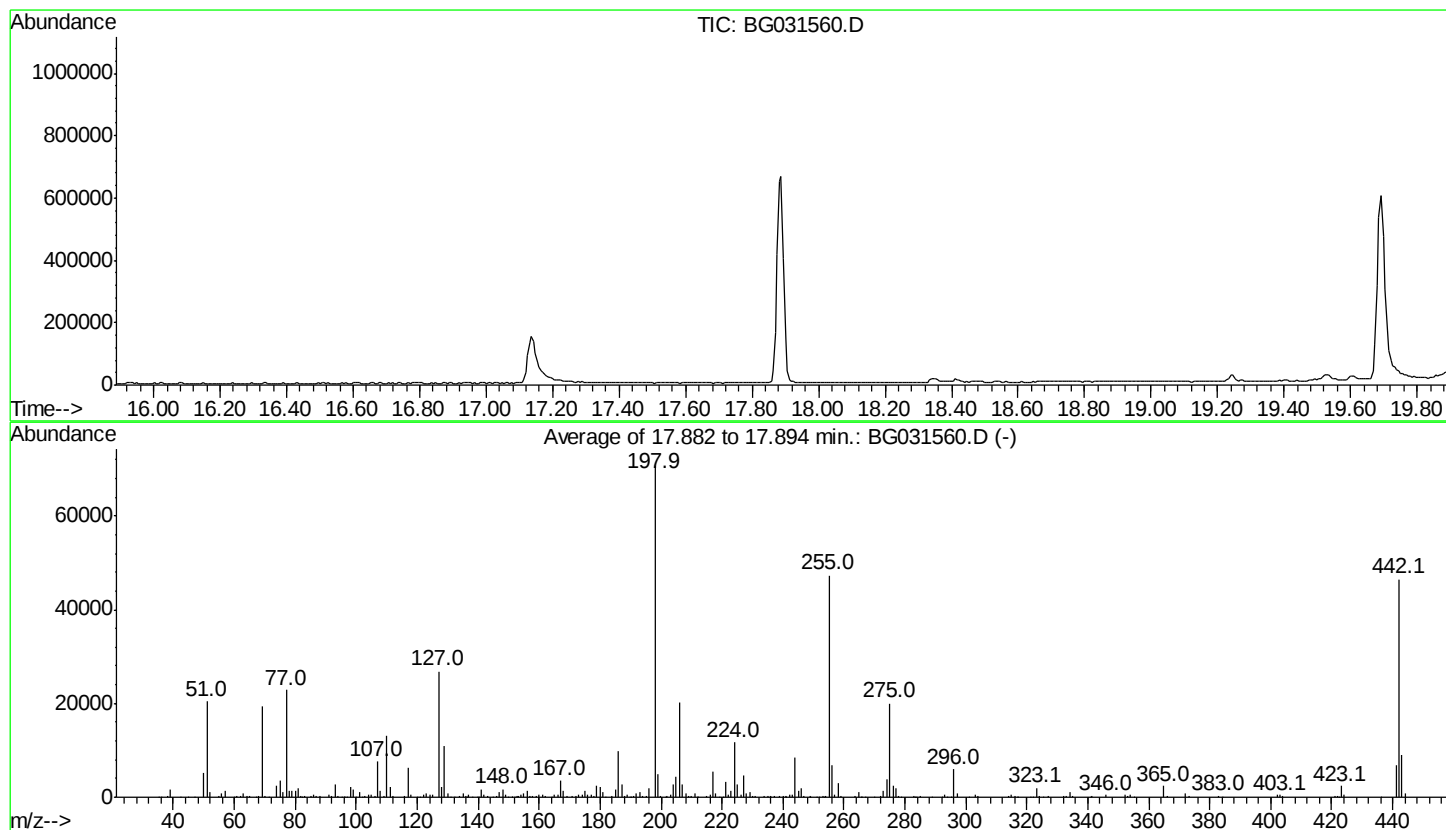

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	20433	PASS
68	69	0.00	2	1.5	286	PASS
69	198	0.00	100	27.5	19453	PASS
70	69	0.00	2	1.0	201	PASS
127	198	10	80	37.9	26813	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70720	PASS
199	198	5	9	7.1	5023	PASS
275	198	10	60	28.3	20035	PASS
365	198	1	100	3.4	2380	PASS
441	442	0.01	24	14.8	6892	PASS
442	198	50	100	65.7	46496	PASS
443	442	15	24	19.3	8994	PASS