

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051504.D
 Acq On : 14 Dec 2021 15:05
 Operator : CG/JU
 Sample : PB141353BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.542	7	9	10	rBV2	1649	1400	0.12%	0.013%
2	3.607	16	20	28	rVB4	8299	14399	1.26%	0.131%
3	3.707	34	37	40	rVB2	2144	1880	0.16%	0.017%
4	3.912	69	72	75	rVB3	1829	2569	0.23%	0.023%
5	3.977	79	83	86	rBV3	1884	2395	0.21%	0.022%
6	4.042	90	94	107	rVV	111503	193755	16.98%	1.768%
7	4.130	107	109	117	rVB3	1922	3526	0.31%	0.032%
8	4.253	129	130	134	rVB2	1036	1311	0.11%	0.012%
9	4.347	142	146	147	rVV	1068	1464	0.13%	0.013%
10	4.394	147	154	157	rVV2	3761	5563	0.49%	0.051%
11	4.594	185	188	192	rVB3	1529	2405	0.21%	0.022%
12	4.635	192	195	197	rBV	1373	1485	0.13%	0.014%
13	4.893	234	239	241	rVB2	1134	1715	0.15%	0.016%
14	5.093	269	273	276	rVB3	1275	1656	0.15%	0.015%
15	5.980	423	424	427	rBV3	1525	1284	0.11%	0.012%
16	6.503	511	513	517	rVB	1396	2146	0.19%	0.020%
17	6.544	517	520	524	rBV	1523	1961	0.17%	0.018%
18	6.585	524	527	530	rBV3	1314	1393	0.12%	0.013%
19	6.908	578	582	586	rBV	921	1457	0.13%	0.013%
20	7.414	660	668	677	rVV	163631	276247	24.21%	2.521%
21	7.590	690	698	706	rBV	108960	183554	16.09%	1.675%
22	7.807	726	735	744	rBV	152683	258158	22.63%	2.356%
23	7.919	749	754	757	rBV3	1264	1769	0.16%	0.016%
24	8.283	806	816	824	rBV	131455	221217	19.39%	2.018%
25	8.459	845	846	851	rVB2	1453	1421	0.12%	0.013%
26	8.729	891	892	896	rVB2	1351	1311	0.11%	0.012%
27	8.847	908	912	913	rBV	1161	1301	0.11%	0.012%
28	8.976	927	934	942	rBV	186643	322130	28.23%	2.939%
29	9.047	942	946	948	rVB3	1443	1391	0.12%	0.013%
30	9.452	1007	1015	1025	rBV	146524	258684	22.67%	2.360%
31	9.846	1079	1082	1086	rBV2	1434	2447	0.21%	0.022%
32	9.887	1087	1089	1093	rVB2	1143	1373	0.12%	0.013%
33	10.186	1130	1140	1150	rBV	115126	209655	18.38%	1.913%
34	10.315	1160	1162	1164	rVB	1590	1345	0.12%	0.012%
35	10.357	1164	1169	1170	rBV	1206	1559	0.14%	0.014%
36	10.727	1225	1232	1239	rVB	185703	324298	28.42%	2.959%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051504.D
 Acq On : 14 Dec 2021 15:05
 Operator : CG/JU
 Sample : PB141353BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	10.950	1266	1270	1274	rVB2	1239	1427	0.13%	0.013%
38	11.120	1290	1299	1308	rVV	176926	319836	28.03%	2.918%
39	11.238	1311	1319	1328	rBV	178998	331276	29.04%	3.023%
40	11.367	1338	1341	1344	rVB3	1207	1490	0.13%	0.014%
41	11.402	1344	1347	1352	rBV3	704	1590	0.14%	0.015%
42	11.766	1406	1409	1412	rBV	1295	1386	0.12%	0.013%
43	11.849	1422	1423	1427	rVB2	1396	1317	0.12%	0.012%
44	12.189	1478	1481	1483	rBV	1364	1458	0.13%	0.013%
45	12.695	1562	1567	1571	rVB4	3536	5318	0.47%	0.049%
46	12.947	1607	1610	1612	rBV	1295	1760	0.15%	0.016%
47	13.188	1648	1651	1655	rBV3	1713	2027	0.18%	0.018%
48	13.353	1678	1679	1683	rVB2	1261	1518	0.13%	0.014%
49	13.517	1702	1707	1709	rBV2	751	1274	0.11%	0.012%
50	13.576	1714	1717	1718	rBV	1344	1494	0.13%	0.014%
51	13.993	1786	1788	1792	rVB2	1095	1322	0.12%	0.012%
52	14.028	1792	1794	1799	rVB3	869	1526	0.13%	0.014%
53	14.122	1804	1810	1812	rBV2	1049	2027	0.18%	0.018%
54	14.310	1834	1842	1849	rBV	377897	543039	47.60%	4.955%
55	14.545	1879	1882	1885	rVB2	1308	1413	0.12%	0.013%
56	14.610	1885	1893	1903	rBV	382223	607641	53.26%	5.544%
57	14.915	1939	1945	1953	rBV	298726	468848	41.09%	4.278%
58	15.021	1960	1963	1965	rVB2	1499	1444	0.13%	0.013%
59	15.074	1965	1972	1979	rBV	180857	294201	25.79%	2.684%
60	15.168	1987	1988	1992	rBV3	1393	1704	0.15%	0.016%
61	15.203	1992	1994	1998	rVV3	1129	1688	0.15%	0.015%
62	15.262	2000	2004	2006	rBV3	1647	2196	0.19%	0.020%
63	15.309	2008	2012	2014	rBV4	1564	2160	0.19%	0.020%
64	15.344	2016	2018	2021	rBV3	1527	1279	0.11%	0.012%
65	15.391	2024	2026	2030	rBV2	1087	1718	0.15%	0.016%
66	15.497	2043	2044	2047	rBV2	1637	1564	0.14%	0.014%
67	15.550	2051	2053	2056	rVV3	1128	1273	0.11%	0.012%
68	15.597	2059	2061	2063	rBV2	1616	1821	0.16%	0.017%
69	15.738	2082	2085	2088	rBV4	1361	1406	0.12%	0.013%
70	15.837	2100	2102	2105	rBV3	1547	1767	0.15%	0.016%
71	15.908	2107	2114	2120	rVV	487201	766797	67.21%	6.997%
72	16.002	2123	2130	2136	rBV2	161142	235801	20.67%	2.152%
73	16.137	2152	2153	2155	rBV2	1398	1286	0.11%	0.012%
74	16.190	2160	2162	2165	rVB2	1594	1497	0.13%	0.014%
75	16.566	2223	2226	2228	rBV2	2271	2268	0.20%	0.021%
76	16.695	2245	2248	2251	rVB4	1732	2712	0.24%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051504.D
 Acq On : 14 Dec 2021 15:05
 Operator : CG/JU
 Sample : PB141353BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	16.818	2265	2269	2273	rBV7	1725	3362	0.29%	0.031%
78	17.065	2309	2311	2312	rBV2	1752	1461	0.13%	0.013%
79	17.124	2319	2321	2322	rBV	2480	1467	0.13%	0.013%
80	17.206	2332	2335	2336	rBV3	1756	1531	0.13%	0.014%
81	17.247	2341	2342	2346	rBV4	1547	2033	0.18%	0.019%
82	17.341	2355	2358	2362	rBV3	1896	3081	0.27%	0.028%
83	17.412	2366	2370	2371	rBV4	1718	1734	0.15%	0.016%
84	17.529	2388	2390	2392	rBV3	1935	1886	0.17%	0.017%
85	17.664	2406	2413	2419	rBV	396666	616146	54.01%	5.622%
86	17.764	2423	2430	2439	rVB	598436	913517	80.07%	8.335%
87	18.058	2478	2480	2482	rBV3	1631	1541	0.14%	0.014%
88	18.181	2499	2501	2502	rBV2	2460	2130	0.19%	0.019%
89	18.252	2511	2513	2514	rBV	3249	2279	0.20%	0.021%
90	18.563	2563	2566	2569	rBV4	3230	3821	0.33%	0.035%
91	18.604	2569	2573	2577	rVB7	4517	7984	0.70%	0.073%
92	18.634	2577	2578	2581	rBV3	3488	4285	0.38%	0.039%
93	18.686	2586	2587	2593	rVB6	2990	4538	0.40%	0.041%
94	18.904	2620	2624	2626	rBV4	3116	5258	0.46%	0.048%
95	18.951	2630	2632	2633	rBV2	2809	1464	0.13%	0.013%
96	19.068	2650	2652	2655	rBV4	3933	4976	0.44%	0.045%
97	20.038	2811	2817	2823	rBV	796623	1140901	100.00%	10.410%
98	21.982	3142	3148	3155	rVB	399846	697353	61.12%	6.363%
99	25.248	3695	3704	3717	rVB2	331117	990222	86.79%	9.035%
100	25.489	3737	3745	3757	rVB2	203311	611498	53.60%	5.580%




Sum of corrected areas: 10959661

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051504.D
Acq On : 14 Dec 2021 15:05
Operator : CG/JU
Sample : PB141353BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

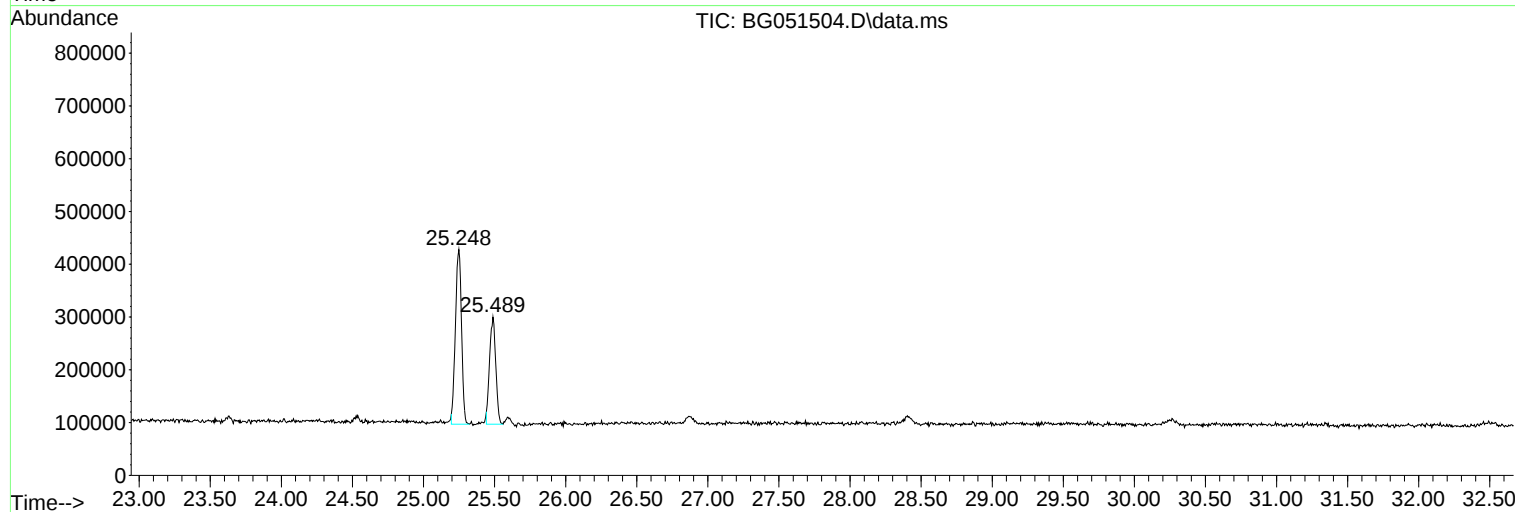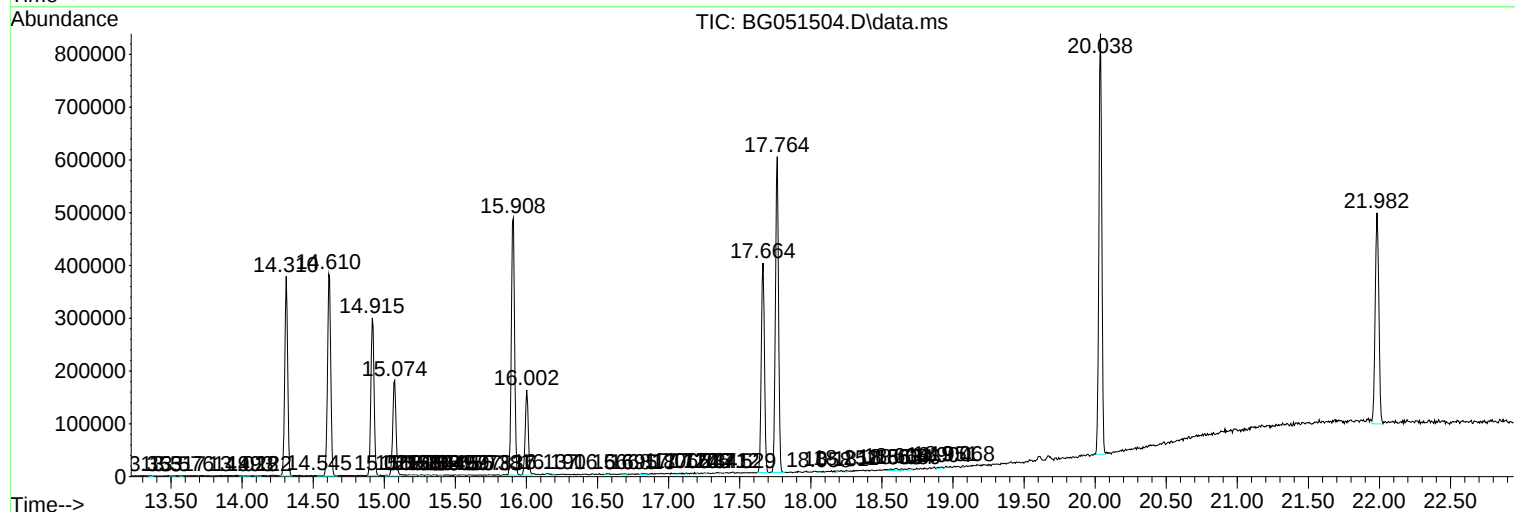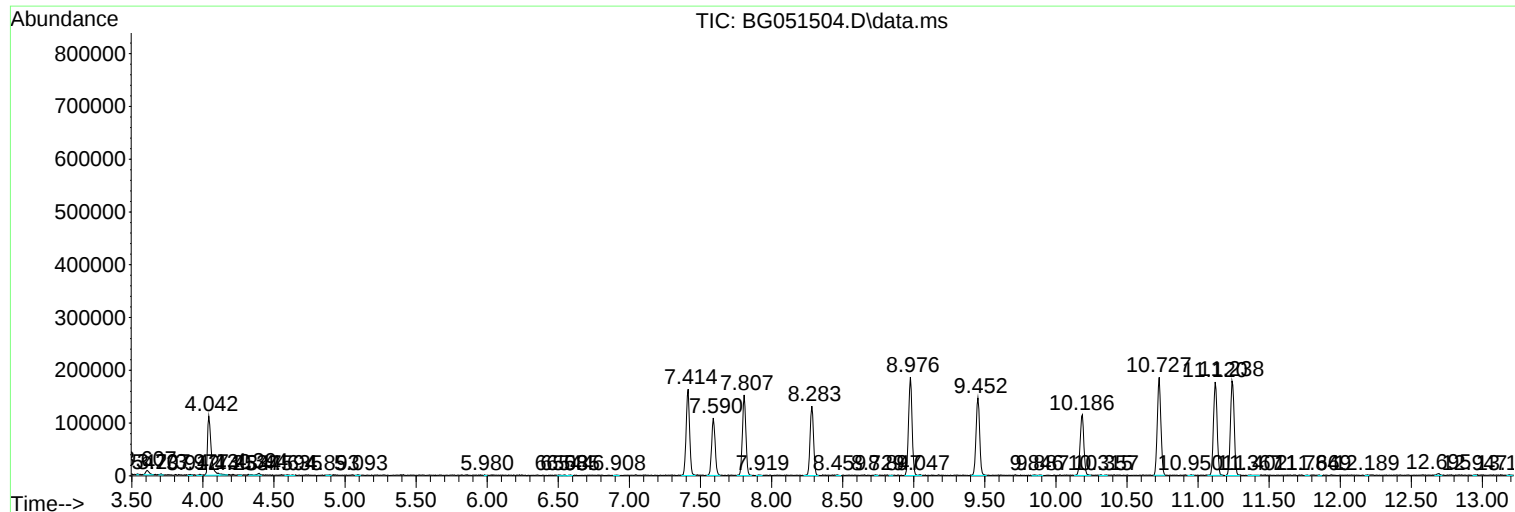

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051504.D
Acq On : 14 Dec 2021 15:05
Operator : CG/JU
Sample : PB141353BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051504.D
Acq On : 14 Dec 2021 15:05
Operator : CG/JU
Sample : PB141353BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc