

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051508.D
 Acq On : 14 Dec 2021 18:01
 Operator : CG/JU
 Sample : PB141304BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.552	9	11	13	rVB2	1745	1336	0.13%	0.013%
2	3.581	13	16	17	rBV3	1679	1801	0.17%	0.018%
3	3.611	17	21	29	rVB	8566	12393	1.18%	0.124%
4	3.811	52	55	58	rVB2	1169	1409	0.13%	0.014%
5	4.040	90	94	104	rBV	104805	175457	16.68%	1.754%
6	4.386	148	153	155	rBV2	1569	2123	0.20%	0.021%
7	4.498	169	172	176	rVB3	1361	1566	0.15%	0.016%
8	4.609	189	191	194	rVB	1633	1443	0.14%	0.014%
9	5.027	259	262	266	rVB3	1312	2258	0.21%	0.023%
10	5.062	266	268	270	rBV2	1268	1246	0.12%	0.012%
11	5.091	270	273	275	rVB3	960	1262	0.12%	0.013%
12	5.238	295	298	301	rVV2	1458	1793	0.17%	0.018%
13	5.332	312	314	318	rBV2	724	1326	0.13%	0.013%
14	5.438	328	332	333	rBV2	1051	1311	0.12%	0.013%
15	5.561	352	353	357	rVB3	1248	1268	0.12%	0.013%
16	5.690	373	375	381	rVB2	697	1278	0.12%	0.013%
17	5.743	381	384	387	rBV3	942	1242	0.12%	0.012%
18	5.837	397	400	402	rVB2	1517	1283	0.12%	0.013%
19	5.990	421	426	429	rVB2	1082	1645	0.16%	0.016%
20	6.407	493	497	499	rBV	1402	1918	0.18%	0.019%
21	6.483	505	510	512	rBV2	1077	1255	0.12%	0.013%
22	6.836	566	570	572	rVB2	1071	1596	0.15%	0.016%
23	6.889	577	579	582	rVV2	1285	1469	0.14%	0.015%
24	6.942	585	588	592	rBV2	1273	1695	0.16%	0.017%
25	7.130	619	620	625	rVB2	1542	1767	0.17%	0.018%
26	7.412	659	668	676	rBV	139929	242334	23.03%	2.422%
27	7.588	691	698	708	rVB	95797	165278	15.71%	1.652%
28	7.688	713	715	719	rVB2	850	1255	0.12%	0.013%
29	7.805	728	735	745	rBV	127751	223147	21.21%	2.230%
30	8.163	792	796	798	rBV3	1270	1403	0.13%	0.014%
31	8.281	807	816	824	rBV	118769	200811	19.09%	2.007%
32	8.974	927	934	942	rBV	164331	283333	26.93%	2.832%
33	9.074	946	951	952	rVV	851	1313	0.12%	0.013%
34	9.450	1008	1015	1022	rVB	130527	227216	21.59%	2.271%
35	10.184	1132	1140	1149	rBV	104553	188116	17.88%	1.880%
36	10.278	1153	1156	1161	rVV	821	1293	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051508.D
 Acq On : 14 Dec 2021 18:01
 Operator : CG/JU
 Sample : PB141304BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	10.372	1169	1172	1174	rVB2	1243	1366	0.13%	0.014%
38	10.601	1208	1211	1217	rVB3	1608	2658	0.25%	0.027%
39	10.725	1225	1232	1240	rVB	167547	290558	27.61%	2.904%
40	11.030	1281	1284	1287	rVB	1432	1255	0.12%	0.013%
41	11.118	1292	1299	1308	rVB	156924	282702	26.87%	2.826%
42	11.242	1312	1320	1326	rBV	158115	292444	27.79%	2.923%
43	11.594	1378	1380	1384	rBV2	870	1225	0.12%	0.012%
44	12.693	1562	1567	1573	rBV	3336	5486	0.52%	0.055%
45	13.392	1681	1686	1687	rVB3	1618	1486	0.14%	0.015%
46	13.838	1759	1762	1767	rBV2	1094	2010	0.19%	0.020%
47	14.003	1785	1790	1791	rBV2	1269	1453	0.14%	0.015%
48	14.308	1836	1842	1849	rBV	344257	498152	47.34%	4.979%
49	14.614	1886	1894	1904	rBV	340654	546842	51.97%	5.466%
50	14.796	1922	1925	1927	rBV2	1156	1550	0.15%	0.015%
51	14.913	1938	1945	1954	rVV	266049	430356	40.90%	4.302%
52	15.072	1965	1972	1977	rBV	171441	269022	25.57%	2.689%
53	15.107	1977	1978	1981	rVV3	2893	2334	0.22%	0.023%
54	15.136	1981	1983	1985	rVB3	1473	1333	0.13%	0.013%
55	15.313	2009	2013	2016	rBV3	2961	3880	0.37%	0.039%
56	15.442	2032	2035	2036	rVB2	1659	1370	0.13%	0.014%
57	15.512	2045	2047	2050	rBV2	1883	1461	0.14%	0.015%
58	15.583	2057	2059	2063	rVB2	1206	1256	0.12%	0.013%
59	15.906	2107	2114	2121	rVB	449392	701994	66.72%	7.017%
60	15.965	2121	2124	2125	rVV3	1840	1979	0.19%	0.020%
61	16.000	2125	2130	2136	rVV	154778	223781	21.27%	2.237%
62	16.047	2136	2138	2143	rVV5	3085	5056	0.48%	0.051%
63	16.088	2143	2145	2147	rVB3	1971	1373	0.13%	0.014%
64	16.141	2152	2154	2159	rVB4	2637	3952	0.38%	0.040%
65	16.299	2178	2181	2183	rBV3	1653	1877	0.18%	0.019%
66	16.323	2183	2185	2188	rVV4	1789	1433	0.14%	0.014%
67	16.358	2188	2191	2193	rVV3	1905	1852	0.18%	0.019%
68	16.464	2207	2209	2210	rBV	2443	1447	0.14%	0.014%
69	16.611	2232	2234	2236	rBV2	1013	1329	0.13%	0.013%
70	16.787	2263	2264	2268	rVB2	2476	1801	0.17%	0.018%
71	16.899	2280	2283	2284	rBV2	2619	2674	0.25%	0.027%
72	16.993	2295	2299	2302	rBV4	1380	2241	0.21%	0.022%
73	17.022	2302	2304	2307	rVB3	1343	1259	0.12%	0.013%
74	17.104	2317	2318	2323	rVB4	1626	1414	0.13%	0.014%
75	17.151	2325	2326	2329	rBV2	2086	1961	0.19%	0.020%
76	17.239	2340	2341	2344	rVB3	2353	1656	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051508.D
 Acq On : 14 Dec 2021 18:01
 Operator : CG/JU
 Sample : PB141304BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	17.339	2356	2358	2360	rVV3	1610	1268	0.12%	0.013%
78	17.374	2363	2364	2366	rBV2	2371	1707	0.16%	0.017%
79	17.515	2387	2388	2391	rBV2	3022	3522	0.33%	0.035%
80	17.562	2393	2396	2397	rVV3	1725	1580	0.15%	0.016%
81	17.662	2406	2413	2419	rBV	392953	574533	54.60%	5.743%
82	17.762	2421	2430	2437	rBV	552823	845600	80.37%	8.452%
83	17.850	2443	2445	2447	rBV3	2166	2732	0.26%	0.027%
84	17.891	2451	2452	2455	rBV3	1888	2020	0.19%	0.020%
85	17.944	2460	2461	2463	rVB2	2546	1544	0.15%	0.015%
86	17.980	2463	2467	2469	rBV5	2939	4059	0.39%	0.041%
87	18.056	2479	2480	2482	rBV2	2727	1433	0.14%	0.014%
88	18.103	2486	2488	2490	rVB2	2165	2034	0.19%	0.020%
89	18.132	2490	2493	2495	rBV4	1791	2258	0.21%	0.023%
90	18.291	2518	2520	2523	rBV4	2628	3037	0.29%	0.030%
91	18.320	2523	2525	2528	rVV3	2937	3217	0.31%	0.032%
92	18.385	2534	2536	2538	rBV3	2089	1556	0.15%	0.016%
93	18.684	2585	2587	2591	rBV5	2539	2431	0.23%	0.024%
94	18.743	2595	2597	2599	rVV3	2552	1748	0.17%	0.017%
95	18.896	2622	2623	2625	rBV2	2771	1377	0.13%	0.014%
96	19.607	2741	2744	2748	rVB5	8956	11816	1.12%	0.118%
97	20.036	2811	2817	2824	rVB	772167	1052189	100.00%	10.517%
98	21.980	3142	3148	3156	rVB	367866	635794	60.43%	6.355%
99	25.240	3694	3703	3714	rVB2	309311	922095	87.64%	9.217%
100	25.481	3736	3744	3754	rVB2	193729	566945	53.88%	5.667%




Sum of corrected areas: 10004412

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051508.D
Acq On : 14 Dec 2021 18:01
Operator : CG/JU
Sample : PB141304BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK304

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

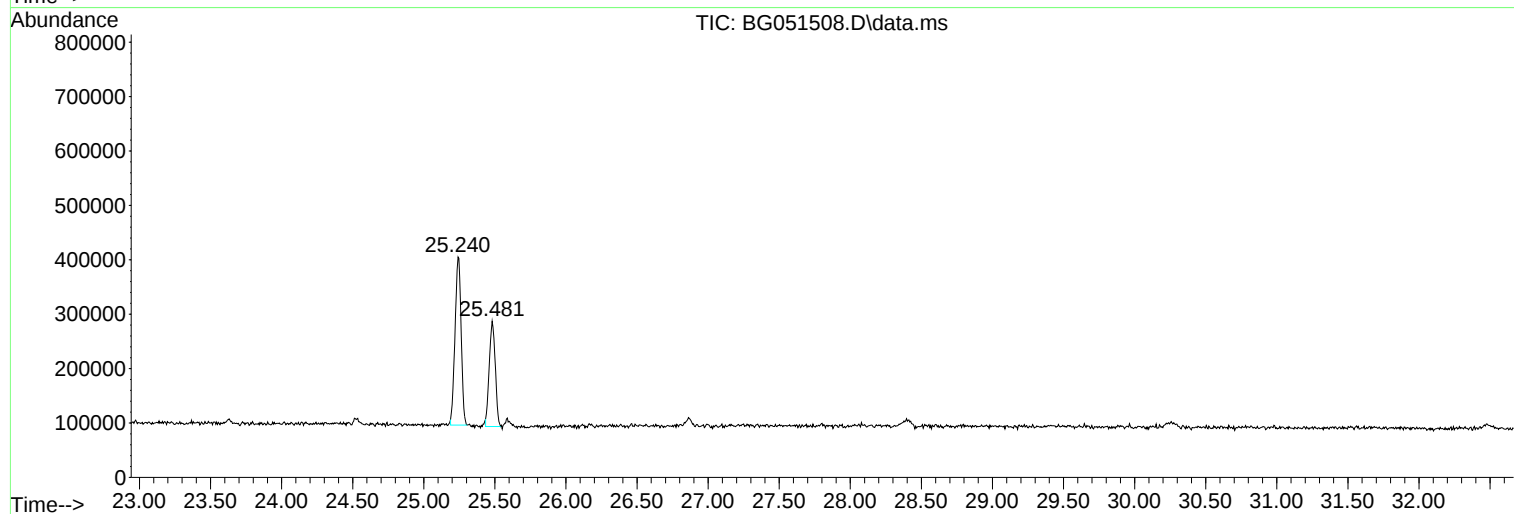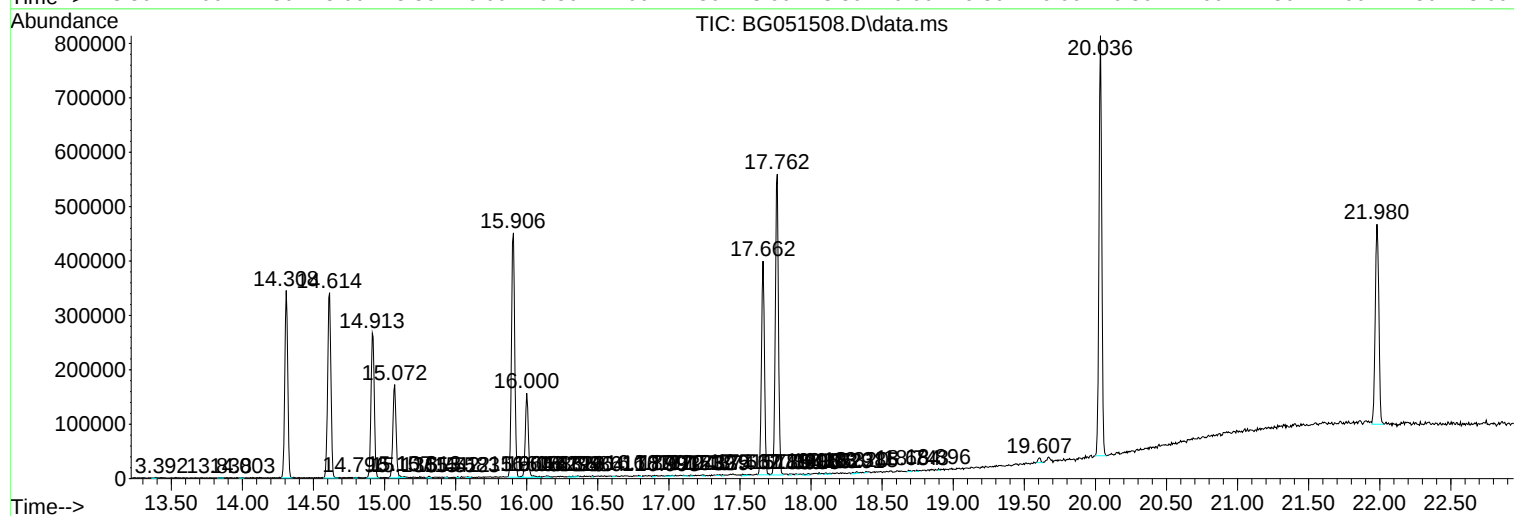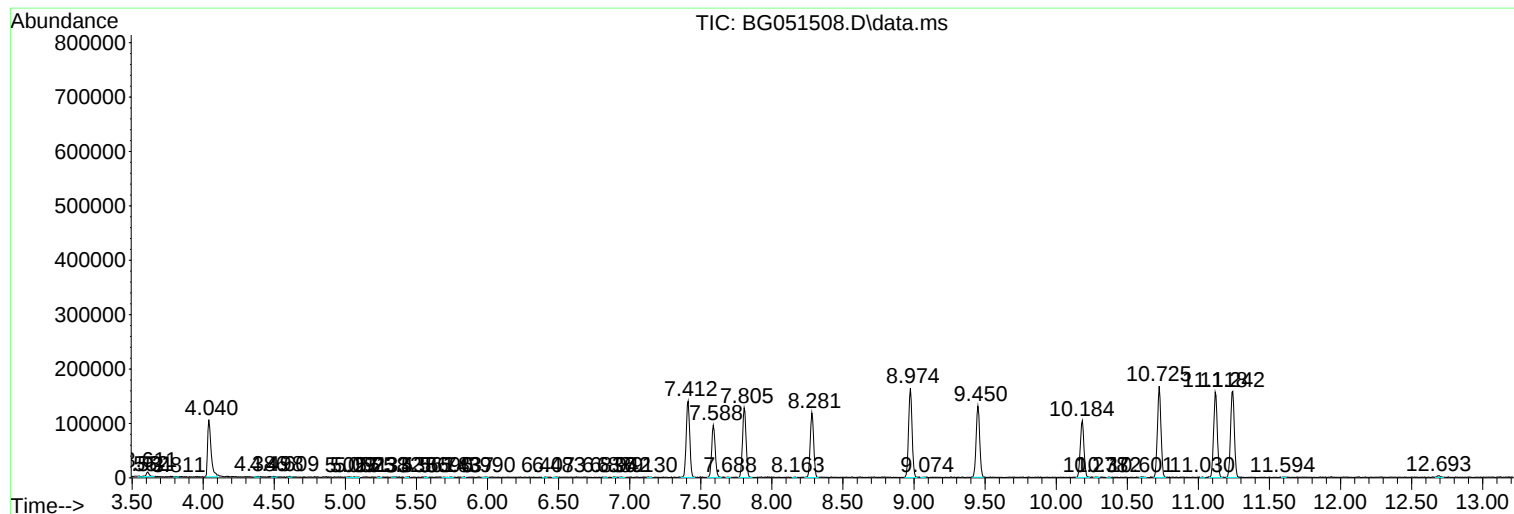

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051508.D
Acq On : 14 Dec 2021 18:01
Operator : CG/JU
Sample : PB141304BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK304

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051508.D
Acq On : 14 Dec 2021 18:01
Operator : CG/JU
Sample : PB141304BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK304

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc