

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051509.D
 Acq On : 14 Dec 2021 18:41
 Operator : CG/JU
 Sample : M5031-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.755	42	45	47	rBV3	1153	1174	0.21%	0.061%
2	3.779	47	49	53	rVB3	1019	838	0.15%	0.044%
3	4.008	85	88	89	rVB2	1673	1383	0.25%	0.072%
4	4.020	89	90	93	rBV2	1282	1050	0.19%	0.055%
5	4.137	109	110	113	rVB	1215	799	0.14%	0.042%
6	4.167	113	115	116	rBV	1207	822	0.15%	0.043%
7	4.214	121	123	125	rVB2	1614	1054	0.19%	0.055%
8	4.243	125	128	129	rBV	954	899	0.16%	0.047%
9	4.384	148	152	154	rBV3	2299	3310	0.59%	0.173%
10	4.455	162	164	167	rBV2	661	803	0.14%	0.042%
11	4.525	175	176	179	rBV2	1602	1237	0.22%	0.065%
12	4.695	201	205	206	rBV2	1083	1182	0.21%	0.062%
13	4.842	227	230	232	rBV2	801	992	0.18%	0.052%
14	4.971	251	252	257	rVB2	1404	1472	0.26%	0.077%
15	5.347	311	316	317	rBV2	1076	1134	0.20%	0.059%
16	5.365	317	319	323	rBV2	929	1158	0.21%	0.060%
17	5.447	331	333	338	rBV	849	1300	0.23%	0.068%
18	5.541	346	349	351	rBV	784	851	0.15%	0.044%
19	5.776	388	389	392	rBV2	1015	779	0.14%	0.041%
20	5.947	414	418	419	rBV	646	935	0.17%	0.049%
21	6.164	453	455	458	rBV	614	810	0.14%	0.042%
22	6.276	469	474	477	rBV2	615	911	0.16%	0.048%
23	6.299	477	478	482	rVB	947	877	0.16%	0.046%
24	6.334	482	484	487	rBV2	646	919	0.16%	0.048%
25	6.387	491	493	497	rVB	812	1077	0.19%	0.056%
26	6.505	510	513	517	rVB	1135	1198	0.21%	0.062%
27	6.675	539	542	543	rVB	1230	840	0.15%	0.044%
28	6.898	578	580	586	rVB	846	1007	0.18%	0.053%
29	7.016	599	600	604	rVB3	1052	1195	0.21%	0.062%
30	7.092	611	613	616	rVB3	1164	1288	0.23%	0.067%
31	7.210	630	633	634	rBV	1326	1075	0.19%	0.056%
32	7.315	647	651	654	rVB3	711	871	0.15%	0.045%
33	7.638	700	706	709	rBV2	1344	2165	0.38%	0.113%
34	7.703	716	717	721	rBV	882	1047	0.19%	0.055%
35	7.803	730	734	739	rVB2	715	1684	0.30%	0.088%
36	7.838	739	740	742	rBV	1001	837	0.15%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051509.D
 Acq On : 14 Dec 2021 18:41
 Operator : CG/JU
 Sample : M5031-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	7.991	765	766	770	rVB	847	960	0.17%	0.050%
38	8.126	786	789	790	rBV	1094	814	0.14%	0.042%
39	8.285	808	816	822	rVB	101586	174363	30.99%	9.095%
40	8.390	831	834	839	rBV	888	1383	0.25%	0.072%
41	8.473	845	848	851	rBV2	1009	1263	0.22%	0.066%
42	8.625	872	874	878	rBV	1240	848	0.15%	0.044%
43	8.966	930	932	935	rVB3	1131	961	0.17%	0.050%
44	9.225	971	976	979	rBV2	1046	1482	0.26%	0.077%
45	9.277	982	985	987	rVV	1137	1025	0.18%	0.053%
46	9.371	997	1001	1002	rBV	902	824	0.15%	0.043%
47	9.465	1014	1017	1020	rVB	873	1117	0.20%	0.058%
48	9.507	1020	1024	1025	rBV	816	986	0.18%	0.051%
49	9.542	1028	1030	1035	rBV	671	970	0.17%	0.051%
50	9.577	1035	1036	1039	rBV	927	860	0.15%	0.045%
51	10.276	1152	1155	1157	rBV2	746	1000	0.18%	0.052%
52	10.300	1157	1159	1163	rVB2	918	908	0.16%	0.047%
53	10.670	1221	1222	1225	rBV	1257	856	0.15%	0.045%
54	11.122	1289	1299	1305	rBV	131752	240551	42.76%	12.547%
55	11.210	1311	1314	1317	rVB	1046	833	0.15%	0.043%
56	11.239	1317	1319	1322	rBV	932	885	0.16%	0.046%
57	11.292	1325	1328	1329	rVB	829	810	0.14%	0.042%
58	11.410	1345	1348	1349	rBV	915	848	0.15%	0.044%
59	11.586	1376	1378	1381	rVB2	1259	1092	0.19%	0.057%
60	11.621	1381	1384	1386	rBV	718	839	0.15%	0.044%
61	12.091	1462	1464	1466	rBV	1064	838	0.15%	0.044%
62	12.150	1471	1474	1475	rVB2	844	809	0.14%	0.042%
63	12.361	1506	1510	1512	rBV2	701	861	0.15%	0.045%
64	12.820	1586	1588	1590	rVV	1110	843	0.15%	0.044%
65	12.861	1592	1595	1598	rVB2	1346	1825	0.32%	0.095%
66	12.984	1614	1616	1618	rBV2	869	932	0.17%	0.049%
67	13.049	1624	1627	1629	rBV2	753	880	0.16%	0.046%
68	13.125	1638	1640	1643	rBV2	994	1274	0.23%	0.066%
69	13.172	1645	1648	1650	rBV	730	799	0.14%	0.042%
70	13.366	1678	1681	1682	rBV	834	847	0.15%	0.044%
71	13.384	1682	1684	1686	rVV	1293	930	0.17%	0.049%
72	13.460	1695	1697	1700	rVB2	816	790	0.14%	0.041%
73	13.642	1726	1728	1731	rBV2	1003	1206	0.21%	0.063%
74	14.265	1831	1834	1836	rBV2	1210	866	0.15%	0.045%
75	14.376	1849	1853	1856	rBV2	1182	2014	0.36%	0.105%
76	14.506	1874	1875	1878	rBV	1278	1232	0.22%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051509.D
 Acq On : 14 Dec 2021 18:41
 Operator : CG/JU
 Sample : M5031-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	14.629	1895	1896	1898	rBV2	1518	944	0.17%	0.049%
78	14.705	1906	1909	1910	rBV2	1055	797	0.14%	0.042%
79	14.776	1919	1921	1924	rVB2	1003	874	0.16%	0.046%
80	14.858	1933	1935	1938	rBV	974	1166	0.21%	0.061%
81	14.917	1938	1945	1951	rVV	235282	356595	63.39%	18.600%
82	15.105	1973	1977	1978	rBV	1325	1540	0.27%	0.080%
83	15.222	1995	1997	2000	rVB2	1317	1590	0.28%	0.083%
84	15.252	2000	2002	2004	rBV	940	960	0.17%	0.050%
85	15.322	2012	2014	2016	rBV2	1271	1074	0.19%	0.056%
86	15.498	2042	2044	2045	rBV	1031	868	0.15%	0.045%
87	15.704	2077	2079	2080	rBV2	1296	1226	0.22%	0.064%
88	15.833	2099	2101	2104	rBV3	873	1025	0.18%	0.053%
89	16.109	2146	2148	2149	rVB2	1640	847	0.15%	0.044%
90	16.150	2152	2155	2156	rBV2	1013	1129	0.20%	0.059%
91	16.321	2183	2184	2189	rBV	1401	1535	0.27%	0.080%
92	16.849	2272	2274	2275	rBV	2127	882	0.16%	0.046%
93	17.155	2324	2326	2329	rBV3	1326	1066	0.19%	0.056%
94	17.378	2362	2364	2365	rVB2	2218	1053	0.19%	0.055%
95	17.660	2406	2412	2418	rVB	319981	483645	85.97%	25.226%
96	18.218	2505	2507	2508	rBV	2449	1455	0.26%	0.076%
97	21.984	3142	3148	3156	rVB	320469	562560	100.00%	29.342%




Sum of corrected areas: 1917228

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051509.D
Acq On : 14 Dec 2021 18:41
Operator : CG/JU
Sample : M5031-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

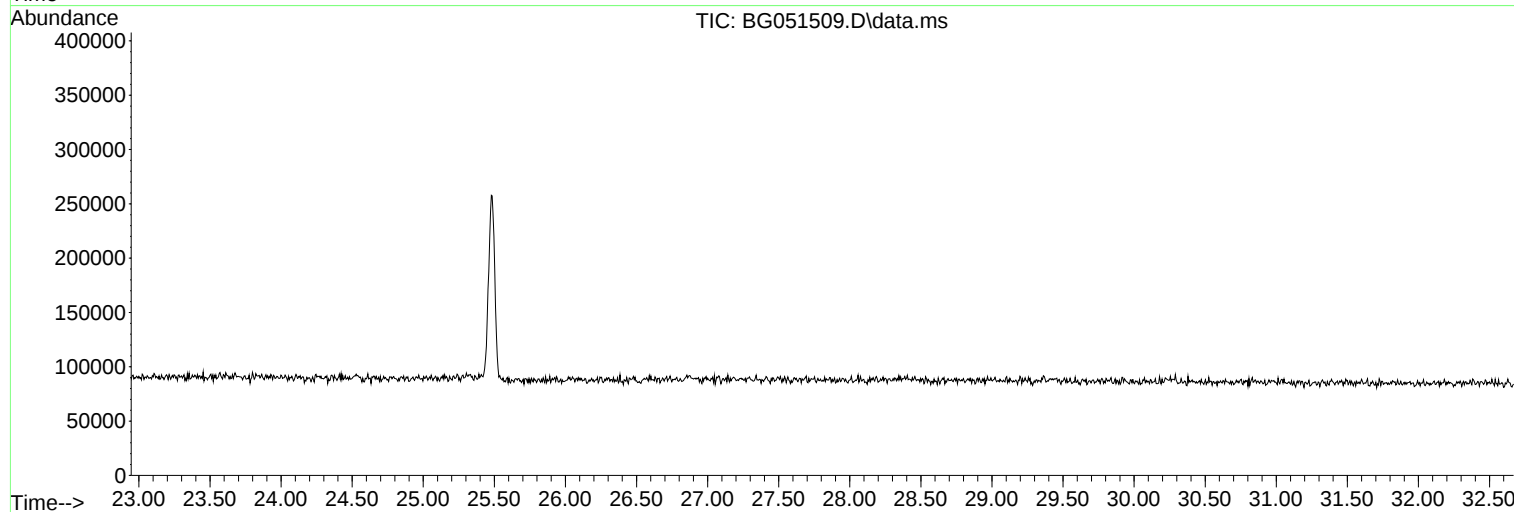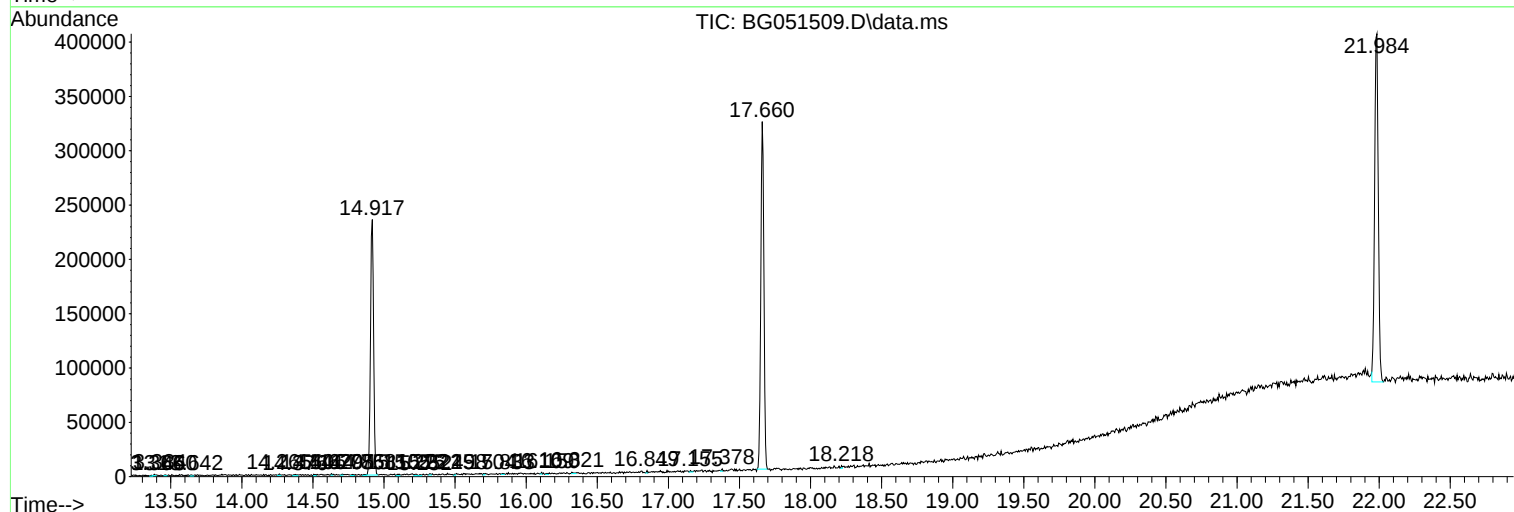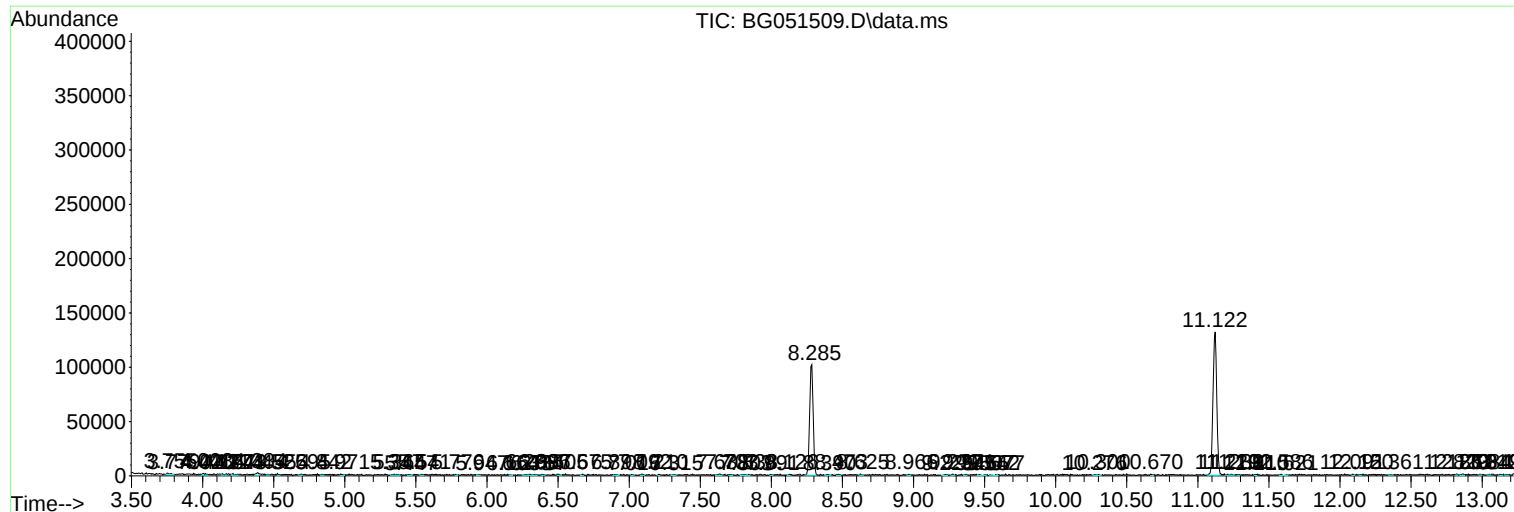

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051509.D
Acq On : 14 Dec 2021 18:41
Operator : CG/JU
Sample : M5031-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051509.D
Acq On : 14 Dec 2021 18:41
Operator : CG/JU
Sample : M5031-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
