

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051518.D
 Acq On : 15 Dec 2021 00:46
 Operator : CG/JU
 Sample : M4995-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.606	15	20	25	rBV2	6580	10055	0.87%	0.104%
2	3.741	41	43	46	rVB2	1705	1819	0.16%	0.019%
3	4.040	90	94	105	rBV	29266	50932	4.39%	0.527%
4	4.176	114	117	119	rBV	1332	1352	0.12%	0.014%
5	4.281	131	135	137	rBV4	1560	2403	0.21%	0.025%
6	4.387	149	153	154	rBV2	2172	1994	0.17%	0.021%
7	4.663	197	200	202	rBV2	1002	1343	0.12%	0.014%
8	4.710	205	208	212	rVV2	1039	1485	0.13%	0.015%
9	4.810	224	225	232	rVB	1598	1814	0.16%	0.019%
10	4.886	237	238	242	rVB	1293	1230	0.11%	0.013%
11	4.945	242	248	250	rBV2	2937	4669	0.40%	0.048%
12	5.333	310	314	320	rBV3	3549	7092	0.61%	0.073%
13	6.801	561	564	568	rVB	1264	1989	0.17%	0.021%
14	7.406	661	667	674	rBV2	29801	53359	4.60%	0.552%
15	7.589	691	698	704	rVV	91581	158357	13.66%	1.639%
16	7.641	704	707	710	rVB	1343	1890	0.16%	0.020%
17	7.800	727	734	746	rBV	95731	170749	14.73%	1.767%
18	8.282	807	816	822	rBV	113779	190283	16.41%	1.970%
19	8.781	899	901	904	rBV	946	1215	0.10%	0.013%
20	8.969	927	933	941	rVB	79964	140305	12.10%	1.452%
21	9.445	1007	1014	1022	rVV	126078	227074	19.59%	2.350%
22	9.521	1025	1027	1031	rVB2	901	1392	0.12%	0.014%
23	9.891	1084	1090	1092	rBV2	946	1188	0.10%	0.012%
24	10.179	1132	1139	1147	rVB	103835	184604	15.92%	1.911%
25	10.720	1222	1231	1240	rBV	145939	266192	22.96%	2.755%
26	11.119	1292	1299	1304	rBV	148378	269130	23.21%	2.786%
27	11.166	1304	1307	1313	rVV2	21982	35503	3.06%	0.367%
28	11.237	1313	1319	1326	rVB2	139303	255616	22.05%	2.646%
29	12.470	1524	1529	1533	rVB2	737	1315	0.11%	0.014%
30	12.605	1550	1552	1554	rBV	1376	1731	0.15%	0.018%
31	12.623	1554	1555	1559	rVV	1776	1466	0.13%	0.015%
32	12.688	1559	1566	1571	rVV4	2858	5055	0.44%	0.052%
33	12.758	1574	1578	1583	rBV	6175	9352	0.81%	0.097%
34	12.876	1596	1598	1601	rVB	1839	1282	0.11%	0.013%
35	12.975	1610	1615	1617	rBV3	1601	2272	0.20%	0.024%
36	13.328	1671	1675	1676	rVB	1694	1434	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051518.D
 Acq On : 15 Dec 2021 00:46
 Operator : CG/JU
 Sample : M4995-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	13.539	1707	1711	1713	rVB	1033	1386	0.12%	0.014%
38	13.892	1768	1771	1774	rBV2	1120	1513	0.13%	0.016%
39	14.156	1813	1816	1819	rVB2	1133	1507	0.13%	0.016%
40	14.303	1835	1841	1848	rBV	358172	515054	44.42%	5.331%
41	14.608	1886	1893	1900	rBV	371302	575542	49.64%	5.957%
42	14.914	1939	1945	1953	rVB	261111	399757	34.48%	4.138%
43	14.979	1953	1956	1958	rBV3	1626	1726	0.15%	0.018%
44	15.067	1965	1971	1978	rBV	37930	61638	5.32%	0.638%
45	15.255	2000	2003	2005	rBV2	1532	1671	0.14%	0.017%
46	15.308	2007	2012	2018	rVB	5347	7610	0.66%	0.079%
47	15.631	2062	2067	2072	rBV3	2267	3672	0.32%	0.038%
48	15.707	2077	2080	2082	rVV2	1680	1697	0.15%	0.018%
49	15.901	2105	2113	2120	rVV	502397	766782	66.13%	7.937%
50	15.960	2120	2123	2124	rVV2	1943	2299	0.20%	0.024%
51	16.001	2124	2130	2138	rVB	163589	252128	21.75%	2.610%
52	16.136	2151	2153	2159	rBV4	2363	3539	0.31%	0.037%
53	16.324	2184	2185	2188	rBV2	1713	1243	0.11%	0.013%
54	16.365	2190	2192	2195	rVB2	1501	1712	0.15%	0.018%
55	16.424	2198	2202	2203	rVB2	1406	1618	0.14%	0.017%
56	16.571	2222	2227	2228	rBV	1492	1921	0.17%	0.020%
57	16.641	2237	2239	2241	rBV	1548	1423	0.12%	0.015%
58	16.776	2259	2262	2263	rVB2	1846	1388	0.12%	0.014%
59	16.823	2268	2270	2274	rVB3	1254	1359	0.12%	0.014%
60	17.199	2332	2334	2337	rVB2	1785	1310	0.11%	0.014%
61	17.270	2345	2346	2350	rVB3	1679	1162	0.10%	0.012%
62	17.305	2350	2352	2353	rBV2	2582	1319	0.11%	0.014%
63	17.440	2371	2375	2377	rBV2	2754	3434	0.30%	0.036%
64	17.569	2396	2397	2399	rBV	1866	1286	0.11%	0.013%
65	17.657	2406	2412	2419	rBV	356894	553881	47.77%	5.733%
66	17.757	2423	2429	2438	rBV2	643378	952258	82.13%	9.856%
67	17.904	2452	2454	2455	rVB	1955	1177	0.10%	0.012%
68	17.928	2455	2458	2459	rBV3	1533	1370	0.12%	0.014%
69	17.998	2469	2470	2472	rVV2	1586	1417	0.12%	0.015%
70	18.057	2476	2480	2485	rVB5	1400	2125	0.18%	0.022%
71	18.092	2485	2486	2490	rBV2	1202	1602	0.14%	0.017%
72	18.303	2518	2522	2524	rBV4	2068	2296	0.20%	0.024%
73	18.345	2527	2529	2530	rBV2	1830	1366	0.12%	0.014%
74	18.415	2537	2541	2543	rBV4	2010	2569	0.22%	0.027%
75	18.474	2548	2551	2552	rBV2	1806	1819	0.16%	0.019%
76	18.527	2556	2560	2567	rBV7	6836	10165	0.88%	0.105%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051518.D
 Acq On : 15 Dec 2021 00:46
 Operator : CG/JU
 Sample : M4995-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	18.591	2569	2571	2572	rBV2	1898	1662	0.14%	0.017%
78	18.744	2593	2597	2599	rBV5	2655	3173	0.27%	0.033%
79	19.044	2646	2648	2649	rBV2	2417	1475	0.13%	0.015%
80	19.120	2658	2661	2662	rBV3	3409	3233	0.28%	0.033%
81	19.596	2740	2742	2746	rVB4	7439	8147	0.70%	0.084%
82	19.672	2751	2755	2759	rBV2	10078	14543	1.25%	0.151%
83	19.784	2772	2774	2775	rBV2	5070	3487	0.30%	0.036%
84	20.031	2810	2816	2824	rBV	796364	1159426	100.00%	12.001%
85	21.981	3141	3148	3155	rVB2	344464	605960	52.26%	6.272%
86	25.235	3691	3702	3714	rVB2	365299	1072483	92.50%	11.101%
87	25.476	3734	3743	3753	rVB	190984	570036	49.17%	5.900%




Sum of corrected areas: 9661307

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051518.D
Acq On : 15 Dec 2021 00:46
Operator : CG/JU
Sample : M4995-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5R7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

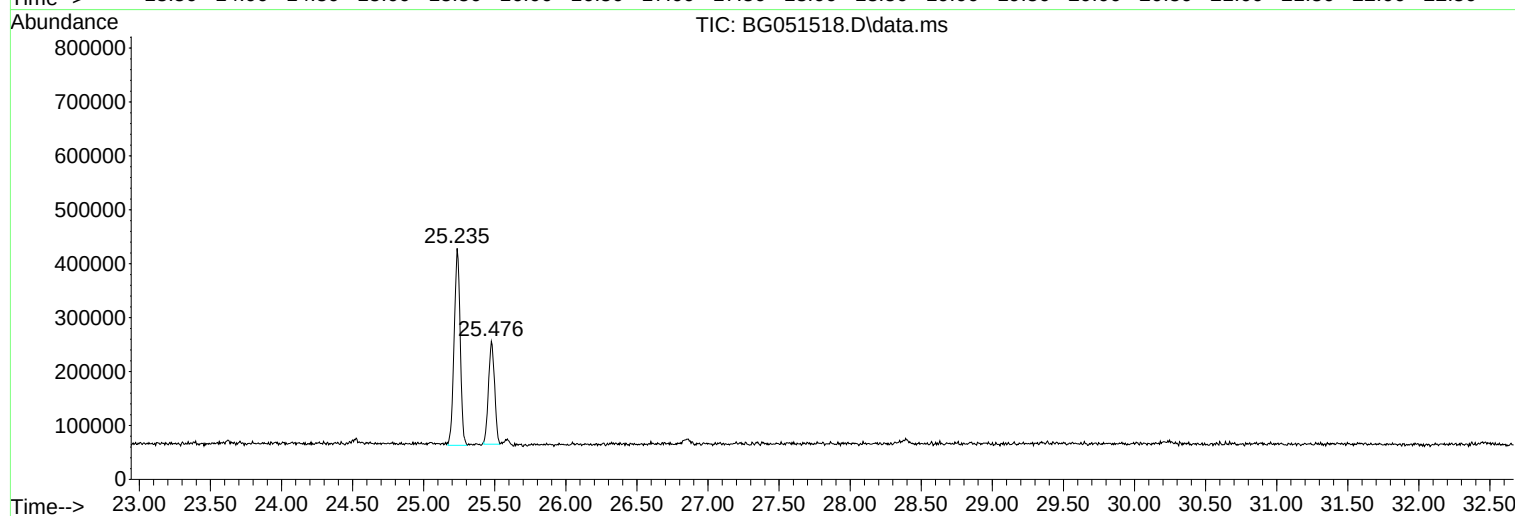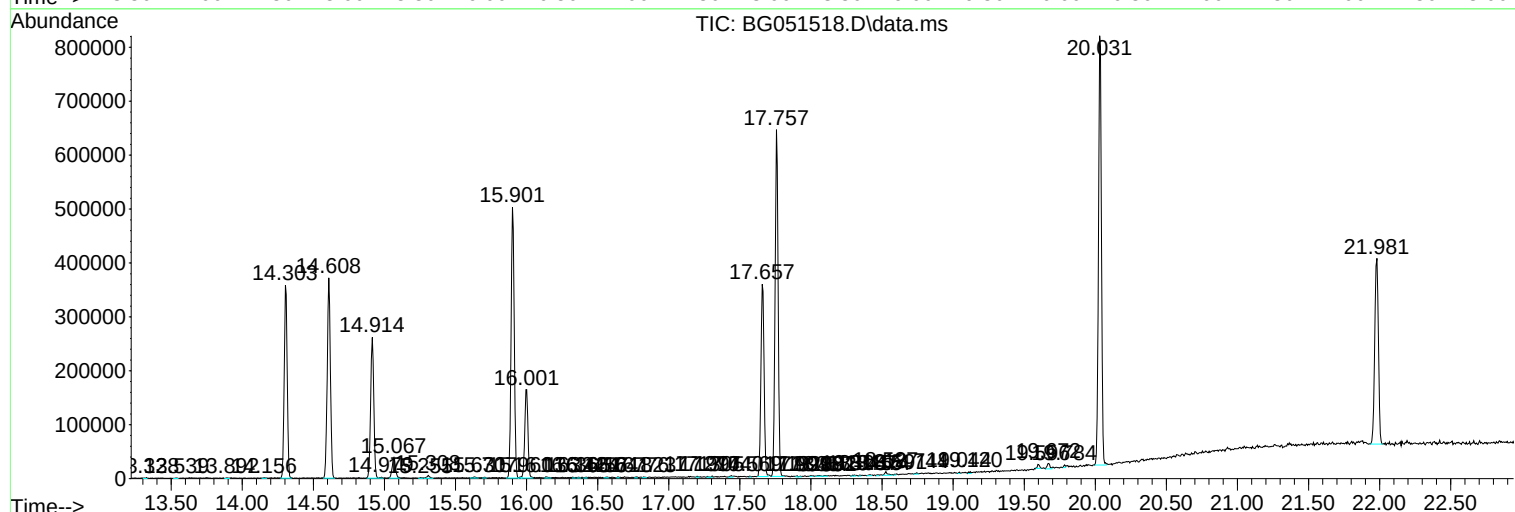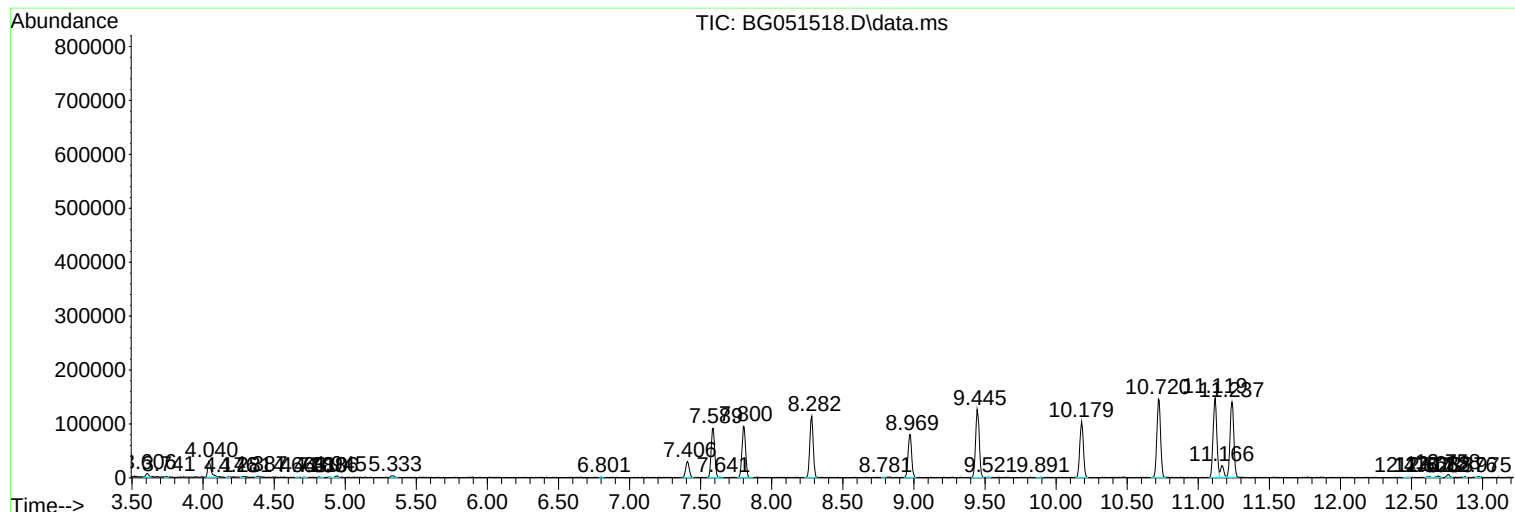

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051518.D
Acq On : 15 Dec 2021 00:46
Operator : CG/JU
Sample : M4995-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5R7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051518.D
Acq On : 15 Dec 2021 00:46
Operator : CG/JU
Sample : M4995-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5R7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc