

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051533.D
 Acq On : 15 Dec 2021 11:29
 Operator : CG/JU
 Sample : M4971-09
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.606	14	20	27	rVB2	8006	12147	0.76%	0.100%
2	4.035	90	93	105	rBV	41169	72664	4.54%	0.597%
3	4.293	130	137	138	rBV4	1808	2345	0.15%	0.019%
4	4.393	149	154	160	rVB2	3790	5426	0.34%	0.045%
5	4.833	223	229	230	rBV3	962	1614	0.10%	0.013%
6	5.339	311	315	318	rVB2	1430	2154	0.13%	0.018%
7	7.406	660	667	676	rVB	53184	89239	5.58%	0.733%
8	7.583	690	697	705	rBV	129712	216041	13.50%	1.775%
9	7.806	728	735	743	rVB	137150	243370	15.21%	1.999%
10	8.276	808	815	824	rBV	115026	188150	11.76%	1.546%
11	8.969	927	933	942	rVB	132687	222741	13.92%	1.830%
12	9.374	998	1002	1007	rBV2	807	1604	0.10%	0.013%
13	9.445	1007	1014	1021	rVV	177362	309420	19.34%	2.542%
14	9.521	1024	1027	1031	rVB2	1409	1771	0.11%	0.015%
15	10.179	1131	1139	1147	rBV	143048	254311	15.90%	2.089%
16	10.720	1224	1231	1238	rBV	219083	393310	24.58%	3.231%
17	11.113	1291	1298	1306	rBV	146553	269104	16.82%	2.211%
18	11.237	1311	1319	1328	rBV	187495	339938	21.25%	2.792%
19	12.411	1515	1519	1524	rBV	946	1677	0.10%	0.014%
20	12.682	1561	1565	1570	rBV3	3652	6430	0.40%	0.053%
21	13.798	1747	1755	1761	rBV5	3521	7403	0.46%	0.061%
22	14.303	1834	1841	1848	rBV	492692	699690	43.74%	5.748%
23	14.608	1886	1893	1900	rBV	492666	771397	48.22%	6.337%
24	14.914	1938	1945	1953	rVV	266606	405699	25.36%	3.333%
25	15.067	1965	1971	1980	rBV2	59185	97470	6.09%	0.801%
26	15.302	2009	2011	2015	rVB3	2595	2913	0.18%	0.024%
27	15.631	2063	2067	2072	rVV4	5128	7745	0.48%	0.064%
28	15.713	2076	2081	2082	rVB4	1376	2024	0.13%	0.017%
29	15.901	2106	2113	2120	rVB2	664687	1033408	64.59%	8.489%
30	15.995	2124	2129	2139	rBV	135240	207276	12.96%	1.703%
31	16.142	2149	2154	2159	rVB5	3406	4539	0.28%	0.037%
32	16.946	2287	2291	2294	rBV3	1438	2321	0.15%	0.019%
33	17.193	2331	2333	2336	rVB4	1584	1928	0.12%	0.016%
34	17.228	2336	2339	2340	rBV	1757	1699	0.11%	0.014%
35	17.657	2405	2412	2418	rBV	387319	564628	35.29%	4.638%
36	17.757	2422	2429	2436	rVV2	855031	1305096	81.58%	10.721%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051533.D
 Acq On : 15 Dec 2021 11:29
 Operator : CG/JU
 Sample : M4971-09
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.822	2438	2440	2443	rVB3	2559	2701	0.17%	0.022%
38	18.021	2469	2474	2476	rBV4	1731	2428	0.15%	0.020%
39	18.110	2485	2489	2490	rBV4	2109	1836	0.11%	0.015%
40	18.139	2490	2494	2496	rBV4	1735	2161	0.14%	0.018%
41	18.215	2506	2507	2510	rBV3	1350	1602	0.10%	0.013%
42	18.315	2520	2524	2528	rBV7	2745	4447	0.28%	0.037%
43	18.521	2558	2559	2562	rBV3	1916	1800	0.11%	0.015%
44	18.679	2585	2586	2589	rBV3	1641	1760	0.11%	0.014%
45	18.762	2598	2600	2602	rBV3	1846	1709	0.11%	0.014%
46	18.820	2607	2610	2611	rVV2	1583	1629	0.10%	0.013%
47	18.879	2618	2620	2623	rBV4	1879	1634	0.10%	0.013%
48	19.008	2640	2642	2645	rBV3	1849	2131	0.13%	0.018%
49	19.284	2688	2689	2691	rBV2	2421	2043	0.13%	0.017%
50	19.402	2707	2709	2710	rBV2	2717	2066	0.13%	0.017%
51	19.596	2739	2742	2747	rBV4	12161	17524	1.10%	0.144%
52	19.666	2750	2754	2759	rVB2	14921	18422	1.15%	0.151%
53	19.807	2776	2778	2779	rVB2	3770	1758	0.11%	0.014%
54	19.831	2779	2782	2783	rBV3	3249	3454	0.22%	0.028%
55	19.901	2792	2794	2797	rBV2	3828	3401	0.21%	0.028%
56	20.031	2810	2816	2823	rBV	1111365	1599837	100.00%	13.142%
57	21.975	3140	3147	3155	rVB2	360352	639840	39.99%	5.256%
58	25.235	3690	3702	3713	rVB2	507608	1516474	94.79%	12.457%
59	25.476	3733	3743	3753	rVB	199051	594052	37.13%	4.880%




Sum of corrected areas: 12173401

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051533.D
Acq On : 15 Dec 2021 11:29
Operator : CG/JU
Sample : M4971-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

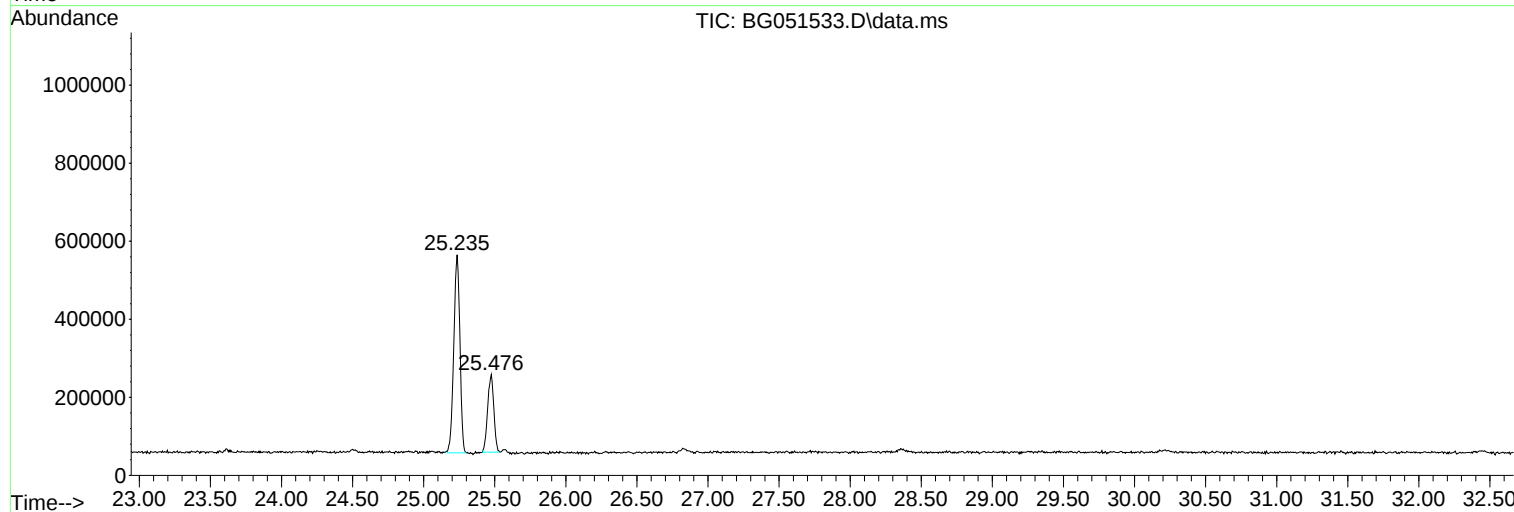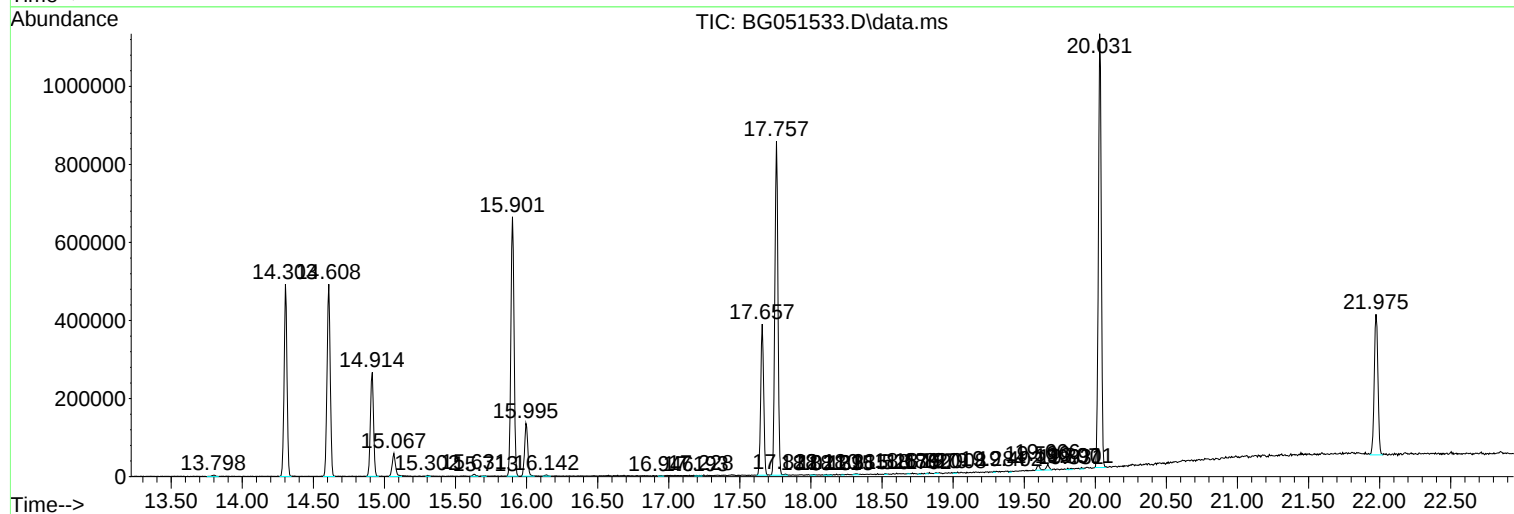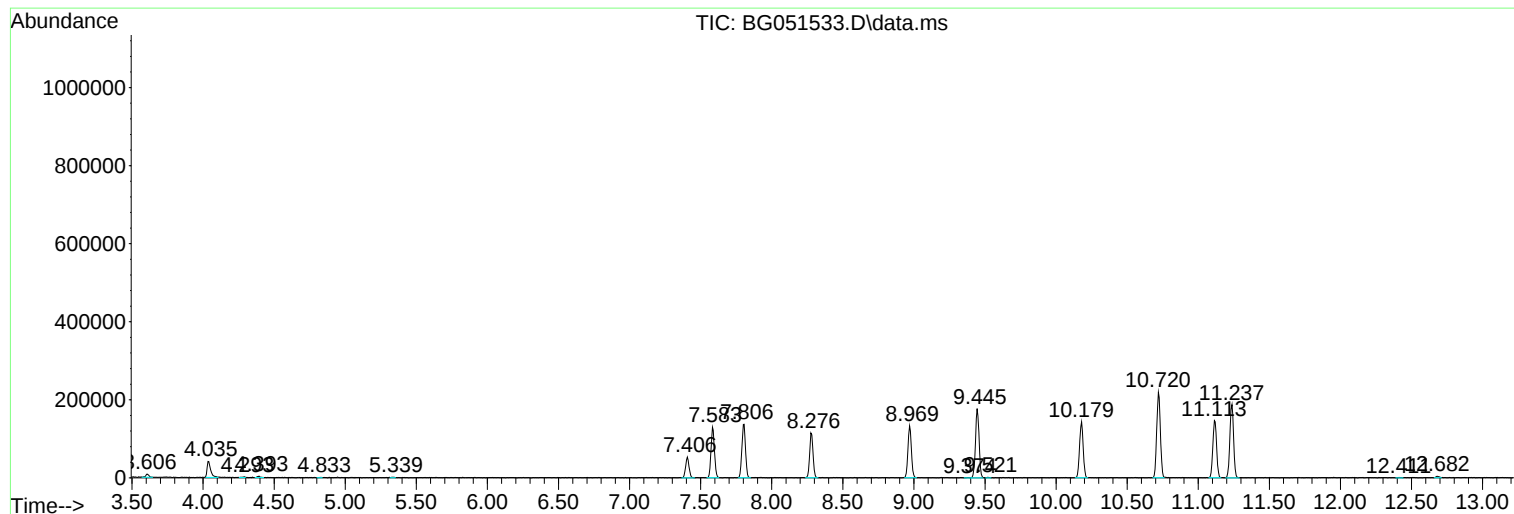

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051533.D
Acq On : 15 Dec 2021 11:29
Operator : CG/JU
Sample : M4971-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051533.D
Acq On : 15 Dec 2021 11:29
Operator : CG/JU
Sample : M4971-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------