

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051561.D
 Acq On : 16 Dec 2021 7:57
 Operator : CG/JU
 Sample : M4971-13
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.565	12	13	16	rBV2	1608	1426	0.12%	0.014%
2	3.606	16	20	27	rVV3	7384	12457	1.02%	0.119%
3	3.741	40	43	47	rBV3	1250	1662	0.14%	0.016%
4	3.982	82	84	88	rBV2	1083	1657	0.14%	0.016%
5	4.041	90	94	106	rBV	16705	32878	2.68%	0.313%
6	4.276	131	134	135	rBV2	1326	1366	0.11%	0.013%
7	4.293	135	137	141	rVB3	1814	1994	0.16%	0.019%
8	4.387	150	153	155	rBV3	2339	2242	0.18%	0.021%
9	5.333	313	314	317	rVB2	1816	1256	0.10%	0.012%
10	5.550	345	351	356	rBV2	4345	7211	0.59%	0.069%
11	7.407	661	667	674	rVB2	43388	74074	6.04%	0.705%
12	7.583	687	697	705	rBV	118957	195241	15.93%	1.858%
13	7.800	727	734	741	rBV	129486	215437	17.58%	2.050%
14	8.276	808	815	822	rVB	117530	200958	16.40%	1.913%
15	8.329	822	824	829	rBV	929	1388	0.11%	0.013%
16	8.640	872	877	883	rVB2	13663	24769	2.02%	0.236%
17	8.969	926	933	941	rVB2	111424	191125	15.60%	1.819%
18	9.445	1006	1014	1022	rBV	153375	279112	22.78%	2.656%
19	9.880	1081	1088	1093	rVB3	2209	3784	0.31%	0.036%
20	10.179	1131	1139	1148	rVB	124253	225639	18.41%	2.147%
21	10.461	1183	1187	1192	rBV2	1053	1845	0.15%	0.018%
22	10.720	1224	1231	1239	rBV	192259	338300	27.61%	3.220%
23	11.113	1290	1298	1305	rBV	158424	284782	23.24%	2.710%
24	11.237	1310	1319	1328	rBV	112765	211042	17.22%	2.008%
25	12.512	1533	1536	1538	rVB	1674	1761	0.14%	0.017%
26	12.676	1561	1564	1565	rBV	2048	1806	0.15%	0.017%
27	13.733	1739	1744	1752	rVB3	2796	4802	0.39%	0.046%
28	14.303	1835	1841	1849	rBV	417457	586045	47.82%	5.577%
29	14.532	1877	1880	1883	rBV	1582	1412	0.12%	0.013%
30	14.609	1886	1893	1902	rVB	416604	665077	54.27%	6.330%
31	14.914	1937	1945	1953	rVB	259497	414261	33.81%	3.943%
32	15.067	1963	1971	1978	rBV	47389	78291	6.39%	0.745%
33	15.302	2005	2011	2014	rVB4	1744	2552	0.21%	0.024%
34	15.631	2063	2067	2073	rBV2	6637	9179	0.75%	0.087%
35	15.701	2073	2079	2083	rBV5	1863	3315	0.27%	0.032%
36	15.901	2106	2113	2120	rVV	565434	866004	70.67%	8.242%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051561.D
 Acq On : 16 Dec 2021 7:57
 Operator : CG/JU
 Sample : M4971-13
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.995	2122	2129	2143	rVV	189234	283532	23.14%	2.698%
38	16.142	2152	2154	2159	rVB2	2414	3434	0.28%	0.033%
39	16.295	2179	2180	2184	rBV2	1536	1478	0.12%	0.014%
40	16.342	2184	2188	2191	rVV3	1303	1804	0.15%	0.017%
41	16.459	2206	2208	2213	rVB3	1240	1707	0.14%	0.016%
42	16.571	2222	2227	2228	rBV2	1632	1674	0.14%	0.016%
43	16.630	2230	2237	2243	rVV3	6996	11963	0.98%	0.114%
44	16.729	2252	2254	2258	rVB2	1251	1363	0.11%	0.013%
45	16.953	2289	2292	2294	rBV	1131	1462	0.12%	0.014%
46	17.011	2299	2302	2306	rVB3	1345	1431	0.12%	0.014%
47	17.387	2361	2366	2367	rBV3	1175	1361	0.11%	0.013%
48	17.446	2373	2376	2381	rVB5	2538	3284	0.27%	0.031%
49	17.605	2402	2403	2405	rBV	2202	1444	0.12%	0.014%
50	17.658	2405	2412	2419	rVV	356128	542014	44.23%	5.158%
51	17.757	2421	2429	2436	rVB2	681821	1025539	83.69%	9.760%
52	17.869	2445	2448	2450	rBV3	1382	1542	0.13%	0.015%
53	17.934	2453	2459	2460	rBV3	1678	2209	0.18%	0.021%
54	17.951	2460	2462	2466	rBV5	1961	2735	0.22%	0.026%
55	18.022	2471	2474	2475	rBV3	1757	1412	0.12%	0.013%
56	18.034	2475	2476	2479	rVB2	1494	1259	0.10%	0.012%
57	18.092	2483	2486	2489	rVV4	1165	1600	0.13%	0.015%
58	18.139	2491	2494	2496	rVB	1355	1259	0.10%	0.012%
59	18.192	2501	2503	2507	rVV4	1090	1361	0.11%	0.013%
60	18.233	2507	2510	2512	rVB2	1336	1248	0.10%	0.012%
61	18.321	2523	2525	2529	rVB3	1938	1467	0.12%	0.014%
62	18.357	2529	2531	2534	rVB3	1486	1455	0.12%	0.014%
63	18.427	2539	2543	2546	rBV4	1979	3181	0.26%	0.030%
64	18.456	2546	2548	2551	rVB3	1274	1367	0.11%	0.013%
65	18.527	2555	2560	2565	rBV6	10823	17087	1.39%	0.163%
66	18.668	2583	2584	2586	rBV	2144	1513	0.12%	0.014%
67	18.715	2589	2592	2595	rBV4	2090	2072	0.17%	0.020%
68	18.821	2606	2610	2612	rBV4	2544	2741	0.22%	0.026%
69	18.921	2625	2627	2629	rBV2	1854	1396	0.11%	0.013%
70	19.020	2641	2644	2646	rBV3	2146	2489	0.20%	0.024%
71	19.079	2652	2654	2656	rVB2	1531	1352	0.11%	0.013%
72	19.097	2656	2657	2659	rBV	2290	1238	0.10%	0.012%
73	19.267	2684	2686	2687	rVB2	2572	1590	0.13%	0.015%
74	19.297	2689	2691	2693	rVV2	1812	1588	0.13%	0.015%
75	19.320	2693	2695	2699	rVV4	2435	3184	0.26%	0.030%
76	19.479	2720	2722	2723	rBV2	2549	1417	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051561.D
 Acq On : 16 Dec 2021 7:57
 Operator : CG/JU
 Sample : M4971-13
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	19.596	2739	2742	2746	rVB2	9634	11008	0.90%	0.105%
78	19.667	2750	2754	2758	rVB	13566	14950	1.22%	0.142%
79	19.702	2758	2760	2762	rBV3	2767	2614	0.21%	0.025%
80	19.784	2771	2774	2777	rVB5	5571	5742	0.47%	0.055%
81	19.843	2783	2784	2787	rBV2	2540	2649	0.22%	0.025%
82	19.884	2789	2791	2794	rBV4	2239	2915	0.24%	0.028%
83	20.031	2810	2816	2824	rBV	837767	1225434	100.00%	11.662%
84	20.148	2834	2836	2837	rBV2	2879	2064	0.17%	0.020%
85	20.430	2882	2884	2886	rBV2	3708	2349	0.19%	0.022%
86	20.577	2908	2909	2910	rBV	4631	2113	0.17%	0.020%
87	21.588	3078	3081	3087	rVB8	9727	14649	1.20%	0.139%
88	21.975	3140	3147	3153	rBV	372666	602781	49.19%	5.737%
89	23.232	3359	3361	3363	rBV2	5950	2902	0.24%	0.028%
90	25.236	3691	3702	3715	rVB2	388340	1171010	95.56%	11.145%
91	25.471	3733	3742	3753	rVB3	183115	551265	44.99%	5.246%
92	26.099	3847	3849	3850	rBV2	5749	3636	0.30%	0.035%




Sum of corrected areas: 10507483

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051561.D
Acq On : 16 Dec 2021 7:57
Operator : CG/JU
Sample : M4971-13
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

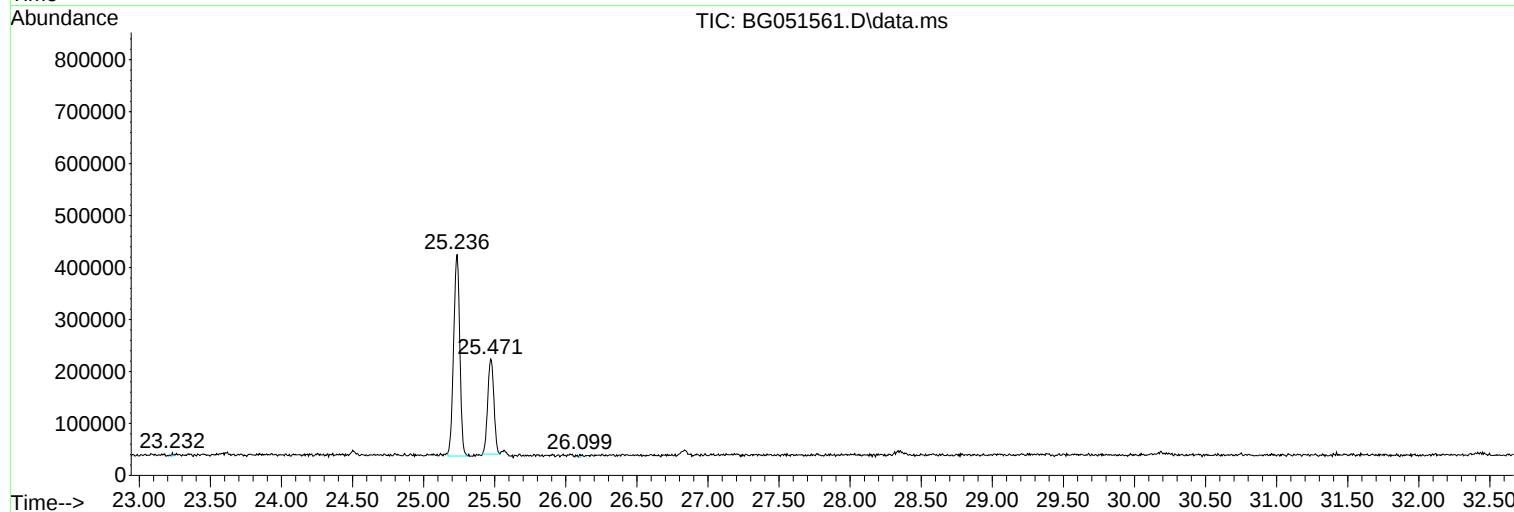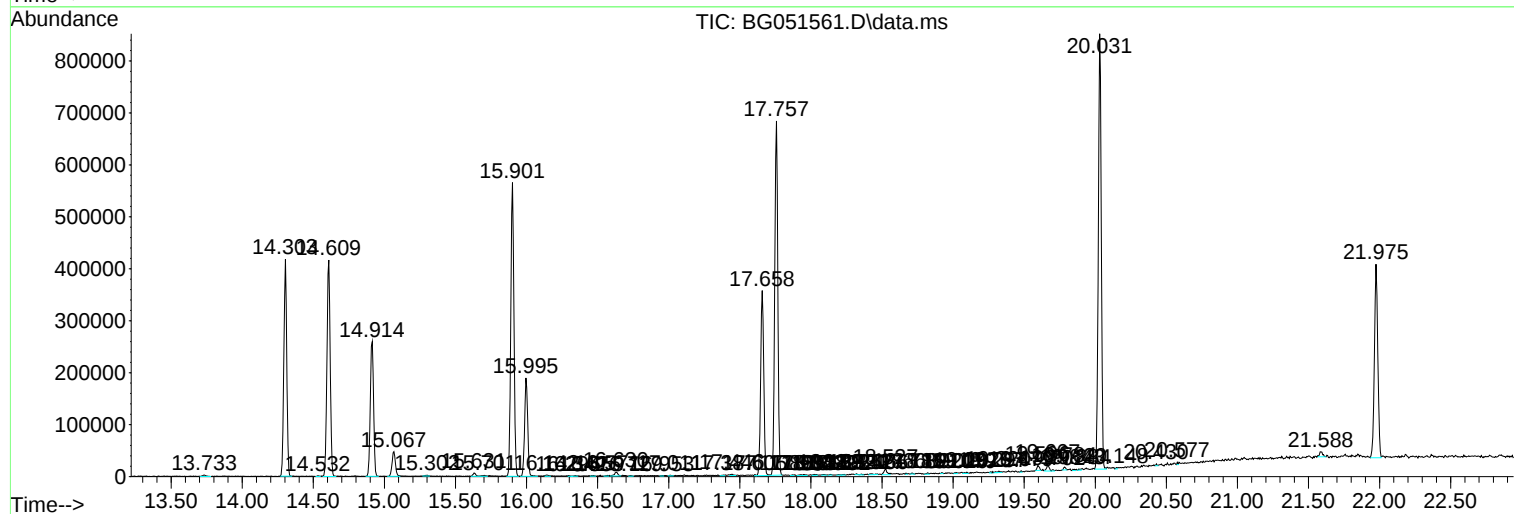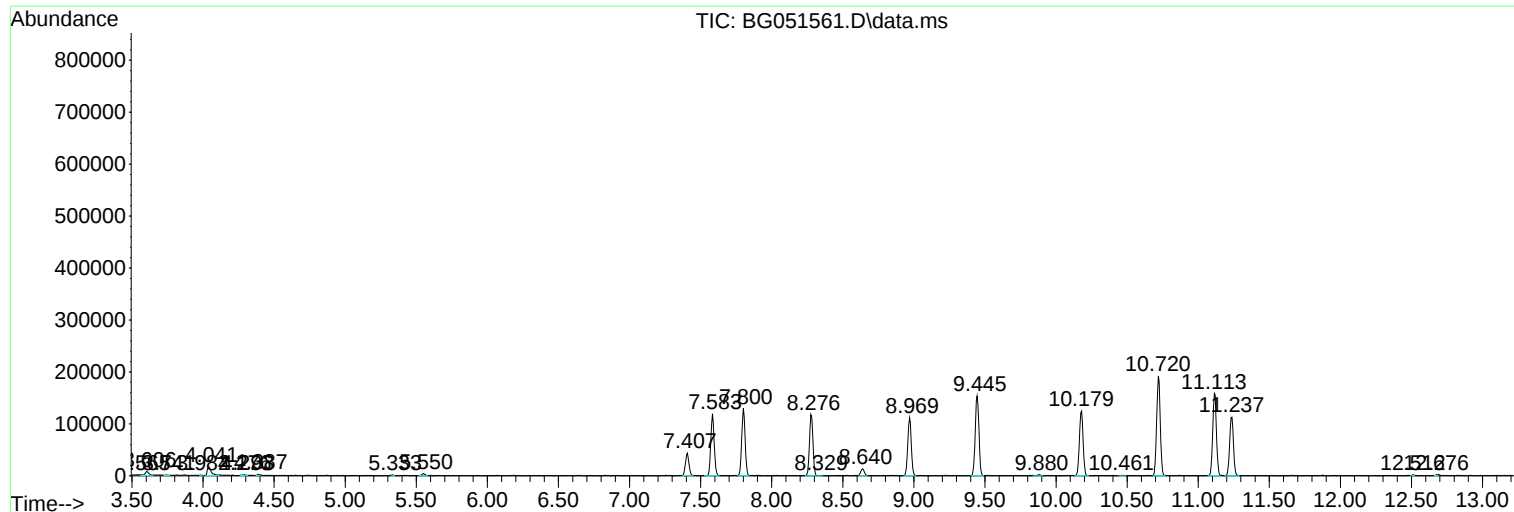

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051561.D
Acq On : 16 Dec 2021 7:57
Operator : CG/JU
Sample : M4971-13
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051561.D
Acq On : 16 Dec 2021 7:57
Operator : CG/JU
Sample : M4971-13
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
