

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051570.D
 Acq On : 16 Dec 2021 14:46
 Operator : CG/JU
 Sample : PB141433BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK433

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	10	14	16	rBV3	973	1582	0.12%	0.013%
2	3.606	16	20	24	rBV2	10434	14848	1.16%	0.122%
3	4.029	88	92	106	rBV	130491	224454	17.56%	1.841%
4	4.322	139	142	148	rVB3	1323	2302	0.18%	0.019%
5	4.387	148	153	159	rBV2	2511	4678	0.37%	0.038%
6	5.597	355	359	363	rBV2	1274	2273	0.18%	0.019%
7	5.732	378	382	386	rVV	891	1607	0.13%	0.013%
8	5.767	386	388	393	rVB2	1274	1403	0.11%	0.012%
9	7.406	659	667	676	rBV	191073	319692	25.01%	2.622%
10	7.583	689	697	705	rBV	126603	212351	16.61%	1.741%
11	7.800	727	734	743	rVB	170434	292675	22.90%	2.400%
12	8.276	809	815	822	rVB	120695	211565	16.55%	1.735%
13	8.969	926	933	943	rVB	219655	377140	29.50%	3.093%
14	9.445	1007	1014	1022	rBV	170210	303918	23.77%	2.492%
15	10.179	1131	1139	1146	rBV	146873	259109	20.27%	2.125%
16	10.720	1225	1231	1241	rVB	227326	397499	31.10%	3.260%
17	11.119	1292	1299	1308	rVV	164950	302269	23.65%	2.479%
18	11.237	1311	1319	1327	rVV	214009	387758	30.33%	3.180%
19	12.688	1559	1566	1570	rBV2	3759	6660	0.52%	0.055%
20	13.892	1768	1771	1776	rVB	1138	1737	0.14%	0.014%
21	14.303	1834	1841	1848	rVV	441896	647476	50.65%	5.310%
22	14.608	1883	1893	1900	rBV	479400	738453	57.77%	6.056%
23	14.914	1938	1945	1952	rVB	284639	454709	35.57%	3.729%
24	15.073	1965	1972	1984	rBV	208870	341915	26.75%	2.804%
25	15.901	2107	2113	2120	rBV	607205	923329	72.23%	7.572%
26	16.001	2123	2130	2139	rBV	185375	274904	21.51%	2.254%
27	16.065	2139	2141	2145	rVB2	1719	1517	0.12%	0.012%
28	16.142	2149	2154	2156	rBV2	2672	3914	0.31%	0.032%
29	16.318	2179	2184	2188	rBV2	778	1528	0.12%	0.013%
30	17.228	2337	2339	2344	rVB2	1019	1429	0.11%	0.012%
31	17.452	2373	2377	2381	rVB4	1854	2769	0.22%	0.023%
32	17.522	2386	2389	2392	rVB2	1916	1657	0.13%	0.014%
33	17.657	2405	2412	2419	rBV	403341	611255	47.82%	5.013%
34	17.757	2423	2429	2438	rVB	671710	1055974	82.61%	8.659%
35	18.021	2471	2474	2476	rVB3	1889	1746	0.14%	0.014%
36	18.209	2503	2506	2509	rBV4	1350	1814	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051570.D
 Acq On : 16 Dec 2021 14:46
 Operator : CG/JU
 Sample : PB141433BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK433

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	18.533	2557	2561	2563	rBV4	1230	1414	0.11%	0.012%
38	18.650	2578	2581	2583	rBV3	1357	1941	0.15%	0.016%
39	18.738	2595	2596	2599	rBV3	1619	1674	0.13%	0.014%
40	18.809	2605	2608	2610	rBV2	2296	2027	0.16%	0.017%
41	19.003	2637	2641	2643	rBV3	2285	3751	0.29%	0.031%
42	19.331	2695	2697	2701	rBV3	1586	2425	0.19%	0.020%
43	19.396	2704	2708	2711	rBV6	2755	4249	0.33%	0.035%
44	19.602	2737	2743	2746	rBV5	11598	18953	1.48%	0.155%
45	19.672	2750	2755	2758	rVV	9037	14008	1.10%	0.115%
46	19.872	2787	2789	2791	rBV3	2297	2425	0.19%	0.020%
47	20.036	2810	2817	2824	rBV	878826	1278314	100.00%	10.483%
48	20.318	2863	2865	2866	rVB2	3197	1588	0.12%	0.013%
49	20.459	2887	2889	2892	rBV4	4785	5216	0.41%	0.043%
50	21.981	3141	3148	3155	rBV	390270	665785	52.08%	5.460%
51	25.241	3692	3703	3714	rVB	389735	1181090	92.39%	9.685%
52	25.482	3734	3744	3755	rVB2	209286	619816	48.49%	5.083%




Sum of corrected areas: 12194585

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051570.D
Acq On : 16 Dec 2021 14:46
Operator : CG/JU
Sample : PB141433BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

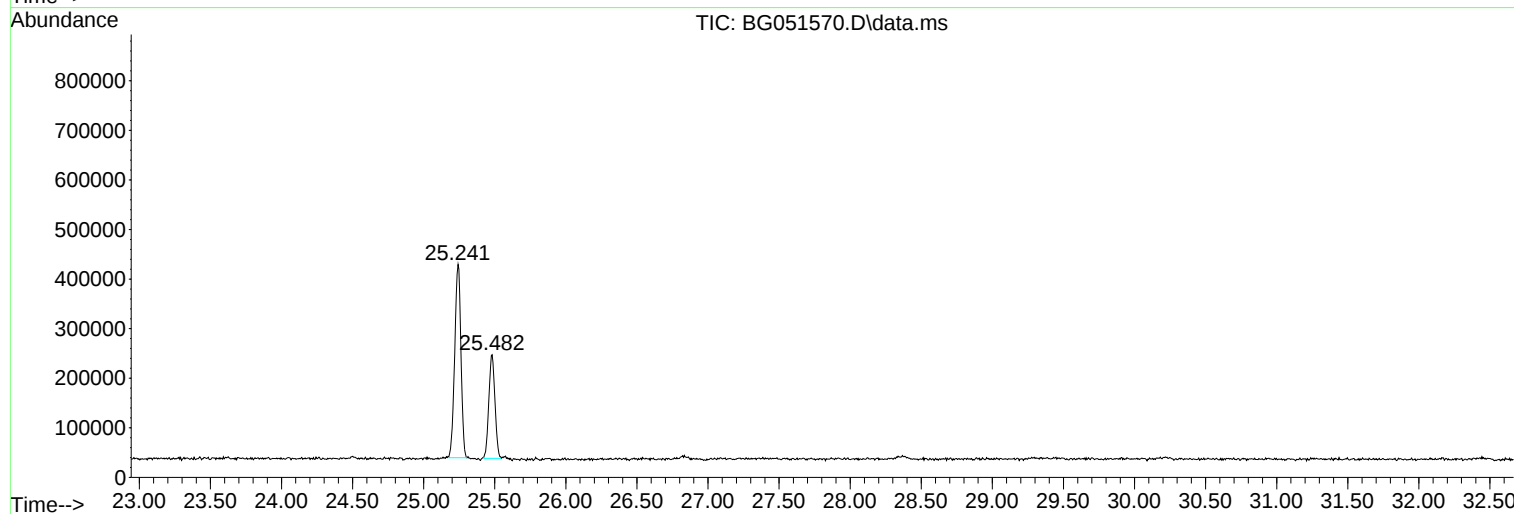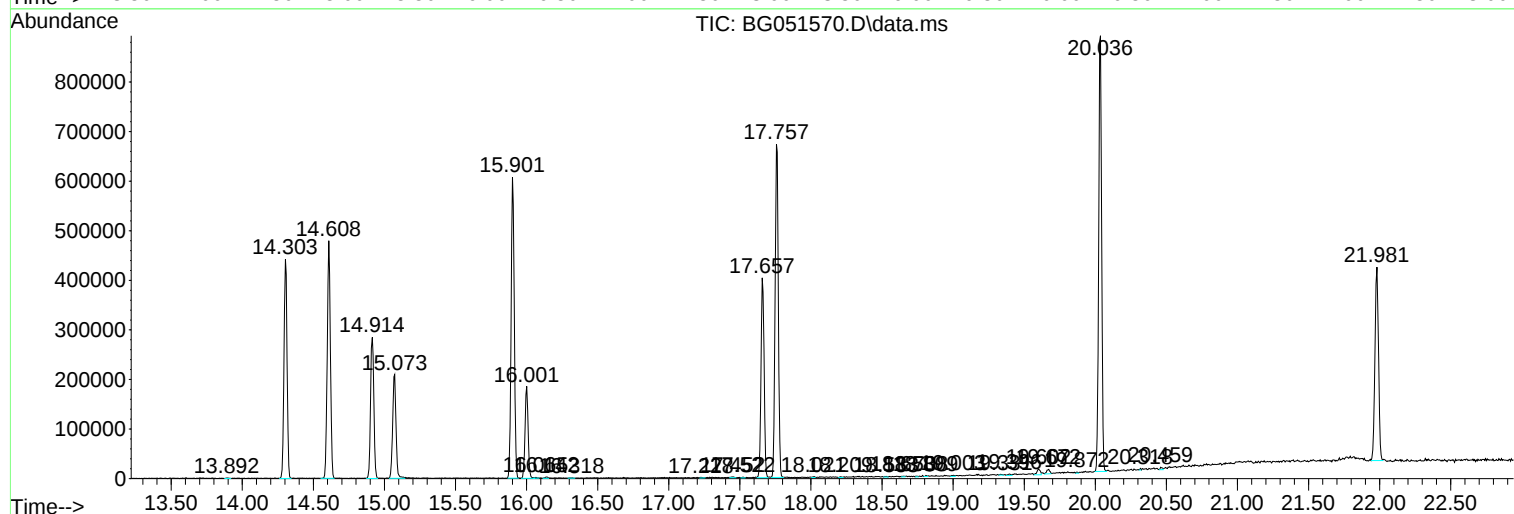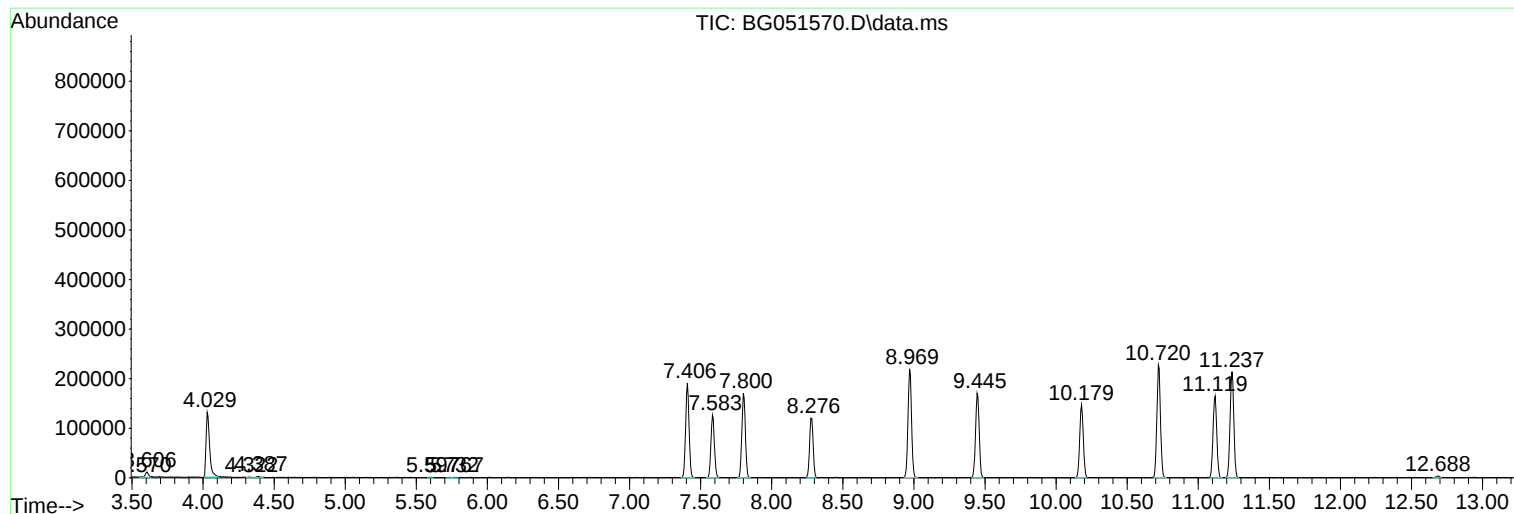

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051570.D
Acq On : 16 Dec 2021 14:46
Operator : CG/JU
Sample : PB141433BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051570.D
Acq On : 16 Dec 2021 14:46
Operator : CG/JU
Sample : PB141433BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK433

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------