

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051571.D
 Acq On : 16 Dec 2021 15:26
 Operator : CG/JU
 Sample : PB141435BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK435

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.606	16	20	24	rBV3	12190	18228	1.31%	0.135%
2	4.029	88	92	103	rBV	151918	266642	19.11%	1.976%
3	4.099	103	104	109	rVB3	2396	2776	0.20%	0.021%
4	4.217	122	124	128	rVB3	1264	1557	0.11%	0.012%
5	4.252	128	130	133	rBV2	1239	1567	0.11%	0.012%
6	4.387	148	153	158	rBV2	2538	3483	0.25%	0.026%
7	4.892	234	239	242	rBV3	1231	1512	0.11%	0.011%
8	5.815	393	396	399	rVB2	1268	1767	0.13%	0.013%
9	7.406	660	667	674	rBV	217150	364521	26.12%	2.701%
10	7.583	690	697	705	rBV	140528	237056	16.99%	1.757%
11	7.800	725	734	744	rBV	196353	331923	23.79%	2.459%
12	8.282	809	816	822	rBV	135339	238464	17.09%	1.767%
13	8.969	926	933	942	rBV	249472	425125	30.47%	3.150%
14	9.445	1005	1014	1023	rVB	190822	343543	24.62%	2.546%
15	10.179	1131	1139	1147	rBV2	165749	296706	21.26%	2.199%
16	10.720	1222	1231	1242	rBV	251401	445642	31.94%	3.302%
17	11.119	1291	1299	1307	rBV	178200	336494	24.11%	2.493%
18	11.237	1311	1319	1327	rBV2	234530	432177	30.97%	3.202%
19	12.682	1562	1565	1572	rVB2	4338	6318	0.45%	0.047%
20	14.303	1834	1841	1849	rBV	492517	704900	50.52%	5.223%
21	14.608	1885	1893	1901	rBV	514824	812301	58.21%	6.019%
22	14.914	1937	1945	1952	rVB	330240	504276	36.14%	3.737%
23	15.067	1965	1971	1979	rBV	236205	374650	26.85%	2.776%
24	15.901	2102	2113	2121	rVB	675589	1020348	73.12%	7.560%
25	16.001	2123	2130	2137	rBV	204584	308625	22.12%	2.287%
26	16.136	2150	2153	2157	rBV3	2331	3197	0.23%	0.024%
27	16.964	2291	2294	2296	rBV2	1211	1450	0.10%	0.011%
28	17.440	2374	2375	2379	rVB3	1925	1869	0.13%	0.014%
29	17.657	2404	2412	2419	rBV	427452	664245	47.60%	4.922%
30	17.716	2419	2422	2423	rBV2	1664	1951	0.14%	0.014%
31	17.757	2423	2429	2438	rVB	778804	1153041	82.63%	8.544%
32	17.951	2459	2462	2464	rVV2	1932	2274	0.16%	0.017%
33	18.022	2472	2474	2478	rVV3	2505	2426	0.17%	0.018%
34	18.063	2478	2481	2485	rVB4	1593	2042	0.15%	0.015%
35	18.127	2491	2492	2497	rVB4	1361	2018	0.14%	0.015%
36	18.627	2575	2577	2581	rVB3	1532	1670	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051571.D
 Acq On : 16 Dec 2021 15:26
 Operator : CG/JU
 Sample : PB141435BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK435

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	19.243	2680	2682	2685	rBV4	1431	1399	0.10%	0.010%
38	19.361	2701	2702	2704	rBV2	1749	1514	0.11%	0.011%
39	19.396	2706	2708	2710	rVV3	2204	1782	0.13%	0.013%
40	19.431	2712	2714	2717	rBV5	1959	2320	0.17%	0.017%
41	19.461	2717	2719	2722	rBV4	2072	2329	0.17%	0.017%
42	19.602	2738	2743	2749	rBV3	11895	18795	1.35%	0.139%
43	19.666	2749	2754	2760	rVV2	11573	17801	1.28%	0.132%
44	19.866	2786	2788	2790	rBV3	1822	1722	0.12%	0.013%
45	20.031	2810	2816	2823	rBV	943128	1395379	100.00%	10.339%
46	20.107	2826	2829	2830	rBV2	3006	2452	0.18%	0.018%
47	20.201	2843	2845	2847	rBV3	3259	2515	0.18%	0.019%
48	20.271	2854	2857	2859	rBV3	3729	4557	0.33%	0.034%
49	21.857	3125	3127	3129	rBV2	5625	4103	0.29%	0.030%
50	21.975	3141	3147	3154	rVB	425167	727083	52.11%	5.387%
51	22.339	3207	3209	3211	rBV3	6030	4760	0.34%	0.035%
52	25.235	3691	3702	3712	rVB2	431771	1289222	92.39%	9.553%
53	25.476	3732	3743	3752	rBV2	224694	701285	50.26%	5.196%




Sum of corrected areas: 13495802

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051571.D
Acq On : 16 Dec 2021 15:26
Operator : CG/JU
Sample : PB141435BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK435

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

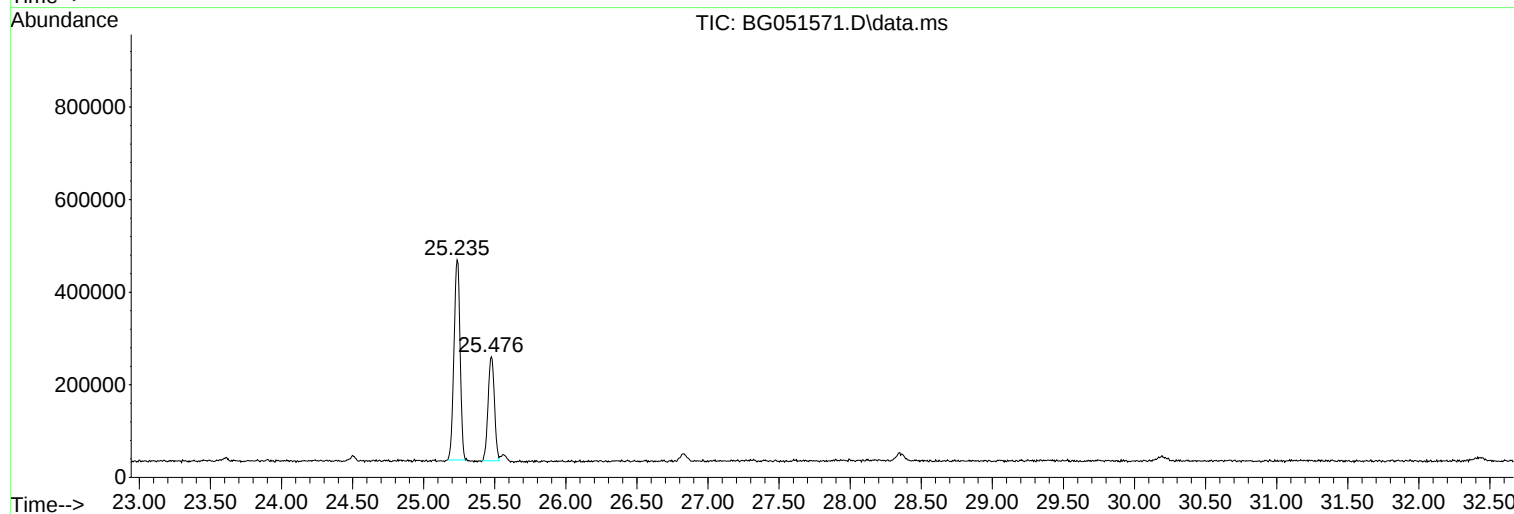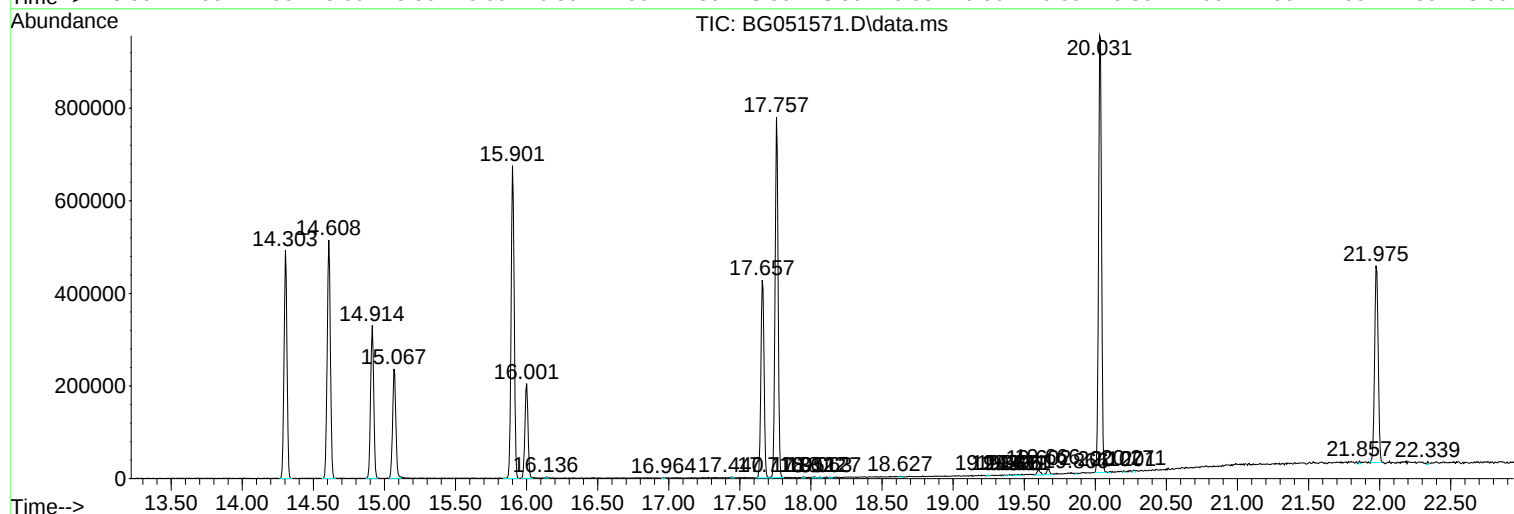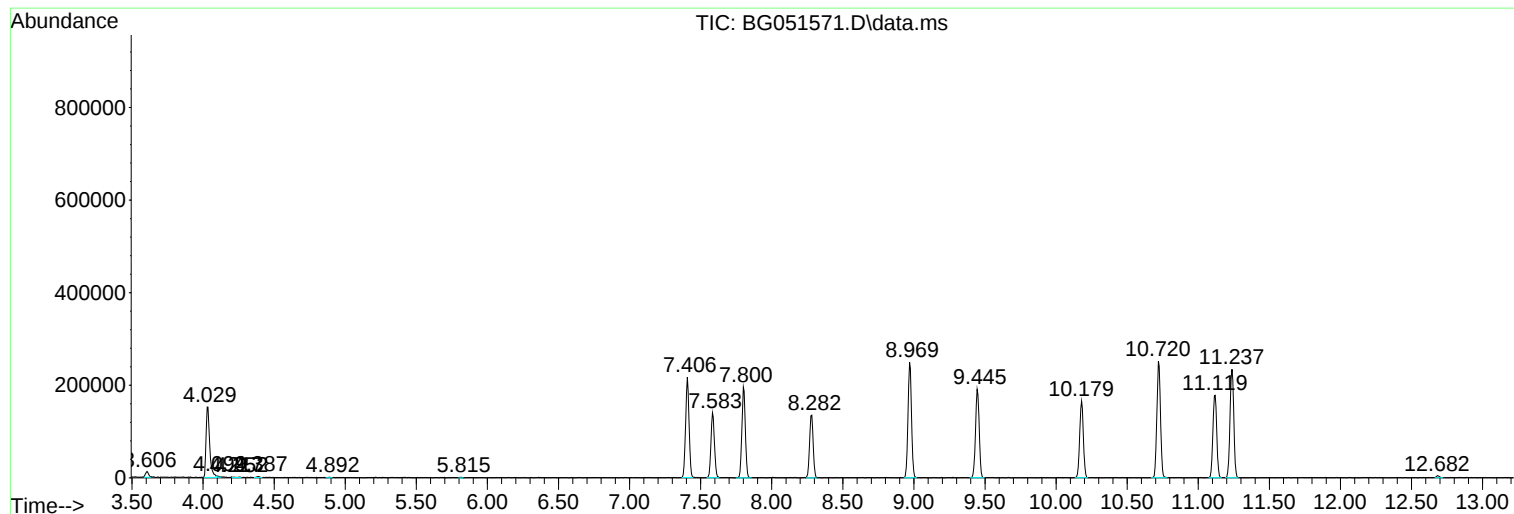

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051571.D
Acq On : 16 Dec 2021 15:26
Operator : CG/JU
Sample : PB141435BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK435

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051571.D
Acq On : 16 Dec 2021 15:26
Operator : CG/JU
Sample : PB141435BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK435

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc