

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051580.D
 Acq On : 16 Dec 2021 21:35
 Operator : CG/JU
 Sample : M5013-01DL2 50X
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.392	150	154	159	rBV5	1804	3983	0.35%	0.073%
2	5.614	357	362	363	rBV	999	1476	0.13%	0.027%
3	7.411	663	668	672	rBV3	2001	2970	0.26%	0.054%
4	7.488	677	681	686	rBV	2189	3203	0.28%	0.059%
5	7.587	693	698	701	rBV2	2939	4546	0.40%	0.083%
6	7.623	701	704	706	rVV	1439	1643	0.15%	0.030%
7	7.805	729	735	741	rVB4	2843	4632	0.41%	0.085%
8	7.922	748	755	761	rVB3	4793	8010	0.71%	0.146%
9	8.275	809	815	823	rVB	111088	189899	16.83%	3.469%
10	8.416	831	839	845	rBV3	6380	12574	1.11%	0.230%
11	8.668	876	882	886	rVB2	4845	7345	0.65%	0.134%
12	8.921	922	925	928	rBV	2323	2304	0.20%	0.042%
13	8.974	930	934	938	rVV2	2219	3968	0.35%	0.072%
14	9.450	1010	1015	1018	rBV2	2563	4138	0.37%	0.076%
15	9.479	1018	1020	1025	rVB3	2338	2403	0.21%	0.044%
16	9.931	1094	1097	1101	rBV3	1161	1538	0.14%	0.028%
17	9.984	1101	1106	1112	rVB3	1557	2787	0.25%	0.051%
18	10.108	1123	1127	1130	rVB	978	1447	0.13%	0.026%
19	10.178	1133	1139	1144	rVV2	1735	3316	0.29%	0.061%
20	10.231	1147	1148	1154	rVB2	1892	2156	0.19%	0.039%
21	10.301	1154	1160	1161	rBV	1164	1477	0.13%	0.027%
22	10.354	1164	1169	1172	rVV3	2825	3594	0.32%	0.066%
23	10.472	1181	1189	1191	rBV2	3243	6674	0.59%	0.122%
24	10.513	1191	1196	1203	rVV5	7832	14685	1.30%	0.268%
25	10.660	1217	1221	1225	rVB3	2710	4296	0.38%	0.078%
26	10.719	1227	1231	1238	rVB2	3224	4826	0.43%	0.088%
27	10.995	1274	1278	1282	rBV3	1213	1725	0.15%	0.032%
28	11.118	1291	1299	1302	rBV	148406	270044	23.93%	4.933%
29	11.165	1302	1307	1317	rVV	608083	1128425	100.00%	20.612%
30	11.282	1320	1327	1333	rVB	7067	11748	1.04%	0.215%
31	12.469	1526	1529	1530	rVV	1906	1987	0.18%	0.036%
32	12.487	1530	1532	1534	rVV2	1653	1673	0.15%	0.031%
33	12.651	1555	1560	1568	rVV2	3922	6942	0.62%	0.127%
34	12.757	1570	1578	1586	rBV	221649	358913	31.81%	6.556%
35	12.869	1591	1597	1604	rVB2	9836	17488	1.55%	0.319%
36	12.974	1604	1615	1624	rBV	125137	204987	18.17%	3.744%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051580.D
 Acq On : 16 Dec 2021 21:35
 Operator : CG/JU
 Sample : M5013-01DL2 50X
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	13.315	1669	1673	1674	rVV	1522	2027	0.18%	0.037%
38	13.750	1740	1747	1752	rVV	30773	47356	4.20%	0.865%
39	13.944	1775	1780	1786	rBV2	10412	14150	1.25%	0.258%
40	14.085	1798	1804	1811	rVB4	9886	23594	2.09%	0.431%
41	14.231	1824	1829	1834	rBV3	14354	23661	2.10%	0.432%
42	14.296	1834	1840	1845	rVV3	12860	23086	2.05%	0.422%
43	14.472	1865	1870	1874	rBV3	3615	6791	0.60%	0.124%
44	14.502	1874	1875	1880	rVV4	2012	1571	0.14%	0.029%
45	14.601	1886	1892	1903	rVV7	12888	28877	2.56%	0.527%
46	14.913	1935	1945	1950	rBV	263377	413784	36.67%	7.558%
47	14.977	1950	1956	1961	rVV	139830	226413	20.06%	4.136%
48	15.030	1961	1965	1970	rVV	8840	13156	1.17%	0.240%
49	15.083	1970	1974	1976	rVB3	1839	2811	0.25%	0.051%
50	15.177	1987	1990	1992	rVB4	1497	1658	0.15%	0.030%
51	15.218	1992	1997	2001	rVB2	2795	3688	0.33%	0.067%
52	15.306	2005	2012	2019	rBV	84388	127685	11.32%	2.332%
53	15.823	2097	2100	2102	rVV2	1664	1695	0.15%	0.031%
54	15.900	2106	2113	2117	rVV3	10729	16139	1.43%	0.295%
55	15.953	2117	2122	2128	rVV	63203	96236	8.53%	1.758%
56	16.005	2128	2131	2133	rVV3	1350	1653	0.15%	0.030%
57	16.082	2140	2144	2147	rVV3	2361	3911	0.35%	0.071%
58	16.117	2147	2150	2154	rVV3	4423	6579	0.58%	0.120%
59	16.205	2160	2165	2168	rVV3	1971	3379	0.30%	0.062%
60	16.246	2168	2172	2179	rVB3	5986	9513	0.84%	0.174%
61	16.393	2191	2197	2205	rBV5	6100	13879	1.23%	0.254%
62	16.622	2229	2236	2242	rVB2	17576	29617	2.62%	0.541%
63	16.799	2262	2266	2269	rVB3	1441	2226	0.20%	0.041%
64	16.922	2283	2287	2289	rBV3	2106	2877	0.25%	0.053%
65	17.098	2314	2317	2319	rBV3	2201	2319	0.21%	0.042%
66	17.239	2337	2341	2345	rBV3	1346	2046	0.18%	0.037%
67	17.304	2347	2352	2358	rVB3	10025	14668	1.30%	0.268%
68	17.439	2372	2375	2377	rBV3	1635	2038	0.18%	0.037%
69	17.474	2377	2381	2386	rVB3	6189	9639	0.85%	0.176%
70	17.656	2404	2412	2417	rBV	358798	561454	49.76%	10.255%
71	17.703	2417	2420	2425	rVV	76541	103162	9.14%	1.884%
72	17.756	2425	2429	2434	rVB	13924	19468	1.73%	0.356%
73	17.850	2440	2445	2448	rBV5	1893	3206	0.28%	0.059%
74	17.985	2464	2468	2471	rVB2	1460	2090	0.19%	0.038%
75	18.050	2473	2479	2485	rBV	40574	62865	5.57%	1.148%
76	18.250	2512	2513	2516	rBV2	1608	1751	0.16%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
 Data File : BG051580.D
 Acq On : 16 Dec 2021 21:35
 Operator : CG/JU
 Sample : M5013-01DL2 50X
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLT0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	18.484	2552	2553	2558	rVB2	1376	1580	0.14%	0.029%
78	18.537	2558	2562	2564	rVB4	1767	2138	0.19%	0.039%
79	18.578	2564	2569	2572	rBV5	3013	5659	0.50%	0.103%
80	18.725	2590	2594	2598	rBV5	3974	5275	0.47%	0.096%
81	18.796	2604	2606	2607	rBV2	1466	1484	0.13%	0.027%
82	18.902	2622	2624	2628	rVB2	2420	2206	0.20%	0.040%
83	19.060	2646	2651	2655	rBV4	3521	5626	0.50%	0.103%
84	19.225	2677	2679	2682	rBV4	1455	1464	0.13%	0.027%
85	19.366	2702	2703	2705	rBV2	1457	1467	0.13%	0.027%
86	19.430	2712	2714	2718	rVB5	2484	2729	0.24%	0.050%
87	19.648	2749	2751	2752	rBV2	2175	1854	0.16%	0.034%
88	19.695	2756	2759	2762	rVV2	6382	7295	0.65%	0.133%
89	19.924	2796	2798	2800	rBV3	2785	2279	0.20%	0.042%
90	20.029	2811	2816	2821	rBV	16882	25251	2.24%	0.461%
91	20.341	2867	2869	2870	rBV2	3004	2744	0.24%	0.050%
92	20.447	2886	2887	2888	rBV	4004	2219	0.20%	0.041%
93	20.576	2907	2909	2910	rBV2	3252	1669	0.15%	0.030%
94	20.922	2966	2968	2970	rBV3	4977	5289	0.47%	0.097%
95	21.980	3141	3148	3154	rVB	345941	584014	51.75%	10.668%
96	25.475	3733	3743	3754	rVB3	185755	562604	49.86%	10.277%
97	25.863	3807	3809	3810	rBV2	4760	2885	0.26%	0.053%
98	25.968	3825	3827	3829	rBV3	4885	2201	0.20%	0.040%
99	29.158	4368	4370	4371	rBV2	5719	3944	0.35%	0.072%
100	32.325	4907	4909	4911	rBV2	6552	4249	0.38%	0.078%




Sum of corrected areas: 5474665

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051580.D
Acq On : 16 Dec 2021 21:35
Operator : CG/JU
Sample : M5013-01DL2 50X
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLT0DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

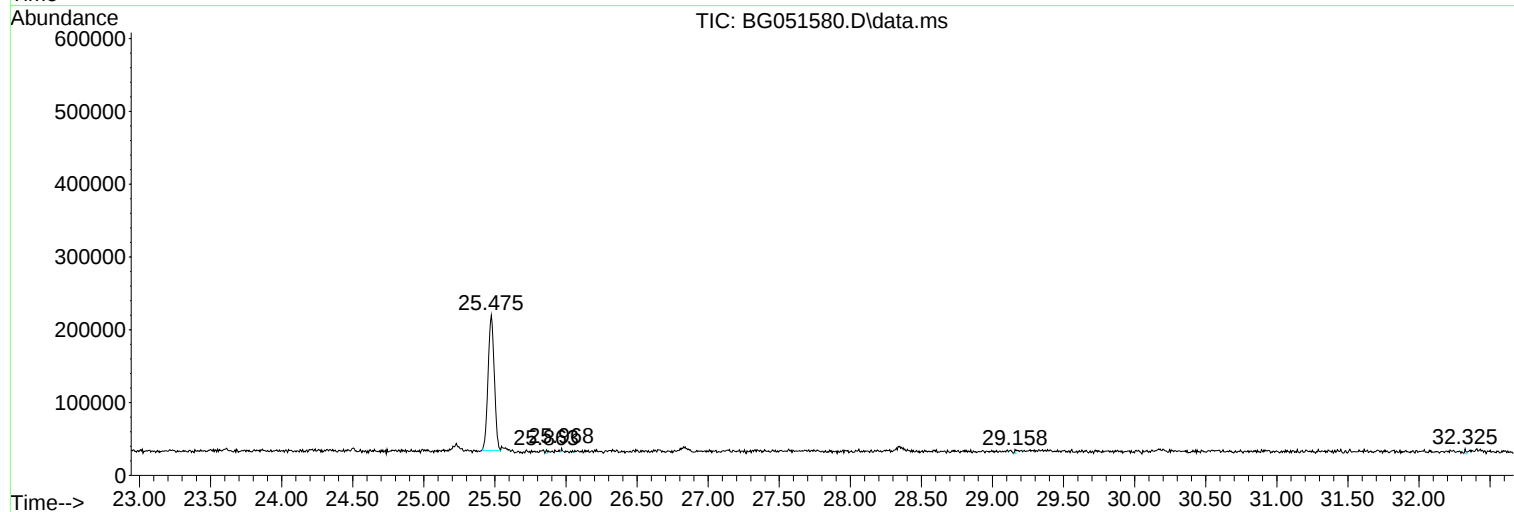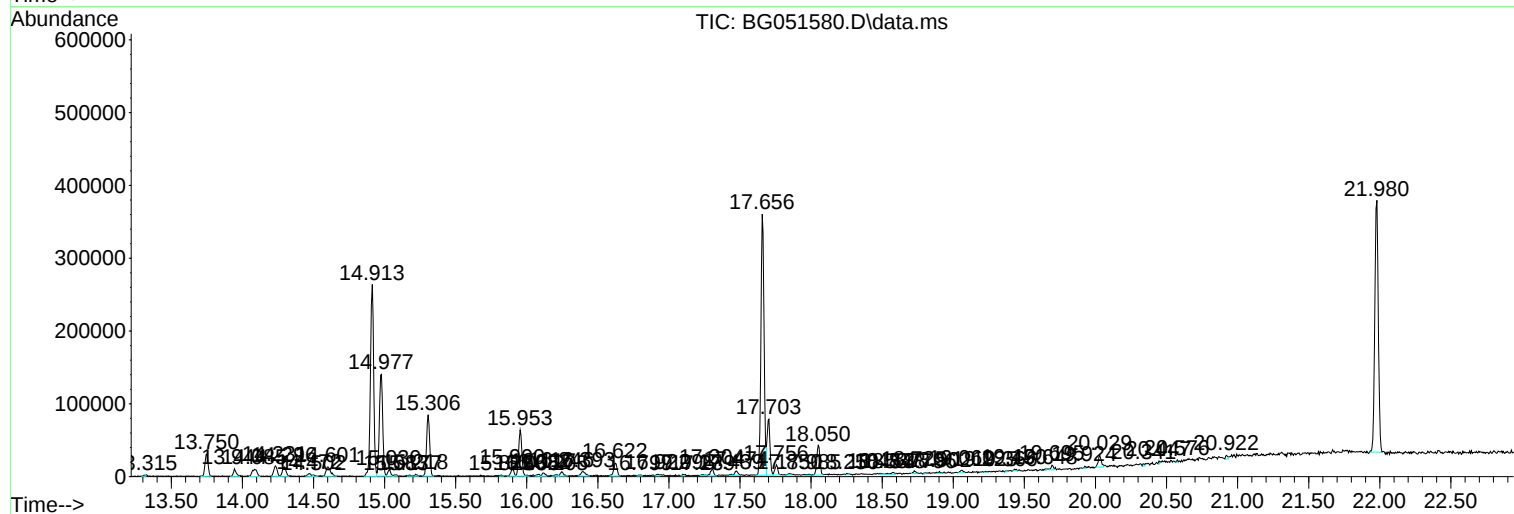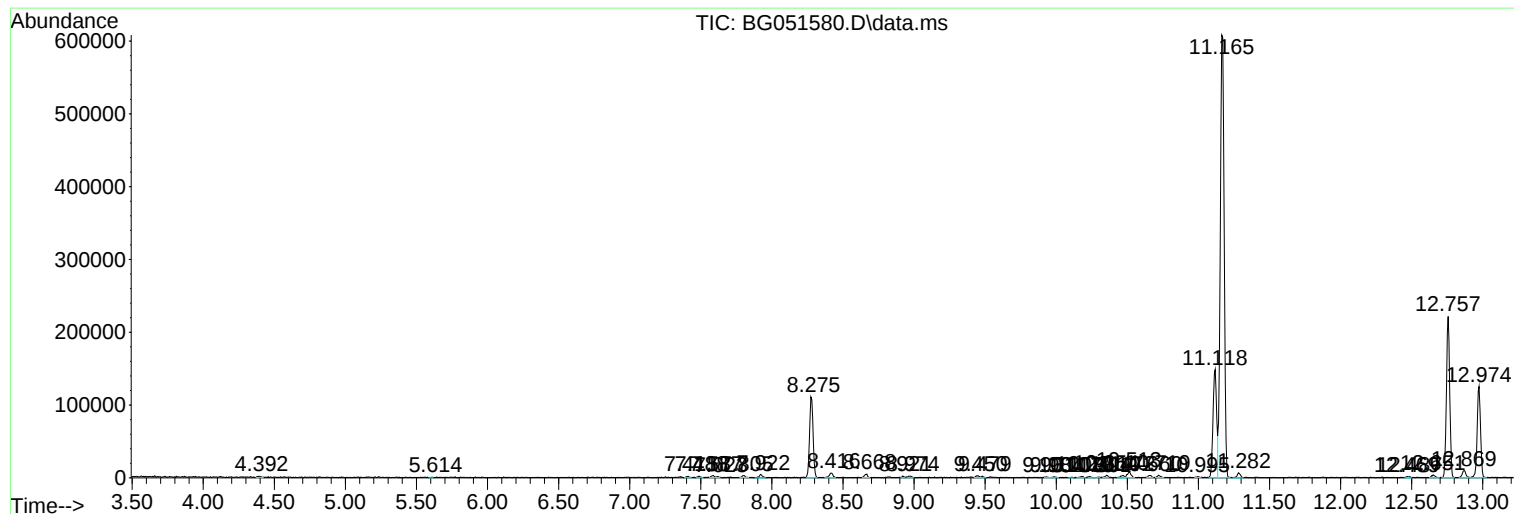

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051580.D
Acq On : 16 Dec 2021 21:35
Operator : CG/JU
Sample : M5013-01DL2 50X
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLT0DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121421\
Data File : BG051580.D
Acq On : 16 Dec 2021 21:35
Operator : CG/JU
Sample : M5013-01DL2 50X
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLT0DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------