
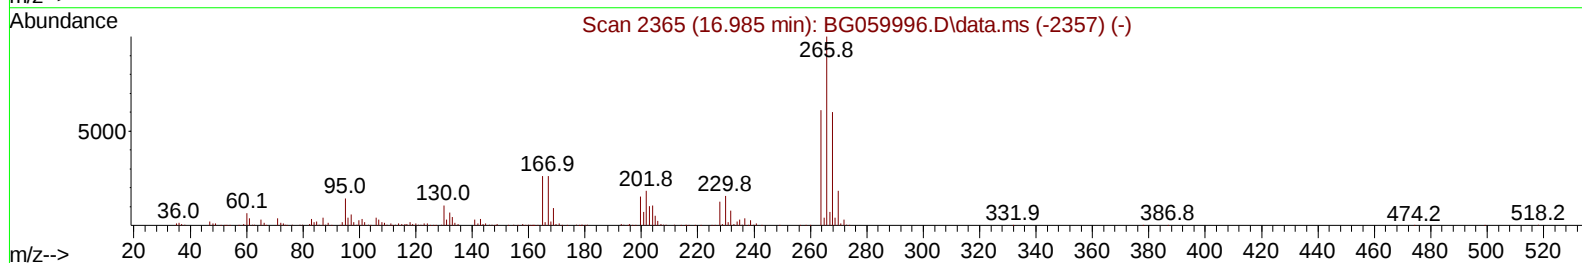
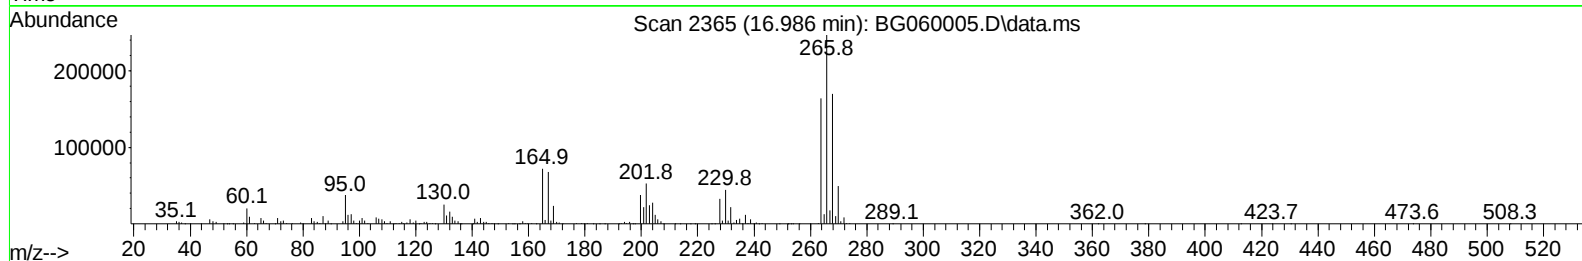


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060005.D
Acq On : 14 Dec 2023 9:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 10:56:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

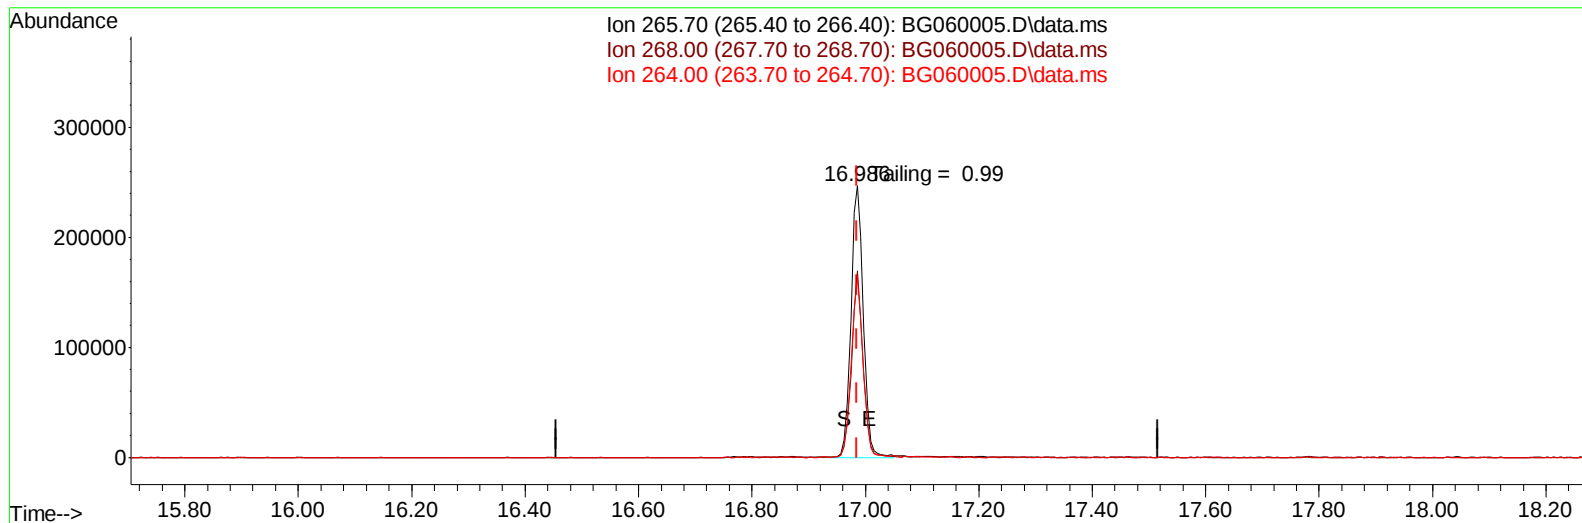




TIC: BG060005.D\data.ms

(70) Pentachlorophenol (C)**16.986min (+ 0.001) 61522.01 ng****response 370761**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	68.70
264.00	61.00	66.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060005.D
Acq On : 14 Dec 2023 9:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 10:56:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

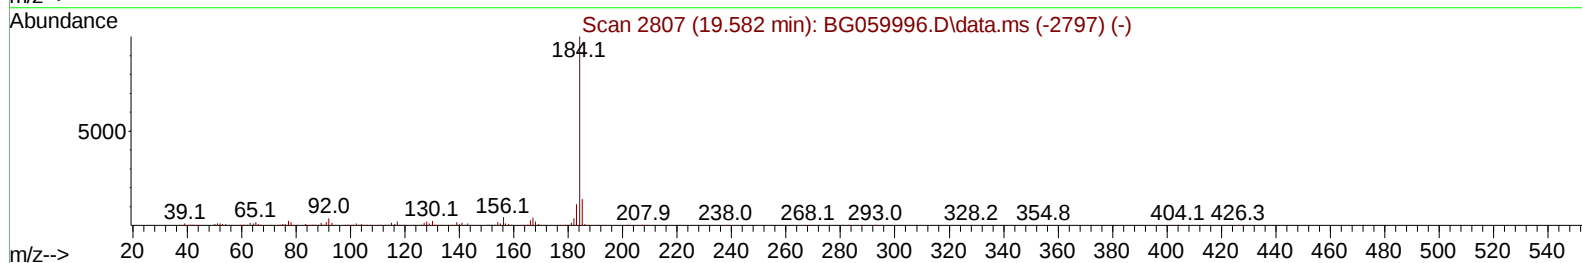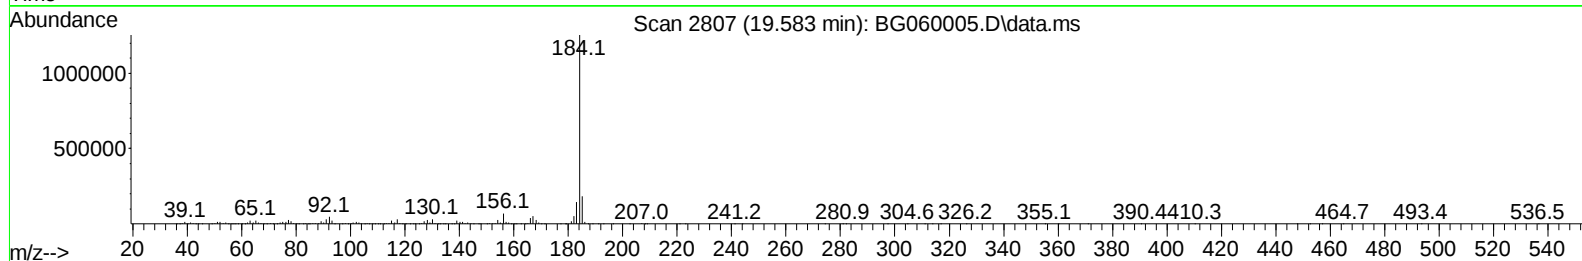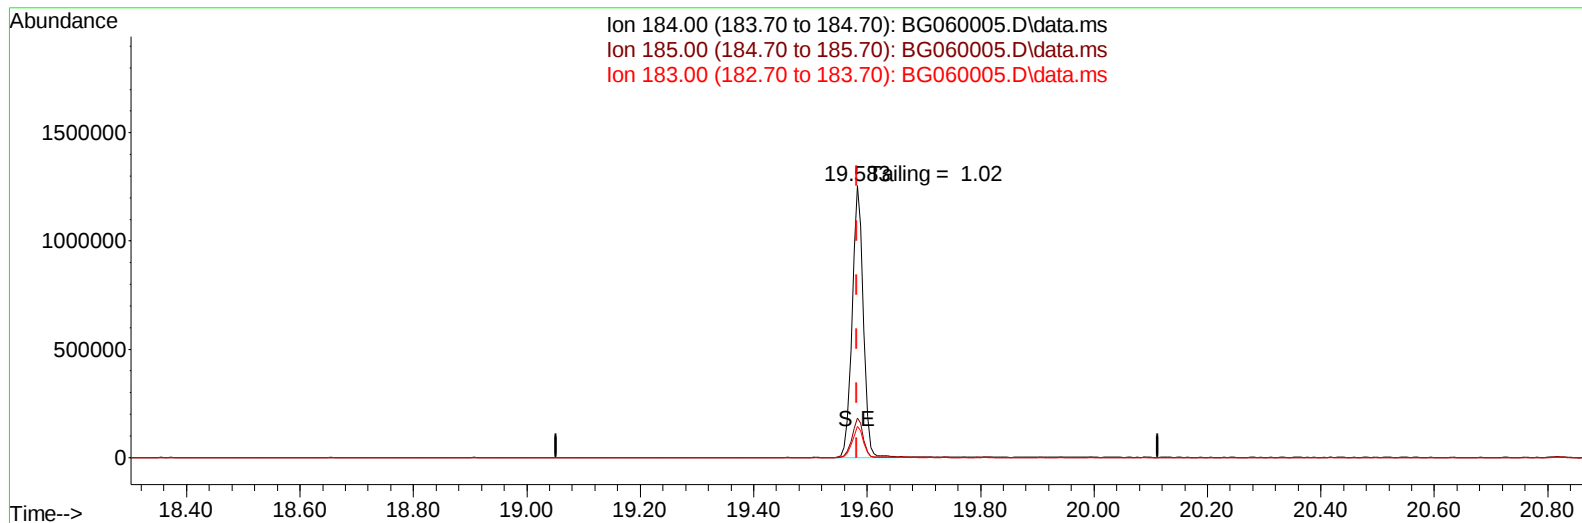

TIC: BG060005.D\data.ms

(77) Benzidine**19.583min (+ 0.000) 3572.42 ng****response 1726121**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.45
183.00	11.20	11.46
0.00	0.00	0.00