
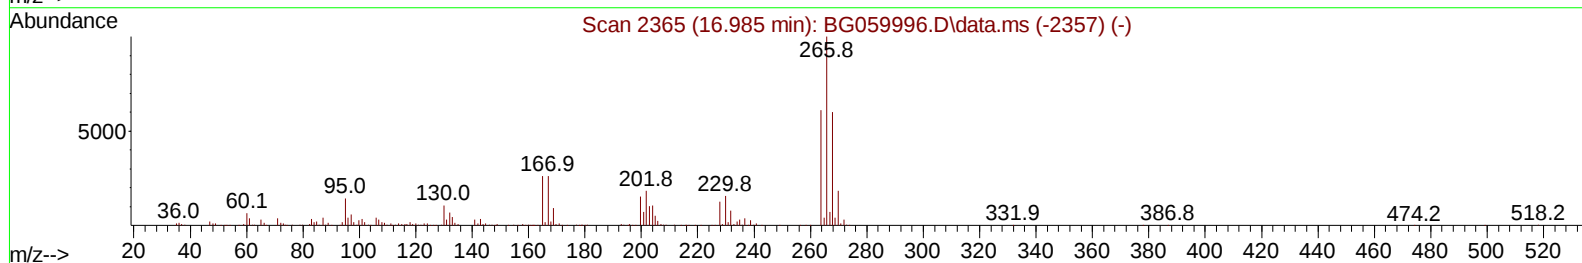
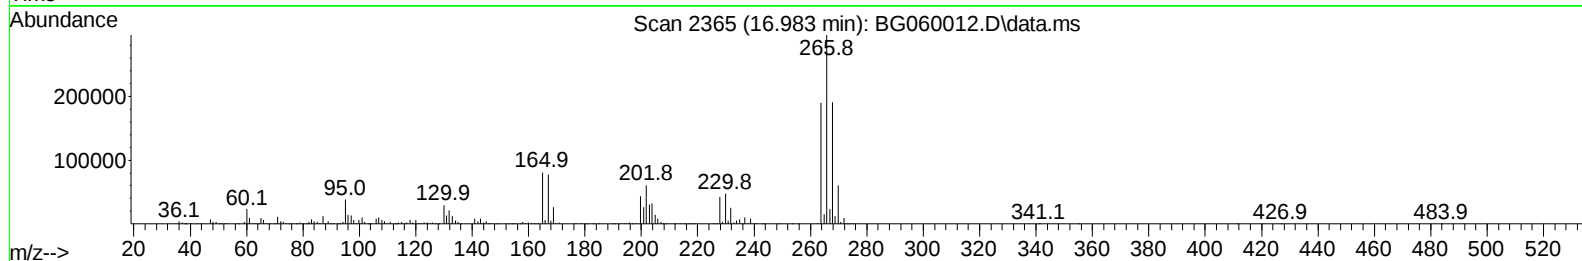


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060012.D
Acq On : 14 Dec 2023 14:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 14:41:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration



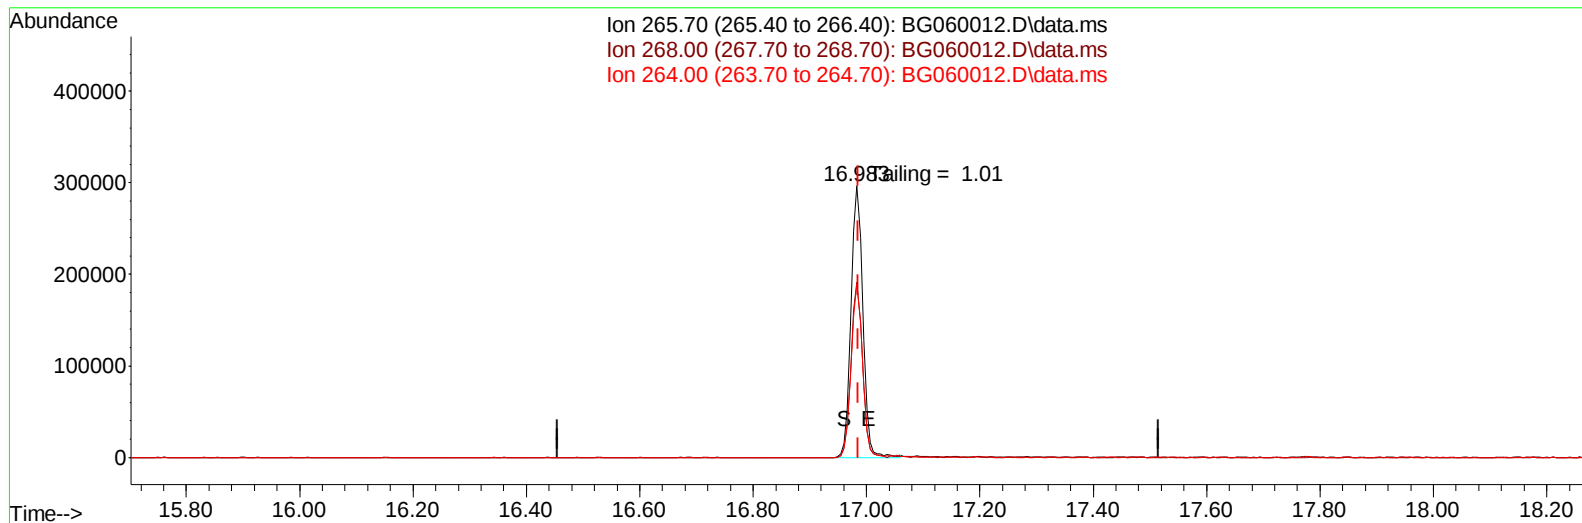


TIC: BG060012.D\data.ms

(70) Pentachlorophenol (C)**16.983min (-0.002) 338317.03 ng****response 430185**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	64.54
264.00	61.00	64.04
0.00	0.00	0.00

Quant Time: Dec 14 14:41:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

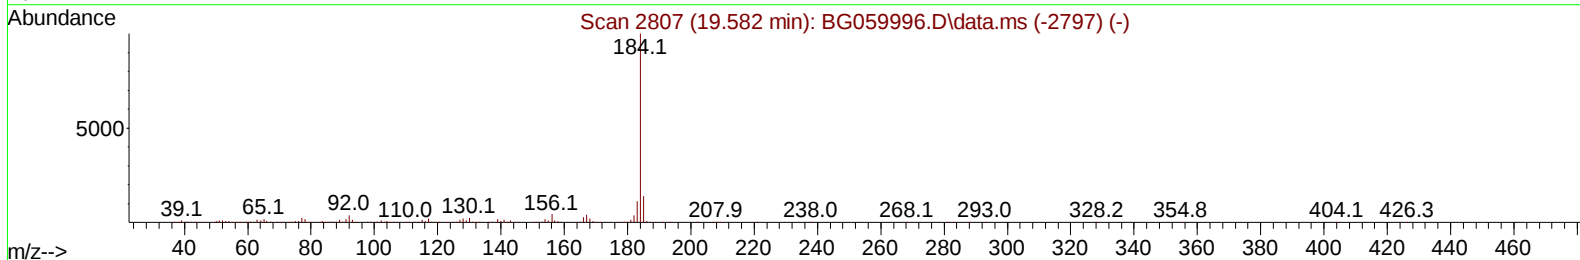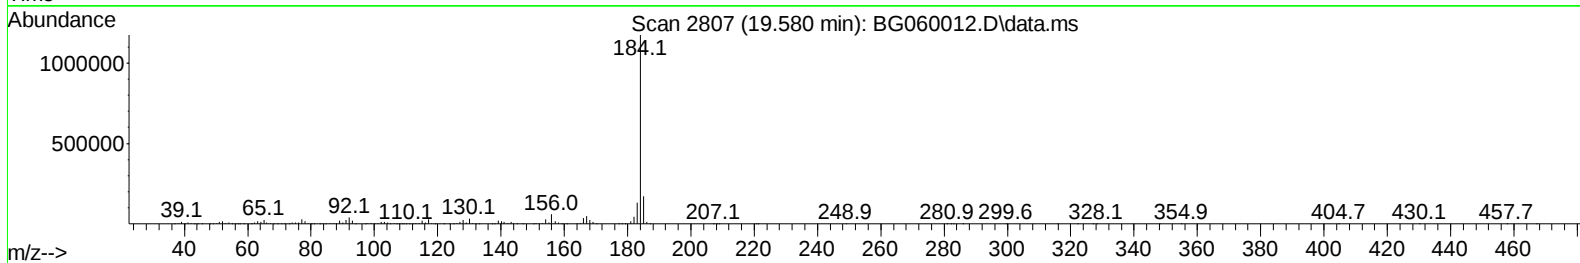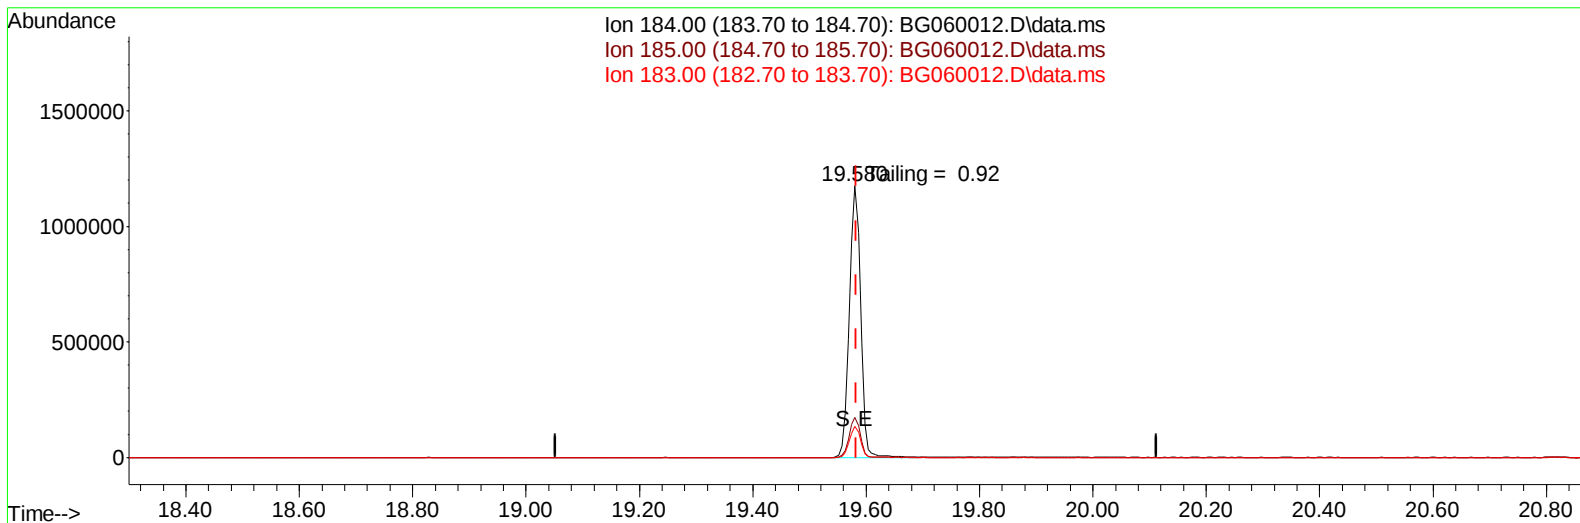

TIC: BG060012.D\data.ms

(77) **Benzidine**

19.580min (-0.002) 81680.83 ng

response **1619914**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.71
183.00	11.20	11.37
0.00	0.00	0.00