

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121423\  
 Data File : BG060014.D  
 Acq On : 14 Dec 2023 16:11  
 Operator : MA/JU  
 Sample : PB157712BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB157712BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060014.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.522       | 406           | 414         | 423          | rVB      | 599512         | 913240        | 8.12%           | 3.146%        |
| 2         | 7.109       | 677           | 684         | 693          | rVB      | 825748         | 1356489       | 12.07%          | 4.672%        |
| 3         | 7.955       | 819           | 828         | 837          | rBV      | 227841         | 378587        | 3.37%           | 1.304%        |
| 4         | 9.112       | 1017          | 1025        | 1033         | rBV      | 460627         | 813621        | 7.24%           | 2.802%        |
| 5         | 10.757      | 1297          | 1305        | 1313         | rBV      | 285596         | 523786        | 4.66%           | 1.804%        |
| 6         | 13.213      | 1716          | 1723        | 1732         | rBV      | 2146594        | 3335957       | 29.68%          | 11.491%       |
| 7         | 14.594      | 1950          | 1958        | 1968         | rVB      | 531782         | 838813        | 7.46%           | 2.889%        |
| 8         | 16.080      | 2202          | 2211        | 2218         | rBV      | 3006942        | 4434628       | 39.45%          | 15.275%       |
| 9         | 17.338      | 2417          | 2425        | 2435         | rBV      | 899345         | 1326037       | 11.80%          | 4.568%        |
| 10        | 19.964      | 2865          | 2872        | 2878         | rBV      | 8658727        | 11240982      | 100.00%         | 38.719%       |
| 11        | 21.609      | 3145          | 3152        | 3157         | rBV2     | 1142520        | 1859075       | 16.54%          | 6.404%        |
| 12        | 24.794      | 3682          | 3694        | 3705         | rBV      | 705378         | 2010774       | 17.89%          | 6.926%        |




Sum of corrected areas: 29031989

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121423\  
Data File : BG060014.D  
Acq On : 14 Dec 2023 16:11  
Operator : MA/JU  
Sample : PB157712BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157712BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

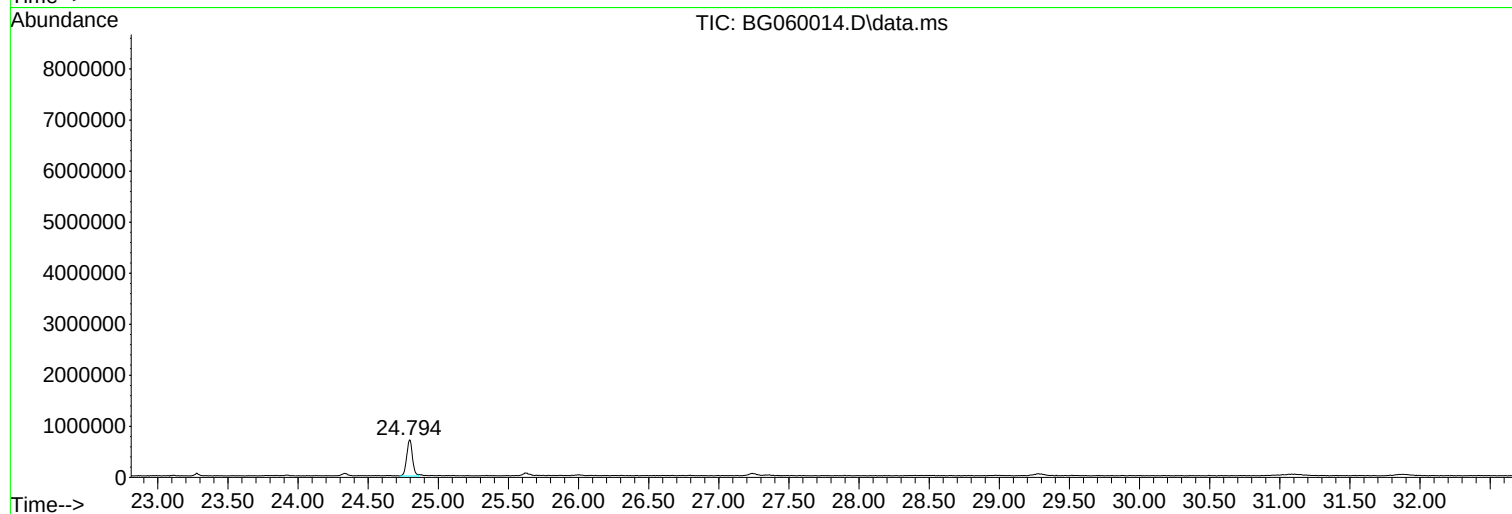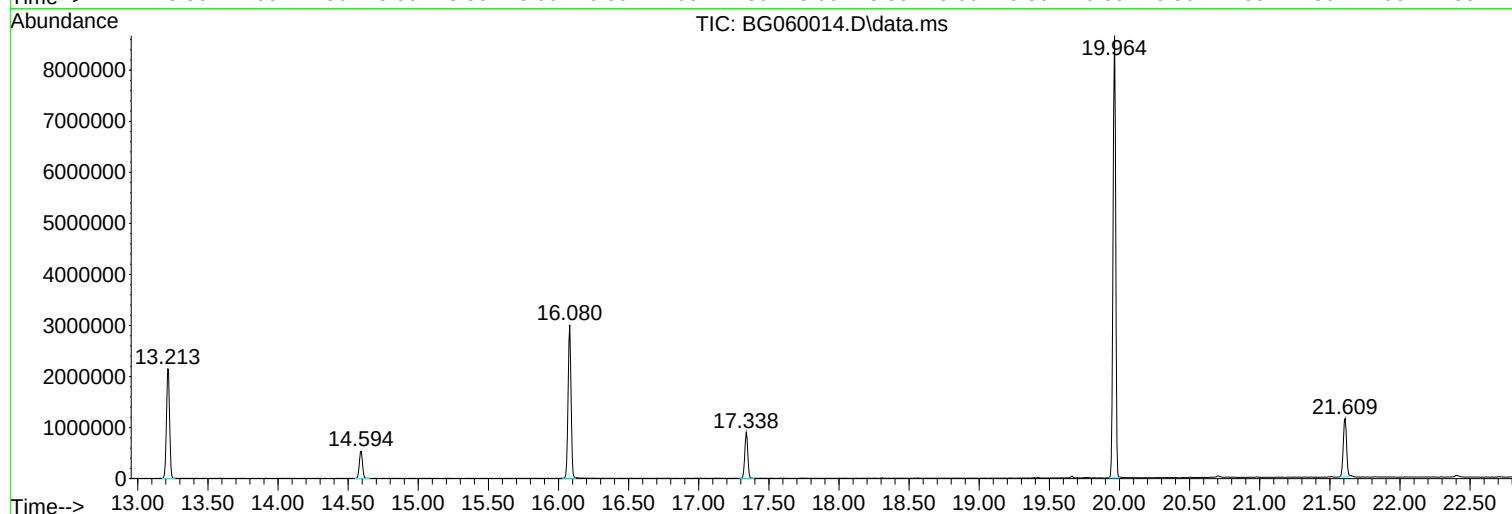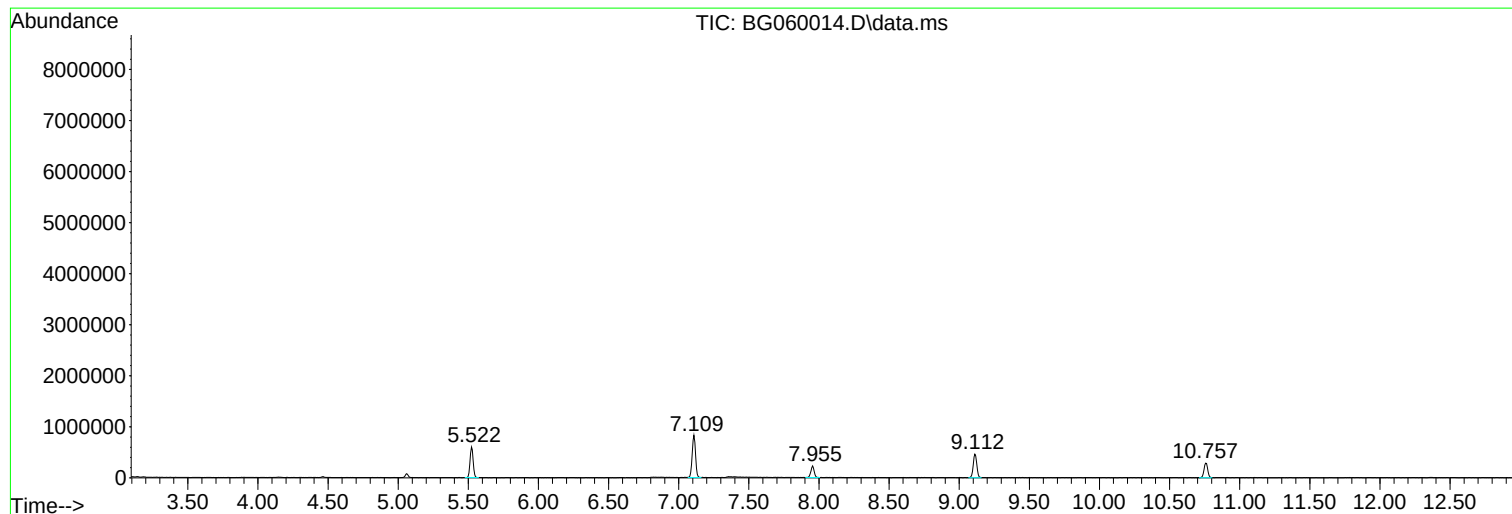

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121423\  
Data File : BG060014.D  
Acq On : 14 Dec 2023 16:11  
Operator : MA/JU  
Sample : PB157712BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157712BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG121423\  
Data File : BG060014.D  
Acq On : 14 Dec 2023 16:11  
Operator : MA/JU  
Sample : PB157712BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB157712BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|