


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060005.D
Acq On : 14 Dec 2023 9:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 14 01:47:12 2023

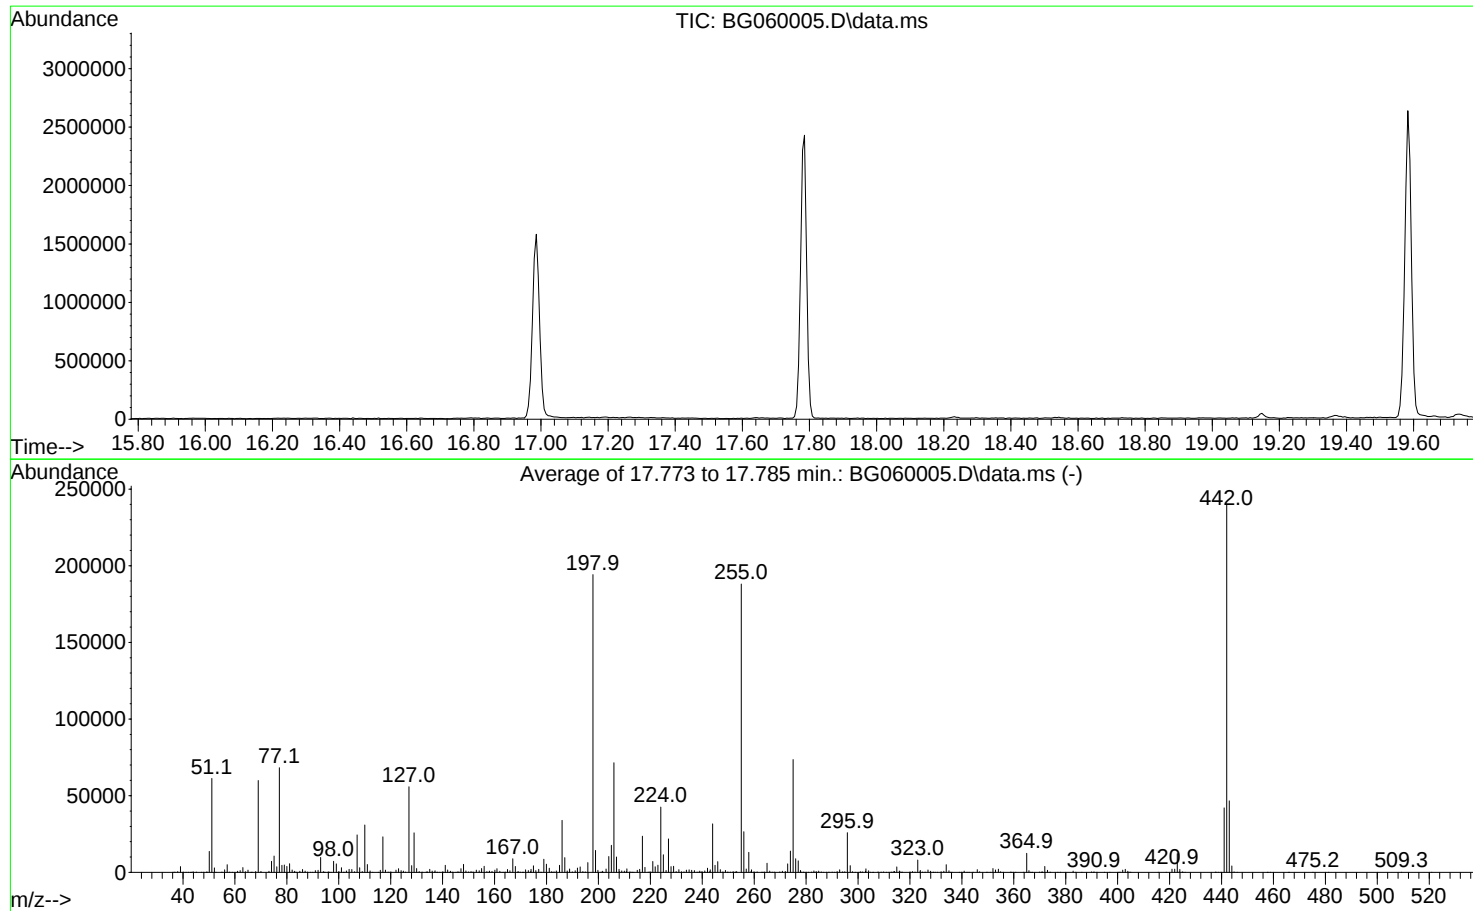




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	61224	PASS
68	69	0.00	2	0.9	538	PASS
69	198	0.00	100	30.8	59872	PASS
70	69	0.00	2	1.0	611	PASS
127	198	10	80	28.7	55819	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	194264	PASS
199	198	5	9	7.4	14343	PASS
275	198	10	60	37.9	73571	PASS
365	198	1	100	6.4	12477	PASS
441	198	0.01	100	21.7	42107	PASS
442	442	50	100	100.0	239933	PASS
443	442	15	24	19.4	46643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060005.D
Acq On : 14 Dec 2023 9:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 14 10:56:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

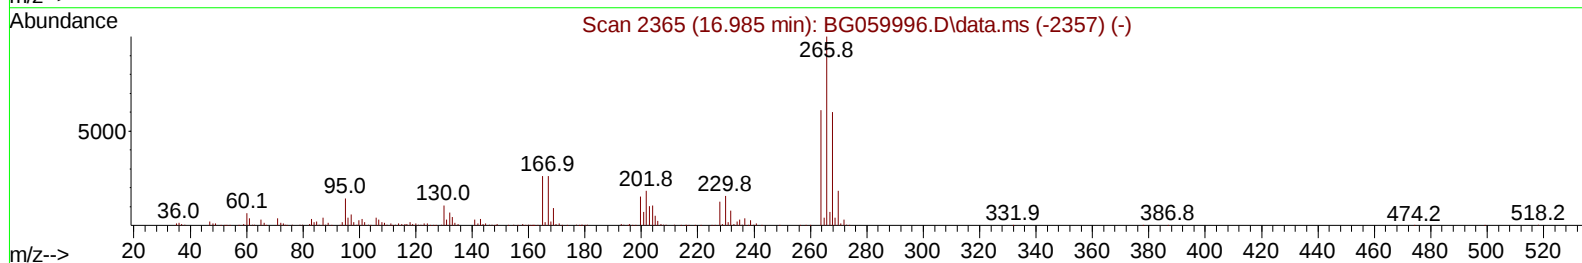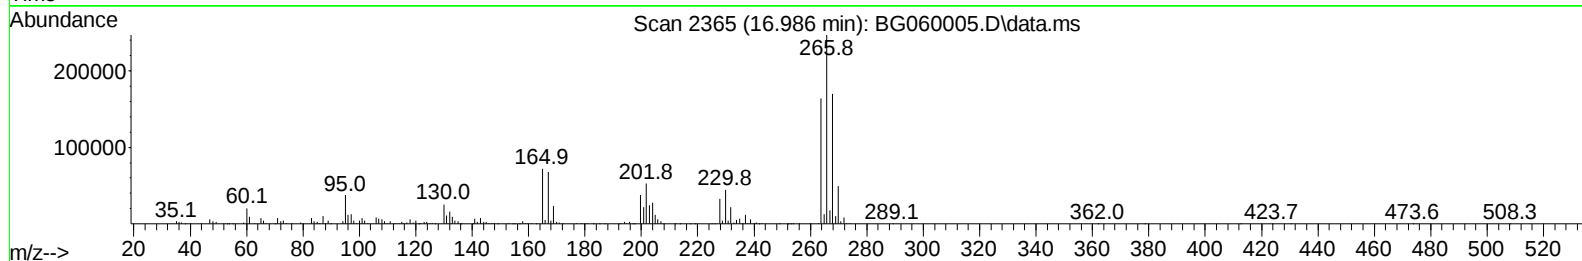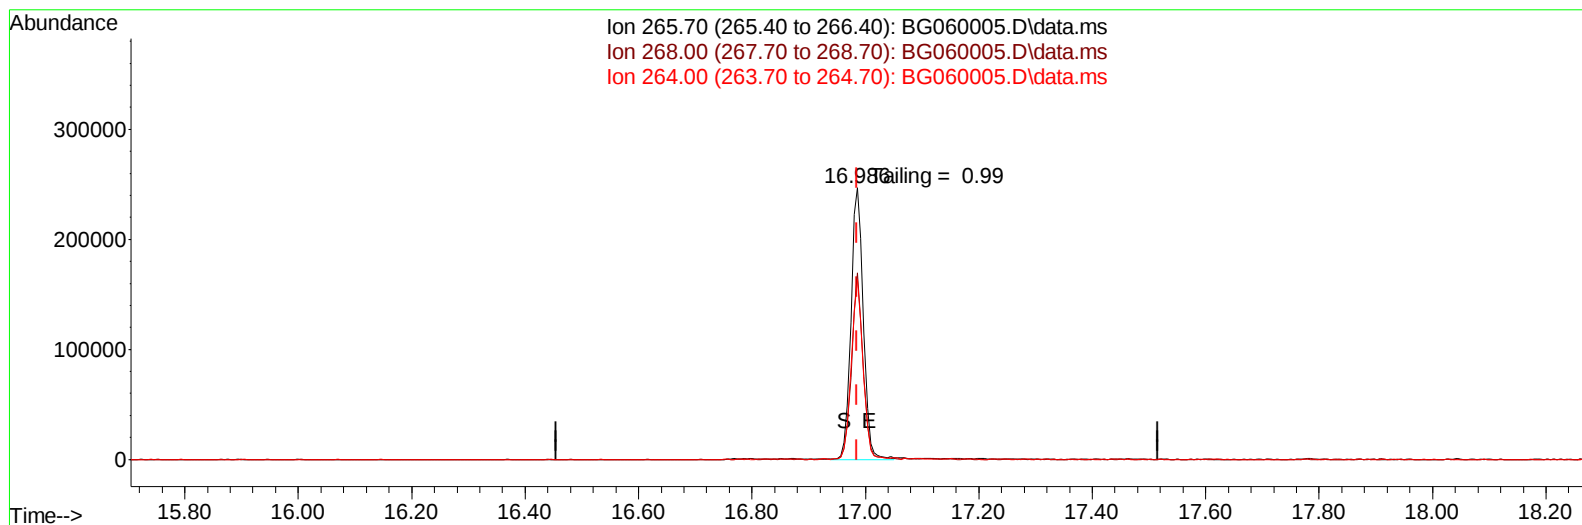

TIC: BG060005.D\data.ms

(70) Pentachlorophenol (C)

16.986min (+ 0.001) 61522.01 ng




response 370761

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	68.70
264.00	61.00	66.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060005.D
Acq On : 14 Dec 2023 9:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 14 10:56:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

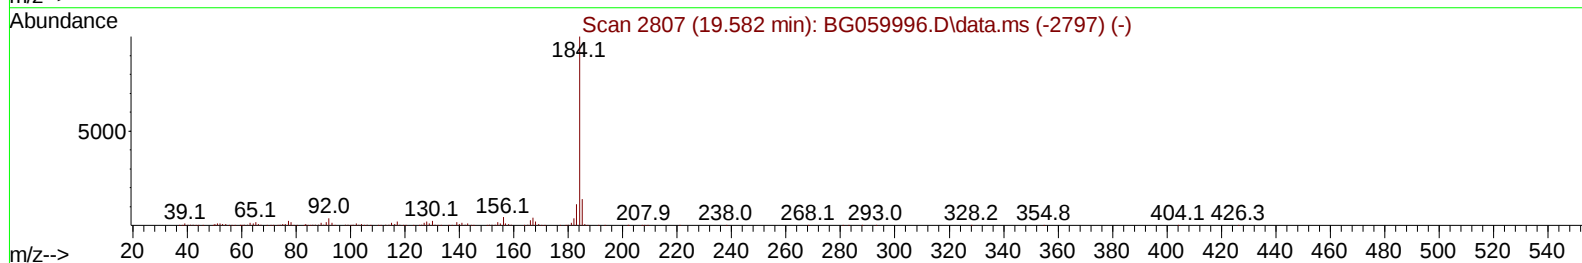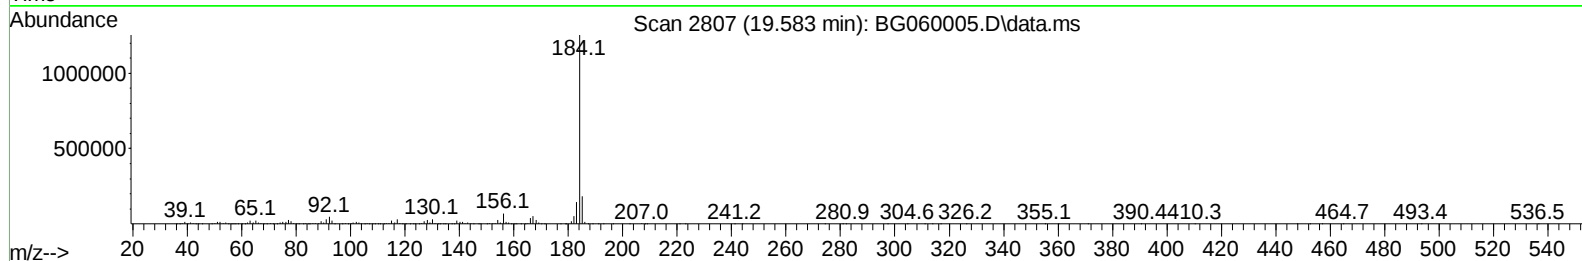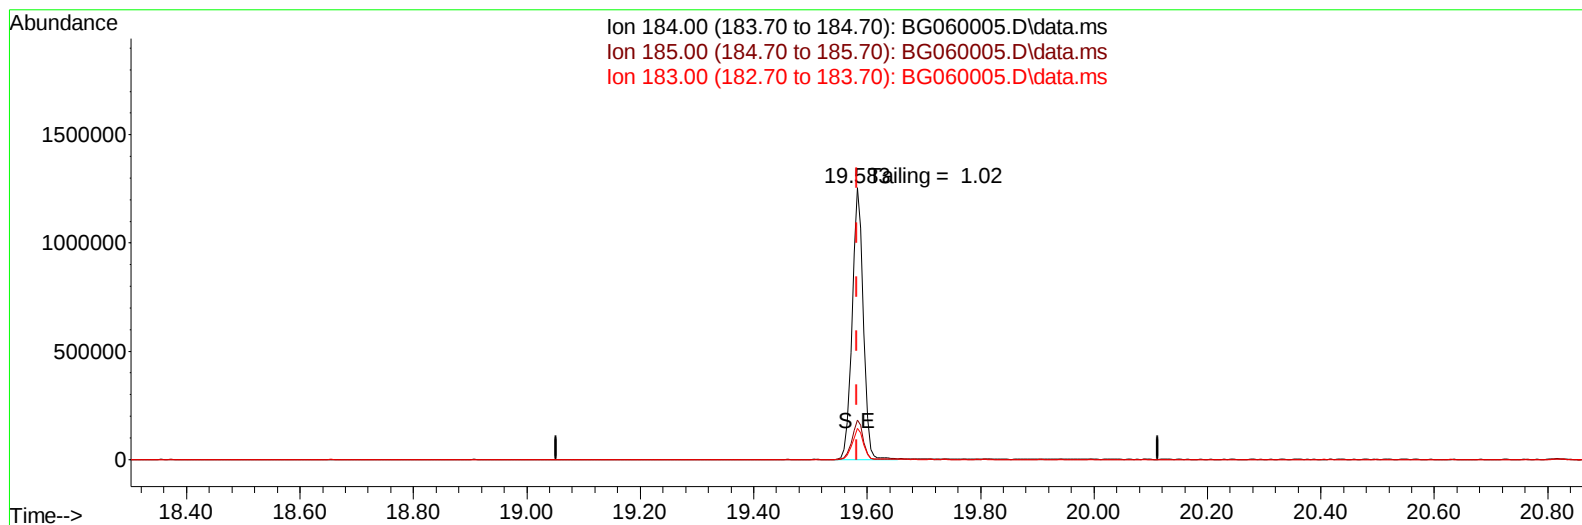

TIC: BG060005.D\data.ms

(77) Benzidine

19.583min (+ 0.000) 3572.42 ng

response 1726121

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.45
183.00	11.20	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2023	BNA_G	<u>BG060005.D</u>
Compound Name	Response	Retention Time
DDT	943587	20.817
DDD	25483	20.376
DDE	3425	19.865
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28908	972495	2.97

Instrument :
BNA_G
ClientSampleId :
DFTPP