
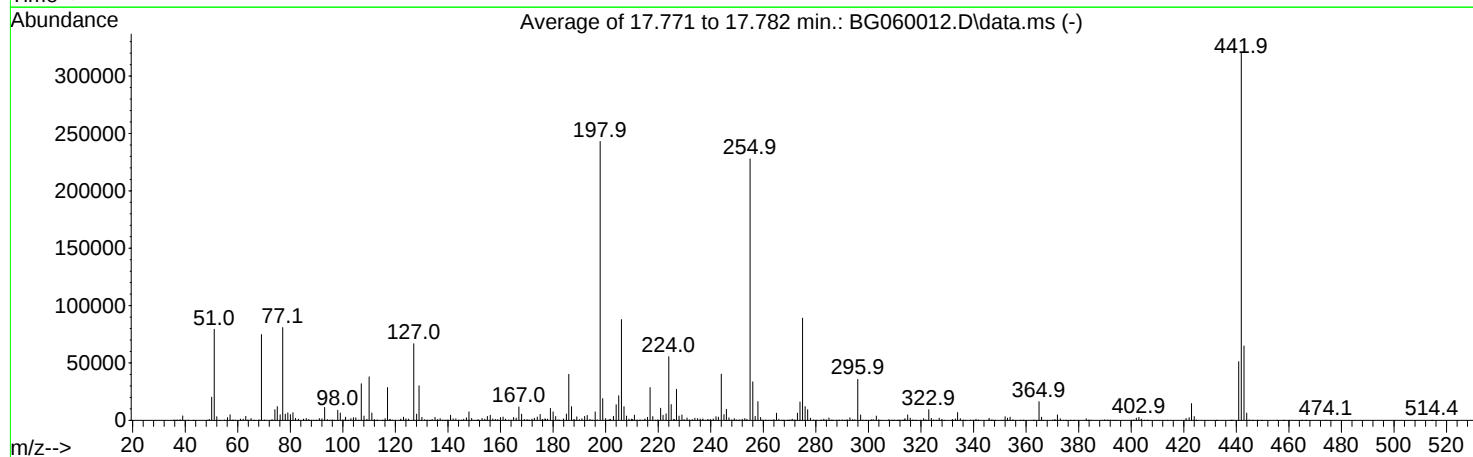


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
 Data File : BG060012.D
 Acq On : 14 Dec 2023 14:10
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 14 01:47:12 2023

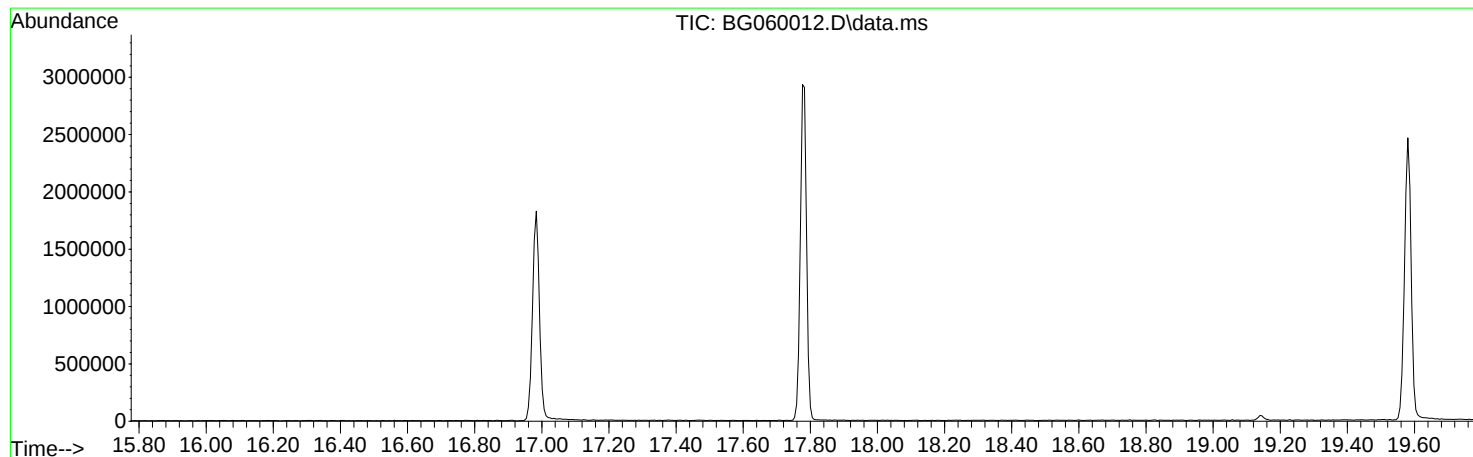




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	79300	PASS
68	69	0.00	2	0.6	480	PASS
69	198	0.00	100	30.8	74768	PASS
70	69	0.00	2	0.4	323	PASS
127	198	10	80	27.5	66824	PASS
197	198	0.00	2	0.2	449	PASS
198	198	100	100	100.0	242987	PASS
199	198	5	9	7.8	18956	PASS
275	198	10	60	36.6	89051	PASS
365	198	1	100	6.7	16268	PASS
441	198	0.01	100	21.1	51171	PASS
442	442	50	100	100.0	320555	PASS
443	442	15	24	20.2	64819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060012.D
Acq On : 14 Dec 2023 14:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 14 14:41:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

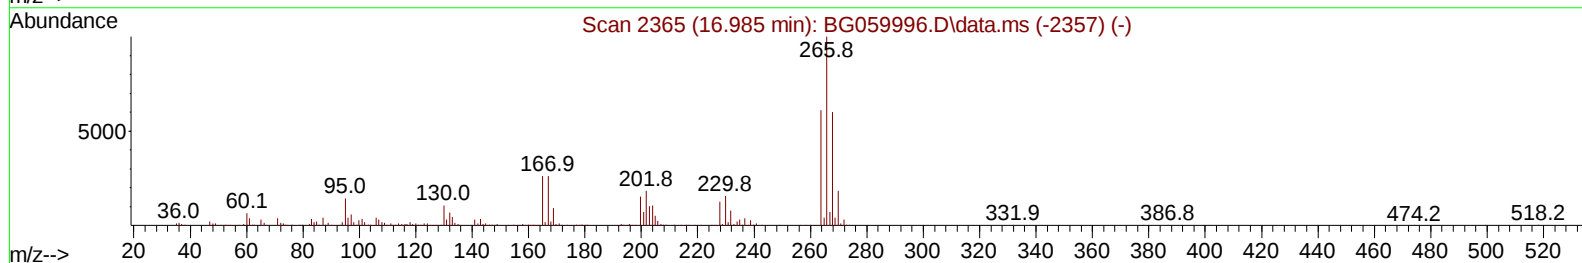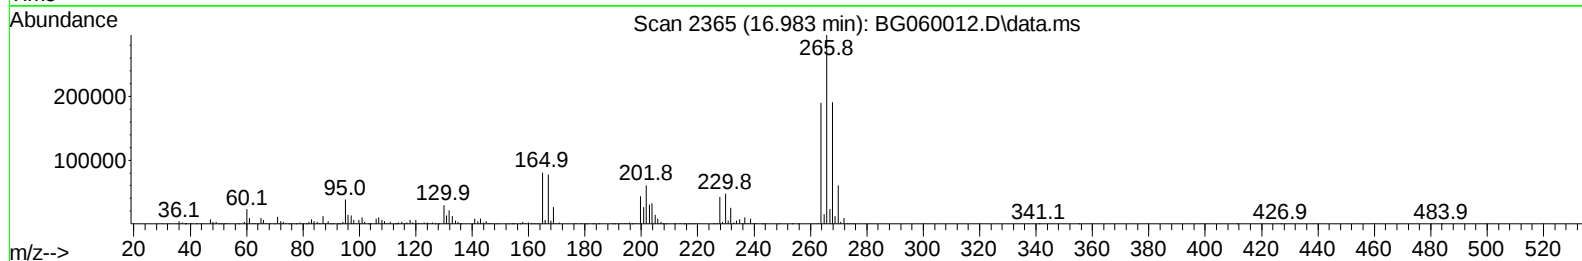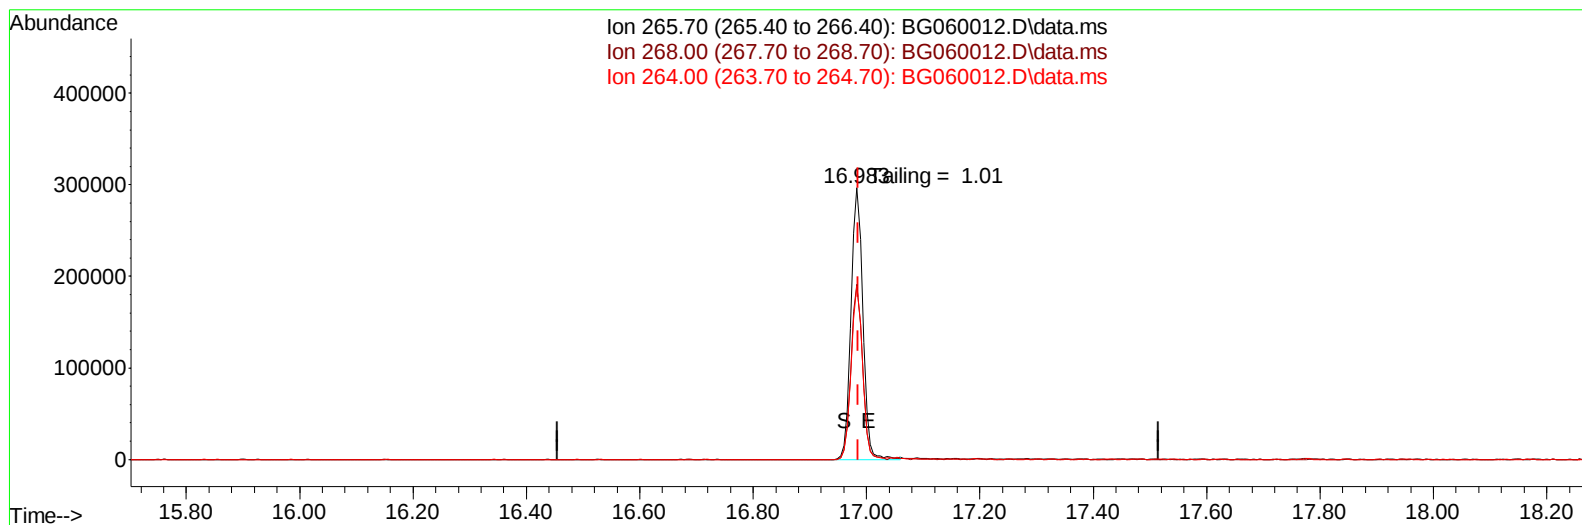

TIC: BG060012.D\data.ms

(70) Pentachlorophenol (C)

16.983min (-0.002) 338317.03 ng




response 430185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	64.54
264.00	61.00	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121423\
Data File : BG060012.D
Acq On : 14 Dec 2023 14:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 14 14:41:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 01:47:12 2023
Response via : Initial Calibration

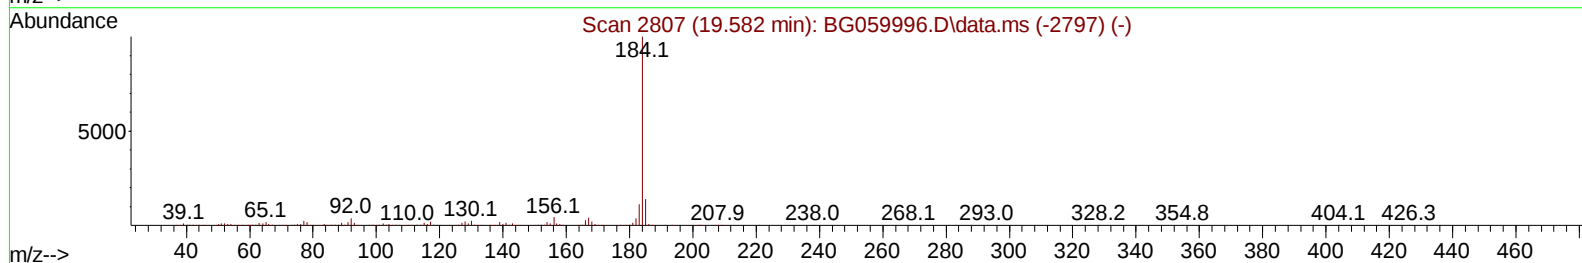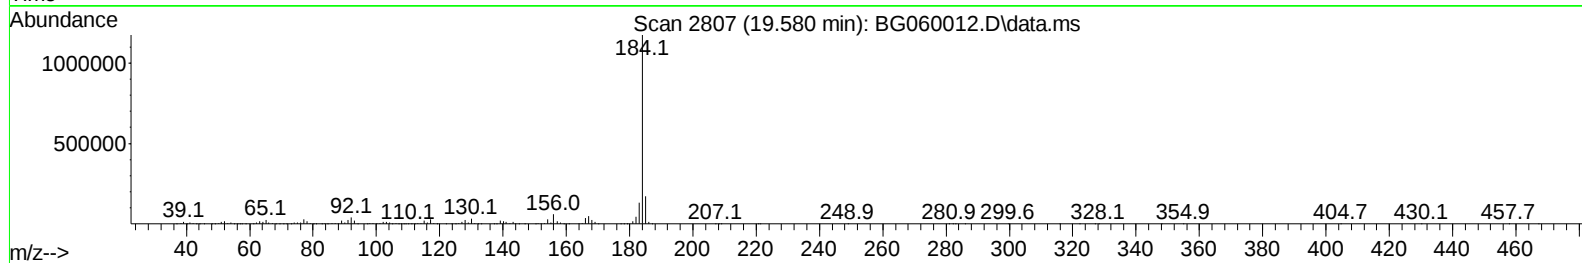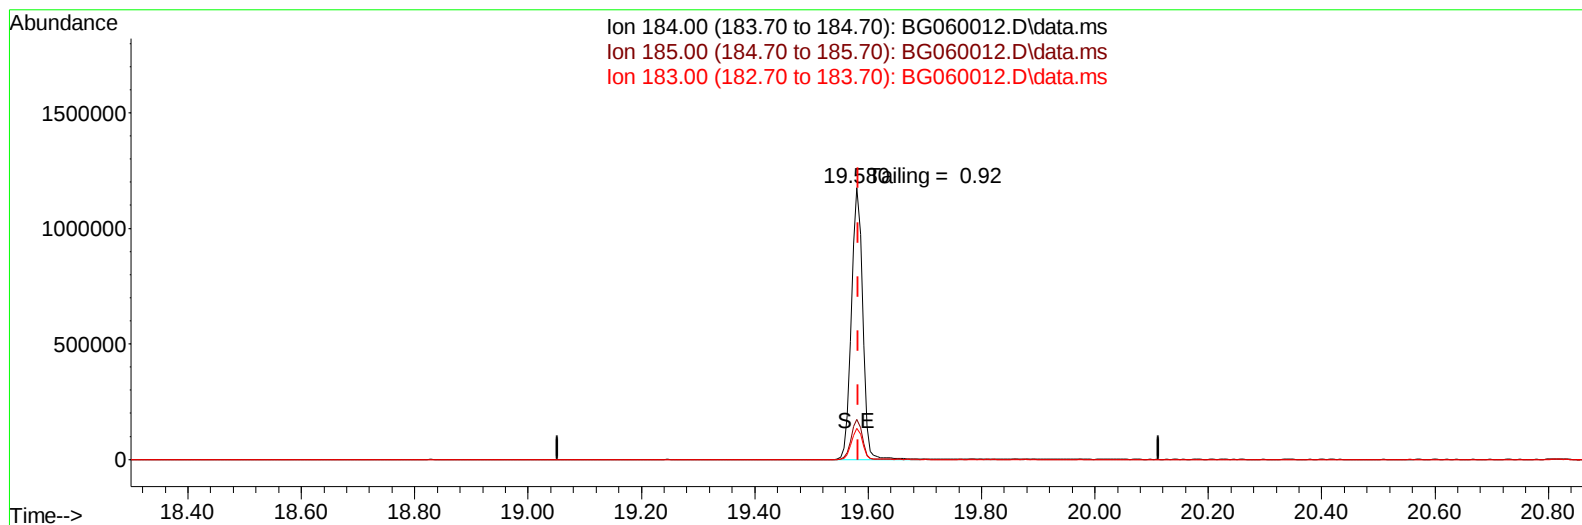

TIC: BG060012.D\data.ms

(77) Benzidine**19.580min (-0.002) 81680.83 ng****response 1619914**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.71
183.00	11.20	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2023	BNA_G	<u>BG060012.D</u>
Compound Name	Response	Retention Time
DDT	959420	20.814
DDD	29919	20.374
DDE	3572	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33491	992911	3.37

Instrument :
BNA_G
ClientSampleId :
DFTPP