

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020151.D
 Acq On : 14 Dec 2015 11:32
 Operator : UM/SJ
 Sample : PB87242BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Quant Time: Dec 15 03:48:48 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 03:46:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	21951	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	98618	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	74769	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	193535	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	207187	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	193777	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	2821	7.10	ng/uL	0.00
5) Phenol-d5	7.24	99	65692	33.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	41904	36.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	51435	36.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	57563	34.77	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	27930	36.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	32604	38.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	60355	34.83	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	84969	43.65	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	229438	37.94	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	255317	36.28	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	37016	34.13	ng/ul	0.00
58) Fluorene-d10	15.72	176	202611	36.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	26914	23.46	ng/ul	0.00
71) Anthracene-d10	17.57	188	331746	37.20	ng/ul	0.00
79) Pyrene-d10	19.85	212	372104	38.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	382011	39.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.80	70	1585	1.16	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020151.D
Acq On : 14 Dec 2015 11:32
Operator : UM/SJ
Sample : PB87242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Time: Dec 15 03:48:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 03:46:07 2015
Response via : Initial Calibration

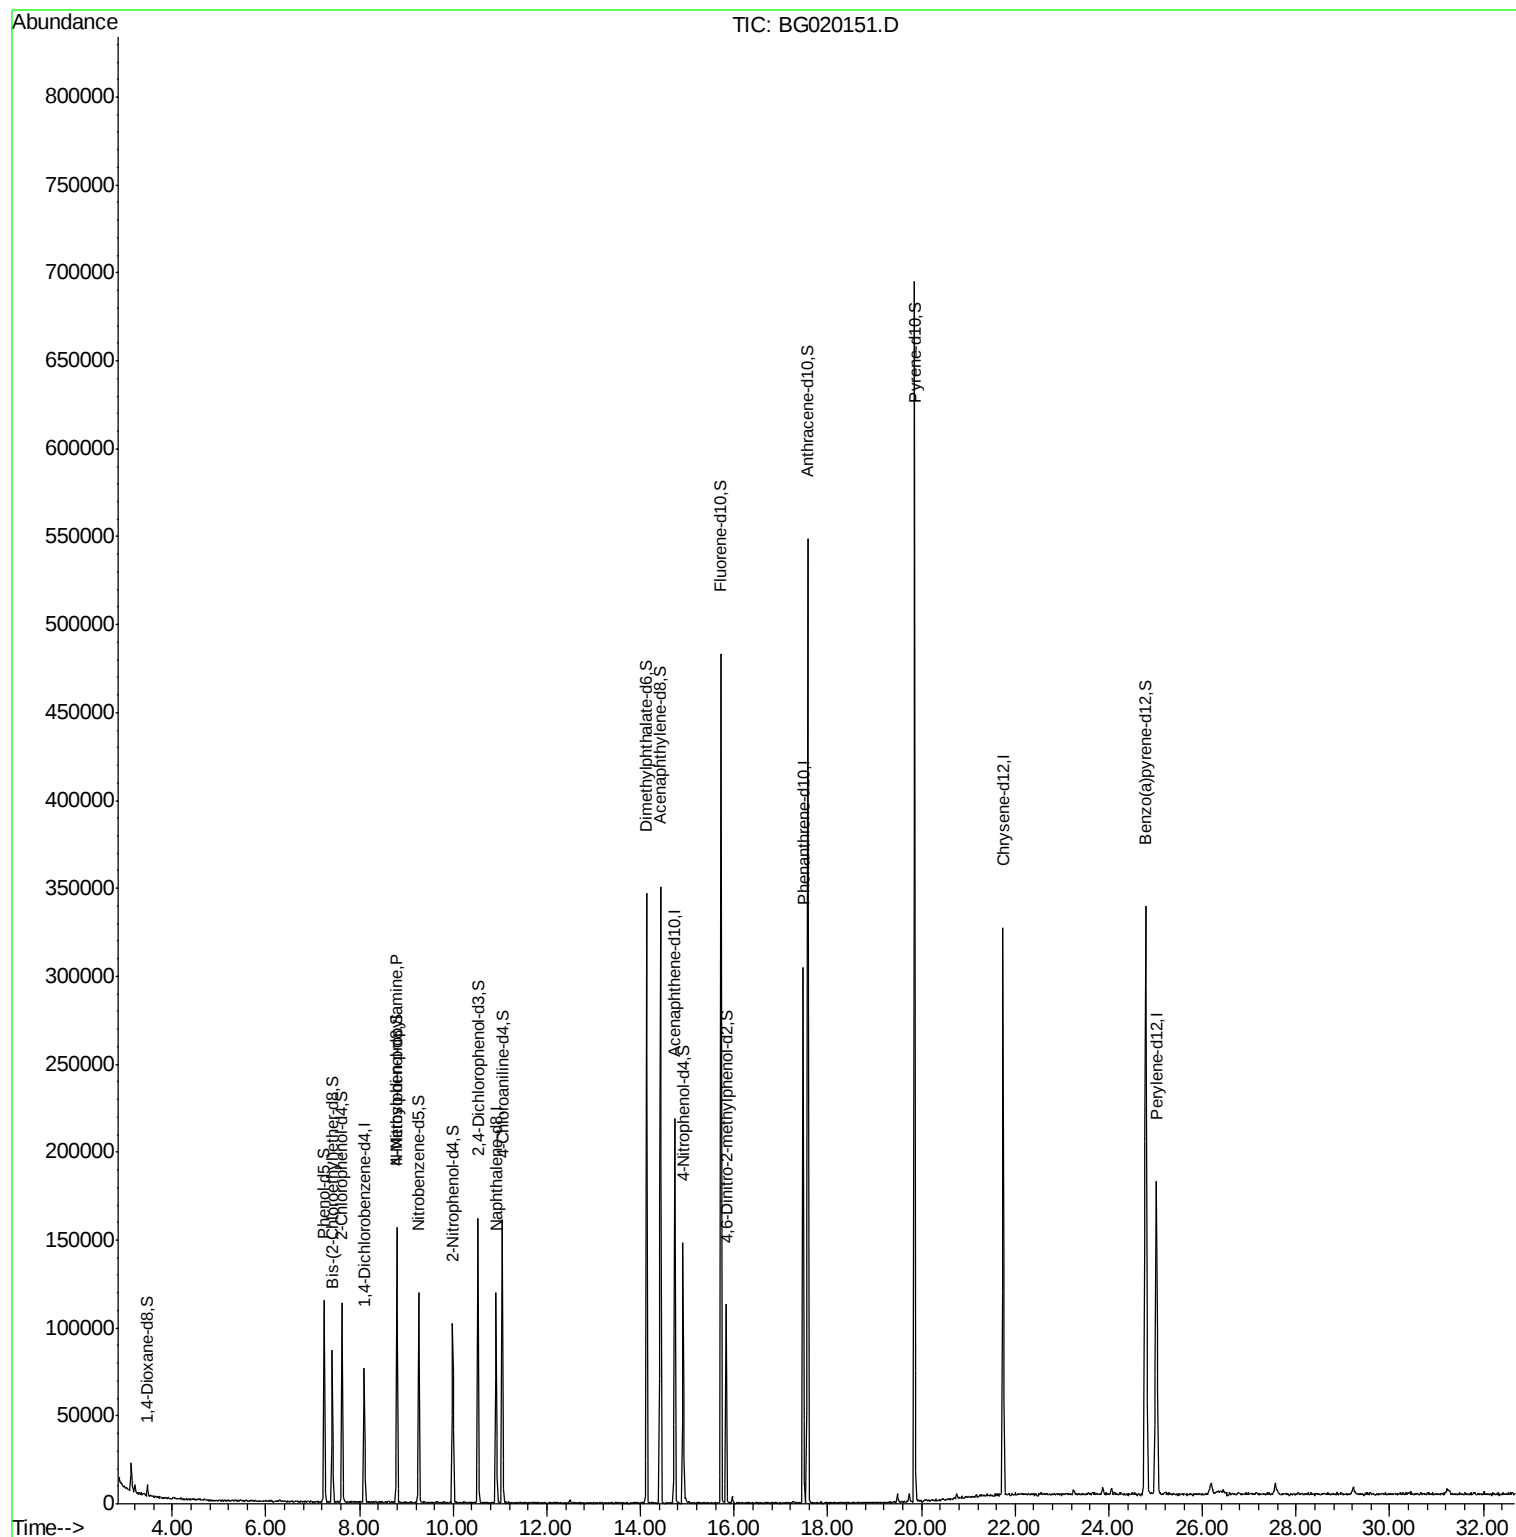

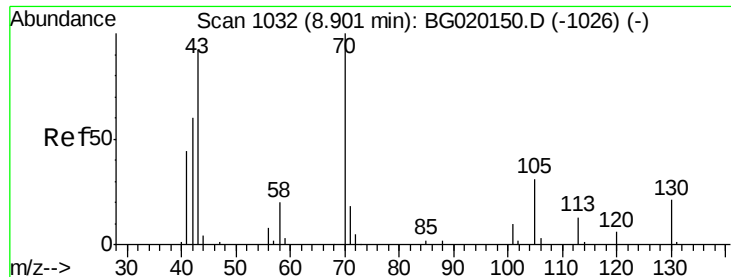

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.16 ng/ul
 RT: 8.80 min Scan# 1015
 Delta R.T. -0.10 min
 Lab File: BG020151.D
 Acq: 14 Dec 2015 11:32

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Tgt Ion: 70 Resp: 1585
 Ion Ratio Lower Upper
 70 100
 42 296.7 44.3 66.5#
 101 0.0 7.6 11.4#
 130 0.0 17.0 25.4#

