

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020152.D
 Acq On : 14 Dec 2015 12:12
 Operator : UM/SJ
 Sample : G4767-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N27

Quant Time: Dec 15 03:48:57 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 03:46:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	20328	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	89839	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	69052	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	184827	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	200903	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	190397	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	1985	5.39	ng/uL	0.00
5) Phenol-d5	7.24	99	49424	27.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	29650	27.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	36650	28.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	42645	27.82	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	20098	28.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	23406	30.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	43988	27.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	57641	32.51	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	170084	30.45	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	182628	28.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	27706	27.66	ng/ul	0.00
58) Fluorene-d10	15.72	176	141819	27.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	27210	24.83	ng/ul	0.00
71) Anthracene-d10	17.57	188	249297	29.27	ng/ul	0.00
79) Pyrene-d10	19.85	212	274938	29.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	282670	29.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.17	163	65891	11.55	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020152.D
Acq On : 14 Dec 2015 12:12
Operator : UM/SJ
Sample : G4767-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N27

Quant Time: Dec 15 03:48:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 03:46:07 2015
Response via : Initial Calibration

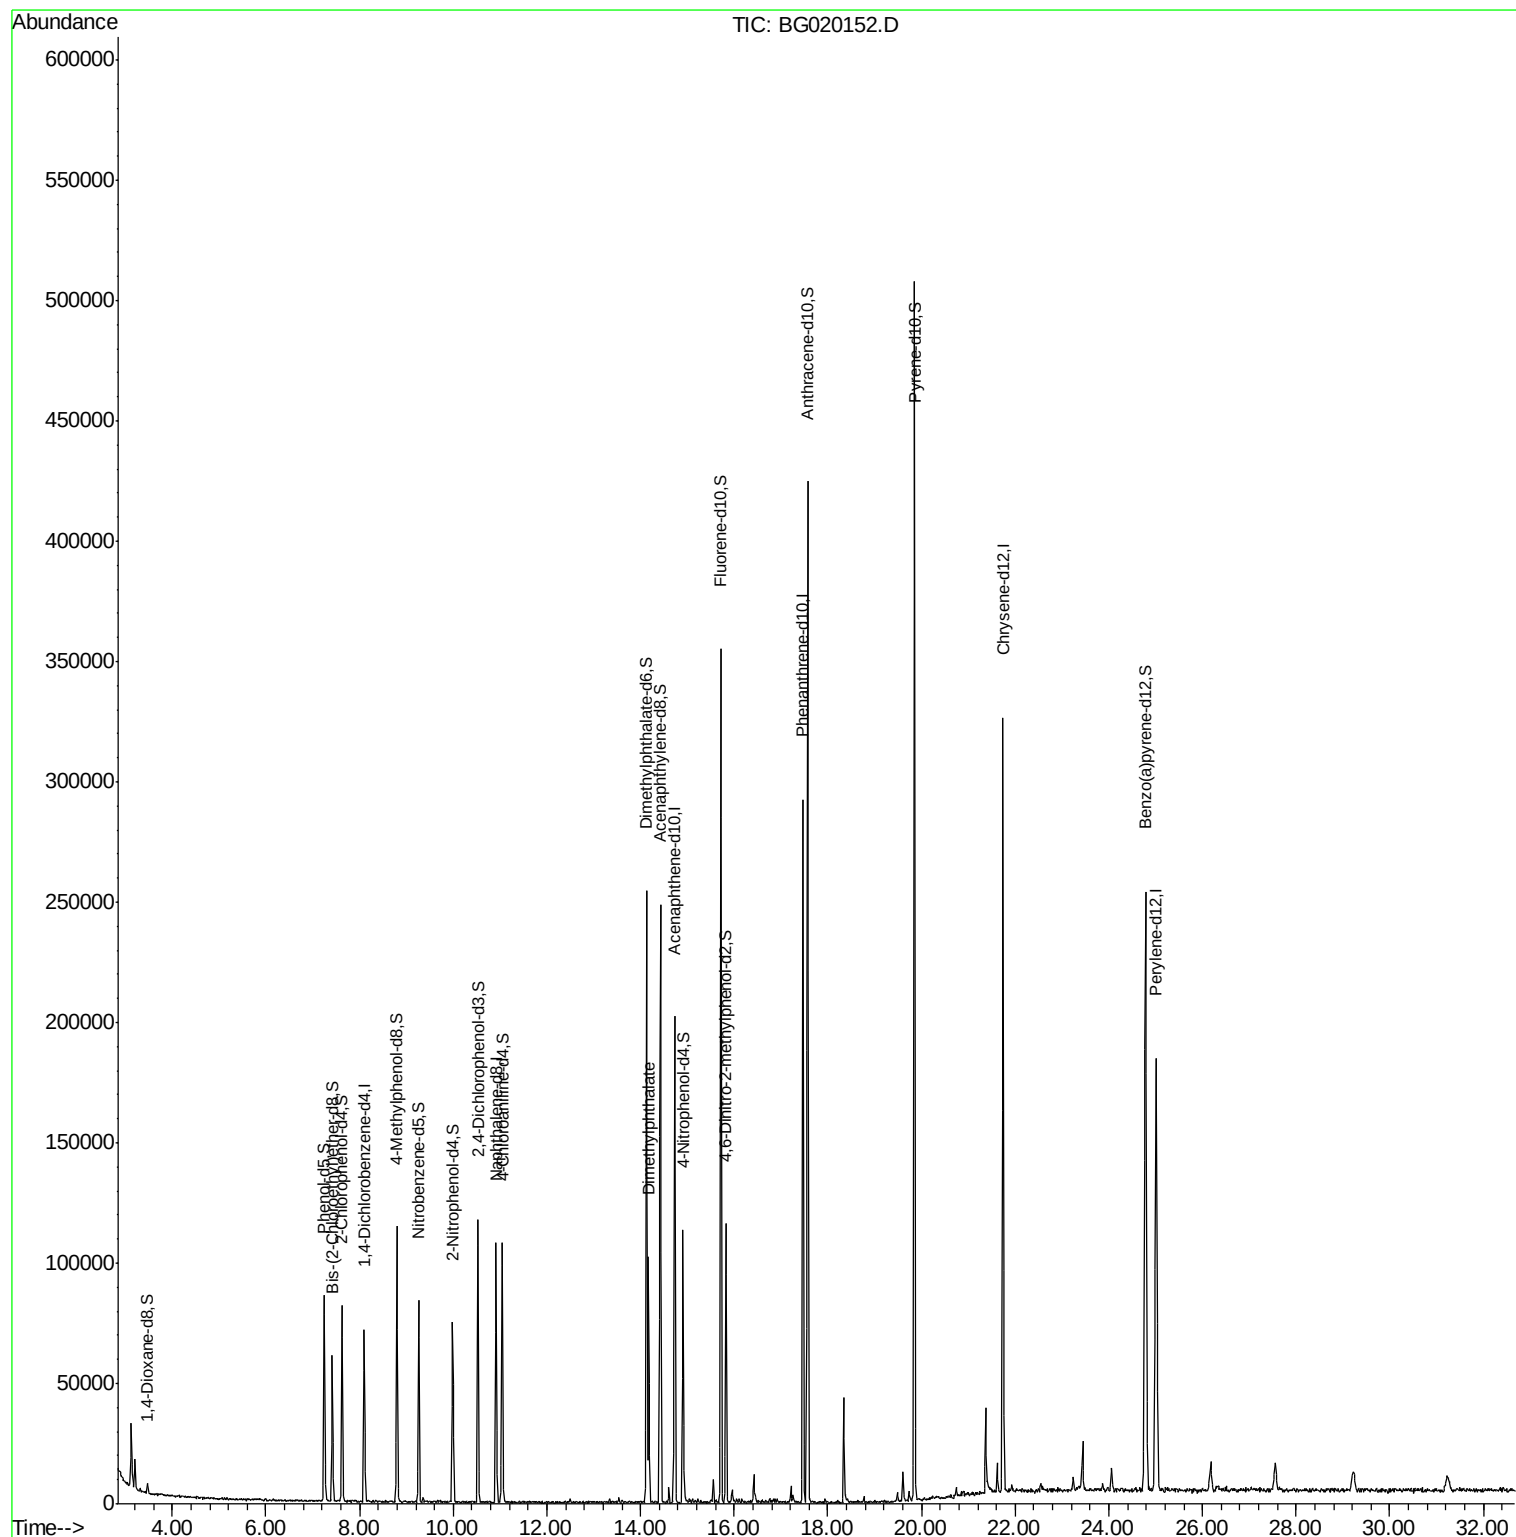

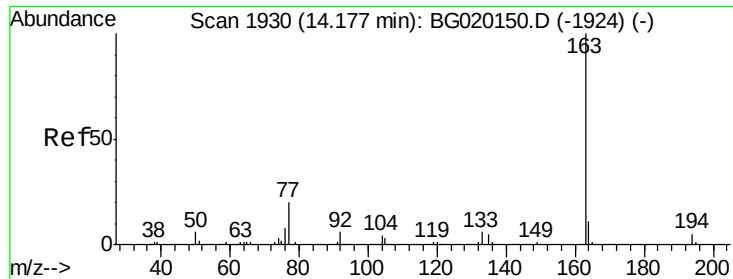

#45

Dimethylphthalate

Concen: 11.55 ng/ul

RT: 14.17 min Scan# 1929

Delta R.T. -0.01 min

Lab File: BG020152.D


Acq: 14 Dec 2015 12:12

Instrument :

BNA_G

ClientSampleId :

D9N27

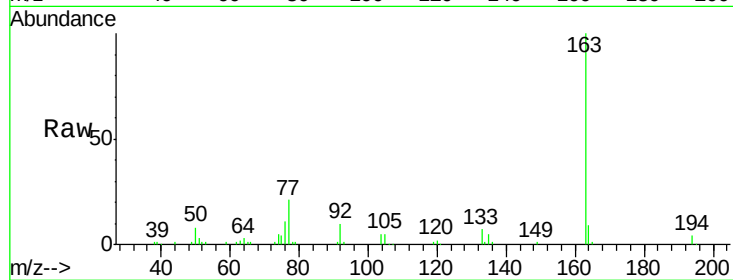

Tgt Ion:163 Resp: 65891

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.5 7.7 11.5

