

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020175.D
 Acq On : 15 Dec 2015 5:30
 Operator : UM/SJ
 Sample : G4787-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9BN0

Quant Time: Dec 15 06:09:10 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 05:59:19 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	22613	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	97509	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	73710	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	196549	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	210753	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	201053	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	2369	5.78	ng/uL	0.00
5) Phenol-d5	7.25	99	57790	28.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	38016	31.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	45201	31.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	51898	30.43	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	24918	32.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	31405	37.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	53411	31.18	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	69491	36.11	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	198689	33.32	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	224774	32.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	31827	29.76	ng/ul	0.00
58) Fluorene-d10	15.72	176	169885	31.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	26231	22.51	ng/ul	0.00
71) Anthracene-d10	17.57	188	284088	31.37	ng/ul	0.00
79) Pyrene-d10	19.85	212	295028	30.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	276905	27.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	84256	13.84	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020175.D
Acq On : 15 Dec 2015 5:30
Operator : UM/SJ
Sample : G4787-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9BN0

Quant Time: Dec 15 06:09:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 05:59:19 2015
Response via : Initial Calibration

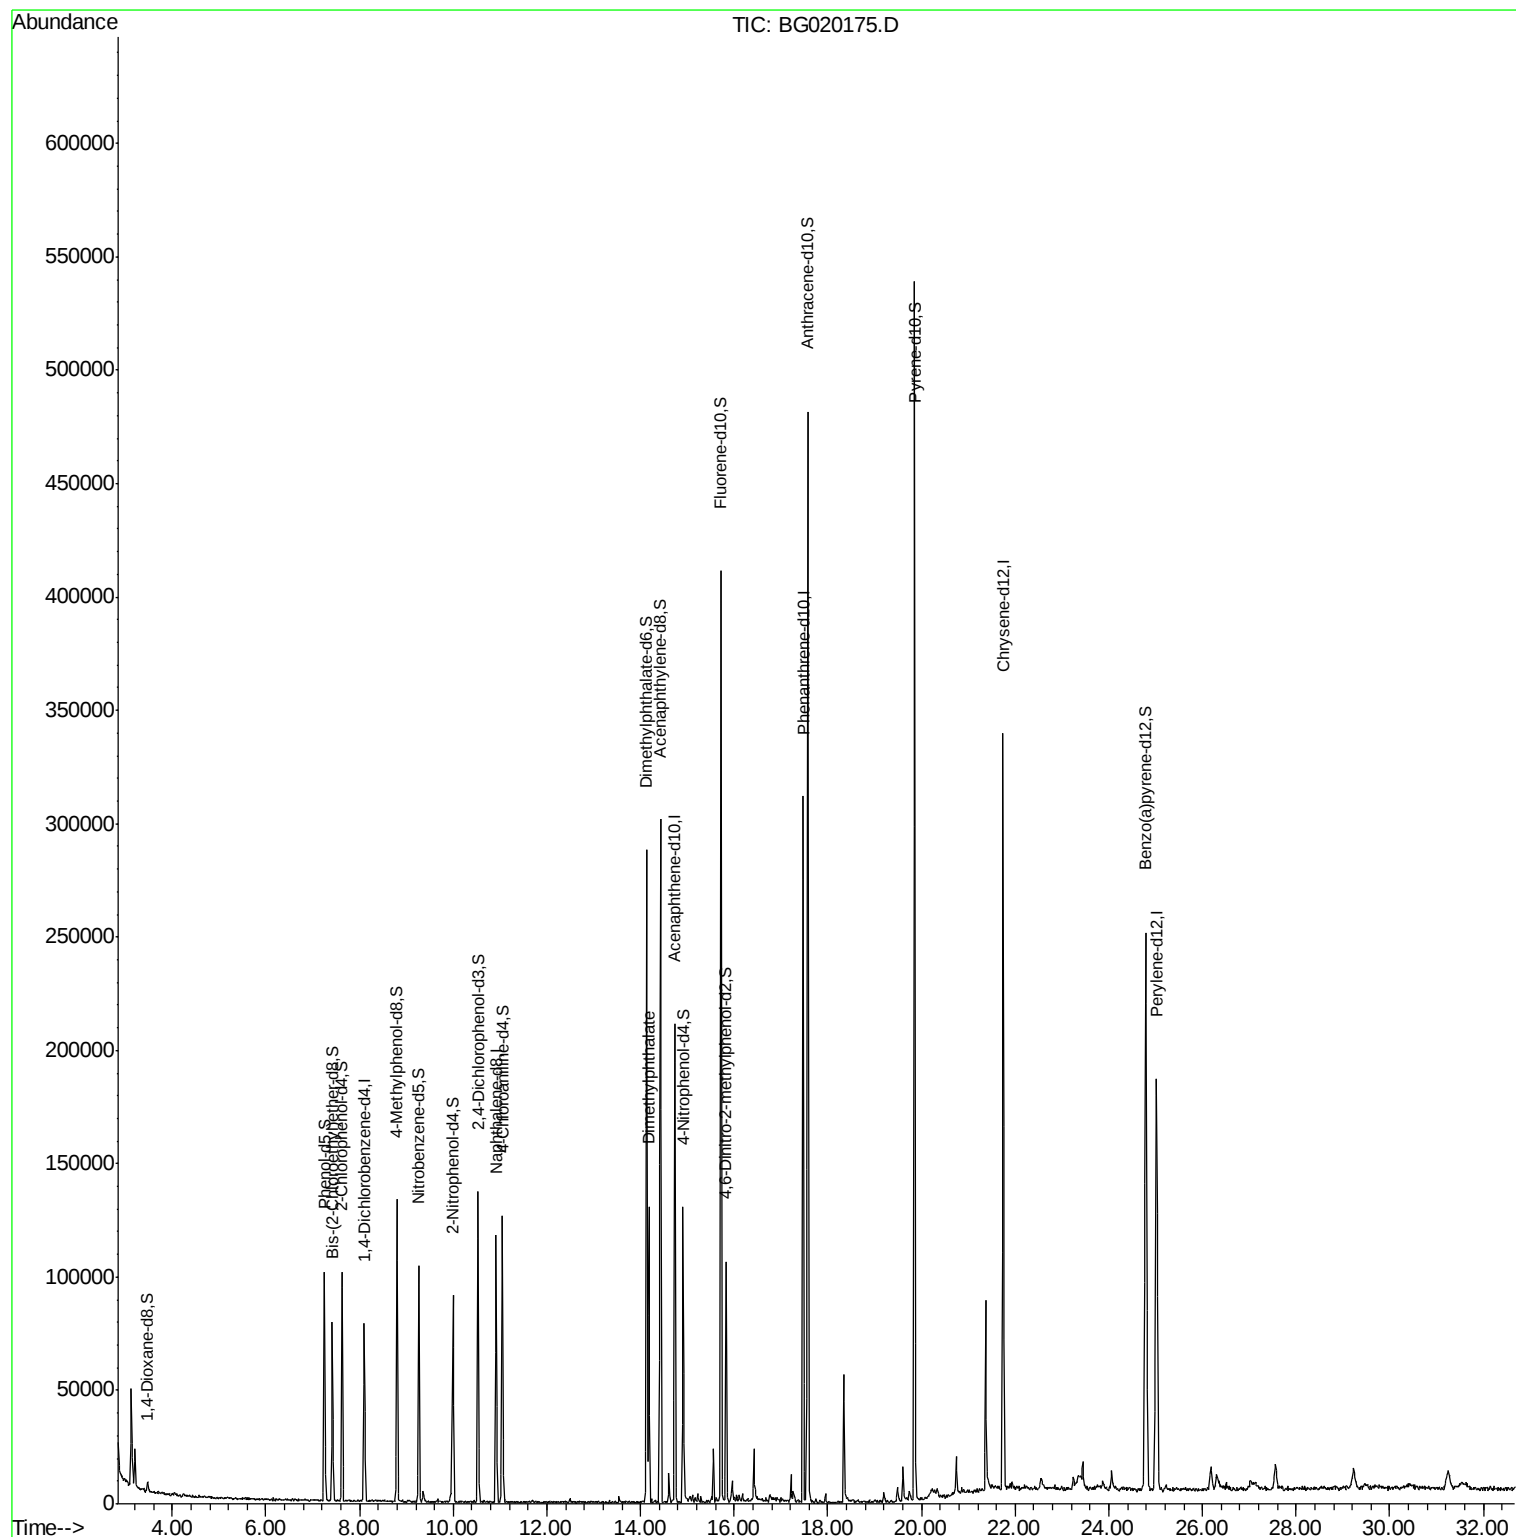

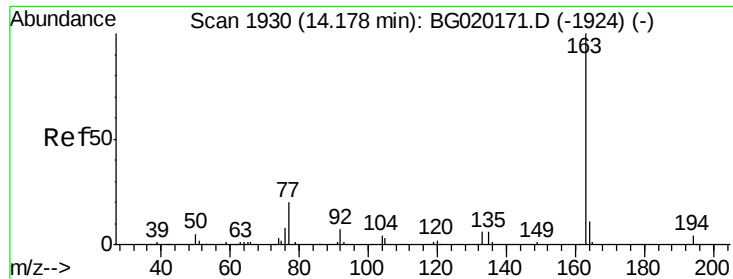

#45

Dimethylphthalate

Concen: 13.84 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.00 min

Lab File: BG020175.D


Acq: 15 Dec 2015 5:30

Instrument :

BNA_G

ClientSampleId :

G9BN0

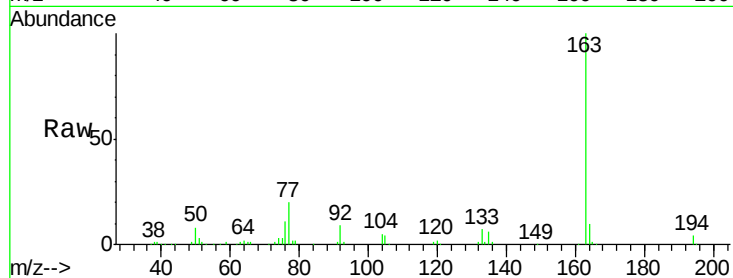

Tgt Ion:	163	Resp:	84256
Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.5	5.3
164	9.8	7.7	11.5

