

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020162.D
 Acq On : 14 Dec 2015 20:58
 Operator : UM/SJ
 Sample : G4767-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N36

Quant Time: Dec 15 04:28:34 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 04:25:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	20021	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	85459	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	65903	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	182676	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	201882	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	189263	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	1935	5.34	ng/uL	0.00
5) Phenol-d5	7.24	99	46116	26.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	29994	28.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	35048	27.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	40309	26.70	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	19430	29.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	22284	30.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	42966	28.62	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	55941	33.17	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	163906	30.75	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	177148	28.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	28239	29.54	ng/ul	0.00
58) Fluorene-d10	15.72	176	135612	28.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	25346	23.40	ng/ul	0.00
71) Anthracene-d10	17.57	188	218920	26.01	ng/ul	0.00
79) Pyrene-d10	19.85	212	243350	25.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	222794	23.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.17	163	51280	9.42	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020162.D
Acq On : 14 Dec 2015 20:58
Operator : UM/SJ
Sample : G4767-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N36

Quant Time: Dec 15 04:28:34 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 04:25:21 2015
Response via : Initial Calibration

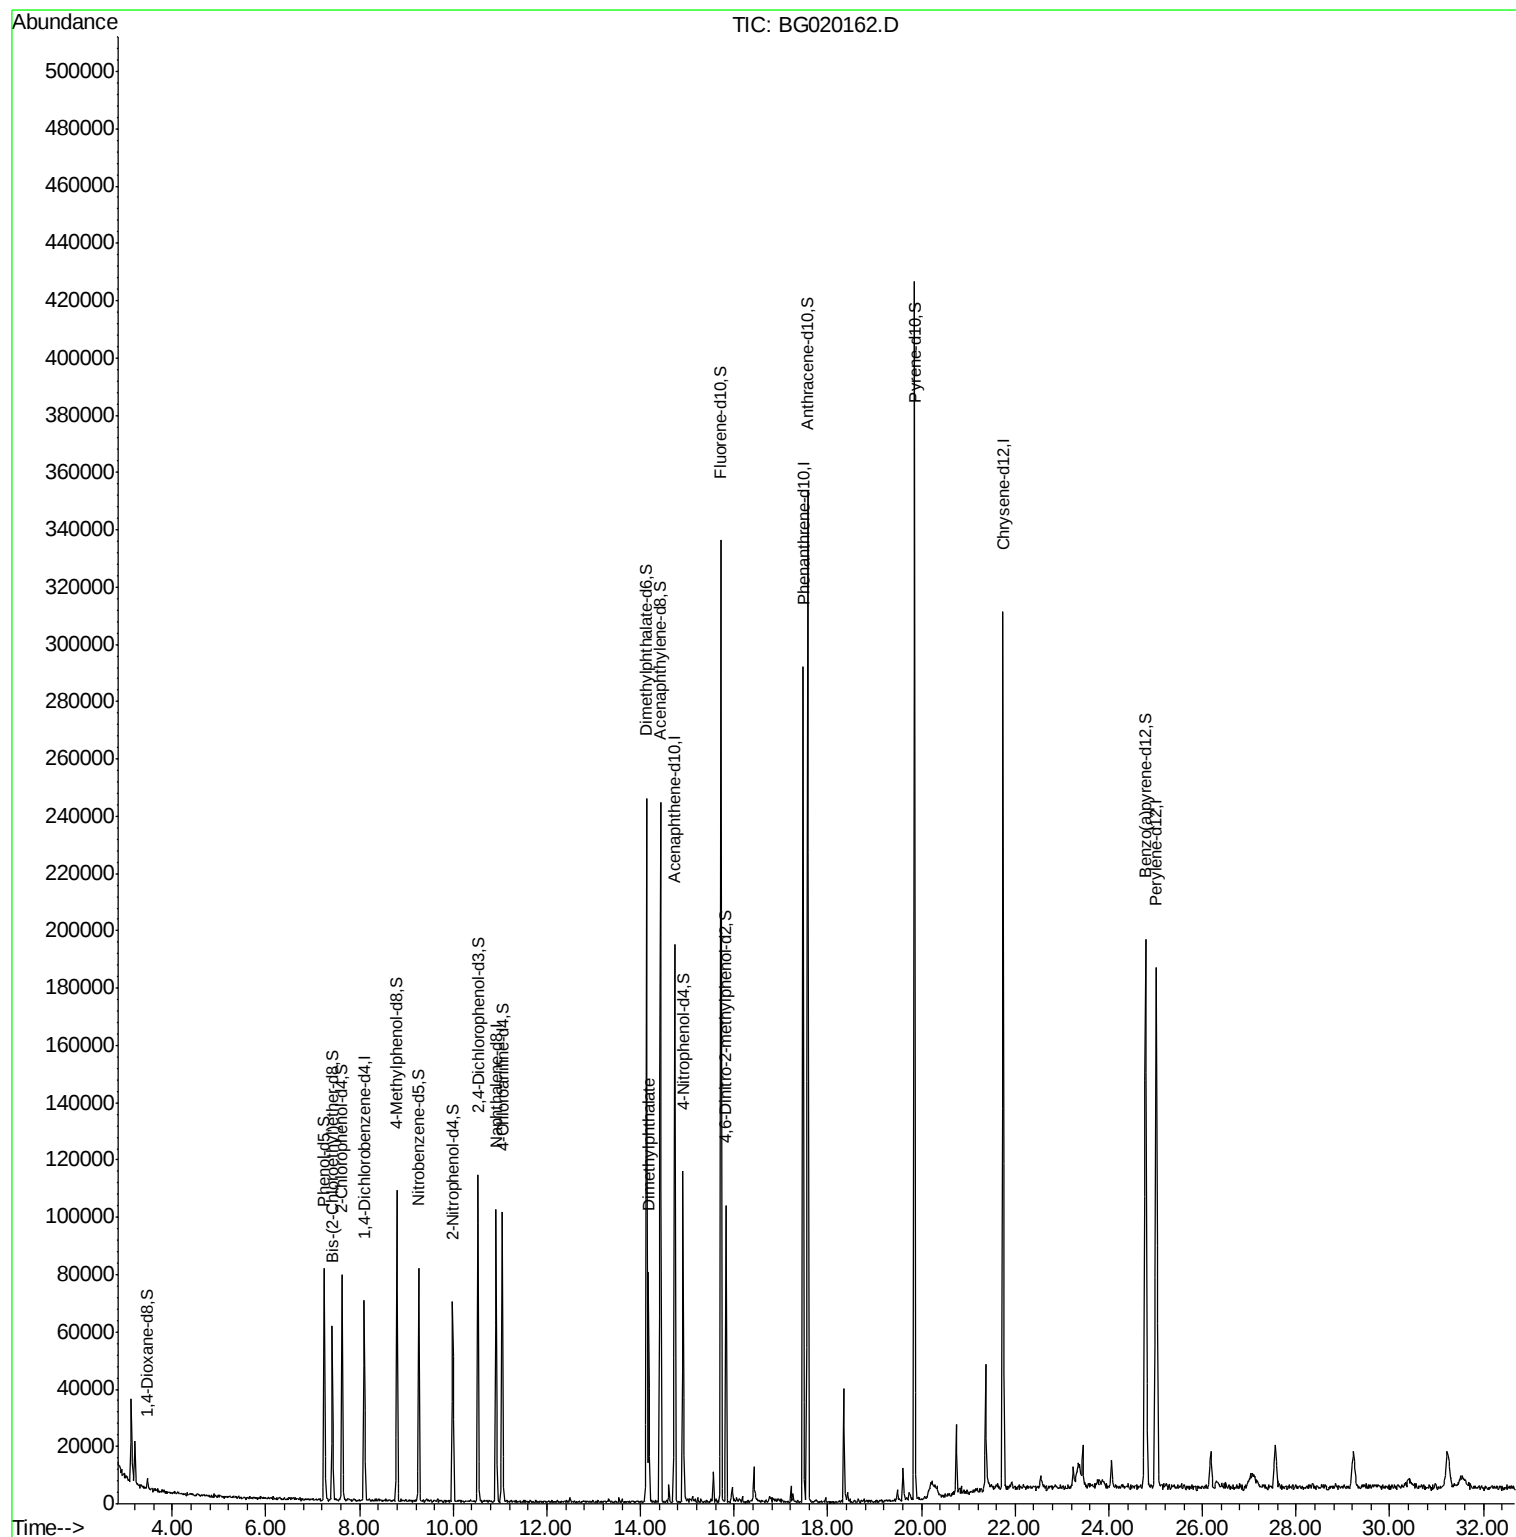

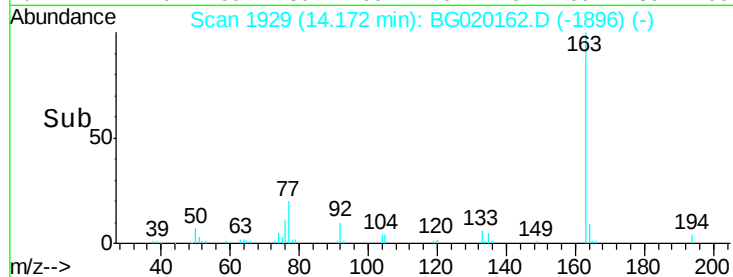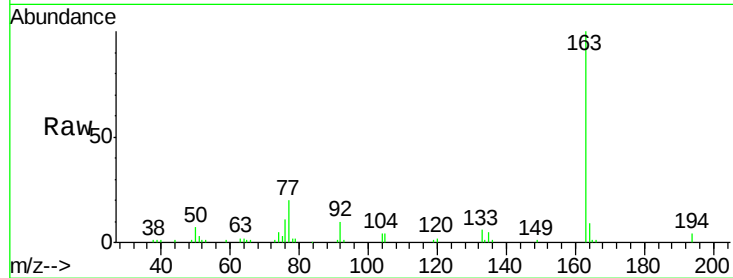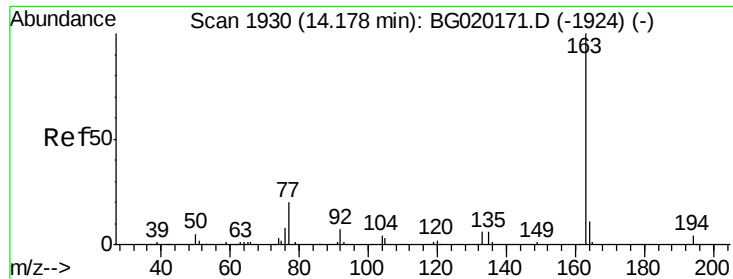

#45

Dimethylphthalate

Concen: 9.42 ng/ul

RT: 14.17 min Scan# 1929

Delta R.T. -0.01 min

Lab File: BG020162.D

Acq: 14 Dec 2015 20:58

Instrument :

BNA_G

ClientSampleId :

D9N36

Tgt Ion:163 Resp: 51280

Ion Ratio Lower Upper

163 100

194 3.9 3.5 5.3

164 9.2 7.7 11.5

