

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
 Data File : BG020169.D
 Acq On : 15 Dec 2015 1:33
 Operator : UM/SJ
 Sample : G4787-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 G9BM5

Quant Time: Dec 15 04:30:39 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 04:25:21 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	23152	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	102007	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	74905	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	198556	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	225412	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	210961	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.47	96	2320	5.53	ng/uL	0.00
5) Phenol-d5	7.25	99	56960	27.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	36763	30.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	44144	29.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	49115	28.13	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	24086	30.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	28263	31.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	53293	29.73	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	67828	33.69	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	188584	31.13	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	217387	30.84	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	30423	28.00	ng/ul	0.00
58) Fluorene-d10	15.72	176	166016	30.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	24512	20.82	ng/ul	0.00
71) Anthracene-d10	17.57	188	268326	29.33	ng/ul	0.00
79) Pyrene-d10	19.85	212	286568	27.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.79	264	272386	25.89	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	89450	14.46	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG121515\
Data File : BG020169.D
Acq On : 15 Dec 2015 1:33
Operator : UM/SJ
Sample : G4787-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
G9BM5

Quant Time: Dec 15 04:30:39 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 04:25:21 2015
Response via : Initial Calibration

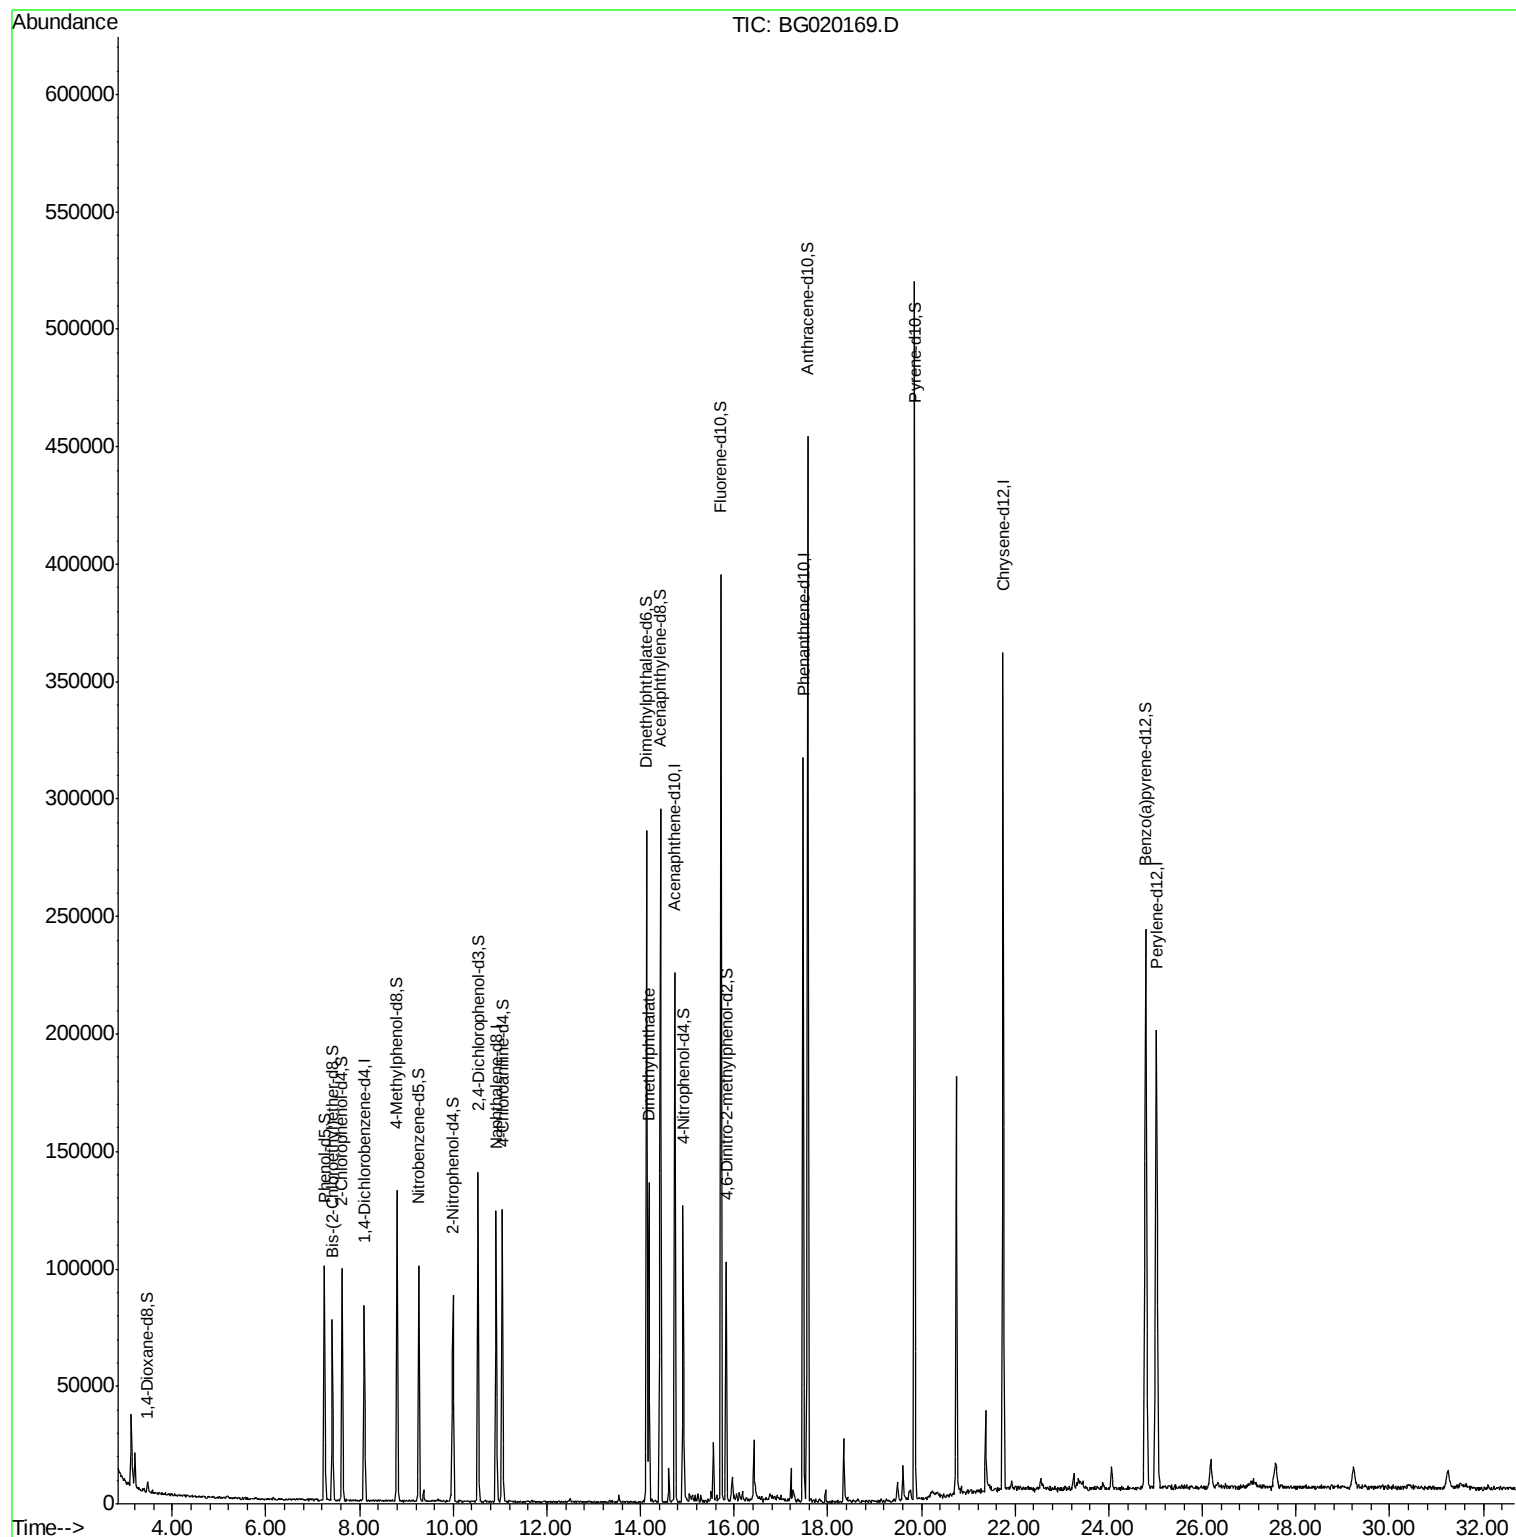

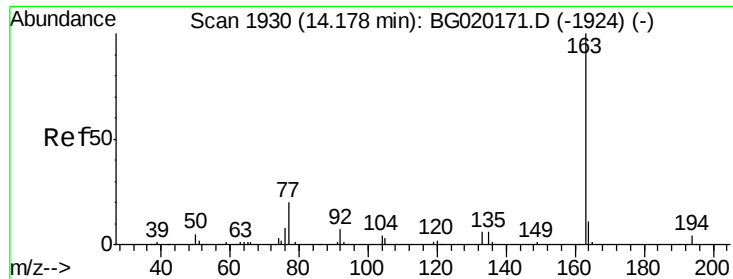

#45

Dimethylphthalate

Concen: 14.46 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.00 min

Lab File: BG020169.D


Acq: 15 Dec 2015 1:33

Instrument :

BNA_G

ClientSampleId :

G9BM5

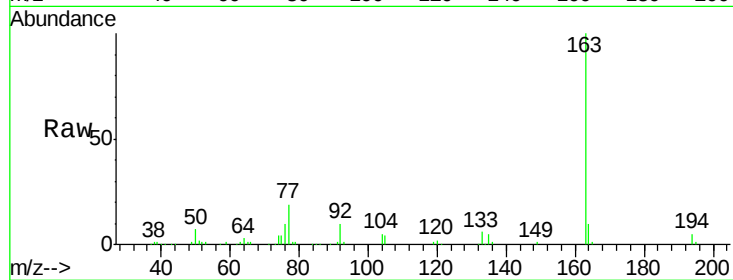

Tgt Ion:163 Resp: 89450

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 10.5 7.7 11.5

